

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ012224\
 Data File : PQ064936.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jan 2024 02:07
 Operator : YP\AJ
 Sample : P1202-06 10X
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 KZZ375Z-1-2

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/23/2024
 Supervised By :Sohil Jodhani 01/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 03:50:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ011724.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 18 00:09:27 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.471	2.743	4975494	12978913	1.336m	1.944m#
2) SA Decachlor...	8.770	7.524	7901307	15143301	2.557m	2.084

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ012224\
Data File : PQ064936.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jan 2024 02:07
Operator : YP\AJ
Sample : P1202-06 10X
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
KZZ375Z-1-2


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/23/2024
Supervised By :Sohil Jodhani 01/23/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 03:50:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ011724.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 18 00:09:27 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

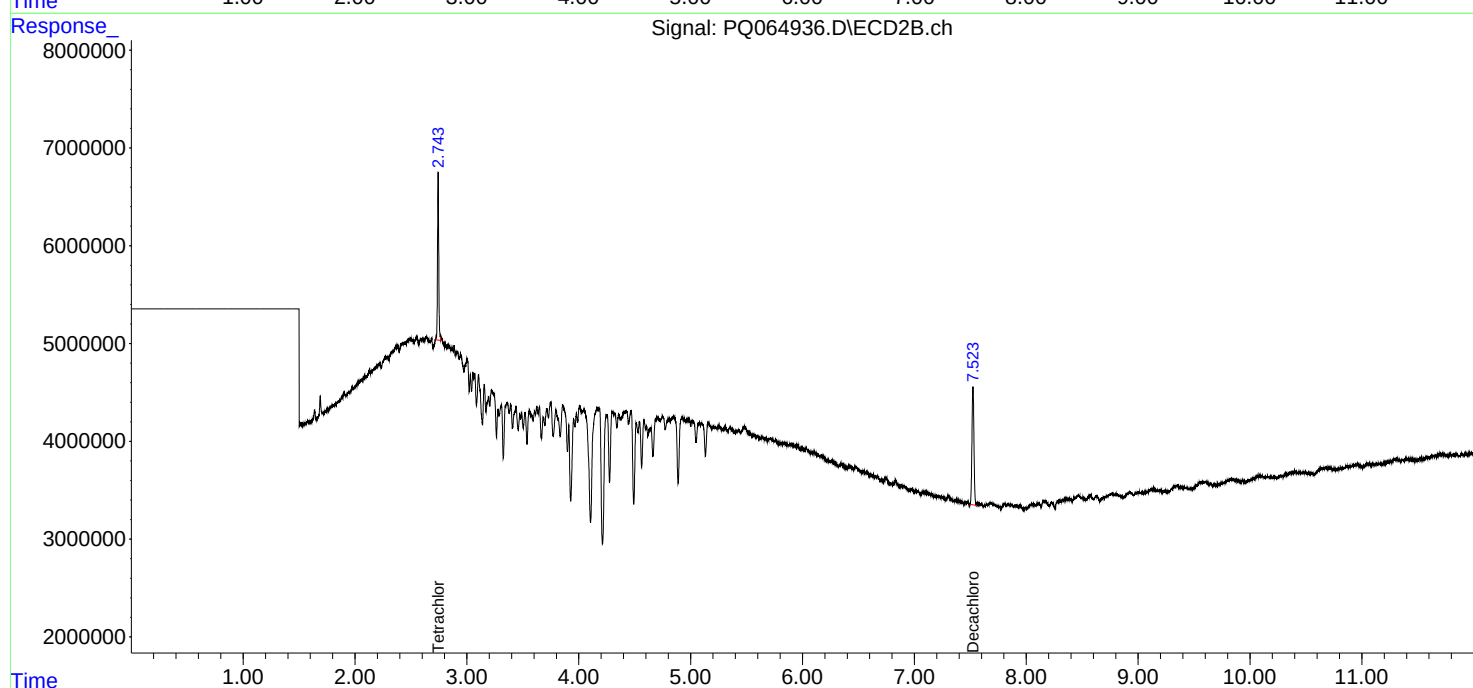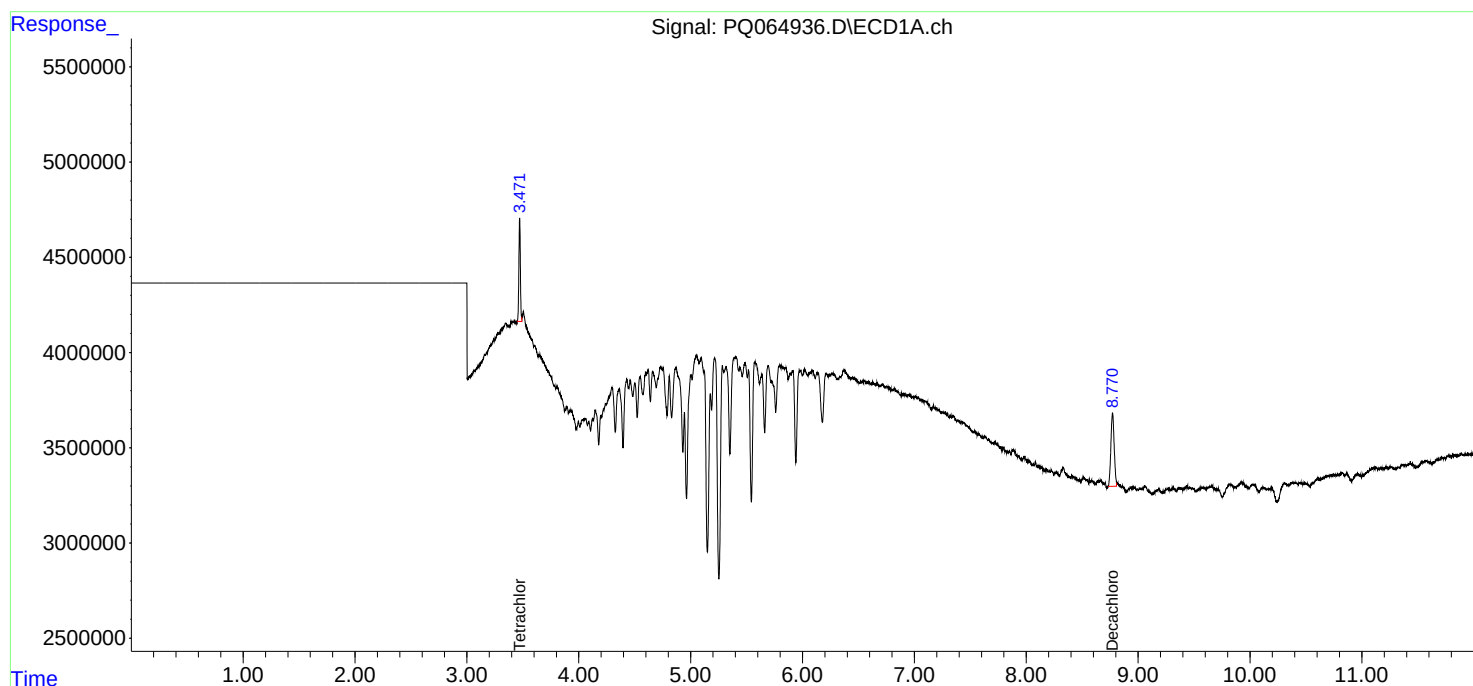

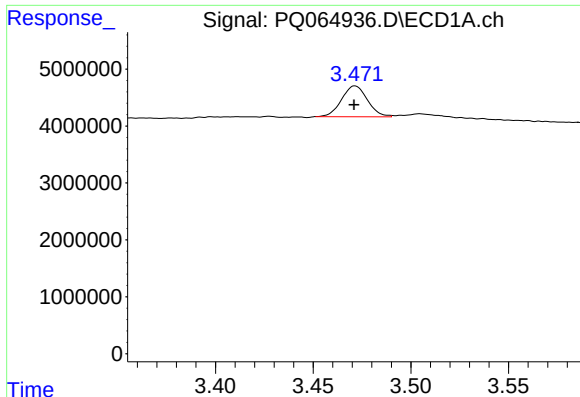


#1 Tetrachloro-m-xylene

R.T.: 3.471 min
Delta R.T.: 0.000 min
Response: 4975494
Conc: 1.34 ng/ml

Instrument :
ECD_Q
ClientSampleId :
KZZ375Z-1-2


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/23/2024
Supervised By :Sohil Jodhani 01/23/2024

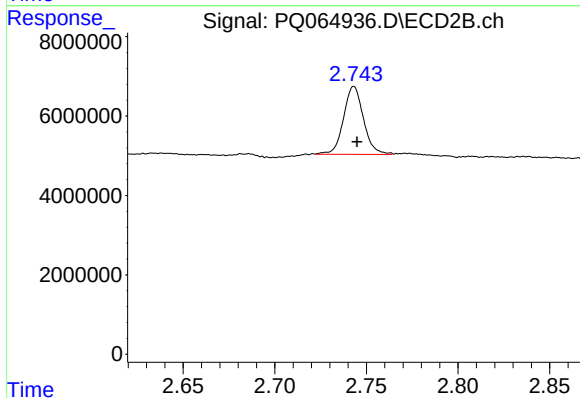


#1 Tetrachloro-m-xylene

R.T.: 2.743 min
Delta R.T.: -0.002 min
Response: 12978913
Conc: 1.94 ng/ml m

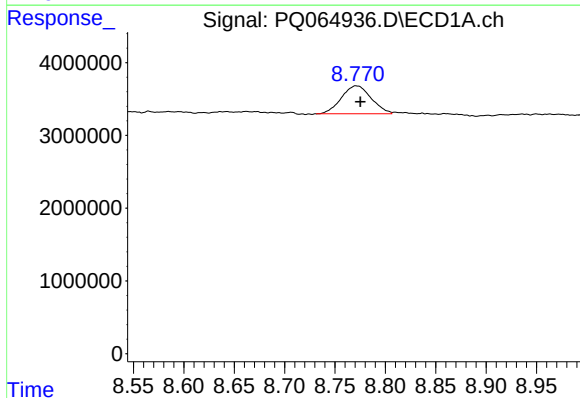

#2 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: -0.005 min
Response: 7901307
Conc: 2.56 ng/ml m

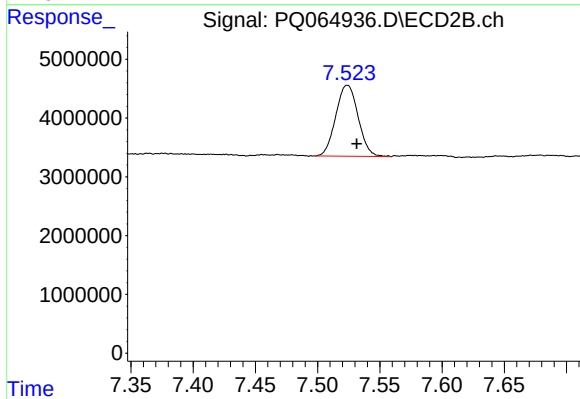

#2 Decachlorobiphenyl

R.T.: 7.524 min
Delta R.T.: -0.007 min
Response: 15143301
Conc: 2.08 ng/ml