

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ012722\
 Data File : PQ056057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2022 03:34
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/28/2022
 Supervised By :Ankita Jodhani 01/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 05:16:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ011922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 20 13:18:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.234	4.293	312.0E6	269.0E6	23.036	23.924
2) SA Decachlor...	11.408	9.649	375.2E6	192.3E6	25.698	24.112m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ012722\
Data File : PQ056057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2022 03:34
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/28/2022
Supervised By :Ankita Jodhani 01/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 05:16:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ011922.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 20 13:18:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

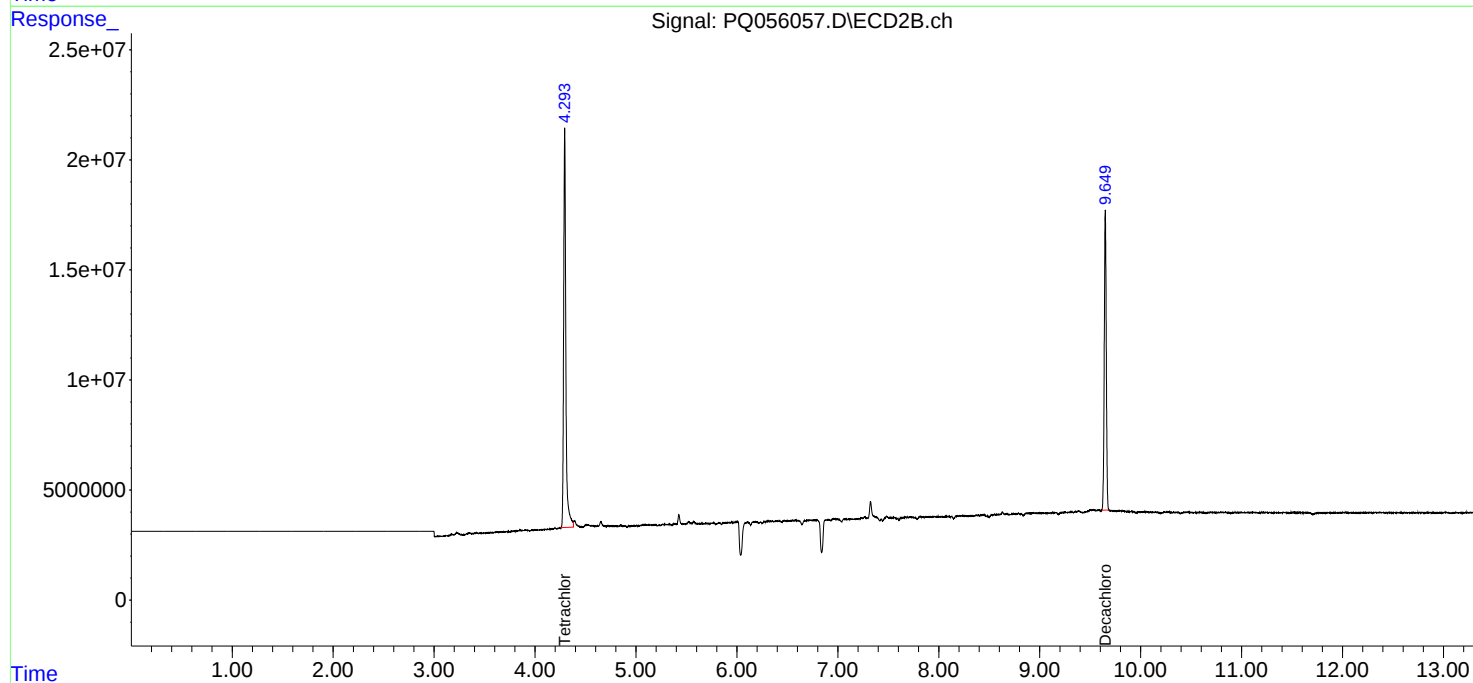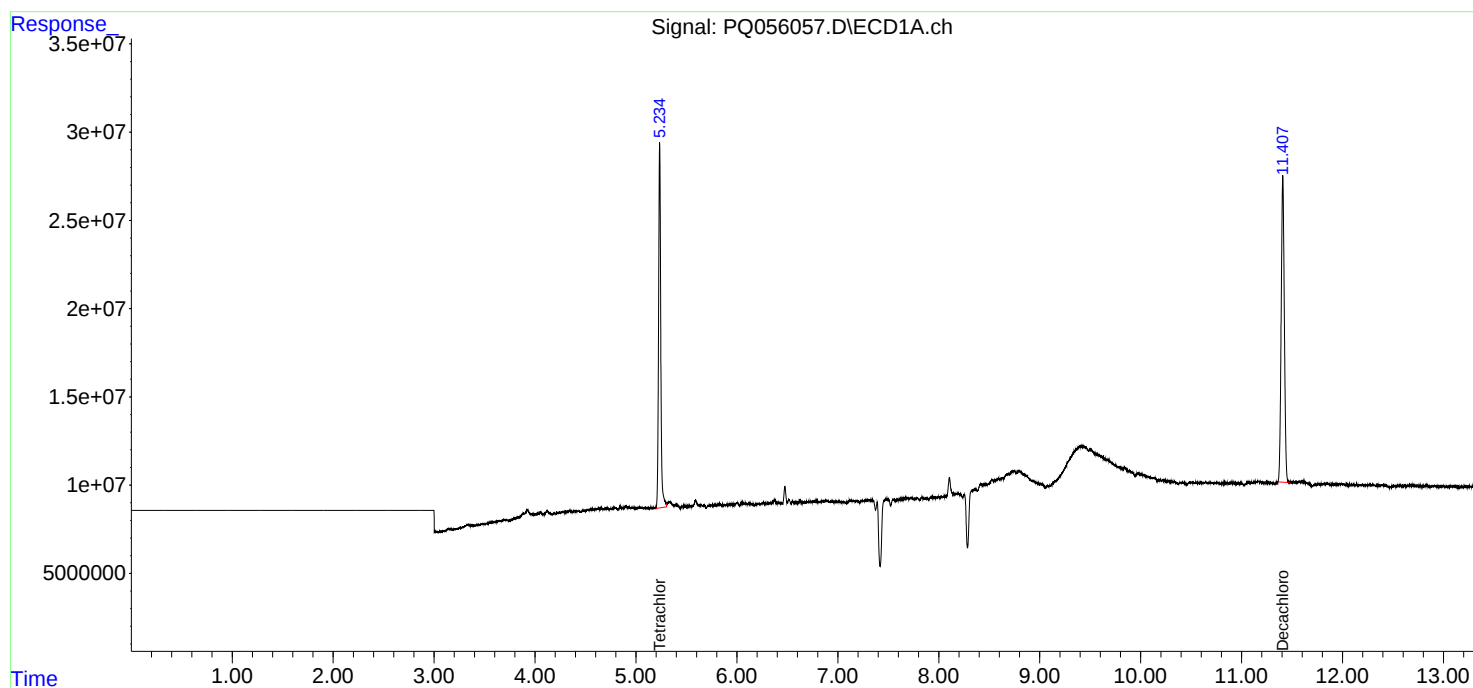

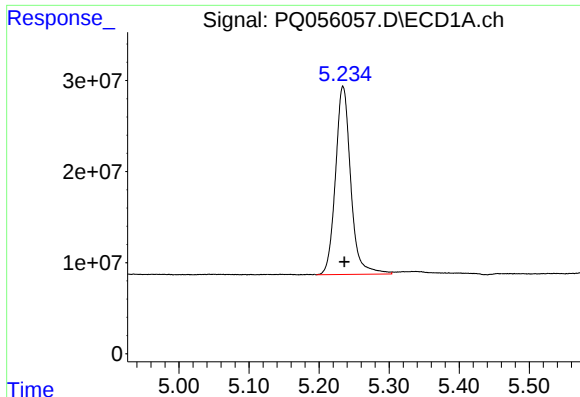

#1 Tetrachloro-m-xylene

R.T.: 5.234 min
Delta R.T.: -0.002 min
Response: 312000605
Conc: 23.04 ng/ml

Instrument :

ECD_Q


ClientSampleId :

I.BLK

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 01/28/2022
Supervised By :Ankita Jodhani 01/28/2022

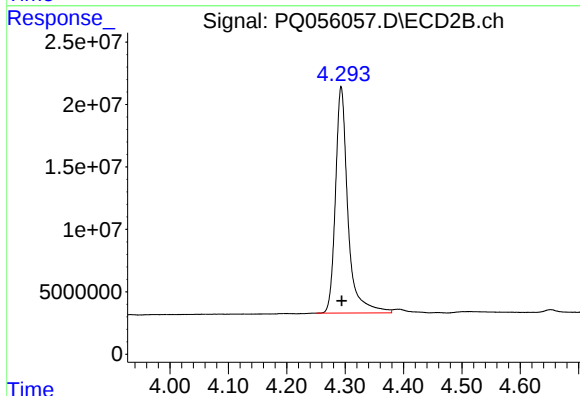


#1 Tetrachloro-m-xylene

R.T.: 4.293 min
Delta R.T.: -0.001 min
Response: 268994578
Conc: 23.92 ng/ml

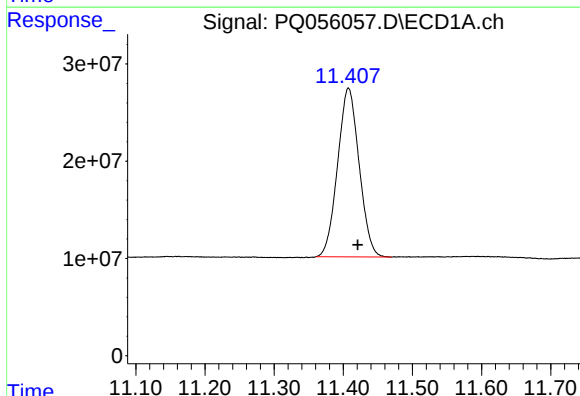

#2 Decachlorobiphenyl

R.T.: 11.408 min
Delta R.T.: -0.013 min
Response: 375151797
Conc: 25.70 ng/ml

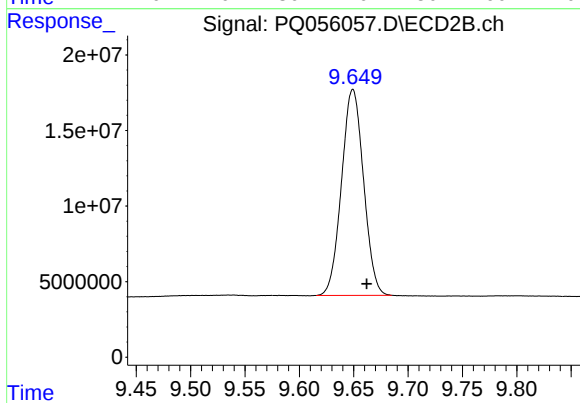

#2 Decachlorobiphenyl

R.T.: 9.649 min
Delta R.T.: -0.013 min
Response: 192300200
Conc: 24.11 ng/ml m