

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ012925\
 Data File : PQ069874.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2025 18:43
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 00:49:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ012825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 28 14:44:45 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.416	2.785	205.3E6	154.9E6	25.405	20.383
2) SA Decachlor...	8.528	7.559	129.0E6	177.4E6	27.728	23.047

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ012925\
Data File : PQ069874.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2025 18:43
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 00:49:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ012825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 28 14:44:45 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

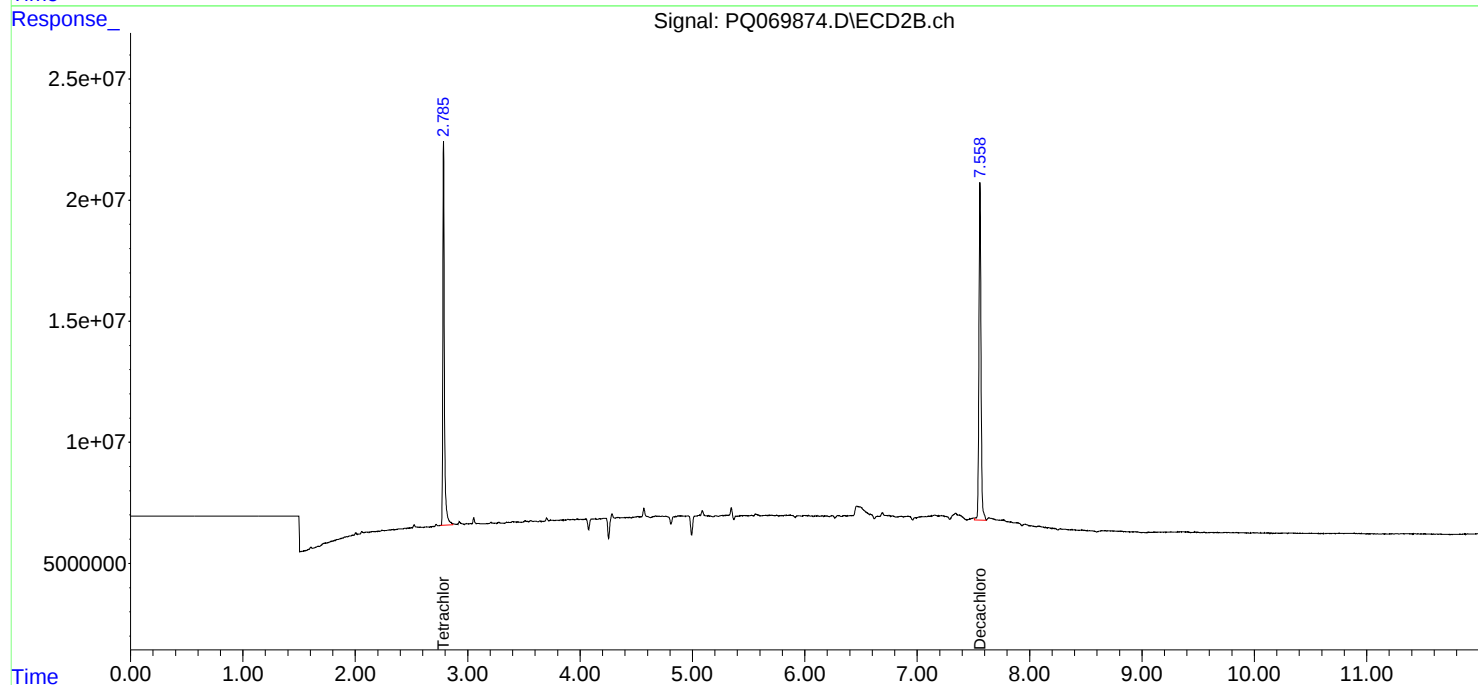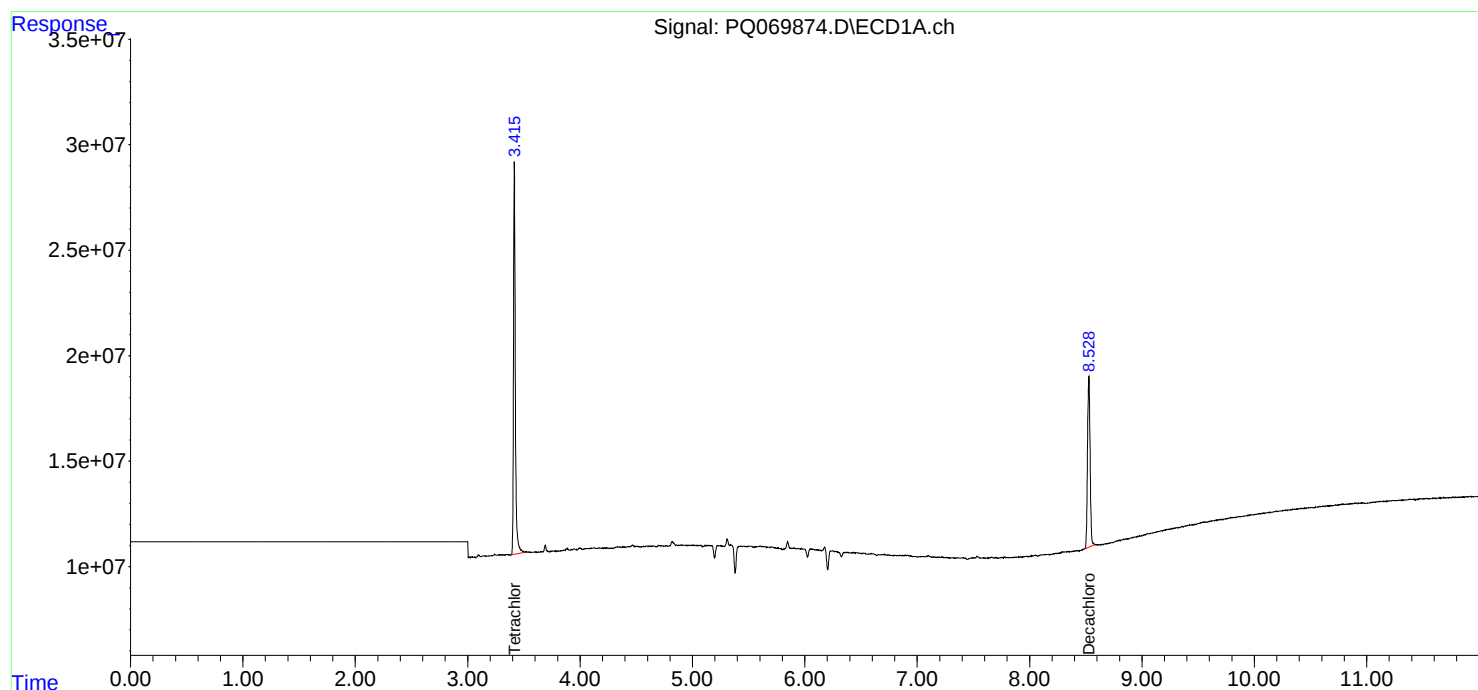


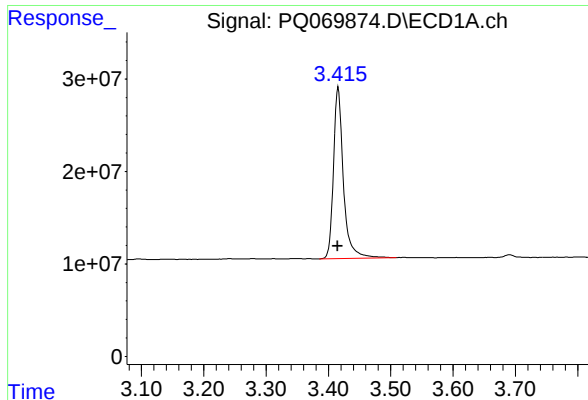

#1 Tetrachloro-m-xylene


R.T.: 3.416 min
Delta R.T.: 0.000 min
Response: 205251770
Conc: 25.40 ng/ml

Instrument :
ECD_Q
ClientSampleId :
I.BLK

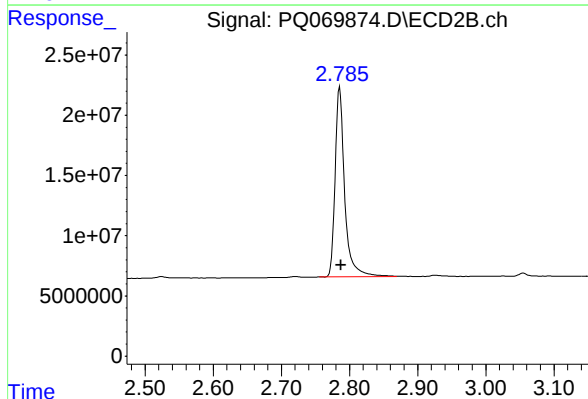


#1 Tetrachloro-m-xylene

R.T.: 2.785 min
Delta R.T.: -0.002 min
Response: 154917306
Conc: 20.38 ng/ml

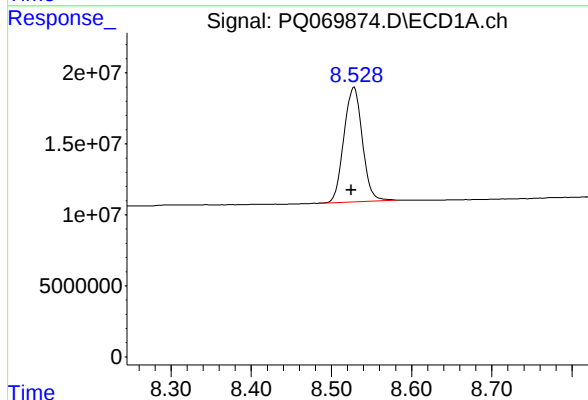

#2 Decachlorobiphenyl

R.T.: 8.528 min
Delta R.T.: 0.004 min
Response: 128961753
Conc: 27.73 ng/ml

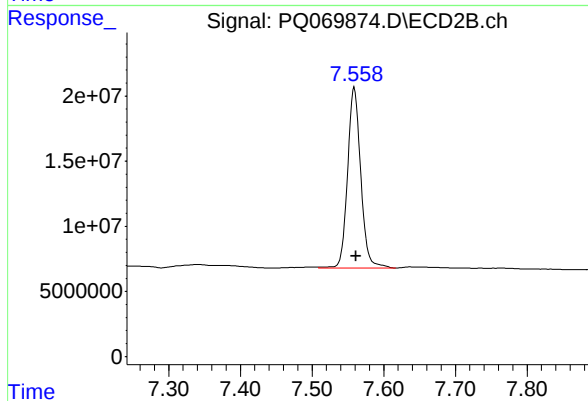

#2 Decachlorobiphenyl

R.T.: 7.559 min
Delta R.T.: -0.002 min
Response: 177431738
Conc: 23.05 ng/ml