

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ013024\
 Data File : PQ065160.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jan 2024 10:51
 Operator : YP\AJ
 Sample : P1271-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 SB-02-20240124-8.5-9.5

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/31/2024
 Supervised By :Sohil Jodhani 01/31/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 00:50:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ011724.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 18 00:09:27 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.465	2.743	70772842	145.5E6	18.998m	21.783
2) SA Decachlor...	8.769	7.518	39597776	98964368	12.813	13.617

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ013024\
Data File : PQ065160.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jan 2024 10:51
Operator : YP\AJ
Sample : P1271-06
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
SB-02-20240124-8.5-9.5


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/31/2024
Supervised By :Sohil Jodhani 01/31/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 00:50:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ011724.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 18 00:09:27 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

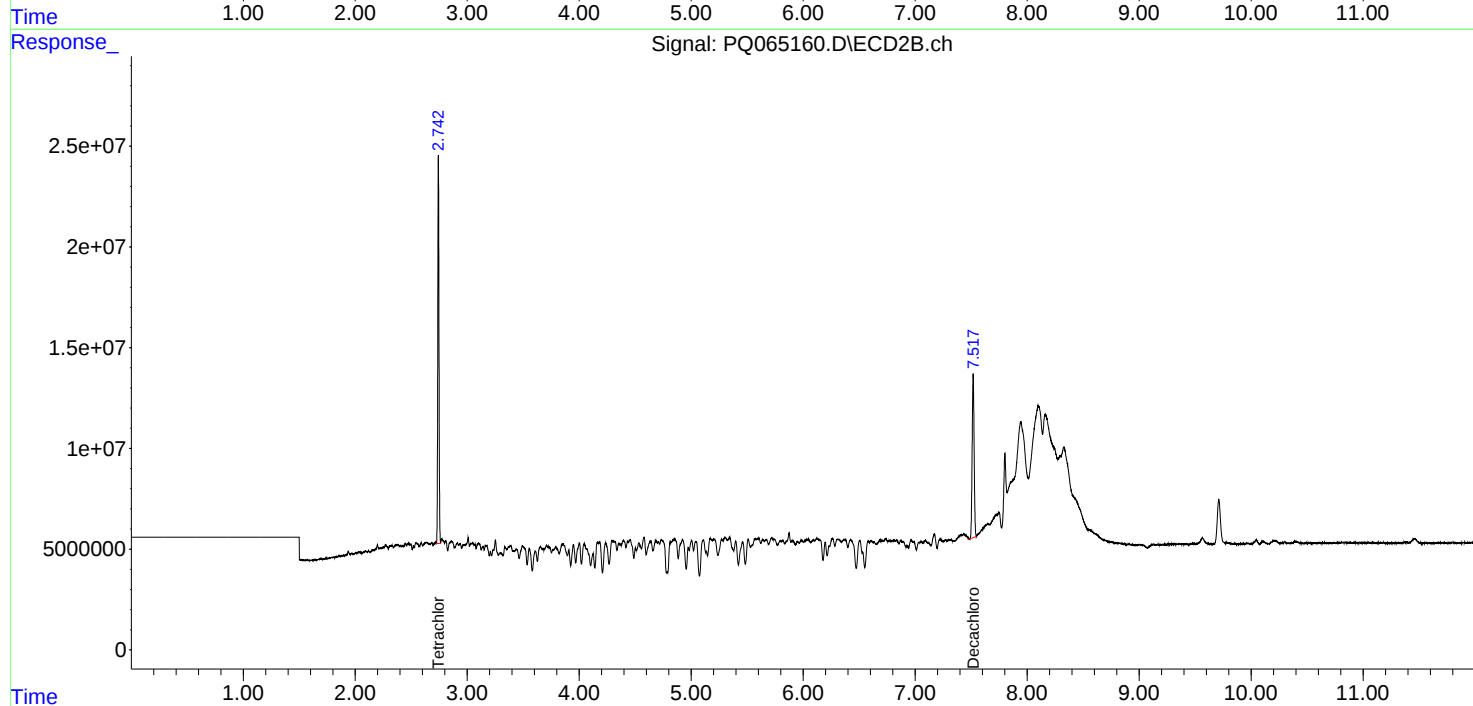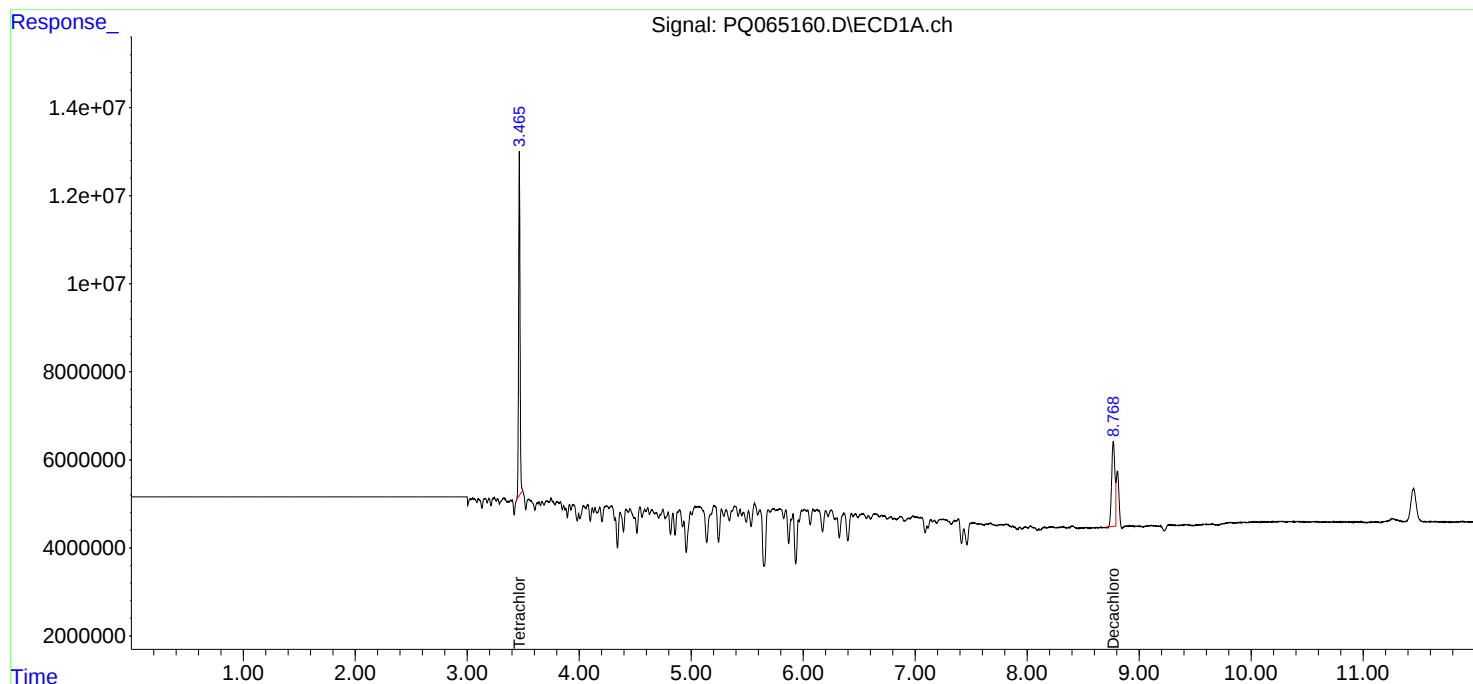

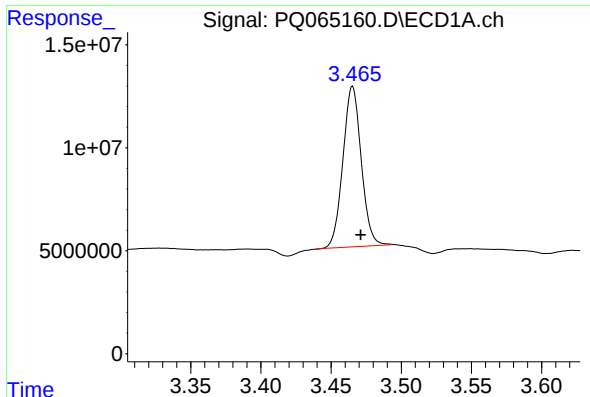


#1 Tetrachloro-m-xylene

R.T.: 3.465 min
Delta R.T.: -0.006 min
Response: 70772842
Conc: 19.00 ng/ml

Instrument :
ECD_Q
ClientSampleId :
SB-02-20240124-8.5-9.5


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/31/2024
Supervised By :Sohil Jodhani 01/31/2024

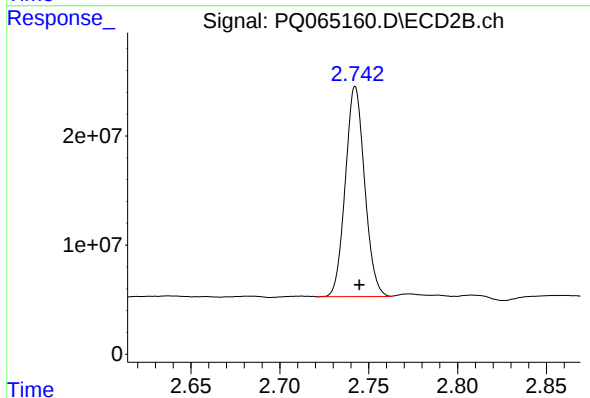


#1 Tetrachloro-m-xylene

R.T.: 2.743 min
Delta R.T.: -0.002 min
Response: 145459956
Conc: 21.78 ng/ml

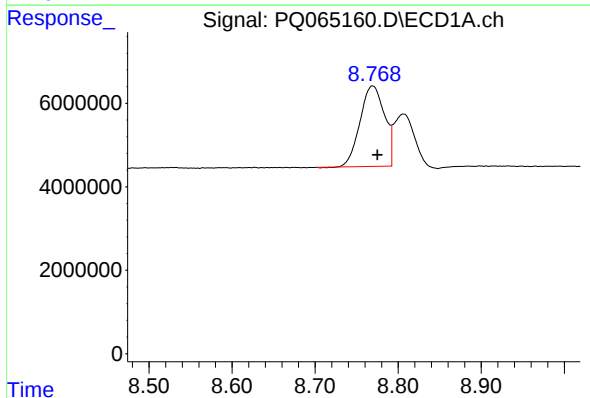

#2 Decachlorobiphenyl

R.T.: 8.769 min
Delta R.T.: -0.006 min
Response: 39597776
Conc: 12.81 ng/ml

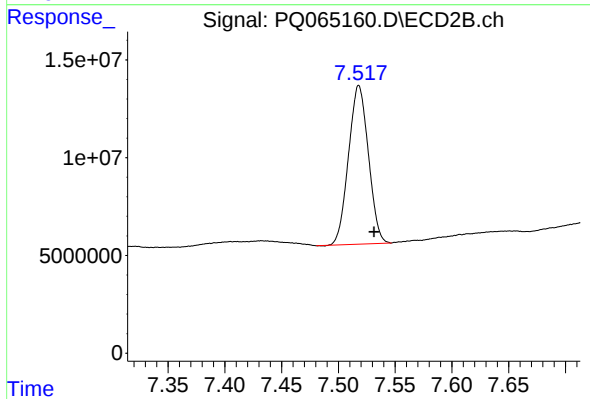

#2 Decachlorobiphenyl

R.T.: 7.518 min
Delta R.T.: -0.013 min
Response: 98964368
Conc: 13.62 ng/ml