

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ020222\
 Data File : PQ056061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Feb 2022 10:51
 Operator : AJ\MA
 Sample : PB142409BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 PB142409BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/03/2022
 Supervised By :Ankita Jodhani 02/03/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 02:24:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ011922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 20 13:18:56 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.236	4.294	267.3E6	228.3E6	19.733	20.306
2) SA Decachlor...	11.405	9.647	315.4E6	165.1E6	21.602m	20.703m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ020222\
Data File : PQ056061.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Feb 2022 10:51
Operator : AJ\MA
Sample : PB142409BL
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
PB142409BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2022
Supervised By :Ankita Jodhani 02/03/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 02:24:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ011922.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 20 13:18:56 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

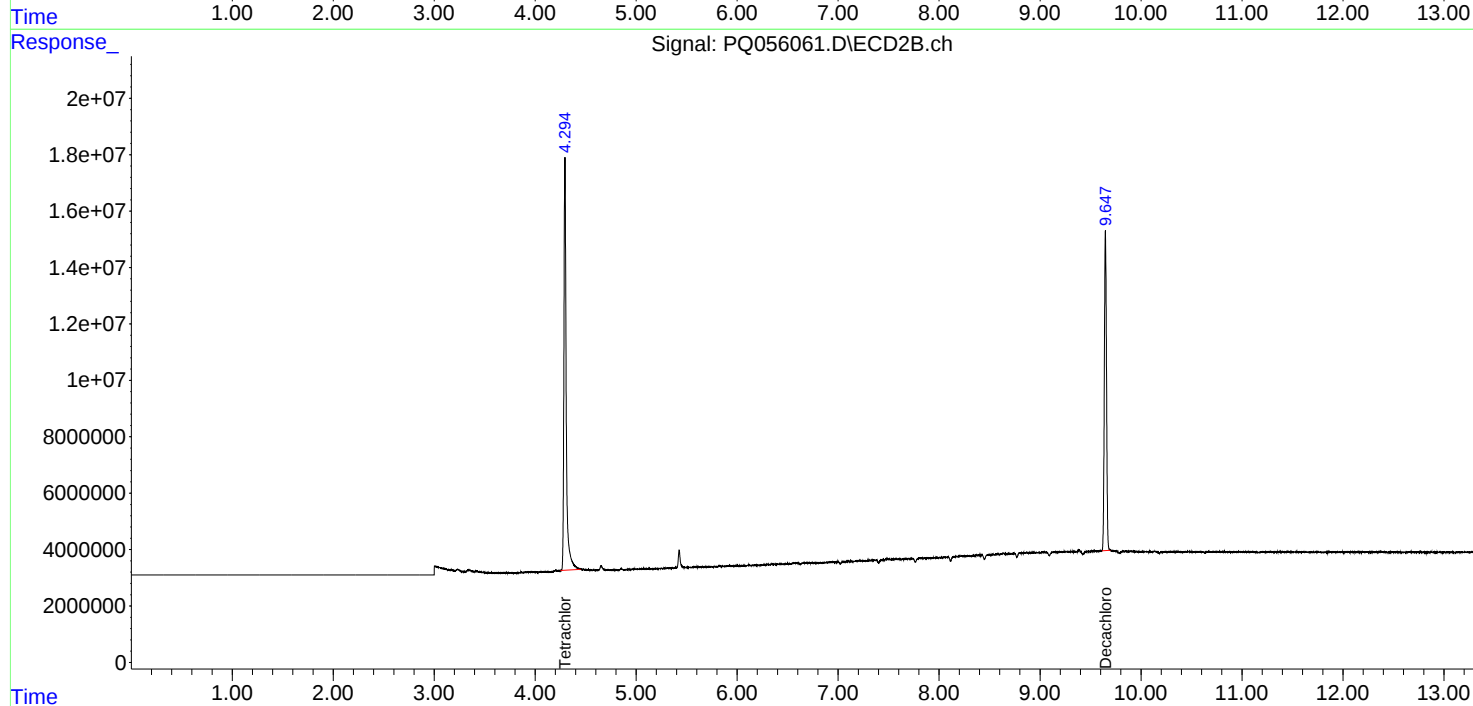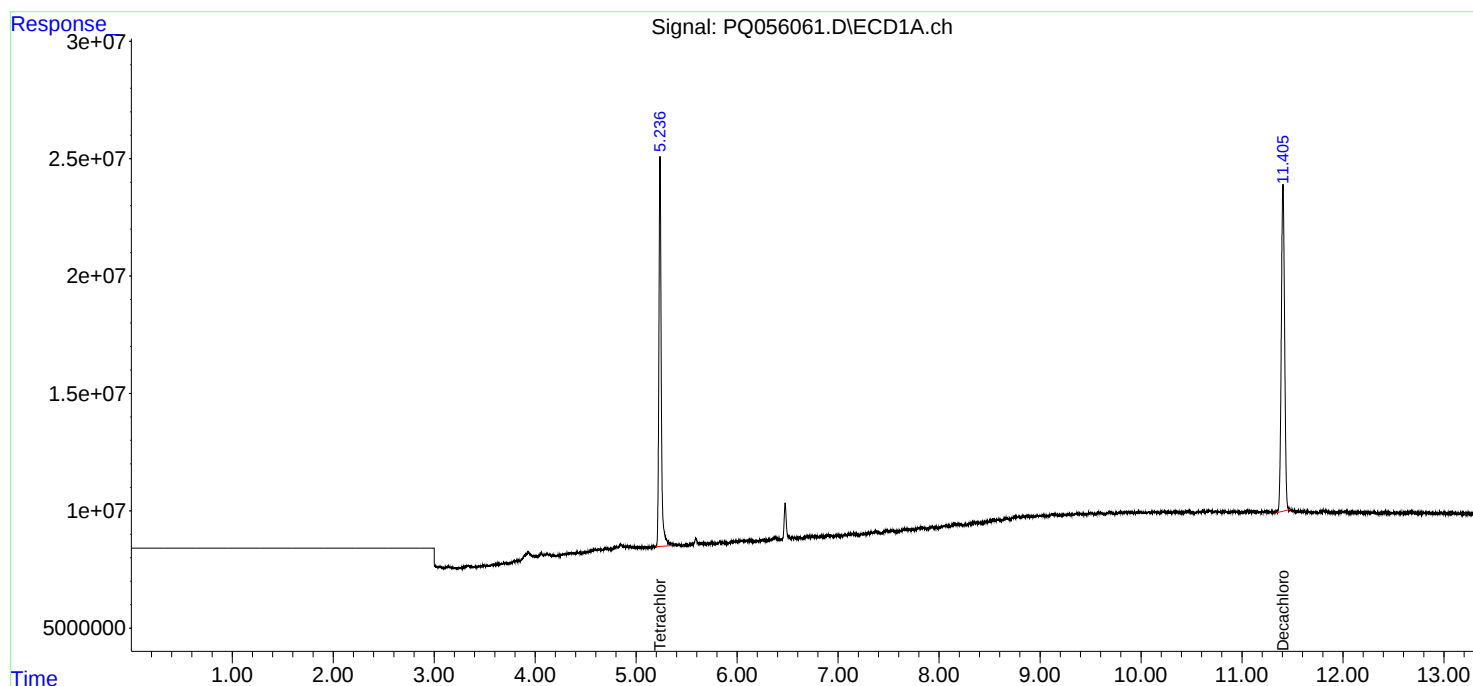

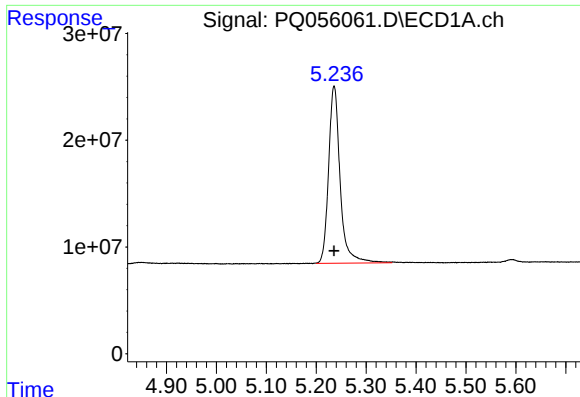


#1 Tetrachloro-m-xylene

R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 267260802
Conc: 19.73 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PB142409BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 02/03/2022
Supervised By :Ankita Jodhani 02/03/2022

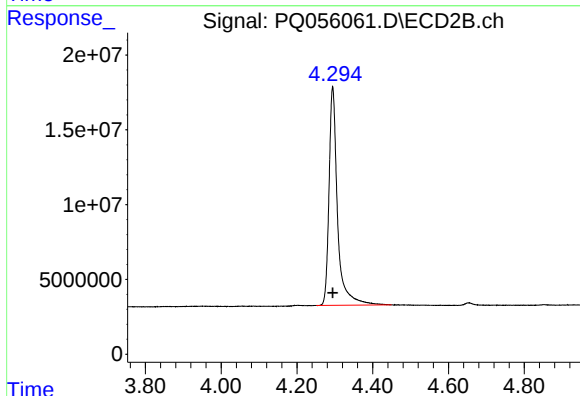


#1 Tetrachloro-m-xylene

R.T.: 4.294 min
Delta R.T.: 0.000 min
Response: 228310713
Conc: 20.31 ng/ml

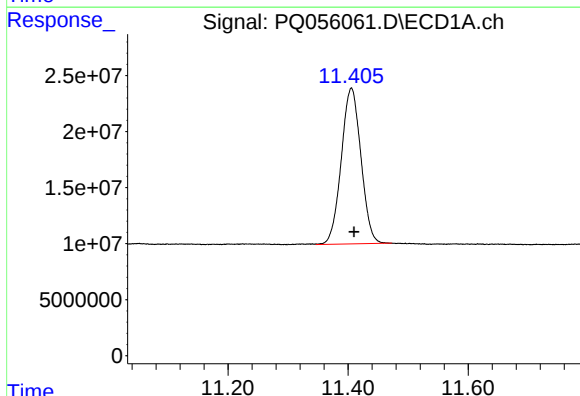

#2 Decachlorobiphenyl

R.T.: 11.405 min
Delta R.T.: -0.005 min
Response: 315354349
Conc: 21.60 ng/ml m

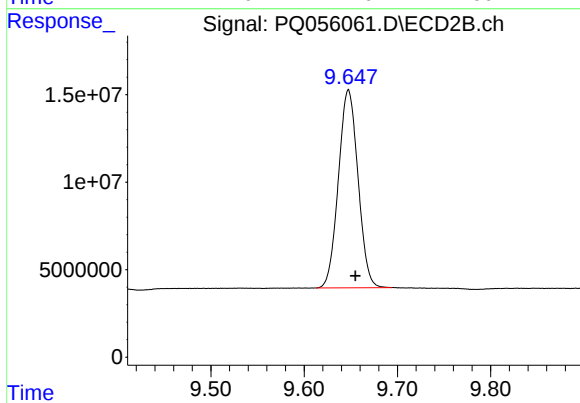

#2 Decachlorobiphenyl

R.T.: 9.647 min
Delta R.T.: -0.008 min
Response: 165111473
Conc: 20.70 ng/ml m