

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ020524\
 Data File : PQ065229.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2024 10:46
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/06/2024
 Supervised By :Sohil Jodhani 02/06/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 11:11:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ011724.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 18 00:09:27 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.475	2.745	60777356	120.5E6	16.315m	18.043
2) SA Decachlor...	8.793	7.521	50953944	127.9E6	16.488	17.593m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ020524\
Data File : PQ065229.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2024 10:46
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/06/2024
Supervised By :Sohil Jodhani 02/06/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 11:11:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ011724.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 18 00:09:27 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

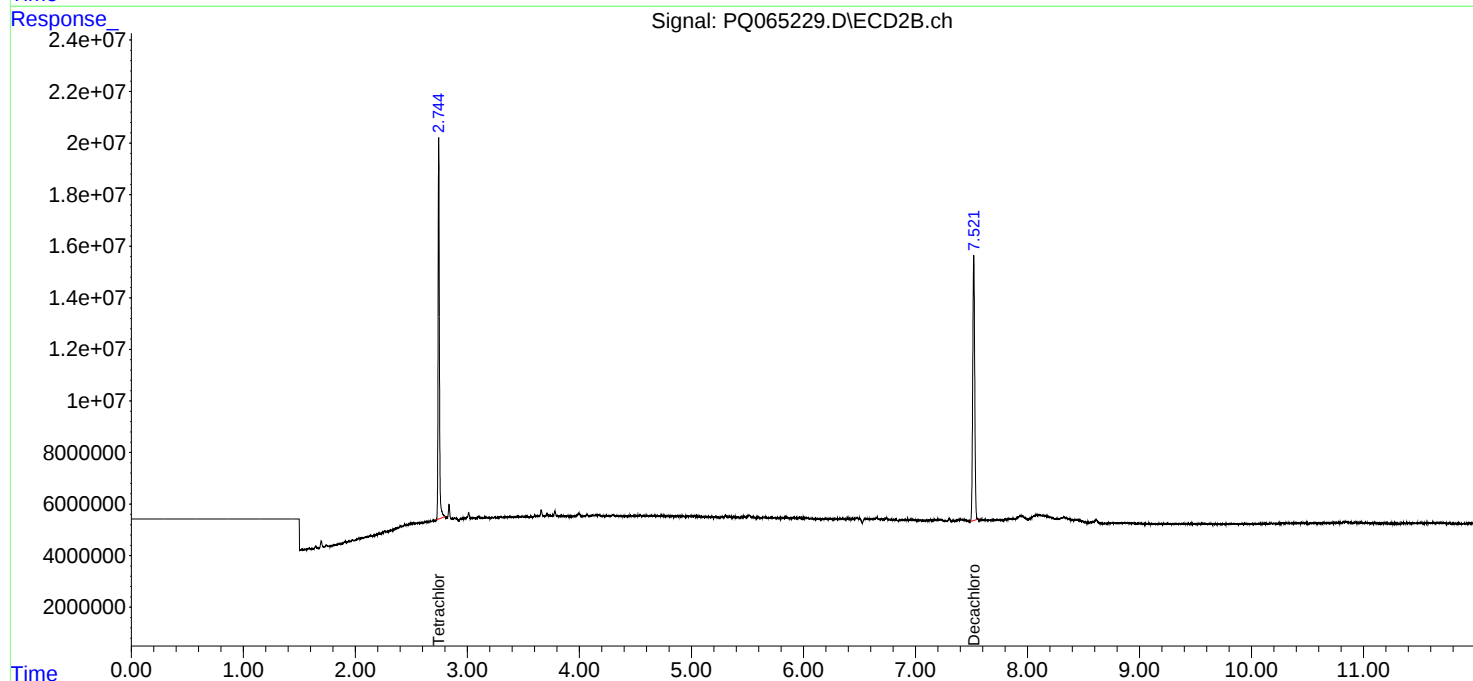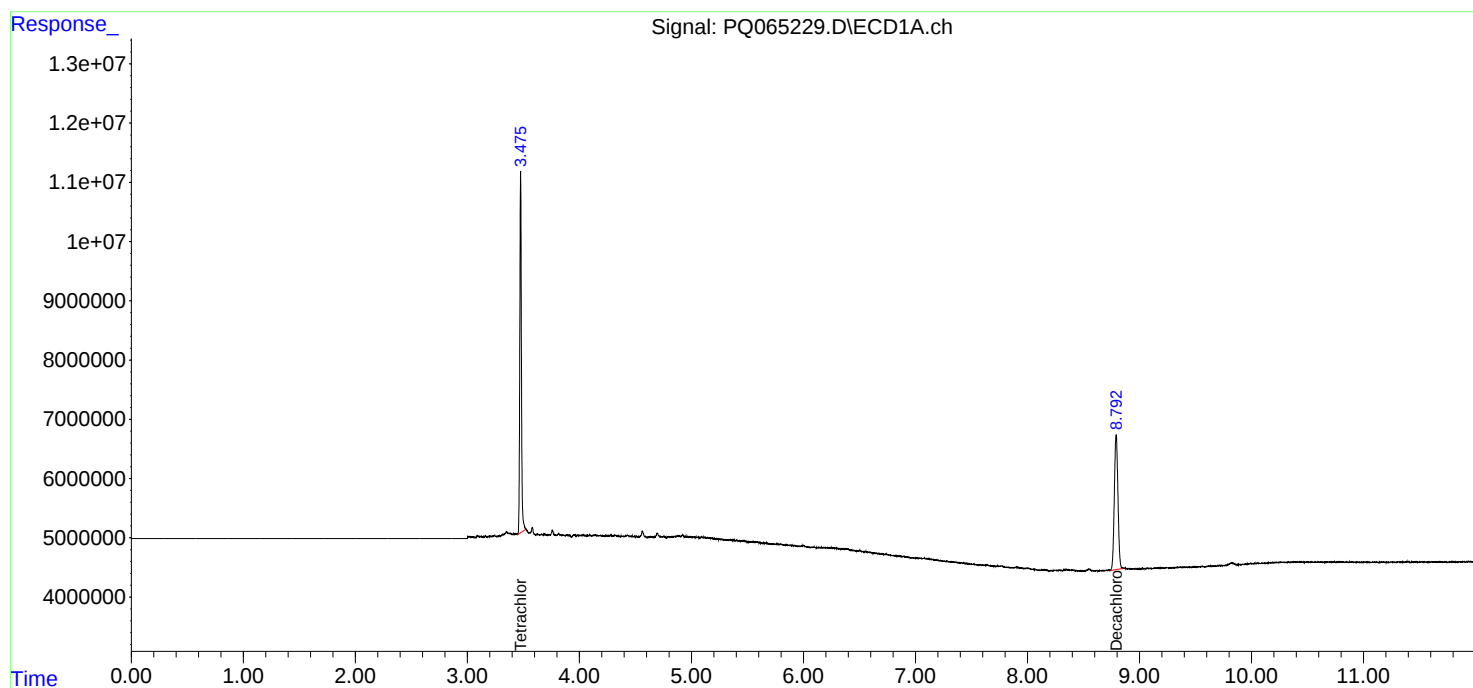

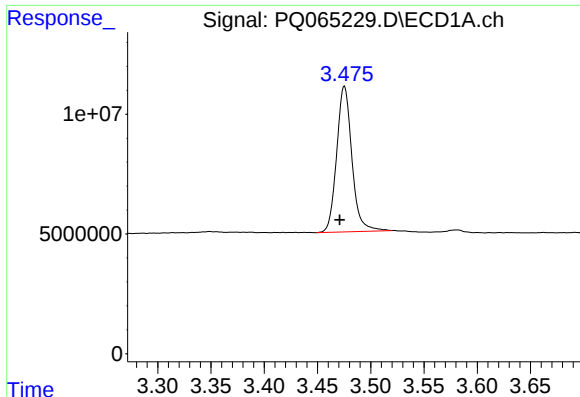


#1 Tetrachloro-m-xylene

R.T.: 3.475 min
Delta R.T.: 0.004 min
Response: 60777356
Conc: 16.31 ng/ml

Instrument :
ECD_Q
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/06/2024
Supervised By :Sohil Jodhani 02/06/2024

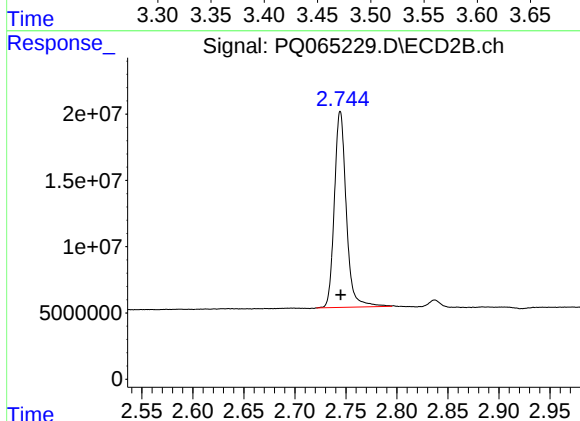


#1 Tetrachloro-m-xylene

R.T.: 2.745 min
Delta R.T.: 0.000 min
Response: 120486148
Conc: 18.04 ng/ml

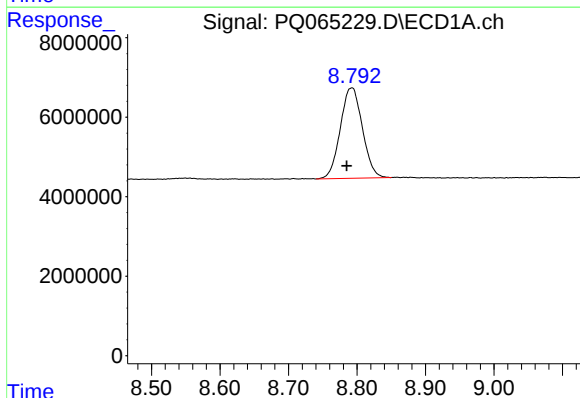

#2 Decachlorobiphenyl

R.T.: 8.793 min
Delta R.T.: 0.008 min
Response: 50953944
Conc: 16.49 ng/ml

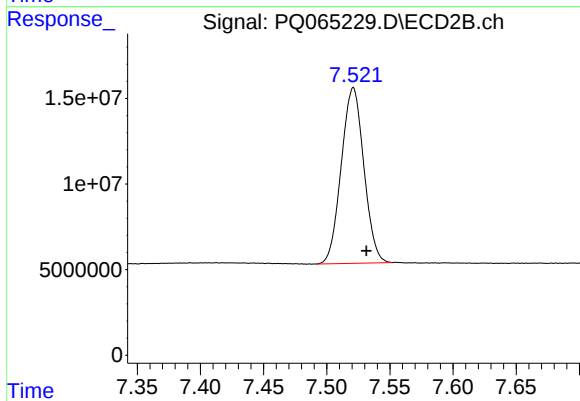

#2 Decachlorobiphenyl

R.T.: 7.521 min
Delta R.T.: -0.010 min
Response: 127856273
Conc: 17.59 ng/ml m