

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ020624\
 Data File : PQ065249.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2024 10:53
 Operator : YP\AJ
 Sample : P1066-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 WC-N-COMP

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/07/2024
 Supervised By :Sohil Jodhani 02/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 11:23:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ011724.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 18 00:09:27 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.467	2.744	61094015	122.2E6	16.400m	18.294
2) SA Decachlor...	8.773	7.518	48797432	100.2E6	15.790	13.793

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ020624\
Data File : PQ065249.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2024 10:53
Operator : YP\AJ
Sample : P1066-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
WC-N-COMP


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/07/2024
Supervised By :Sohil Jodhani 02/07/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 11:23:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ011724.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 18 00:09:27 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

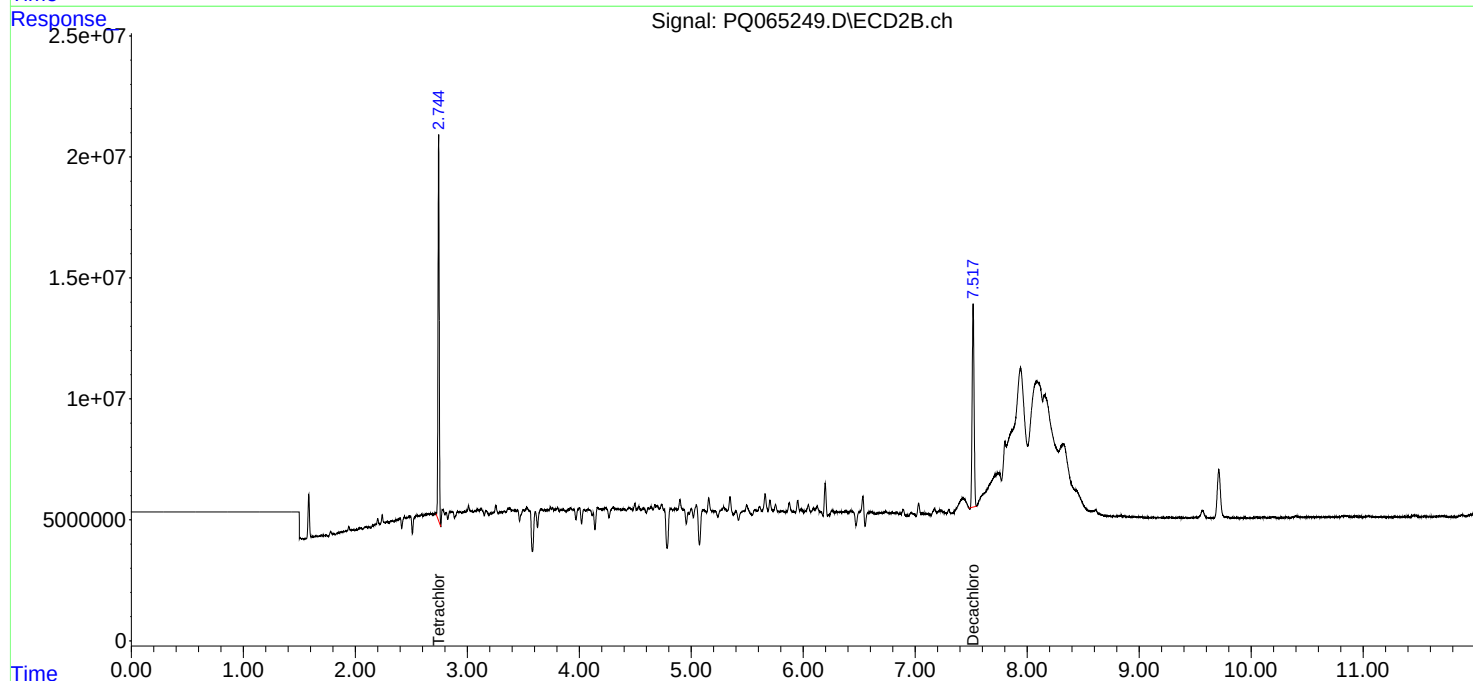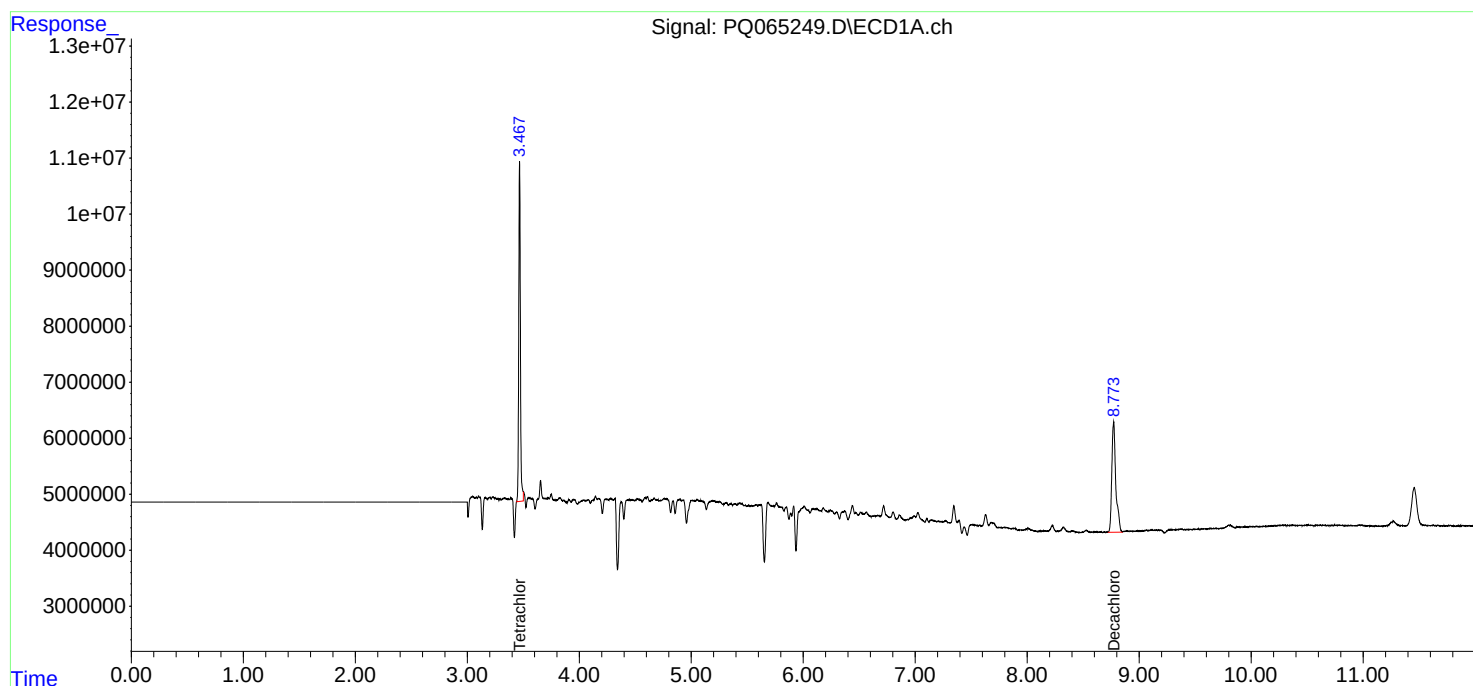

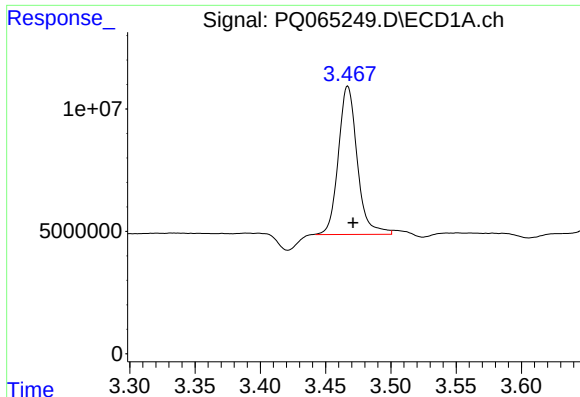


#1 Tetrachloro-m-xylene

R.T.: 3.467 min
Delta R.T.: -0.004 min
Response: 61094015
Conc: 16.40 ng/ml

Instrument :
ECD_Q
ClientSampleId :
WC-N-COMP


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/07/2024
Supervised By :Sohil Jodhani 02/07/2024

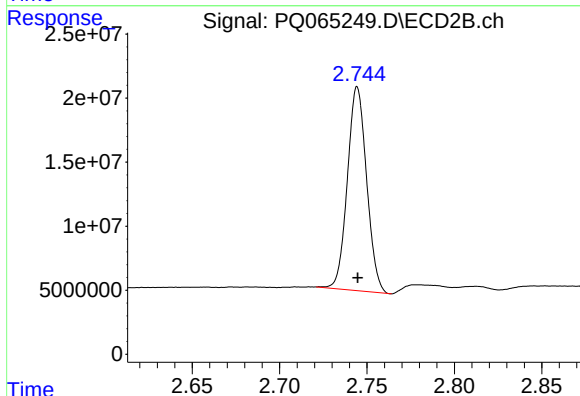


#1 Tetrachloro-m-xylene

R.T.: 2.744 min
Delta R.T.: 0.000 min
Response: 122160797
Conc: 18.29 ng/ml

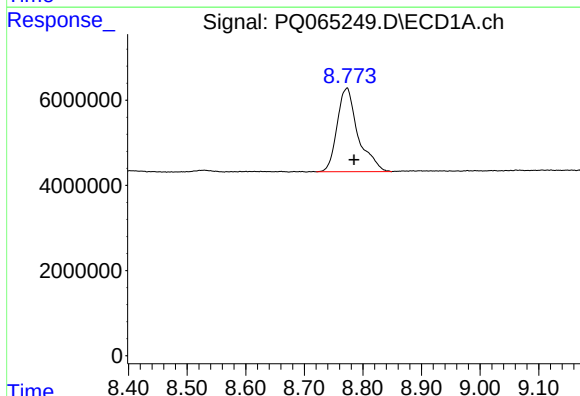

#2 Decachlorobiphenyl

R.T.: 8.773 min
Delta R.T.: -0.012 min
Response: 48797432
Conc: 15.79 ng/ml

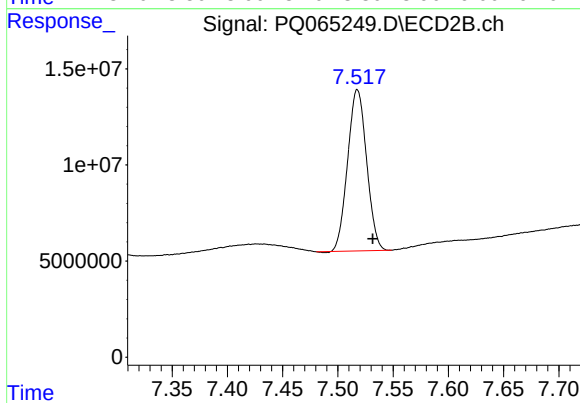

#2 Decachlorobiphenyl

R.T.: 7.518 min
Delta R.T.: -0.014 min
Response: 100236687
Conc: 13.79 ng/ml