

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ020819\
 Data File : PQ037115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2019 21:15
 Operator : SM\SJ
 Sample : K1404-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 A0C12-SS1-7.5-8.0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 21:54:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ020619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 06 18:32:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.307	3.693	46645068	36733617	10.498	15.906 #
2) SA Decachlor...	0.000	8.611	0	22976810	N.D.	12.229 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ020819\
Data File : PQ037115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2019 21:15
Operator : SM\SJ
Sample : K1404-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
A0C12-SS1-7.5-8.0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 21:54:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ020619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 06 18:32:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

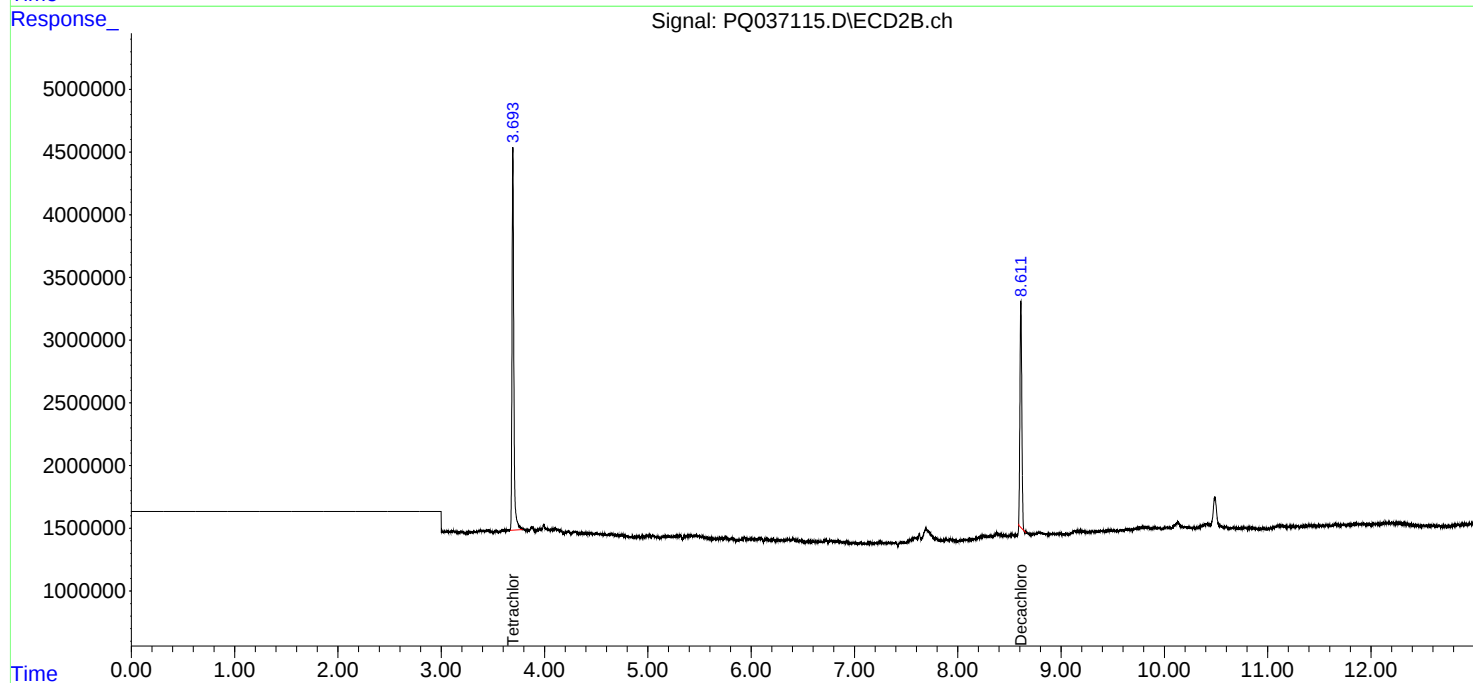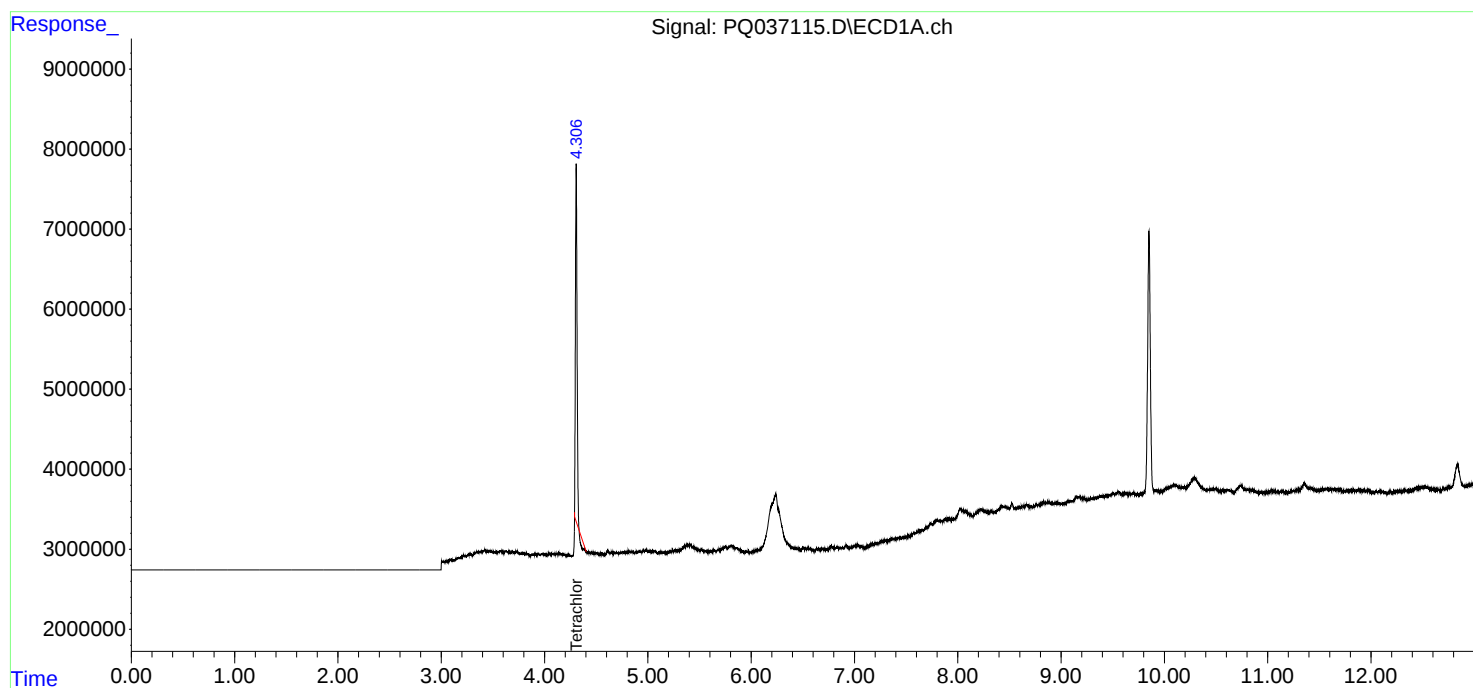


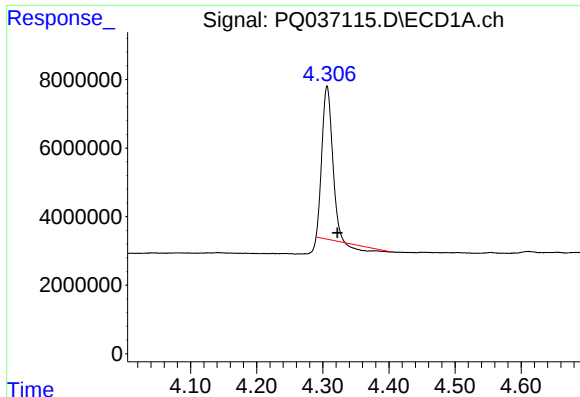

#1 Tetrachloro-m-xylene


R.T.: 4.307 min
Delta R.T.: -0.015 min
Response: 46645068
Conc: 10.50 ng/ml

Instrument :
ECD_Q
ClientSampleId :
A0C12-SS1-7.5-8.0

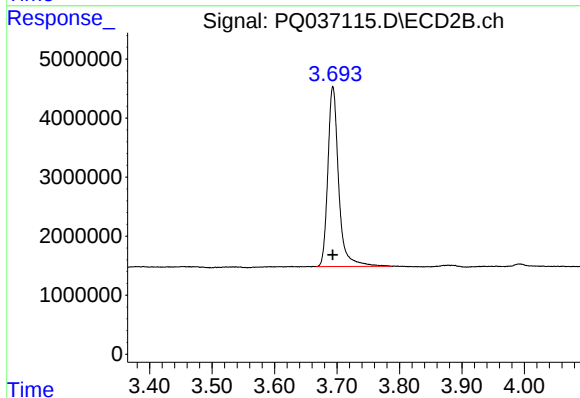


#1 Tetrachloro-m-xylene

R.T.: 3.693 min
Delta R.T.: 0.000 min
Response: 36733617
Conc: 15.91 ng/ml

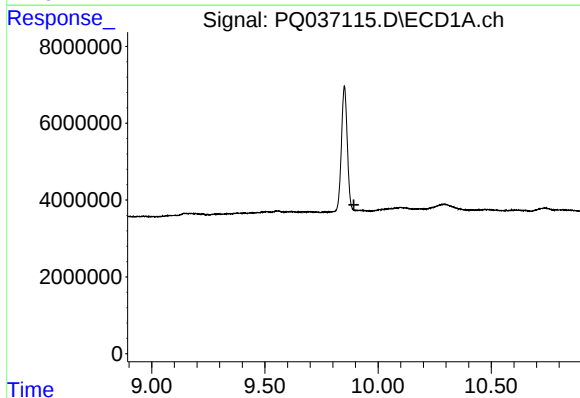

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.893 min
Response: 0
Conc: N.D.

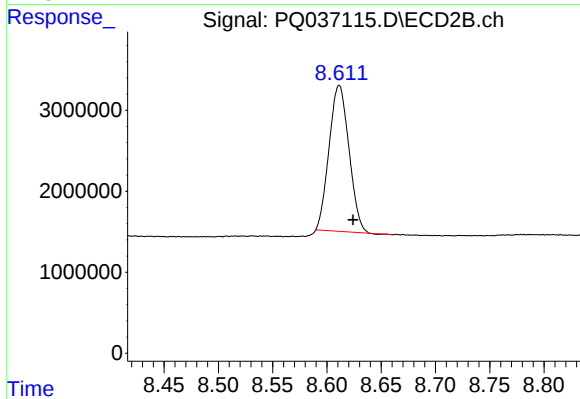

#2 Decachlorobiphenyl

R.T.: 8.611 min
Delta R.T.: -0.013 min
Response: 22976810
Conc: 12.23 ng/ml