

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ020819\
 Data File : PQ037123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2019 23:19
 Operator : SM\SJ
 Sample : K1404-08
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 A0C12-SS4-10.0-10.5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 00:24:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ020619.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Feb 06 18:32:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.300	3.686	-33683180	50103177	N.D.	21.695
2) SA Decachlor...	0.000	8.610	0	23816681	N.D.	12.676 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ020819\
Data File : PQ037123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2019 23:19
Operator : SM\SJ
Sample : K1404-08
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
A0C12-SS4-10.0-10.5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 00:24:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ020619.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Feb 06 18:32:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

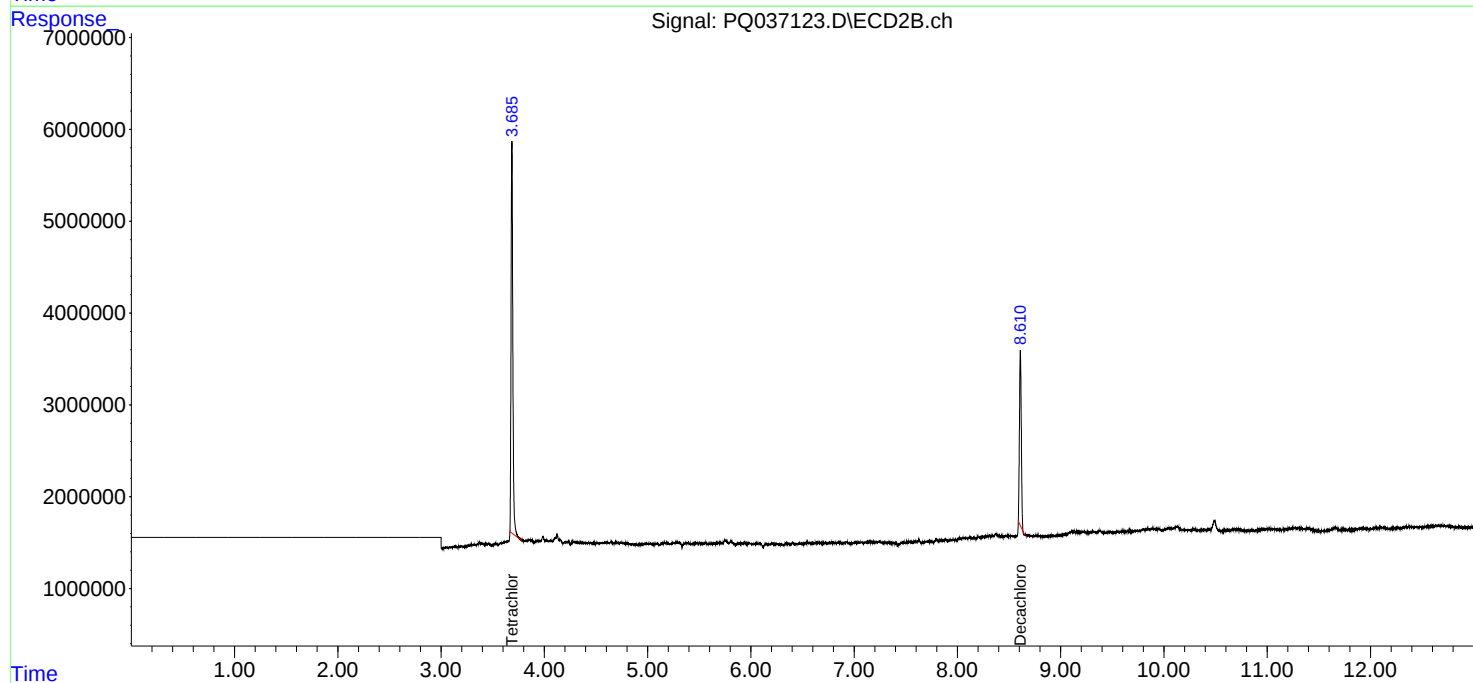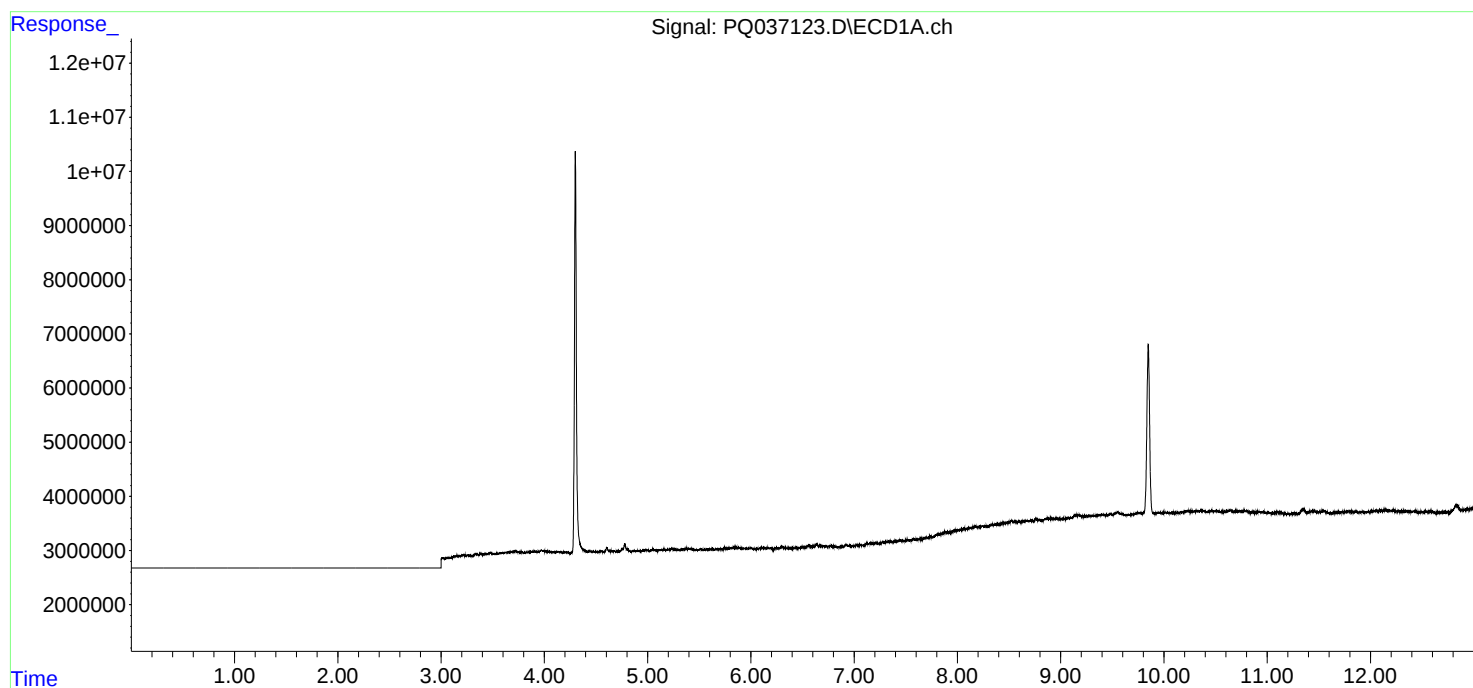


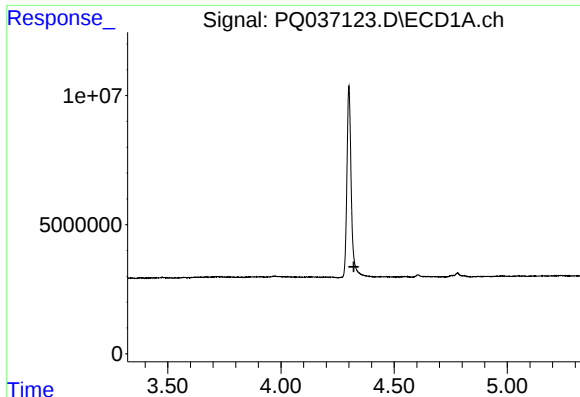

#1 Tetrachloro-m-xylene


R.T.: 4.300 min
Delta R.T.: -0.022 min
Response: -33683180
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
A0C12-SS4-10.0-10.5

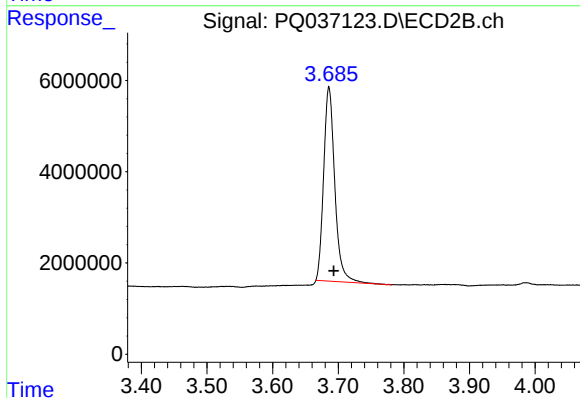


#1 Tetrachloro-m-xylene

R.T.: 3.686 min
Delta R.T.: -0.007 min
Response: 50103177
Conc: 21.69 ng/ml

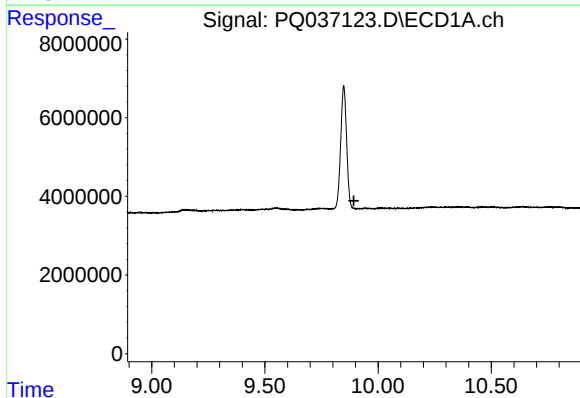

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.893 min
Response: 0
Conc: N.D.

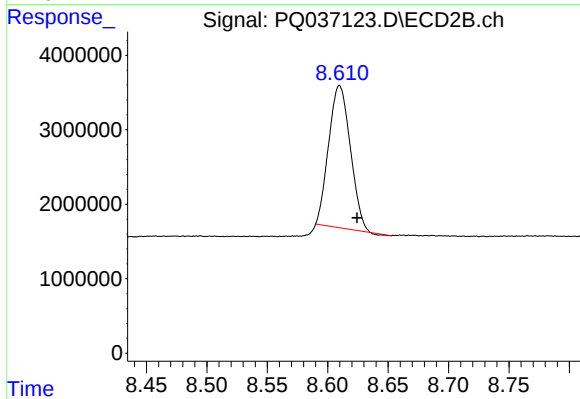

#2 Decachlorobiphenyl

R.T.: 8.610 min
Delta R.T.: -0.014 min
Response: 23816681
Conc: 12.68 ng/ml