

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ020821\
 Data File : PQ052108.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2021 05:01
 Operator : DD\AJ
 Sample : M1324-03 500X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 03-A-03-B-03-C

Manual Integrations
 APPROVED

Ankita
 2/9/2021 10:49:15 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 06:54:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ020821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 09 06:20:03 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
26)	L6	AR-1254-1	7.447f	6.397f	96921.9E6	51287.0E6 102750.653m 103912.025
27)	L6	AR-1254-2	7.672f	6.557f	73766.7E6	50752.2E6 50605.492m 119815.762 #
28)	L6	AR-1254-3	8.058f	6.980f	61120.9E6	68724.6E6 39412.157m 99920.060 #
29)	L6	AR-1254-4	8.383	7.213	67480.6E6	52382.6E6 64009.573 130632.398 #
30)	L6	AR-1254-5	8.776f	7.667f	103659.2E6	86208.1E6 89748.686m 148786.788m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ020821\
Data File : PQ052108.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2021 05:01
Operator : DD\AJ
Sample : M1324-03 500X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
2/9/2021 10:49:15 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 06:54:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ020821.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 09 06:20:03 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

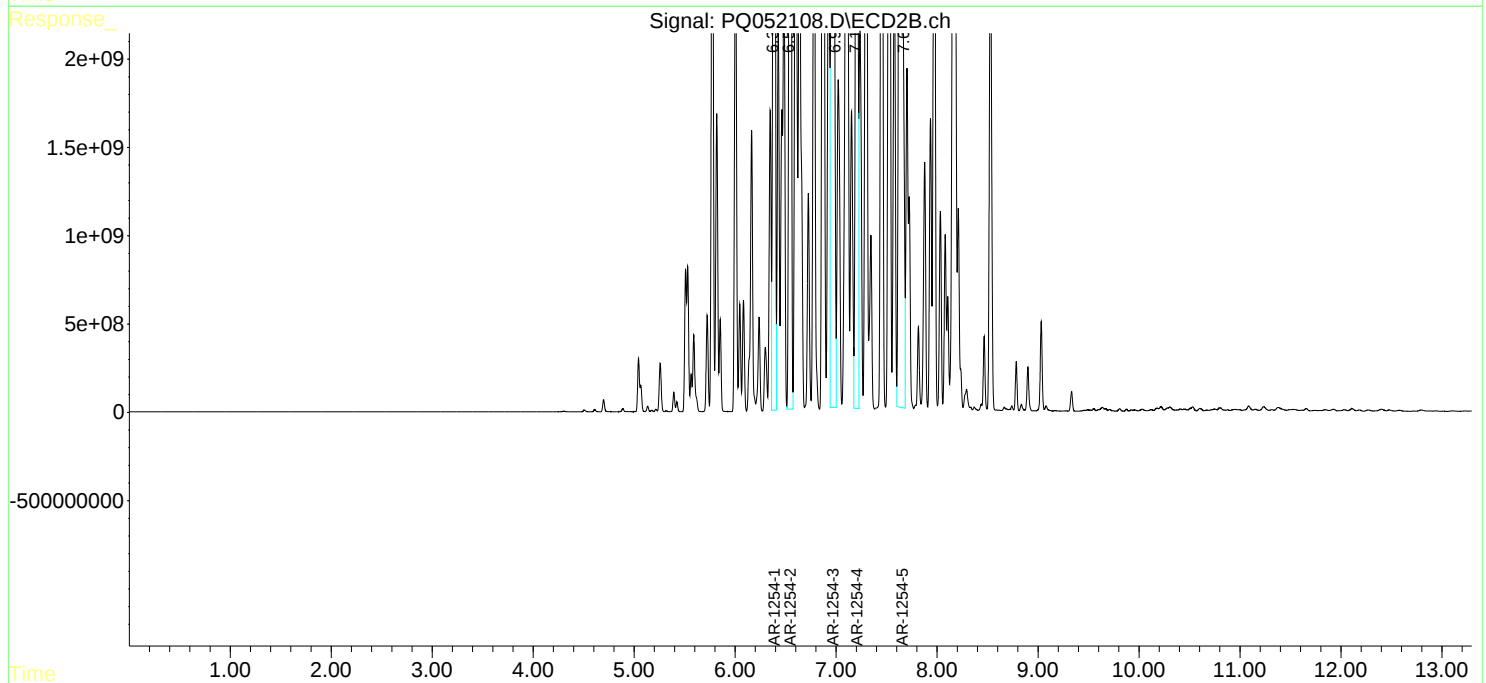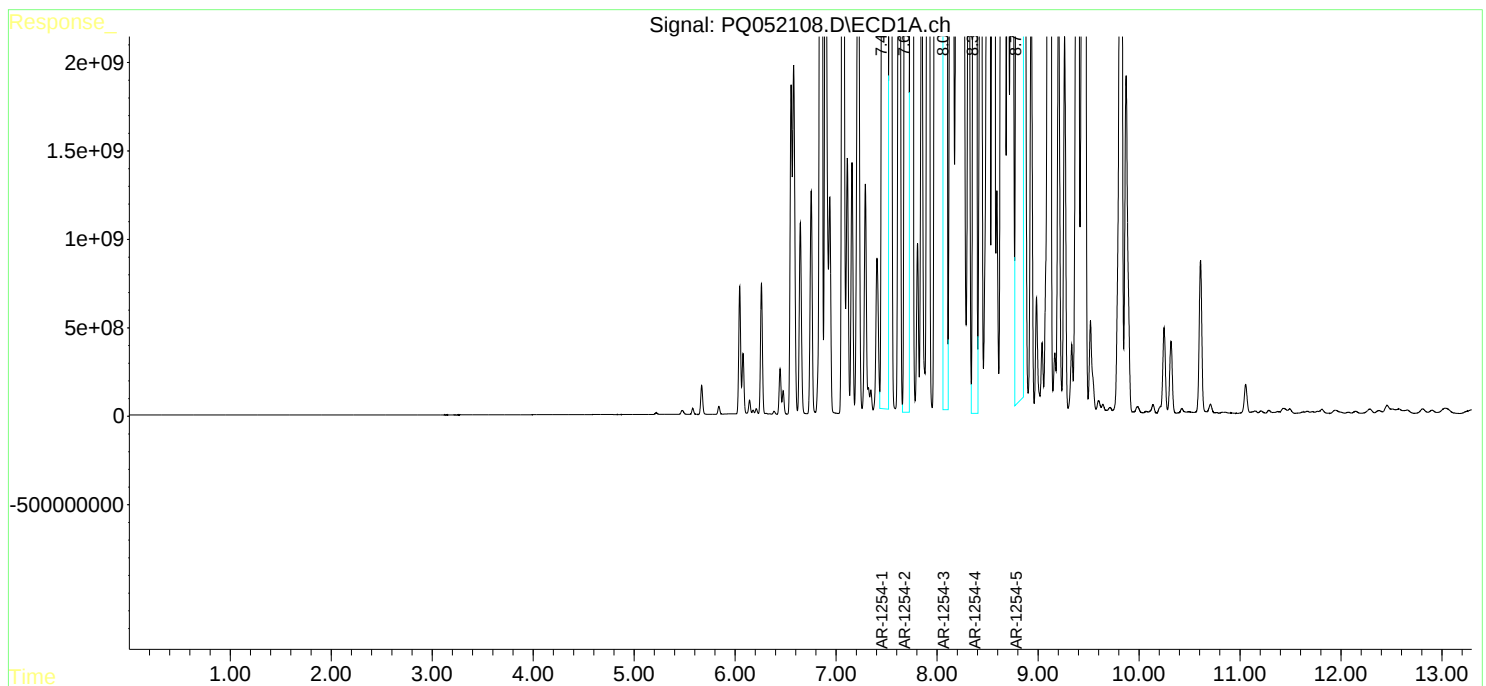

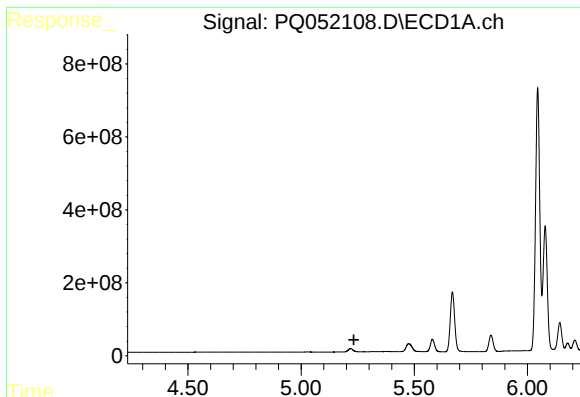


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.233 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
2/9/2021 10:49:15 AM

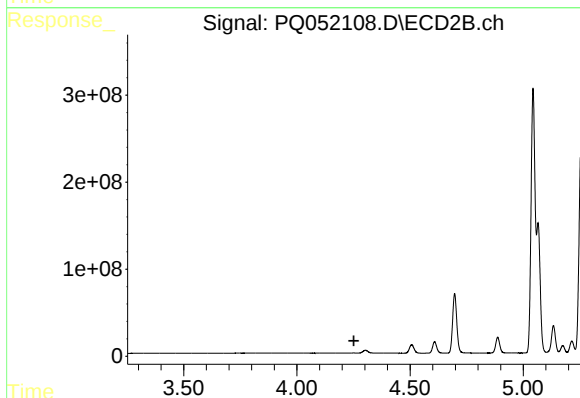


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.252 min
Response: 0
Conc: N.D.

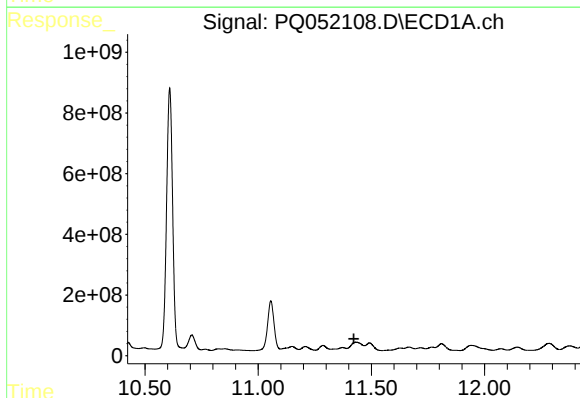


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.423 min
Response: 0
Conc: N.D.

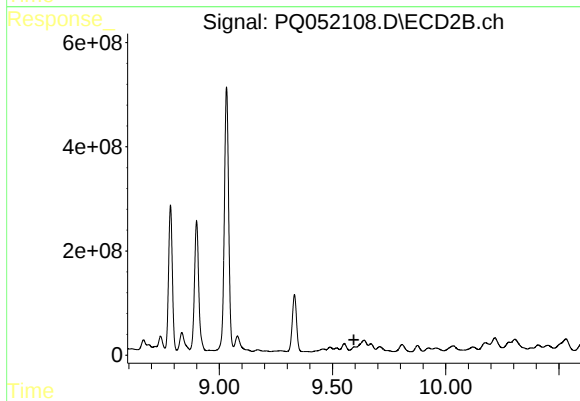

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.595 min
Response: 0
Conc: N.D.

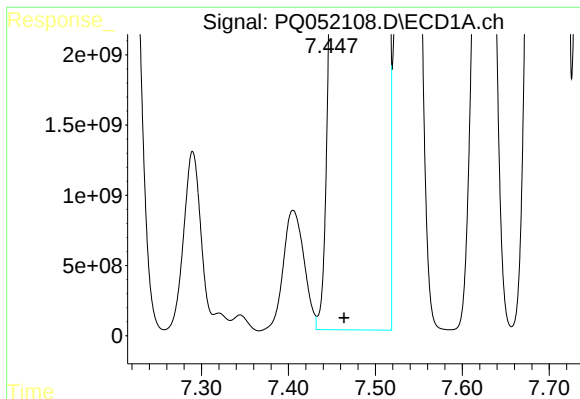


#26 AR-1254-1

R.T.: 7.447 min
Delta R.T.: -0.018 min
Response: 96921854827
Conc: 102750.65 ng/ml m

Instrument :
ECD_Q
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
2/9/2021 10:49:15 AM

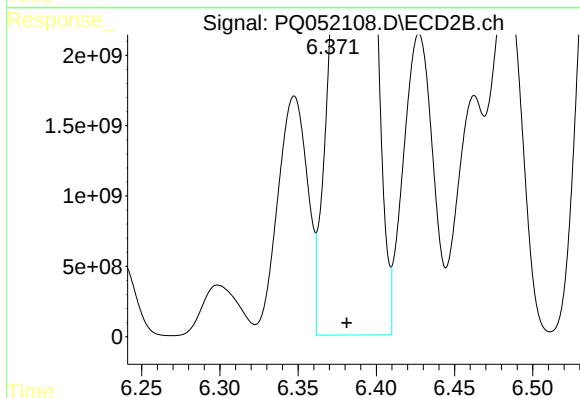


#26 AR-1254-1

R.T.: 6.397 min
Delta R.T.: 0.015 min
Response: 51286978811
Conc: 103912.03 ng/ml

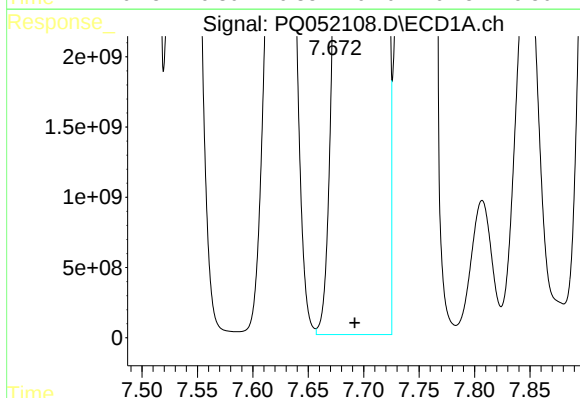


#27 AR-1254-2

R.T.: 7.672 min
Delta R.T.: -0.020 min
Response: 73766664931
Conc: 50605.49 ng/ml m

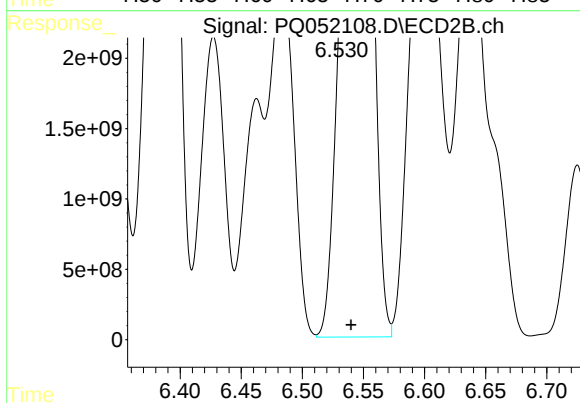

#27 AR-1254-2

R.T.: 6.557 min
Delta R.T.: 0.017 min
Response: 50752237502
Conc: 119815.76 ng/ml

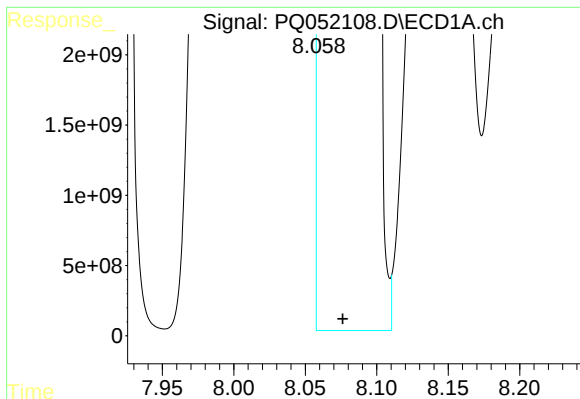


#28 AR-1254-3

R.T.: 8.058 min
Delta R.T.: -0.019 min
Response: 61120853475
Conc: 39412.16 ng/ml m

Instrument :
ECD_Q
ClientSampleId :
03-A-03-B-03-C


Manual Integrations
APPROVED

Ankita
2/9/2021 10:49:15 AM

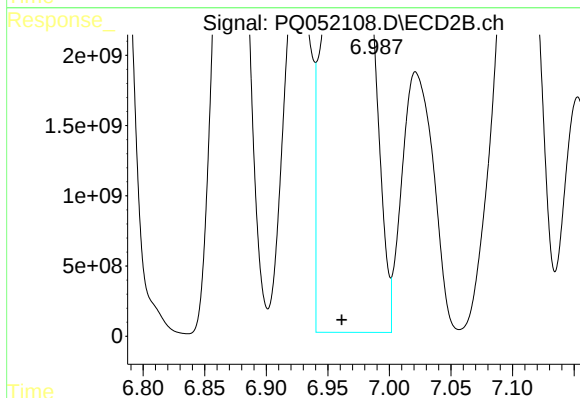


#28 AR-1254-3

R.T.: 6.980 min
Delta R.T.: 0.019 min
Response: 68724639889
Conc: 99920.06 ng/ml

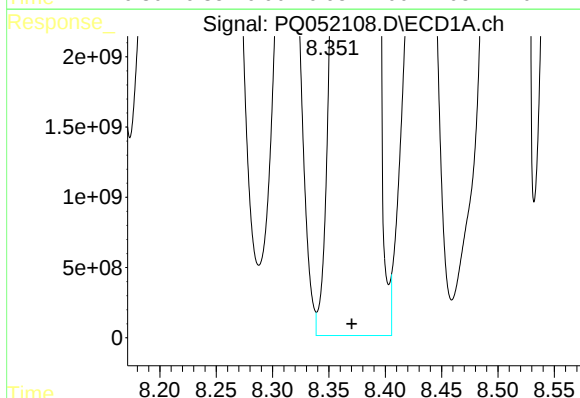


#29 AR-1254-4

R.T.: 8.383 min
Delta R.T.: 0.013 min
Response: 67480620175
Conc: 64009.57 ng/ml

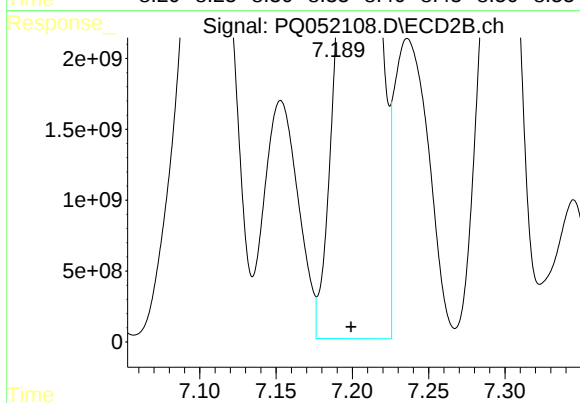

#29 AR-1254-4

R.T.: 7.213 min
Delta R.T.: 0.014 min
Response: 52382597791
Conc: 130632.40 ng/ml

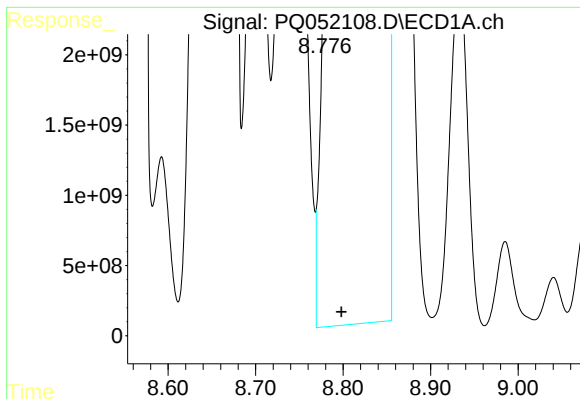


#30 AR-1254-5

R.T.: 8.776 min
Delta R.T.: -0.022 min
Response: 1.03659e+011
Conc: 89748.69 ng/ml m

Instrument :
ECD_Q
ClientSampleId :
03-A-03-B-03-C

Manual Integrations
APPROVED

Ankita
2/9/2021 10:49:15 AM

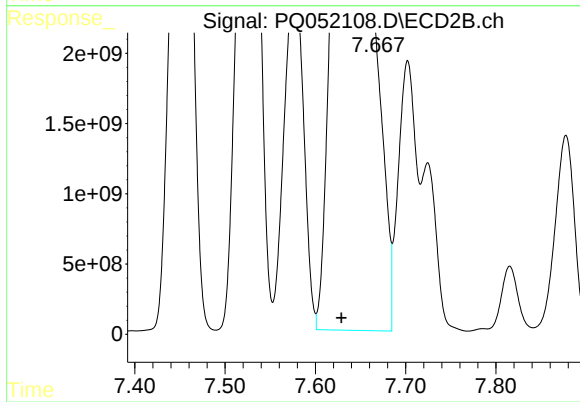

#30 AR-1254-5

R.T.: 7.667 min
Delta R.T.: 0.038 min
Response: 86208083931
Conc: 148786.79 ng/ml m