

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ020824\
 Data File : PQ065344.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2024 23:52
 Operator : YP\AJ
 Sample : P1413-03
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 ETGI-347

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/09/2024
 Supervised By :Sohil Jodhani 02/09/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 00:50:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ011724.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 18 00:09:27 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.471	2.740	62026661	131.3E6	16.650m	19.661
2) SA Decachlor...	8.784	7.514	52229998	94372352	16.900	12.986m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ020824\
Data File : PQ065344.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2024 23:52
Operator : YP\AJ
Sample : P1413-03
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
ETGI-347


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/09/2024
Supervised By :Sohil Jodhani 02/09/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 00:50:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ011724.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 18 00:09:27 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

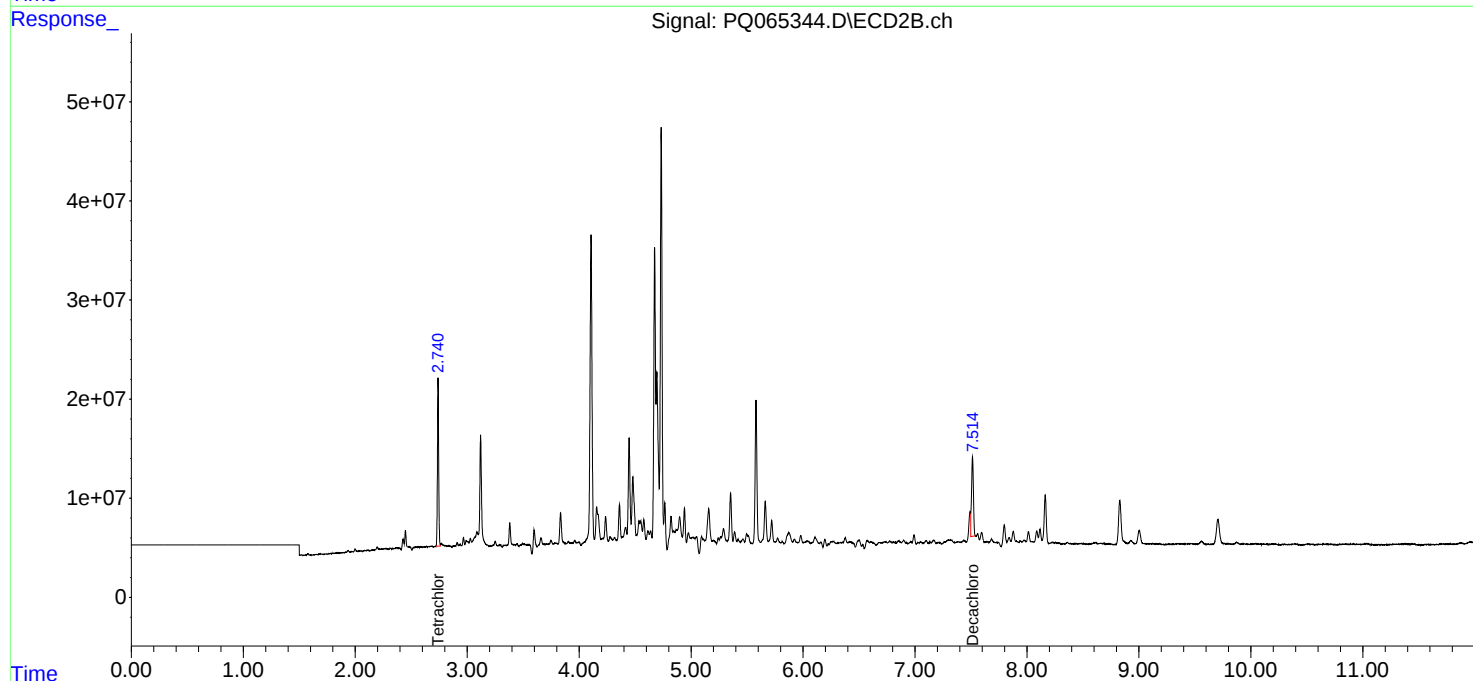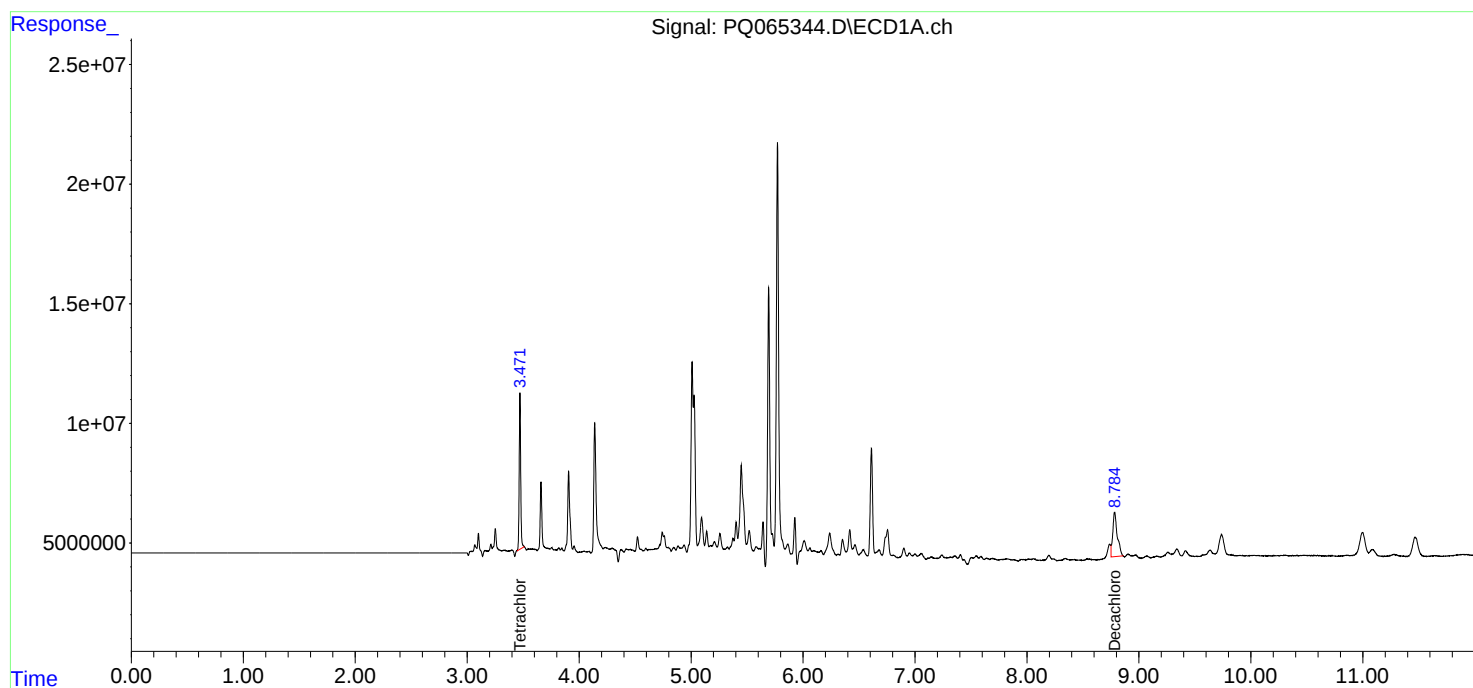

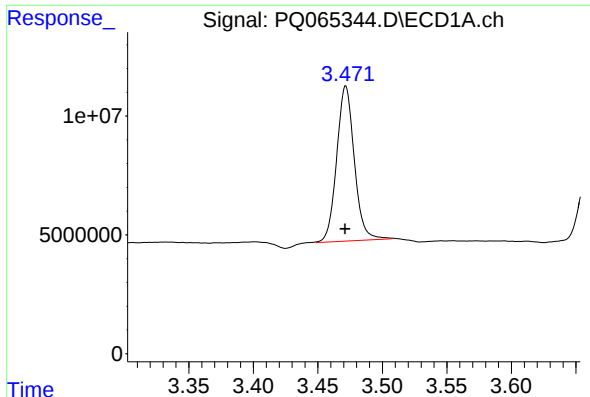


#1 Tetrachloro-m-xylene

R.T.: 3.471 min
Delta R.T.: 0.000 min
Response: 62026661
Conc: 16.65 ng/ml

Instrument :
ECD_Q
ClientSampleId :
ETGI-347


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/09/2024
Supervised By :Sohil Jodhani 02/09/2024

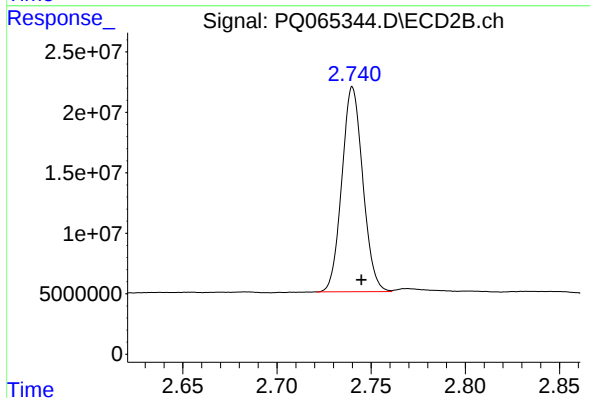


#1 Tetrachloro-m-xylene

R.T.: 2.740 min
Delta R.T.: -0.005 min
Response: 131289024
Conc: 19.66 ng/ml

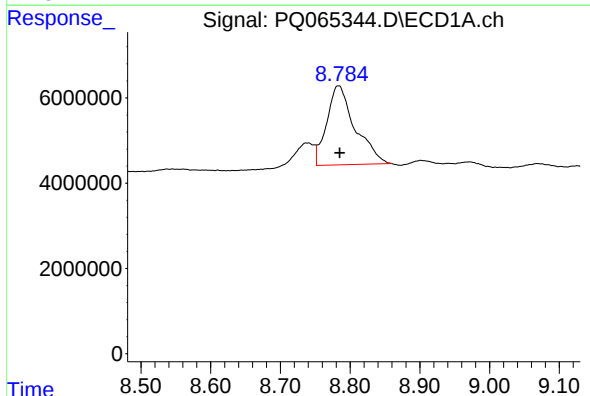

#2 Decachlorobiphenyl

R.T.: 8.784 min
Delta R.T.: -0.001 min
Response: 52229998
Conc: 16.90 ng/ml

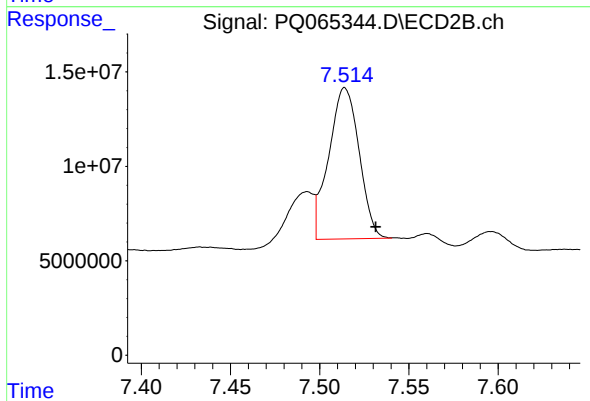

#2 Decachlorobiphenyl

R.T.: 7.514 min
Delta R.T.: -0.018 min
Response: 94372352
Conc: 12.99 ng/ml m