

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ020924\
 Data File : PQ065363.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2024 11:16
 Operator : YP\AJ
 Sample : P1413-05RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 ETGI-358RE

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 02/12/2024
 Supervised By :Sohil Jodhani 02/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 21:51:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ011724.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 18 00:09:27 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.472	2.740	66318142	134.2E6	17.802m	20.104
2) SA Decachlor...	8.785	7.562f	166.7E6	261.4E6	53.933	35.964m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ020924\
Data File : PQ065363.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2024 11:16
Operator : YP\AJ
Sample : P1413-05RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
ETGI-358RE


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/12/2024
Supervised By :Sohil Jodhani 02/12/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 21:51:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ011724.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 18 00:09:27 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

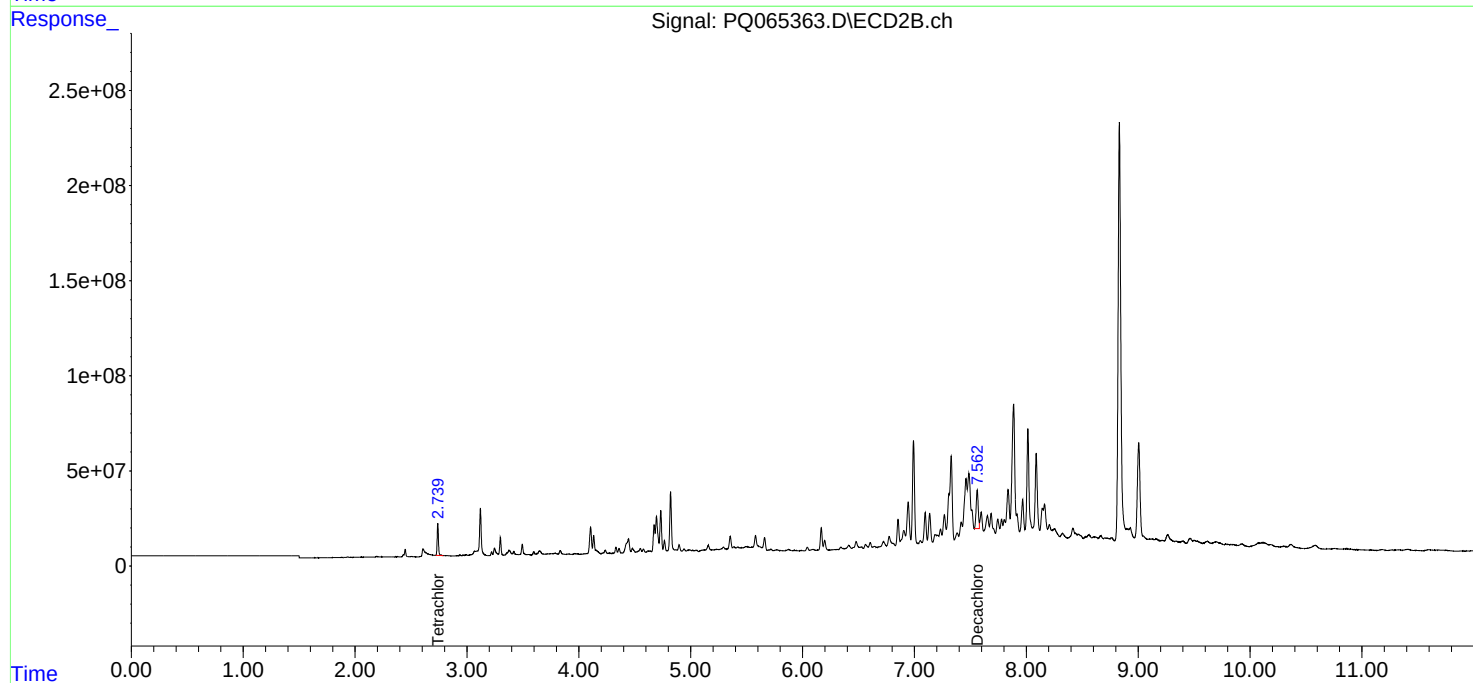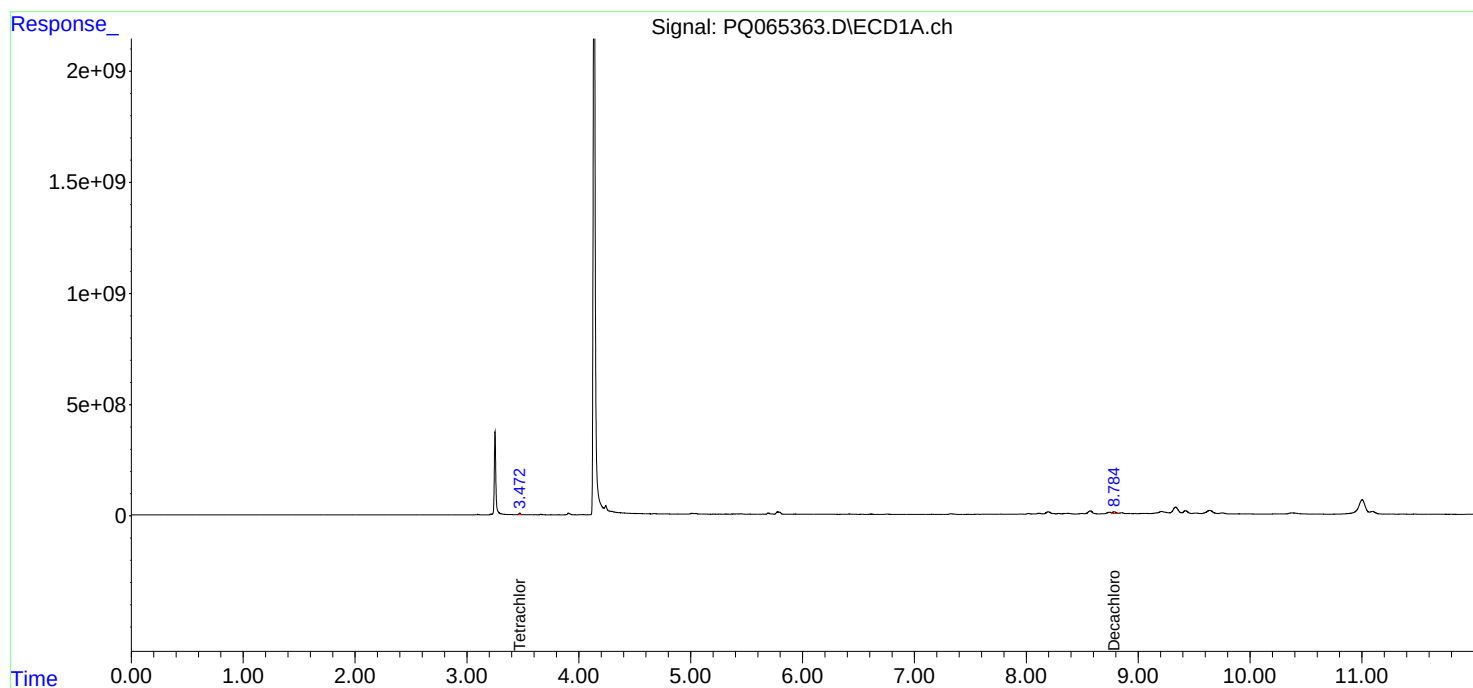

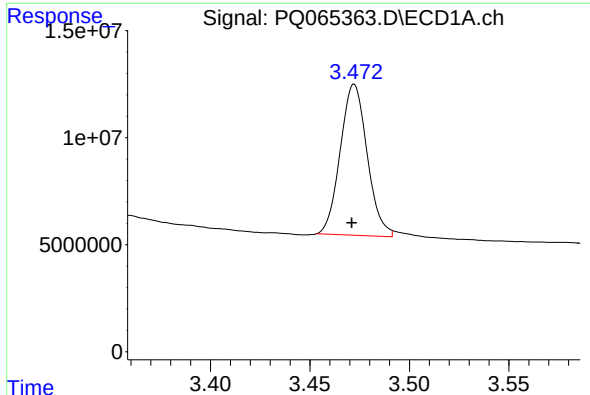


#1 Tetrachloro-m-xylene

R.T.: 3.472 min
Delta R.T.: 0.000 min
Response: 66318142
Conc: 17.80 ng/ml

Instrument :
ECD_Q
ClientSampleId :
ETGI-358RE


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 02/12/2024
Supervised By :Sohil Jodhani 02/12/2024

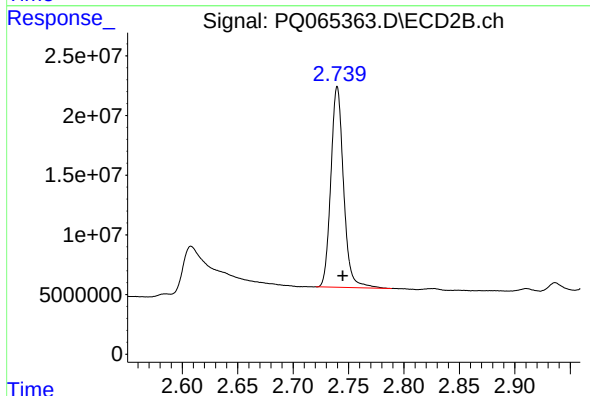


#1 Tetrachloro-m-xylene

R.T.: 2.740 min
Delta R.T.: -0.005 min
Response: 134248206
Conc: 20.10 ng/ml

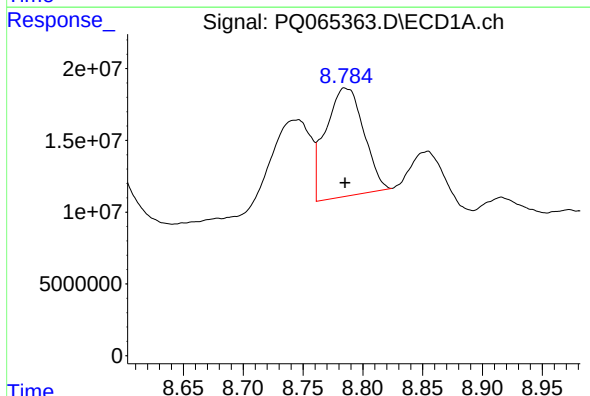

#2 Decachlorobiphenyl

R.T.: 8.785 min
Delta R.T.: 0.000 min
Response: 166677955
Conc: 53.93 ng/ml

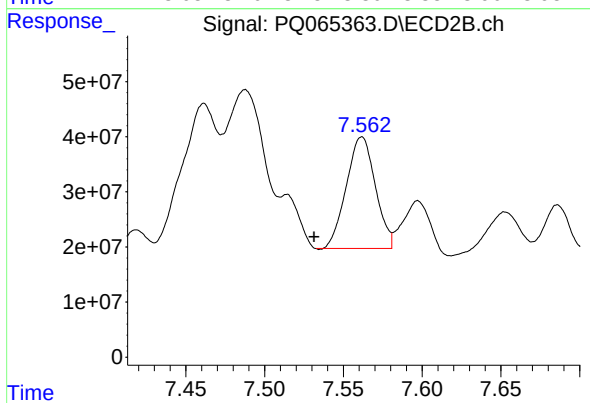

#2 Decachlorobiphenyl

R.T.: 7.562 min
Delta R.T.: 0.030 min
Response: 261365695
Conc: 35.96 ng/ml m