

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ030619\
 Data File : PQ037814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2019 12:12
 Operator : SM\SJ
 Sample : PB117625BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1



Instrument :
 ECD_Q
 ClientSampleId :
 ALCS25

Manual Integrations
 APPROVED

Sohil
 3/8/2019 2:37:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 01:07:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ022619CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 26 04:57:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

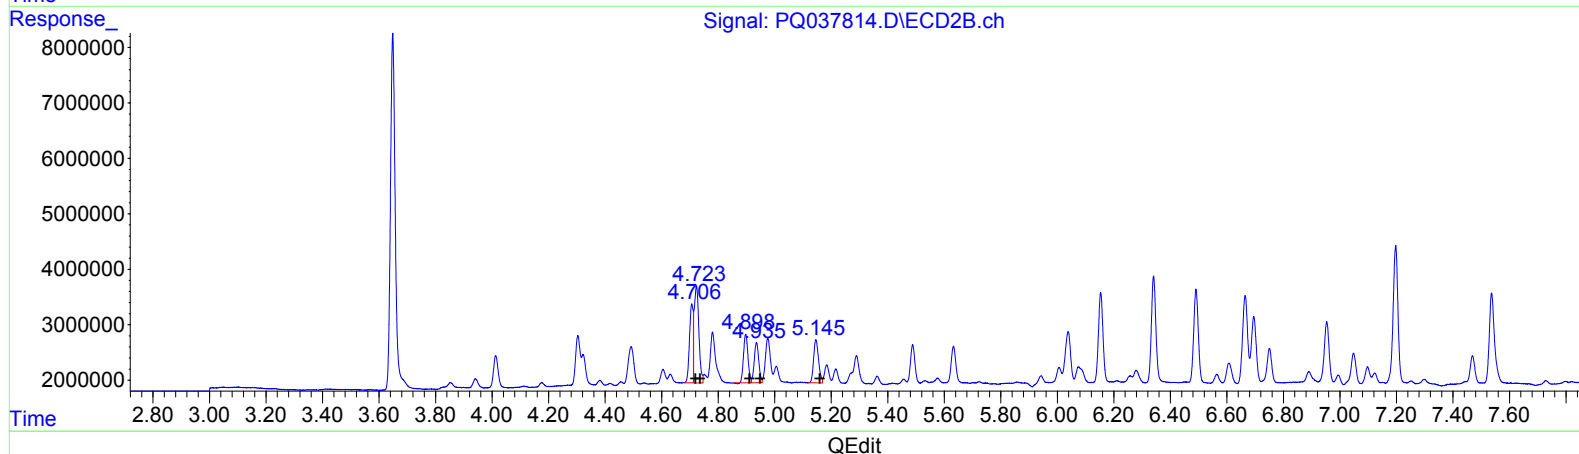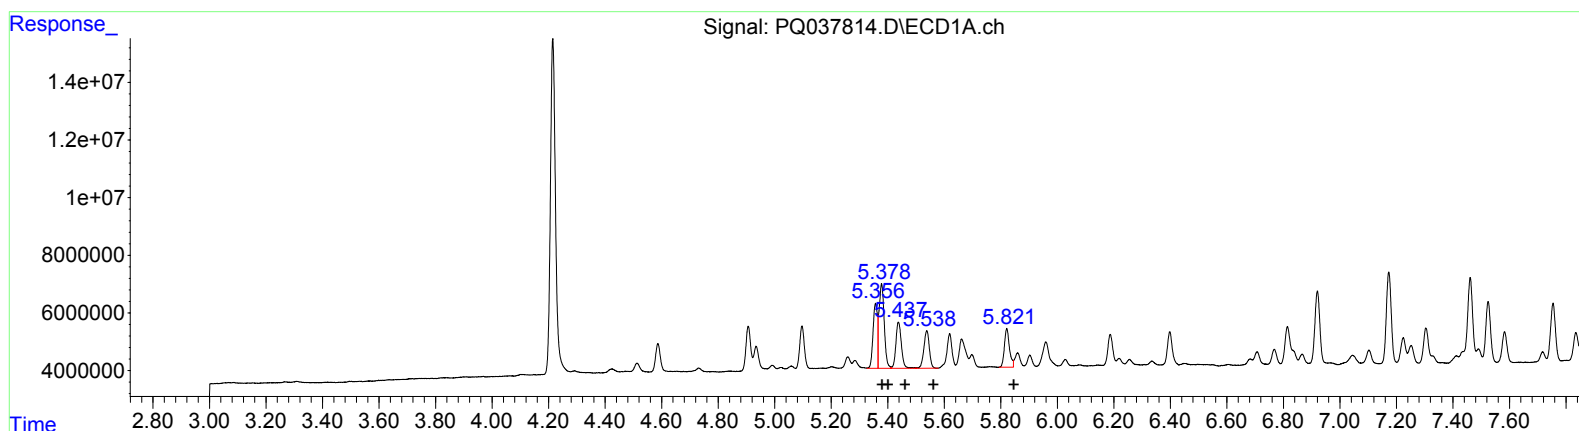

(3) AR-1016-1 #2 (L1)
 R.T. Response Conc
 5.36 24691048 85.43
 5.38 37543846 84.01
 5.44 21661003 82.41
 5.54 17519339 79.69
 5.82 16713448 77.75

(3) AR-1016-1 #2 (L1)
 R.T. Response Conc
 4.71 12875853 83.46
 4.72 19946177 83.09
 4.90 9608865 78.91
 4.94 8111581 86.85
 5.15 9417166 75.18

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ030619\
Data File : PQ037814.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2019 12:12
Operator : SM\SJ
Sample : PB117625BS
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampled :
ALCS25

Manual Integrations
APPROVED

Sohil
3/8/2019 2:37:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 01:07:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ022619CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 26 04:57:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

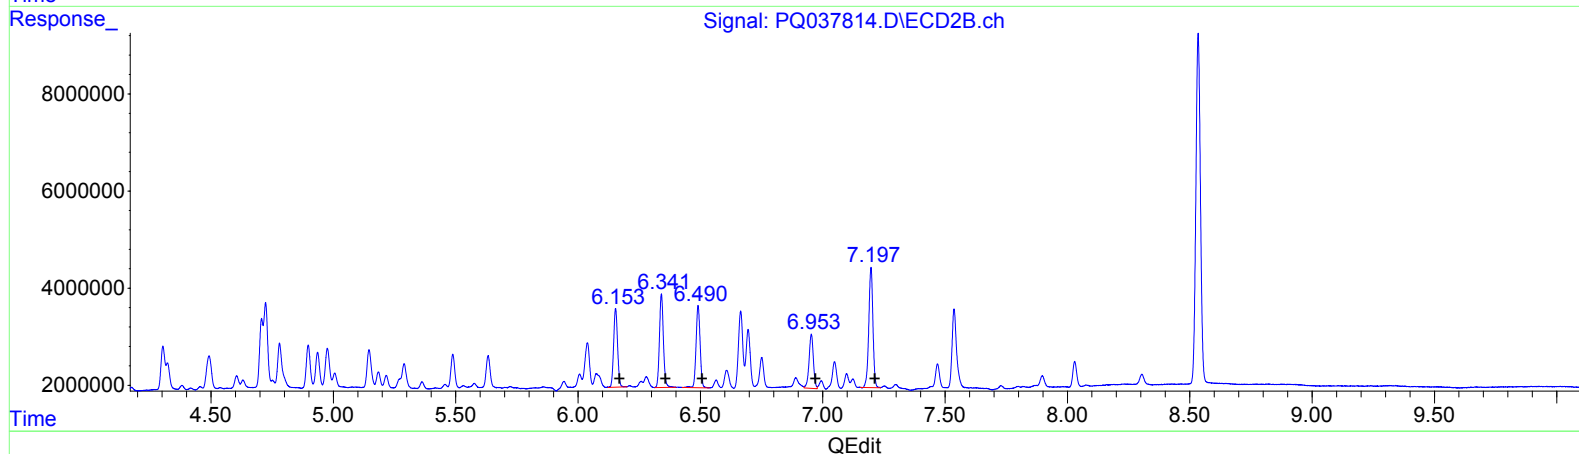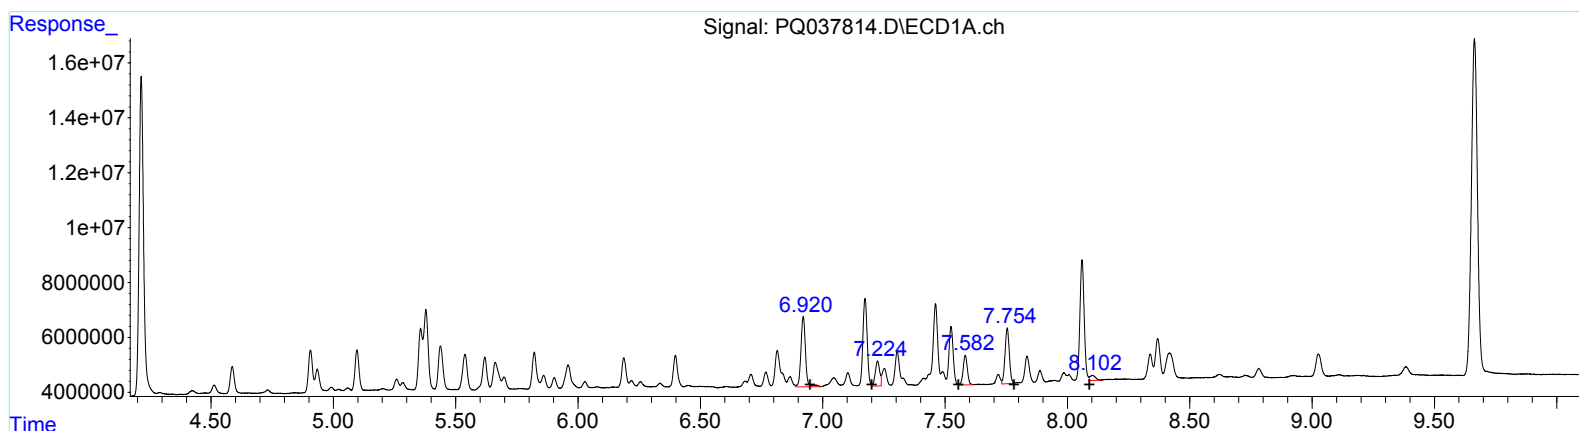

(31) AR-1260-1 (L7)
R.T. Response Conc
6.92 33420217 75.22
7.22 11371576 19.67
7.58 12912339 28.90
7.75 24693750 56.38
8.10 2955496 2.95

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
6.15 18129872 71.51
6.34 21570734 70.18
6.49 19462540 68.54
6.95 13640180 61.97
7.20 29270040 55.44

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ030619\
Data File : PQ037814.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2019 12:12
Operator : SM\SJ
Sample : PB117625BS
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
ALCS25

Manual Integrations
APPROVED

Sohil
3/8/2019 2:37:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 01:07:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ022619CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 26 04:57:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

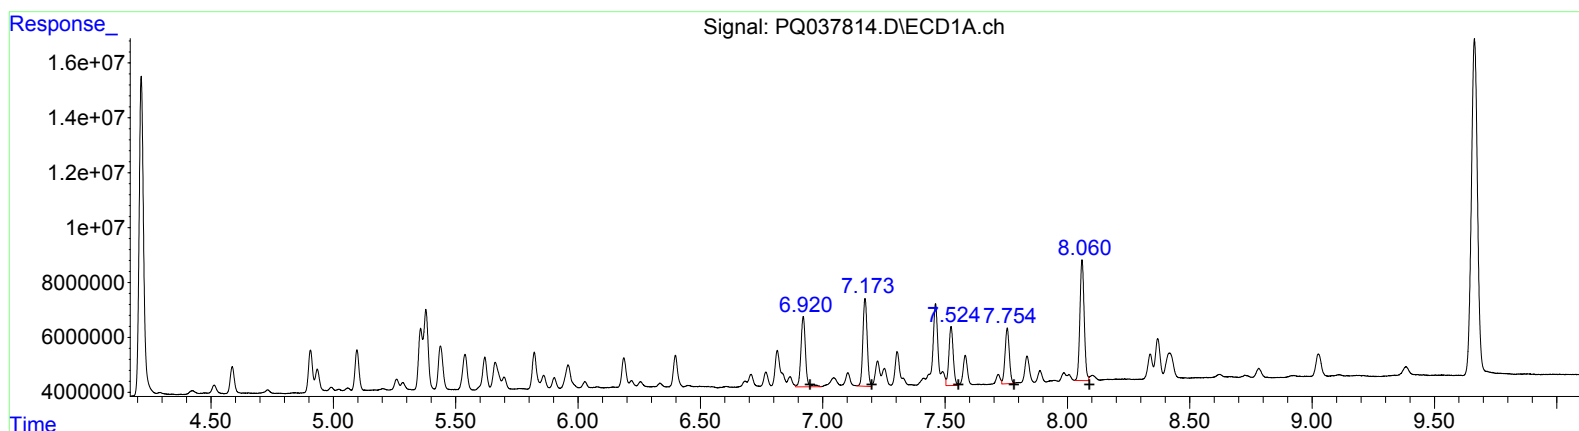

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
6.92 33420217 75.22
7.17 39273598 67.92
7.52 26434009 59.17
7.75 24693750 56.38
8.06 53687891 53.56

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
6.15 18129872 71.51
6.34 21570734 70.18
6.49 19462540 68.54
6.95 13640180 61.97
7.20 29270040 55.44

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ030619\
 Data File : PQ037814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2019 12:12
 Operator : SM\SJ
 Sample : PB117625BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1



Instrument :
 ECD_Q
 ClientSampleId :
 ALCS25

Manual Integrations
 APPROVED

Sohil
 3/8/2019 2:37:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 01:07:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ022619CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 26 04:57:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

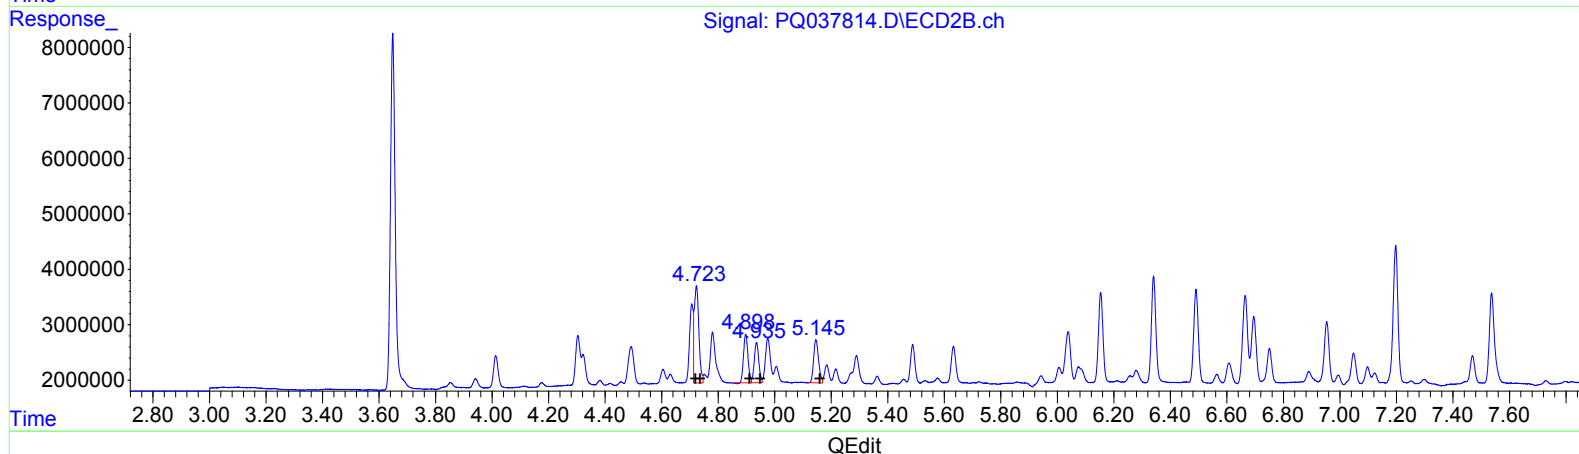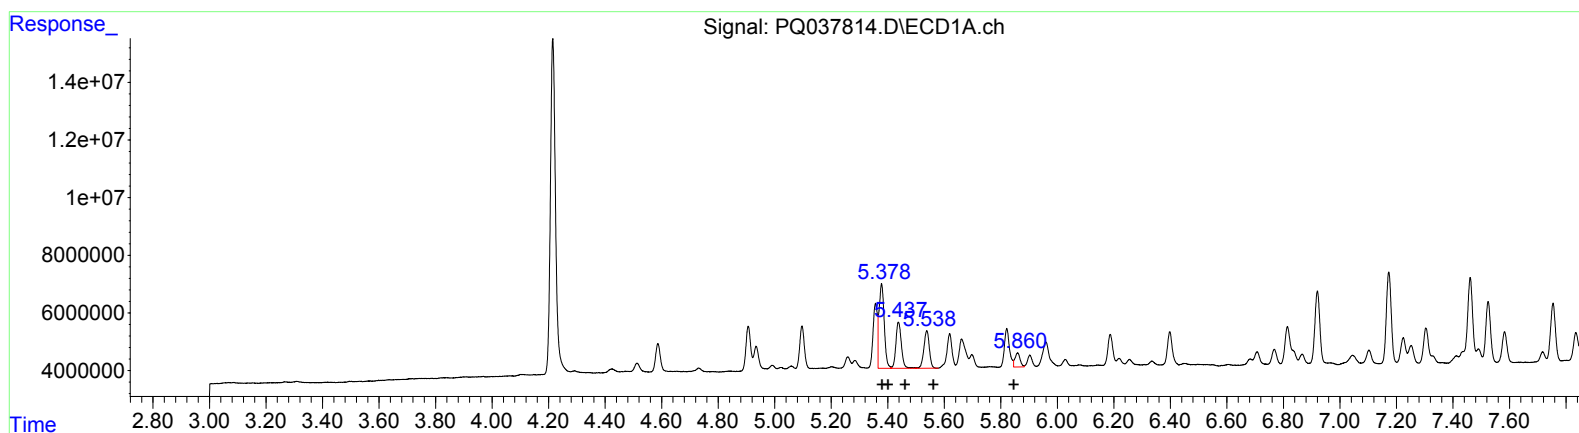

(3) AR-1016-1 (L1)

R.T.	Response	Conc
5.38	37543846	129.90
5.38	37543846	84.01
5.44	21661003	82.41
5.54	17519339	79.69
5.86	6191629	28.80

(3) AR-1016-1 #2 (L1)

R.T.	Response	Conc
4.72	19946177	129.29
4.72	19946177	83.09
4.90	9608865	78.91
4.94	8111581	86.85
5.15	9417166	75.18

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ030619\
 Data File : PQ037814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2019 12:12
 Operator : SM\SJ
 Sample : PB117625BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_Q
 Client Sampled :
 ALCS25

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 01:07:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ022619CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 26 04:57:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Manual Integrations
 APPROVED

Sohil
 3/8/2019 2:37:33 PM

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.215	3.649	146.1E6	76703365	25.676	29.120
2) SA Decachlor...	9.664	8.534	215.2E6	93821345	42.607	40.440
Target Compounds						
3) L1 AR-1016-1	5.356	4.706	24691048	12875853	85.429m	83.458m
4) L1 AR-1016-2	5.378	4.723	37543846	19946177	84.013	83.094
5) L1 AR-1016-3	5.438	4.897	21661003	9608865	82.413	78.911
6) L1 AR-1016-4	5.538	4.936	17519339	8111581	79.687	86.853
7) L1 AR-1016-5	5.821	5.146	16713448	9417166	77.753m	75.183
31) L7 AR-1260-1	6.920	6.154	33420217	18129872	75.216	71.509
32) L7 AR-1260-2	7.173	6.341	39273598	21570734	67.924m	70.178
33) L7 AR-1260-3	7.524	6.491	26434009	19462540	59.171m	68.535
34) L7 AR-1260-4	7.754	6.953	24693750	13640180	56.379	61.975
35) L7 AR-1260-5	8.060	7.197	53687891	29270040	53.562m	55.437

3.7
 03/07/19

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.