

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031022\
 Data File : PD068447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Mar 2022 08:55
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 22:39:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 01 06:48:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.174	26095699	217.2E6	22.261	22.632
28)	SA Decachlor...	8.210	9.369	28499226	134.5E6	24.490	22.689
Target Compounds							
2)	A alpha-BHC	0.000	4.560	0	1311070	N.D.	0.096 #
7)	B delta-BHC	0.000	5.231f	0	1966176	N.D.	0.158 #
8)	B Heptachlo...	0.000	6.070f	0	362847	N.D.	0.034 #
10)	B gamma-Chl...	0.000	6.318	0	1661475	N.D.	0.157 #
21)	B Endrin ke...	0.000	7.967	0	1414352	N.D.	0.168 #
22)	Mirex	7.363f	8.443f	156093	179394	0.123	0.028 #
23)	Chlordane-1	4.346f	0.000	162471	0	3.724	N.D. #
24)	Chlordane-2	0.000	5.672	0	250088	N.D.	0.622 #
25)	Chlordane-3	0.000	6.318	0	1661475	N.D.	1.168 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD031022\
Data File : PD068447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Mar 2022 08:55
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 22:39:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD030122.M
Quant Title : GC Extractables
QLast Update : Tue Mar 01 06:48:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

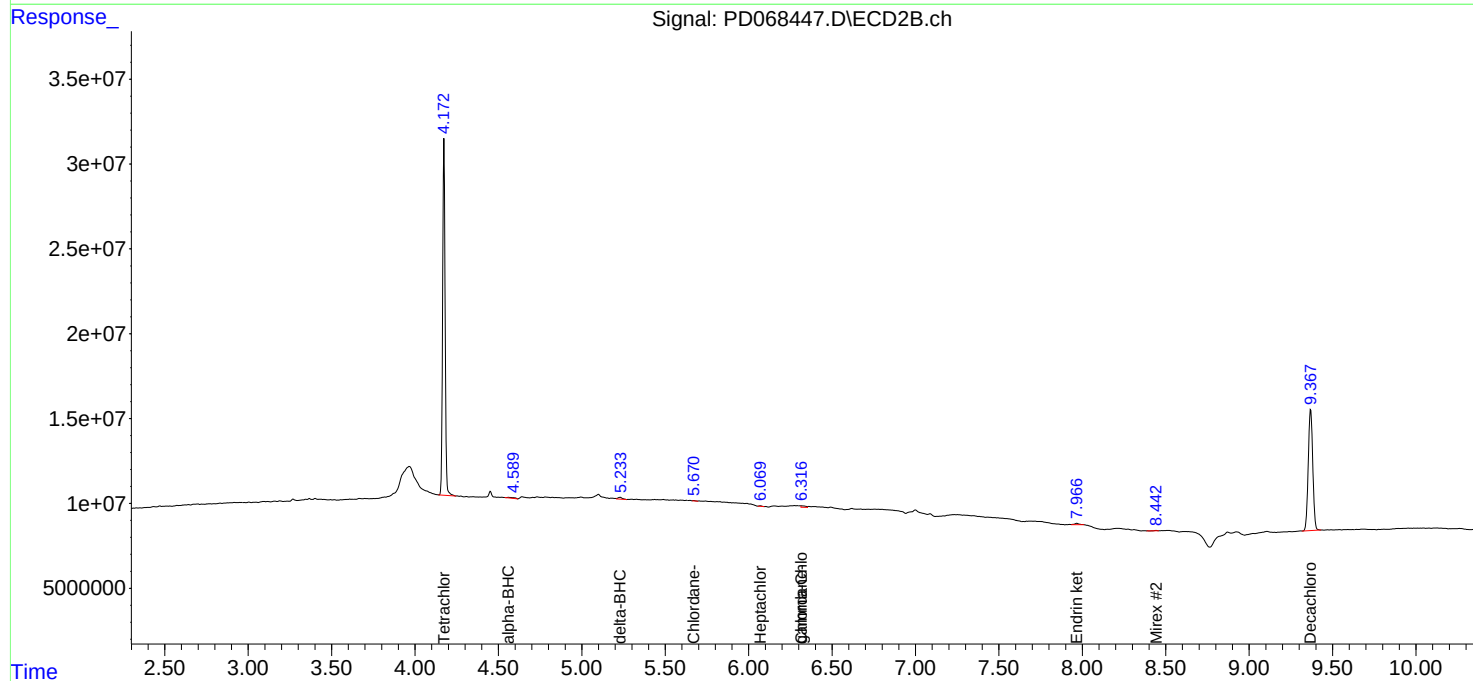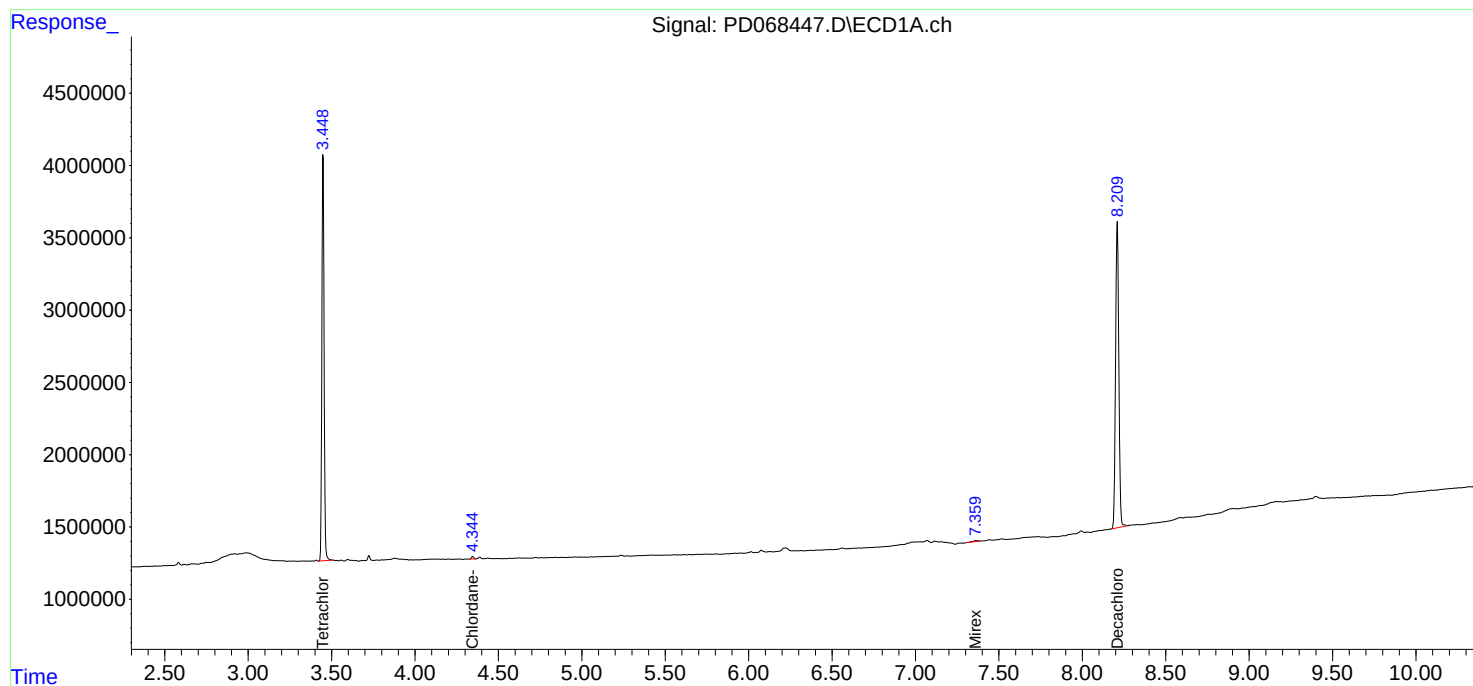


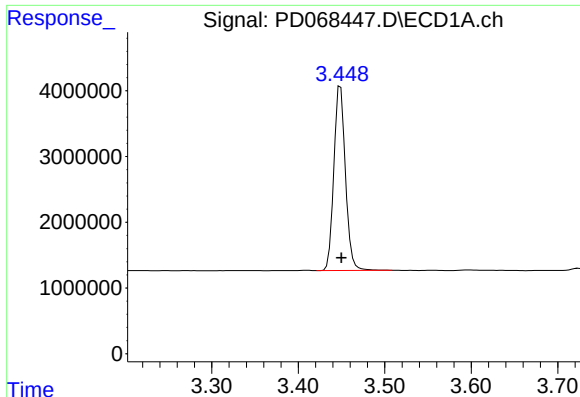

#1 Tetrachloro-m-xylene


R.T.: 3.449 min
Delta R.T.: -0.001 min
Response: 26095699
Conc: 22.26 ng/ml

Instrument :
ECD_Q
ClientSampleId :

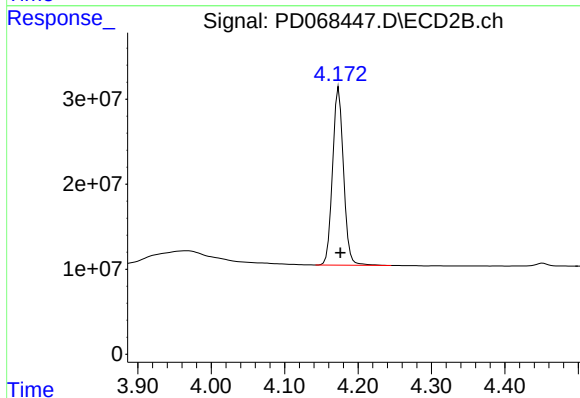


#1 Tetrachloro-m-xylene

R.T.: 4.174 min
Delta R.T.: -0.002 min
Response: 217220857
Conc: 22.63 ng/ml

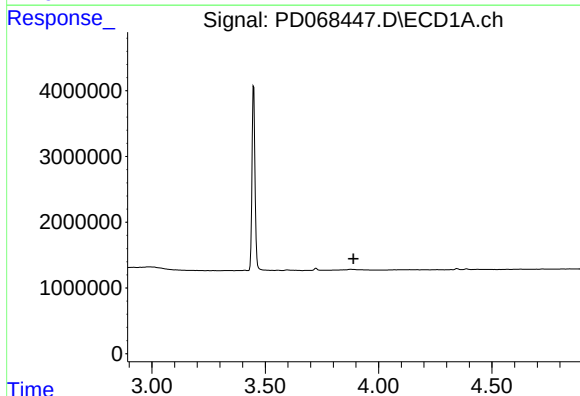


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.890 min
Response: 0
Conc: N.D.

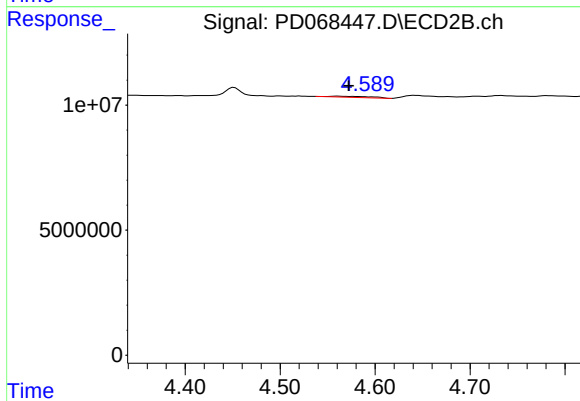

#2 alpha-BHC

R.T.: 4.560 min
Delta R.T.: -0.012 min
Response: 1311070
Conc: 0.10 ng/ml

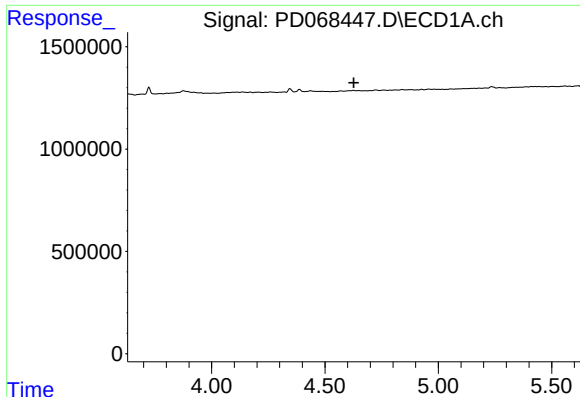

#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.628 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :

#7 delta-BHC


R.T.: 5.231 min
Delta R.T.: -0.020 min
Response: 1966176
Conc: 0.16 ng/ml

#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.165 min
Response: 0
Conc: N.D.

#8 Heptachlor epoxide


R.T.: 6.070 min
Delta R.T.: -0.021 min
Response: 362847
Conc: 0.03 ng/ml

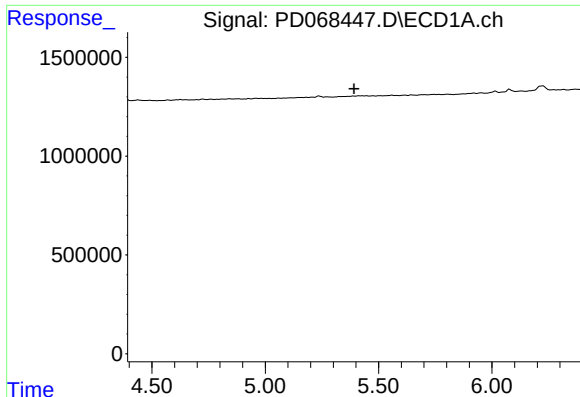

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :

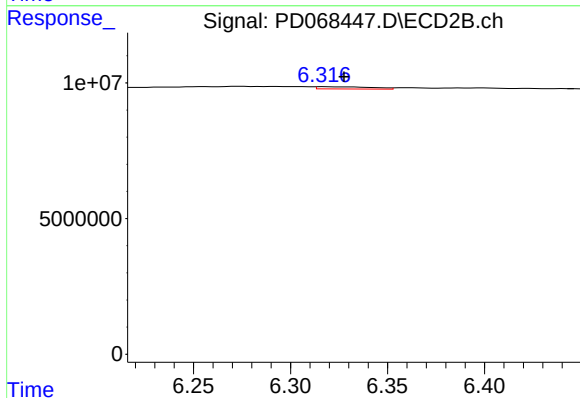


#10 gamma-Chlordane

R.T.: 6.318 min
Delta R.T.: -0.009 min
Response: 1661475
Conc: 0.16 ng/ml

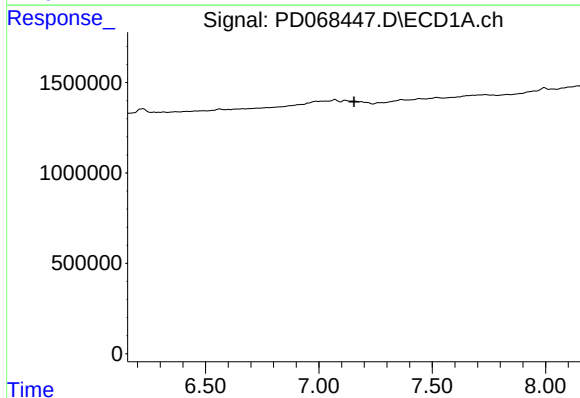


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.155 min
Response: 0
Conc: N.D.

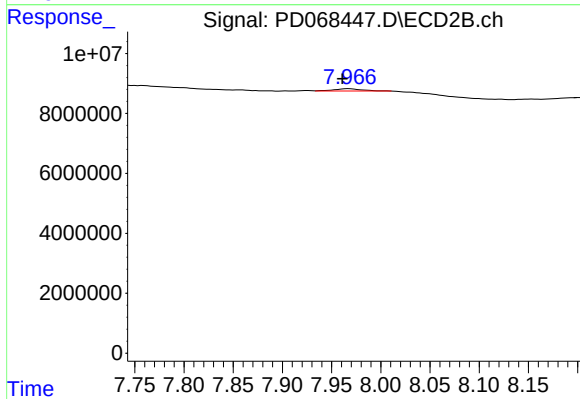

#21 Endrin ketone


R.T.: 7.967 min
Delta R.T.: 0.006 min
Response: 1414352
Conc: 0.17 ng/ml

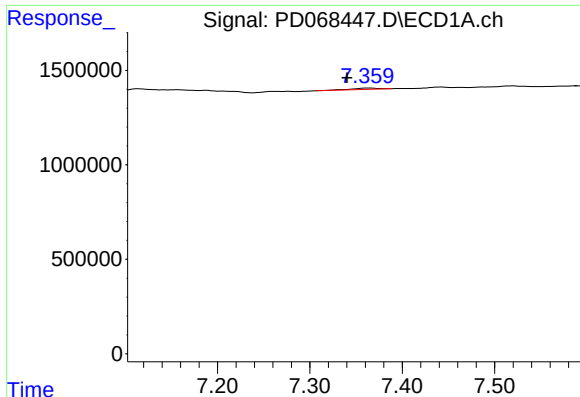

#22 Mirex

R.T.: 7.363 min
Delta R.T.: 0.023 min
Response: 156093
Conc: 0.12 ng/ml

Instrument :
ECD_Q
ClientSampleId :

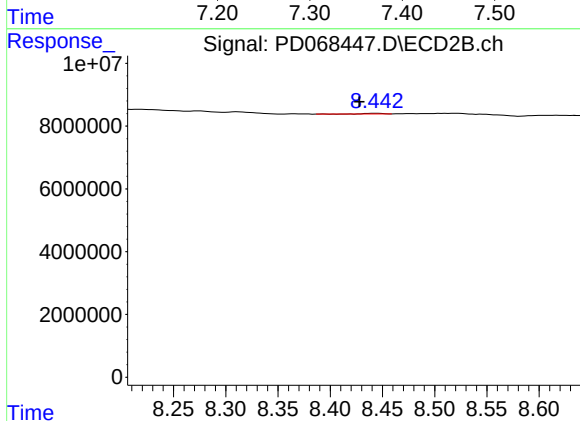

#22 Mirex


R.T.: 8.443 min
Delta R.T.: 0.016 min
Response: 179394
Conc: 0.03 ng/ml

#23 Chlordane-1

R.T.: 4.346 min
Delta R.T.: 0.025 min
Response: 162471
Conc: 3.72 ng/ml

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.199 min
Response: 0
Conc: N.D.

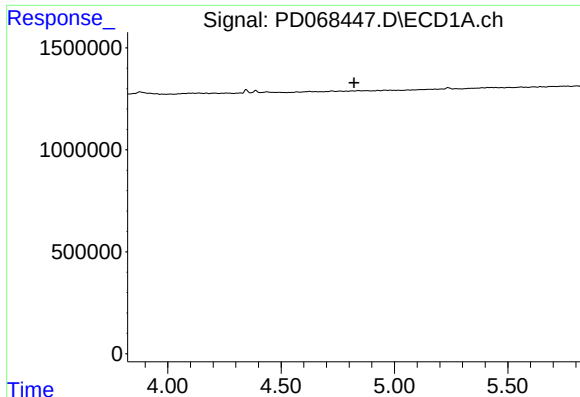

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.822 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :

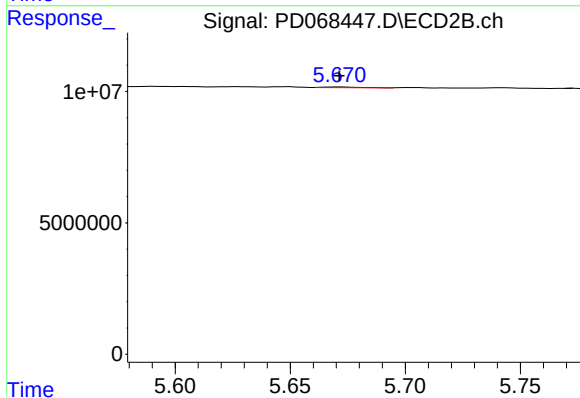


#24 Chlordane-2

R.T.: 5.672 min
Delta R.T.: 0.000 min
Response: 250088
Conc: 0.62 ng/ml

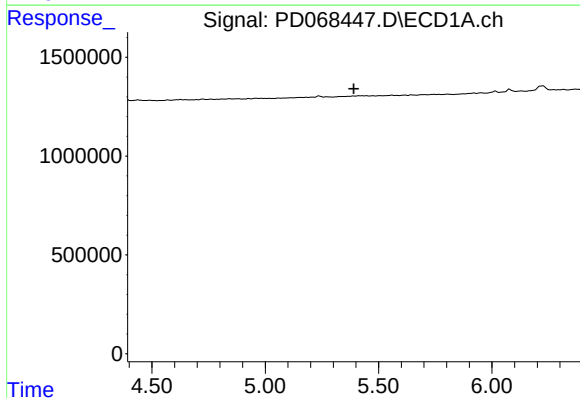


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.391 min
Response: 0
Conc: N.D.

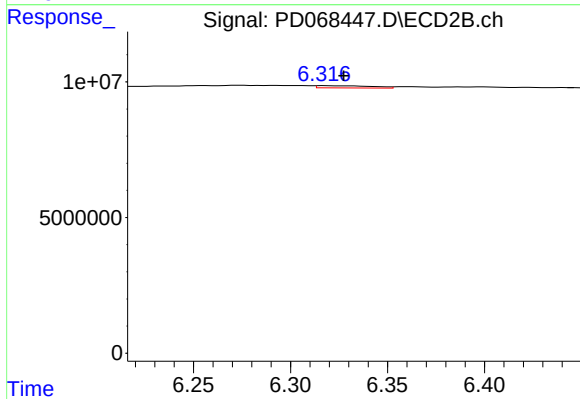

#25 Chlordane-3


R.T.: 6.318 min
Delta R.T.: -0.009 min
Response: 1661475
Conc: 1.17 ng/ml

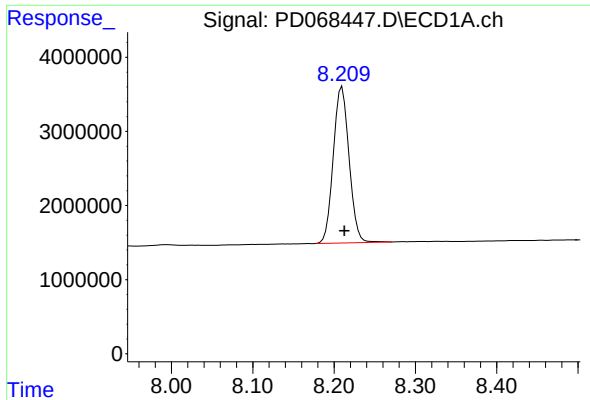

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: -0.003 min
Response: 28499226
Conc: 24.49 ng/ml

Instrument :
ECD_Q
ClientSampleId :

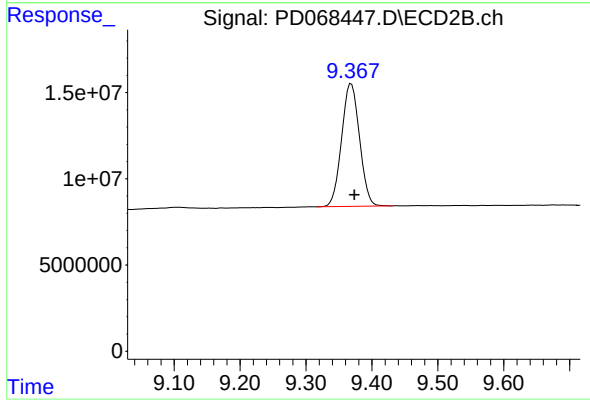

#28 Decachlorobiphenyl

R.T.: 9.369 min
Delta R.T.: -0.005 min
Response: 134520058
Conc: 22.69 ng/ml