

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ031124\
 Data File : PQ065709.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2024 12:14
 Operator : YP\AJ
 Sample : P1721-05 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 BC274767-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/12/2024
 Supervised By :Ankita Jodhani 03/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 01:41:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ022624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 27 08:43:13 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.443	2.737	2720298	5026063	0.686	0.739
2) SA Decachlor...	8.653	7.506	2467761	7005620	1.010m	0.906

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ031124\
Data File : PQ065709.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2024 12:14
Operator : YP\AJ
Sample : P1721-05 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
BC274767-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/12/2024
Supervised By :Ankita Jodhani 03/12/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 01:41:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ022624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 27 08:43:13 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

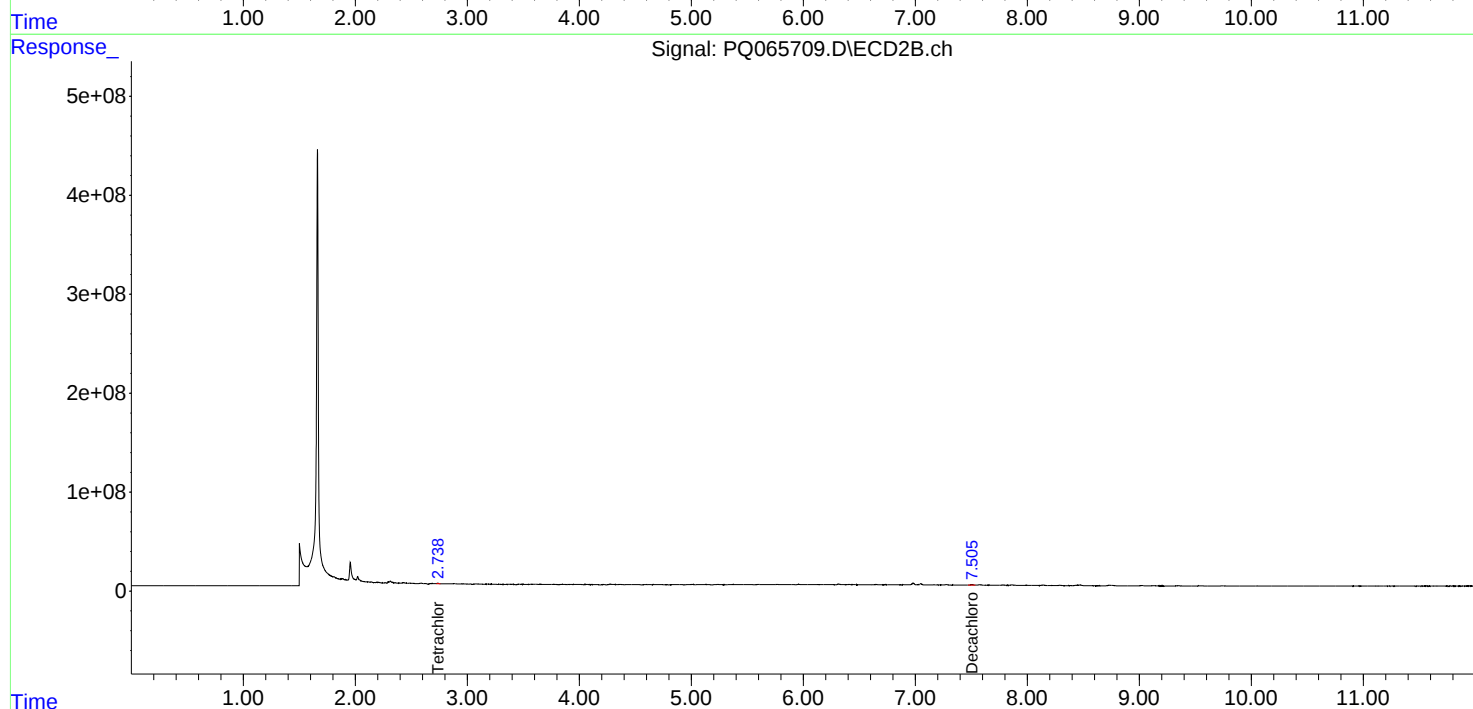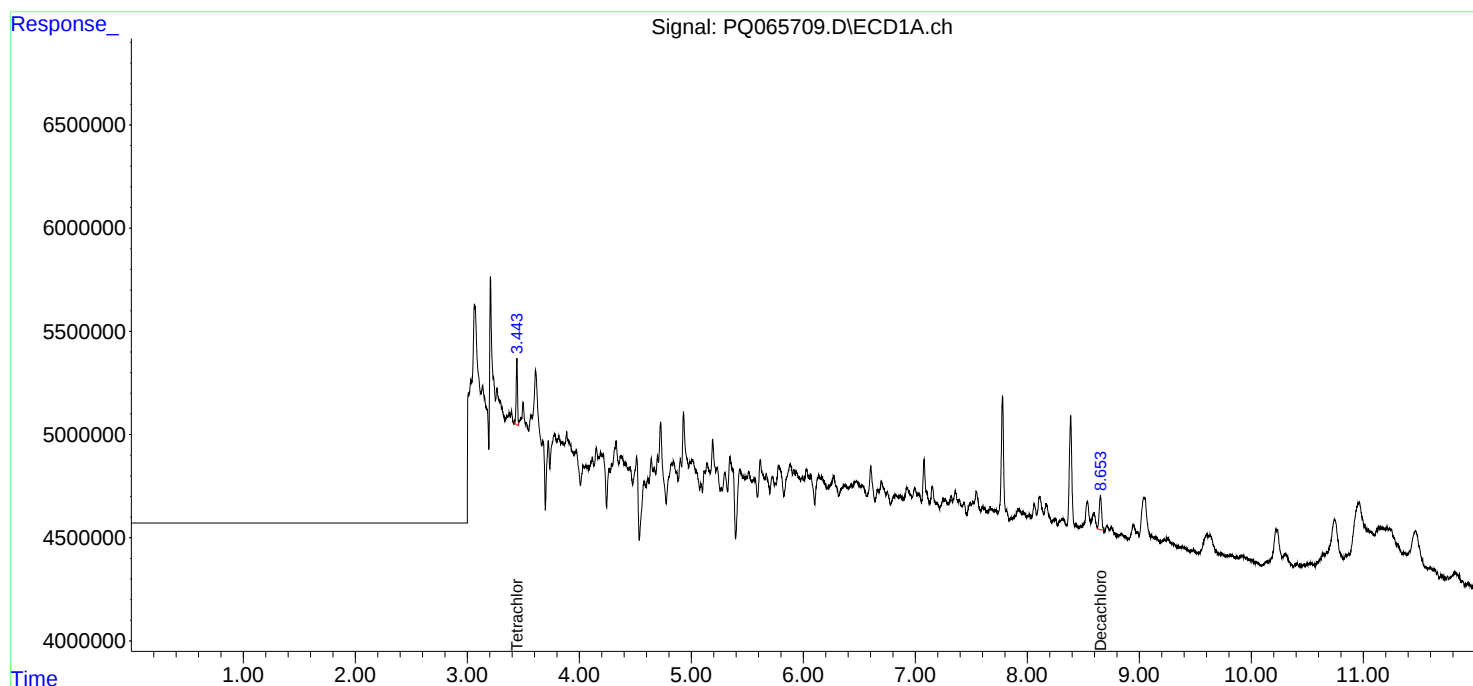

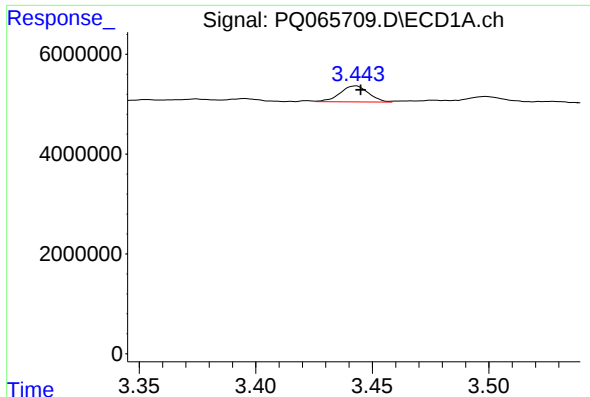


#1 Tetrachloro-m-xylene

R.T.: 3.443 min
Delta R.T.: -0.002 min
Response: 2720298
Conc: 0.69 ng/ml

Instrument :
ECD_Q
ClientSampleId :
BC274767-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/12/2024
Supervised By :Ankita Jodhani 03/12/2024

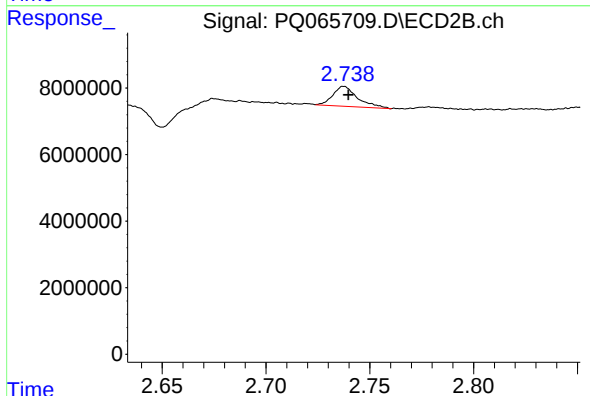


#1 Tetrachloro-m-xylene

R.T.: 2.737 min
Delta R.T.: -0.002 min
Response: 5026063
Conc: 0.74 ng/ml

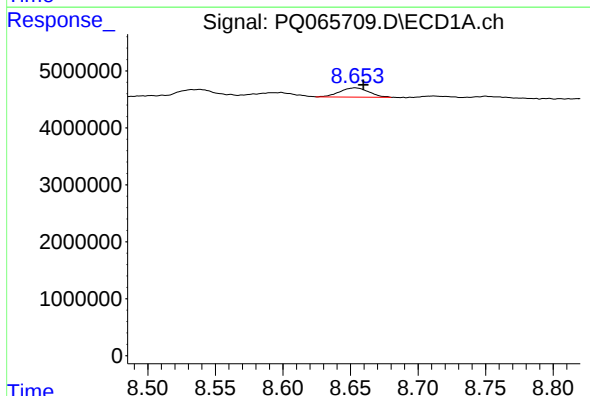

#2 Decachlorobiphenyl

R.T.: 8.653 min
Delta R.T.: -0.006 min
Response: 2467761
Conc: 1.01 ng/ml m

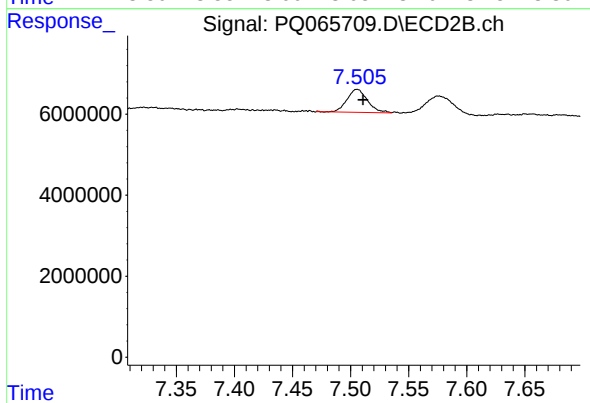

#2 Decachlorobiphenyl

R.T.: 7.506 min
Delta R.T.: -0.005 min
Response: 7005620
Conc: 0.91 ng/ml