

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ031124\
 Data File : PQ065711.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2024 12:44
 Operator : YP\AJ
 Sample : P1721-07 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 BC274767-2-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/12/2024
 Supervised By :Ankita Jodhani 03/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 01:42:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ022624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 27 08:43:13 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.443	2.738	6764019	12961001	1.706m	1.906
2) SA Decachlor...	8.650	7.505	4749584	9247401	1.945m	1.196 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ031124\
Data File : PQ065711.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2024 12:44
Operator : YP\AJ
Sample : P1721-07 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
BC274767-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/12/2024
Supervised By :Ankita Jodhani 03/12/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 01:42:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ022624.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 27 08:43:13 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

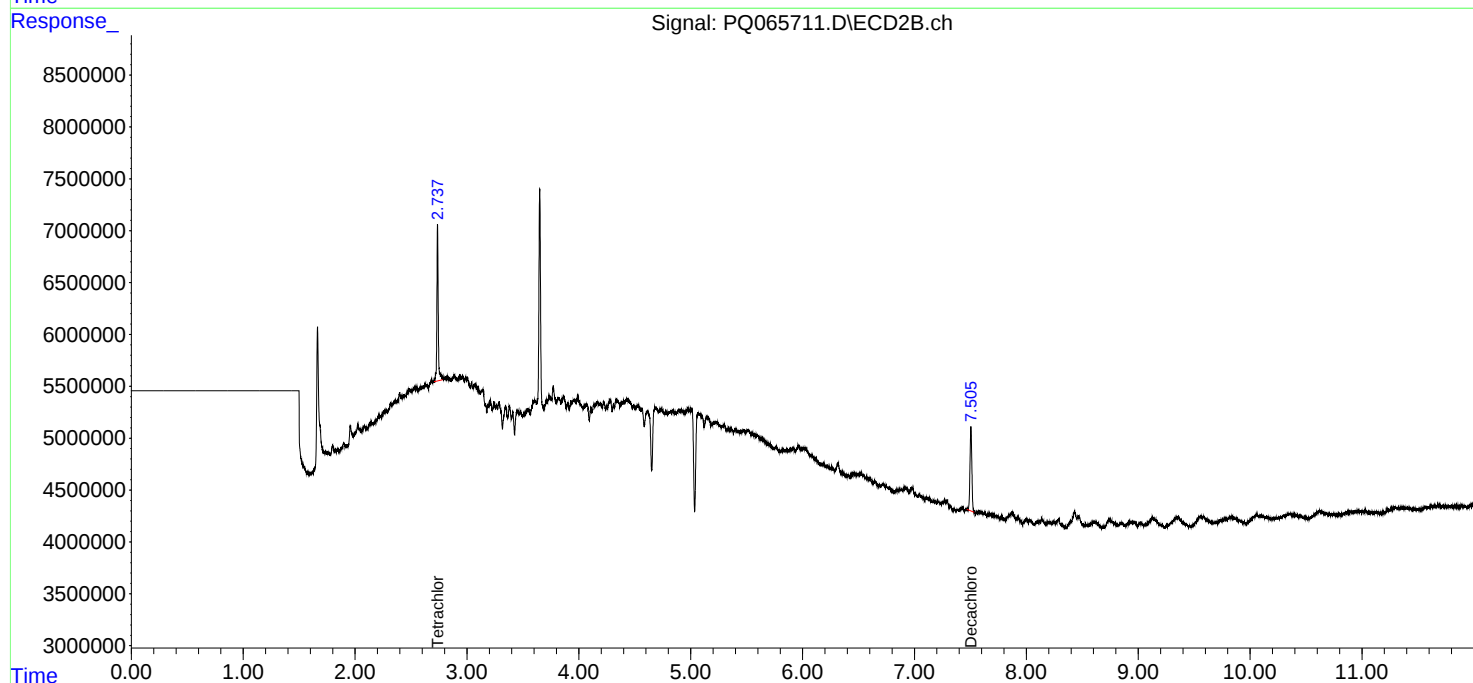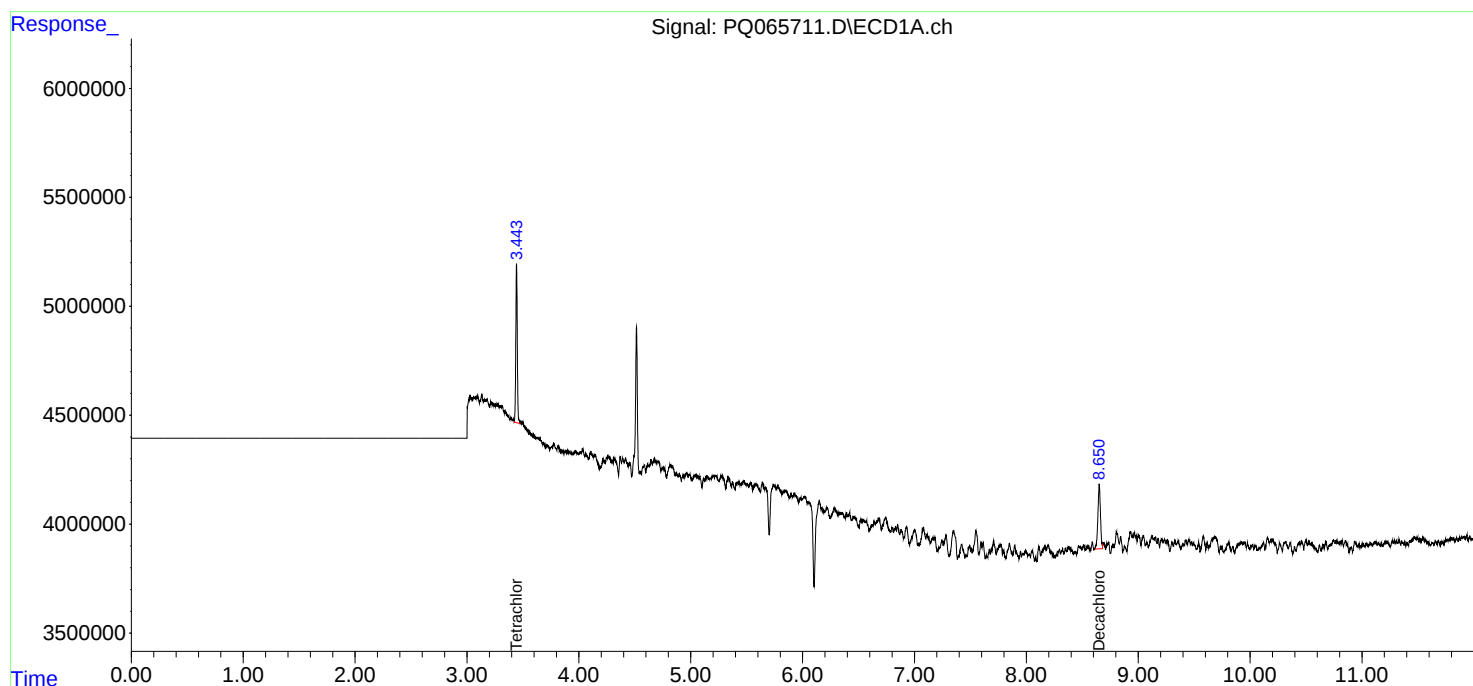

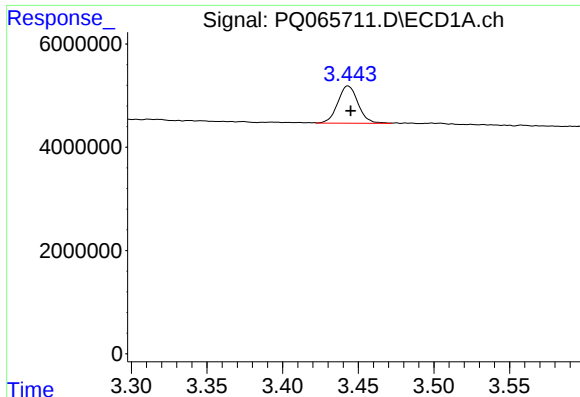

#1 Tetrachloro-m-xylene

R.T.: 3.443 min
Delta R.T.: -0.002 min
Response: 6764019
Conc: 1.71 ng/ml

Instrument :

ECD_Q


ClientSampleId :

BC274767-2-1

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 03/12/2024
Supervised By :Ankita Jodhani 03/12/2024

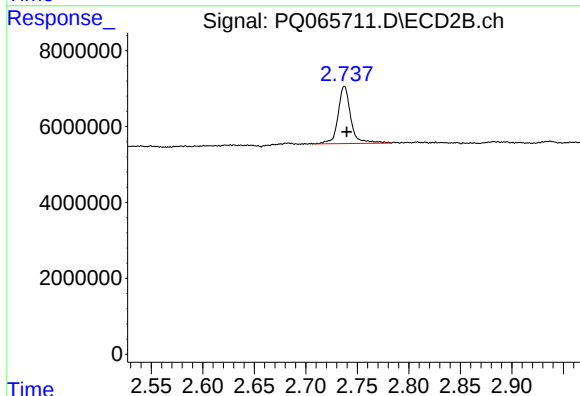


#1 Tetrachloro-m-xylene

R.T.: 2.738 min
Delta R.T.: -0.002 min
Response: 12961001
Conc: 1.91 ng/ml

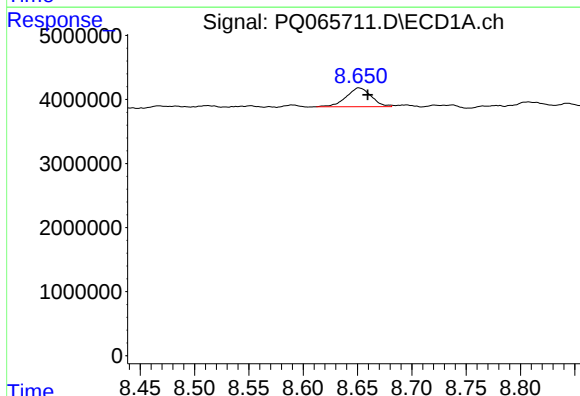

#2 Decachlorobiphenyl

R.T.: 8.650 min
Delta R.T.: -0.009 min
Response: 4749584
Conc: 1.94 ng/ml m

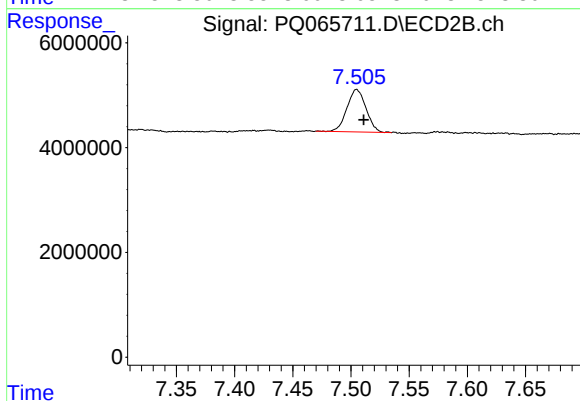

#2 Decachlorobiphenyl

R.T.: 7.505 min
Delta R.T.: -0.006 min
Response: 9247401
Conc: 1.20 ng/ml