

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ031221\
 Data File : PQ052572.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2021 14:44
 Operator : DD\AJ
 Sample : M1458-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MDL-WATER-03-QT1-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 12 02:14:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ031021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 11 04:11:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.226	4.242	440.9E6	154.0E6	17.359	16.931
2)	SA Decachlor...	11.414	9.586	453.3E6	173.8E6	18.184	17.922
Target Compounds							
26)	L6 AR-1254-1	7.460	6.375	23384400	12558533	25.994	24.378
27)	L6 AR-1254-2	7.689	6.534	37420597	11256681	26.485	25.156
28)	L6 AR-1254-3	8.072	6.955	40587998	17819107	26.150	24.097
29)	L6 AR-1254-4	8.365	7.193	27027515	12062386	23.587	24.154
30)	L6 AR-1254-5	8.794	7.622	28616526	17618134	23.532	25.806



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ031221\
Data File : PQ052572.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2021 14:44
Operator : DD\AJ
Sample : M1458-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT1-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 12 02:14:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ031021.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 11 04:11:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

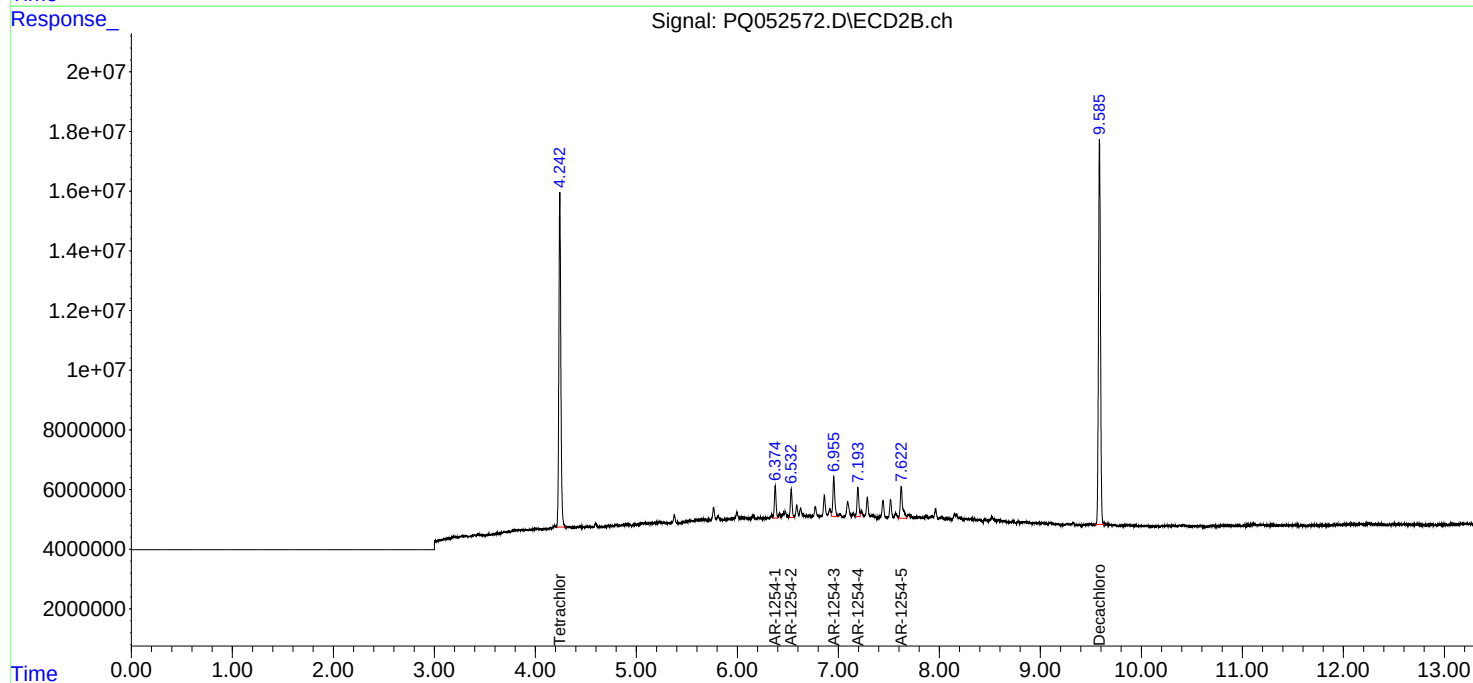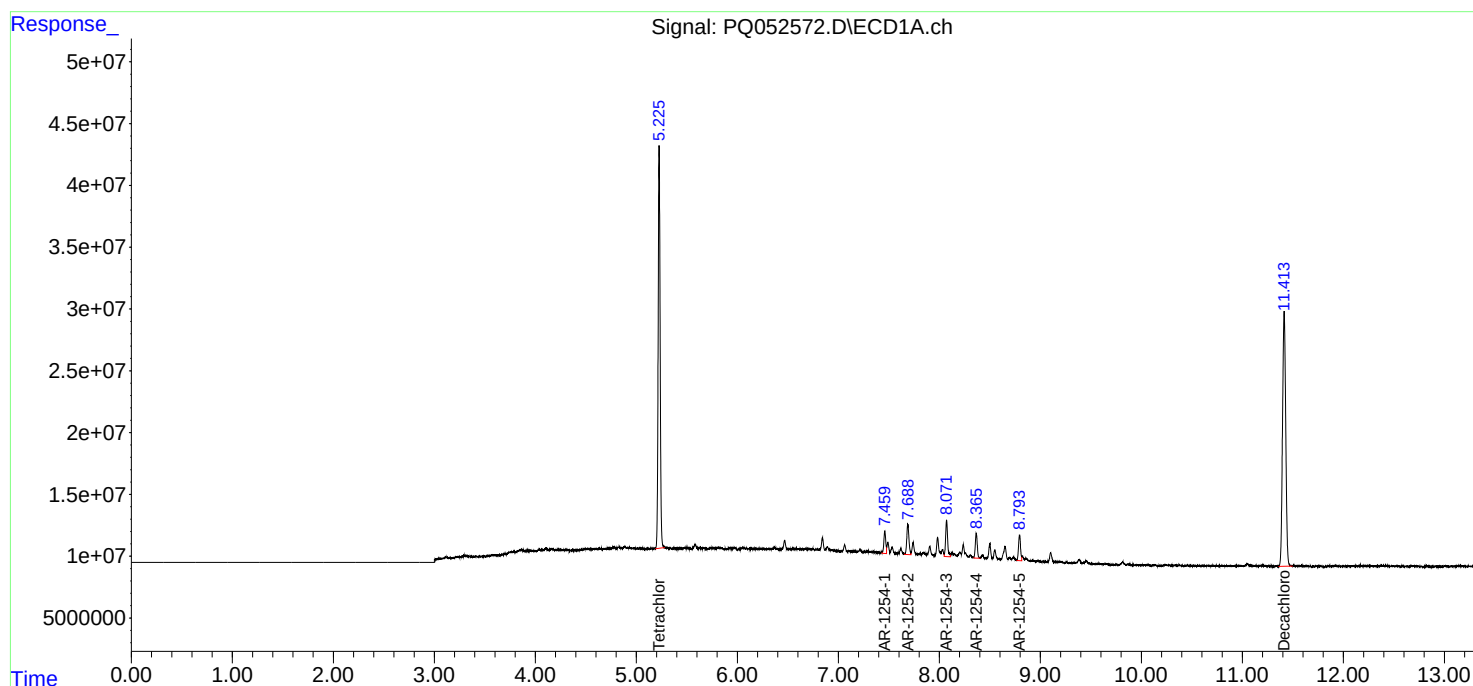


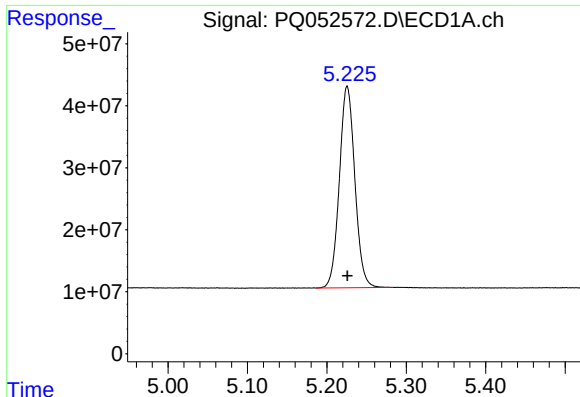

#1 Tetrachloro-m-xylene


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 440933624
Conc: 17.36 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT1-2021

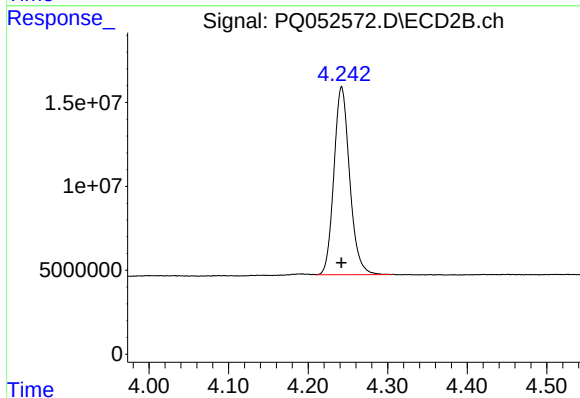


#1 Tetrachloro-m-xylene

R.T.: 4.242 min
Delta R.T.: 0.000 min
Response: 154013754
Conc: 16.93 ng/ml

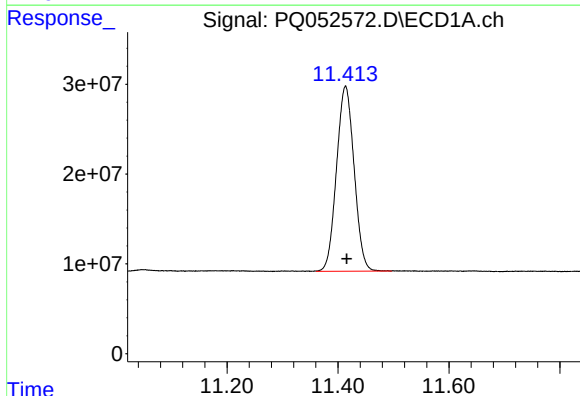


#2 Decachlorobiphenyl

R.T.: 11.414 min
Delta R.T.: -0.002 min
Response: 453338508
Conc: 18.18 ng/ml

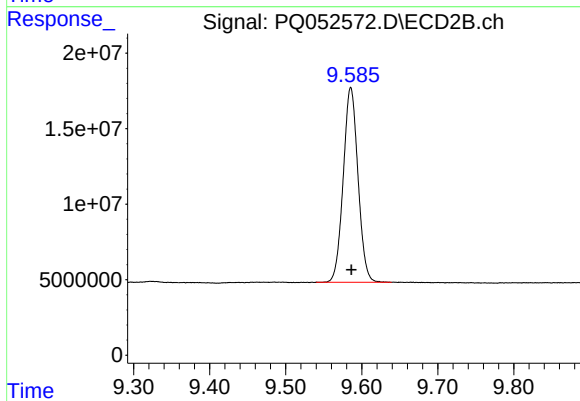

#2 Decachlorobiphenyl


R.T.: 9.586 min
Delta R.T.: 0.000 min
Response: 173831546
Conc: 17.92 ng/ml

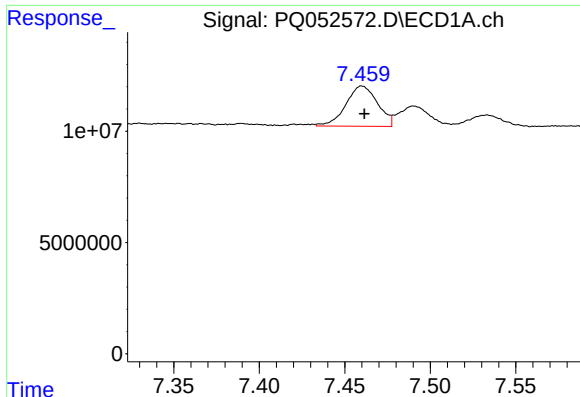

#26 AR-1254-1


R.T.: 7.460 min
Delta R.T.: -0.001 min
Response: 23384400
Conc: 25.99 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT1-2021

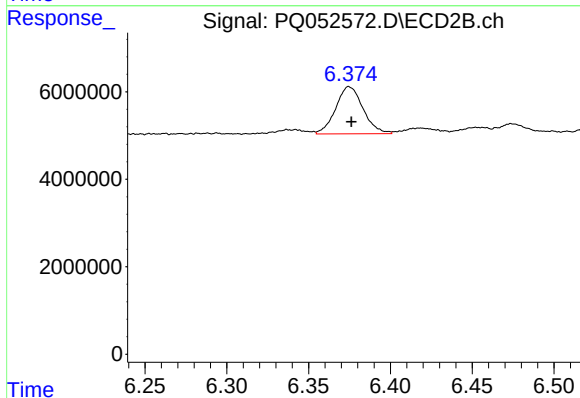


#26 AR-1254-1

R.T.: 6.375 min
Delta R.T.: -0.002 min
Response: 12558533
Conc: 24.38 ng/ml

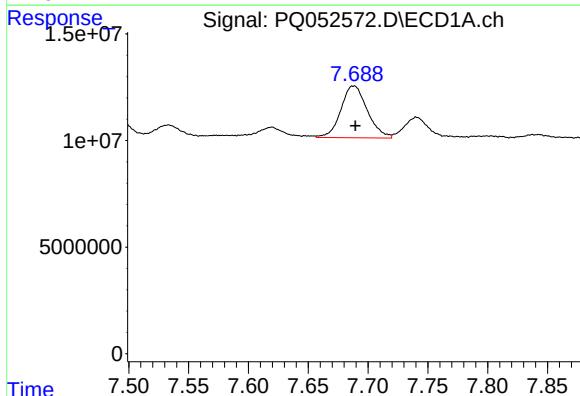


#27 AR-1254-2

R.T.: 7.689 min
Delta R.T.: 0.000 min
Response: 37420597
Conc: 26.49 ng/ml

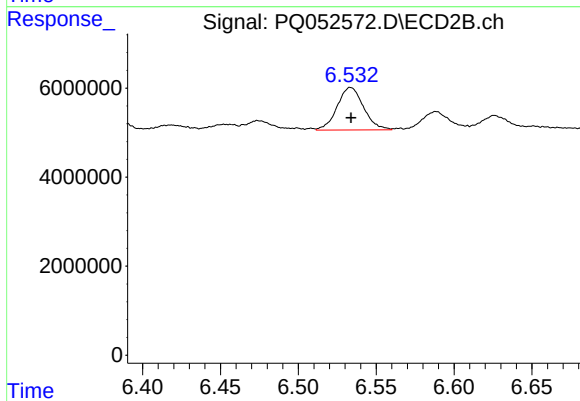

#27 AR-1254-2


R.T.: 6.534 min
Delta R.T.: 0.000 min
Response: 11256681
Conc: 25.16 ng/ml

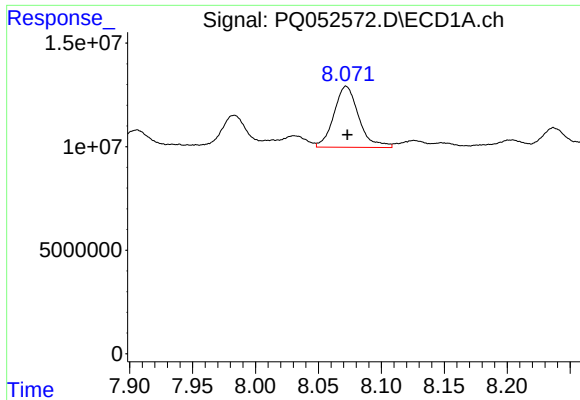

#28 AR-1254-3


R.T.: 8.072 min
Delta R.T.: -0.001 min
Response: 40587998
Conc: 26.15 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT1-2021

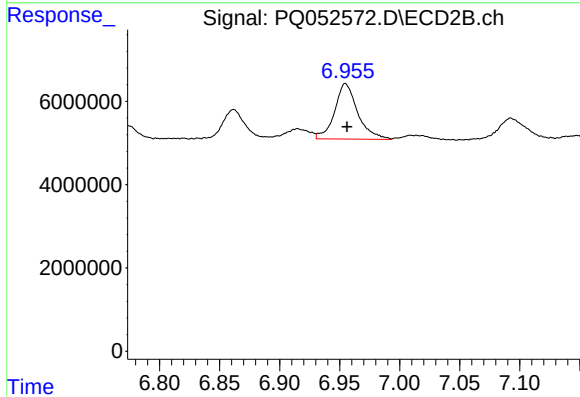


#28 AR-1254-3

R.T.: 6.955 min
Delta R.T.: -0.001 min
Response: 17819107
Conc: 24.10 ng/ml

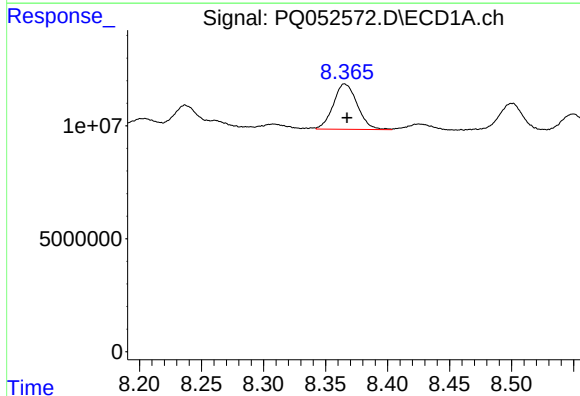


#29 AR-1254-4

R.T.: 8.365 min
Delta R.T.: -0.002 min
Response: 27027515
Conc: 23.59 ng/ml

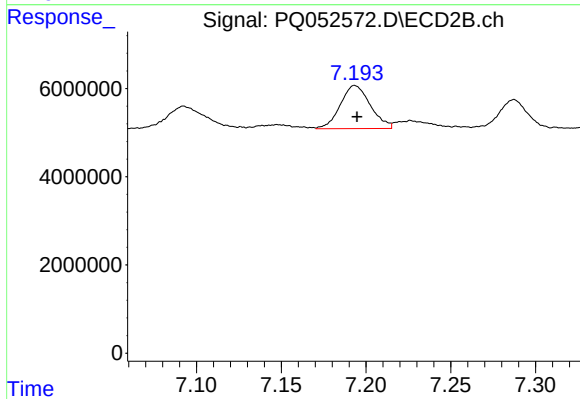

#29 AR-1254-4


R.T.: 7.193 min
Delta R.T.: -0.001 min
Response: 12062386
Conc: 24.15 ng/ml

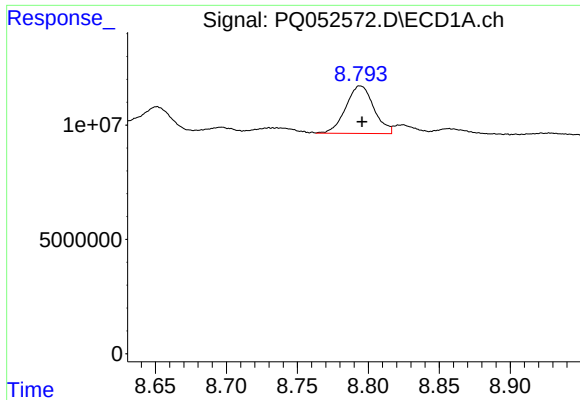

#30 AR-1254-5

R.T.: 8.794 min
Delta R.T.: -0.002 min
Response: 28616526
Conc: 23.53 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-WATER-03-QT1-2021

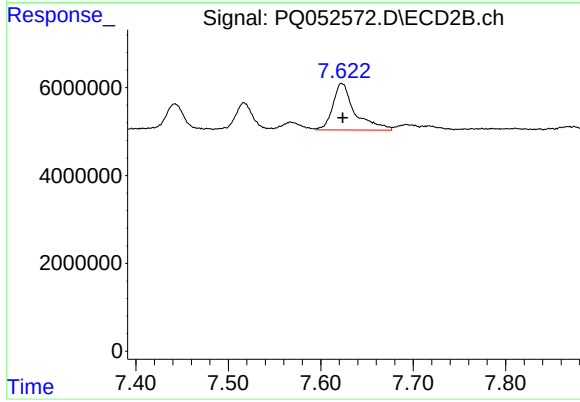

#30 AR-1254-5

R.T.: 7.622 min
Delta R.T.: -0.001 min
Response: 17618134
Conc: 25.81 ng/ml