

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ031521\
 Data File : PQ052623.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2021 15:12
 Operator : DD\AJ
 Sample : M1665-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 41739

Manual Integrations
 APPROVED

Ankita
 3/16/2021 11:07:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 01:48:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ031321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 13 08:26:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.227	4.244	535.9E6	196.6E6	23.711m	23.902m
2) SA Decachlor...	11.417	9.587	503.4E6	177.3E6	18.706	18.267

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ031521\
Data File : PQ052623.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2021 15:12
Operator : DD\AJ
Sample : M1665-02
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
41739


Manual Integrations
APPROVED

Ankita
3/16/2021 11:07:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 01:48:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ031321.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 13 08:26:53 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

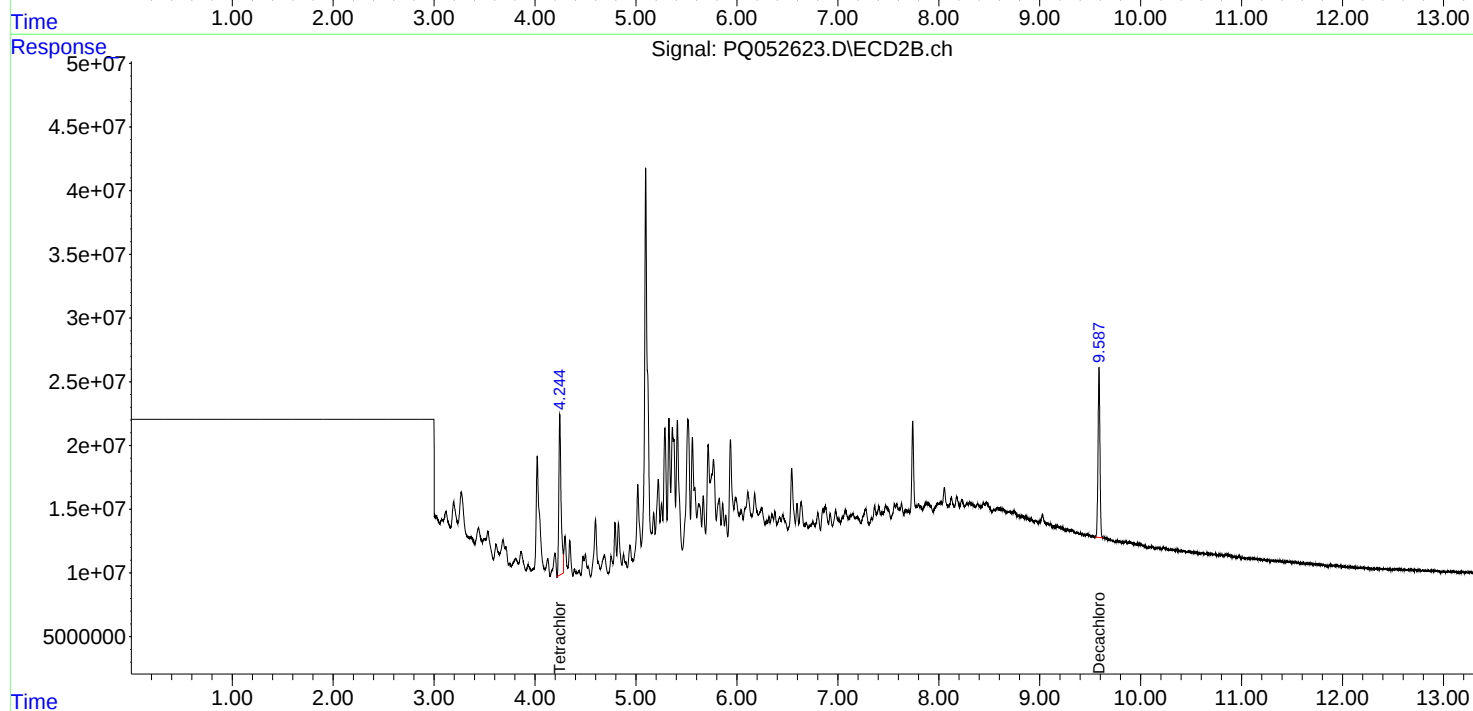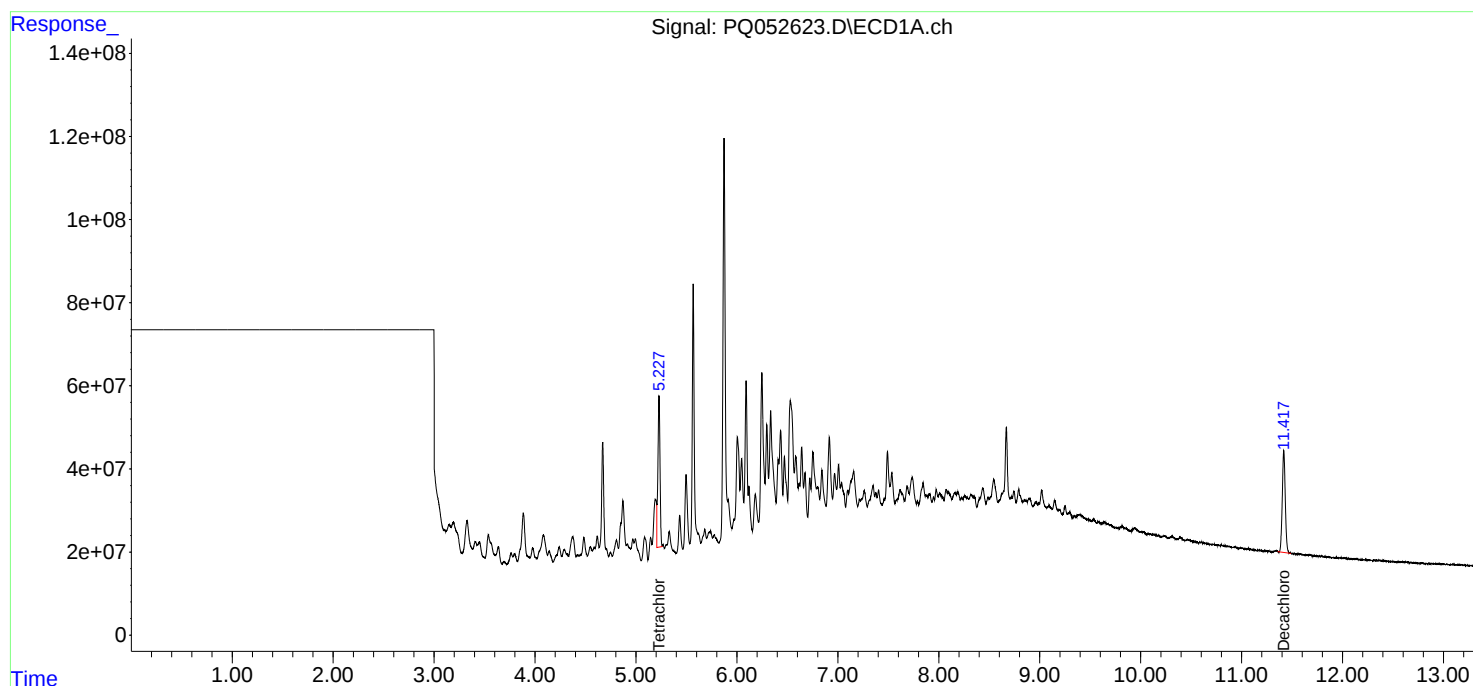

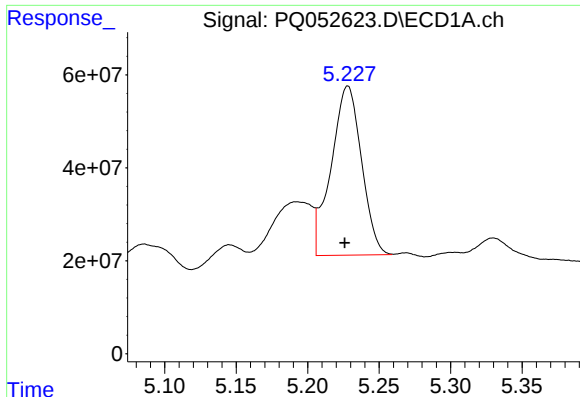


#1 Tetrachloro-m-xylene

R.T.: 5.227 min
Delta R.T.: 0.001 min
Response: 535906735
Conc: 23.71 ng/ml m

Instrument :
ECD_Q
ClientSampleId :
41739


Manual Integrations
APPROVED

Ankita
3/16/2021 11:07:08 AM

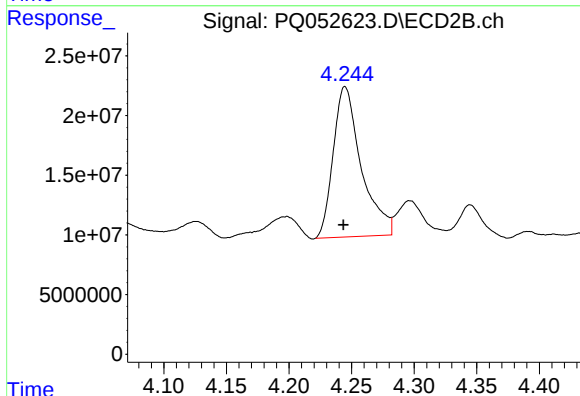


#1 Tetrachloro-m-xylene

R.T.: 4.244 min
Delta R.T.: 0.000 min
Response: 196643127
Conc: 23.90 ng/ml m

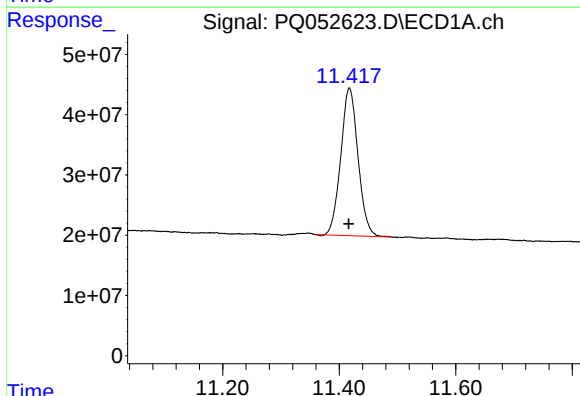

#2 Decachlorobiphenyl

R.T.: 11.417 min
Delta R.T.: 0.000 min
Response: 503424905
Conc: 18.71 ng/ml

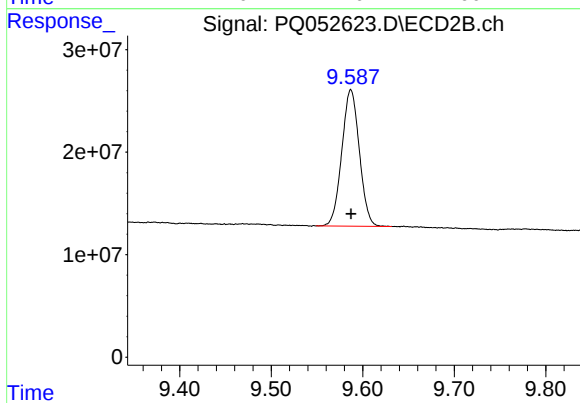

#2 Decachlorobiphenyl

R.T.: 9.587 min
Delta R.T.: 0.000 min
Response: 177326954
Conc: 18.27 ng/ml