

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ031521\
 Data File : PQ052628.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2021 16:34
 Operator : DD\AJ
 Sample : M1677-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 D2470-D2800(WATER)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 01:52:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ031321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Mar 13 08:26:53 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.228	4.245	583.9E6	236.3E6	25.834	28.720
2) SA Decachlor...	11.416	9.586	355.5E6	131.6E6	13.208	13.558

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ031521\
Data File : PQ052628.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2021 16:34
Operator : DD\AJ
Sample : M1677-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
D2470-D2800(WATER)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 01:52:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ031321.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Mar 13 08:26:53 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

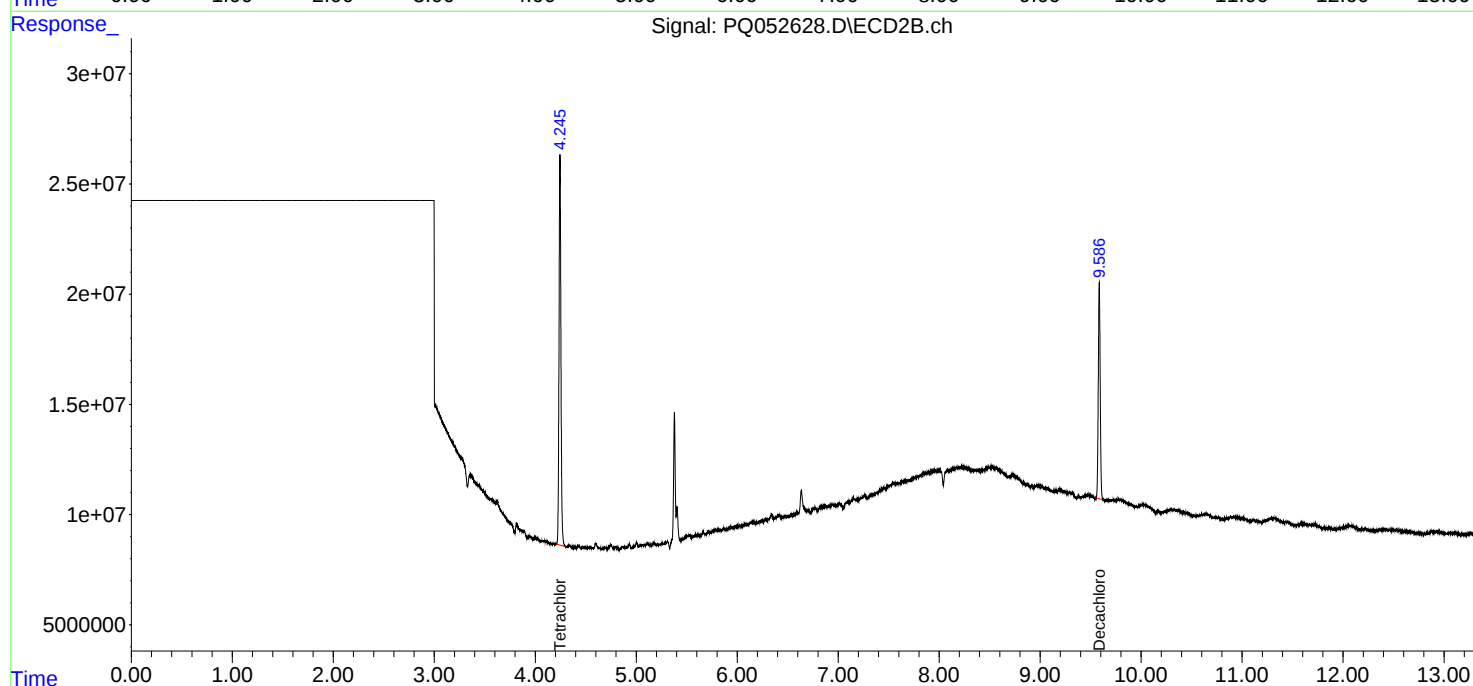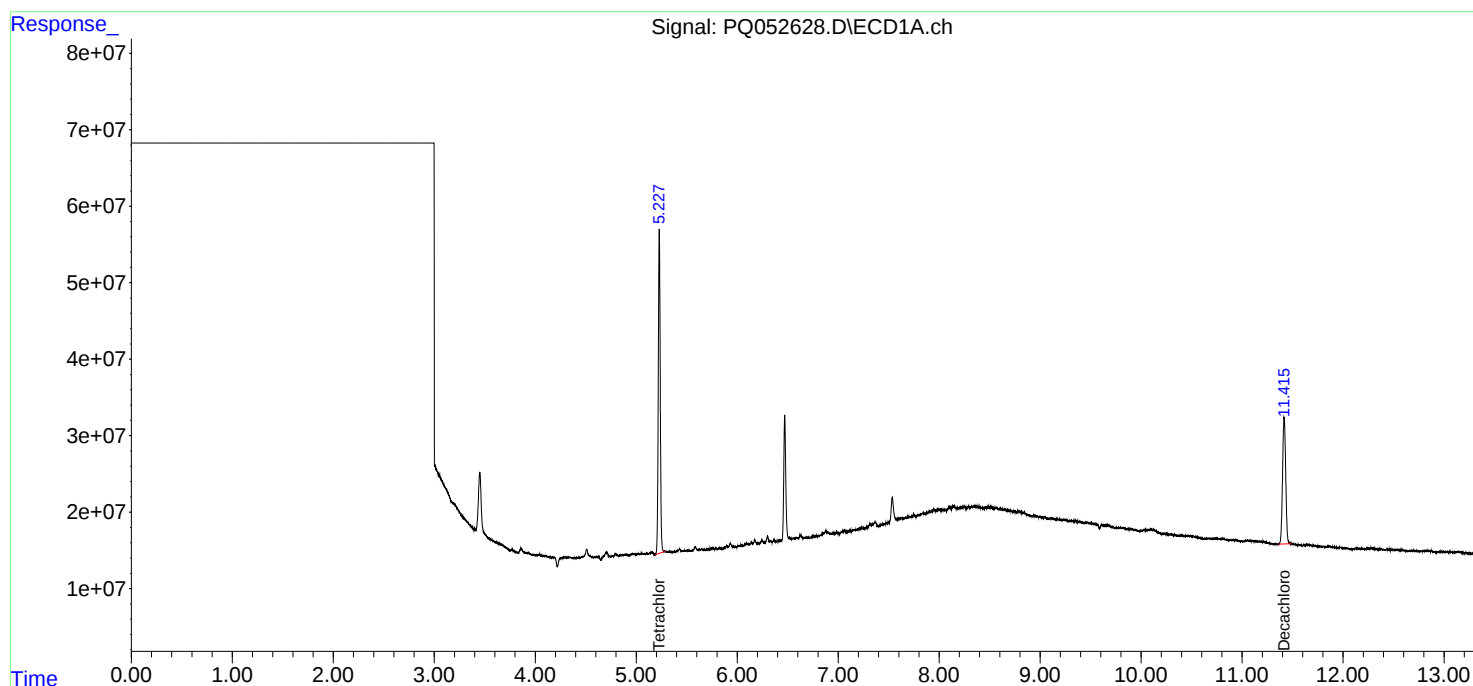


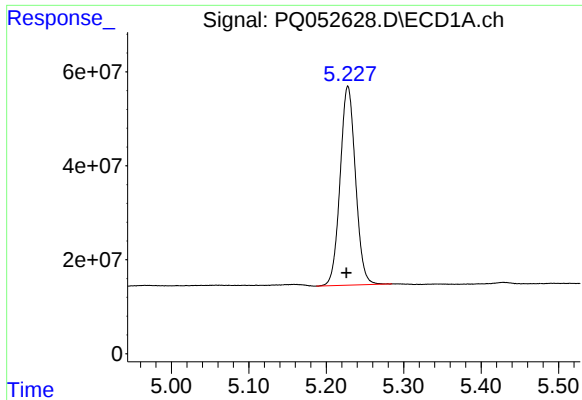

#1 Tetrachloro-m-xylene


R.T.: 5.228 min
Delta R.T.: 0.002 min
Response: 583903624
Conc: 25.83 ng/ml

Instrument :
ECD_Q
ClientSampleId :
D2470-D2800(WATER)

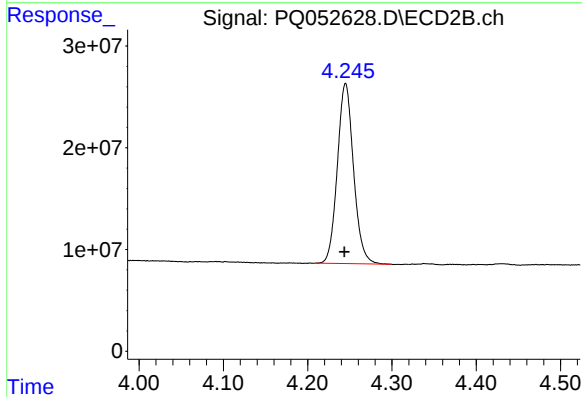


#1 Tetrachloro-m-xylene

R.T.: 4.245 min
Delta R.T.: 0.001 min
Response: 236279225
Conc: 28.72 ng/ml

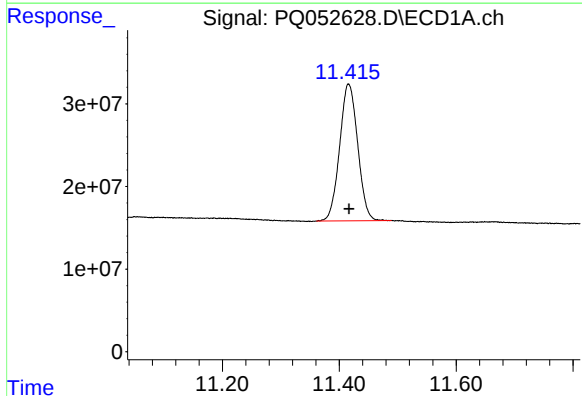

#2 Decachlorobiphenyl

R.T.: 11.416 min
Delta R.T.: 0.000 min
Response: 355471357
Conc: 13.21 ng/ml

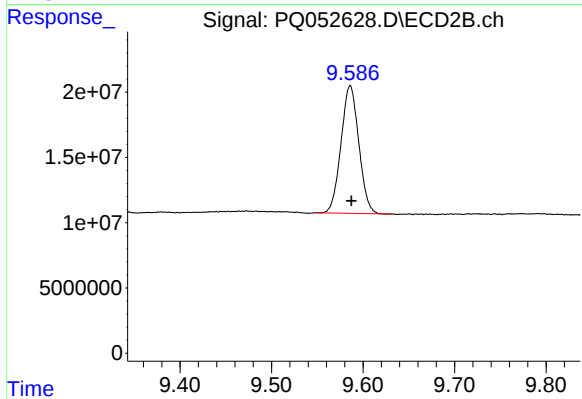

#2 Decachlorobiphenyl

R.T.: 9.586 min
Delta R.T.: -0.001 min
Response: 131619806
Conc: 13.56 ng/ml