

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ032024\
 Data File : PQ065847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Mar 2024 20:35
 Operator : YP\AJ
 Sample : P1807-03 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 3436-37

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/21/2024
 Supervised By :Ankita Jodhani 03/21/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 23:11:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ031824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 12:55:45 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.442	2.735	6906720	12716009	1.390	1.715
2) SA Decachlor...	8.650	7.510	4624921	10730056	1.594	1.284m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ032024\
Data File : PQ065847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Mar 2024 20:35
Operator : YP\AJ
Sample : P1807-03 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
3436-37


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/21/2024
Supervised By :Ankita Jodhani 03/21/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 23:11:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ031824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 12:55:45 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

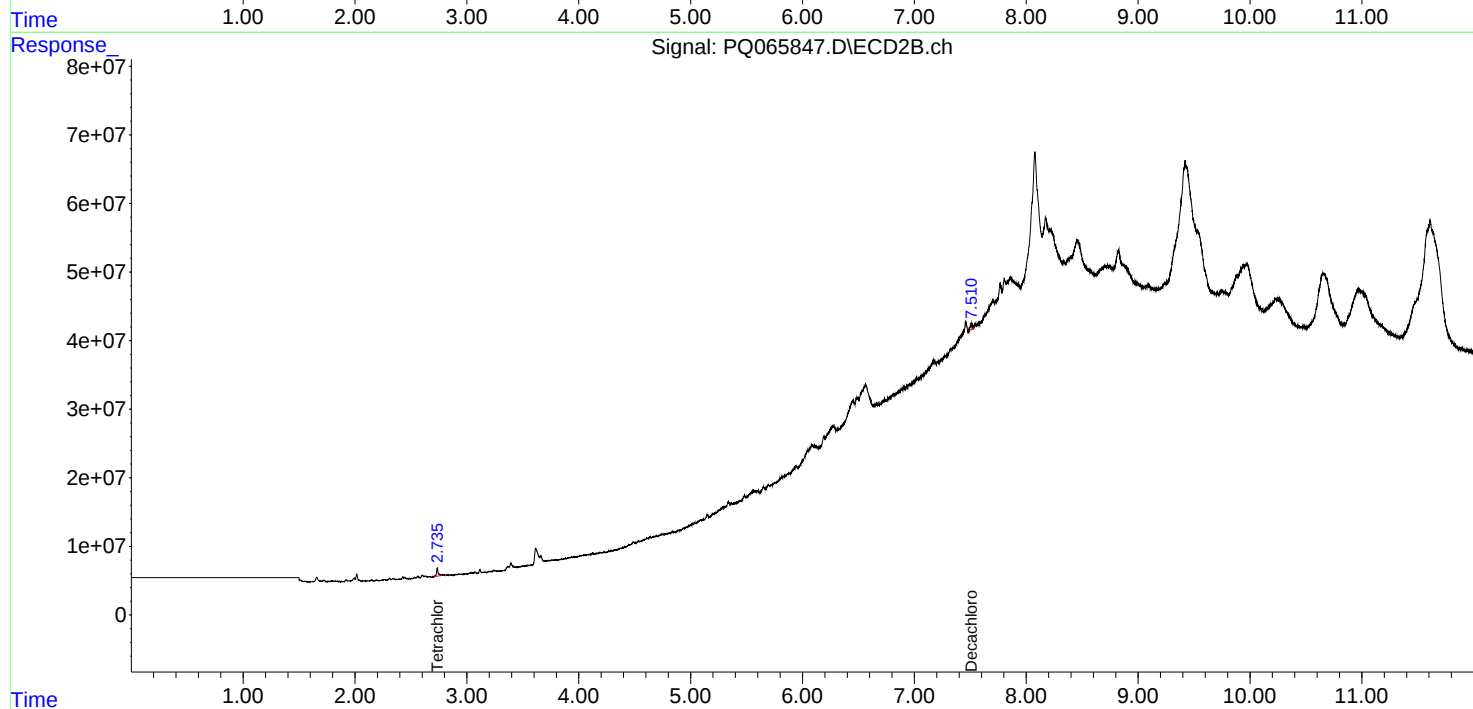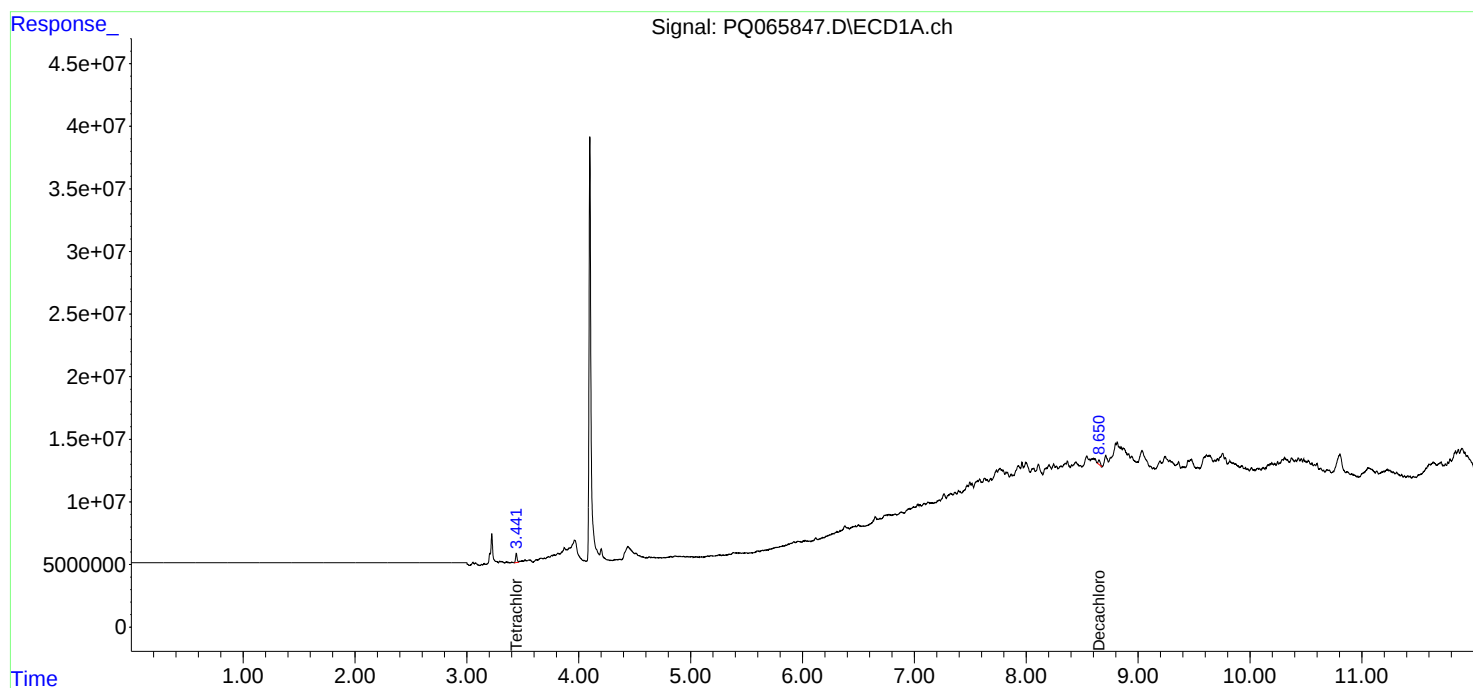

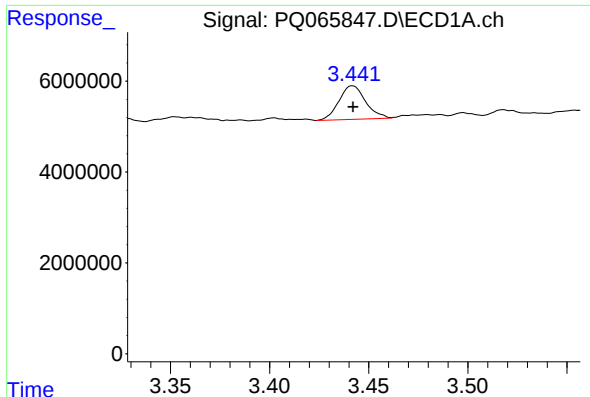


#1 Tetrachloro-m-xylene

R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 6906720
Conc: 1.39 ng/ml

Instrument :
ECD_Q
ClientSampleId :
3436-37


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/21/2024
Supervised By :Ankita Jodhani 03/21/2024

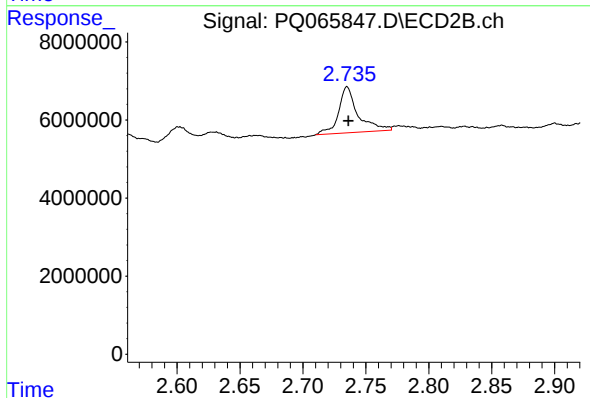


#1 Tetrachloro-m-xylene

R.T.: 2.735 min
Delta R.T.: 0.000 min
Response: 12716009
Conc: 1.71 ng/ml

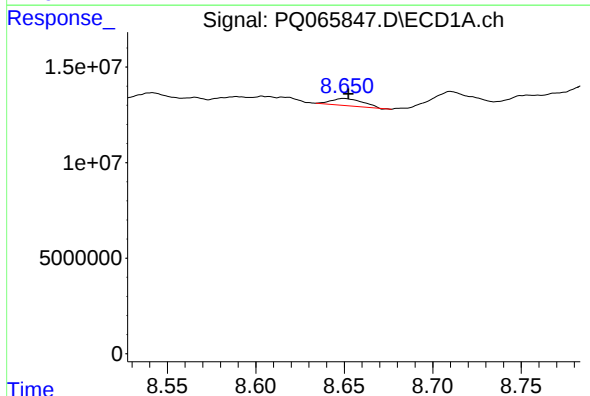

#2 Decachlorobiphenyl

R.T.: 8.650 min
Delta R.T.: -0.002 min
Response: 4624921
Conc: 1.59 ng/ml

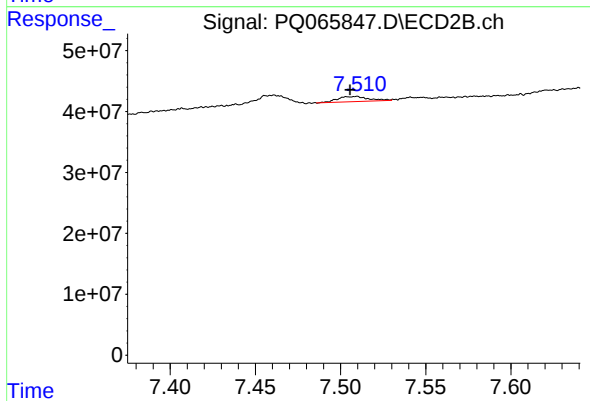

#2 Decachlorobiphenyl

R.T.: 7.510 min
Delta R.T.: 0.004 min
Response: 10730056
Conc: 1.28 ng/ml m