

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ032419\
Data File : PQ038241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2019 13:08
Operator : SM\SJ
Sample : PB118209BS
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampled :
ALCS09

Manual Integrations
APPROVED

Sohil
3/25/2019 1:12:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 07:16:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ032419CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 05:45:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

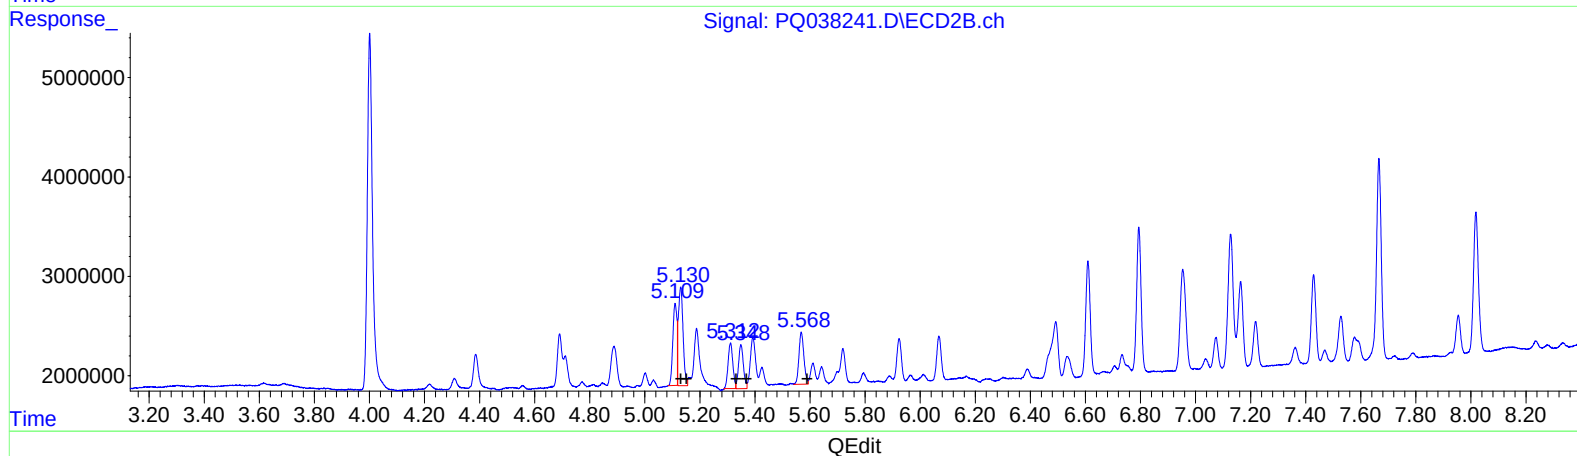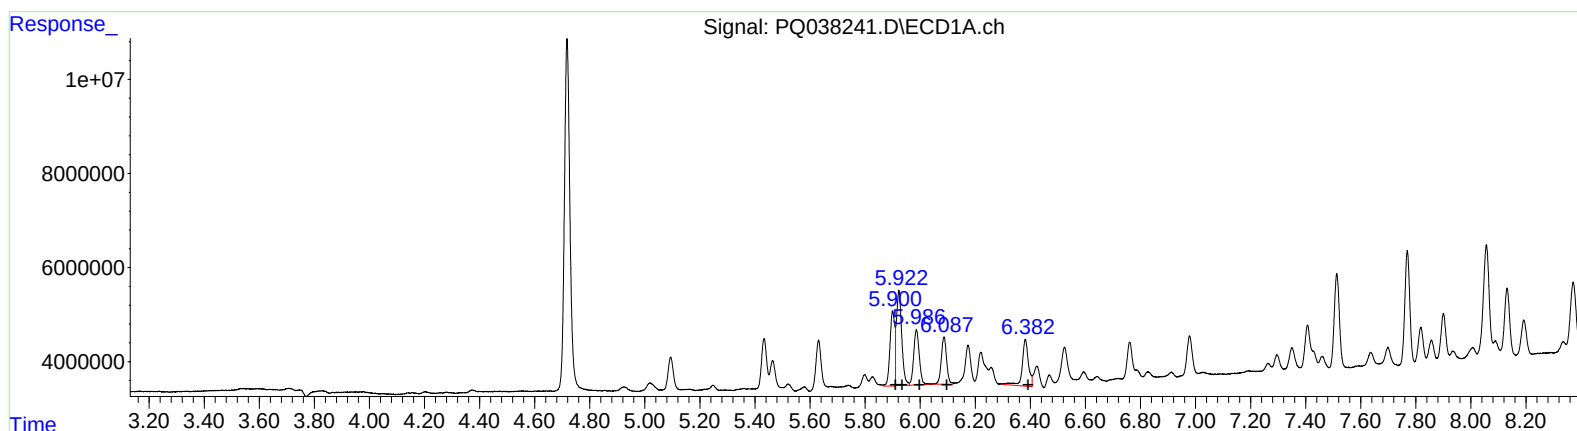

(3) AR-1016-1 #2 (L1)
R.T. Response Conc
5.90 19252685 80.62
5.92 27362075 75.37
5.99 16505629 74.15
6.09 13432745 72.86
6.38 15671470 84.90

(3) AR-1016-1 #2 (L1)
R.T. Response Conc
5.11 8207047 76.82
5.13 11331690 73.15
5.31 5464753 68.15
5.35 5436580 85.62
5.57 6540191 74.67

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ032419\
Data File : PQ038241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2019 13:08
Operator : SM\SJ
Sample : PB118209BS
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampled :
ALCS09

Manual Integrations
APPROVED

Sohil
3/25/2019 1:12:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 07:16:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ032419CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 05:45:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

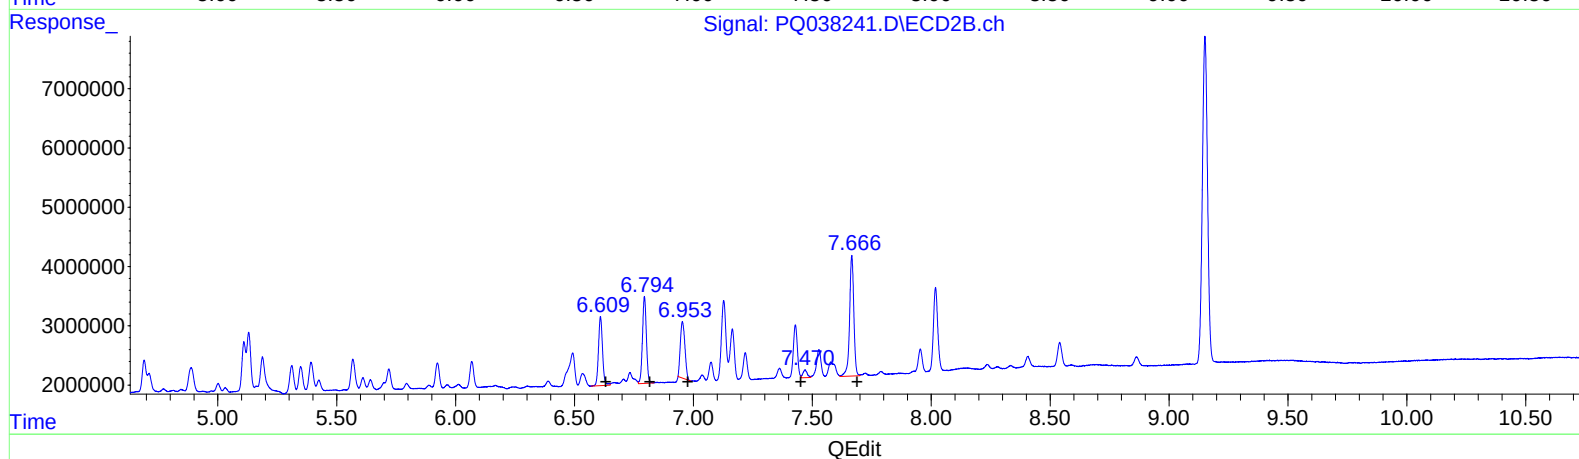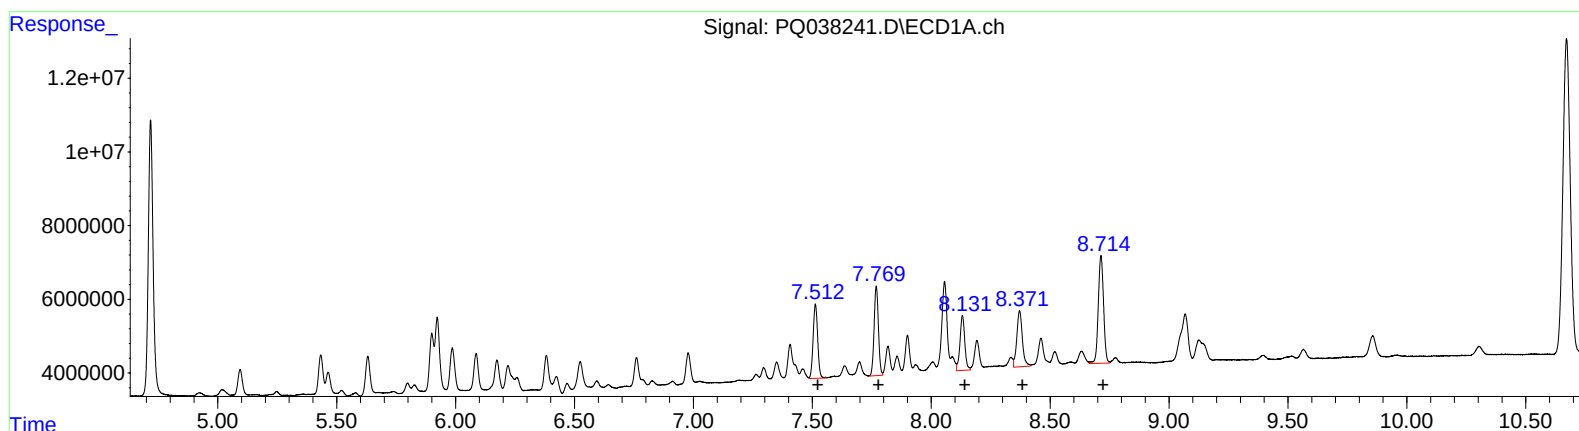

QEdit

(31) AR-1260-1 (L7)	R.T.	Response	Conc
	7.51	26697675	62.75
	7.77	30650717	59.71
	8.13	20929562	54.11
	8.37	24547948	53.82
	8.71	45093055	47.62

(31) AR-1260-1 #2 (L7)	R.T.	Response	Conc
	6.61	13733096	67.17
	6.79	16790353	65.55
	6.95	12735109	53.24
	7.47	1675585	8.47
	7.67	25275329	51.41

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ032419\
Data File : PQ038241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2019 13:08
Operator : SM\SJ
Sample : PB118209BS
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampled :
ALCS09

Manual Integrations
APPROVED

Sohil
3/25/2019 1:12:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 07:16:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ032419CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 05:45:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

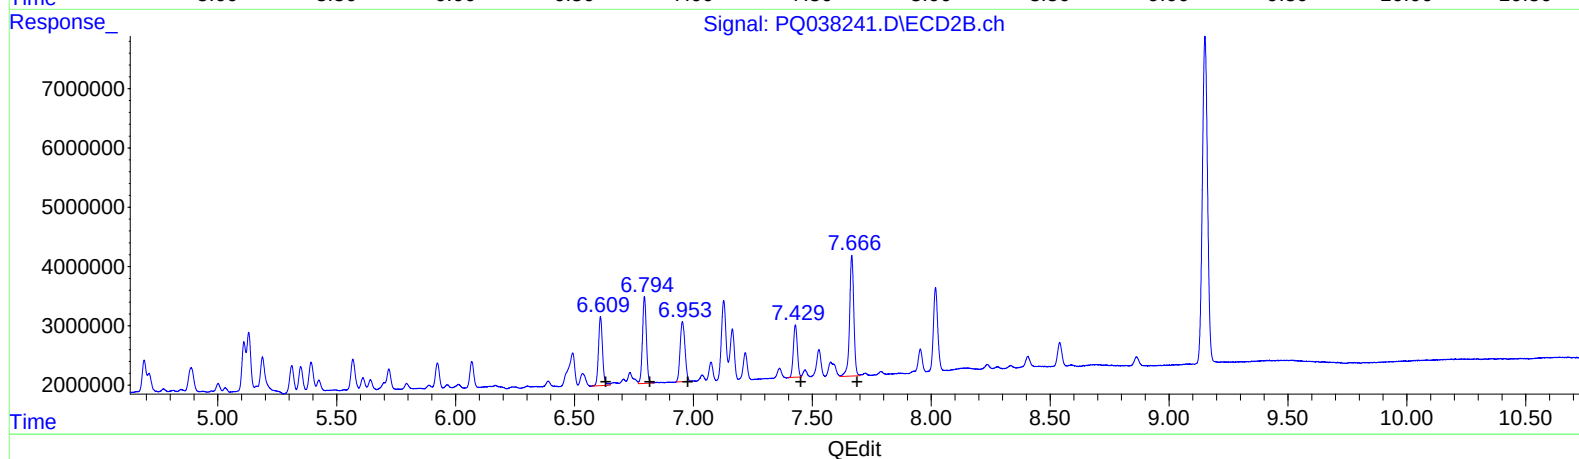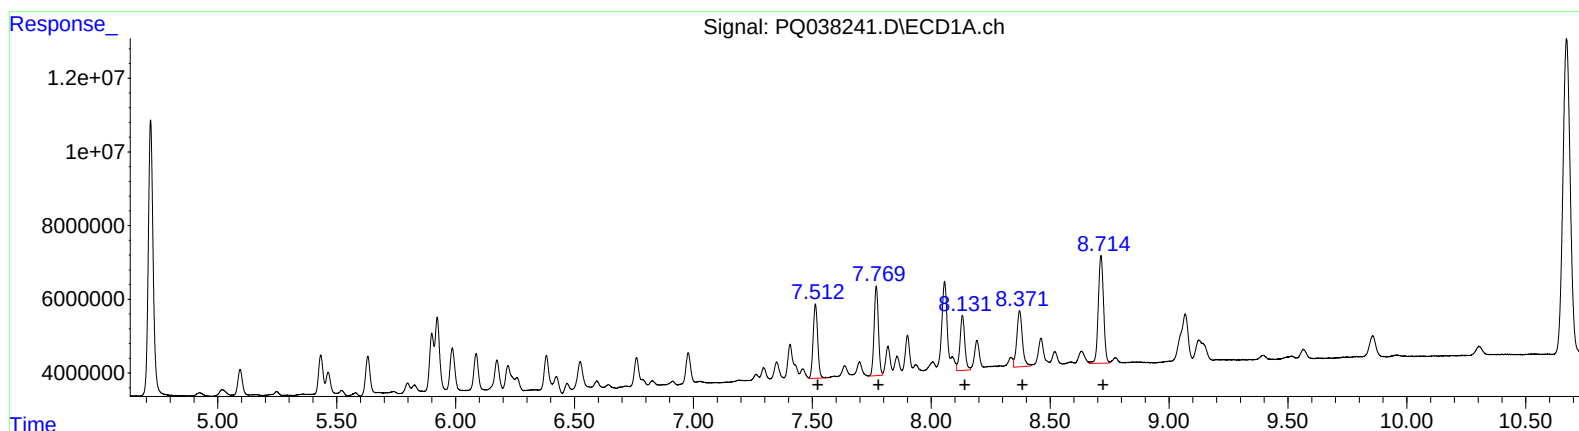

QEdit

(31) AR-1260-1 #2 (L7)	R.T.	Response	Conc
	7.51	26697675	62.75
	7.77	30650717	59.71
	8.13	20929562	54.11
	8.37	24547948	53.82
	8.71	45093055	47.62

(31) AR-1260-1 #2 (L7)	R.T.	Response	Conc
	6.61	13733096	67.17
	6.79	16790353	65.55
	6.95	14447790	60.39
	7.43	10266013	51.87
	7.67	25275329	51.41

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ032419\
Data File : PQ038241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2019 13:08
Operator : SM\SJ
Sample : PB118209BS
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampled :
ALCS09

Manual Integrations
APPROVED

Sohil
3/25/2019 1:12:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 07:16:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ032419CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 05:45:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

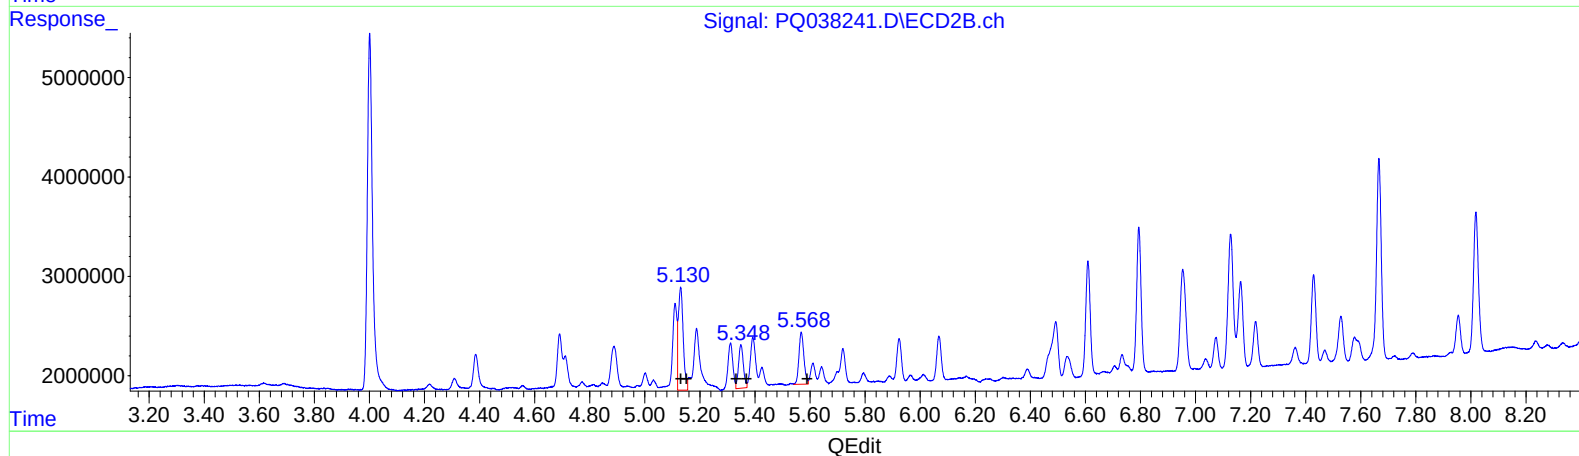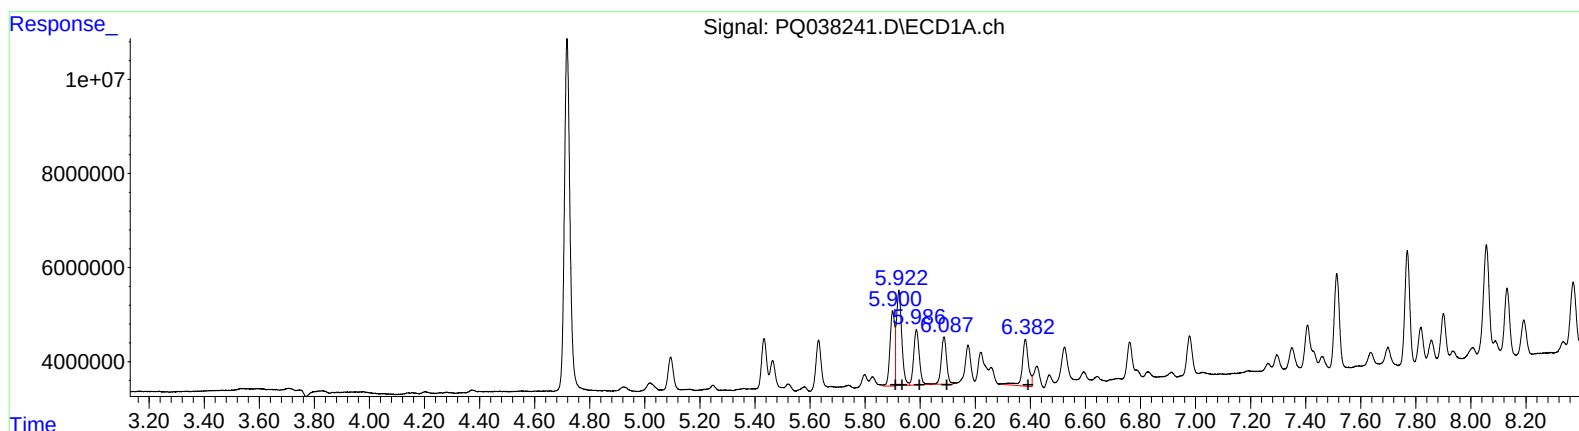

(3) AR-1016-1 (L1)

R.T.	Response	Conc
5.90	19252685	80.62
5.92	27362075	75.37
5.99	16505629	74.15
6.09	13432745	72.86
6.38	15671470	84.90

(3) AR-1016-1 #2 (L1)

R.T.	Response	Conc
5.13	12683911	118.72
5.13	12683911	81.88
5.35	5362718	66.88
5.35	5362718	84.46
5.57	6540191	74.67

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ032419\
 Data File : PQ038241.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2019 13:08
 Operator : SM\SJ
 Sample : PB118209BS
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 ALCS09

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 07:16:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ032419CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 05:45:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Manual Integrations
 APPROVED

Sohil
 3/25/2019 1:12:29 PM

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.718	4.001	105.0E6	46928121	25.466	27.805
2) SA Decachlor...	10.672	9.151	183.2E6	83591989	33.685	35.332
Target Compounds						
3) L1 AR-1016-1	5.900	5.109	19252685	8207047	80.623	76.817m
4) L1 AR-1016-2	5.923	5.130	27362075	11331690	75.372	73.150m
5) L1 AR-1016-3	5.986	5.312	16505629	5464753	74.152	68.153m
6) L1 AR-1016-4	6.087	5.348	13432745	5436580	72.864	85.622m
7) L1 AR-1016-5	6.382	5.568	15671470	6540191	84.901	74.670
31) L7 AR-1260-1	7.513	6.609	26697675	13733096	62.750	67.170
32) L7 AR-1260-2	7.769	6.794	30650717	16790353	59.707	65.547
33) L7 AR-1260-3	8.131	6.953	20929562	14447790	54.106	60.395m
34) L7 AR-1260-4	8.372	7.429	24547948	10266013	53.817	51.865m
35) L7 AR-1260-5	8.714	7.666	45093055	25275329	47.619	51.406

53
 03/26/19

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.