

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040319\
 Data File : PQ038658.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2019 22:11
 Operator : AJ\SJ
 Sample : K1560-07
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 03:01:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 04 03:26:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.704	3.986	171.5E6	89140584	23.189	21.753
2) SA Decachlor...	10.642	9.102	114.1E6	63767082	21.913	20.457
Target Compounds						
8) L2 AR-1221-1	4.913	4.199	3889475	2217412	55.170m	54.965m
9) L2 AR-1221-2	5.003	4.289	4332279	2337117	86.404m	79.463m
10) L2 AR-1221-3	5.079	4.366	9443171	4980448	58.910	51.744m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040319\
Data File : PQ038658.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2019 22:11
Operator : AJ\SJ
Sample : K1560-07
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 03:01:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ040319.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 04 03:26:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

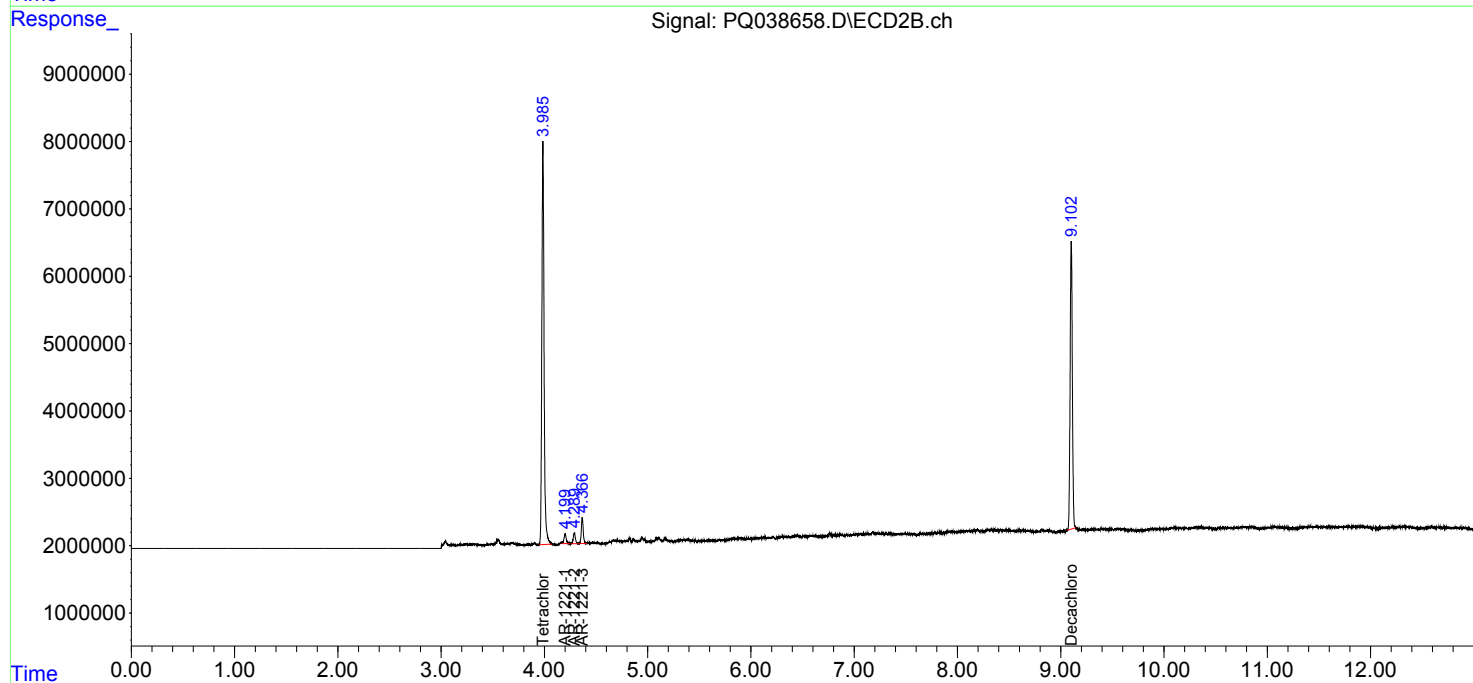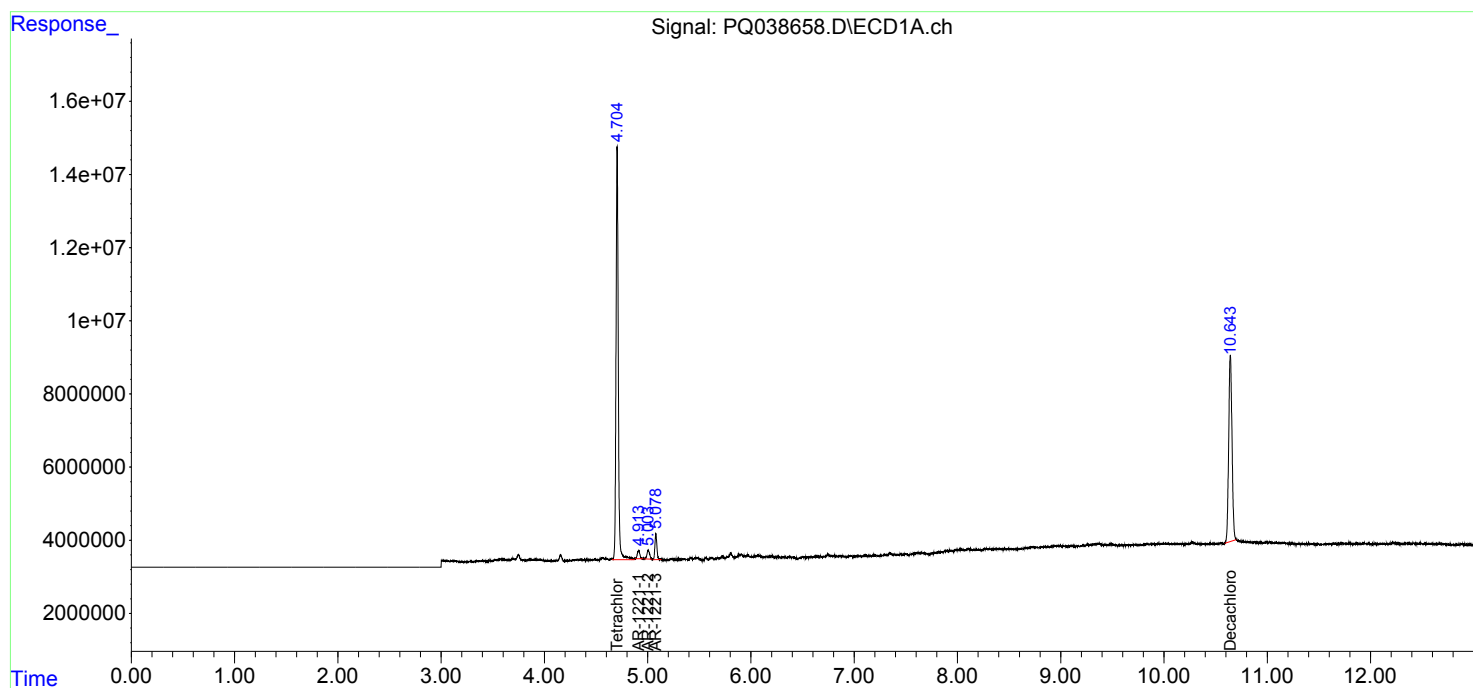


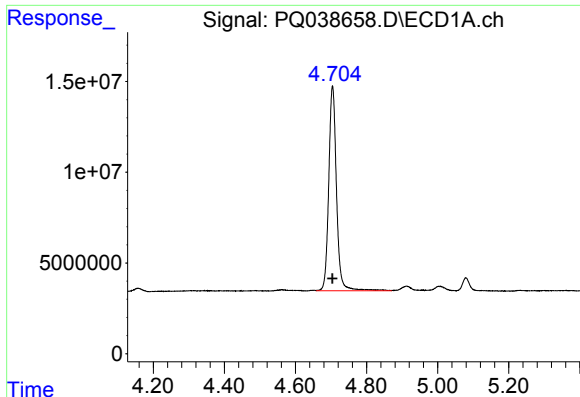

#1 Tetrachloro-m-xylene


R.T.: 4.704 min
Delta R.T.: 0.000 min
Response: 171525278
Conc: 23.19 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

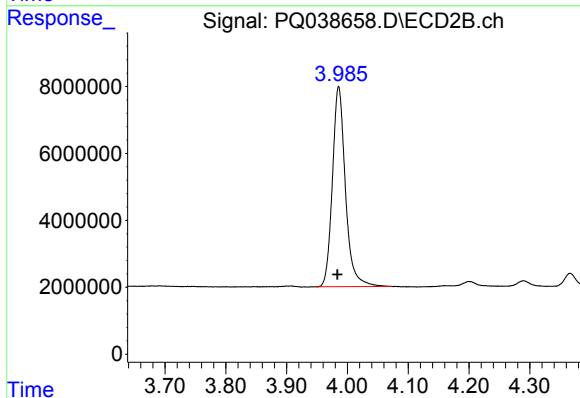


#1 Tetrachloro-m-xylene

R.T.: 3.986 min
Delta R.T.: 0.002 min
Response: 89140584
Conc: 21.75 ng/ml

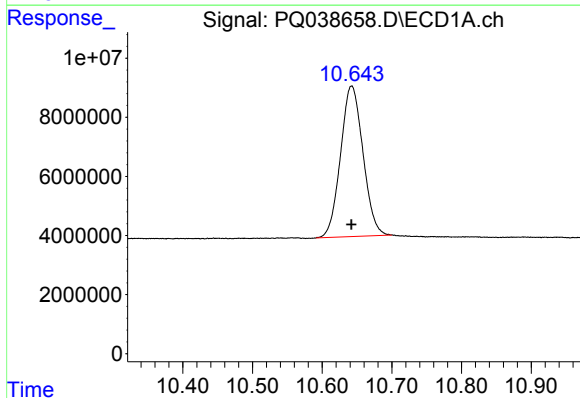


#2 Decachlorobiphenyl

R.T.: 10.642 min
Delta R.T.: 0.000 min
Response: 114075162
Conc: 21.91 ng/ml

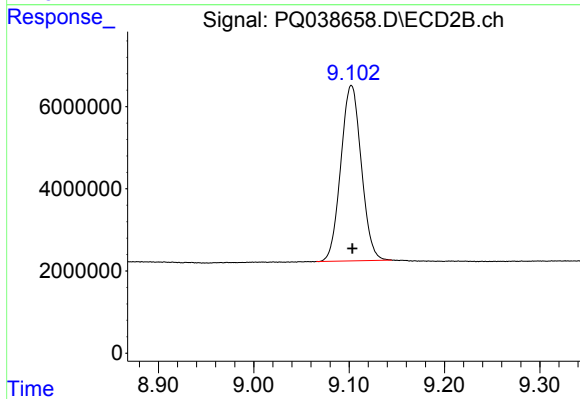

#2 Decachlorobiphenyl


R.T.: 9.102 min
Delta R.T.: 0.000 min
Response: 63767082
Conc: 20.46 ng/ml

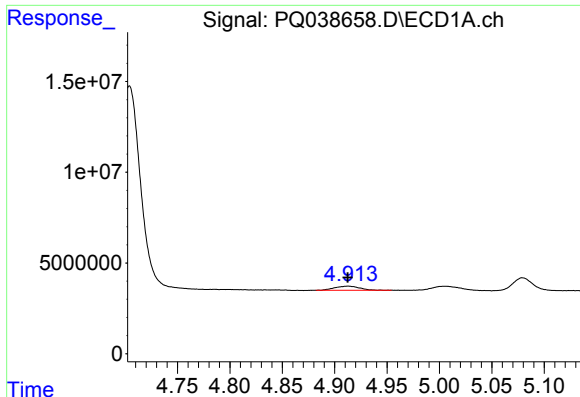

#8 AR-1221-1


R.T.: 4.913 min
Delta R.T.: 0.000 min
Response: 3889475
Conc: 55.17 ng/ml m

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

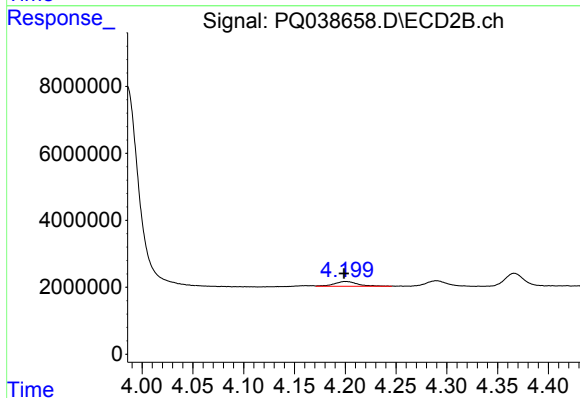


#8 AR-1221-1

R.T.: 4.199 min
Delta R.T.: 0.000 min
Response: 2217412
Conc: 54.96 ng/ml m

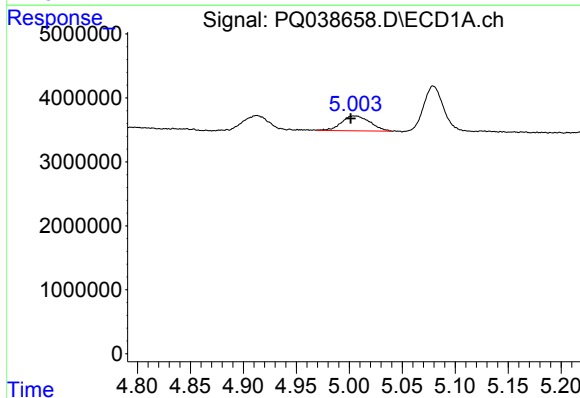


#9 AR-1221-2

R.T.: 5.003 min
Delta R.T.: 0.002 min
Response: 4332279
Conc: 86.40 ng/ml m

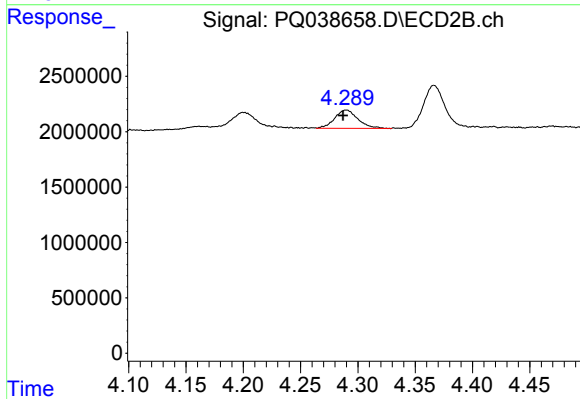

#9 AR-1221-2


R.T.: 4.289 min
Delta R.T.: 0.001 min
Response: 2337117
Conc: 79.46 ng/ml m

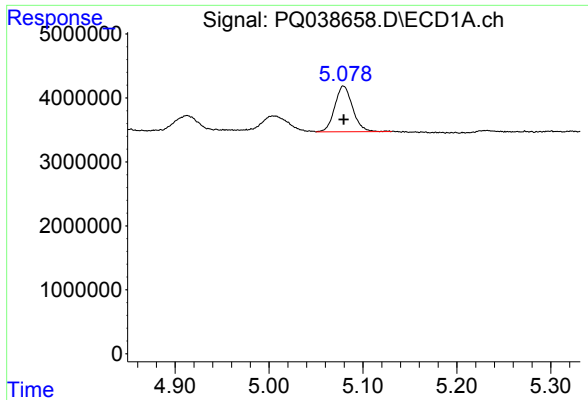

#10 AR-1221-3

R.T.: 5.079 min
Delta R.T.: 0.000 min
Response: 9443171
Conc: 58.91 ng/ml

Instrument :
ECD_Q
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

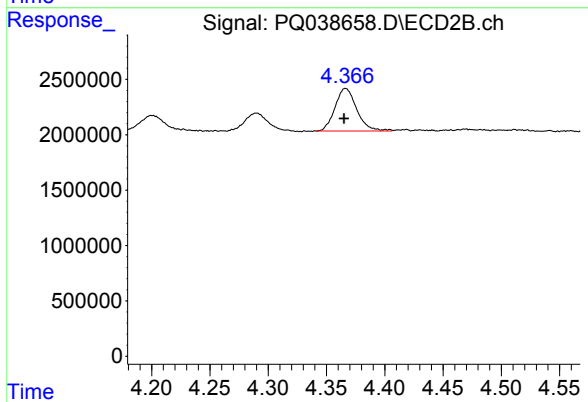

#10 AR-1221-3

R.T.: 4.366 min
Delta R.T.: 0.000 min
Response: 4980448
Conc: 51.74 ng/ml m