

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040323\
 Data File : PQ060769.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Apr 2023 14:37
 Operator : YP\AJ
 Sample : 02161-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 WC-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 03 21:43:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ032723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 27 17:20:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.405	2.763	194.4E6	78722600	24.763	20.028
2) SA Decachlor...	8.583	7.541	136.0E6	88064478	24.093	18.686

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ040323\
Data File : PQ060769.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Apr 2023 14:37
Operator : YP\AJ
Sample : 02161-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
WC-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 03 21:43:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ032723.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 27 17:20:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

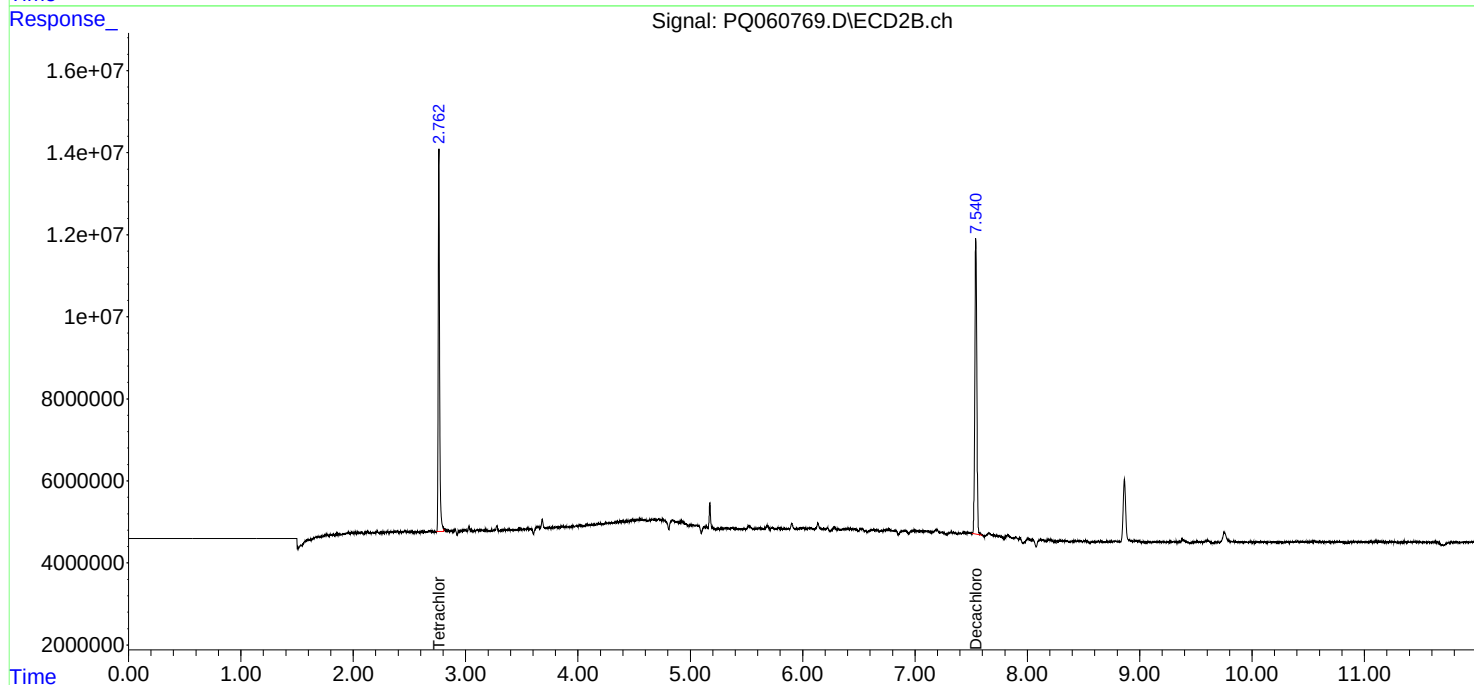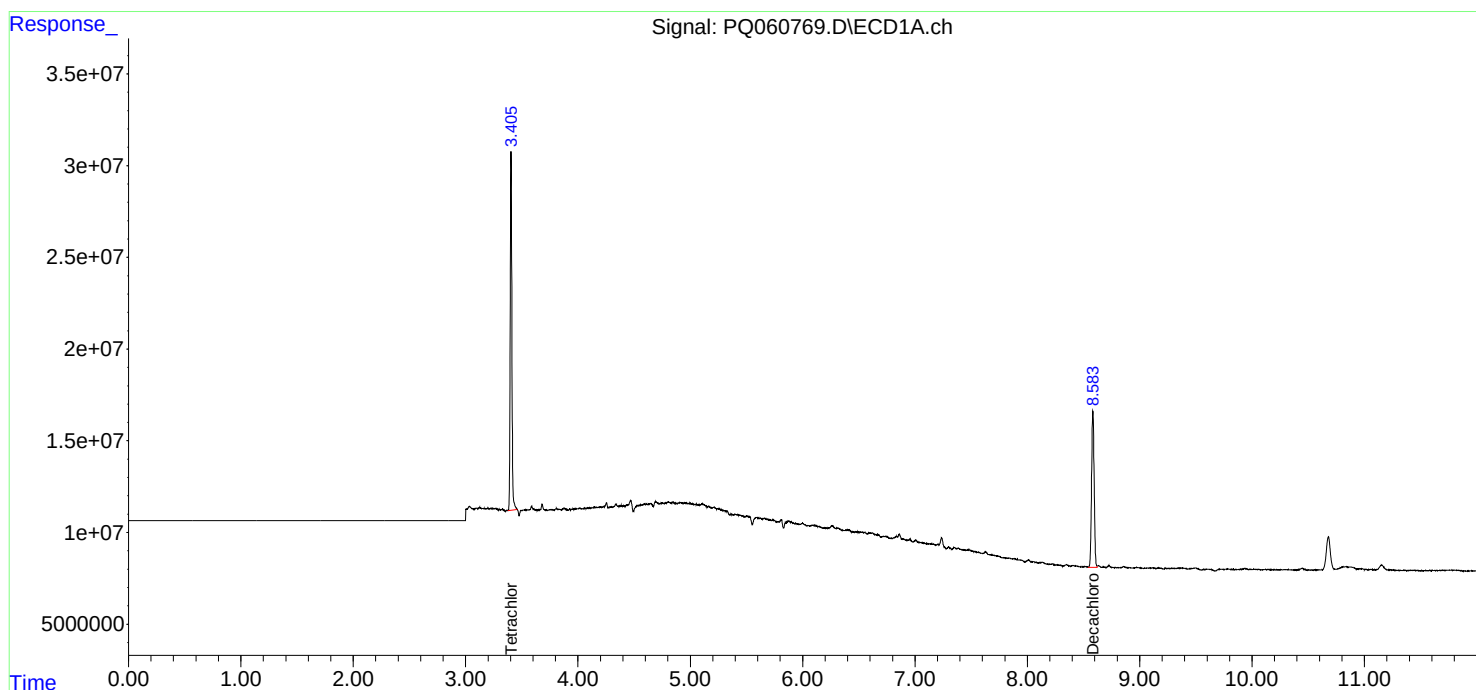


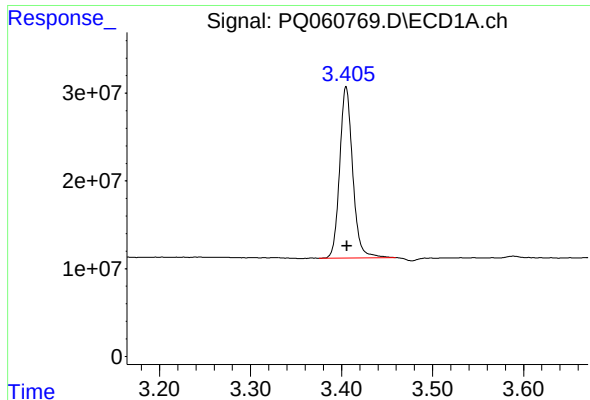

#1 Tetrachloro-m-xylene


R.T.: 3.405 min
Delta R.T.: 0.000 min
Response: 194393298
Conc: 24.76 ng/ml

Instrument :
ECD_Q
ClientSampleId :
WC-6

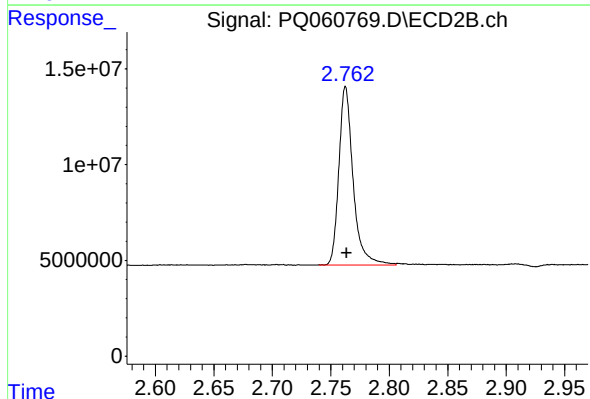


#1 Tetrachloro-m-xylene

R.T.: 2.763 min
Delta R.T.: 0.000 min
Response: 78722600
Conc: 20.03 ng/ml

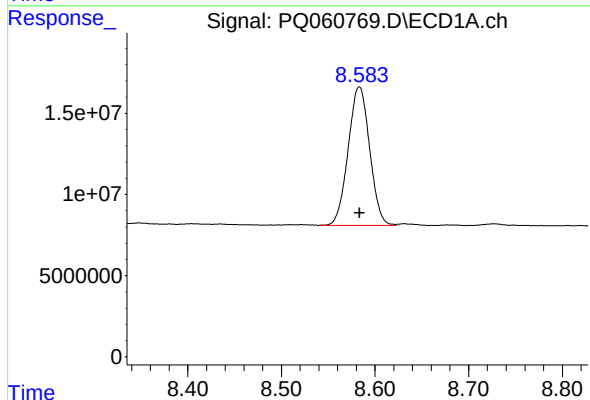

#2 Decachlorobiphenyl

R.T.: 8.583 min
Delta R.T.: 0.000 min
Response: 135960376
Conc: 24.09 ng/ml

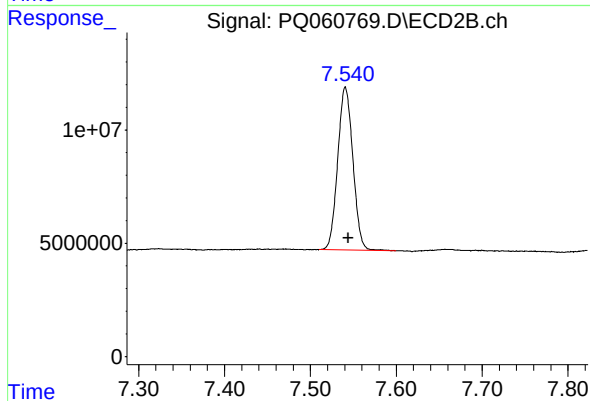

#2 Decachlorobiphenyl

R.T.: 7.541 min
Delta R.T.: -0.003 min
Response: 88064478
Conc: 18.69 ng/ml