

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040521\
 Data File : PL065879.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2021 15:06
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 02:33:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.276	3.781	57613123	60056102	22.116	21.879
28)	SA Decachlor...	7.909	8.727	55851131	51213509	24.115	22.716
Target Compounds							
4)	MA Heptachlor	4.231f	4.943	1019767	600523	0.283	0.170 #
6)	B beta-BHC	4.231	4.630	1019767	10997592	0.640	6.314 #
7)	B delta-BHC	0.000	4.863f	0	336333	N.D.	0.113 #
8)	B Heptachlo...	0.000	5.613	0	880278	N.D.	0.283 #
14)	MA Endrin	5.752	0.000	934176	0	0.346	N.D. #
17)	MA 4,4'-DDT	6.109	0.000	666998	0	0.317	N.D. #
18)	B Endrin al...	6.184	6.748f	358320	509171	0.189	0.268 #
23)	Chlordane-1	4.140f	0.000	963145	0	10.675	N.D. #
27)	Chlordane-5	0.000	6.710	0	736310	N.D.	8.831 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040521\
Data File : PL065879.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2021 15:06
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 02:33:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

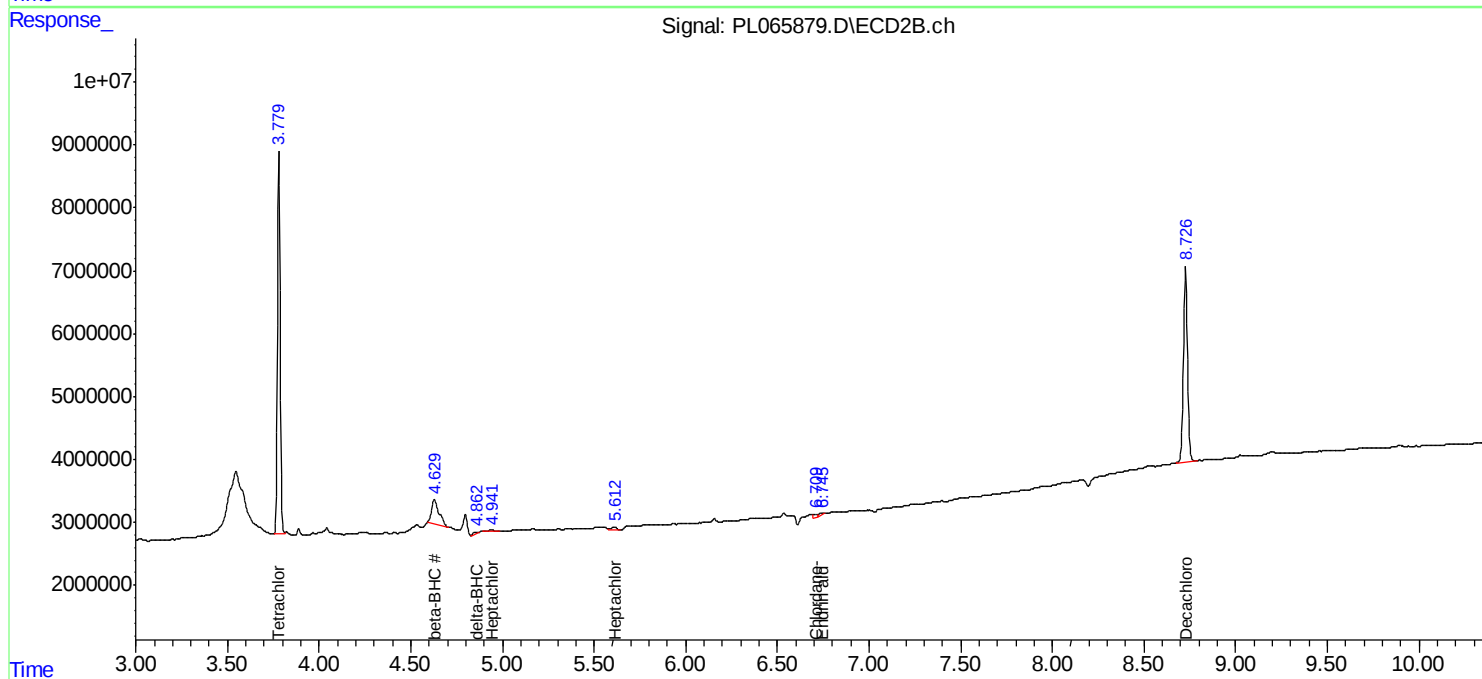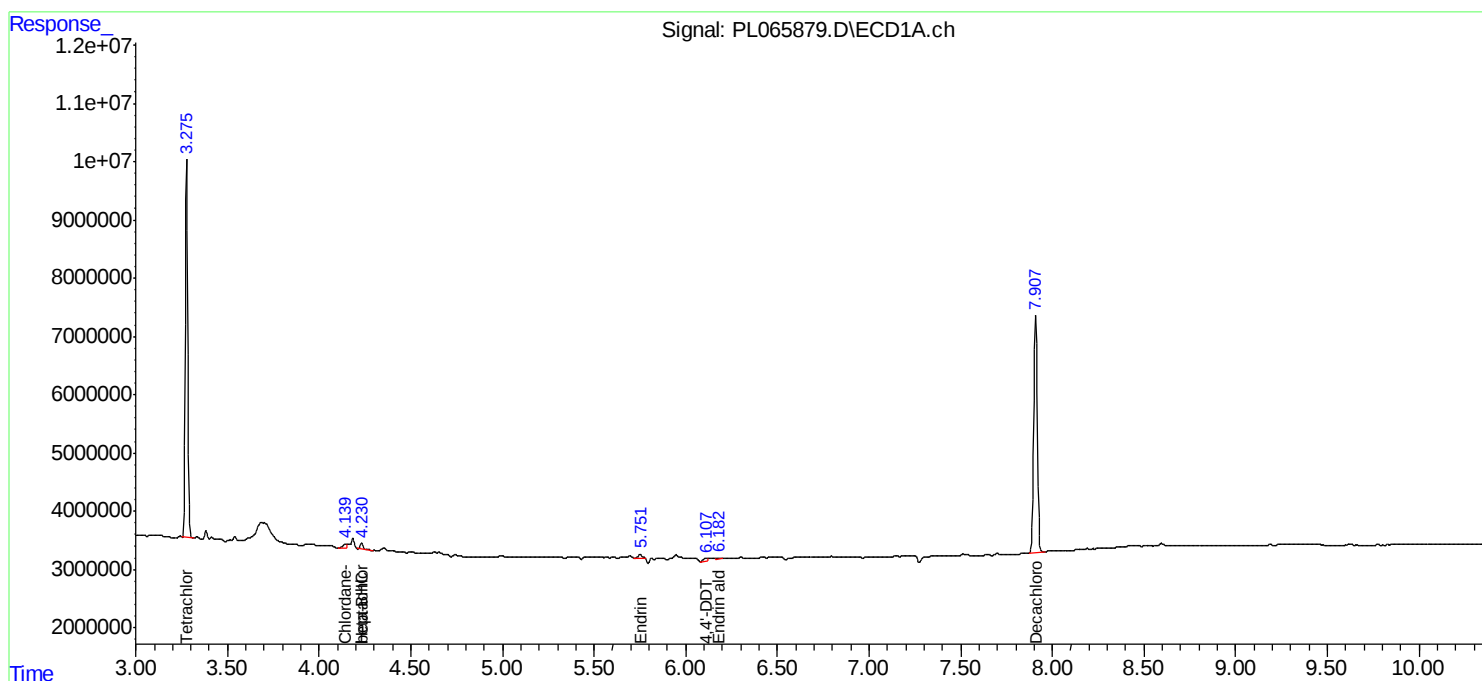


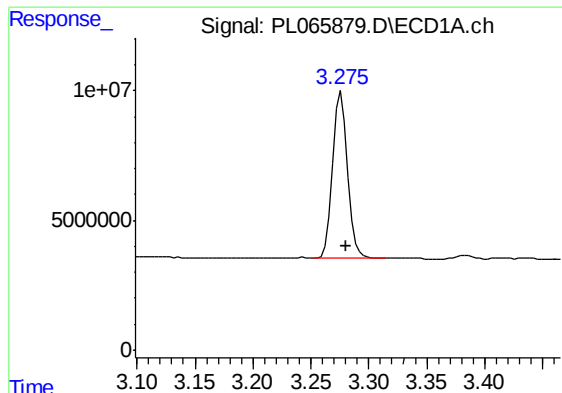

#1 Tetrachloro-m-xylene


R.T.: 3.276 min
Delta R.T.: -0.004 min
Response: 57613123
Conc: 22.12 ng/ml

Instrument :
ECD_Q
ClientSampleId :
I.BLK

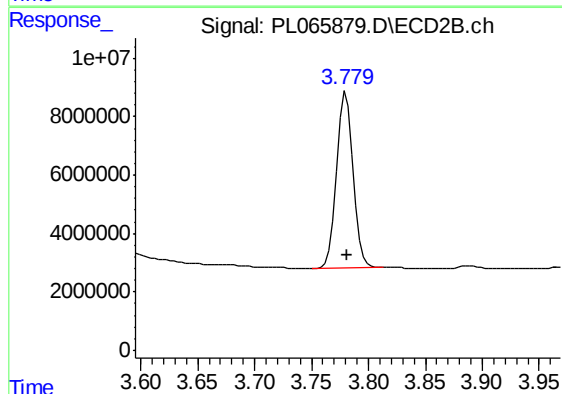


#1 Tetrachloro-m-xylene

R.T.: 3.781 min
Delta R.T.: -0.001 min
Response: 60056102
Conc: 21.88 ng/ml

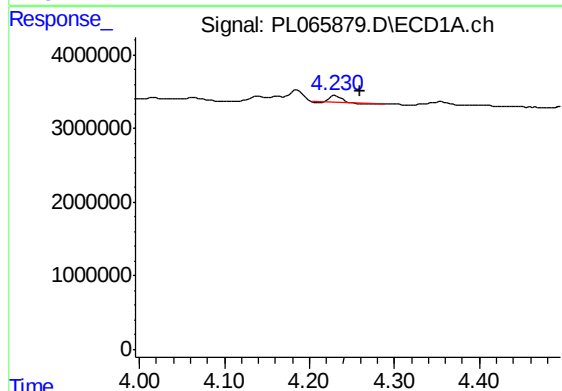


#4 Heptachlor

R.T.: 4.231 min
Delta R.T.: -0.029 min
Response: 1019767
Conc: 0.28 ng/ml

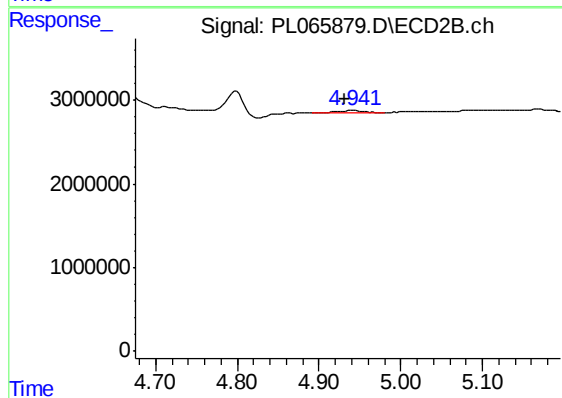

#4 Heptachlor


R.T.: 4.943 min
Delta R.T.: 0.012 min
Response: 600523
Conc: 0.17 ng/ml

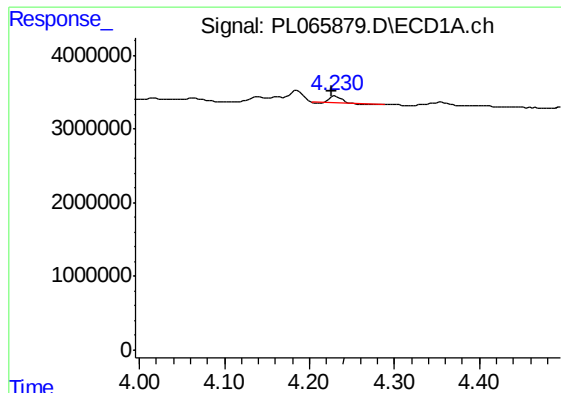

#6 beta-BHC


R.T.: 4.231 min
Delta R.T.: 0.005 min
Response: 1019767
Conc: 0.64 ng/ml

Instrument :
ECD_Q
ClientSampleId :
I.BLK

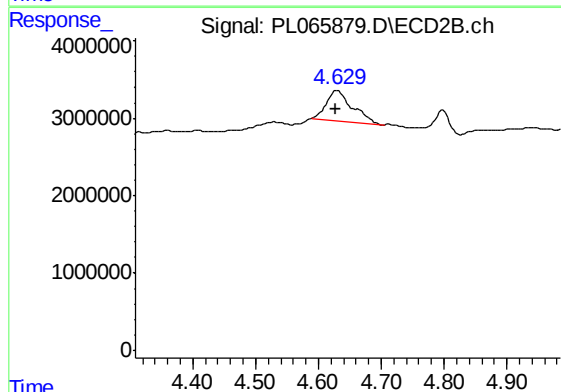


#6 beta-BHC

R.T.: 4.630 min
Delta R.T.: 0.002 min
Response: 10997592
Conc: 6.31 ng/ml

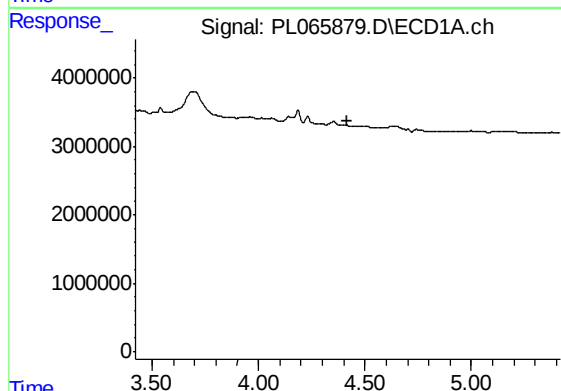


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.419 min
Response: 0
Conc: N.D.

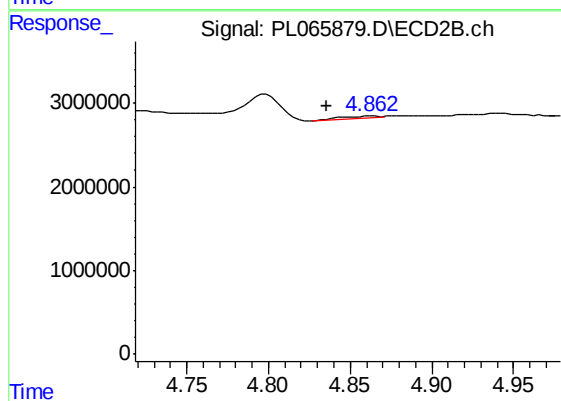

#7 delta-BHC


R.T.: 4.863 min
Delta R.T.: 0.027 min
Response: 336333
Conc: 0.11 ng/ml

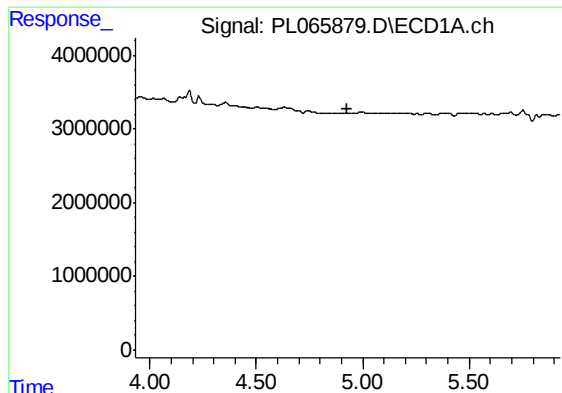

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
I.BLK

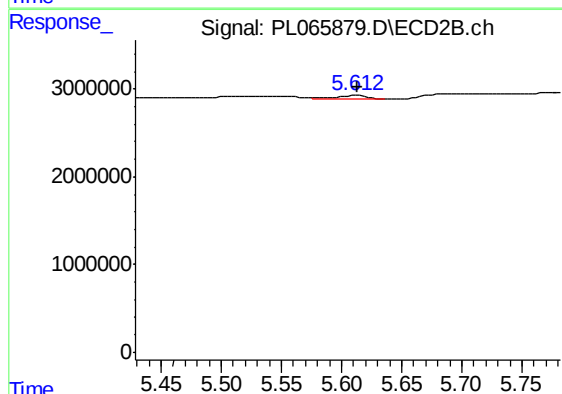


#8 Heptachlor epoxide

R.T.: 5.613 min
Delta R.T.: 0.000 min
Response: 880278
Conc: 0.28 ng/ml

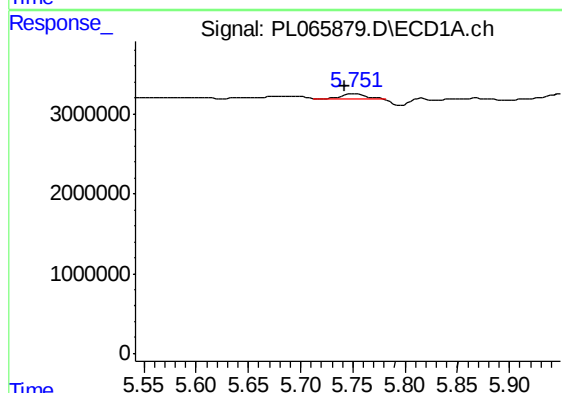


#14 Endrin

R.T.: 5.752 min
Delta R.T.: 0.010 min
Response: 934176
Conc: 0.35 ng/ml

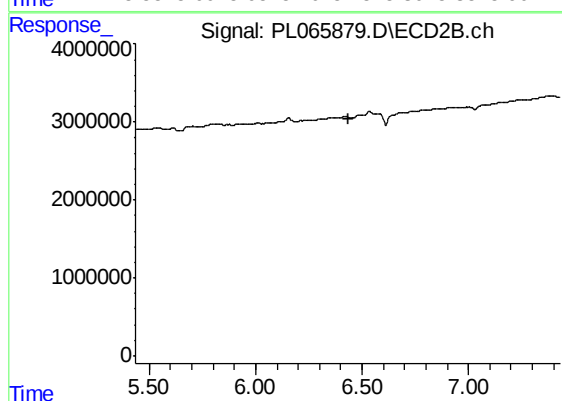

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

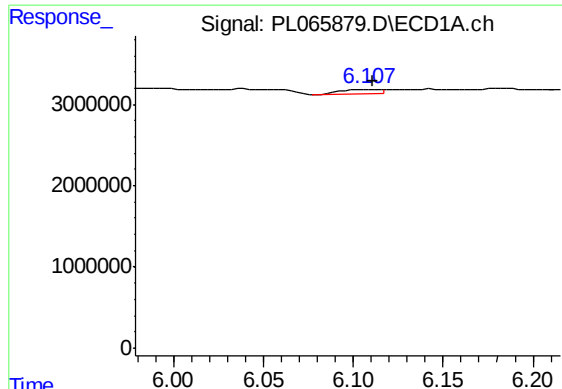

#17 4,4'-DDT


R.T.: 6.109 min
Delta R.T.: -0.003 min
Response: 666998
Conc: 0.32 ng/ml

Instrument :
ECD_Q
ClientSampleId :
I.BLK

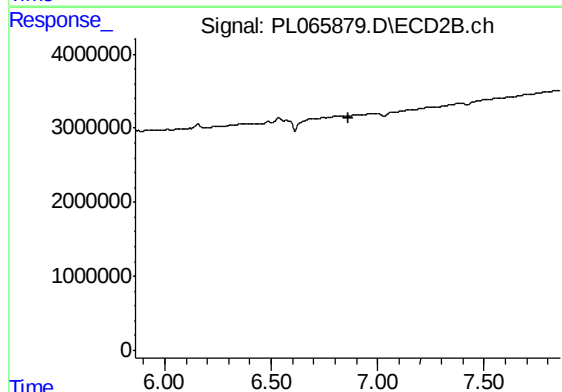


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.861 min
Response: 0
Conc: N.D.

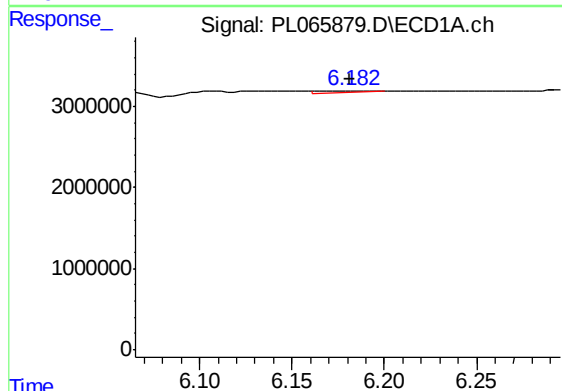


#18 Endrin aldehyde

R.T.: 6.184 min
Delta R.T.: 0.002 min
Response: 358320
Conc: 0.19 ng/ml

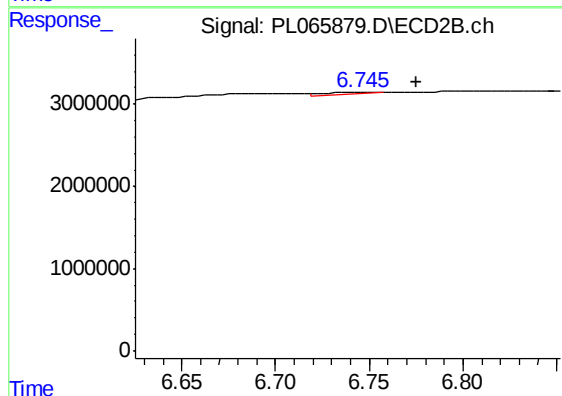

#18 Endrin aldehyde


R.T.: 6.748 min
Delta R.T.: -0.028 min
Response: 509171
Conc: 0.27 ng/ml

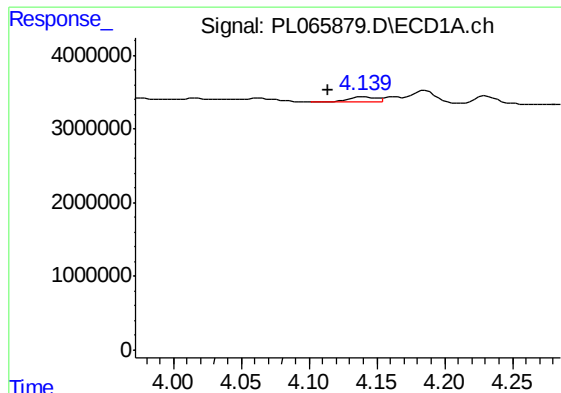

#23 Chlordane-1


R.T.: 4.140 min
Delta R.T.: 0.027 min
Response: 963145
Conc: 10.67 ng/ml

Instrument :
ECD_Q
ClientSampleId :
I.BLK

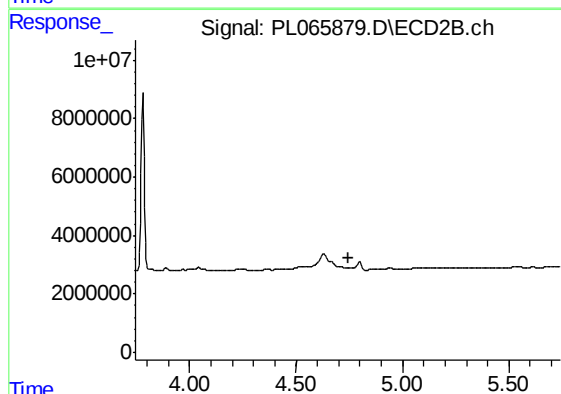


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.745 min
Response: 0
Conc: N.D.

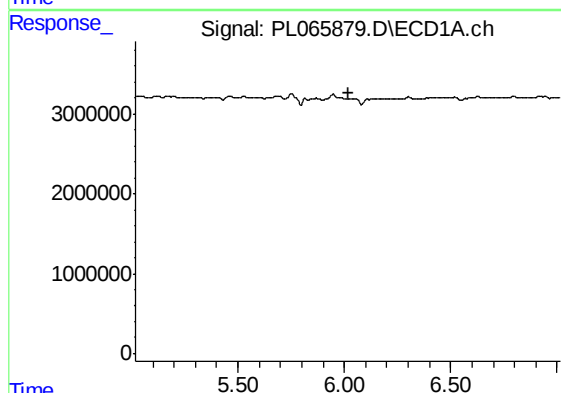


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.017 min
Response: 0
Conc: N.D.

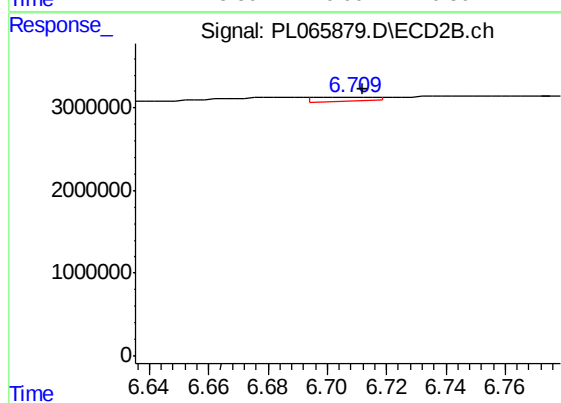

#27 Chlordane-5


R.T.: 6.710 min
Delta R.T.: -0.002 min
Response: 736310
Conc: 8.83 ng/ml

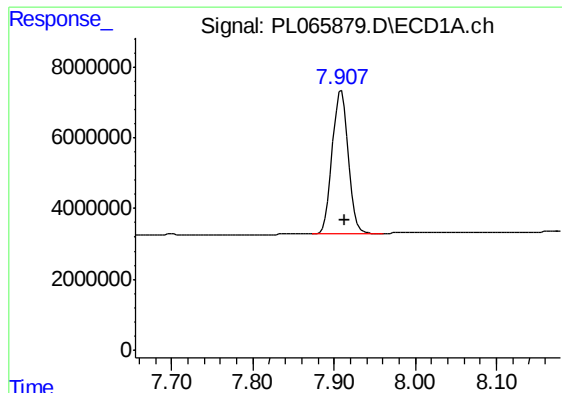

#28 Decachlorobiphenyl

R.T.: 7.909 min
Delta R.T.: -0.005 min
Response: 55851131
Conc: 24.12 ng/ml

Instrument :
ECD_Q
ClientSampleId :
I.BLK

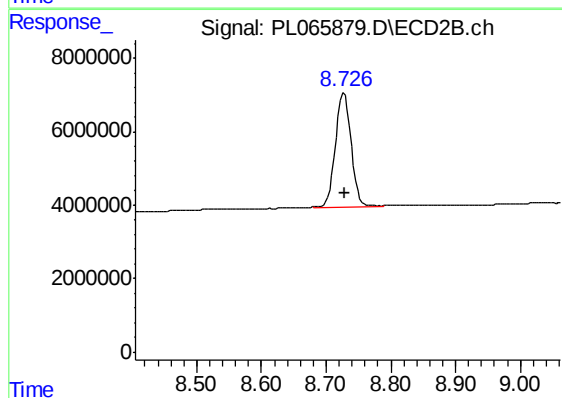

#28 Decachlorobiphenyl

R.T.: 8.727 min
Delta R.T.: 0.000 min
Response: 51213509
Conc: 22.72 ng/ml