

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040521\
 Data File : PL065882.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2021 16:53
 Operator : AR\AJ
 Sample : PB135524BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 PB135524BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 02:34:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.276	3.780	53312871	56374262	20.465	20.537
28)	SA Decachlor...	7.909	8.728	53820416	49317196	23.238	21.875
Target Compounds							
4)	MA Heptachlor	0.000	4.944	0	723846	N.D.	0.205 #
6)	B beta-BHC	0.000	4.628	0	4916529	N.D.	2.823 #
8)	B Heptachlo...	0.000	5.612	0	773602	N.D.	0.249 #
14)	MA Endrin	5.752	0.000	445127	0	0.165	N.D. #
15)	B Endosulfa...	0.000	6.677f	0	2409759	N.D.	1.020 #
20)	A Methoxychlor	0.000	7.341	0	114674	N.D.	0.091 #
23)	Chlordane-1	4.141f	0.000	857936	0	9.509	N.D. #
27)	Chlordane-5	0.000	6.706	0	424939	N.D.	5.097 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040521\
Data File : PL065882.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2021 16:53
Operator : AR\AJ
Sample : PB135524BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
PB135524BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 02:34:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

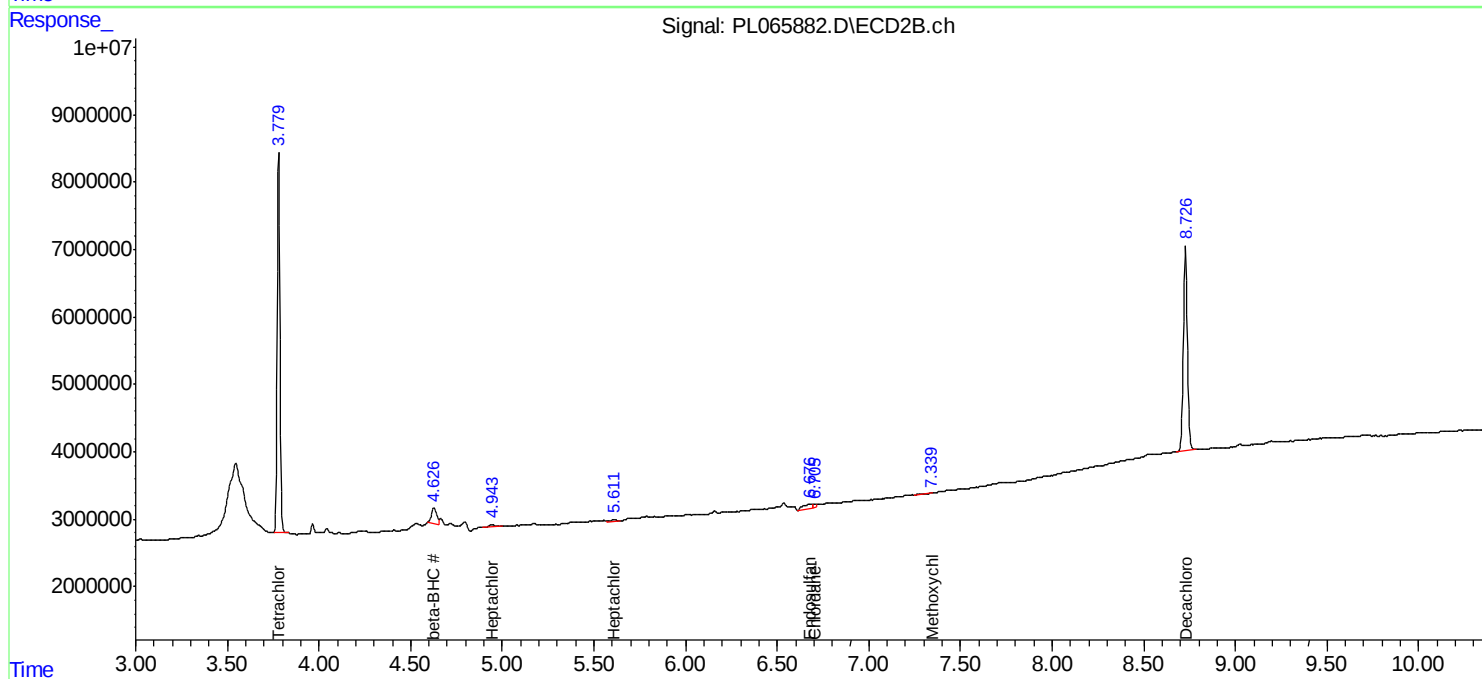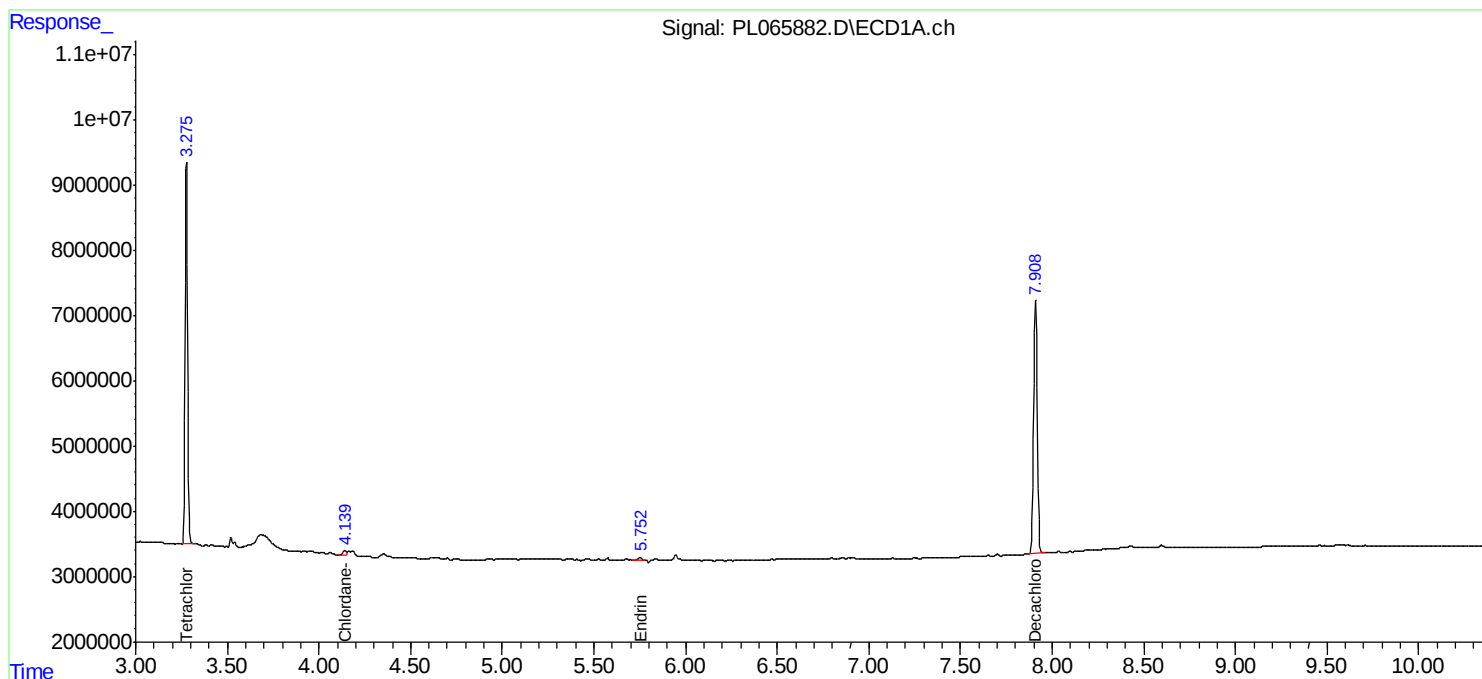


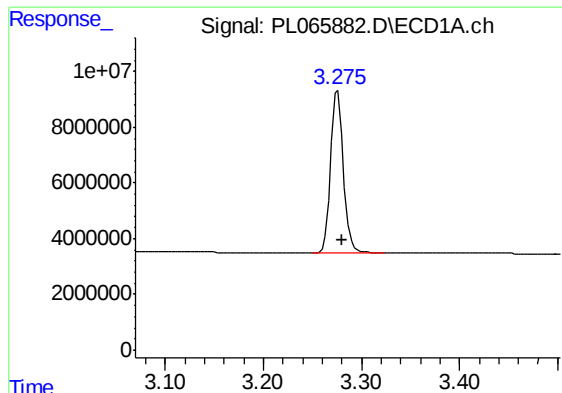

#1 Tetrachloro-m-xylene


R.T.: 3.276 min
Delta R.T.: -0.004 min
Response: 53312871
Conc: 20.47 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PB135524BL

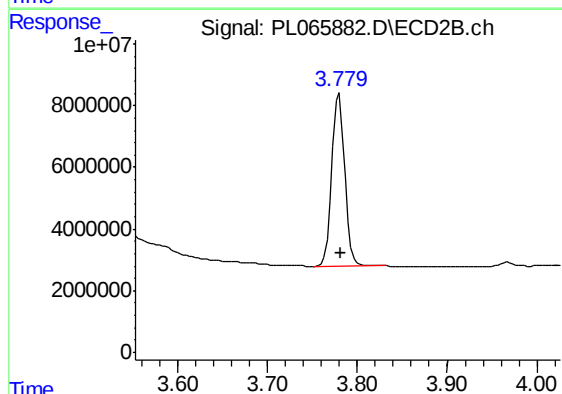


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.002 min
Response: 56374262
Conc: 20.54 ng/ml

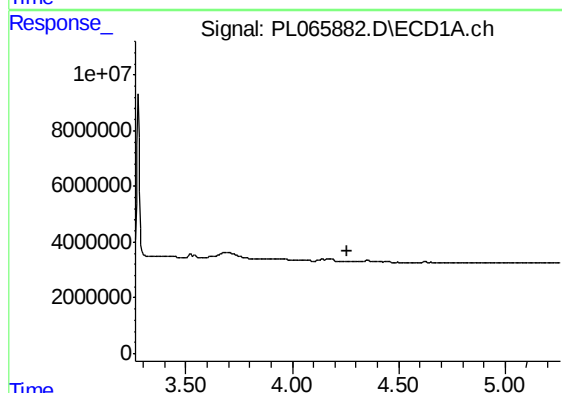


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.260 min
Response: 0
Conc: N.D.

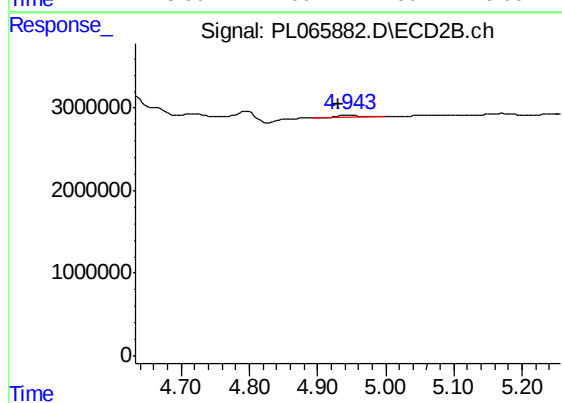

#4 Heptachlor


R.T.: 4.944 min
Delta R.T.: 0.013 min
Response: 723846
Conc: 0.21 ng/ml

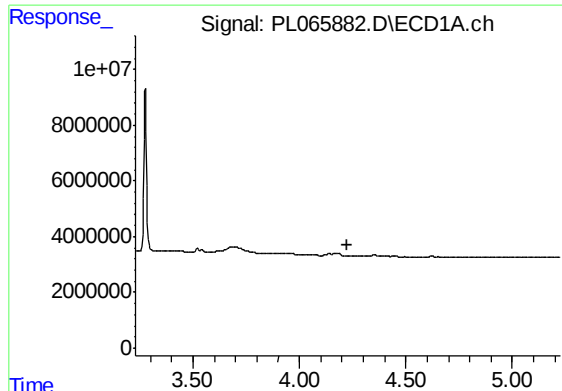

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.226 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
PB135524BL

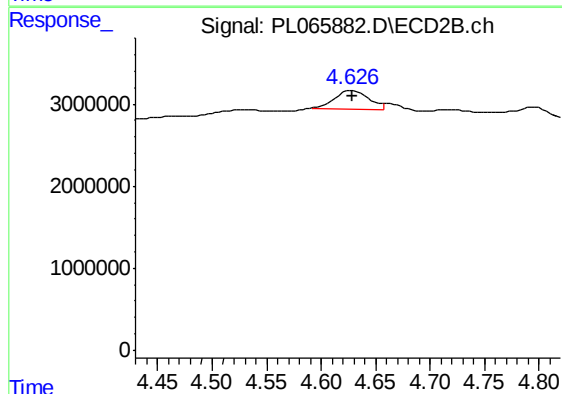


#6 beta-BHC

R.T.: 4.628 min
Delta R.T.: 0.000 min
Response: 4916529
Conc: 2.82 ng/ml

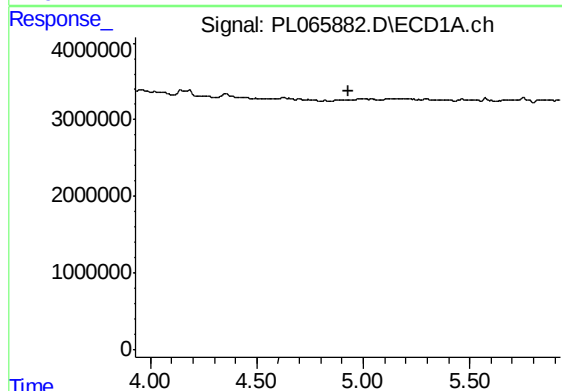


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.929 min
Response: 0
Conc: N.D.

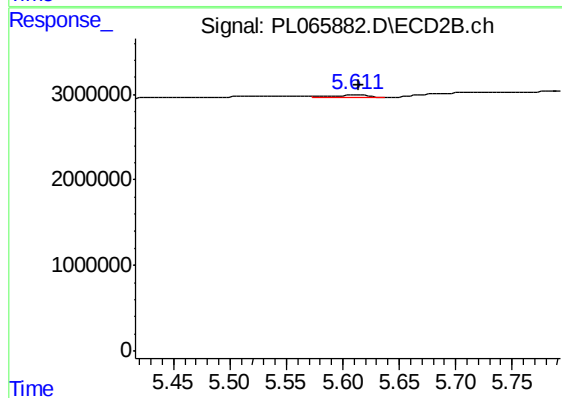

#8 Heptachlor epoxide


R.T.: 5.612 min
Delta R.T.: -0.001 min
Response: 773602
Conc: 0.25 ng/ml

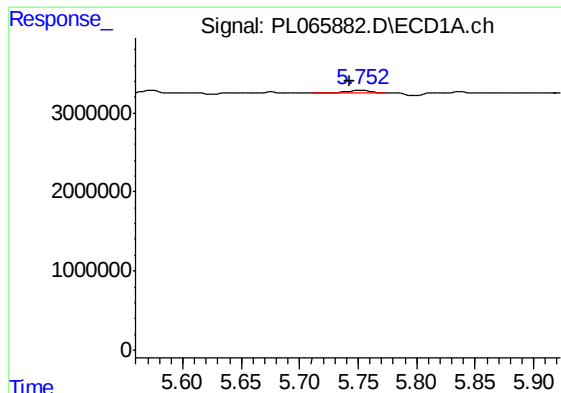

#14 Endrin


R.T.: 5.752 min
Delta R.T.: 0.010 min
Response: 445127
Conc: 0.16 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PB135524BL

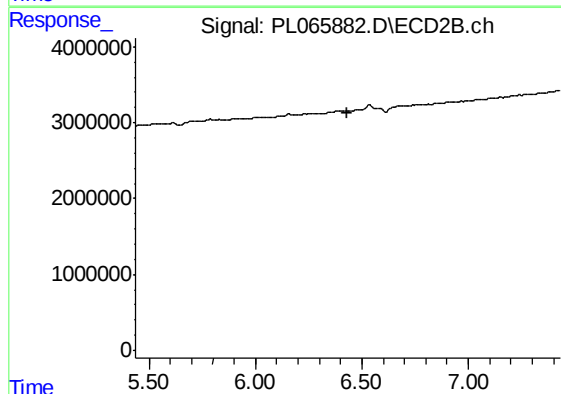


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

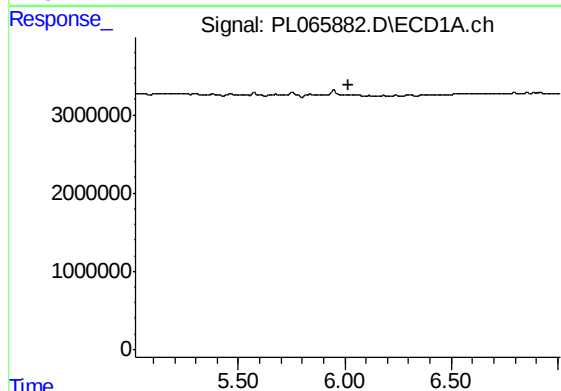


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.015 min
Response: 0
Conc: N.D.

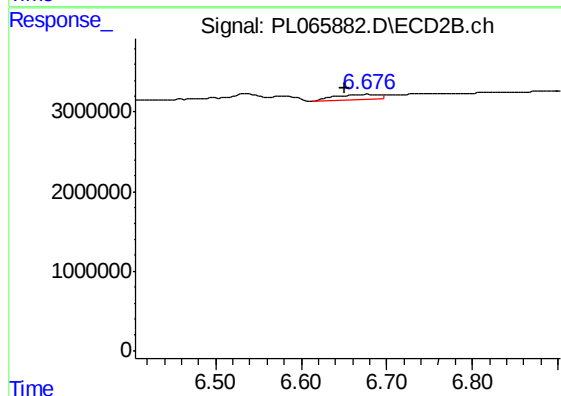

#15 Endosulfan II


R.T.: 6.677 min
Delta R.T.: 0.025 min
Response: 2409759
Conc: 1.02 ng/ml

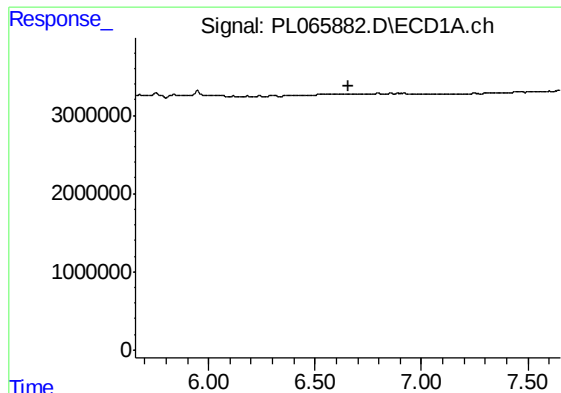

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.656 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
PB135524BL

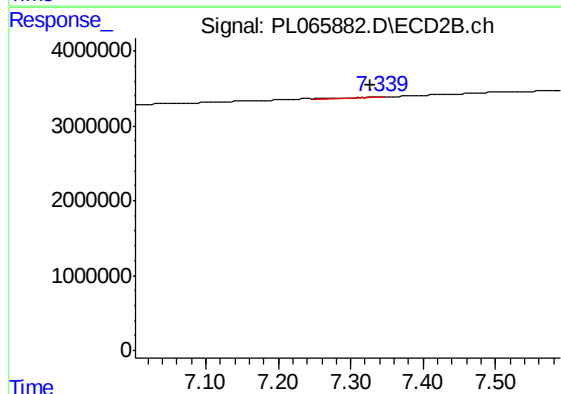


#20 Methoxychlor

R.T.: 7.341 min
Delta R.T.: 0.015 min
Response: 114674
Conc: 0.09 ng/ml

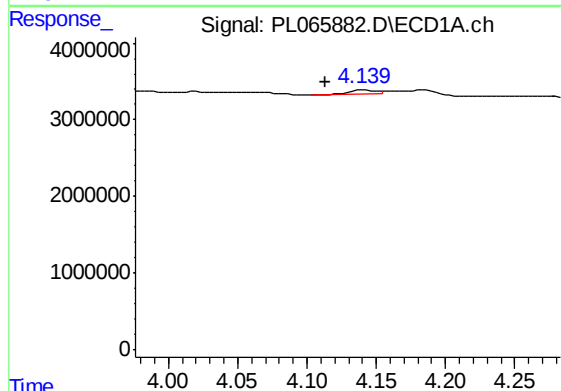


#23 Chlordane-1

R.T.: 4.141 min
Delta R.T.: 0.027 min
Response: 857936
Conc: 9.51 ng/ml

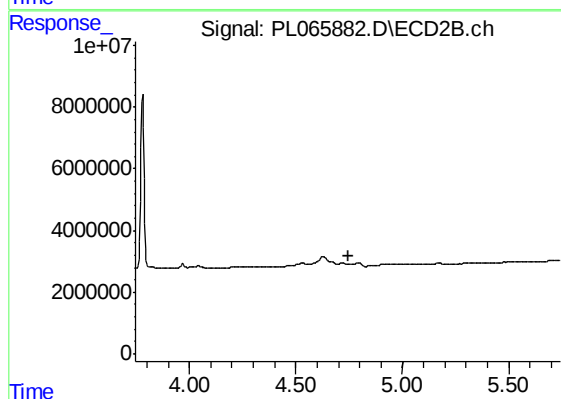

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.745 min
Response: 0
Conc: N.D.

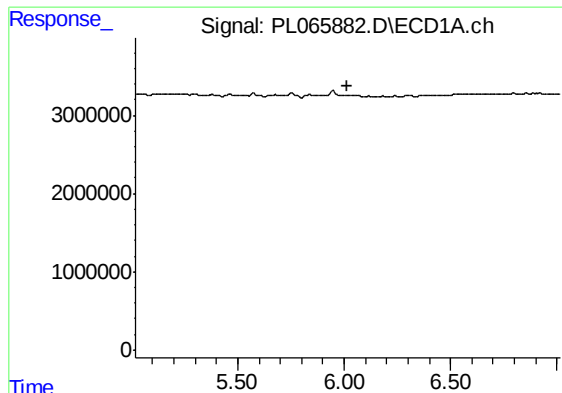

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.017 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
PB135524BL

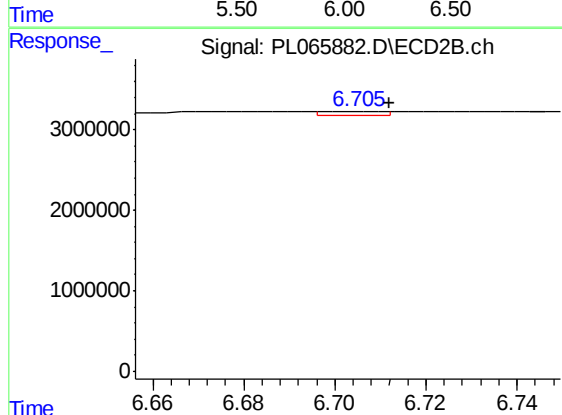


#27 Chlordane-5

R.T.: 6.706 min
Delta R.T.: -0.006 min
Response: 424939
Conc: 5.10 ng/ml

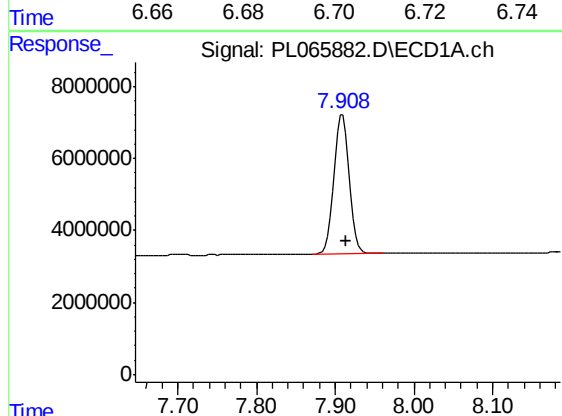

#28 Decachlorobiphenyl

R.T.: 7.909 min
Delta R.T.: -0.004 min
Response: 53820416
Conc: 23.24 ng/ml

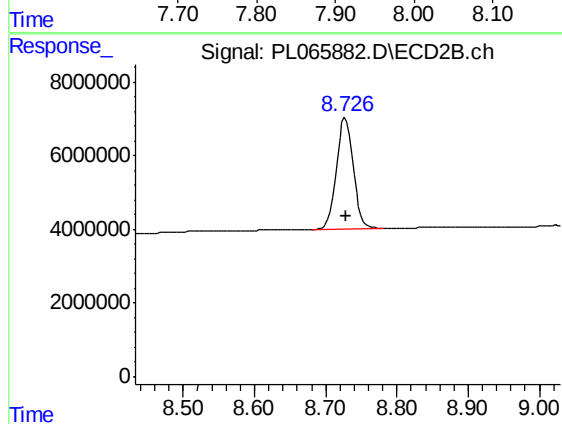

#28 Decachlorobiphenyl

R.T.: 8.728 min
Delta R.T.: 0.000 min
Response: 49317196
Conc: 21.87 ng/ml