

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040521\
 Data File : PL065883.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2021 17:07
 Operator : AR\AJ
 Sample : PB135533TB
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 PB135533TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 02:35:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 31 15:57:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.276	3.780	50948025	54326388	19.558	19.791
28)	SA Decachlor...	7.908	8.728	51010607	46589810	22.025	20.665
Target Compounds							
2)	A alpha-BHC	3.687f	0.000	1399796	0	0.342	N.D. #
4)	MA Heptachlor	0.000	4.941	0	508907	N.D.	0.144 #
6)	B beta-BHC	0.000	4.631	0	7732311	N.D.	4.439 #
8)	B Heptachlo...	0.000	5.610	0	484875	N.D.	0.156 #
18)	B Endrin al...	0.000	6.750f	0	60324	N.D.	0.032 #
20)	A Methoxychlor	0.000	7.347f	0	126130	N.D.	0.100 #
21)	B Endrin ke...	0.000	7.457	0	59228	N.D.	0.023 #
23)	Chlordane-1	4.141f	0.000	786576	0	8.718	N.D. #
27)	Chlordane-5	0.000	6.683f	0	316822	N.D.	3.800 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL040521\
Data File : PL065883.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2021 17:07
Operator : AR\AJ
Sample : PB135533TB
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
PB135533TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 02:35:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL033121.M
Quant Title : GC Extractables
QLast Update : Wed Mar 31 15:57:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

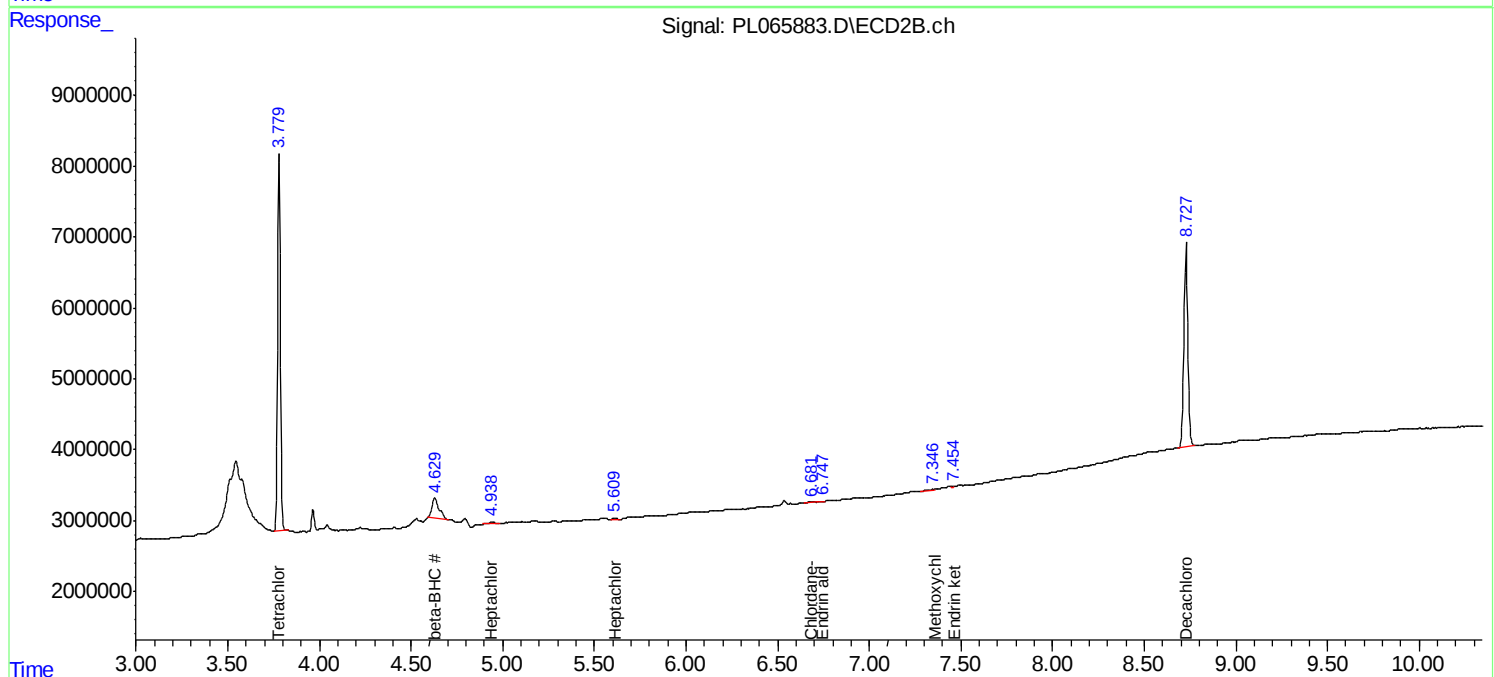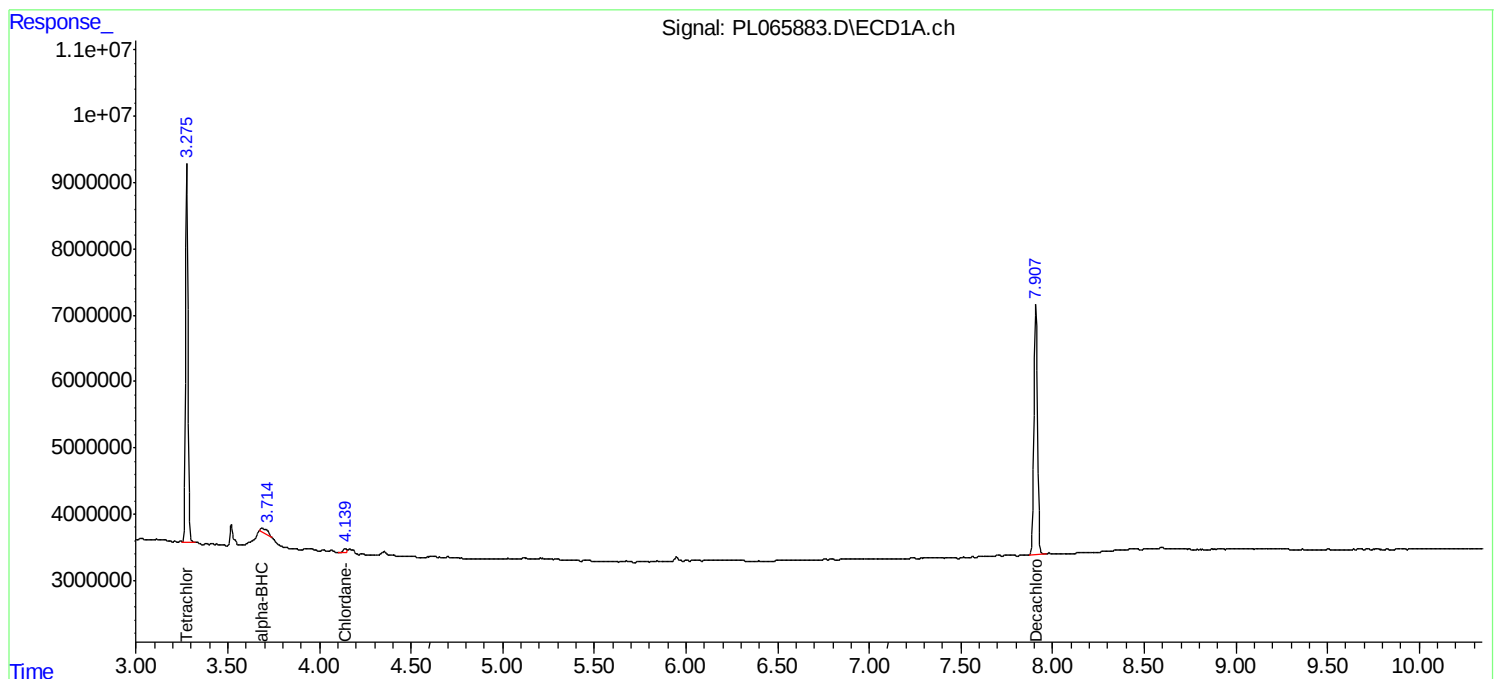


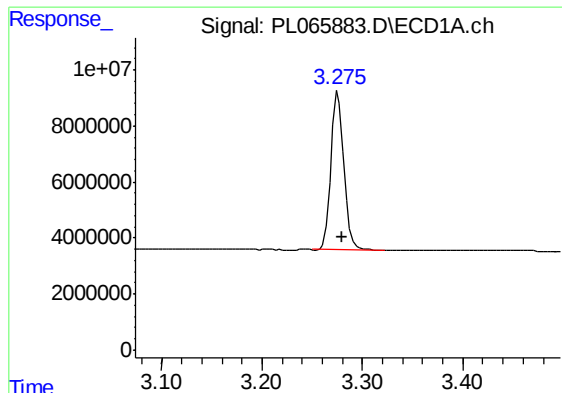

#1 Tetrachloro-m-xylene


R.T.: 3.276 min
Delta R.T.: -0.004 min
Response: 50948025
Conc: 19.56 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PB135533TB

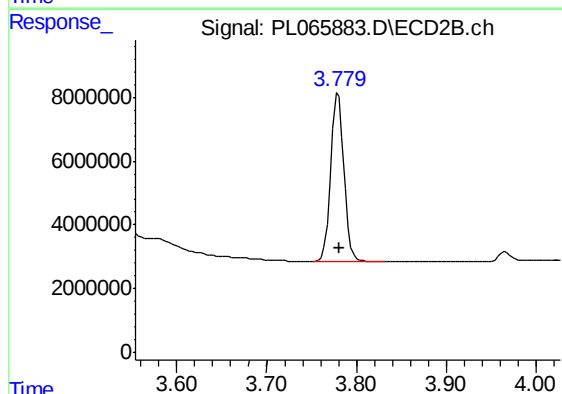


#1 Tetrachloro-m-xylene

R.T.: 3.780 min
Delta R.T.: -0.002 min
Response: 54326388
Conc: 19.79 ng/ml

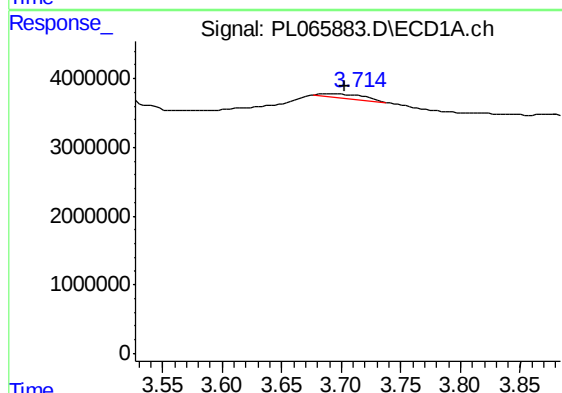


#2 alpha-BHC

R.T.: 3.687 min
Delta R.T.: -0.015 min
Response: 1399796
Conc: 0.34 ng/ml

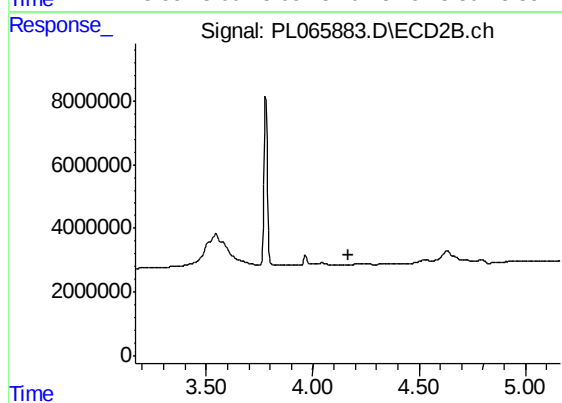

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.167 min
Response: 0
Conc: N.D.

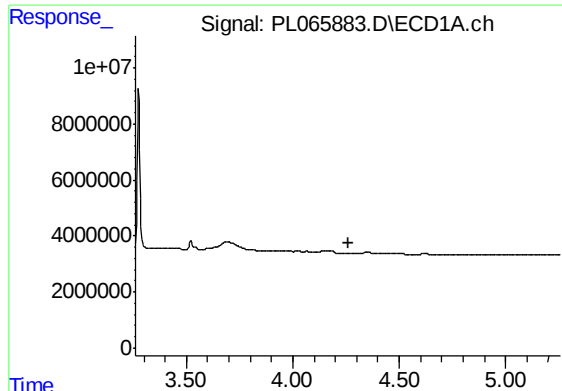

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.260 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
PB135533TB

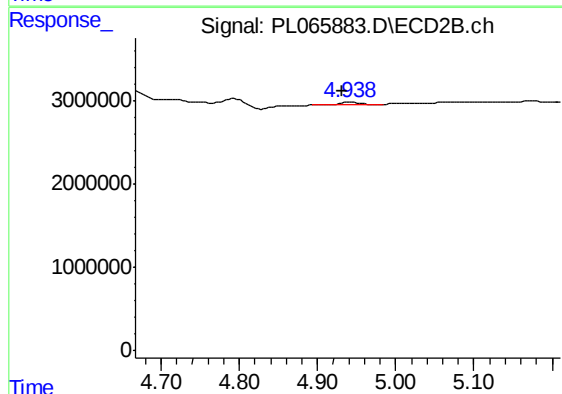


#4 Heptachlor

R.T.: 4.941 min
Delta R.T.: 0.010 min
Response: 508907
Conc: 0.14 ng/ml

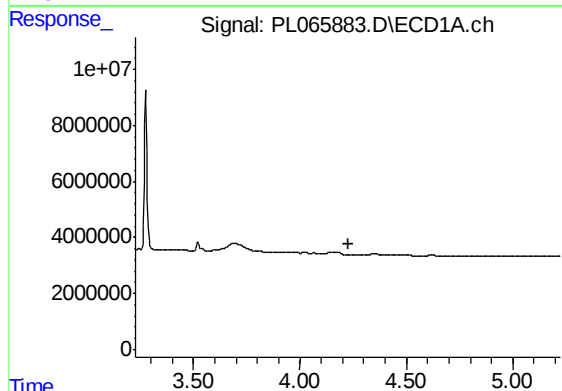


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.226 min
Response: 0
Conc: N.D.

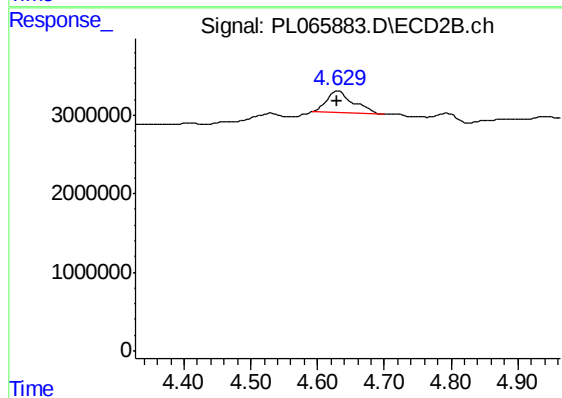

#6 beta-BHC


R.T.: 4.631 min
Delta R.T.: 0.002 min
Response: 7732311
Conc: 4.44 ng/ml

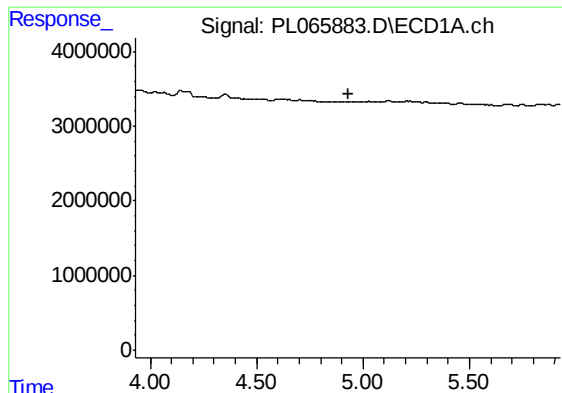

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
PB135533TB

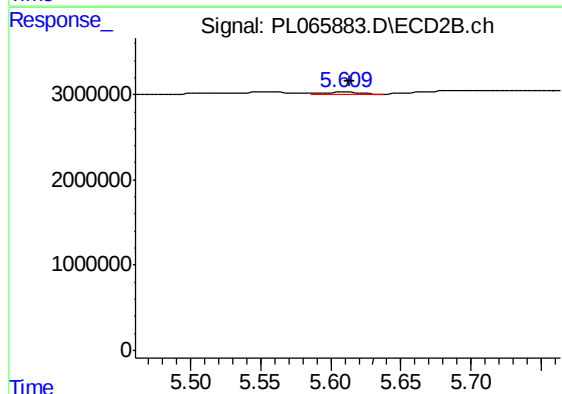


#8 Heptachlor epoxide

R.T.: 5.610 min
Delta R.T.: -0.004 min
Response: 484875
Conc: 0.16 ng/ml

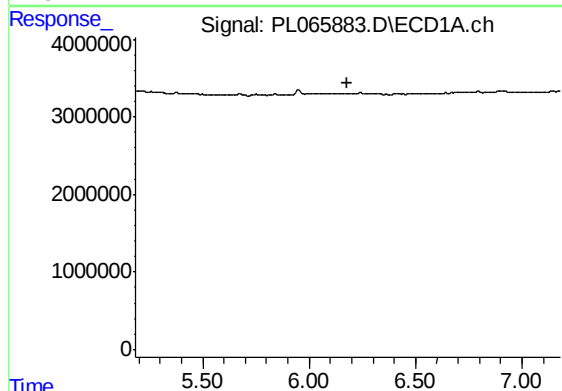


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.181 min
Response: 0
Conc: N.D.

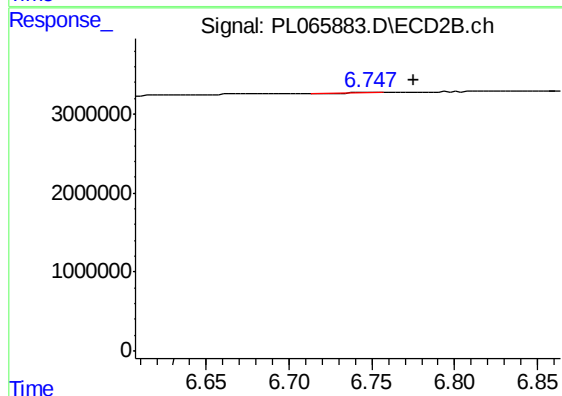

#18 Endrin aldehyde


R.T.: 6.750 min
Delta R.T.: -0.026 min
Response: 60324
Conc: 0.03 ng/ml

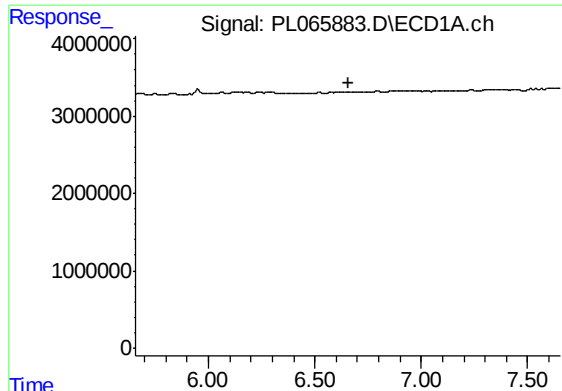

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.656 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
PB135533TB

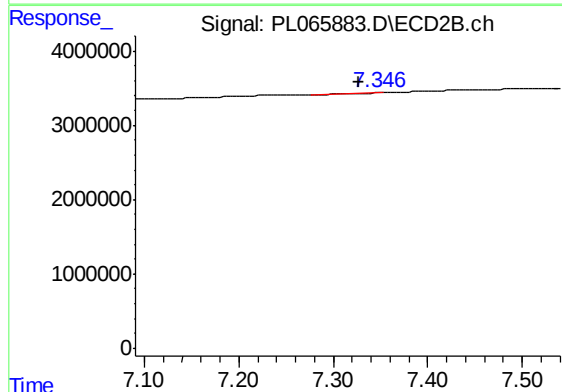


#20 Methoxychlor

R.T.: 7.347 min
Delta R.T.: 0.021 min
Response: 126130
Conc: 0.10 ng/ml

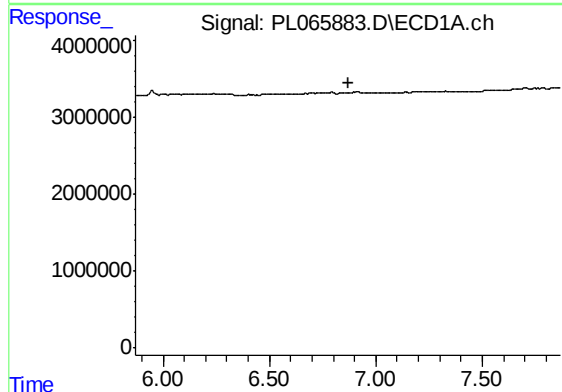


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.870 min
Response: 0
Conc: N.D.

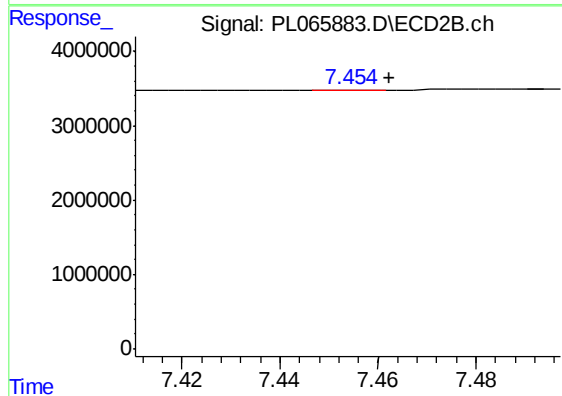

#21 Endrin ketone


R.T.: 7.457 min
Delta R.T.: -0.005 min
Response: 59228
Conc: 0.02 ng/ml

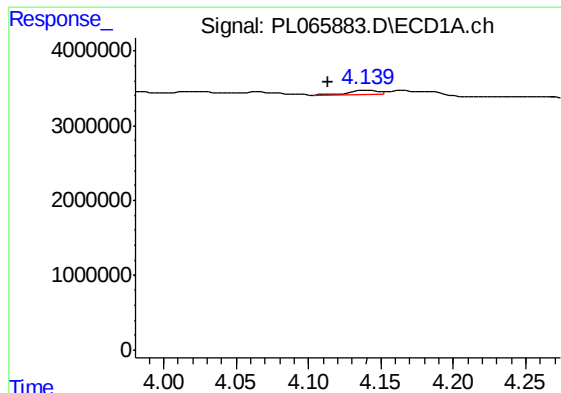

#23 Chlordane-1


R.T.: 4.141 min
Delta R.T.: 0.027 min
Response: 786576
Conc: 8.72 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PB135533TB

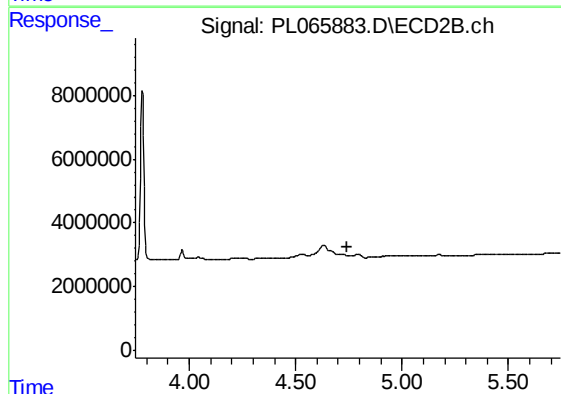


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.745 min
Response: 0
Conc: N.D.

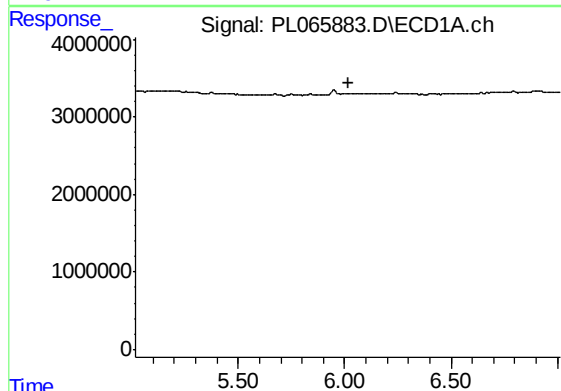


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.017 min
Response: 0
Conc: N.D.

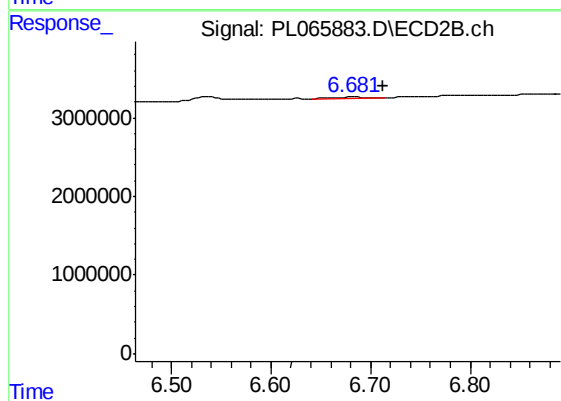

#27 Chlordane-5


R.T.: 6.683 min
Delta R.T.: -0.029 min
Response: 316822
Conc: 3.80 ng/ml

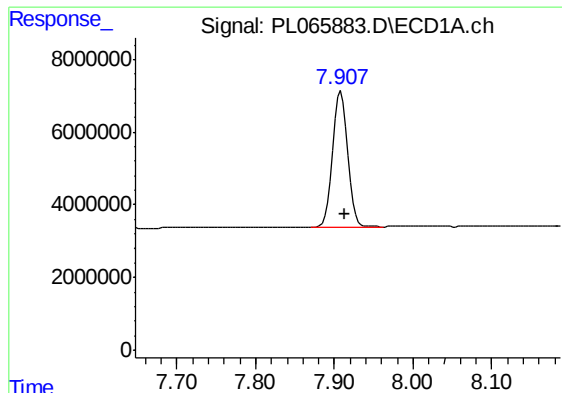

#28 Decachlorobiphenyl

R.T.: 7.908 min
Delta R.T.: -0.005 min
Response: 51010607
Conc: 22.03 ng/ml

Instrument :
ECD_Q
ClientSampleId :
PB135533TB

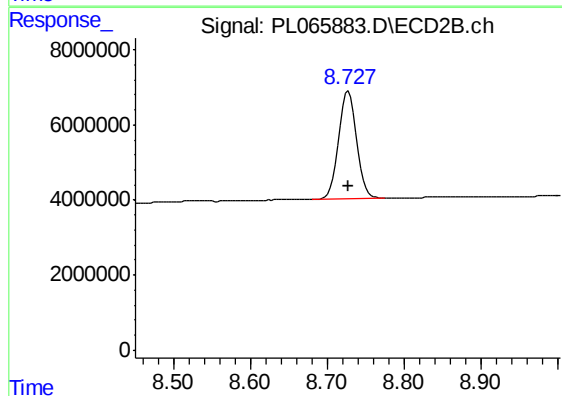

#28 Decachlorobiphenyl

R.T.: 8.728 min
Delta R.T.: 0.000 min
Response: 46589810
Conc: 20.67 ng/ml