Quantitation Report (Not Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ041219\
Data File : PQ039070.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2019 17:37
Operator : AJ\SJ
Sample : K1560-09
Misc : AR1242 MDL 25 PPB
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 00:57:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ041219.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Apr 13 00:36:36 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	
	System Monitoring Compounds							
1) SA	Tetrachlo...	5.720	4.816	75001100	37339614	16.923	16.745	
2) SA	Decachlor...	12.122	10.576	140.7E6	71760188	20.278	20.566	
	Target Compounds							
3) L1	AR-1016-1	7.165	6.267	3830810	2839641	21.080	27.963	#
4) L1	AR-1016-2	7.189	6.289	5185677	4094839	19.138	27.647	#
5) L1	AR-1016-3	7.261	6.503	3430935	1509359	20.591	20.229	
6) L1	AR-1016-4	7.374	6.557	2449757	765193	17.679	12.273	#
7) L1	AR-1016-5	7.708	6.810	3306250	1780813	23.296	20.068	
9) L2	AR-1221-2	6.112	5.237	2066919	809208	60.887	38.806	#
10) L2	AR-1221-3	6.205	5.343	2116982	895222	19.281	14.590	
11) L3	AR-1232-1	6.205	5.343	2116982	895222	26.616	23.607	
12) L3	AR-1232-2	6.848	6.289	2845347	4094839	68.013	88.106	#
13) L3	AR-1232-3	7.189	6.503	5185677	1509359	58.249	71.161	
14) L3	AR-1232-4	7.374	6.606	2449757	1318915	47.808	62.647	#
15) L3	AR-1232-5	7.478	6.810	2325765	1780813	56.505	73.065	#
16) L4	AR-1242-1	7.165	6.267	3830810	2839641	34.162	48.376	#
17) L4	AR-1242-2	7.189	6.289	5185677	4094839	31.577	47.645	#
18) L4	AR-1242-3	7.261	6.503	3430935	1509359	31.500	35.749	
19) L4	AR-1242-4	7.374	6.606	2449757	1318915	28.306	29.449	
20) L4	AR-1242-5	8.195	7.218	4545582	2500125	46.011	38.555	
21) L5	AR-1248-1	7.165	6.267	3830810	2839641	46.334	63.720	#
22) L5	AR-1248-2	7.478	6.557	2325765	765193	20.356	12.816	#
23) L5	AR-1248-3	7.708	6.606	3306250	1318915	24.118	20.603	
24) L5	AR-1248-4	8.153	6.810	3584484	1780813	22.968	21.643	
25) L5	AR-1248-5	8.195	7.264	4545582	1967306	29.719	23.616	
26) L6	AR-1254-1	8.123	7.218	3804391	2500125	22.096	17.496	
27) L6	AR-1254-2	8.366	7.385	3676717	609976	13.429	4.804	#
28) L6	AR-1254-3	8.757	7.830	1435035	3005418	4.672	13.434	#
29) L6	AR-1254-4	9.057	8.079	2088218	1695317	9.401	12.085	#
30) L6	AR-1254-5	9.558	0.000	1702457	0	6.558	N.D.	#
31) L7	AR-1260-1	0.000	7.988	0	4296317	N.D.	23.313	#
32) L7	AR-1260-2	9.197	8.168	2450997	1049012	7.327	4.756	#
33) L7	AR-1260-3	9.558	8.341	1702457	679541	6.181	3.335	#
34) L7	AR-1260-4	9.800	0.000	1572866	0	4.813	N.D.	#
35) L7	AR-1260-5	10.207	9.091	13258603	508948	19.935	1.139	#
36) L8	AR-1262-1	0.000	8.623	0	718795	N.D.	3.229	#
37) L8	AR-1262-2	10.207	9.091	13258603	508948	20.911	1.179	#
38) L8	AR-1262-3	10.496	9.401	4400037	693709	9.943	4.116	#
39) L8	AR-1262-4	0.000	9.401	0	693709	N.D.	2.068	#
40) L8	AR-1262-5	11.269	0.000	2829704	0	11.193	N.D.	#
41) L9	AR-1268-1	10.496	9.401	4400037	693709	5.445	1.343	#
42) L9	AR-1268-2	0.000	9.401	0	693709	N.D.	1.406	#

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ041219\
Data File : PQ039070.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2019 17:37
Operator : AJ\SJ
Sample : K1560-09
Misc : AR1242 MDL 25 PPB
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 00:57:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ041219.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Apr 13 00:36:36 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	
43)	L9 AR-1268-3	10.848	9.663	15640321	1319228	23.721	3.310	#
44)	L9 AR-1268-4	11.269	0.000	2829704	0	10.110	N.D.	#
45)	L9 AR-1268-5	11.758	10.294	2338726	1601840	1.027	1.255	

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ041219\
Data File : PQ039070.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2019 17:37
Operator : AJ\SJ
Sample : K1560-09
Misc : AR1242 MDL 25 PPB
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 00:57:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ041219.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Apr 13 00:36:36 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

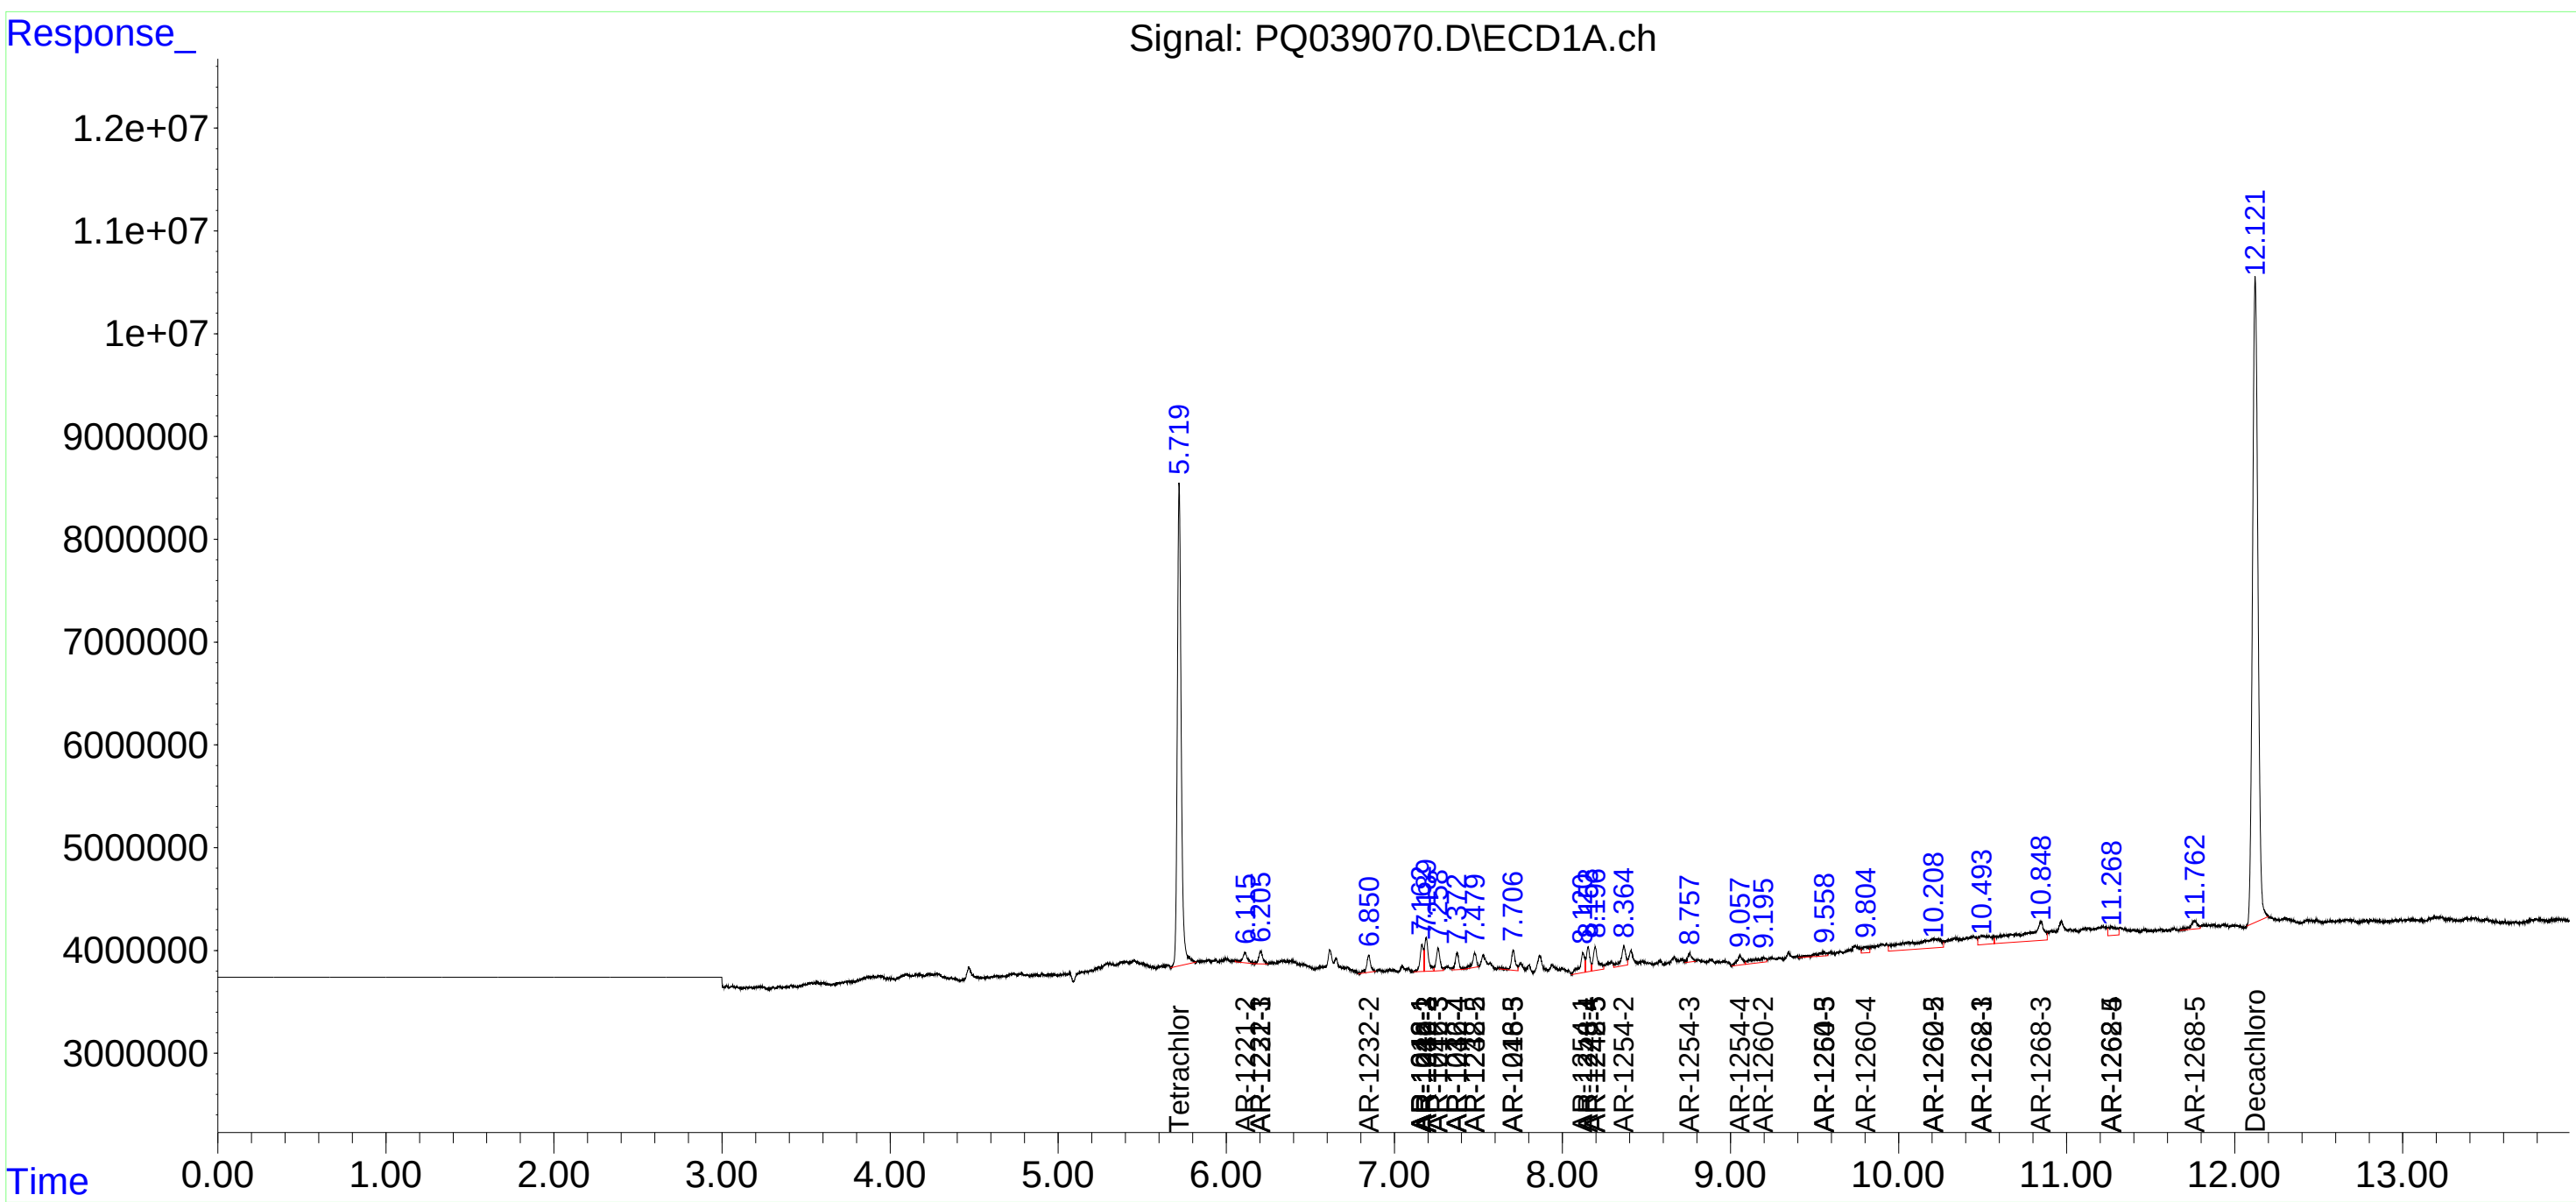

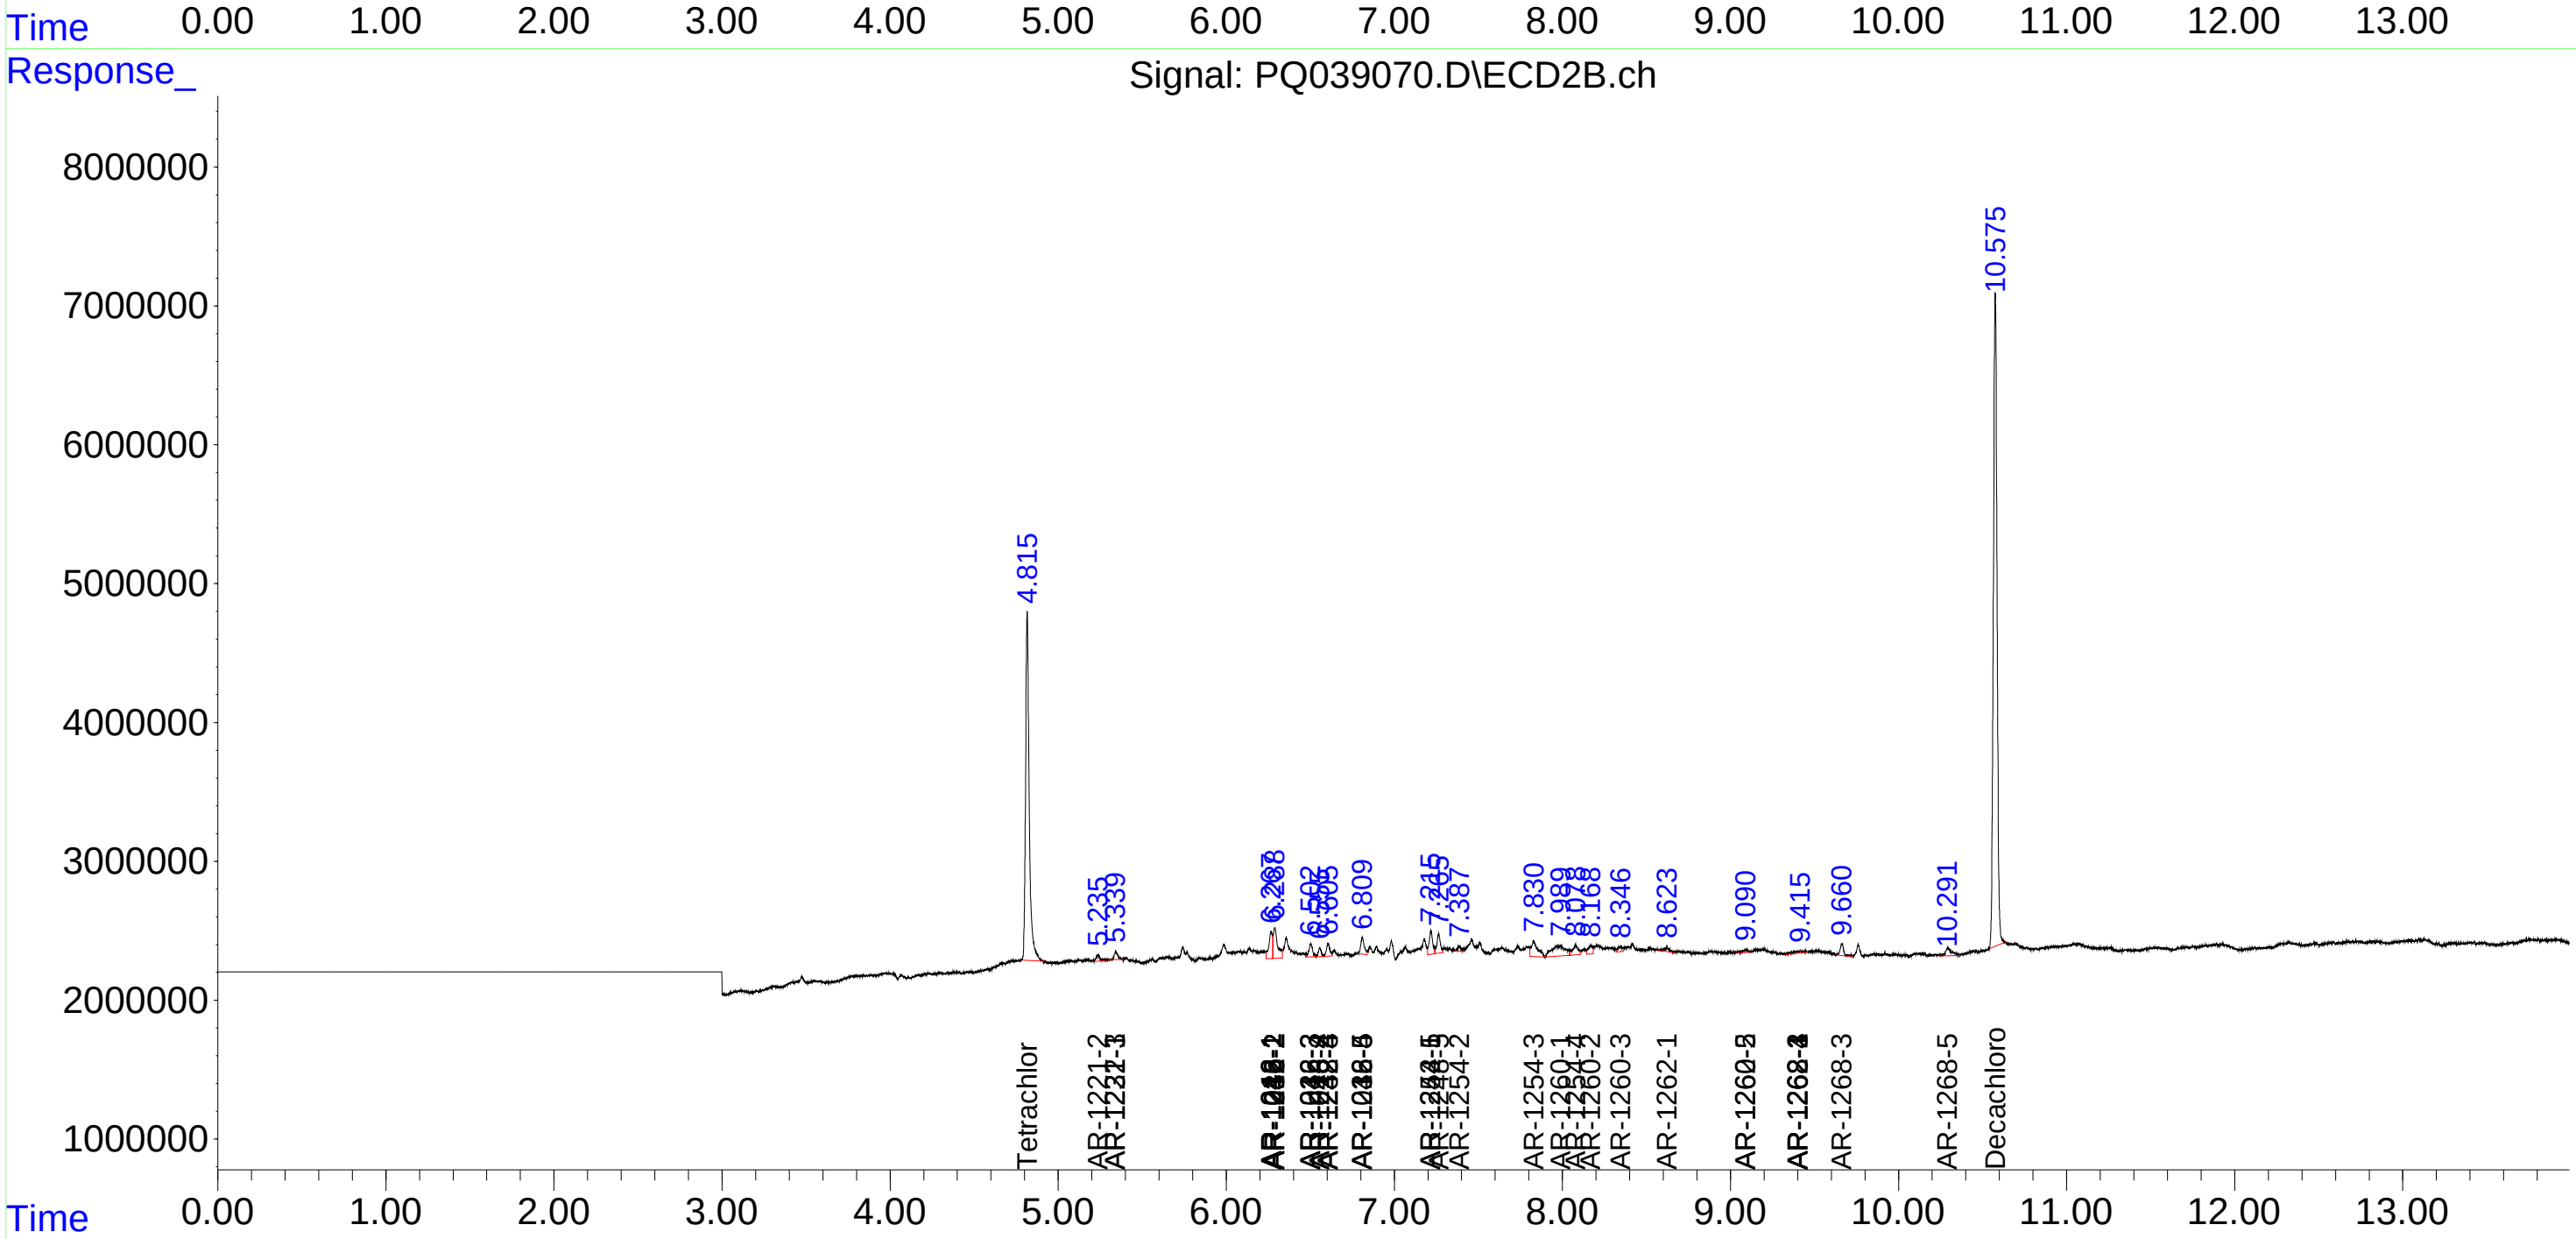

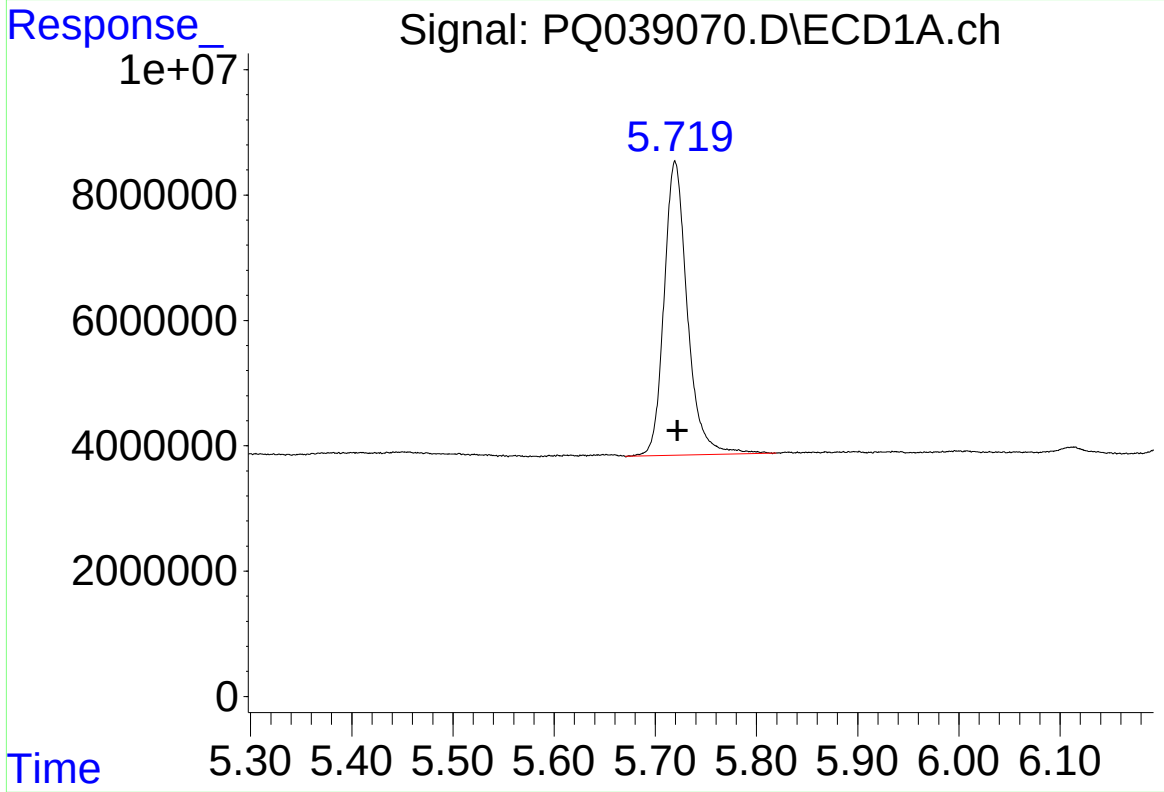

#1 Tetrachloro-m-xylene

R.T.: 5.720 min
Delta R.T.: -0.002 min
Response: 75001100
Conc: 16.92 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

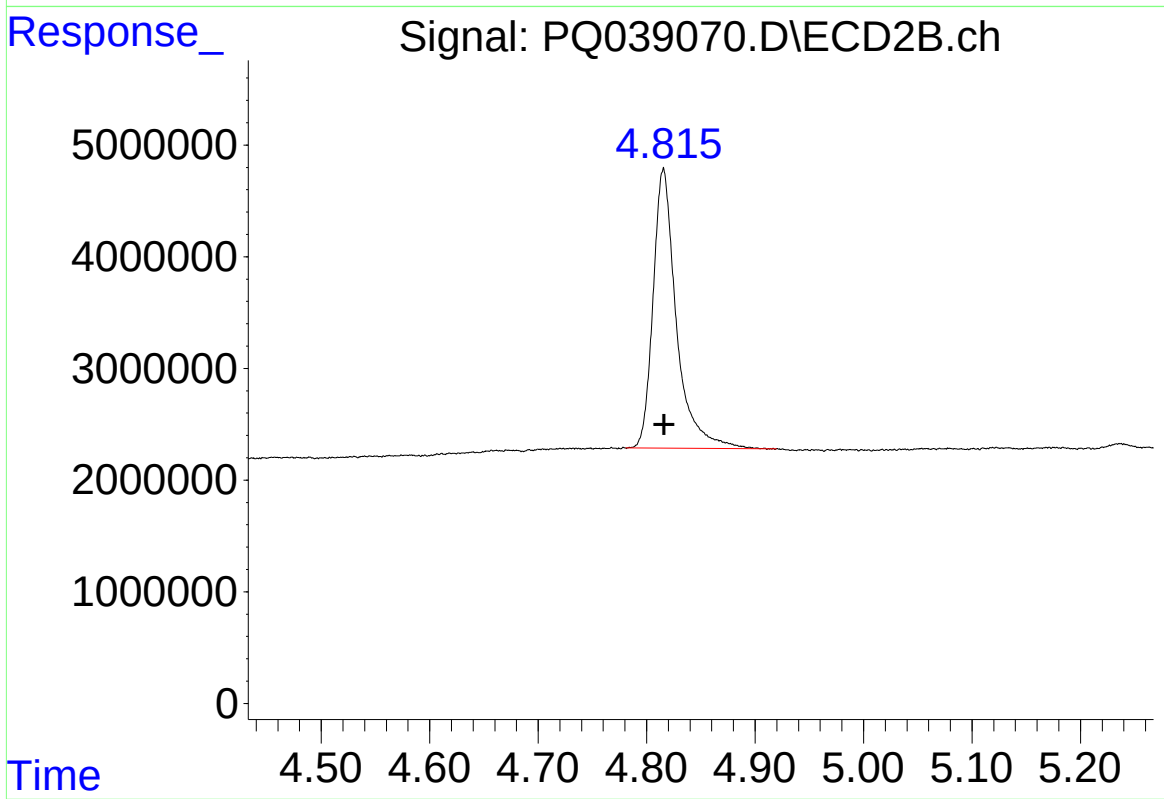

#1 Tetrachloro-m-xylene

R.T.: 4.816 min
Delta R.T.: 0.000 min
Response: 37339614
Conc: 16.75 ng/ml

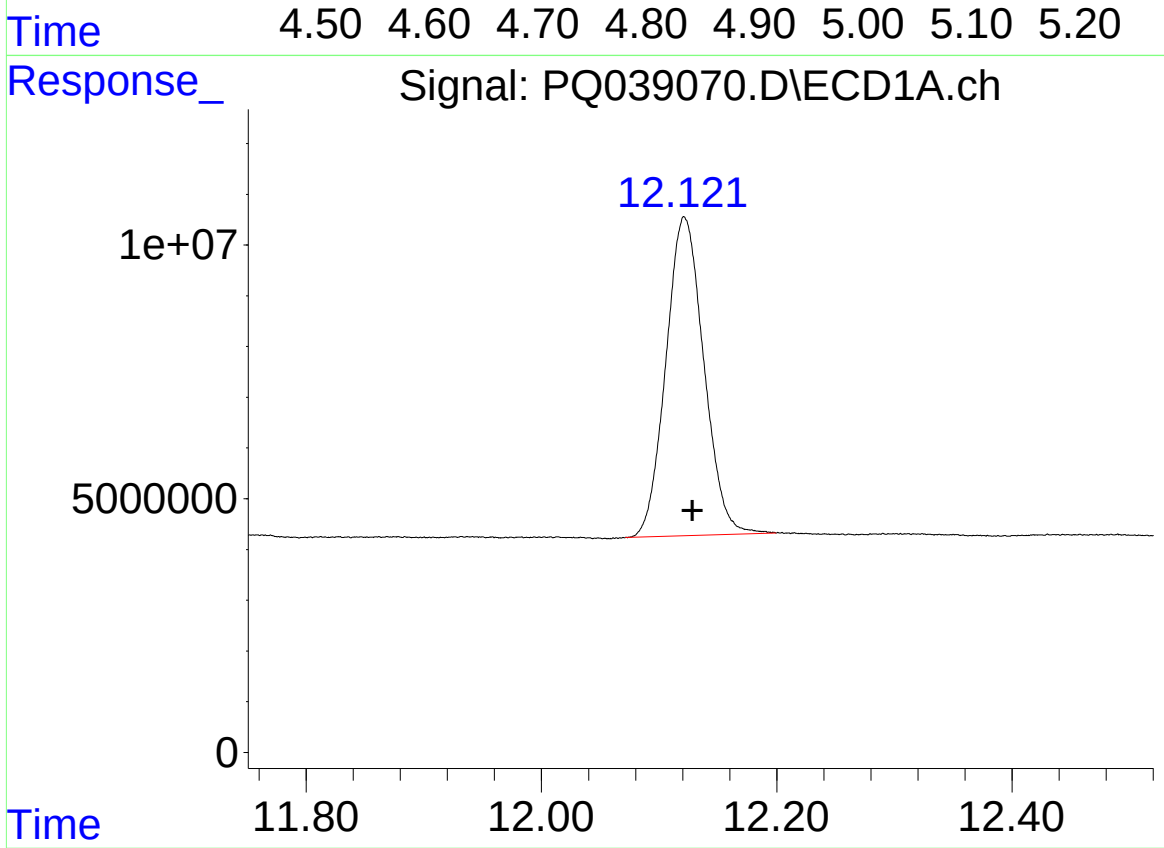

#2 Decachlorobiphenyl

R.T.: 12.122 min
Delta R.T.: -0.007 min
Response: 140701363
Conc: 20.28 ng/ml

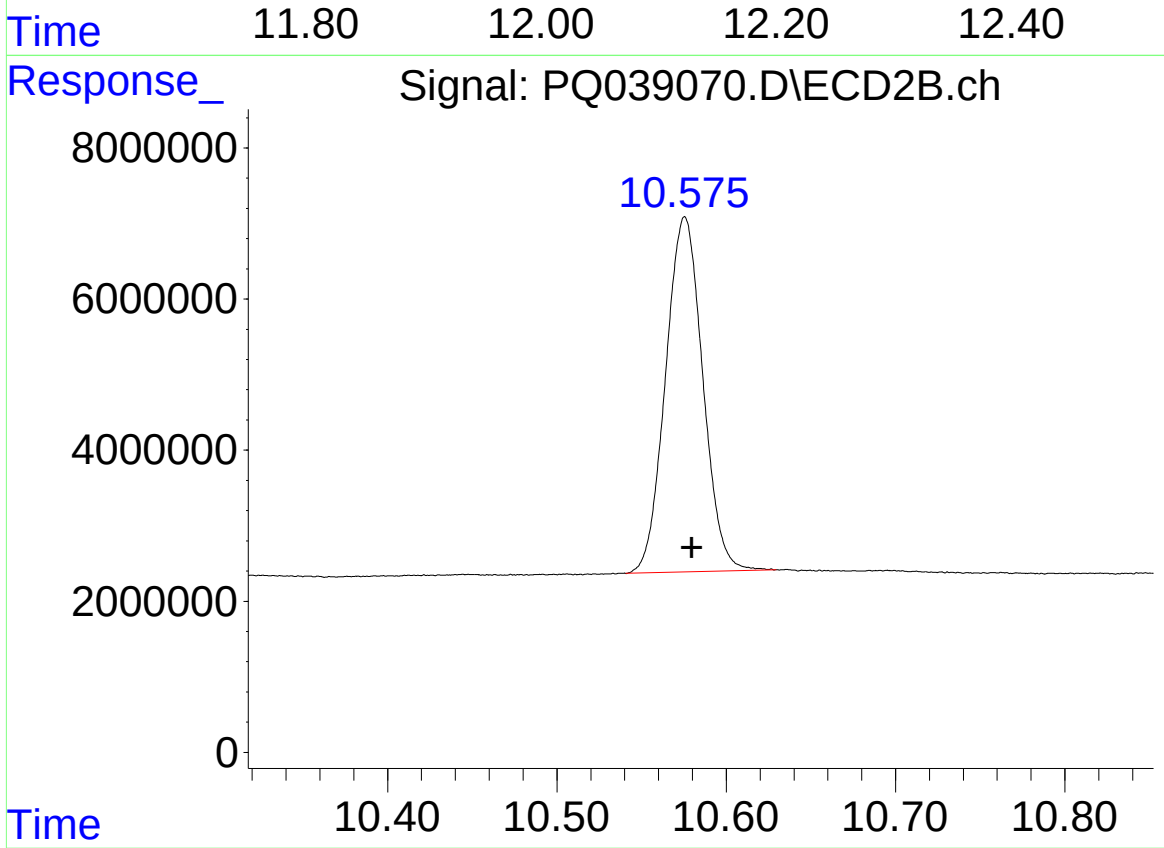

#2 Decachlorobiphenyl

R.T.: 10.576 min
Delta R.T.: -0.004 min
Response: 71760188
Conc: 20.57 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

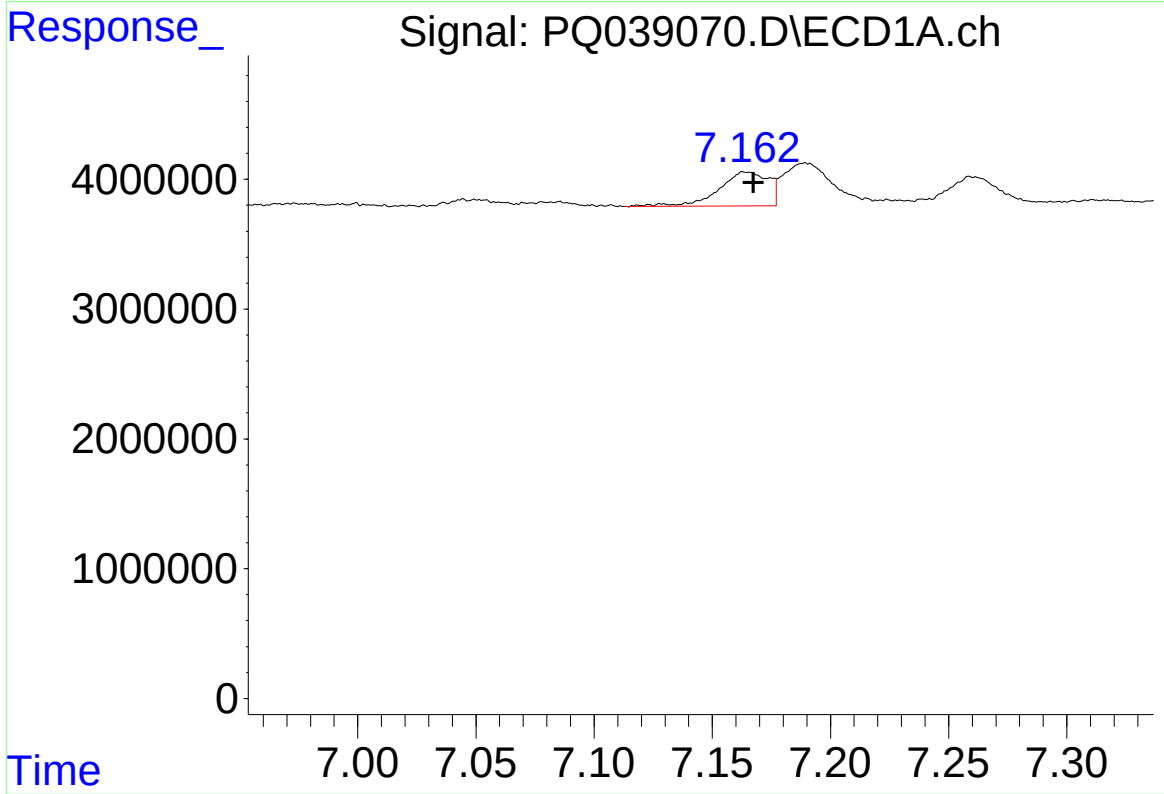

#3 AR-1016-1

R.T.: 7.165 min
Delta R.T.: -0.003 min
Response: 3830810
Conc: 21.08 ng/ml

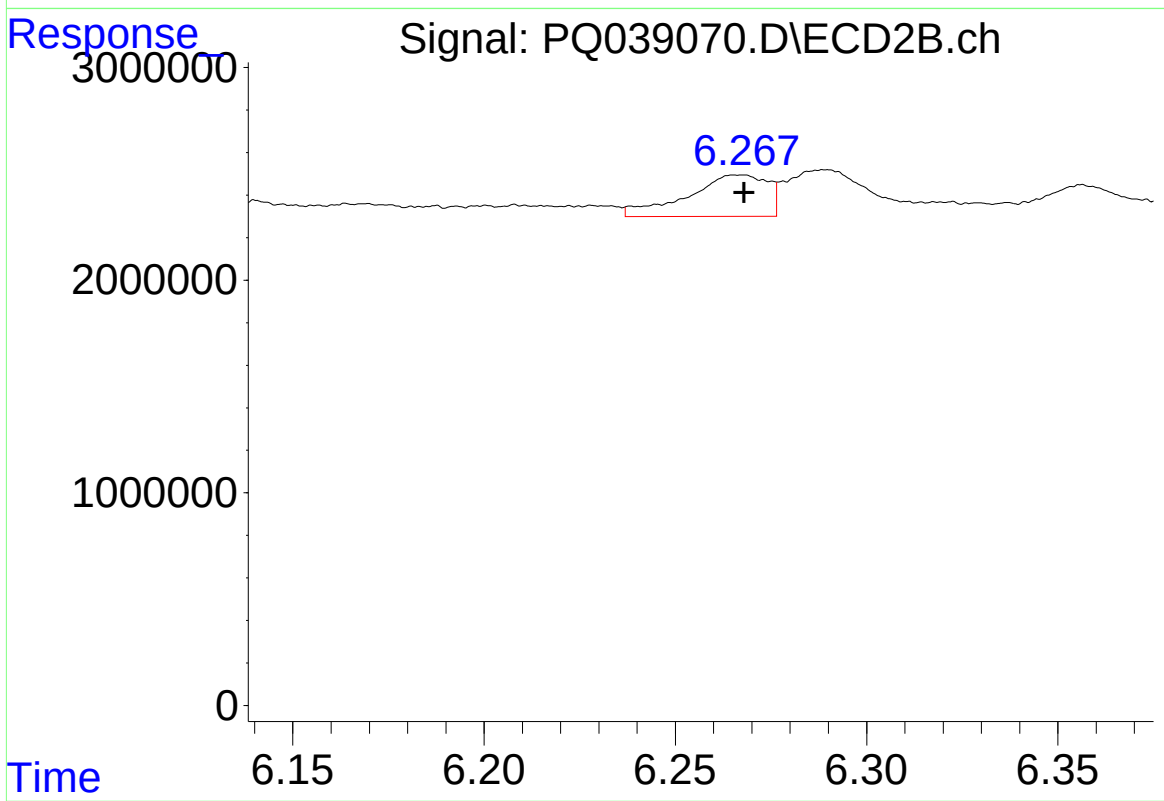

#3 AR-1016-1

R.T.: 6.267 min
Delta R.T.: -0.001 min
Response: 2839641
Conc: 27.96 ng/ml

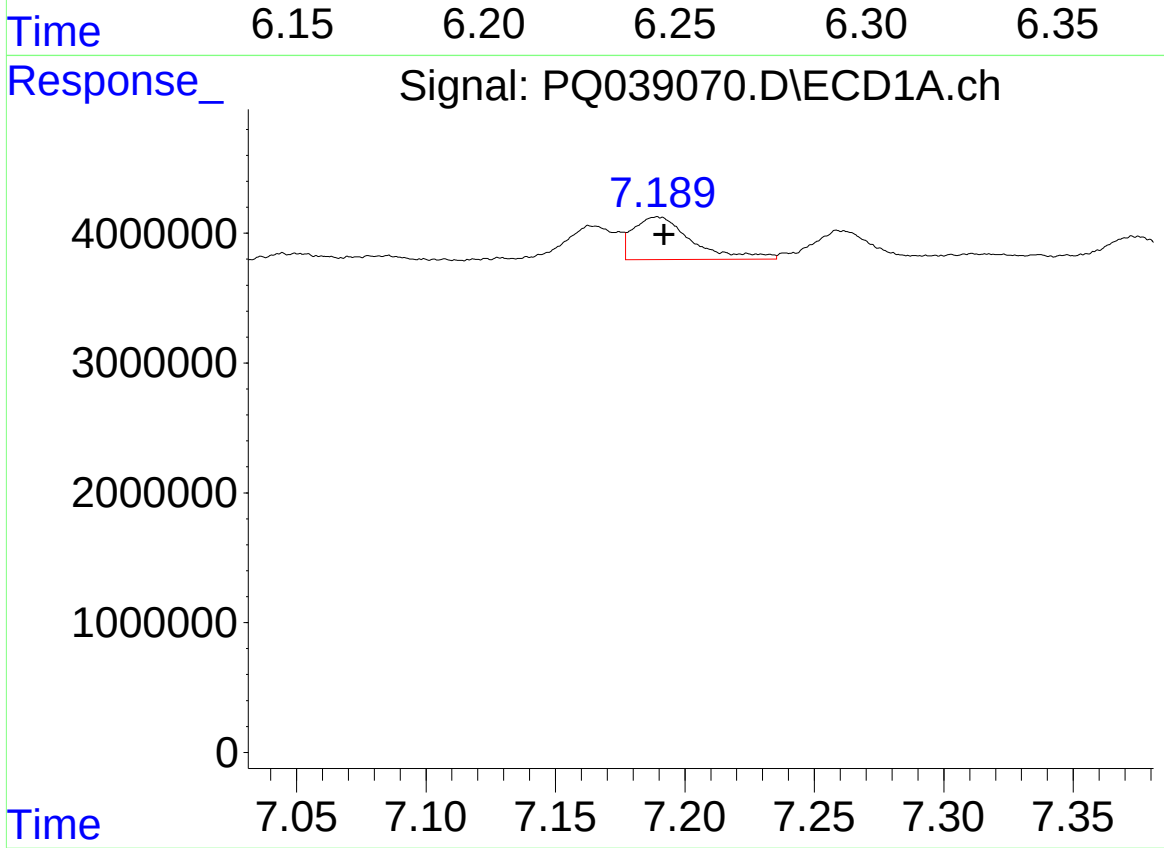

#4 AR-1016-2

R.T.: 7.189 min
Delta R.T.: -0.003 min
Response: 5185677
Conc: 19.14 ng/ml

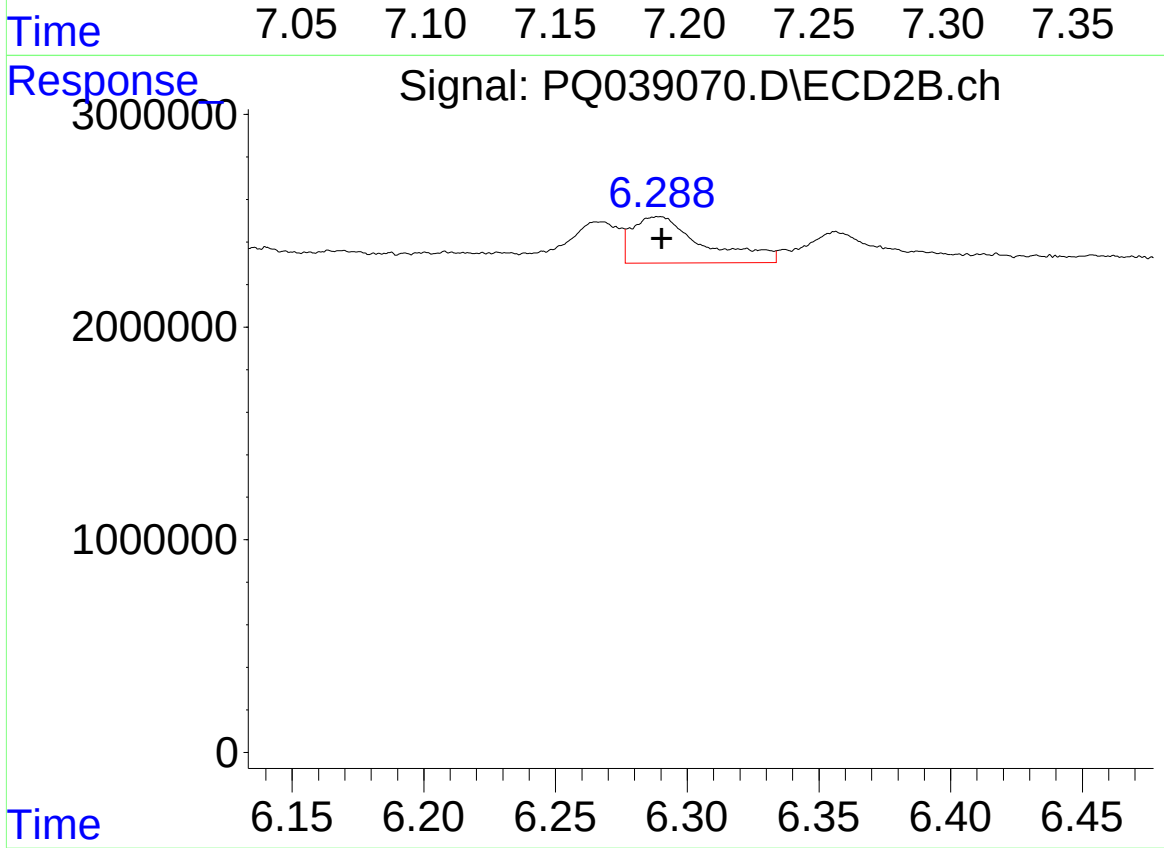

#4 AR-1016-2

R.T.: 6.289 min
Delta R.T.: -0.002 min
Response: 4094839
Conc: 27.65 ng/ml

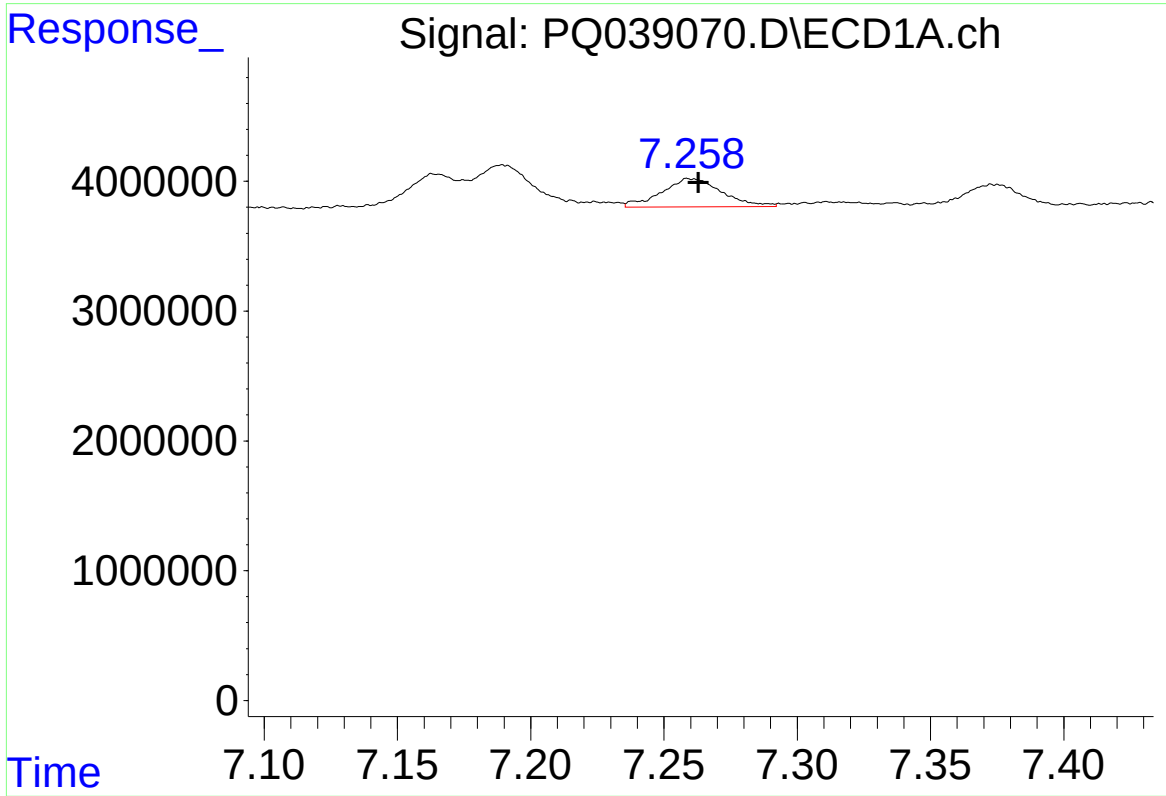

#5 AR-1016-3

R.T.:	7.261 min
Delta R.T.:	-0.002 min
Response:	3430935
Conc:	20.59 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

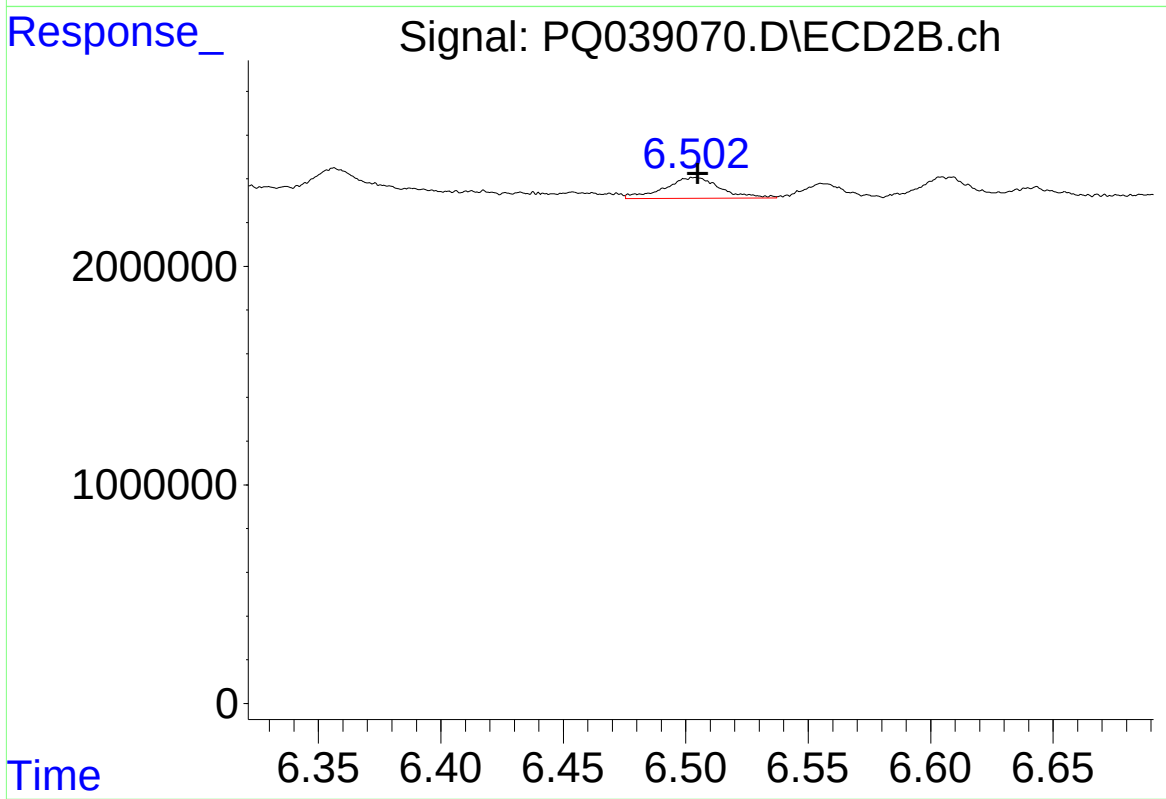

#5 AR-1016-3

R.T.:	6.503 min
Delta R.T.:	-0.001 min
Response:	1509359
Conc:	20.23 ng/ml

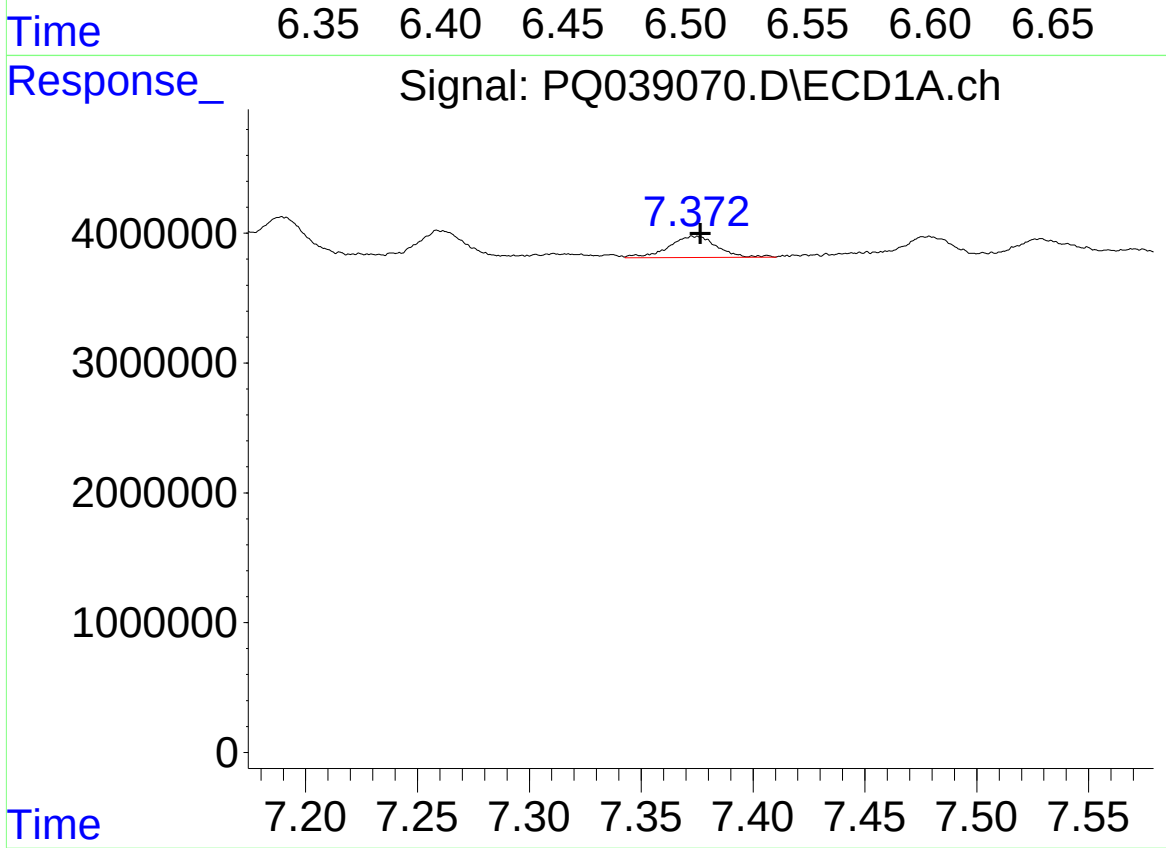

#6 AR-1016-4

R.T.:	7.374 min
Delta R.T.:	-0.002 min
Response:	2449757
Conc:	17.68 ng/ml

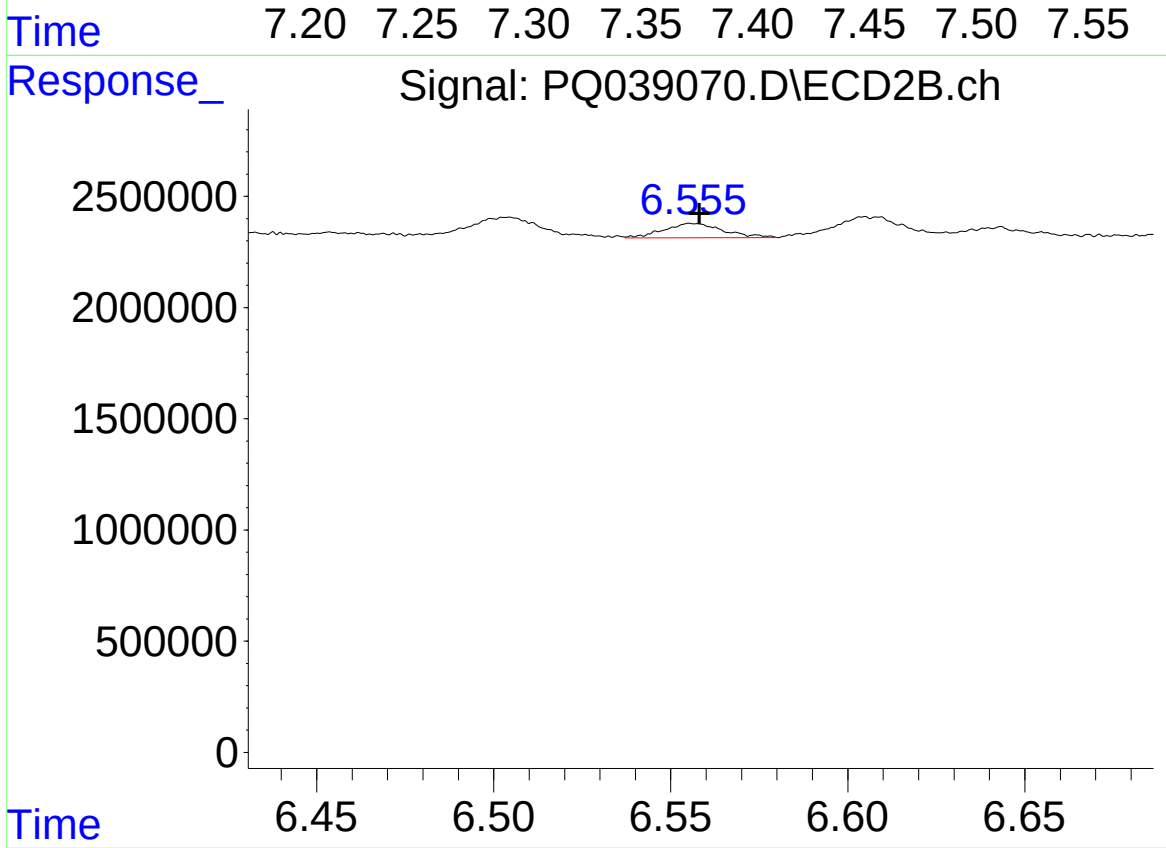

#6 AR-1016-4

R.T.:	6.557 min
Delta R.T.:	-0.002 min
Response:	765193
Conc:	12.27 ng/ml

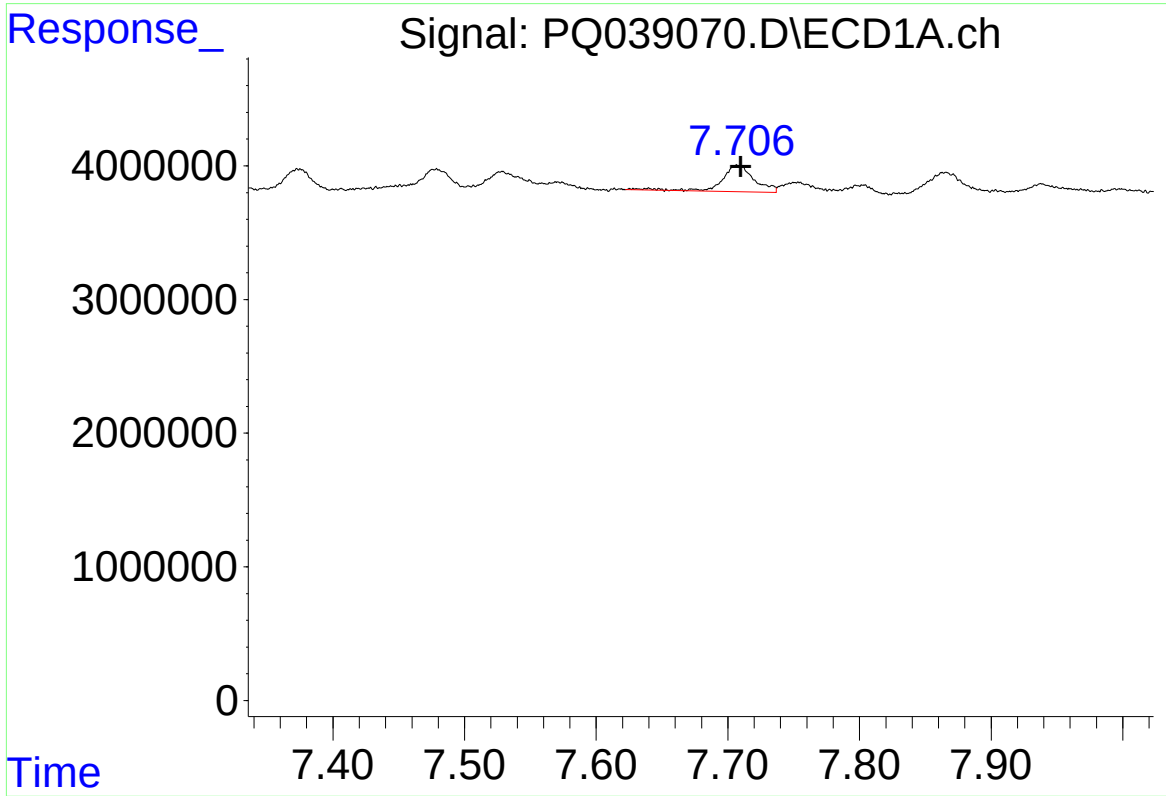

#7 AR-1016-5

R.T.: 7.708 min
Delta R.T.: -0.002 min
Response: 3306250
Conc: 23.30 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

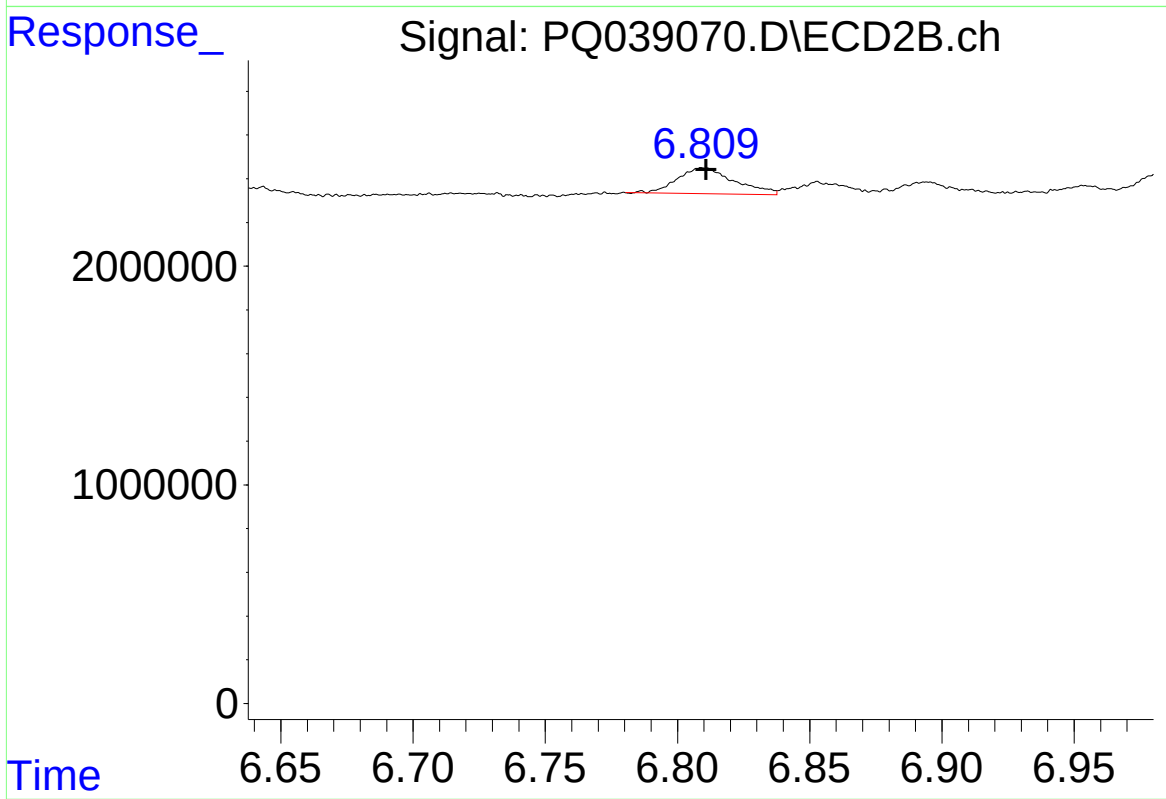

#7 AR-1016-5

R.T.: 6.810 min
Delta R.T.: 0.000 min
Response: 1780813
Conc: 20.07 ng/ml

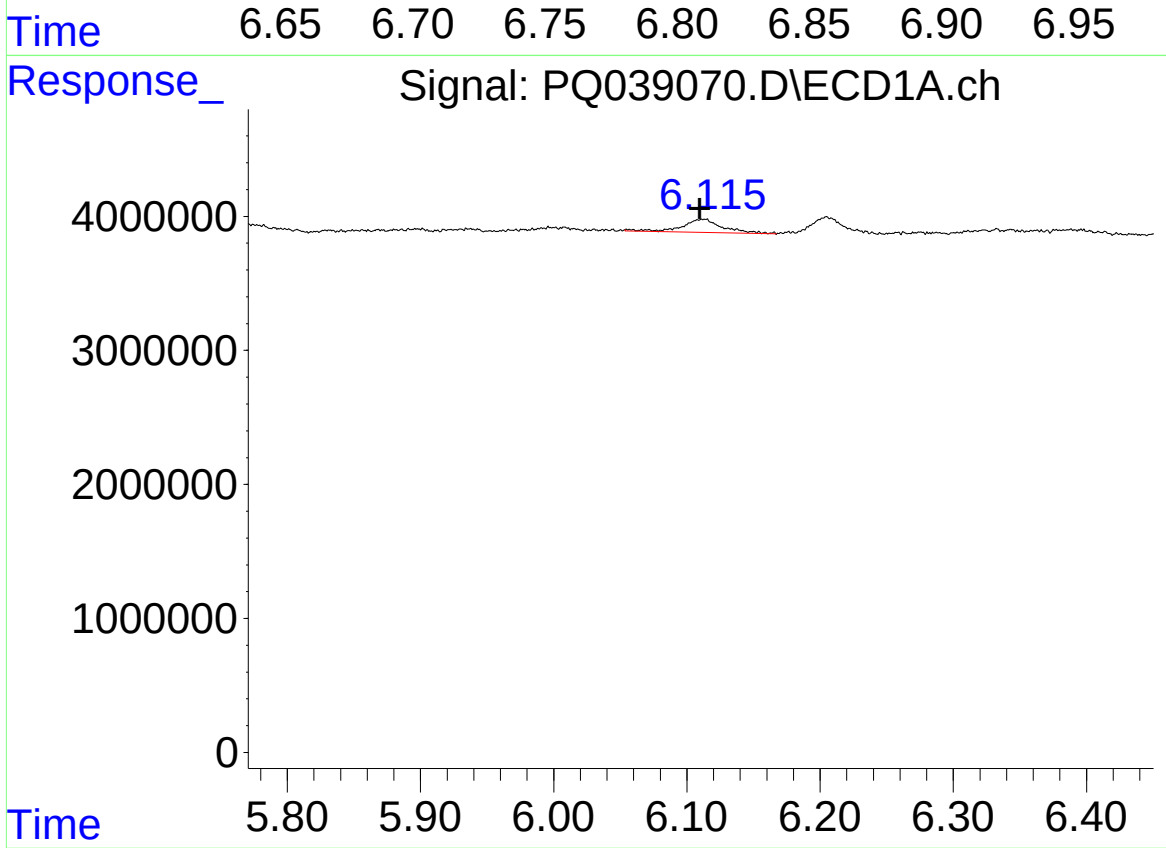

#9 AR-1221-2

R.T.: 6.112 min
Delta R.T.: 0.002 min
Response: 2066919
Conc: 60.89 ng/ml

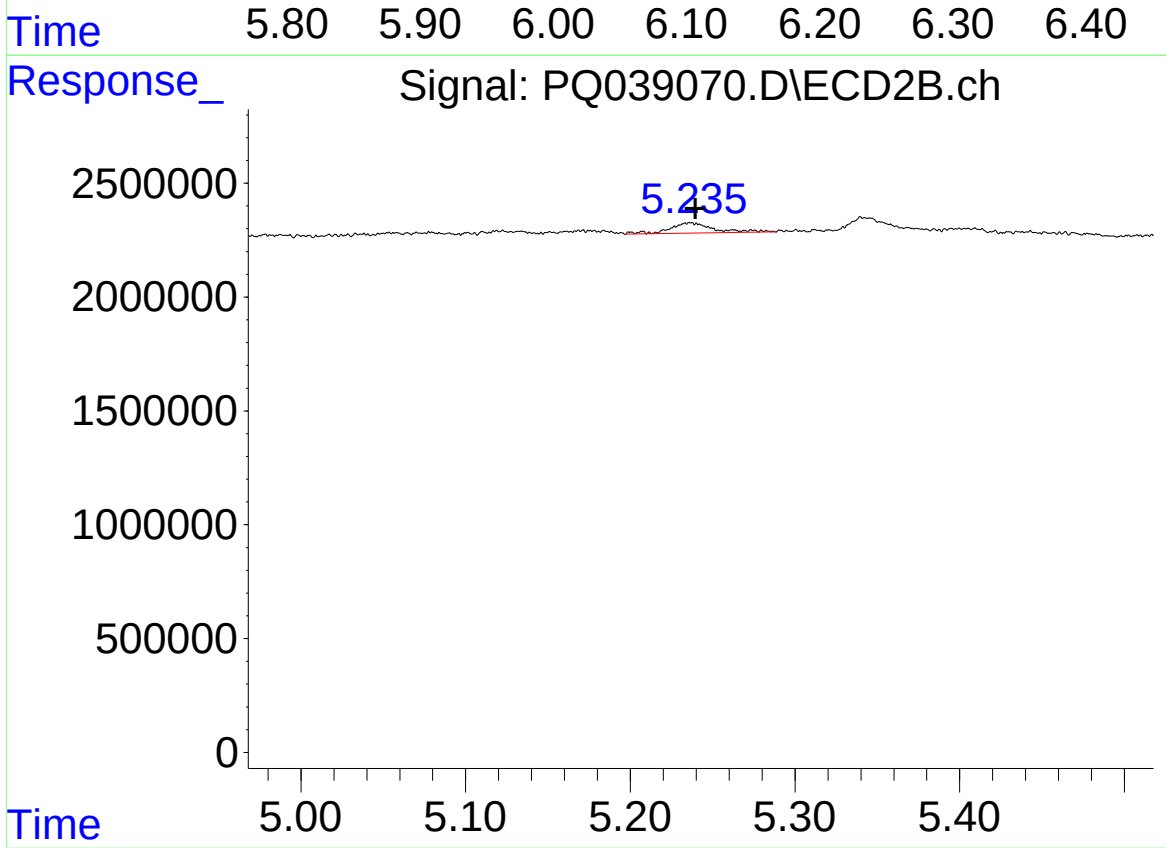

#9 AR-1221-2

R.T.: 5.237 min
Delta R.T.: -0.003 min
Response: 809208
Conc: 38.81 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

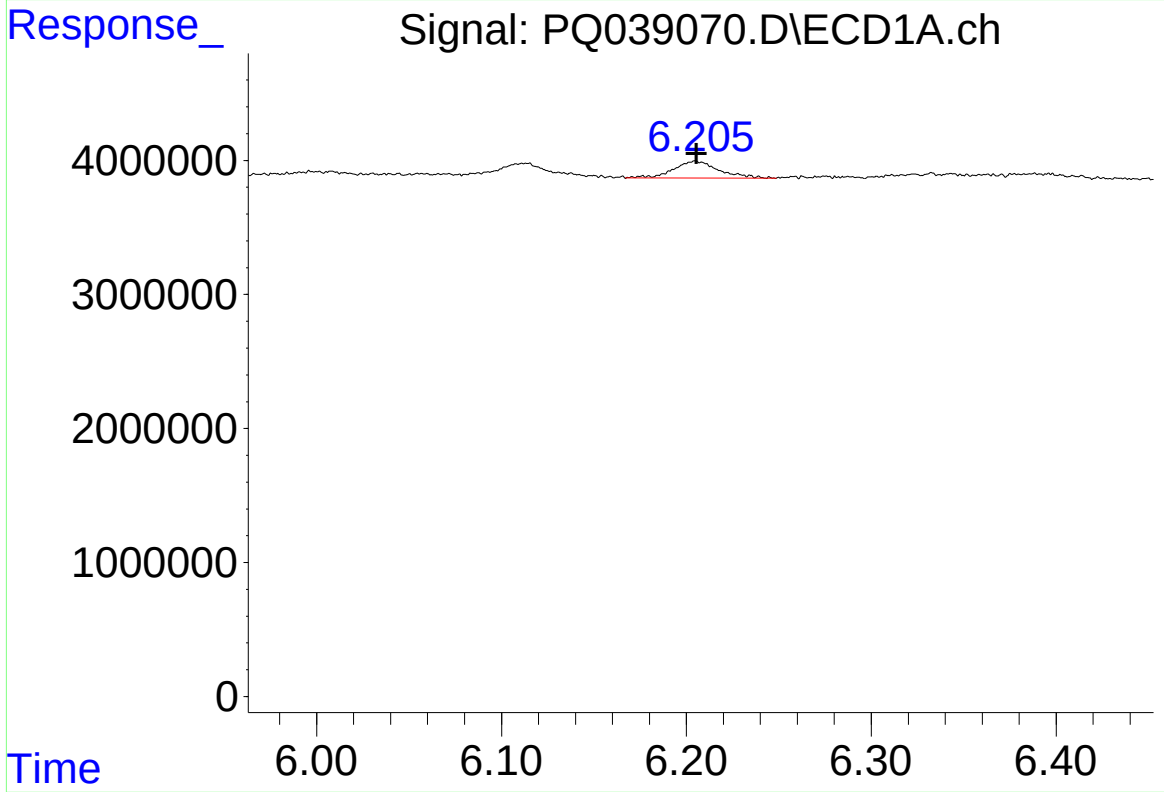


```
#10  AR-1221-3

      R.T.:    6.205 min
Delta R.T.:    0.000 min
  Response:   2116982
      Conc:   19.28 ng/ml
```

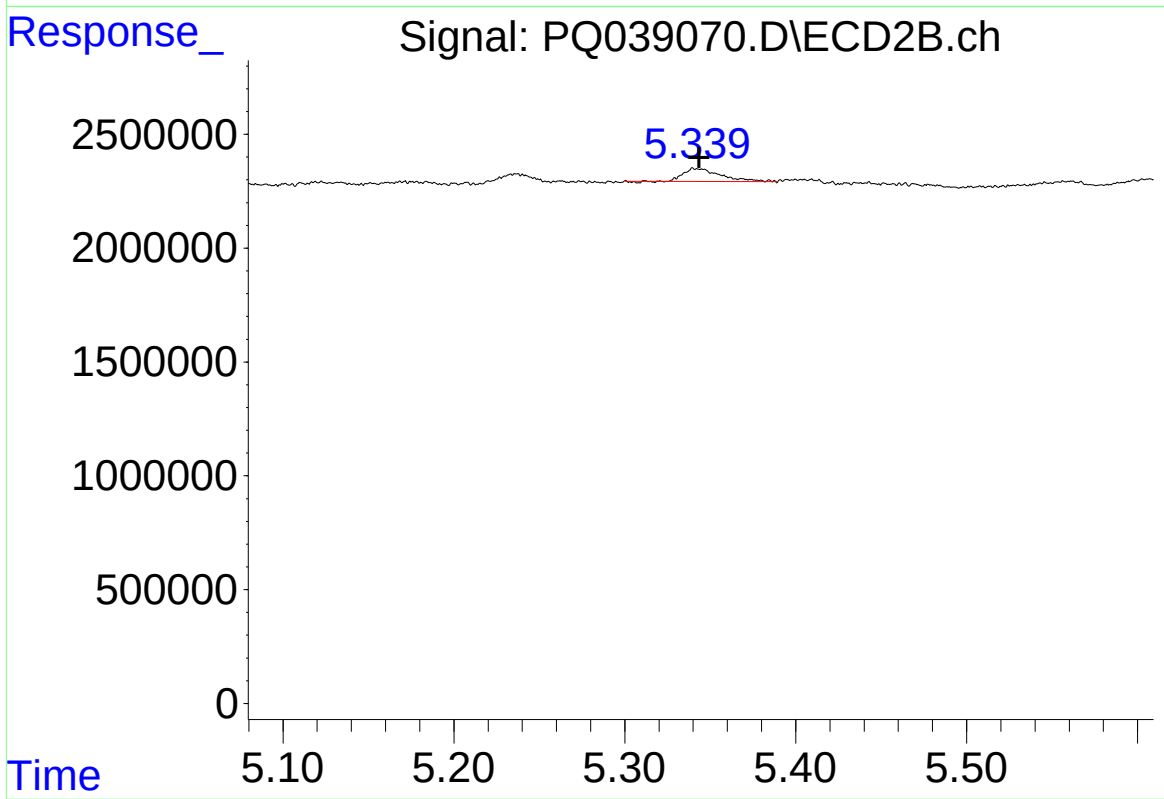


```
#10  AR-1221-3

      R.T.:    5.343 min
Delta R.T.:    0.000 min
  Response:    895222
      Conc:   14.59 ng/ml
```

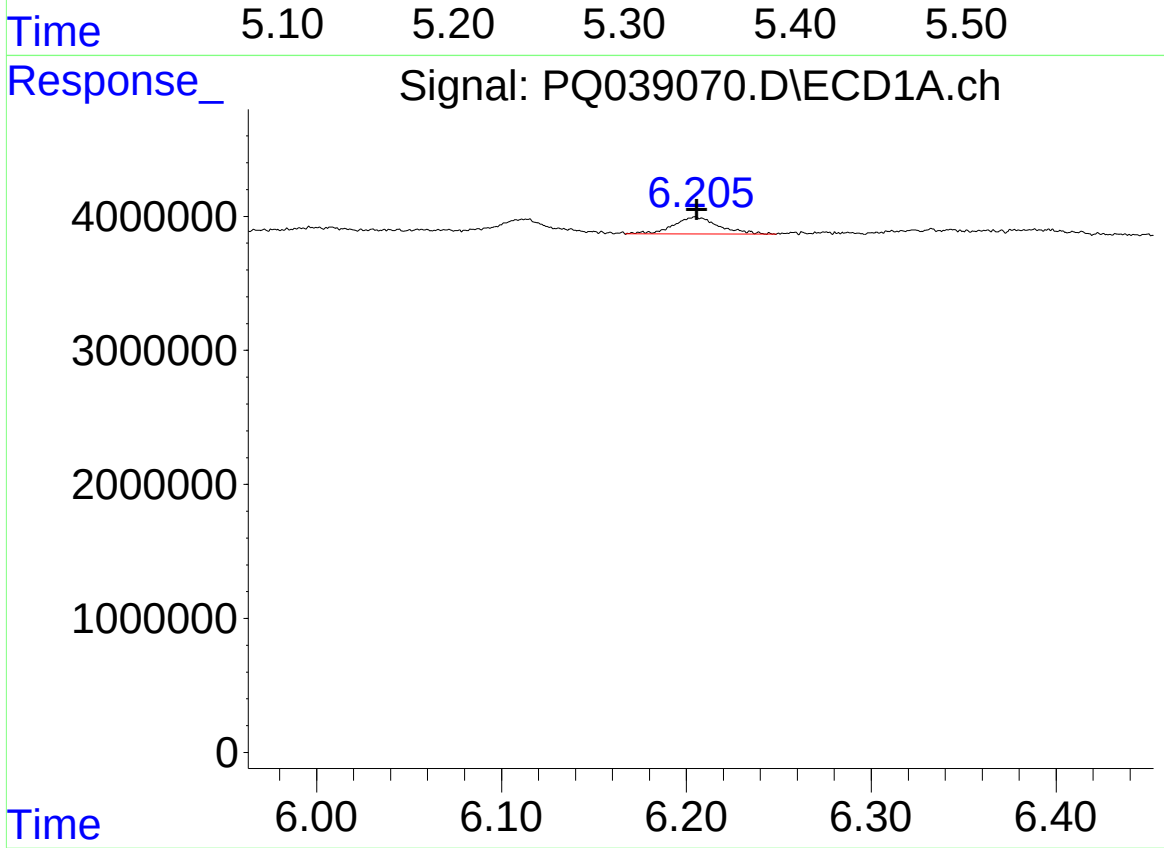


```
#11  AR-1232-1

      R.T.:    6.205 min
Delta R.T.:    0.000 min
  Response:   2116982
      Conc:   26.62 ng/ml
```

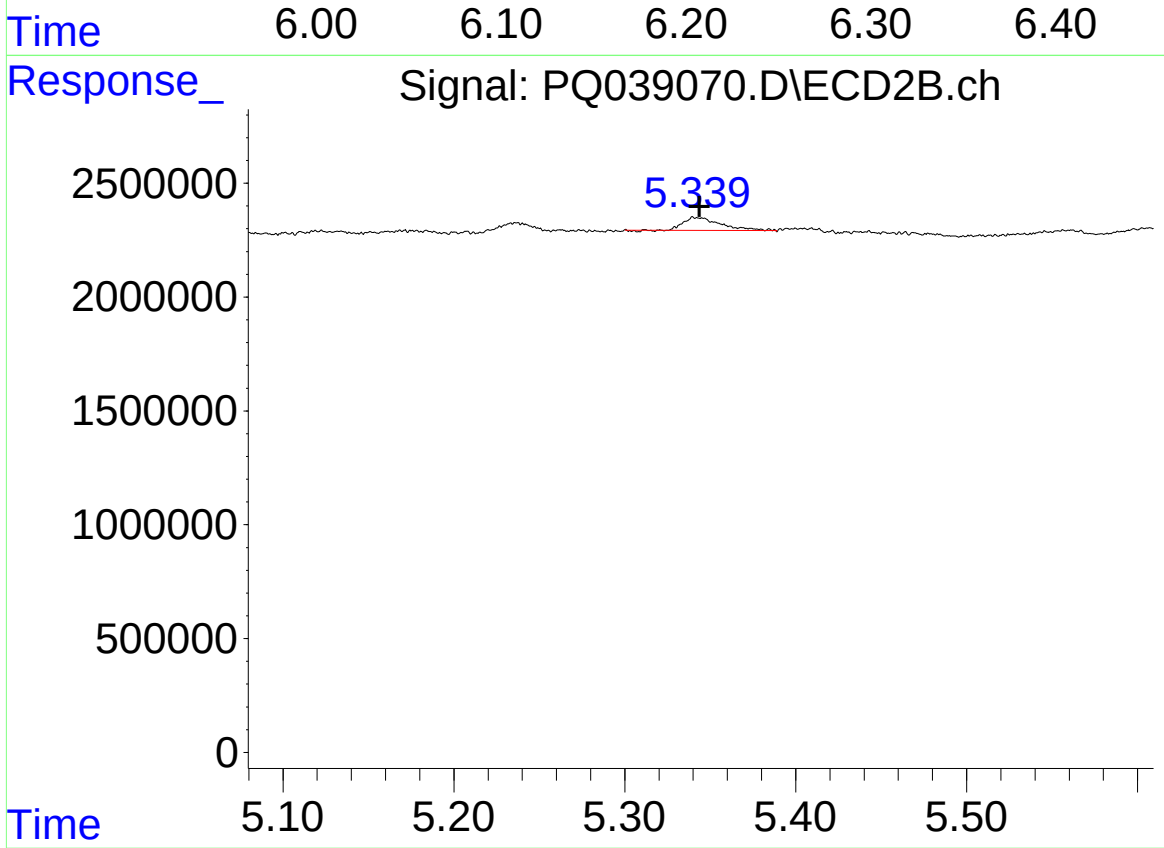


```
#11  AR-1232-1

      R.T.:    5.343 min
Delta R.T.:    0.000 min
  Response:    895222
      Conc:   23.61 ng/ml
```

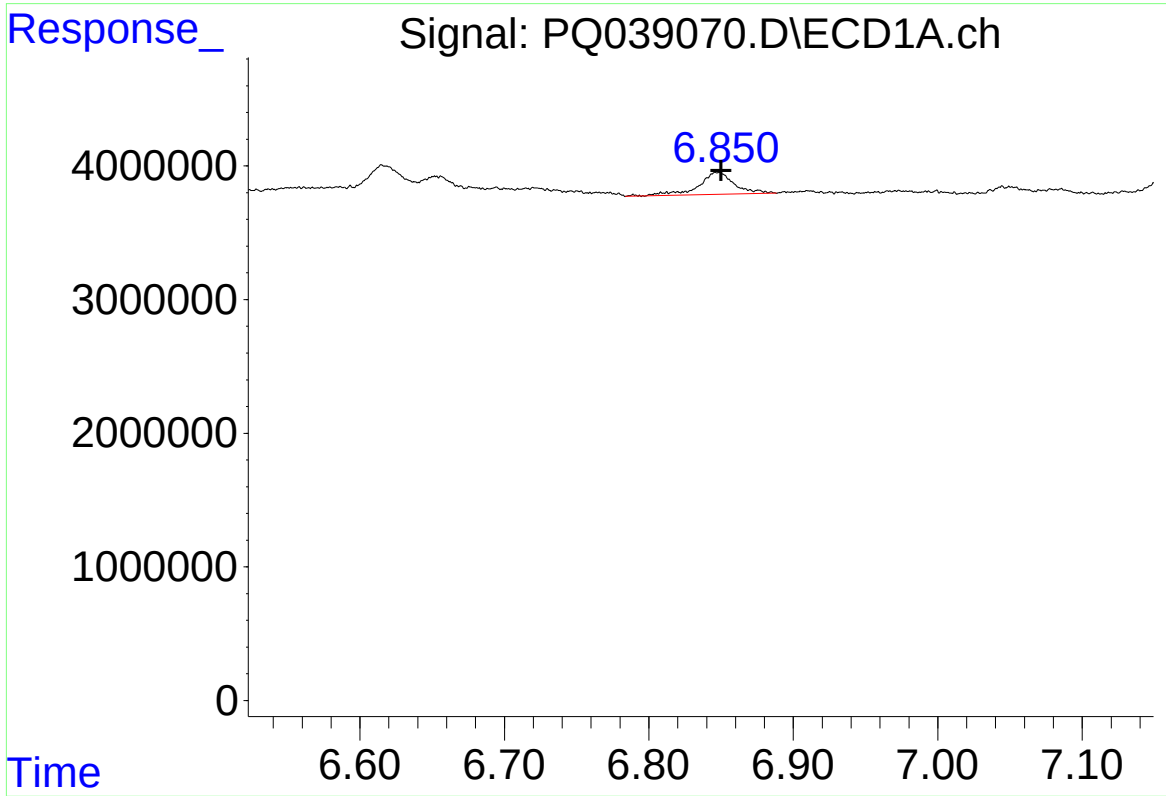

#12 AR-1232-2

R.T.: 6.848 min
Delta R.T.: -0.002 min
Response: 2845347
Conc: 68.01 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

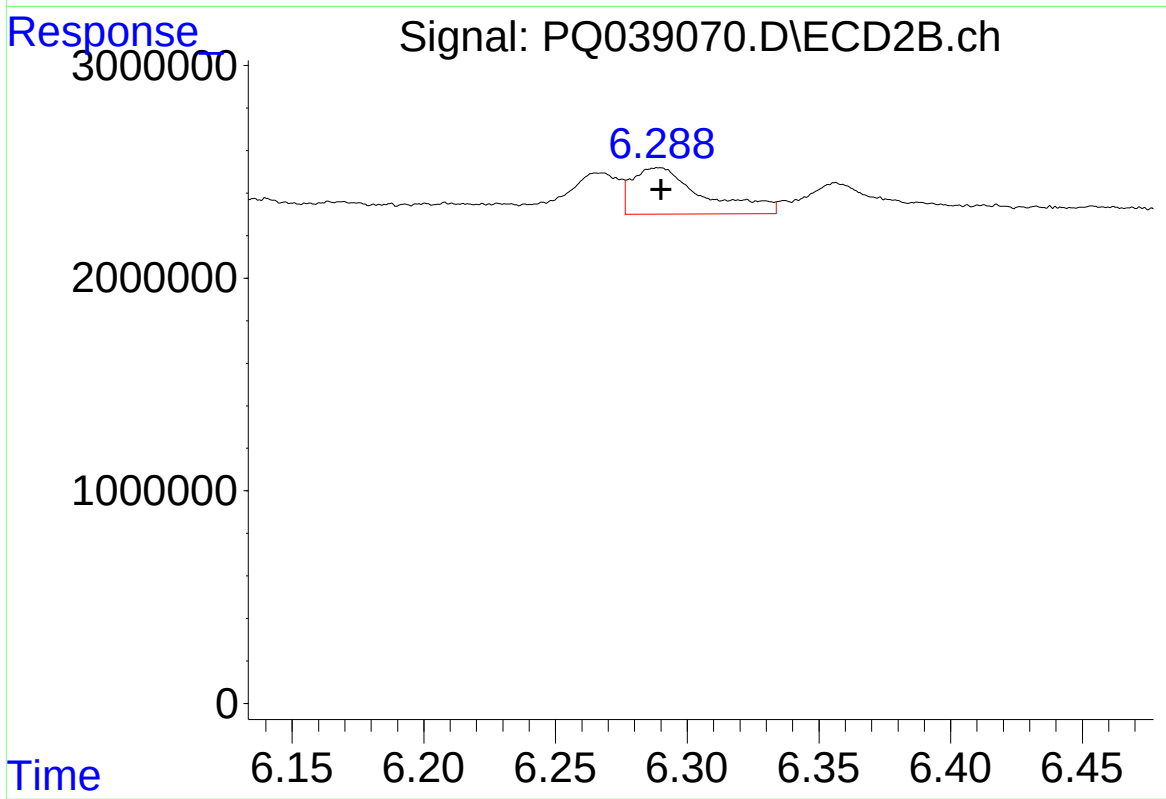

#12 AR-1232-2

R.T.: 6.289 min
Delta R.T.: -0.001 min
Response: 4094839
Conc: 88.11 ng/ml

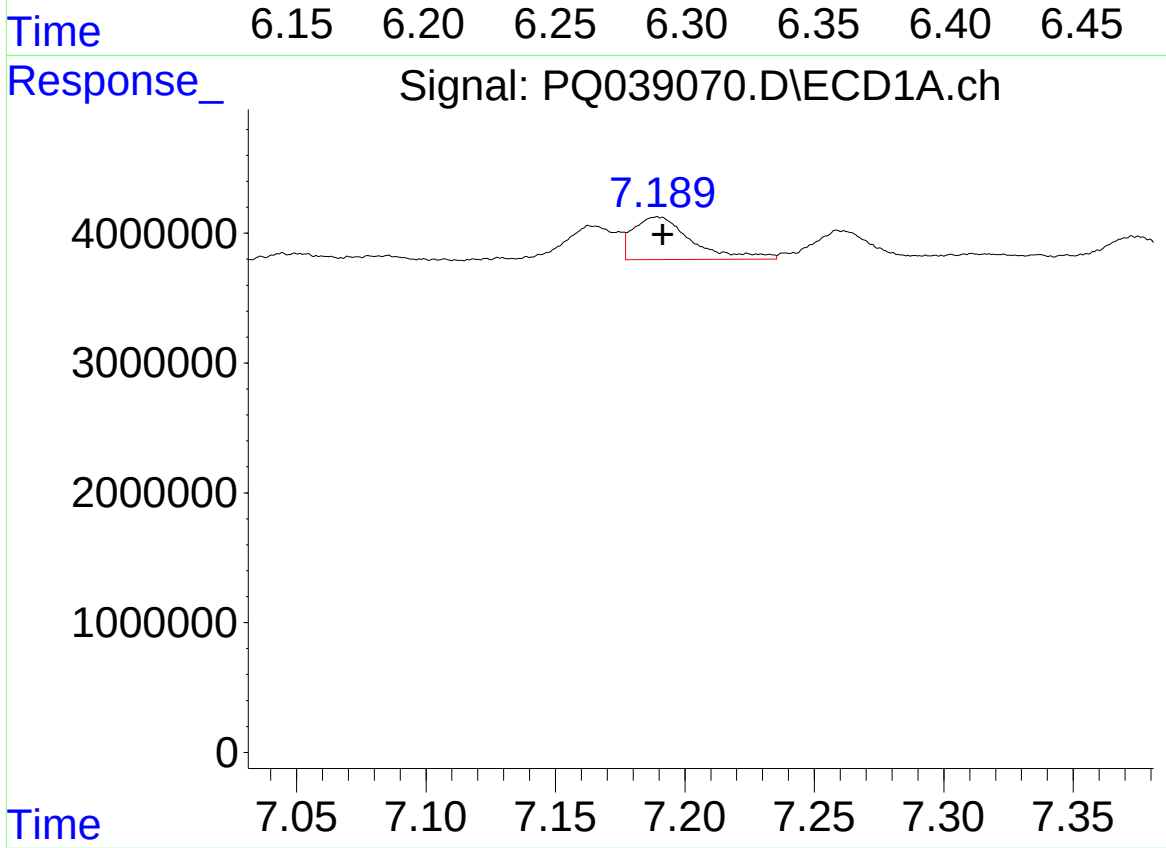

#13 AR-1232-3

R.T.: 7.189 min
Delta R.T.: -0.002 min
Response: 5185677
Conc: 58.25 ng/ml

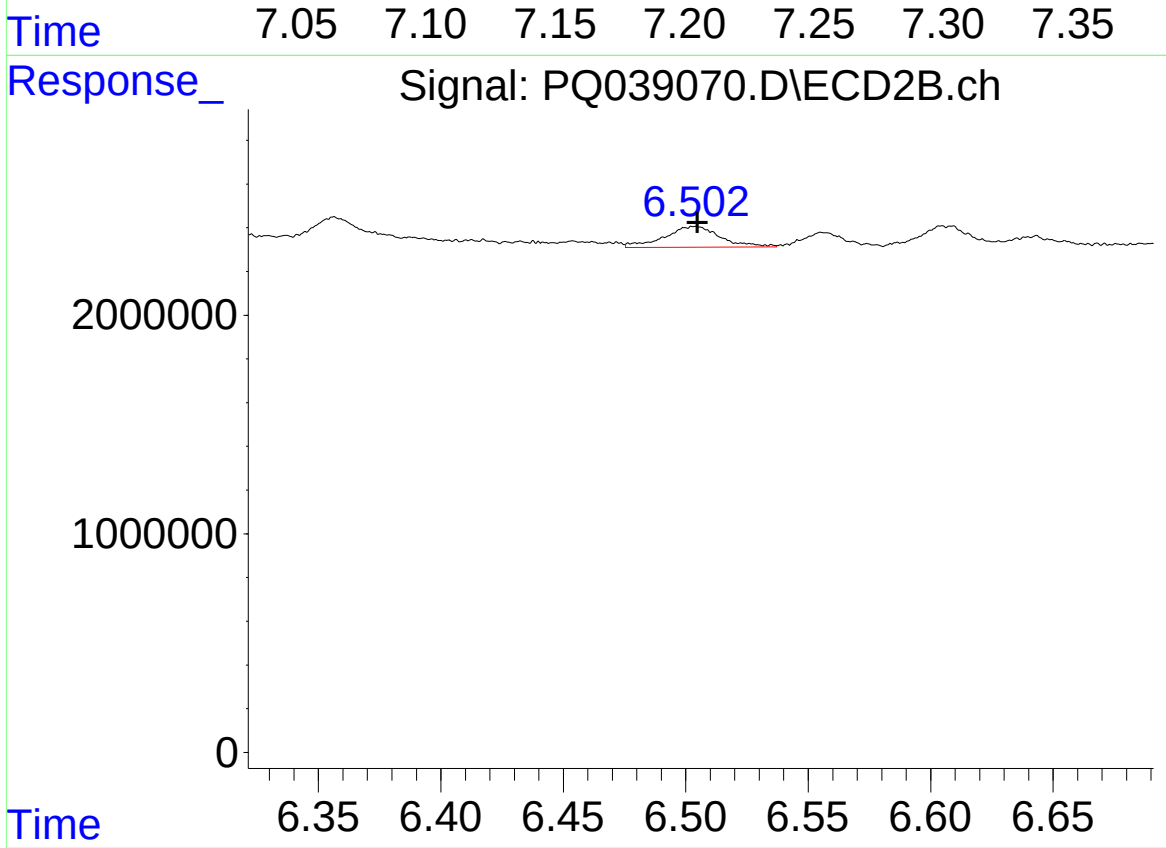

#13 AR-1232-3

R.T.: 6.503 min
Delta R.T.: -0.001 min
Response: 1509359
Conc: 71.16 ng/ml

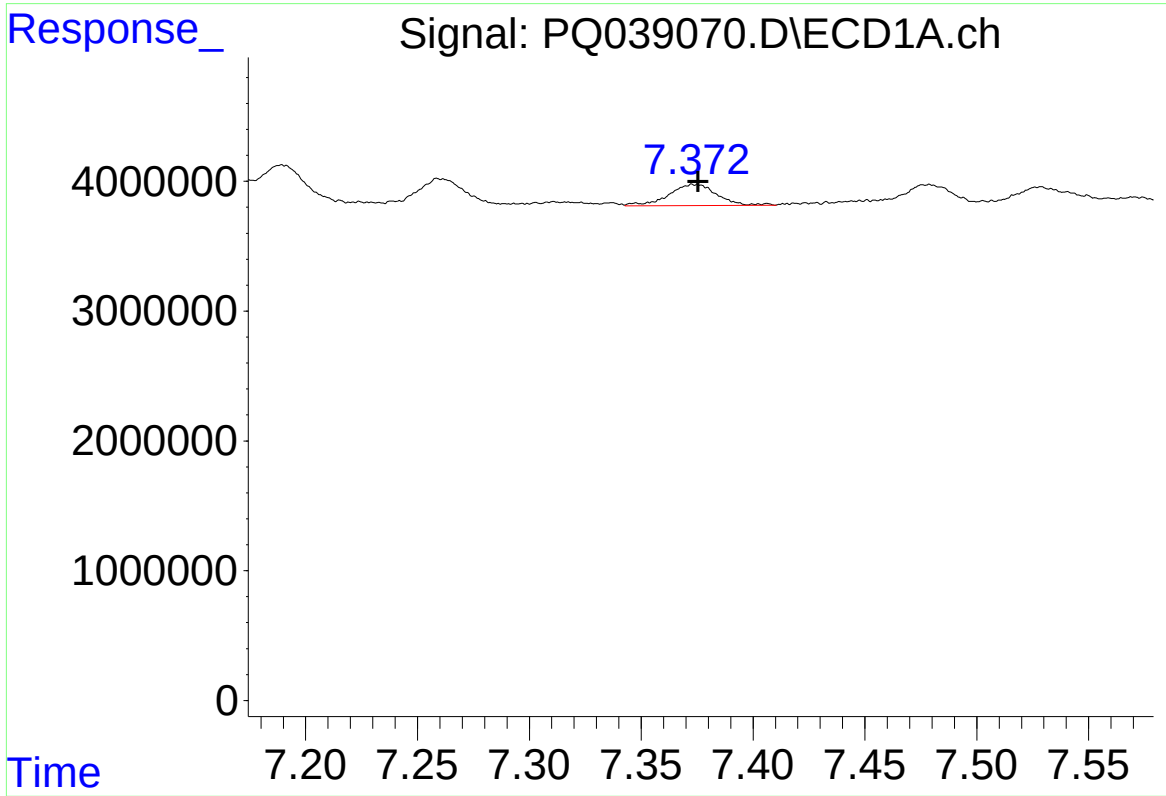

#14 AR-1232-4

R.T.: 7.374 min
Delta R.T.: -0.001 min
Response: 2449757
Conc: 47.81 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

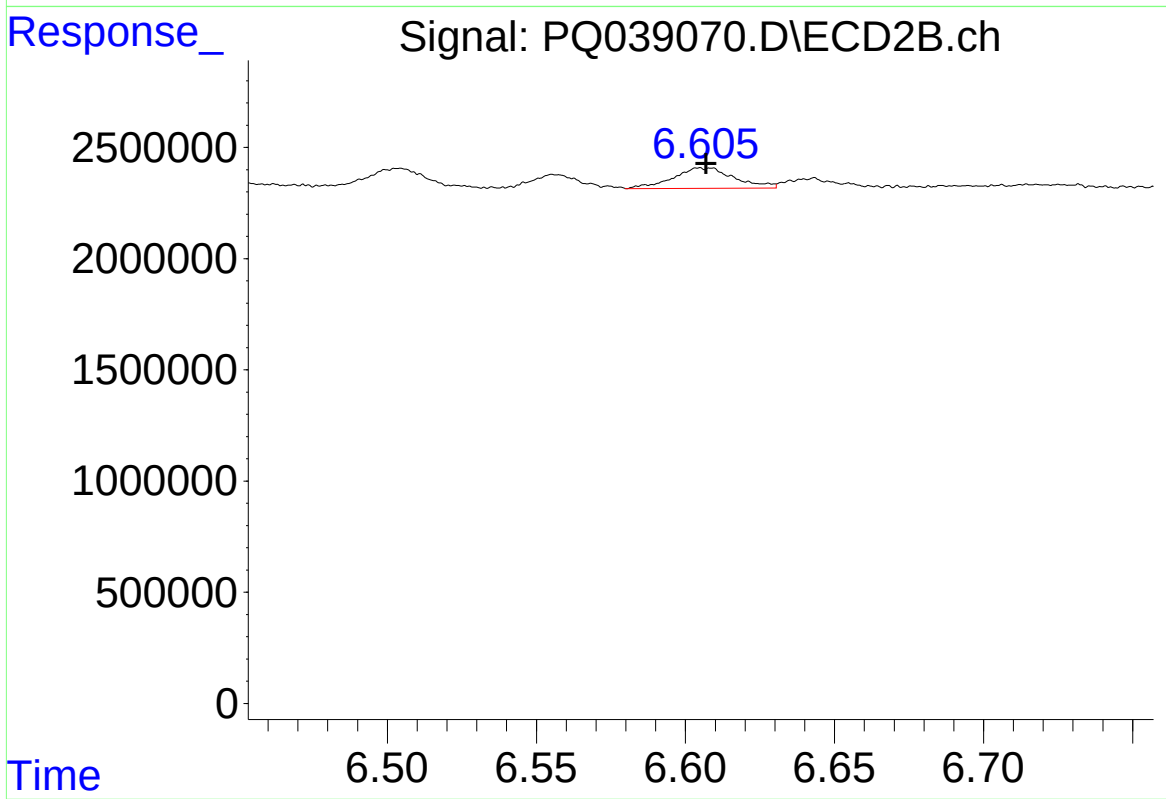

#14 AR-1232-4

R.T.: 6.606 min
Delta R.T.: 0.000 min
Response: 1318915
Conc: 62.65 ng/ml

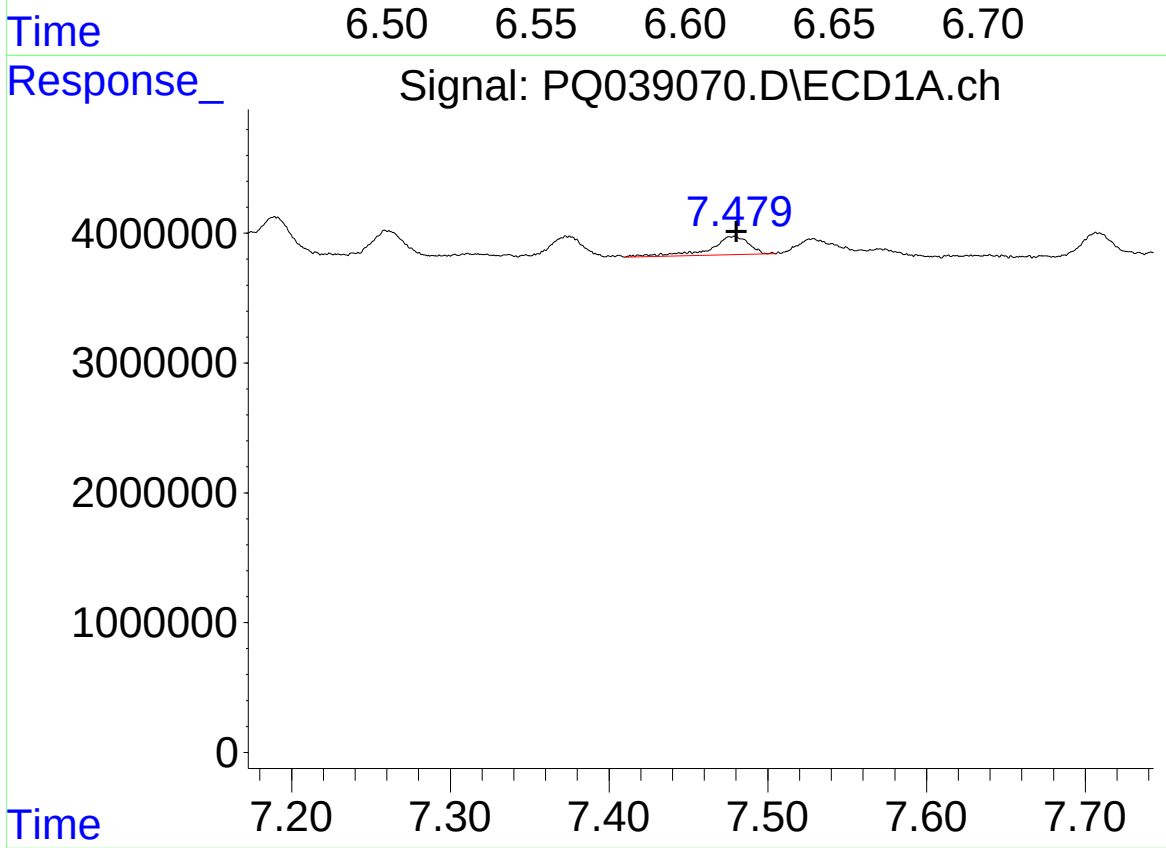

#15 AR-1232-5

R.T.: 7.478 min
Delta R.T.: -0.002 min
Response: 2325765
Conc: 56.50 ng/ml

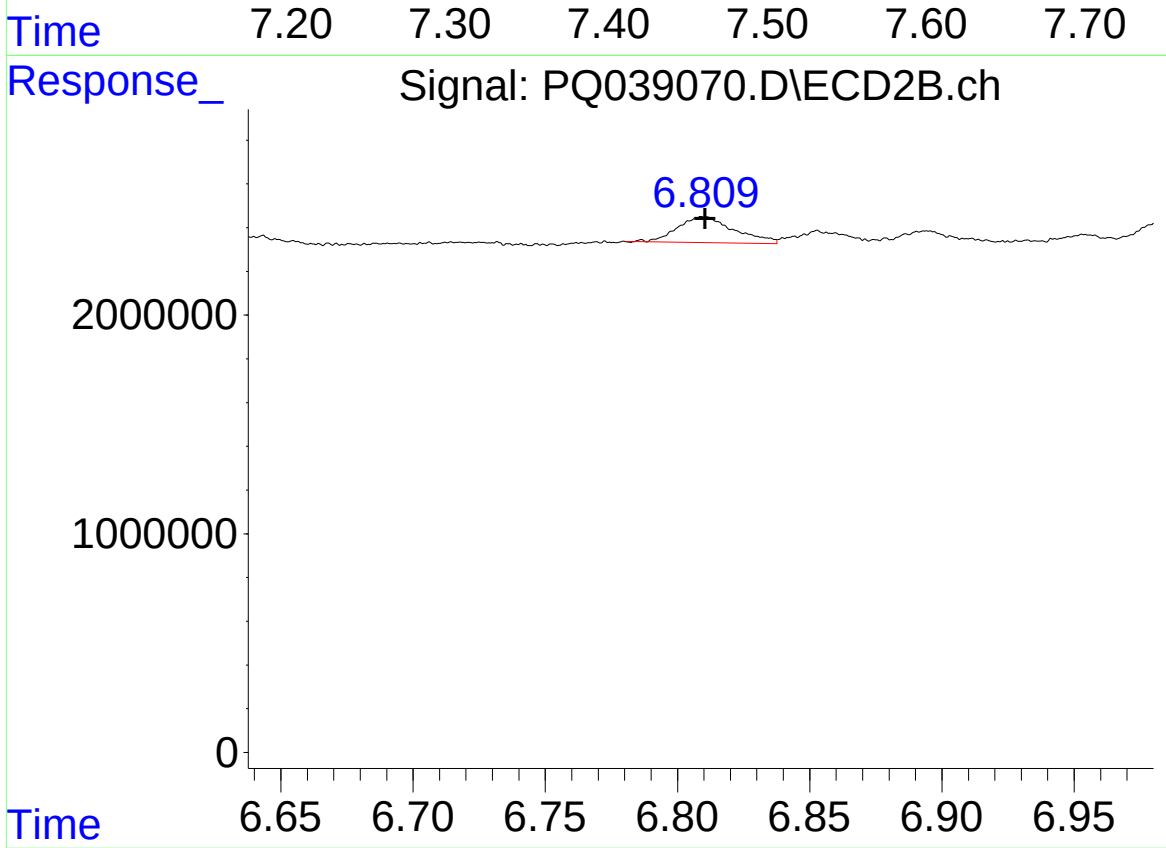

#15 AR-1232-5

R.T.: 6.810 min
Delta R.T.: 0.000 min
Response: 1780813
Conc: 73.07 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

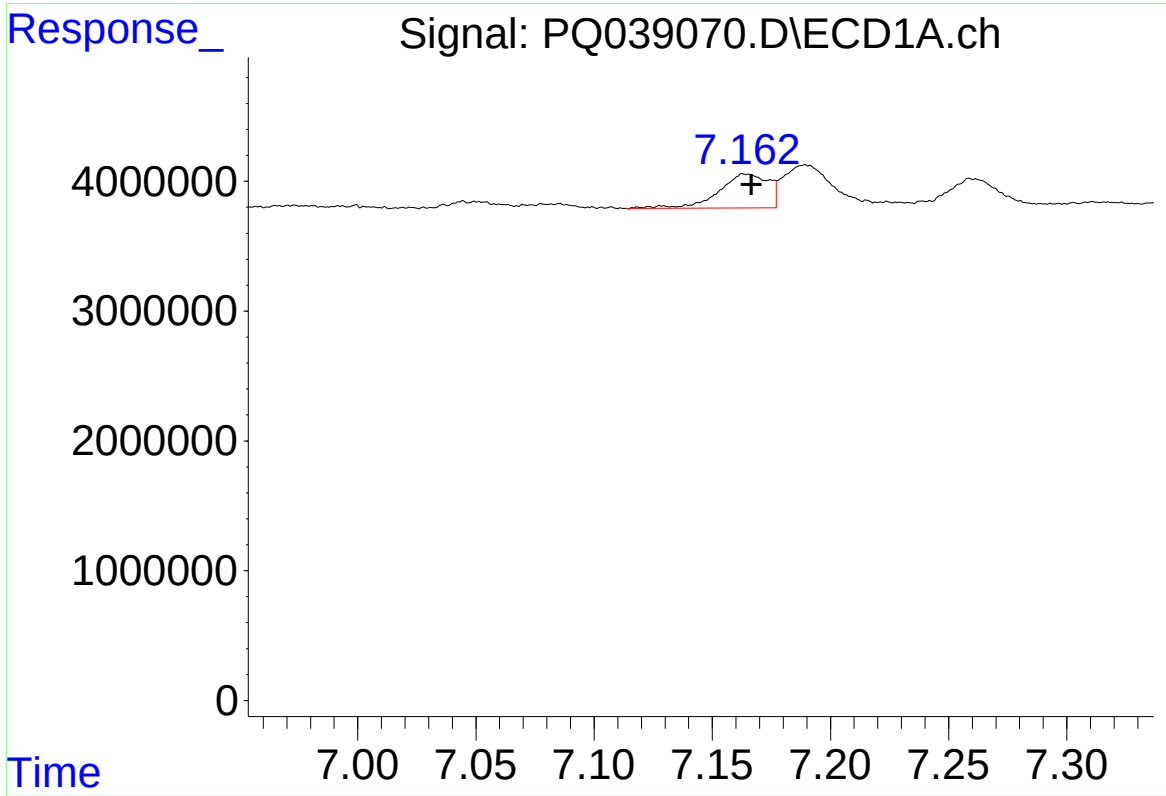

#16 AR-1242-1

R.T.: 7.165 min
Delta R.T.: -0.002 min
Response: 3830810
Conc: 34.16 ng/ml

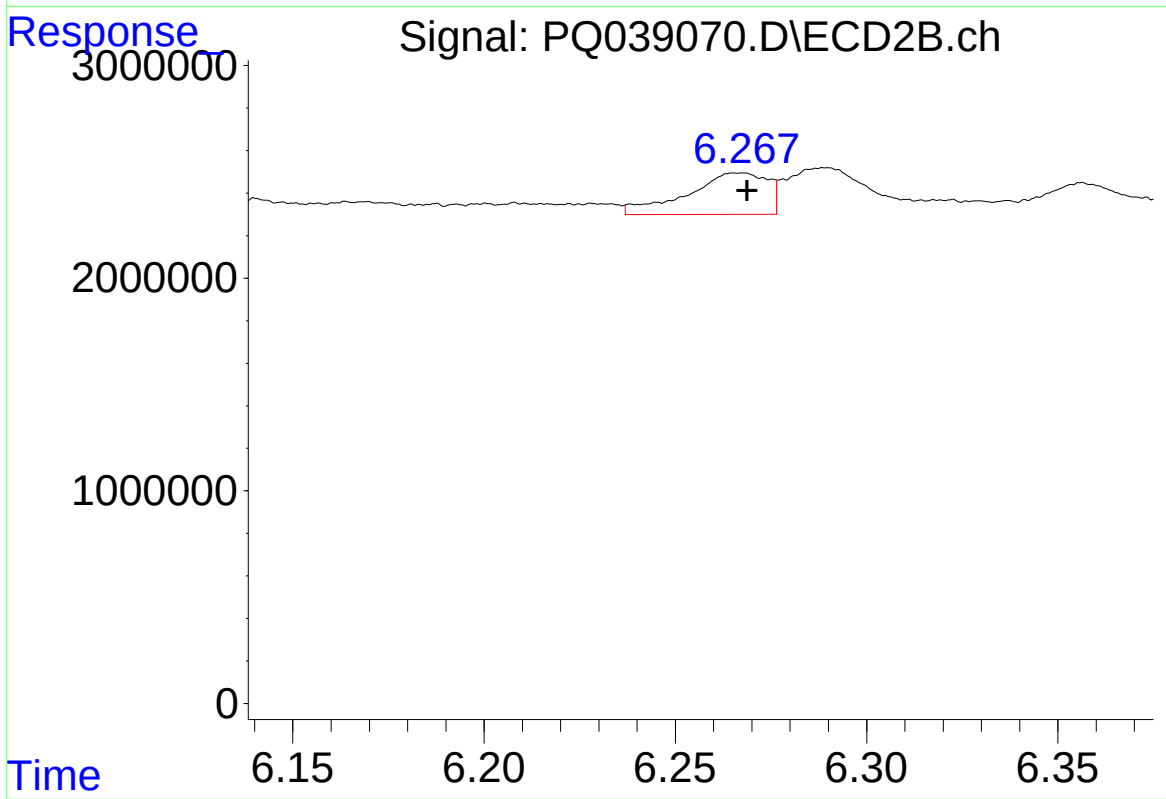

#16 AR-1242-1

R.T.: 6.267 min
Delta R.T.: -0.002 min
Response: 2839641
Conc: 48.38 ng/ml

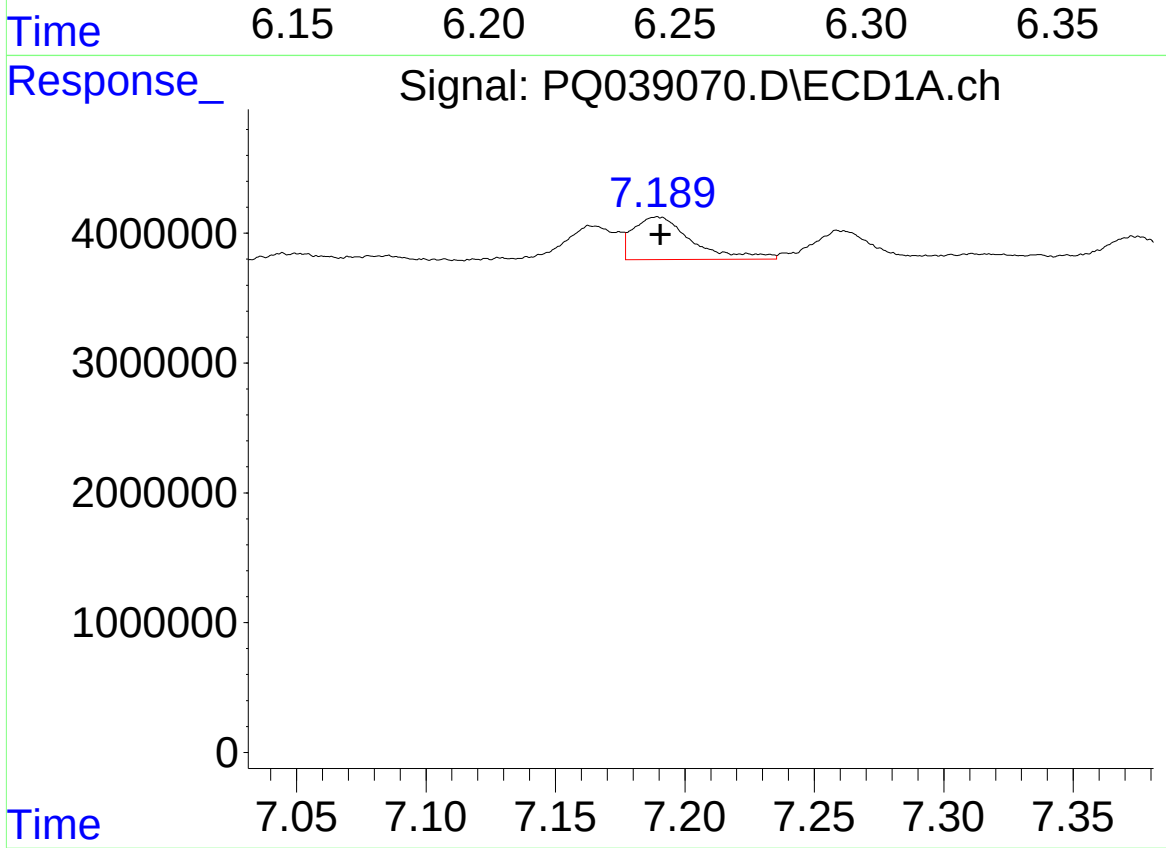

#17 AR-1242-2

R.T.: 7.189 min
Delta R.T.: -0.001 min
Response: 5185677
Conc: 31.58 ng/ml

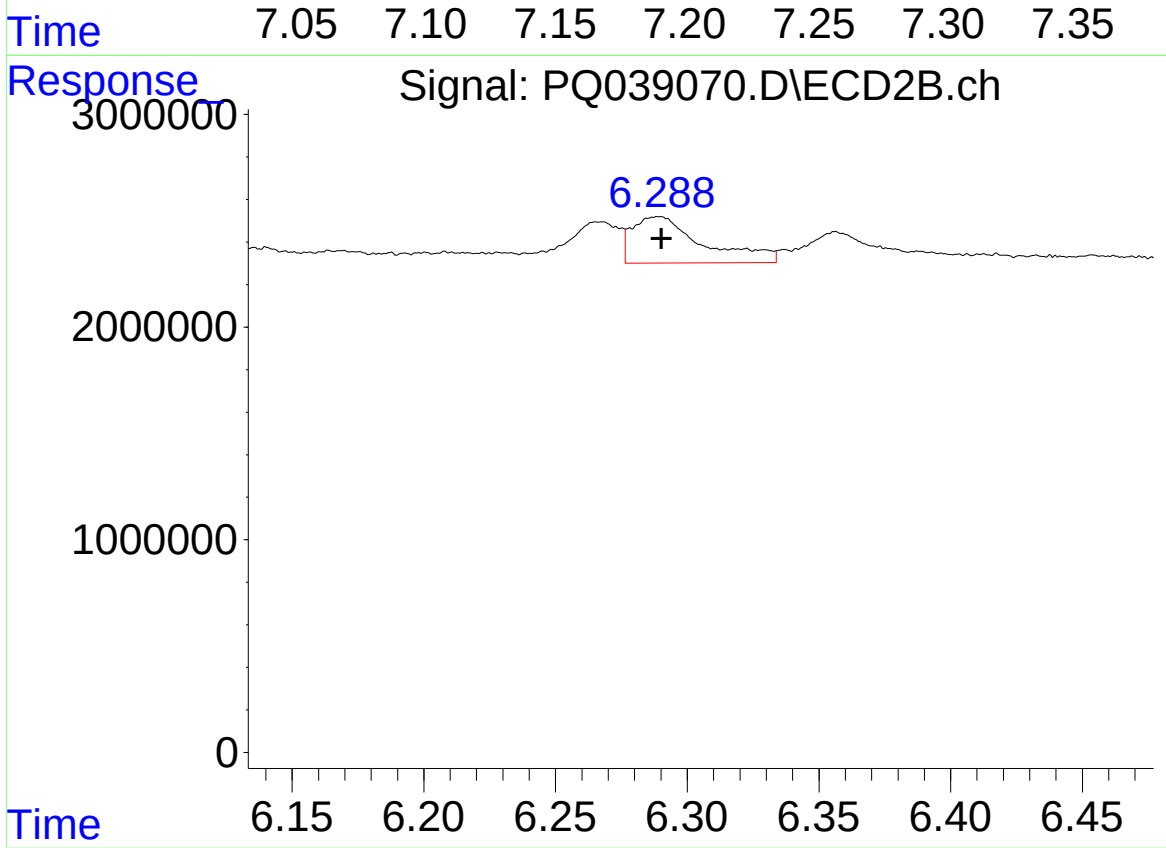

#17 AR-1242-2

R.T.: 6.289 min
Delta R.T.: -0.002 min
Response: 4094839
Conc: 47.65 ng/ml

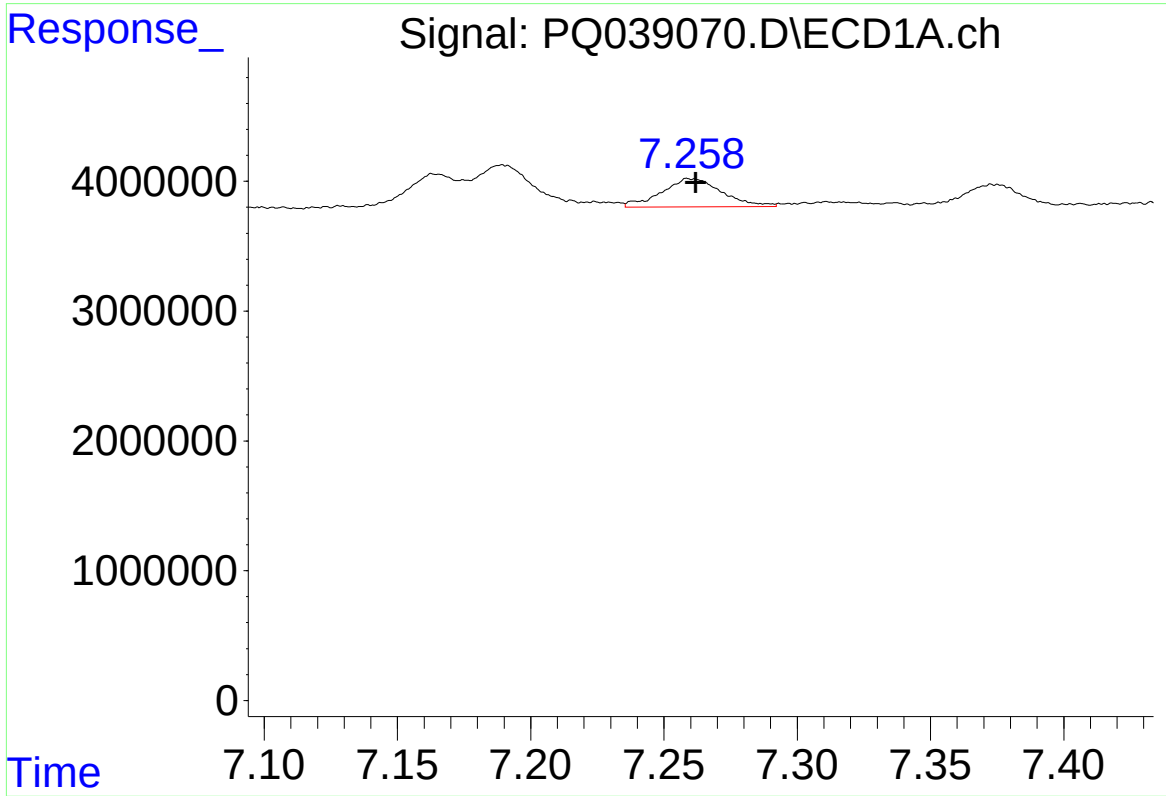

#18 AR-1242-3

R.T.: 7.261 min
Delta R.T.: -0.001 min
Response: 3430935
Conc: 31.50 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

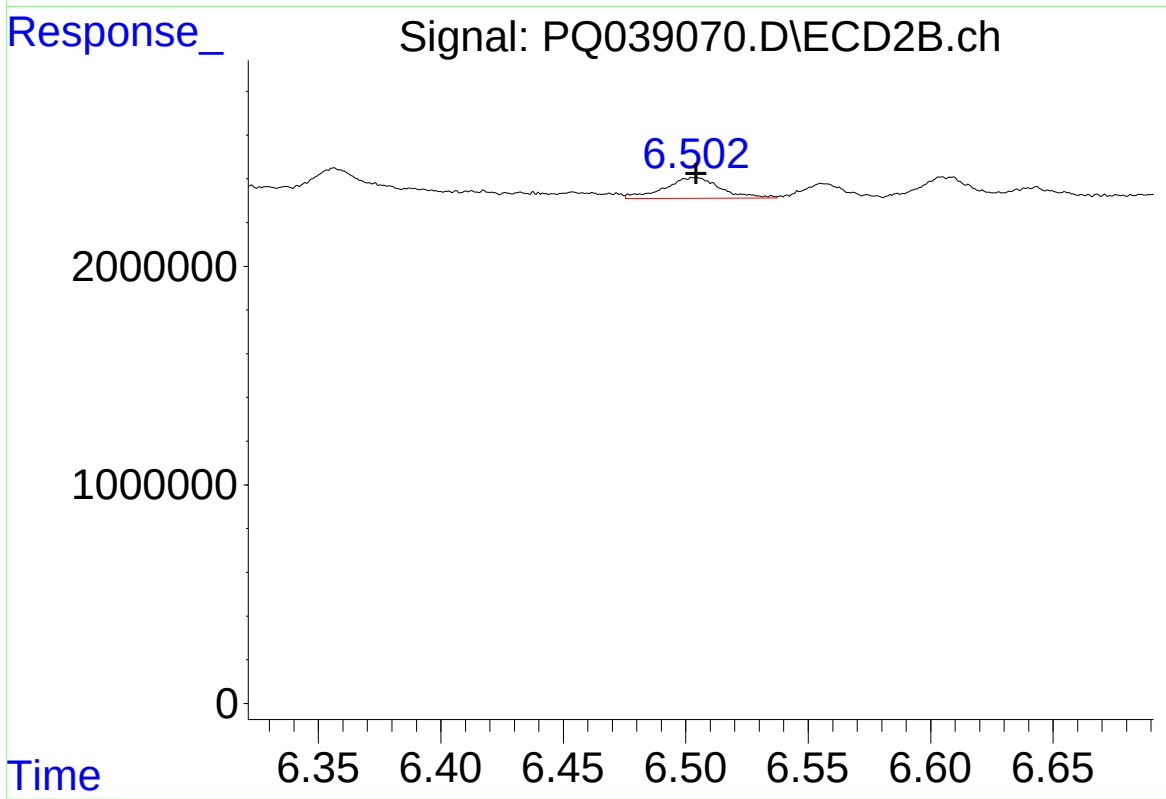

#18 AR-1242-3

R.T.: 6.503 min
Delta R.T.: 0.000 min
Response: 1509359
Conc: 35.75 ng/ml

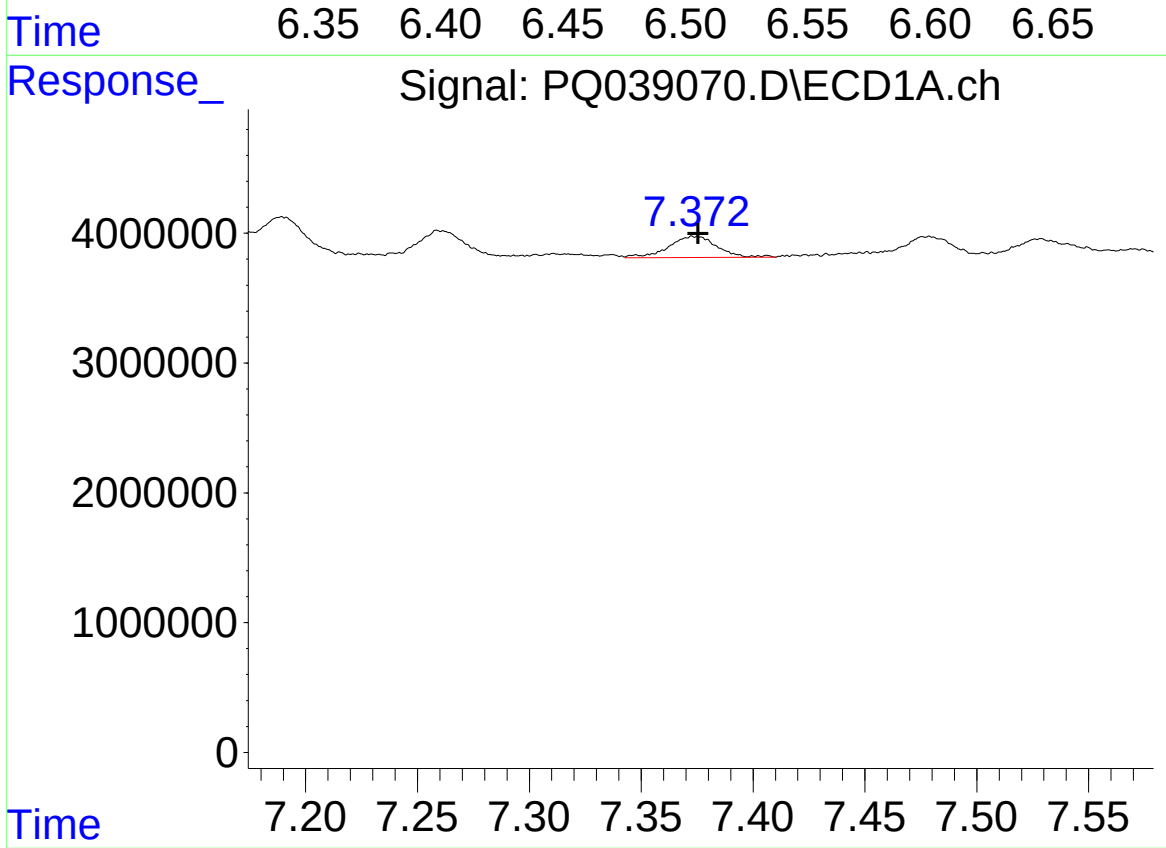

#19 AR-1242-4

R.T.: 7.374 min
Delta R.T.: -0.001 min
Response: 2449757
Conc: 28.31 ng/ml

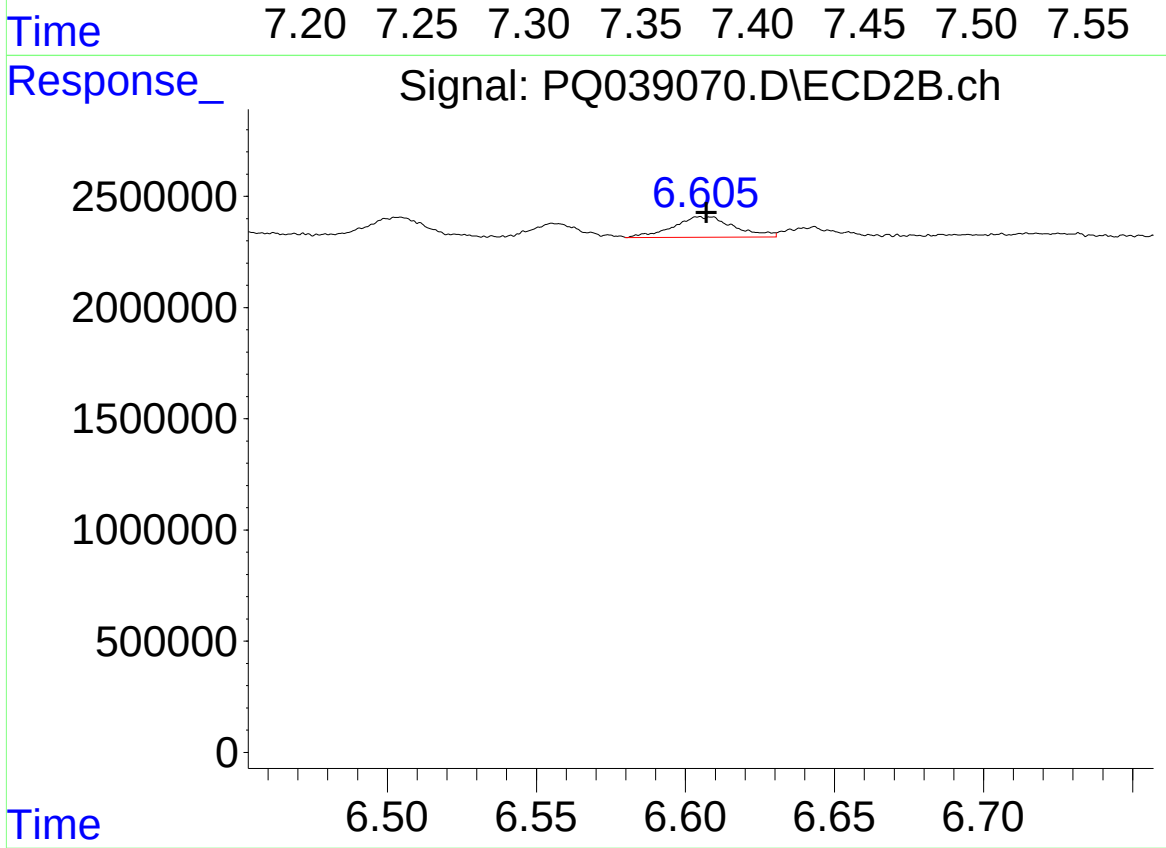

#19 AR-1242-4

R.T.: 6.606 min
Delta R.T.: 0.000 min
Response: 1318915
Conc: 29.45 ng/ml

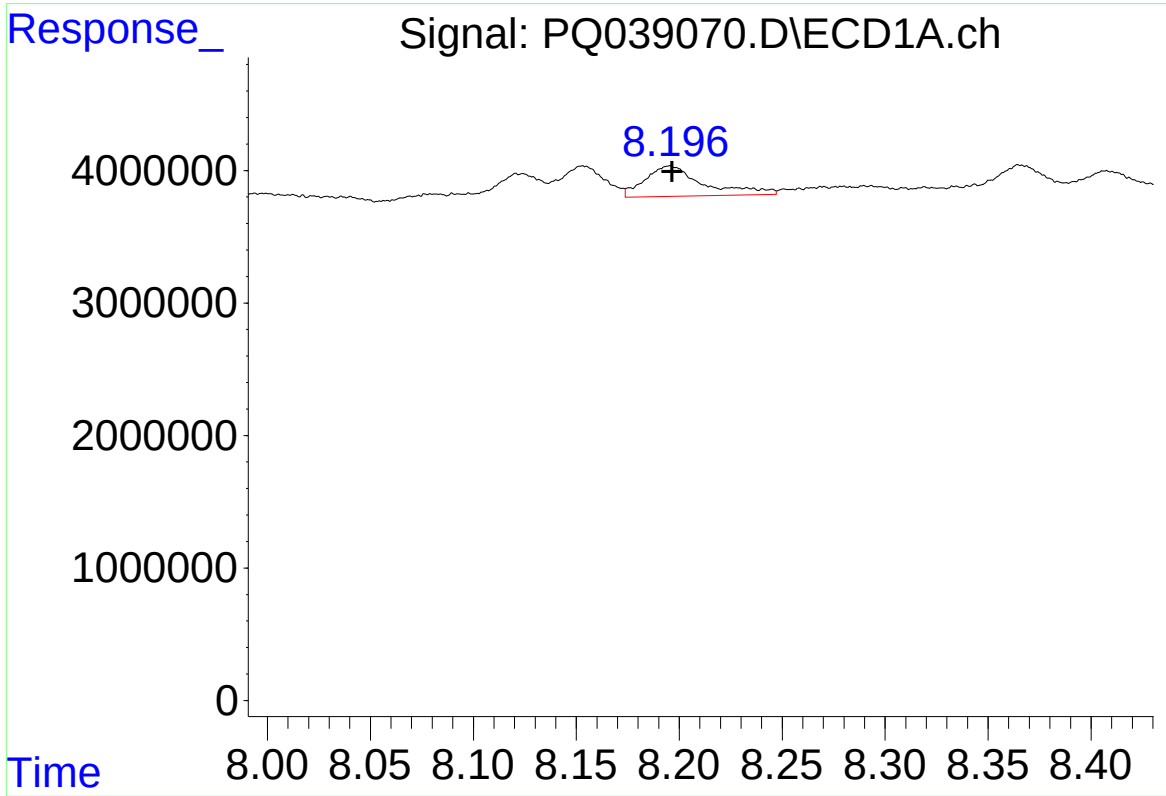

#20 AR-1242-5

R.T.: 8.195 min
Delta R.T.: -0.001 min
Response: 4545582
Conc: 46.01 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

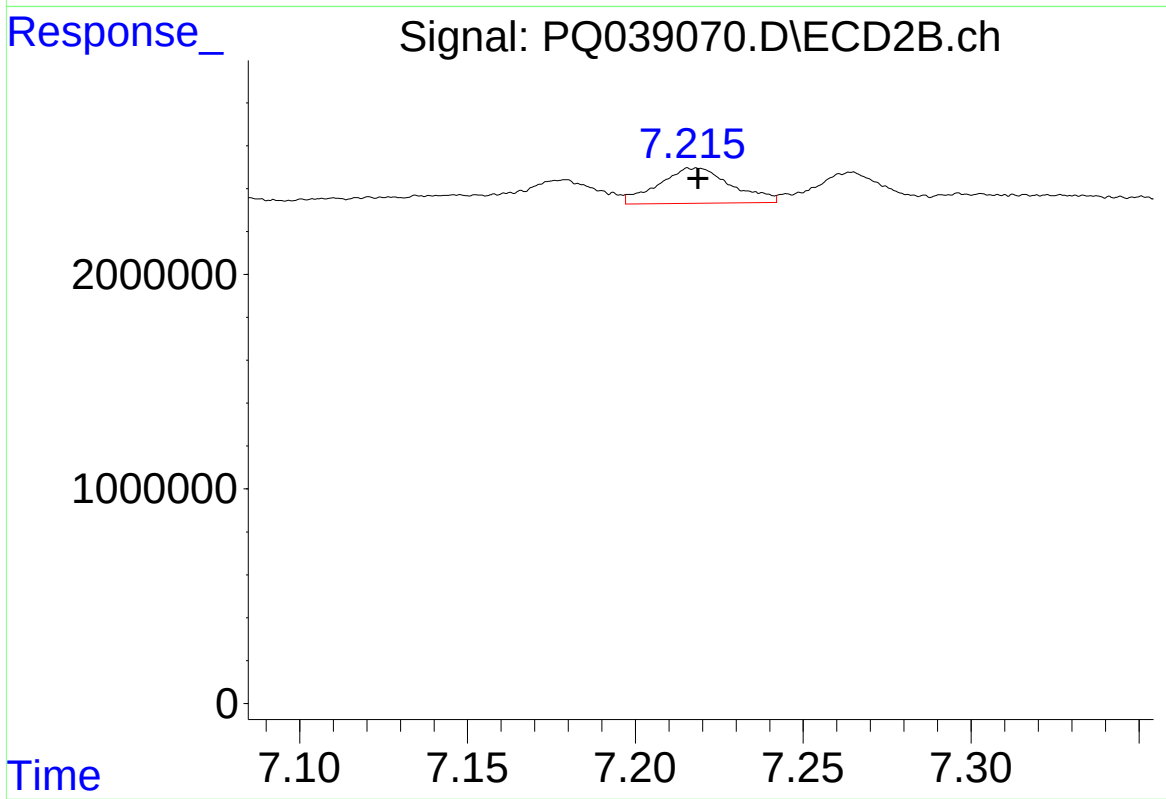

#20 AR-1242-5

R.T.: 7.218 min
Delta R.T.: 0.000 min
Response: 2500125
Conc: 38.55 ng/ml

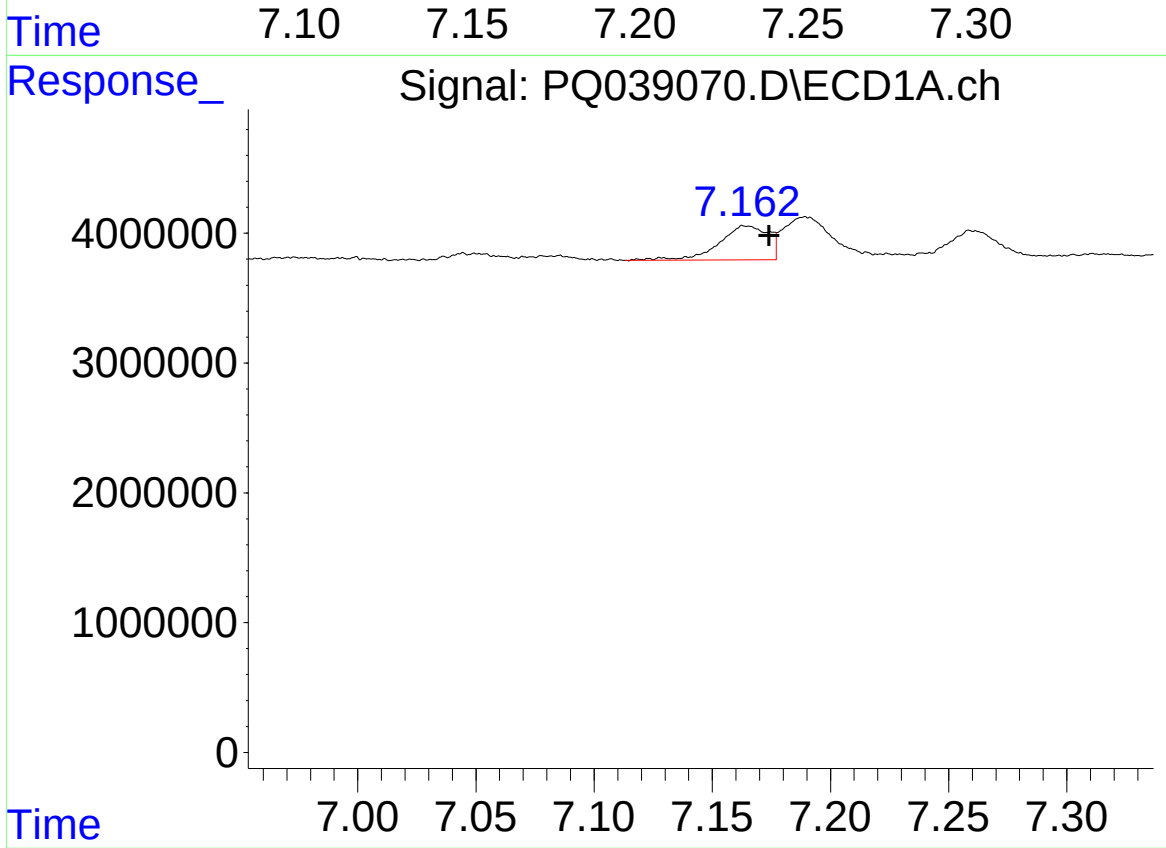

#21 AR-1248-1

R.T.: 7.165 min
Delta R.T.: -0.009 min
Response: 3830810
Conc: 46.33 ng/ml

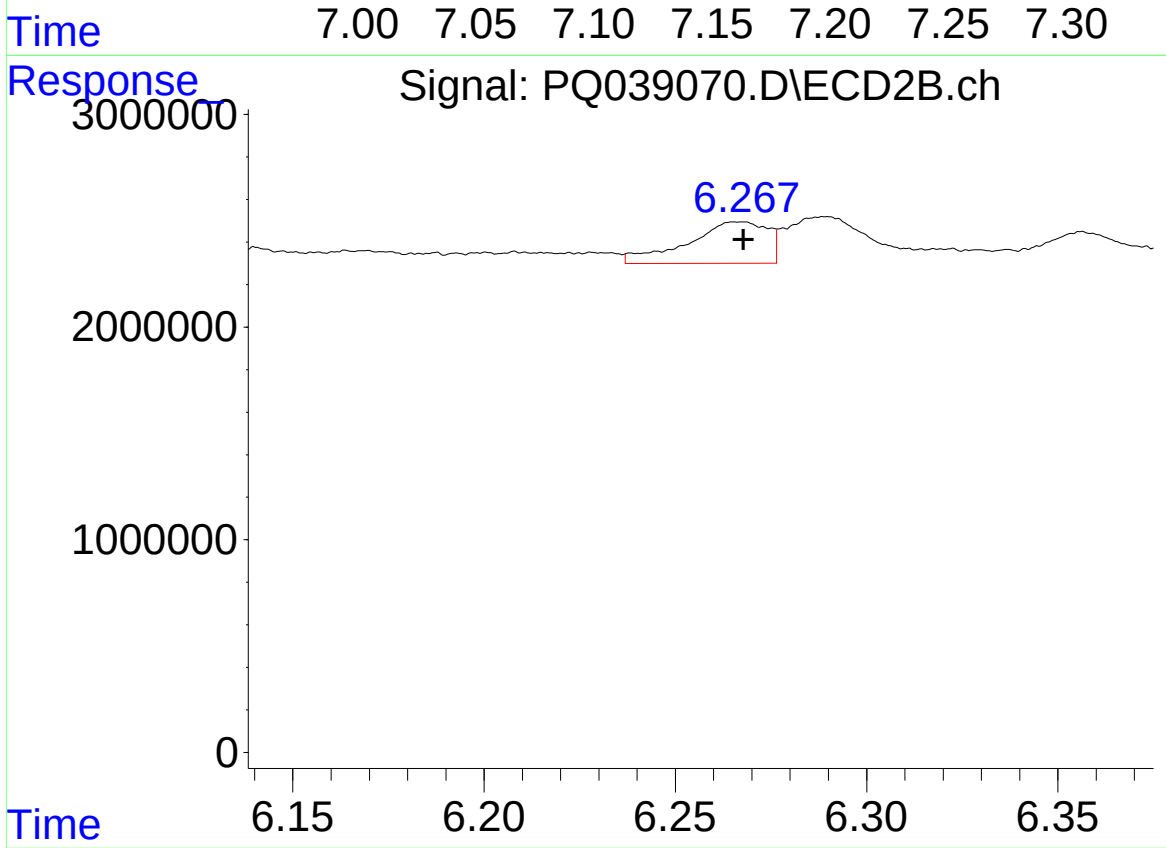

#21 AR-1248-1

R.T.: 6.267 min
Delta R.T.: 0.000 min
Response: 2839641
Conc: 63.72 ng/ml

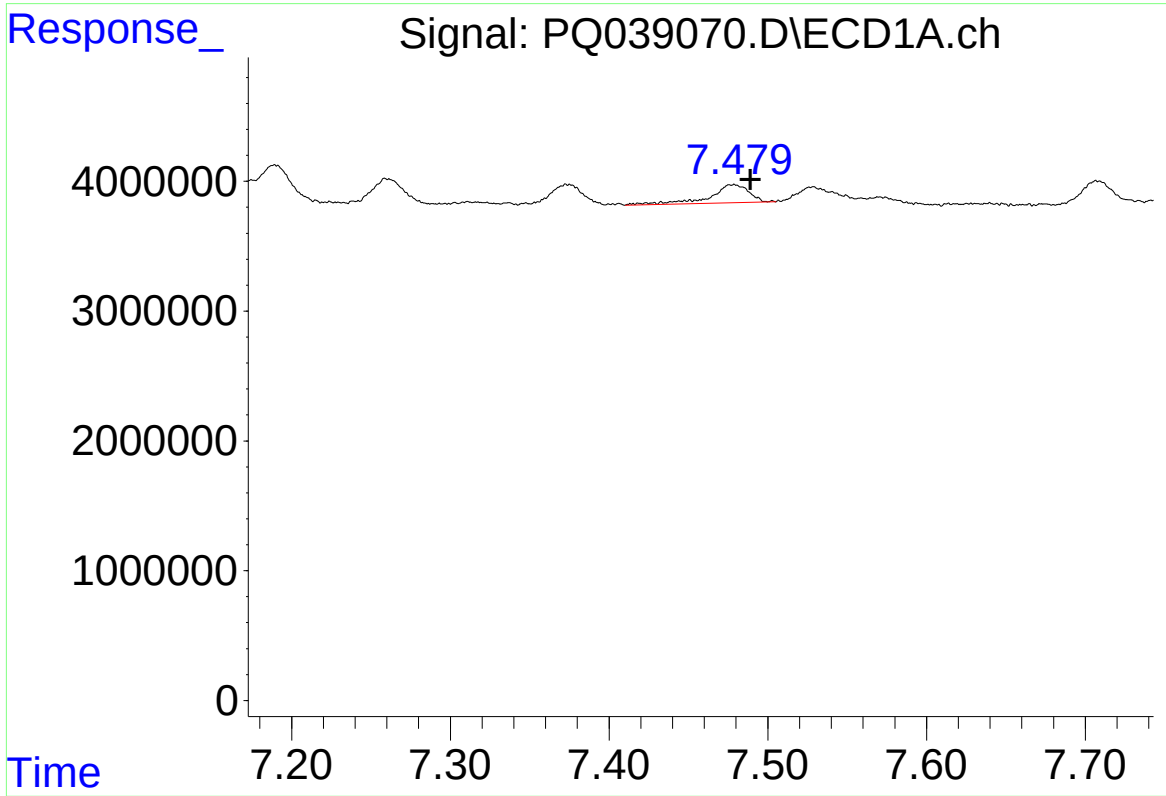

#22 AR-1248-2

R.T.: 7.478 min
Delta R.T.: -0.011 min
Response: 2325765
Conc: 20.36 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

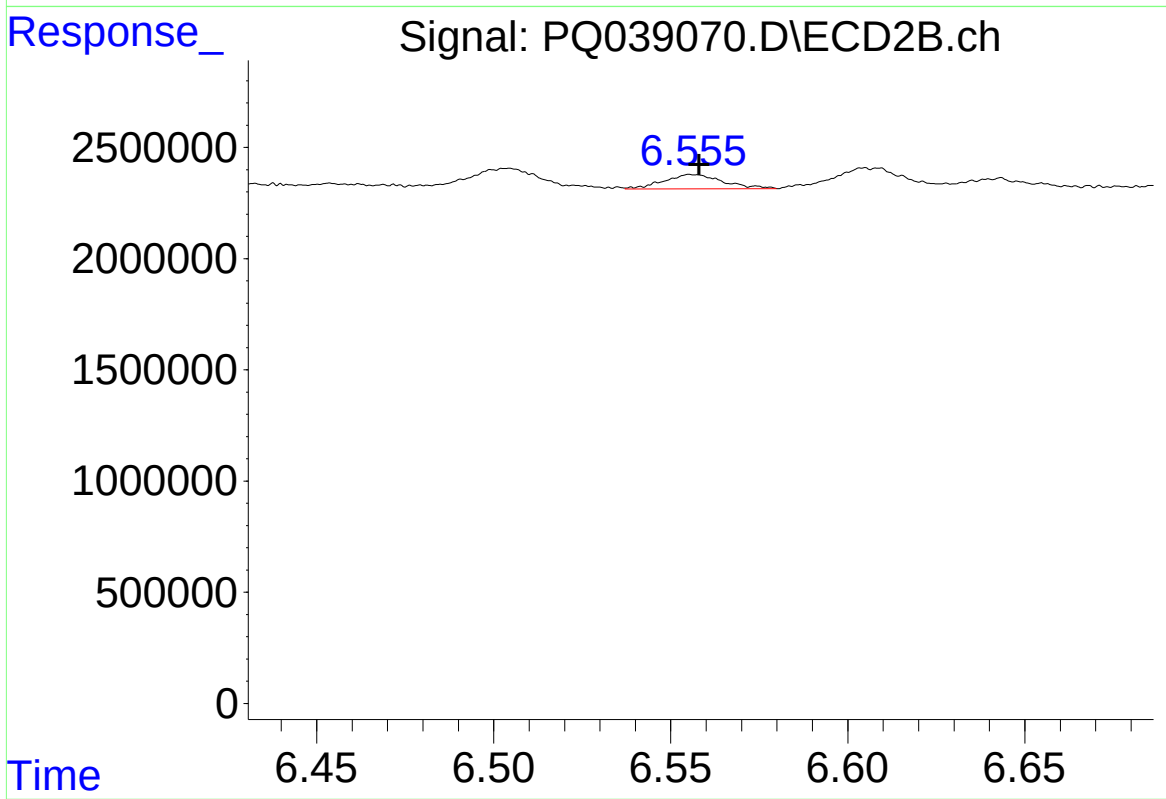

#22 AR-1248-2

R.T.: 6.557 min
Delta R.T.: -0.001 min
Response: 765193
Conc: 12.82 ng/ml

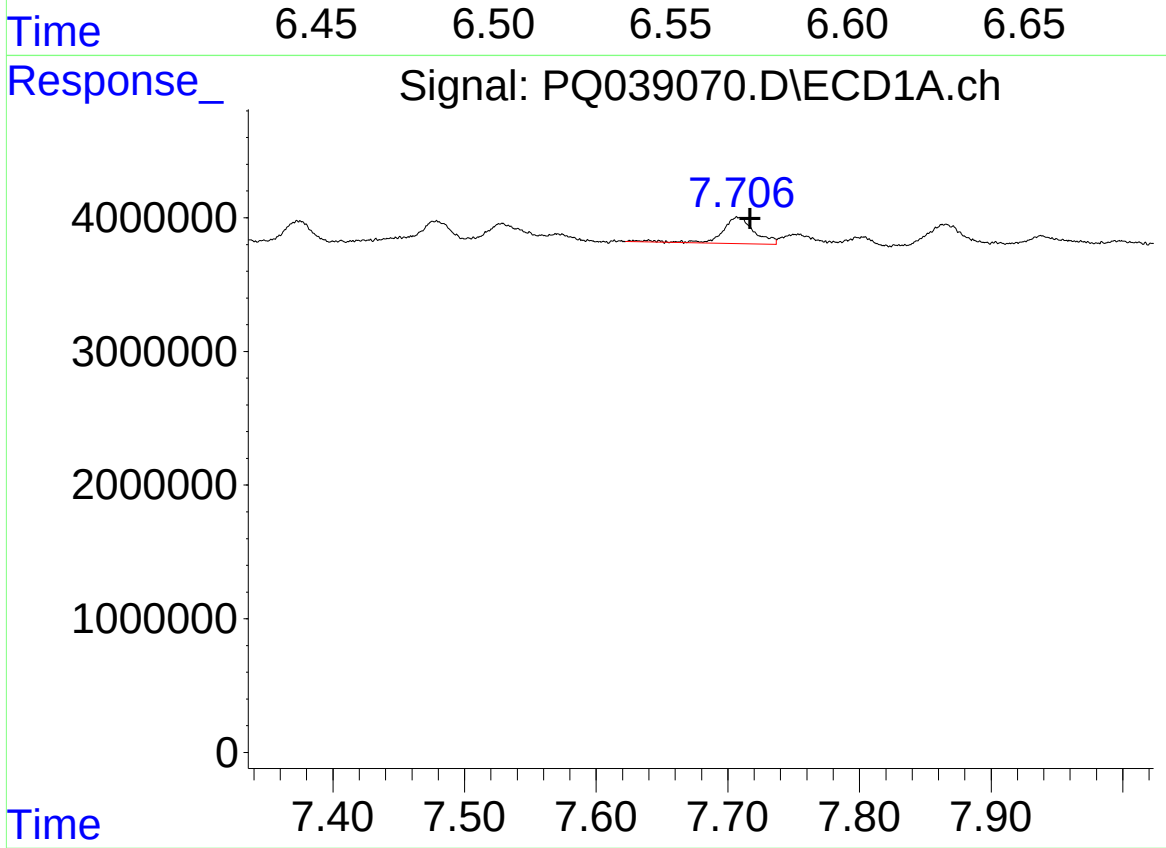

#23 AR-1248-3

R.T.: 7.708 min
Delta R.T.: -0.009 min
Response: 3306250
Conc: 24.12 ng/ml

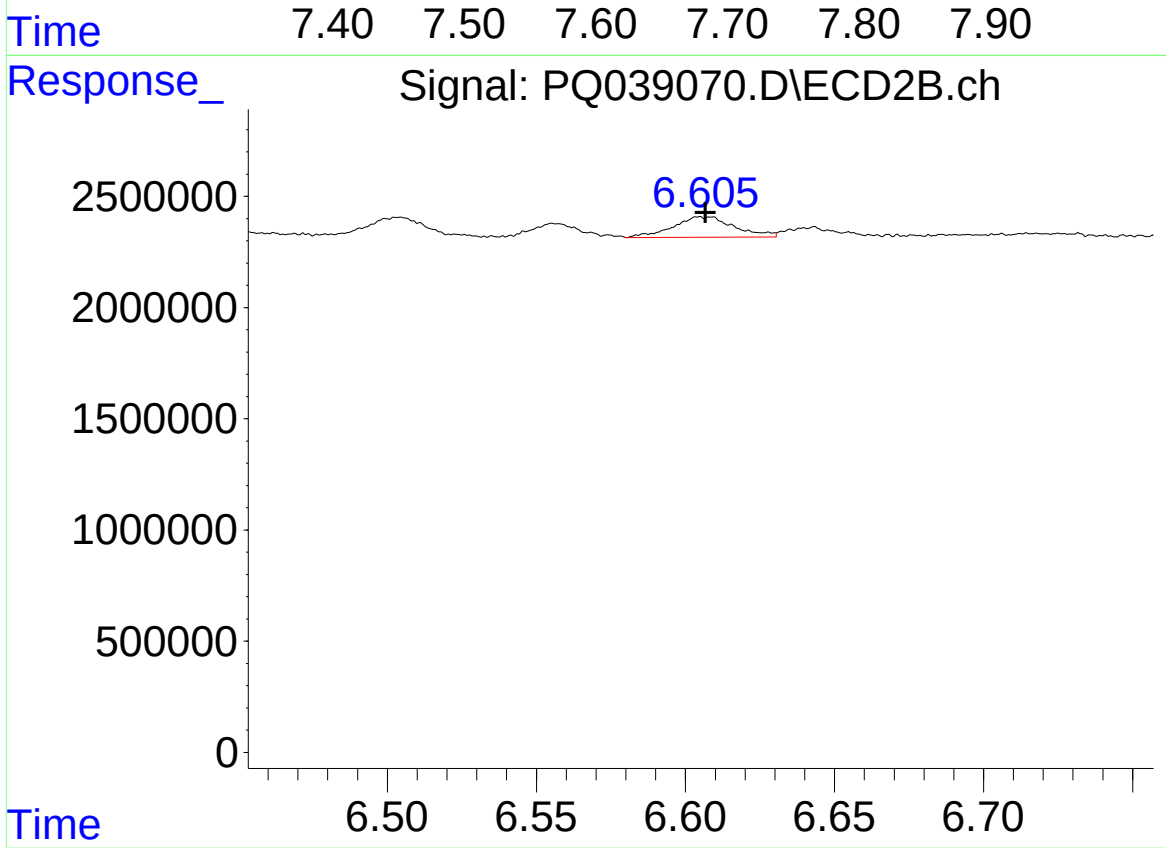

#23 AR-1248-3

R.T.: 6.606 min
Delta R.T.: 0.000 min
Response: 1318915
Conc: 20.60 ng/ml

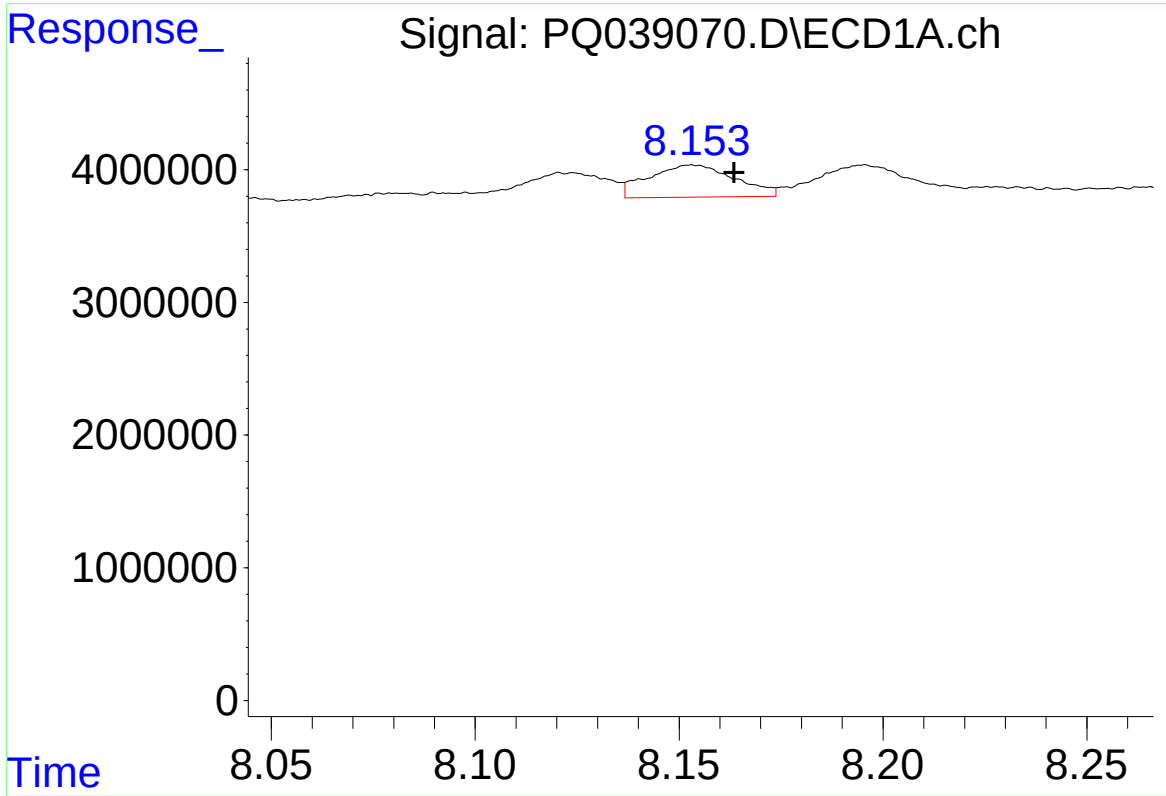

#24 AR-1248-4

R.T.: 8.153 min
Delta R.T.: -0.010 min
Response: 3584484
Conc: 22.97 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

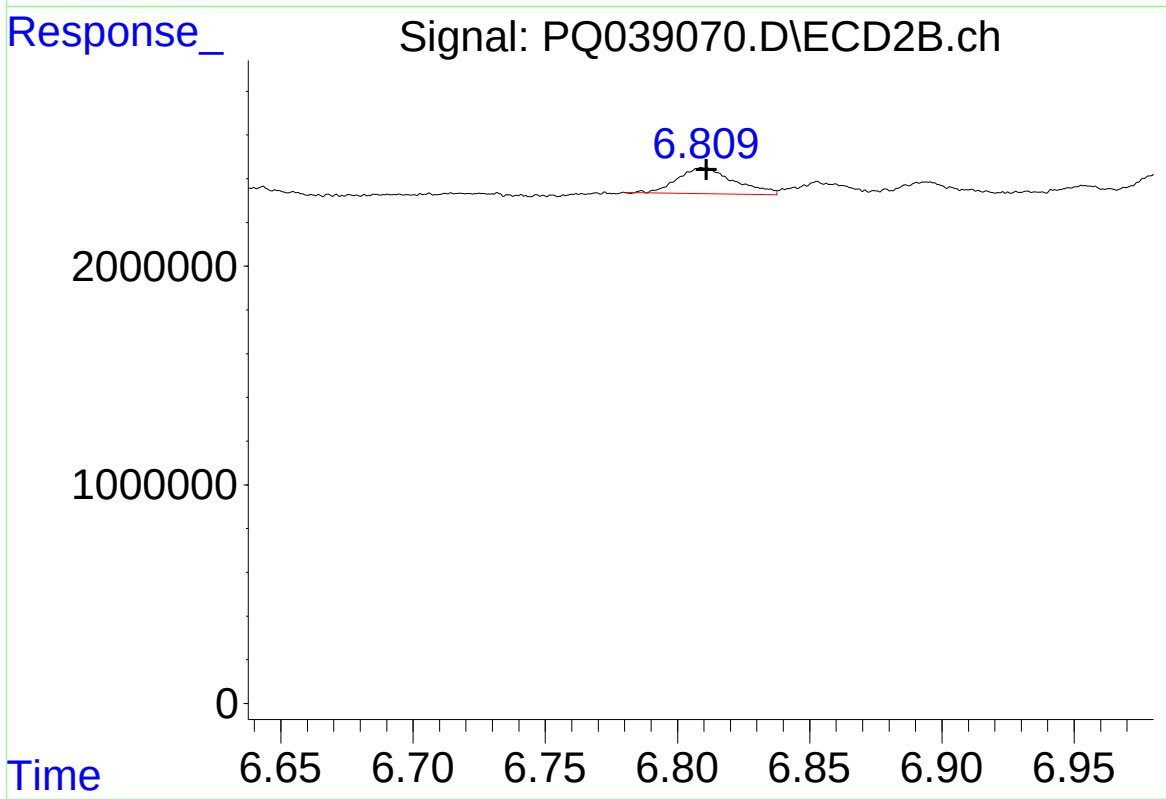

#24 AR-1248-4

R.T.: 6.810 min
Delta R.T.: -0.001 min
Response: 1780813
Conc: 21.64 ng/ml

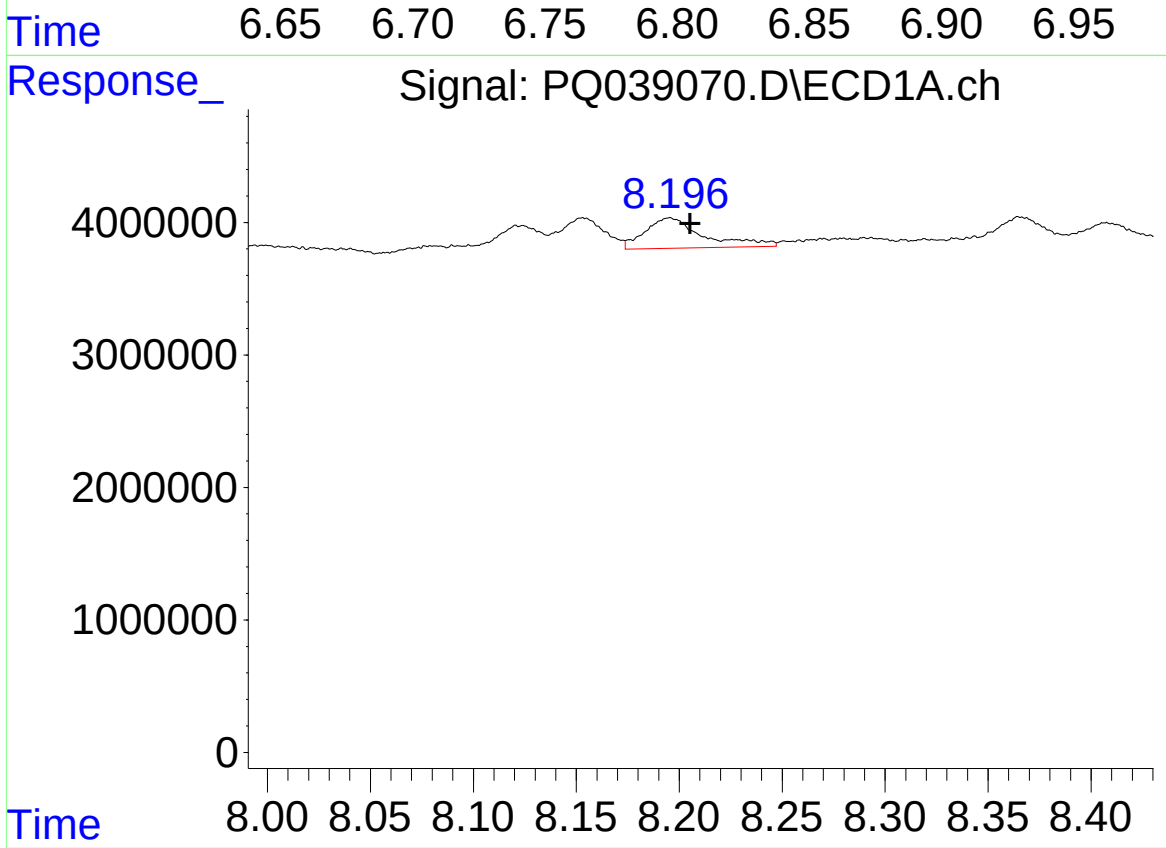

#25 AR-1248-5

R.T.: 8.195 min
Delta R.T.: -0.010 min
Response: 4545582
Conc: 29.72 ng/ml

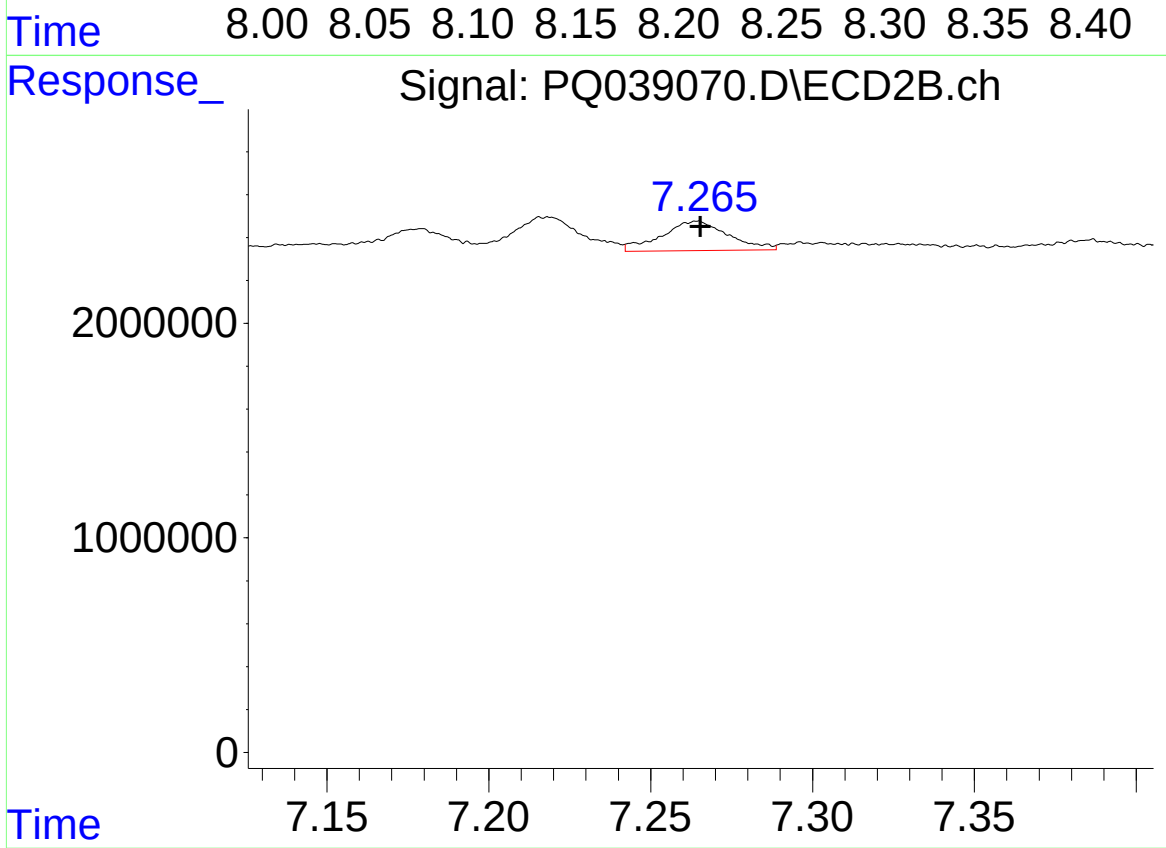

#25 AR-1248-5

R.T.: 7.264 min
Delta R.T.: -0.001 min
Response: 1967306
Conc: 23.62 ng/ml

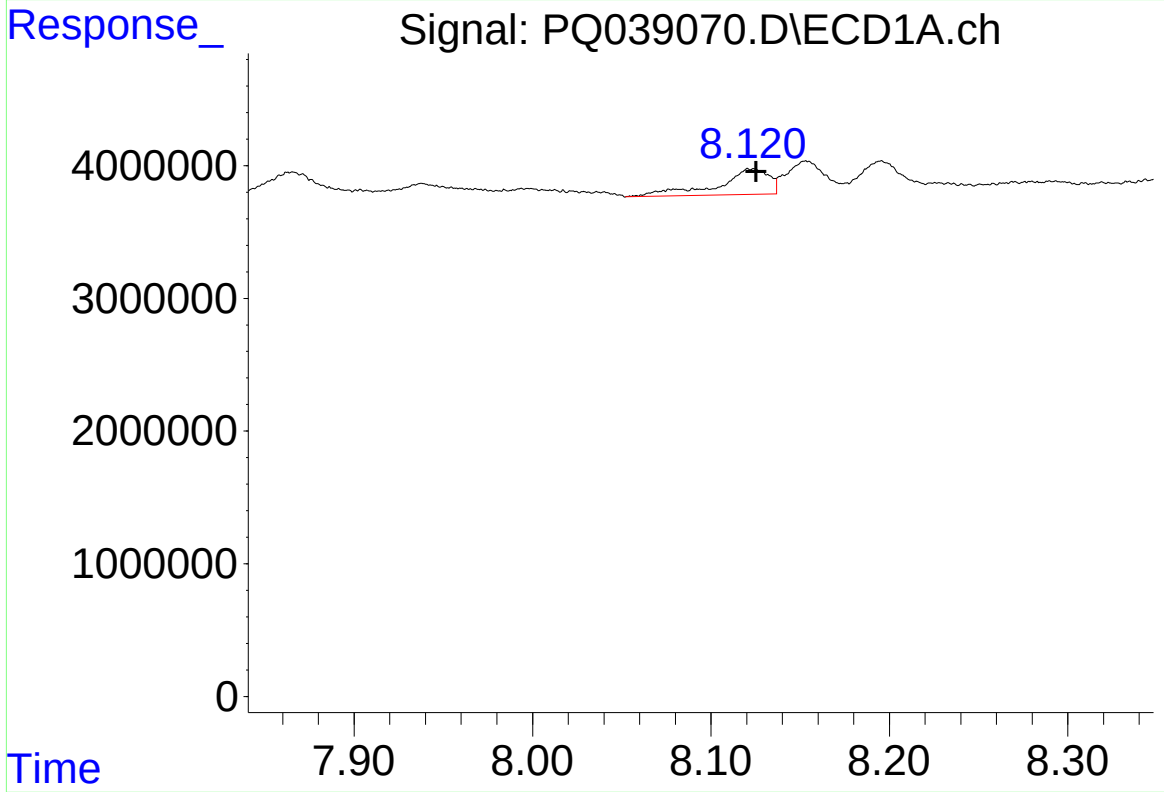

#26 AR-1254-1

R.T.: 8.123 min
Delta R.T.: -0.002 min
Response: 3804391
Conc: 22.10 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

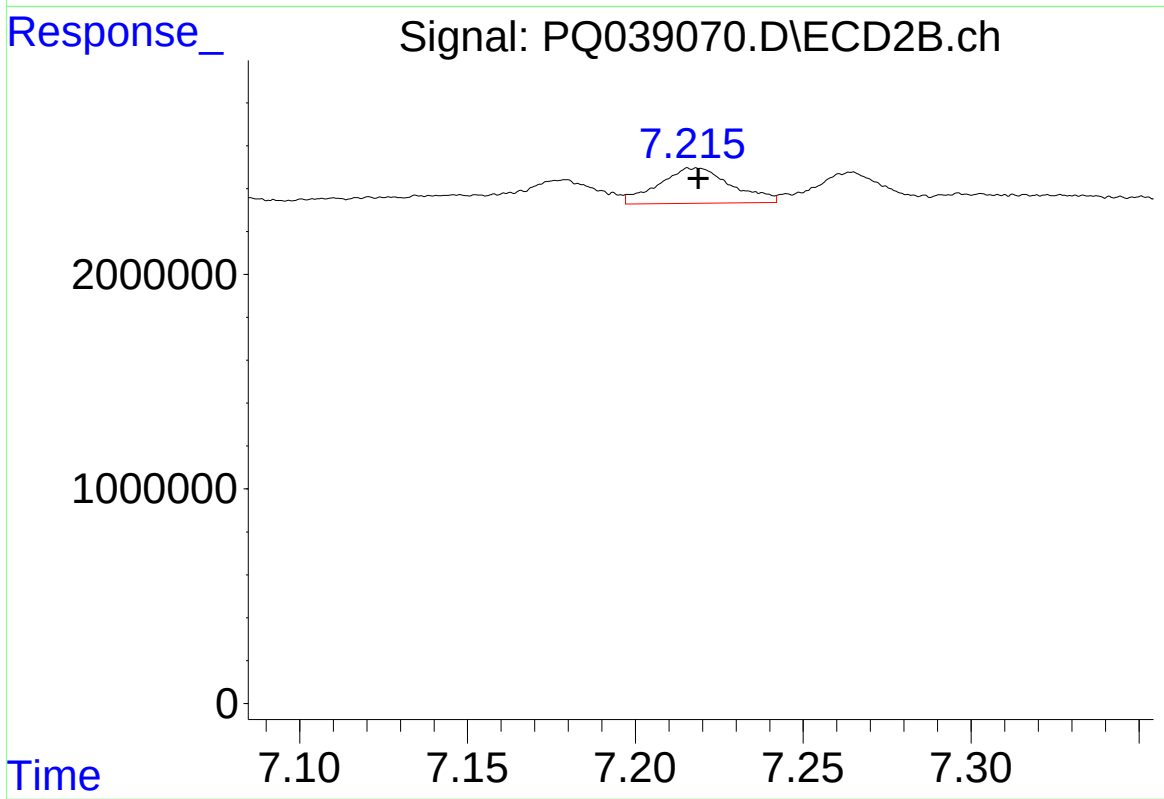

#26 AR-1254-1

R.T.: 7.218 min
Delta R.T.: 0.000 min
Response: 2500125
Conc: 17.50 ng/ml

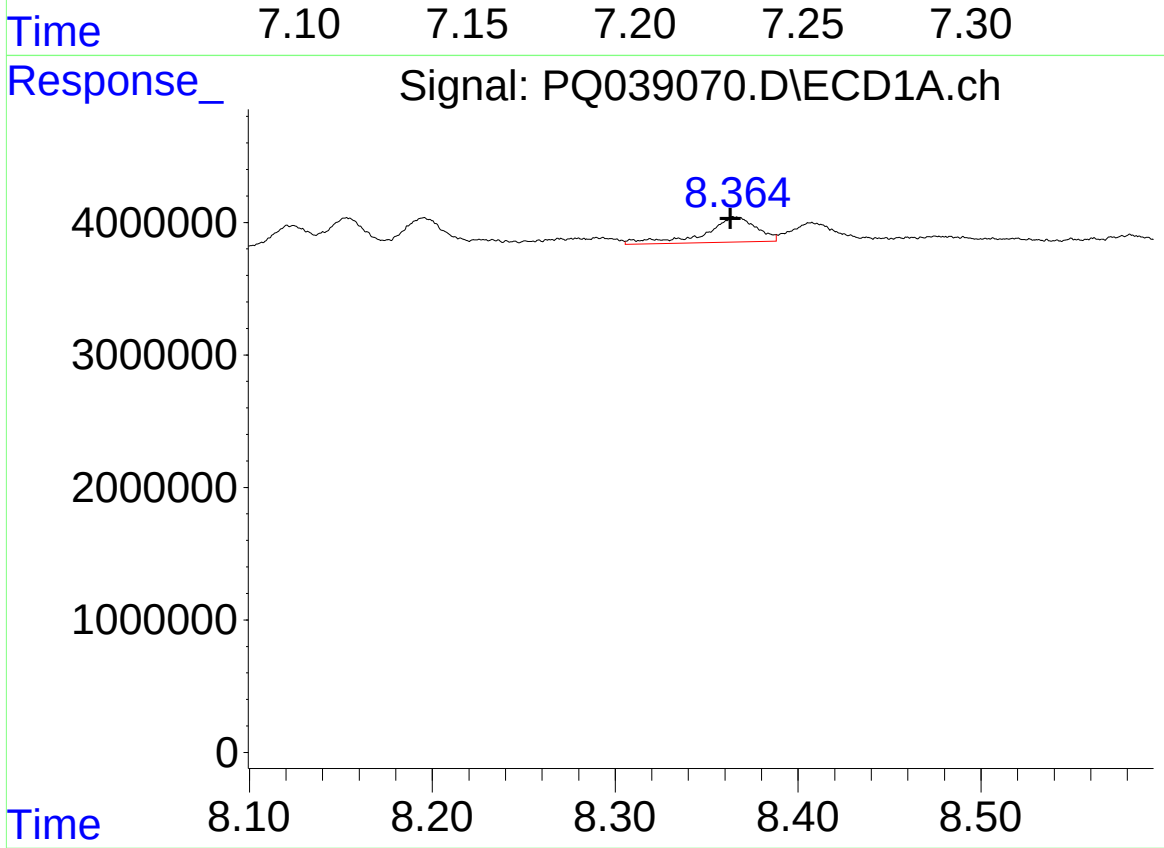

#27 AR-1254-2

R.T.: 8.366 min
Delta R.T.: 0.003 min
Response: 3676717
Conc: 13.43 ng/ml

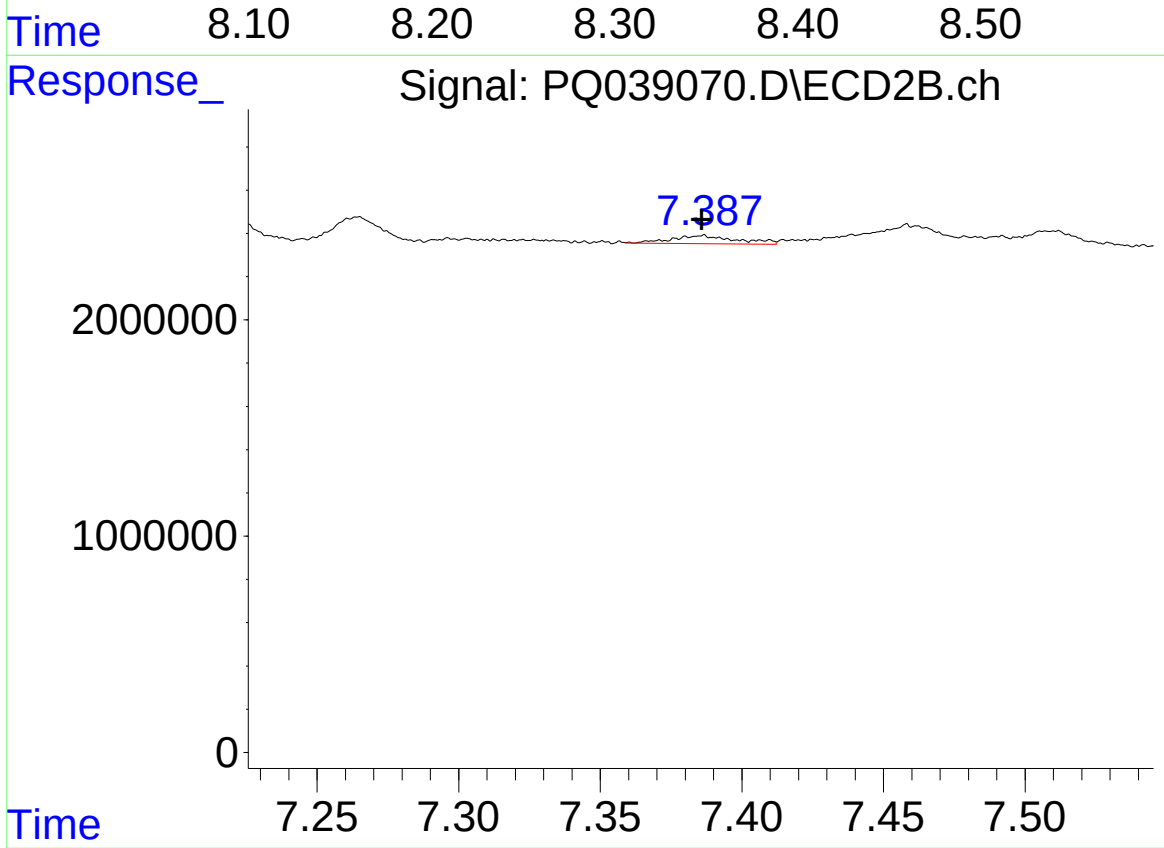

#27 AR-1254-2

R.T.: 7.385 min
Delta R.T.: 0.000 min
Response: 609976
Conc: 4.80 ng/ml

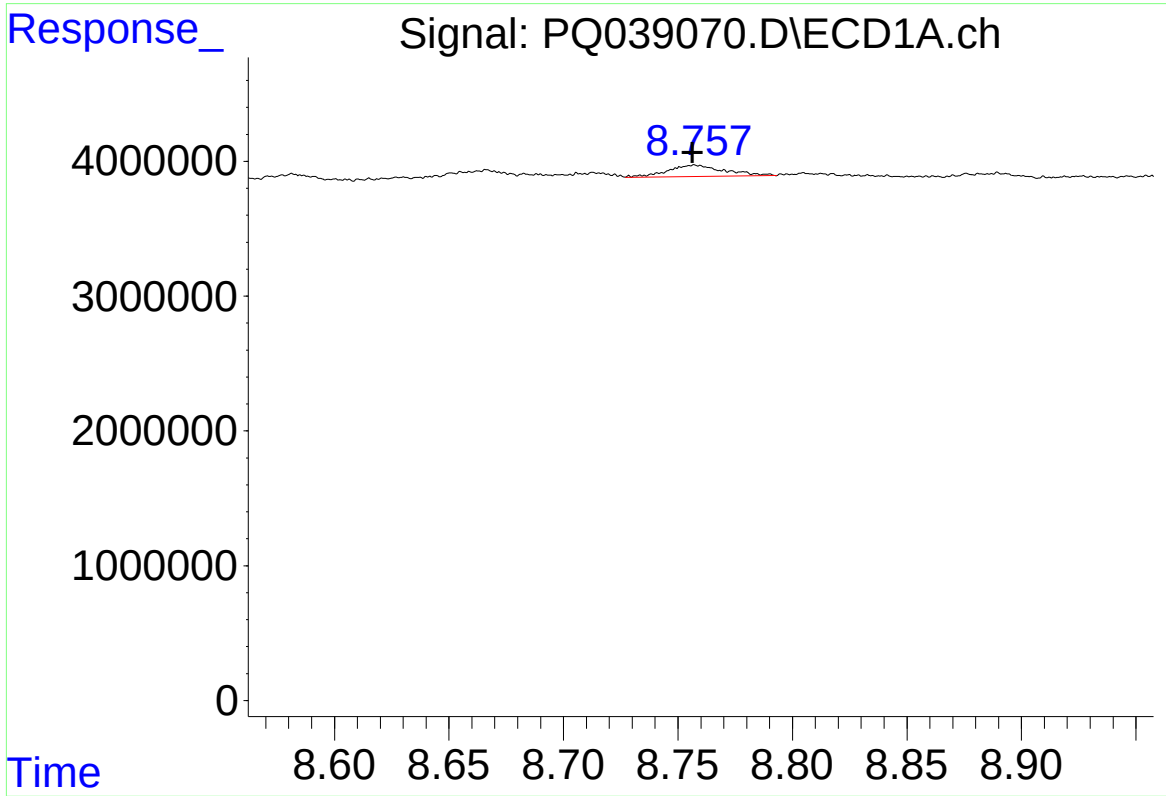

#28 AR-1254-3

R.T.: 8.757 min
Delta R.T.: 0.000 min
Response: 1435035
Conc: 4.67 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

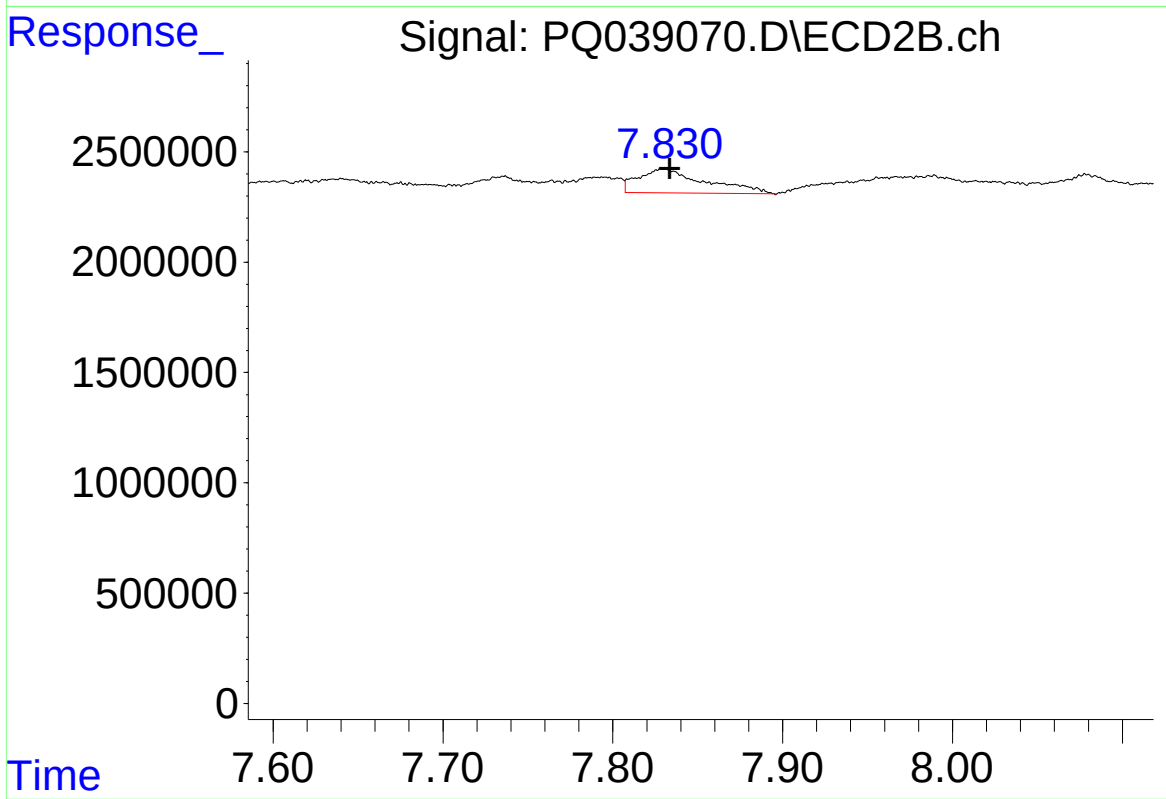

#28 AR-1254-3

R.T.: 7.830 min
Delta R.T.: -0.004 min
Response: 3005418
Conc: 13.43 ng/ml

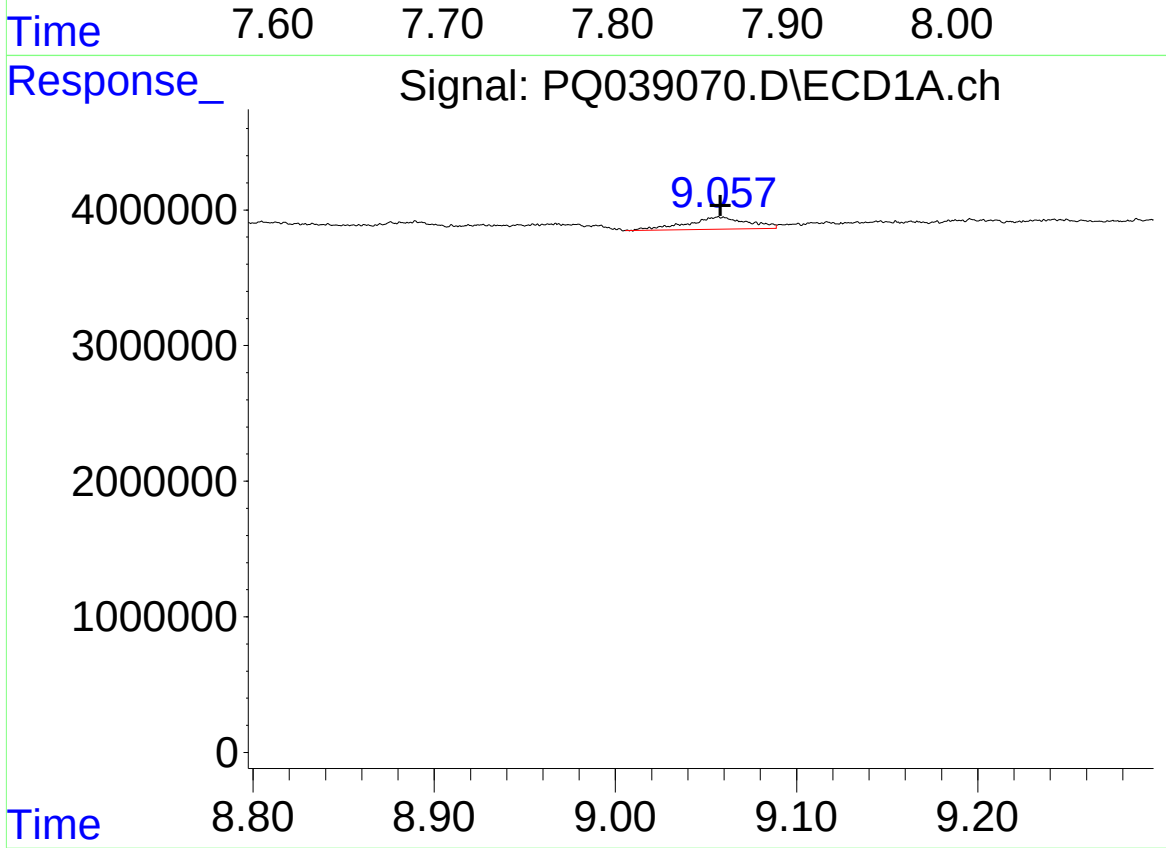

#29 AR-1254-4

R.T.: 9.057 min
Delta R.T.: 0.000 min
Response: 2088218
Conc: 9.40 ng/ml

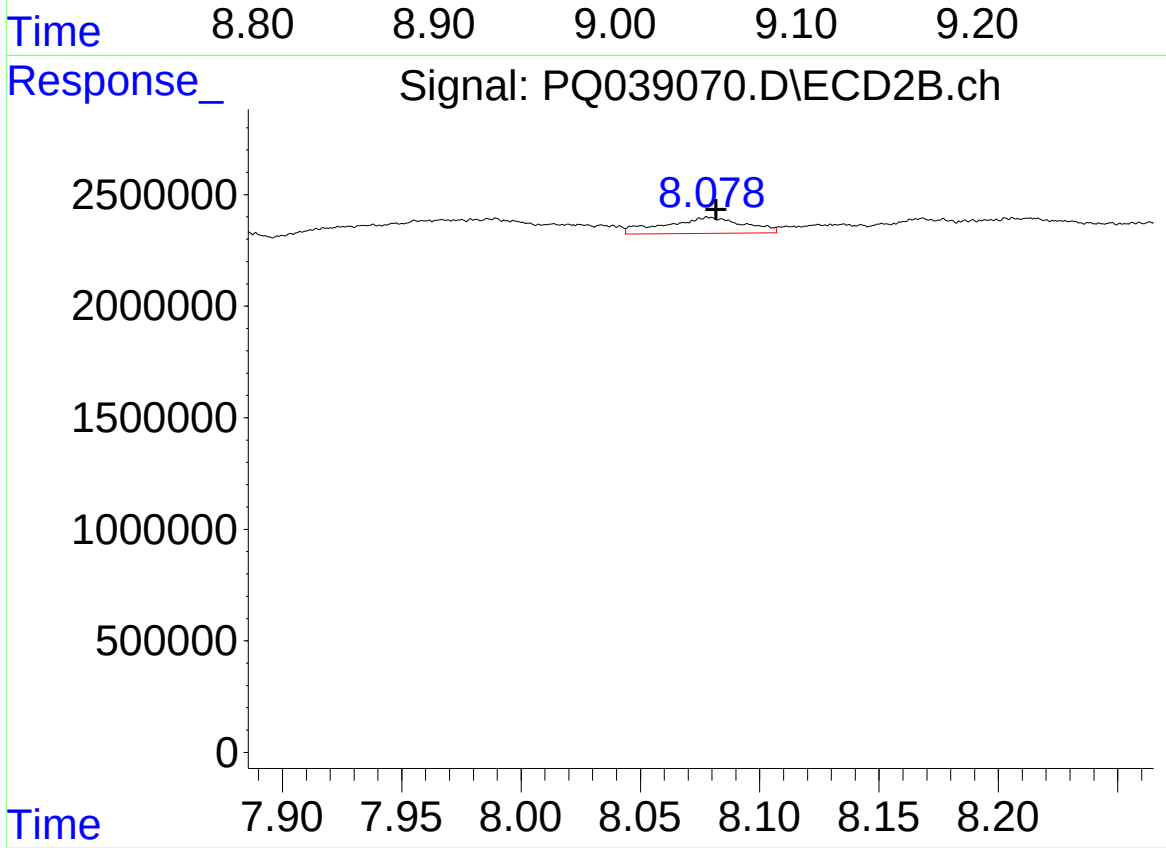

#29 AR-1254-4

R.T.: 8.079 min
Delta R.T.: -0.003 min
Response: 1695317
Conc: 12.09 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

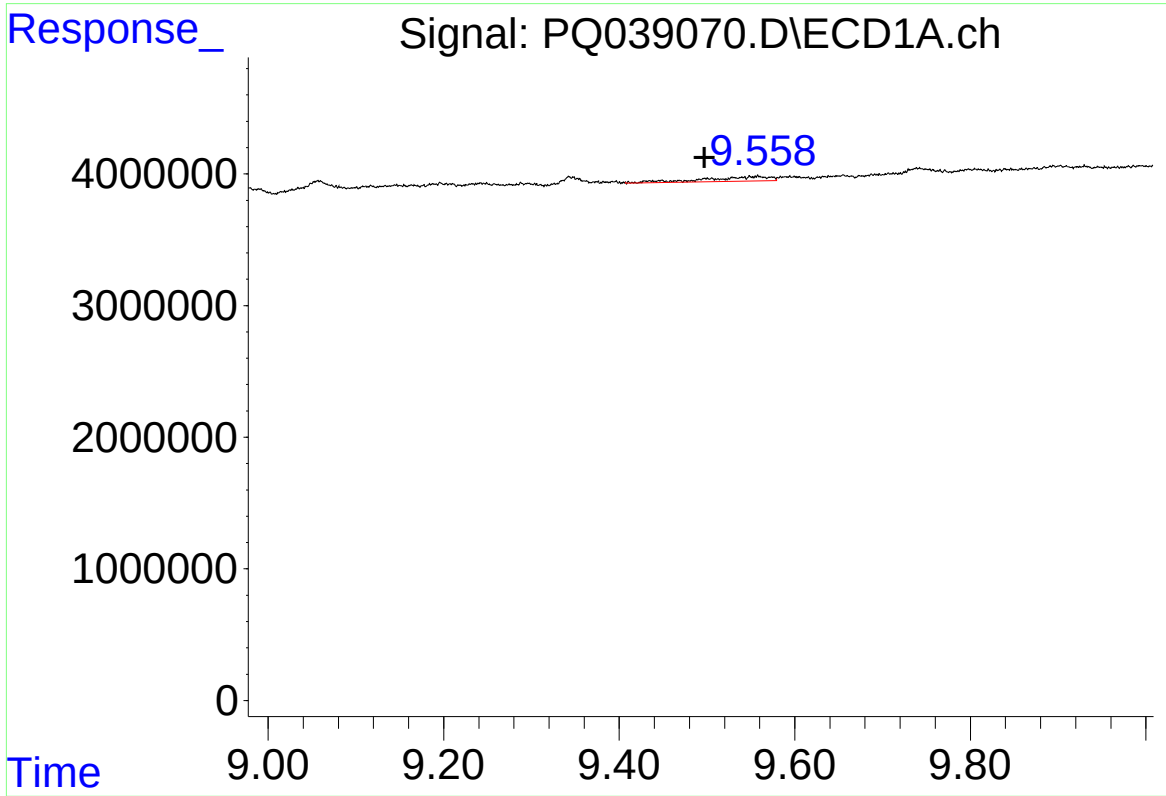

#30 AR-1254-5

```
     R.T.:    9.558 min
Delta R.T.:    0.061 min
  Response:   1702457
     Conc:   6.56 ng/ml
```

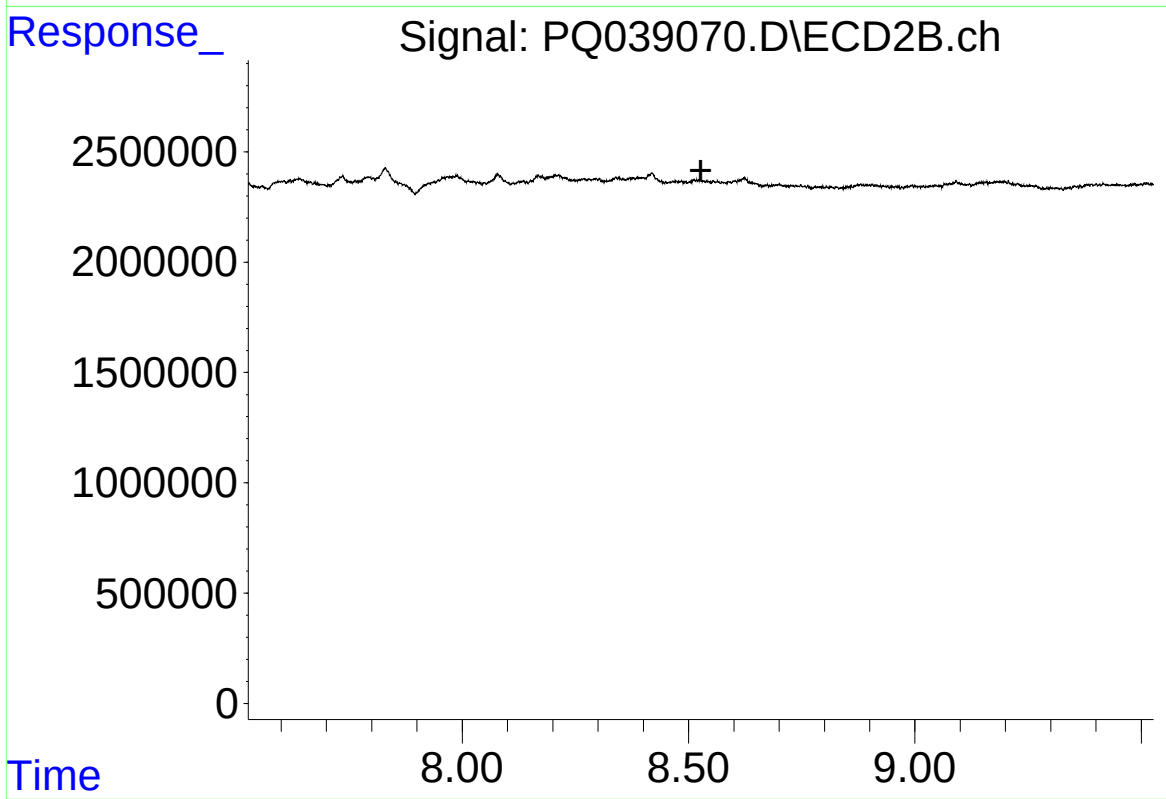

#30 AR-1254-5

```
     R.T.:    0.000 min
Exp R.T.  :    8.527 min
  Response:         0
     Conc:   N.D.
```

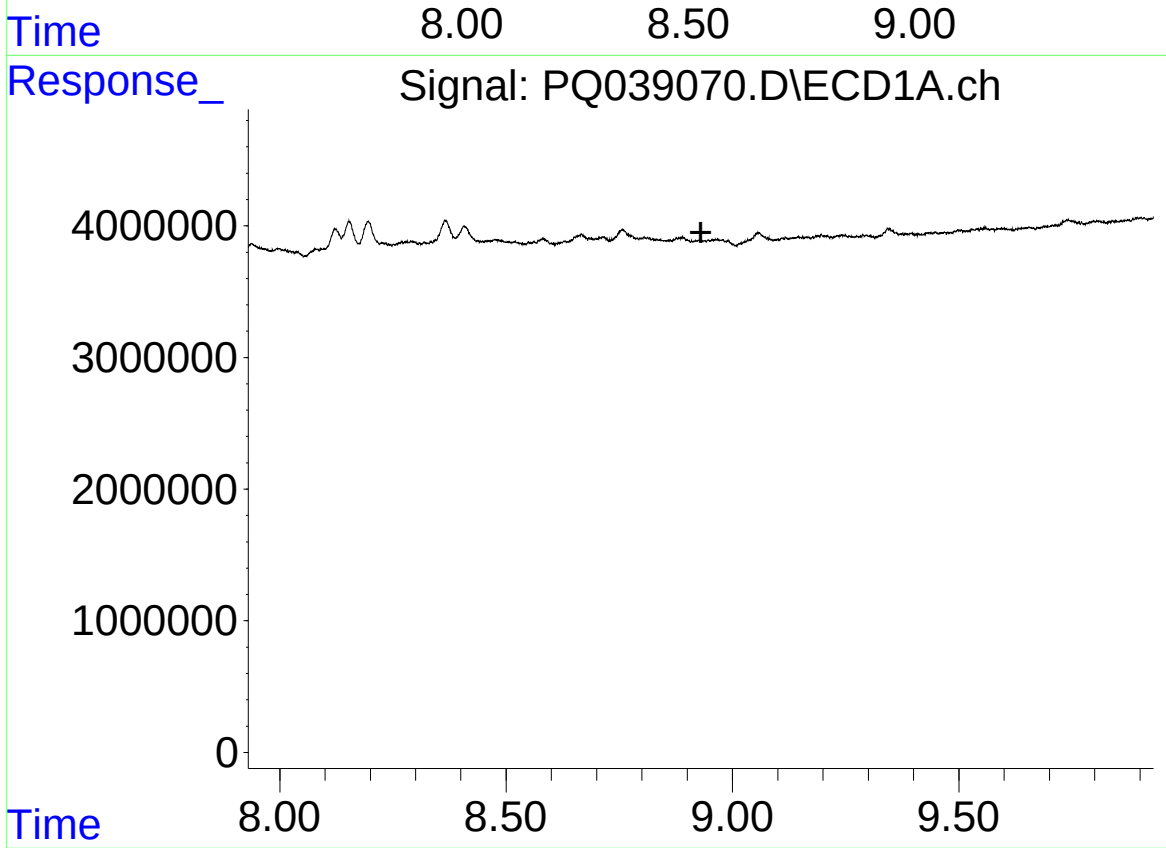

#31 AR-1260-1

```
     R.T.:    0.000 min
Exp R.T.  :    8.930 min
  Response:         0
     Conc:   N.D.
```

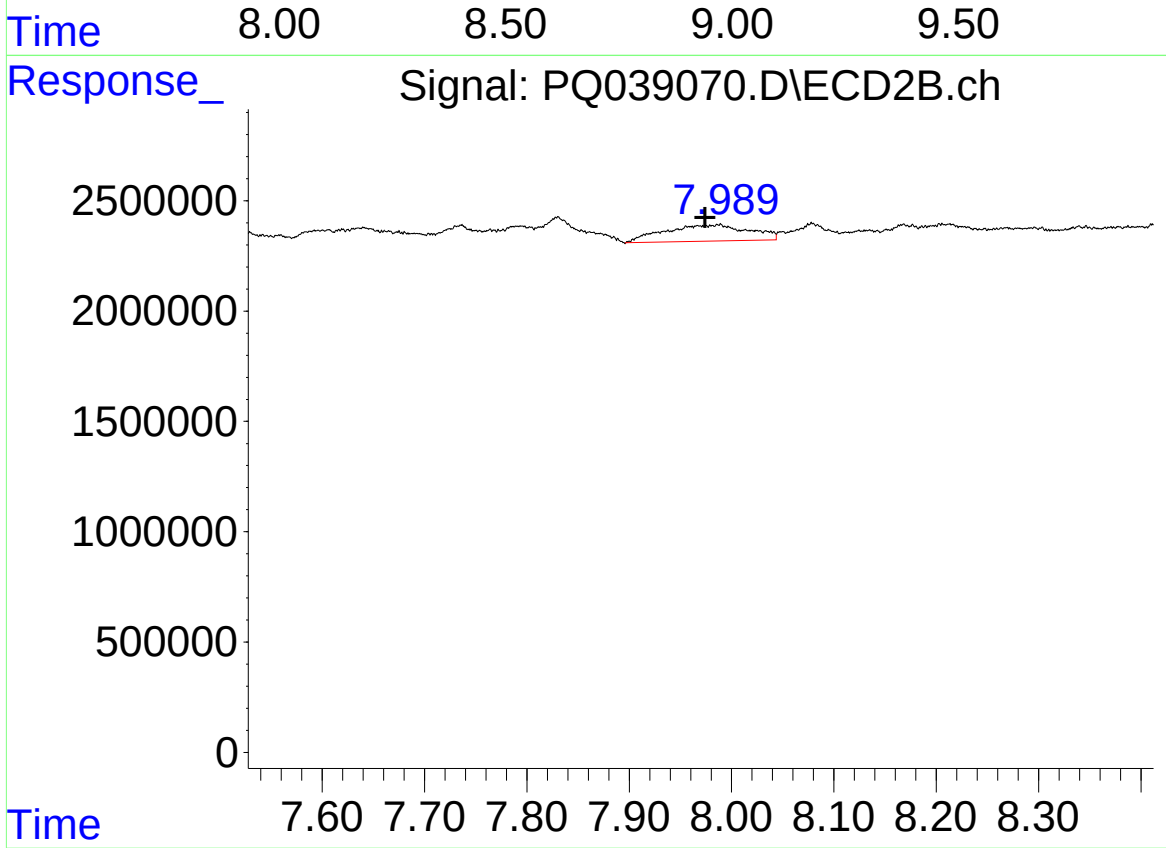

#31 AR-1260-1

```
     R.T.:    7.988 min
Delta R.T.:    0.013 min
  Response:   4296317
     Conc:  23.31 ng/ml
```

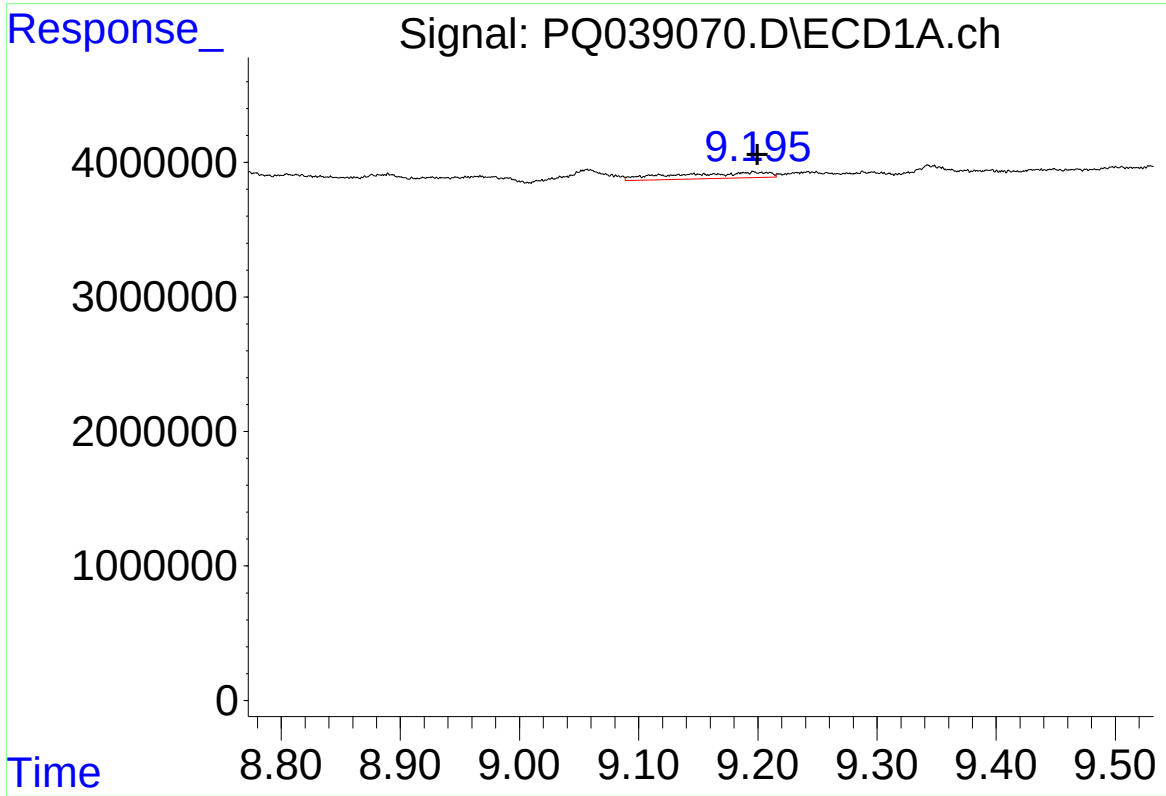

#32 AR-1260-2

R.T.: 9.197 min
Delta R.T.: -0.003 min
Response: 2450997
Conc: 7.33 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

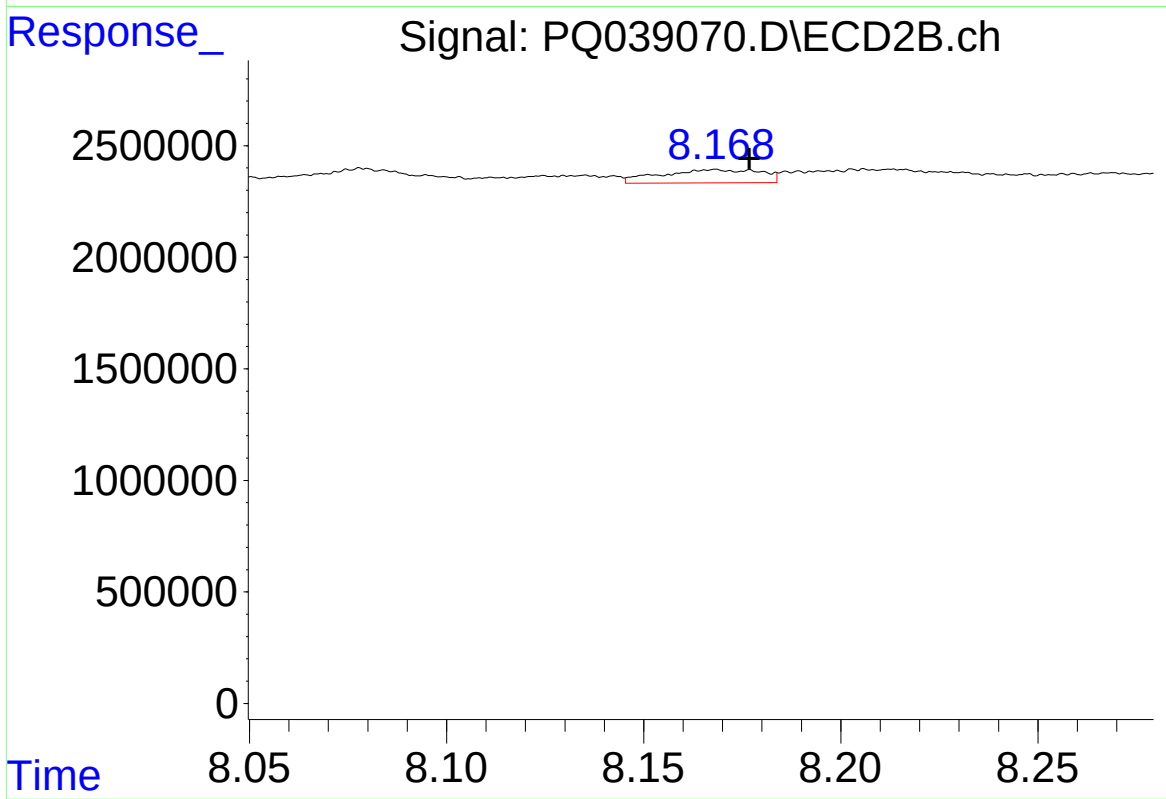

#32 AR-1260-2

R.T.: 8.168 min
Delta R.T.: -0.009 min
Response: 1049012
Conc: 4.76 ng/ml

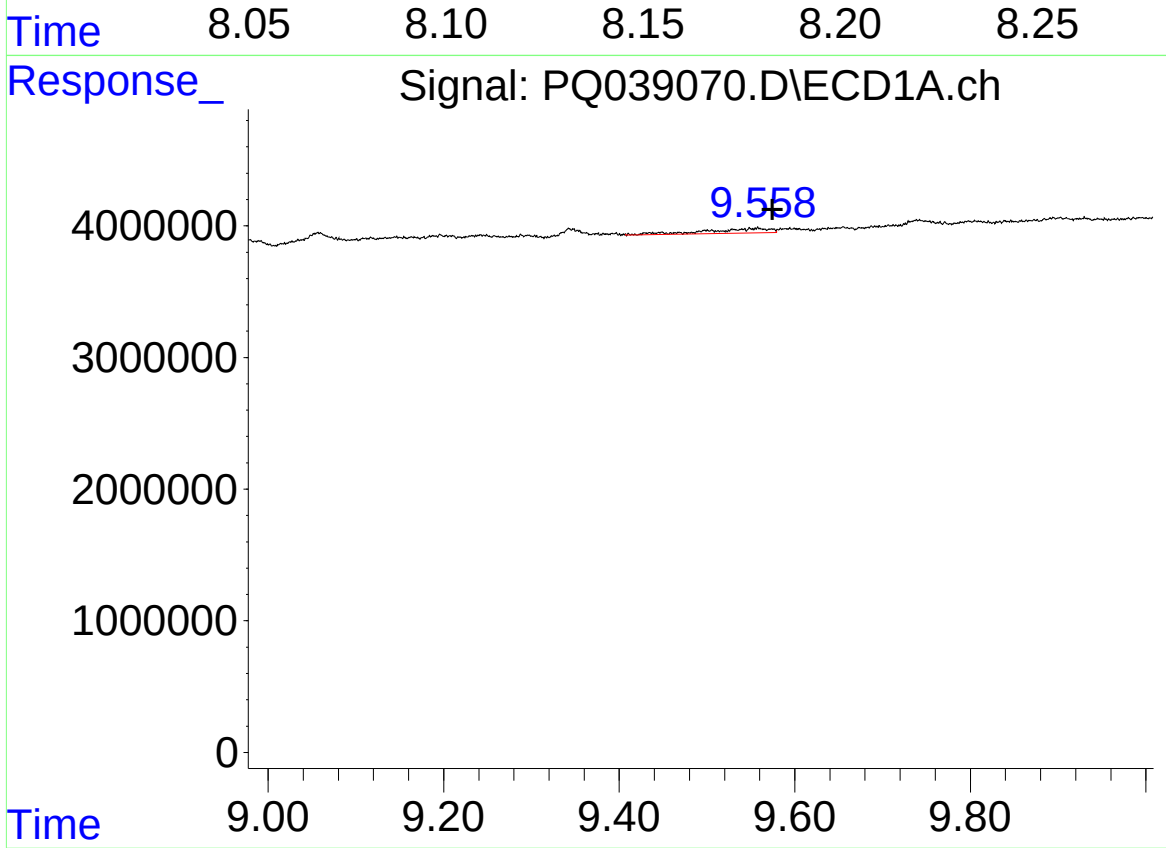

#33 AR-1260-3

R.T.: 9.558 min
Delta R.T.: -0.017 min
Response: 1702457
Conc: 6.18 ng/ml

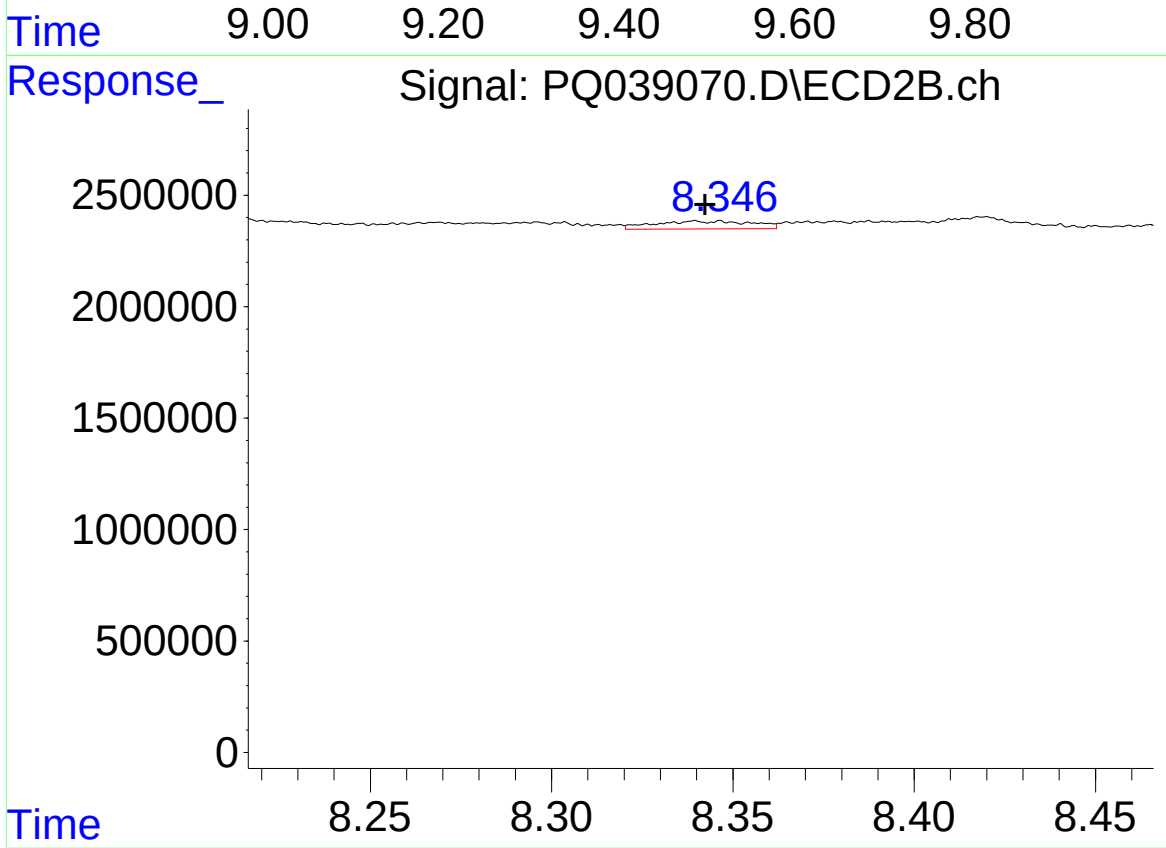

#33 AR-1260-3

R.T.: 8.341 min
Delta R.T.: -0.002 min
Response: 679541
Conc: 3.34 ng/ml

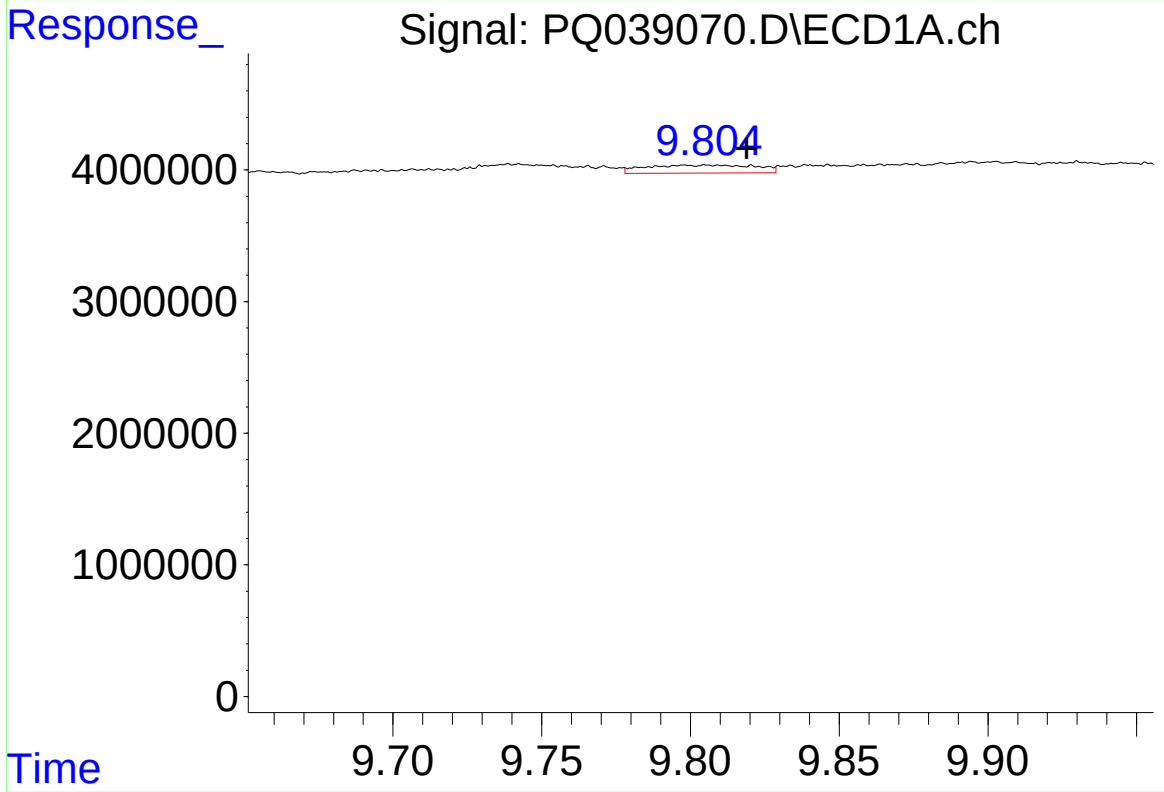

#34 AR-1260-4

R.T.: 9.800 min
Delta R.T.: -0.019 min
Response: 1572866
Conc: 4.81 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

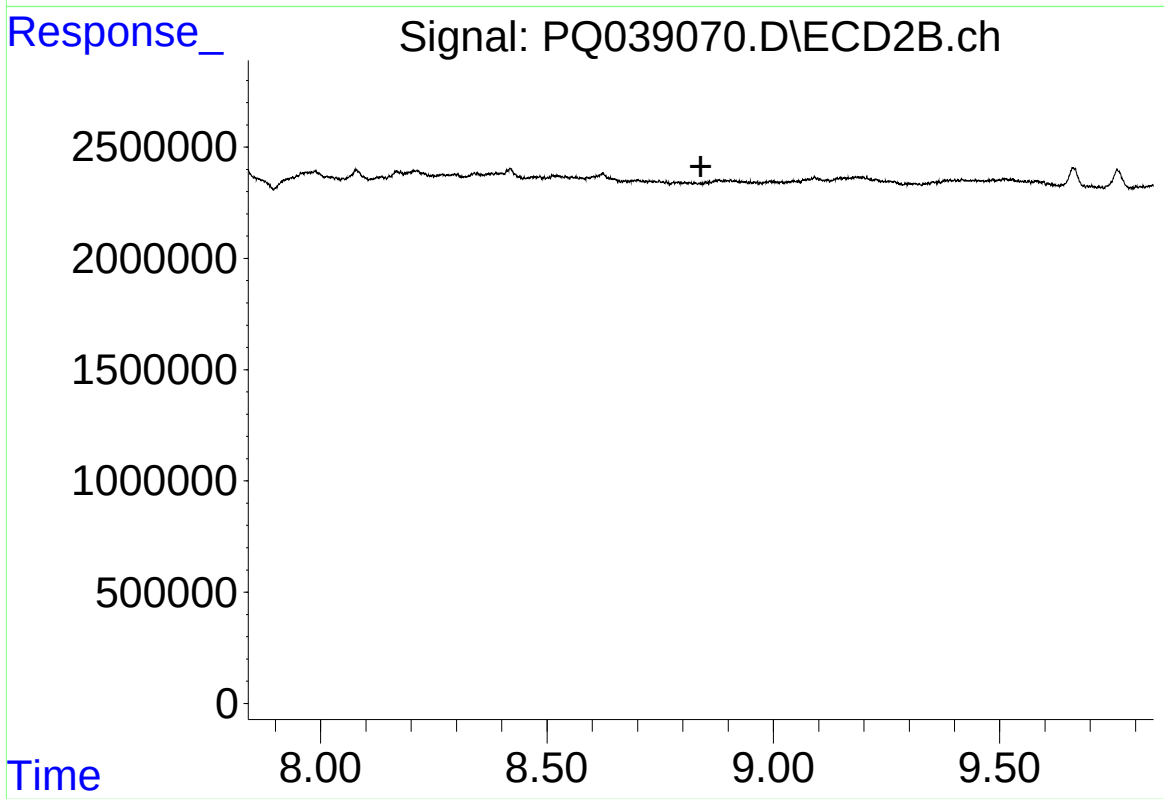

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 8.840 min
Response: 0
Conc: N.D.

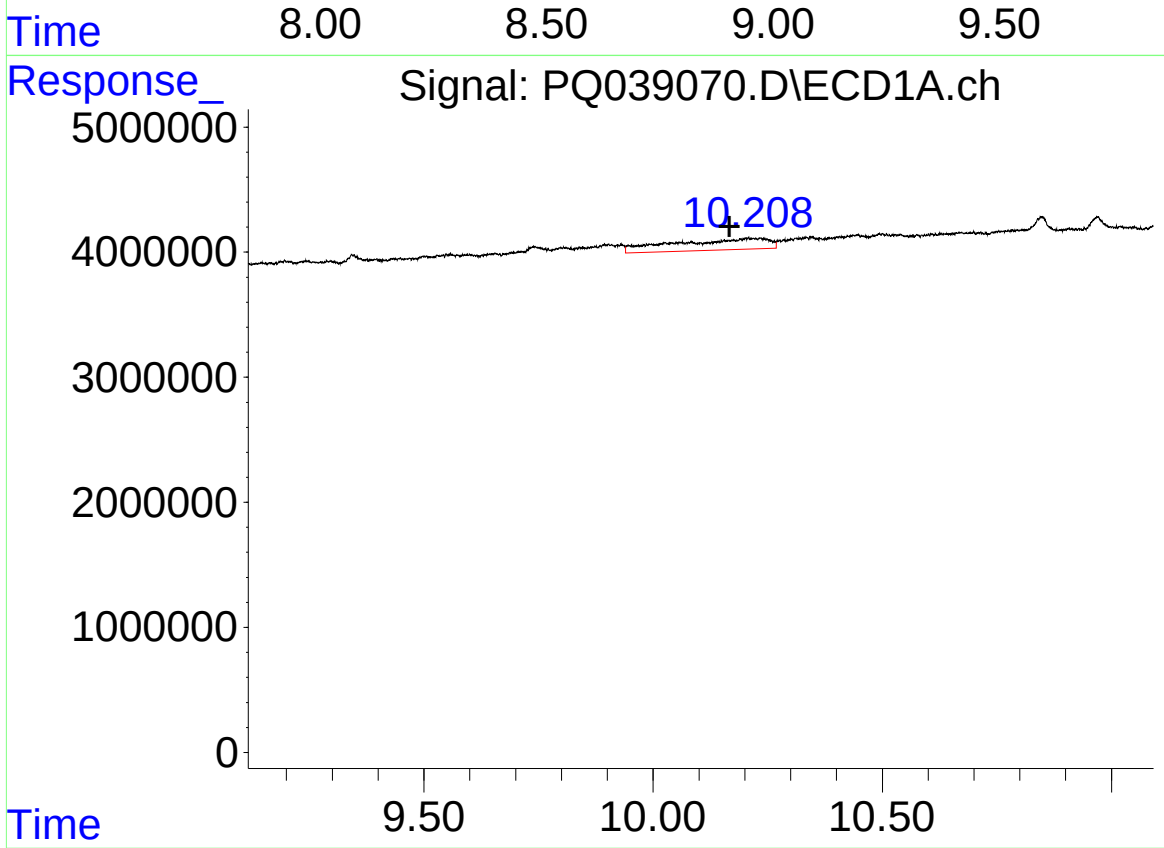

#35 AR-1260-5

R.T.: 10.207 min
Delta R.T.: 0.040 min
Response: 13258603
Conc: 19.93 ng/ml

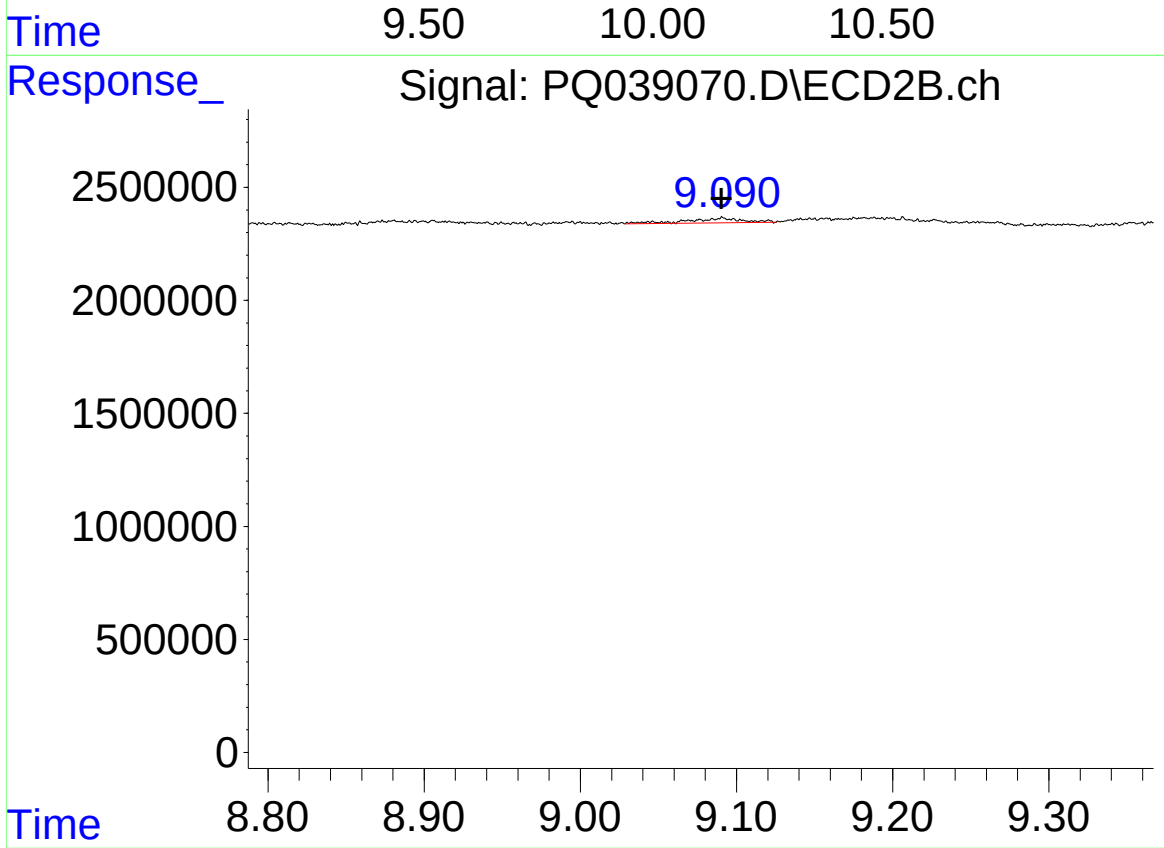

#35 AR-1260-5

R.T.: 9.091 min
Delta R.T.: 0.000 min
Response: 508948
Conc: 1.14 ng/ml

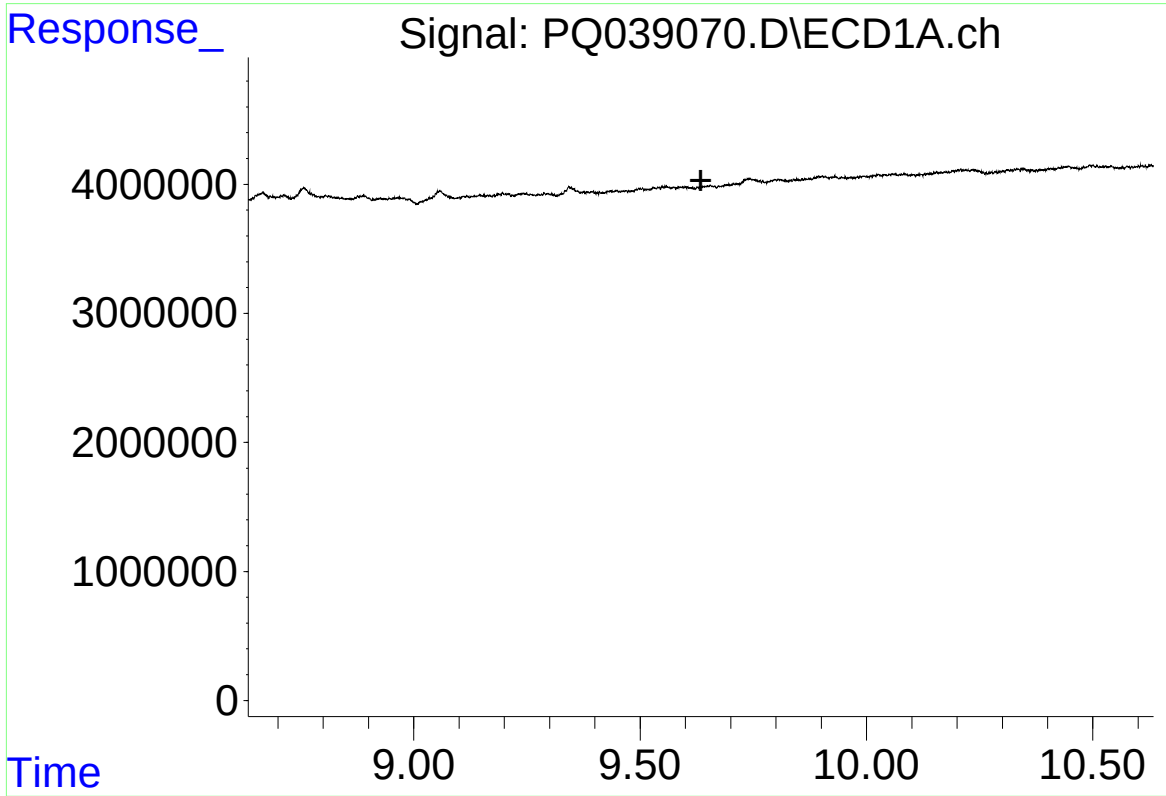

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 9.634 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

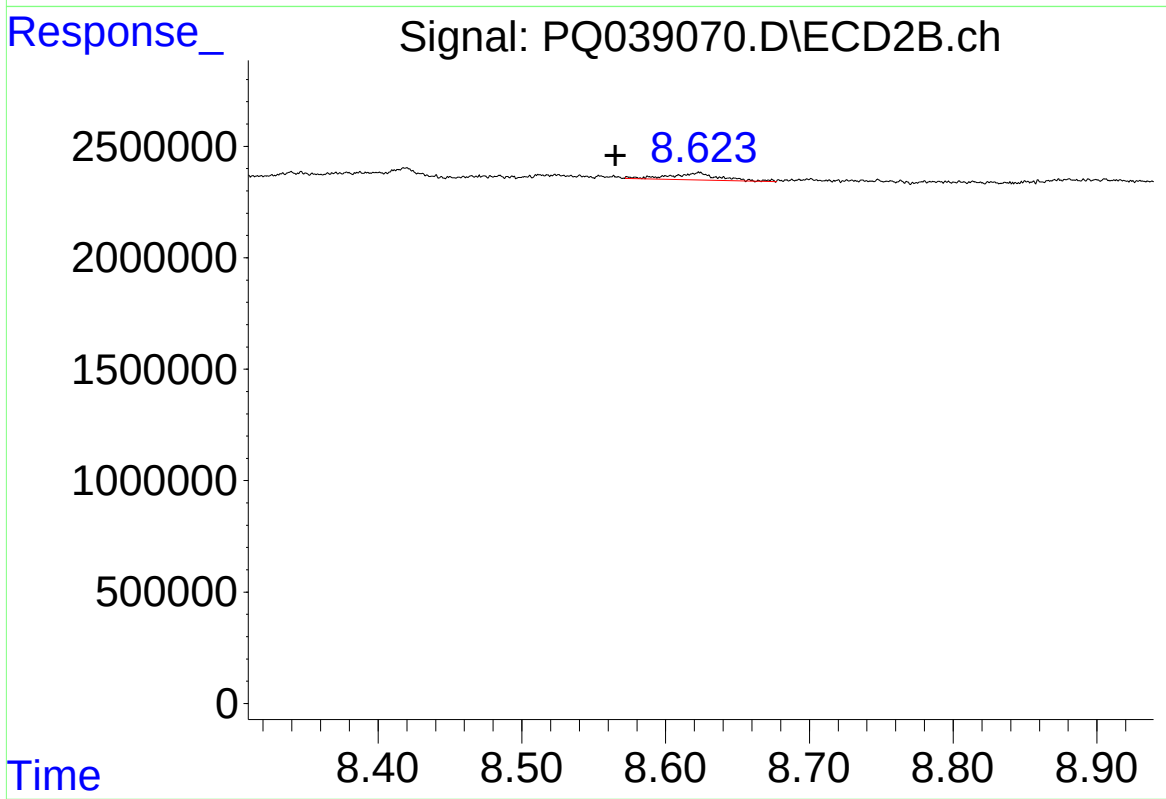

#36 AR-1262-1

R.T.: 8.623 min
Delta R.T.: 0.058 min
Response: 718795
Conc: 3.23 ng/ml

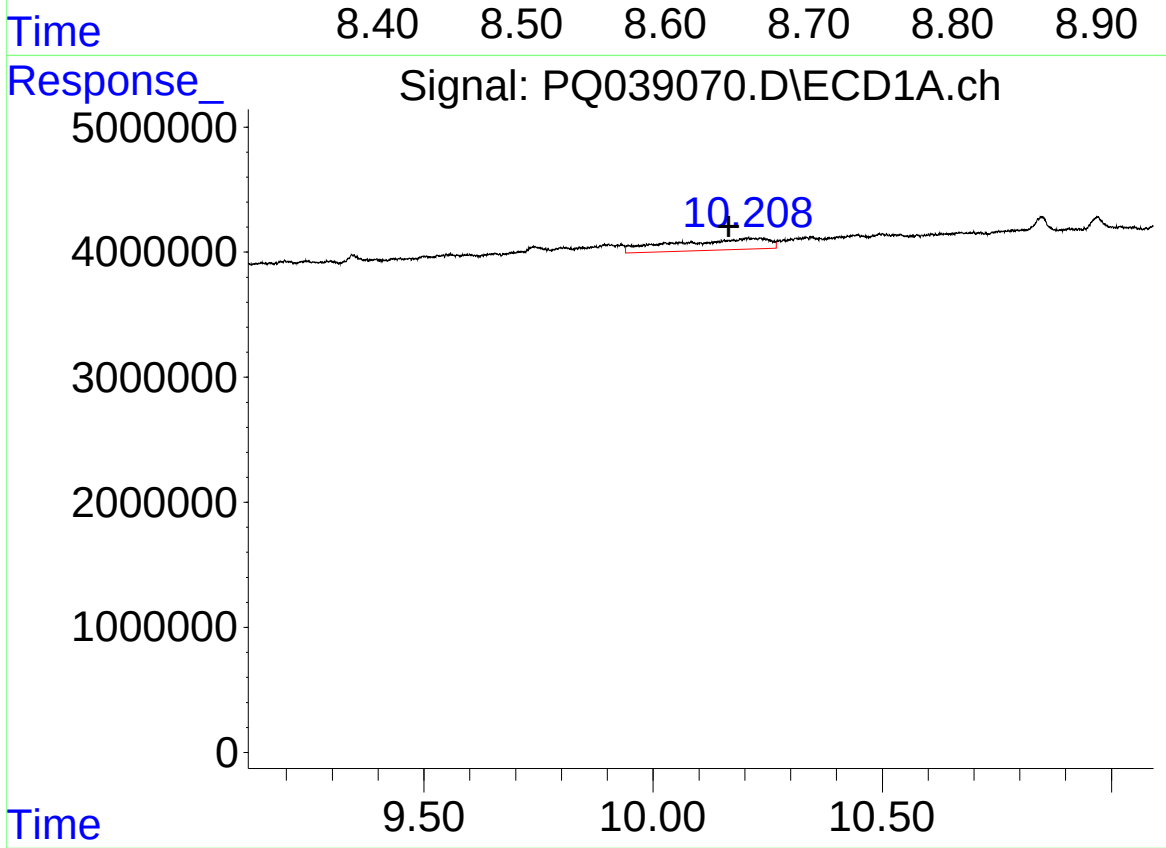

#37 AR-1262-2

R.T.: 10.207 min
Delta R.T.: 0.042 min
Response: 13258603
Conc: 20.91 ng/ml

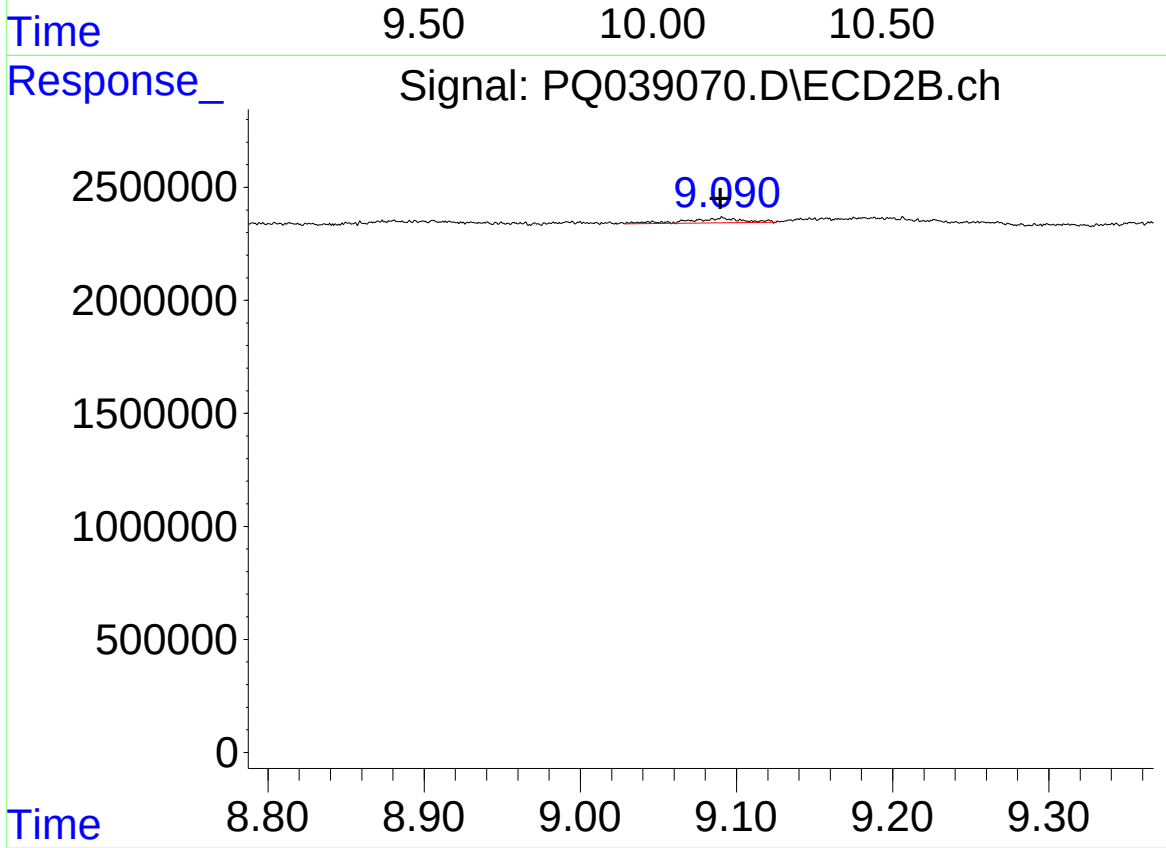

#37 AR-1262-2

R.T.: 9.091 min
Delta R.T.: 0.000 min
Response: 508948
Conc: 1.18 ng/ml

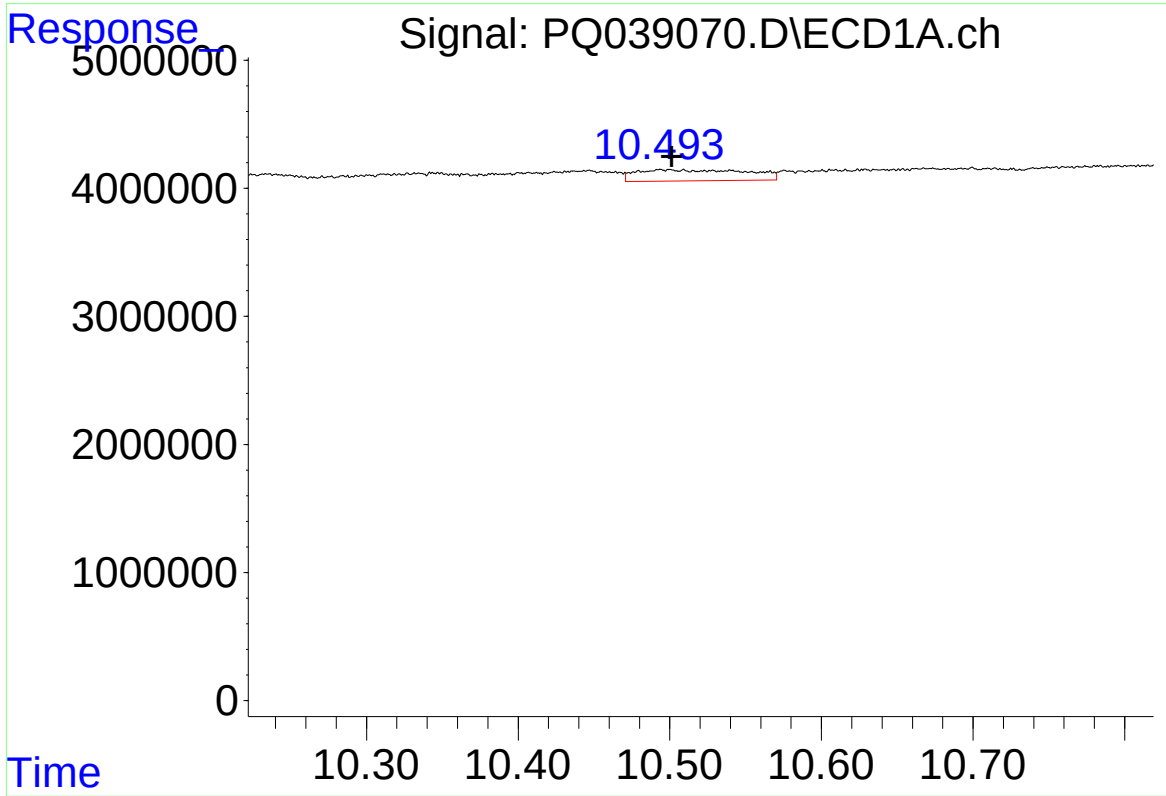

#38 AR-1262-3

R.T.: 10.496 min
Delta R.T.: -0.006 min
Response: 4400037
Conc: 9.94 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

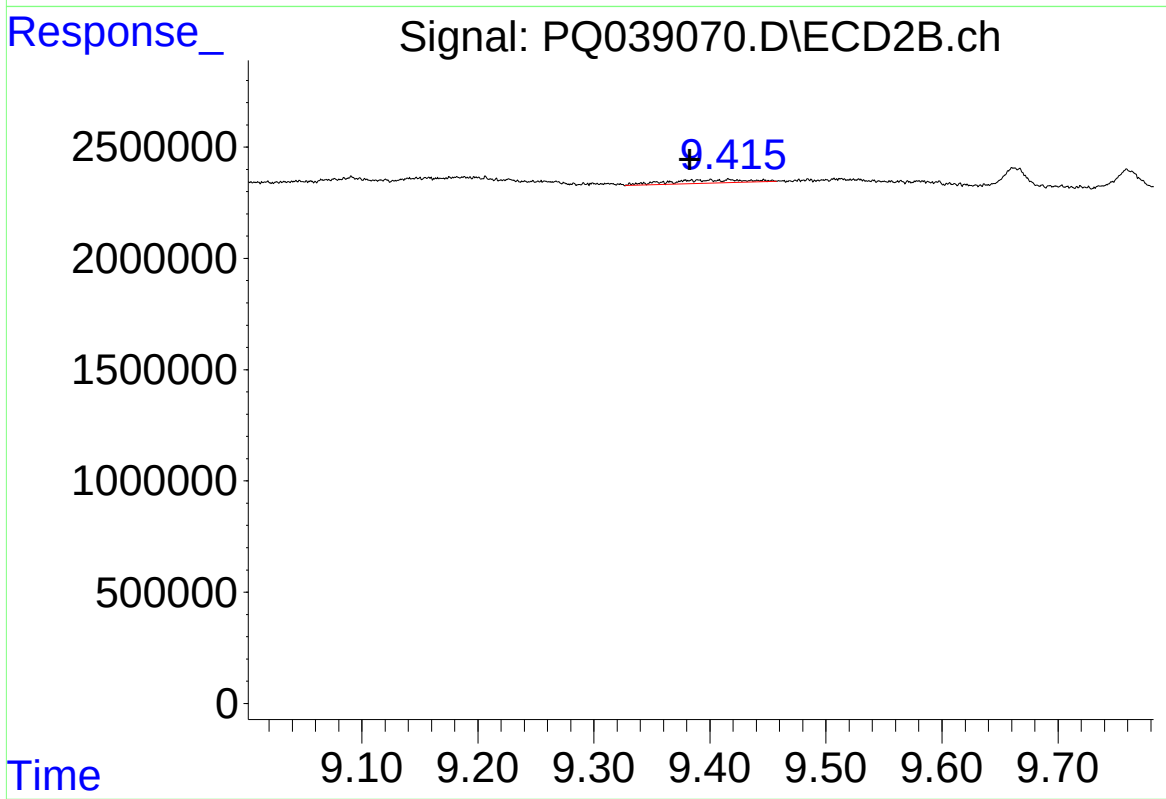

#38 AR-1262-3

R.T.: 9.401 min
Delta R.T.: 0.018 min
Response: 693709
Conc: 4.12 ng/ml

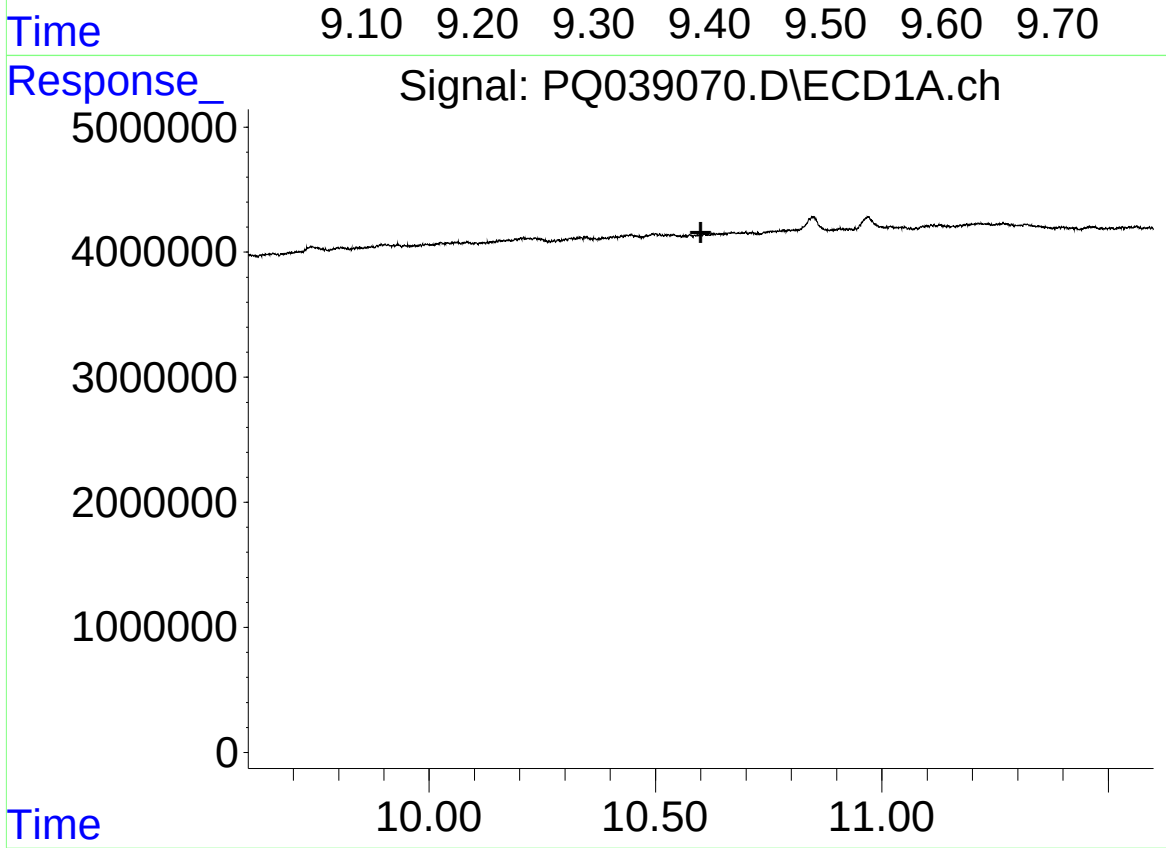

#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 10.600 min
Response: 0
Conc: N.D.

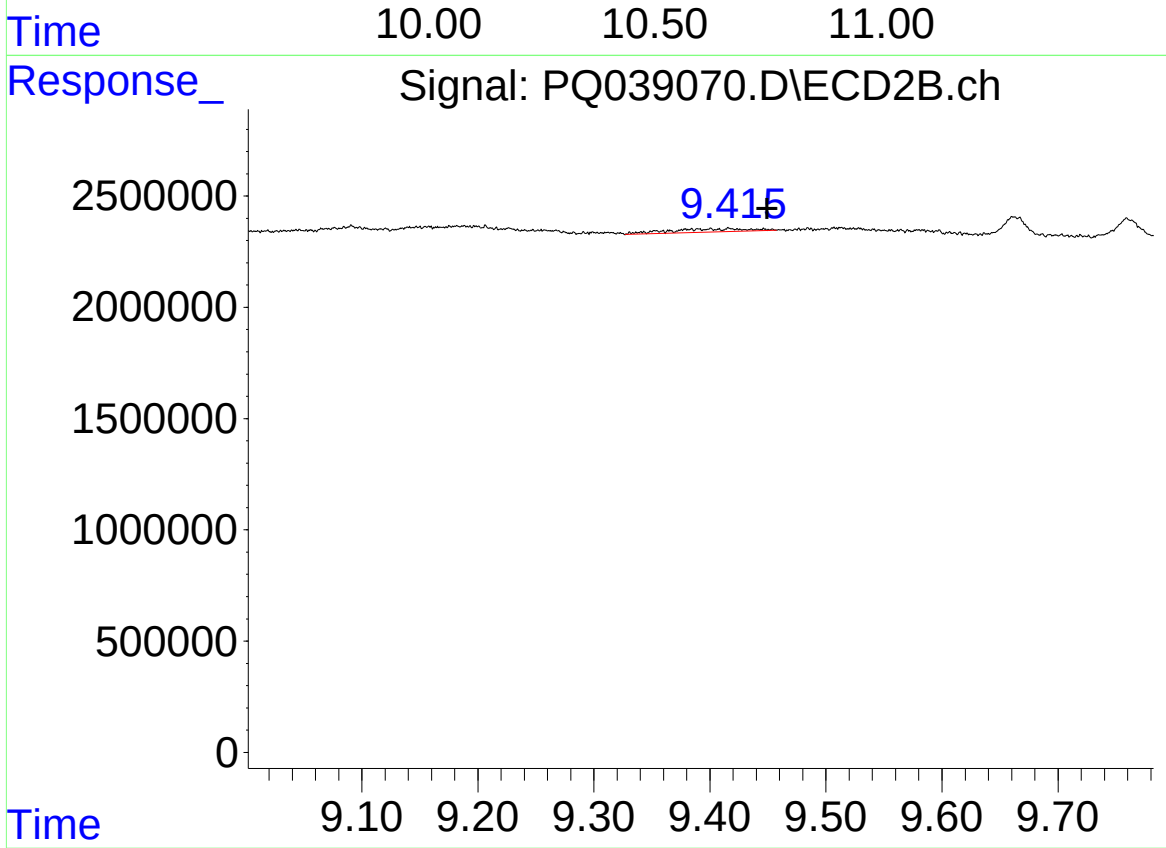

#39 AR-1262-4

R.T.: 9.401 min
Delta R.T.: -0.049 min
Response: 693709
Conc: 2.07 ng/ml

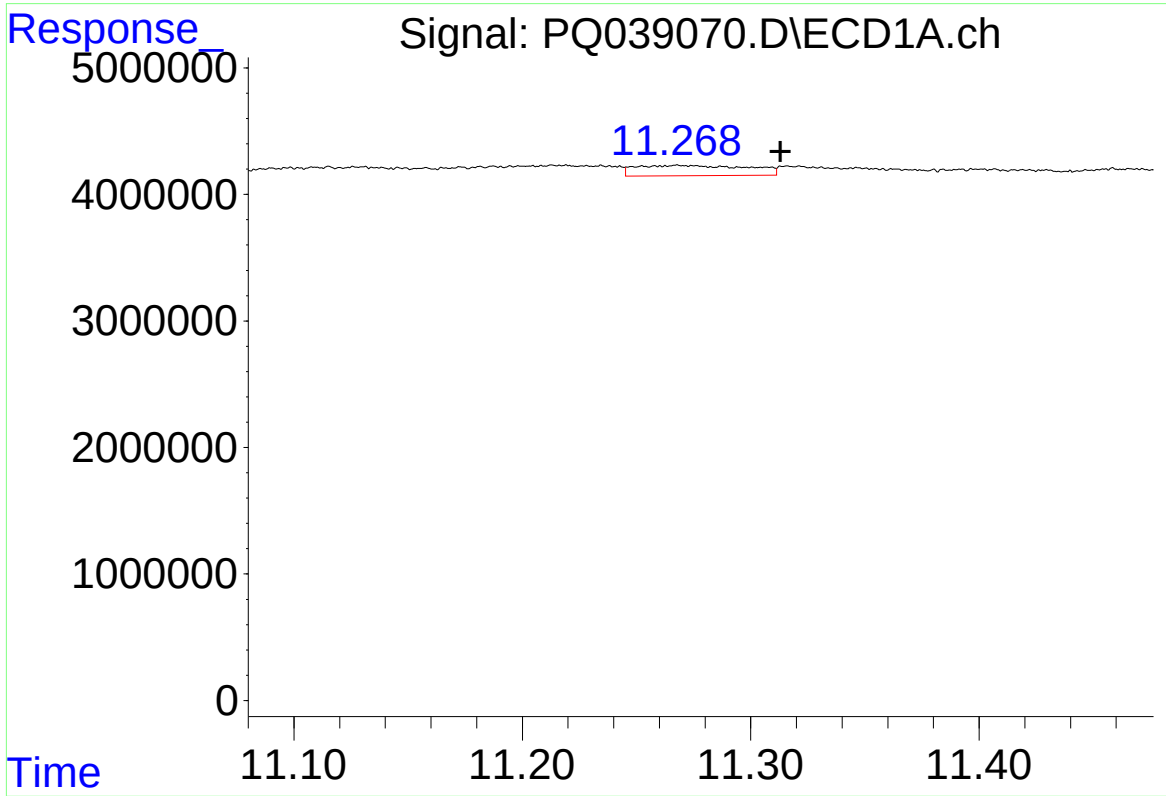

#40 AR-1262-5

R.T.: 11.269 min
Delta R.T.: -0.044 min
Response: 2829704
Conc: 11.19 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

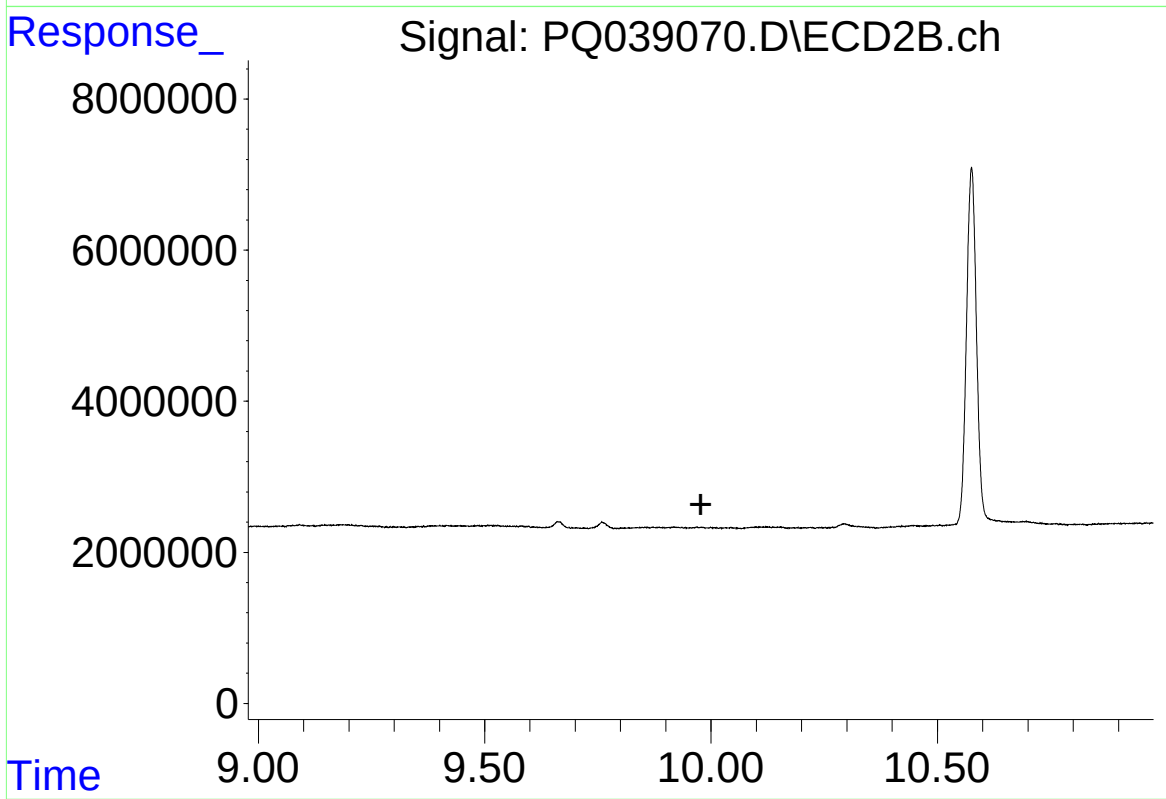

#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.977 min
Response: 0
Conc: N.D.

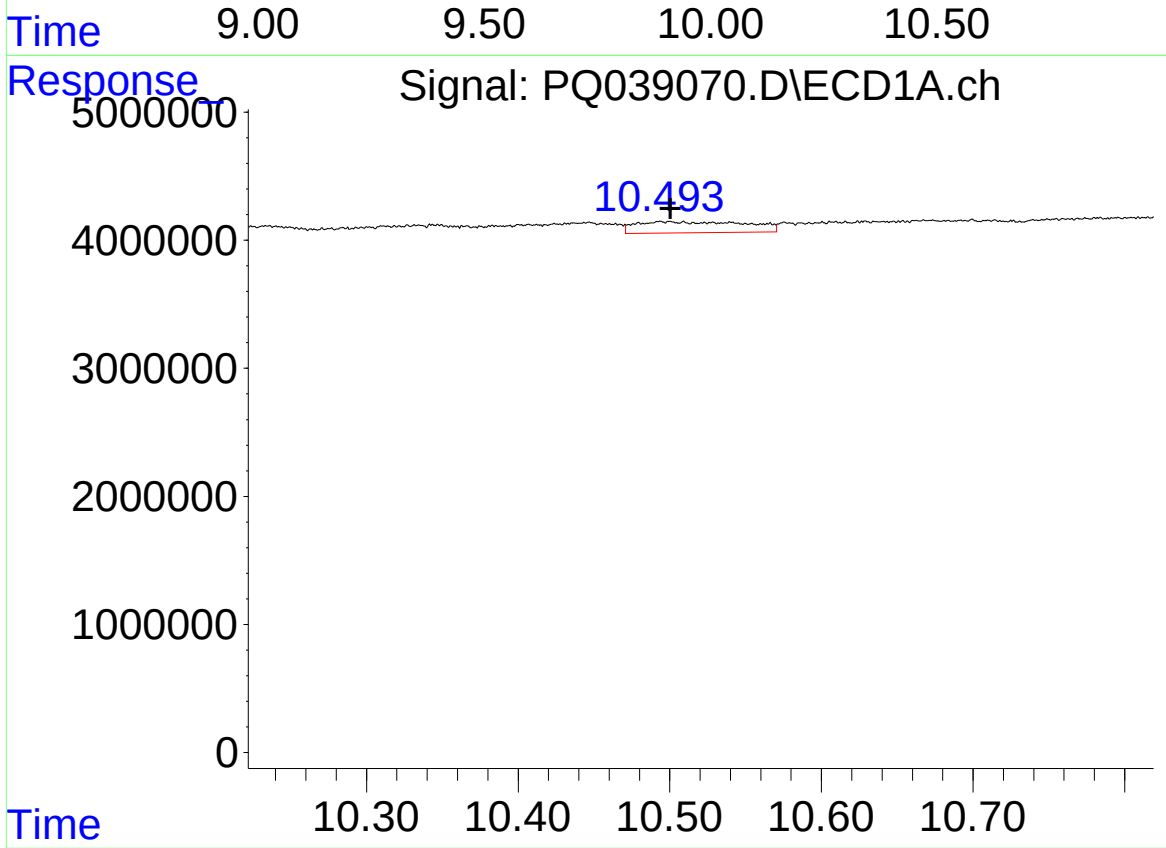

#41 AR-1268-1

R.T.: 10.496 min
Delta R.T.: -0.005 min
Response: 4400037
Conc: 5.44 ng/ml

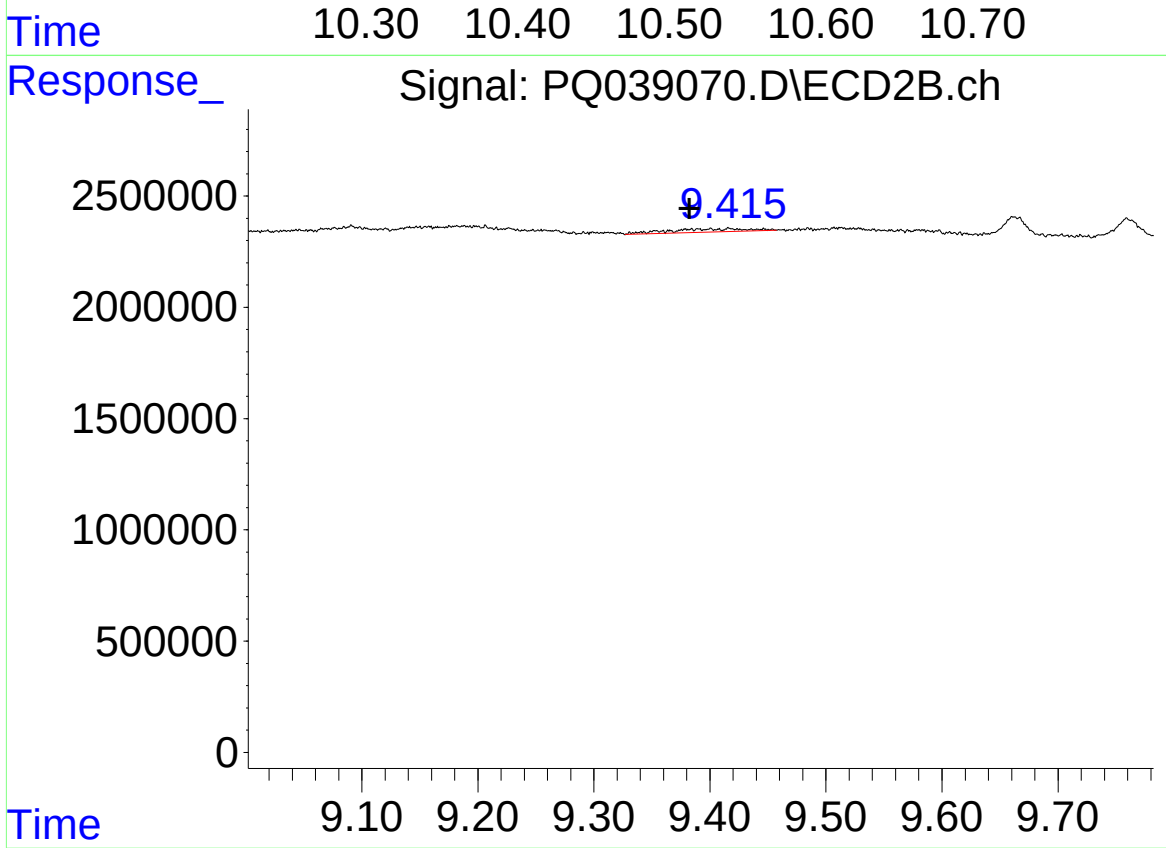

#41 AR-1268-1

R.T.: 9.401 min
Delta R.T.: 0.018 min
Response: 693709
Conc: 1.34 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

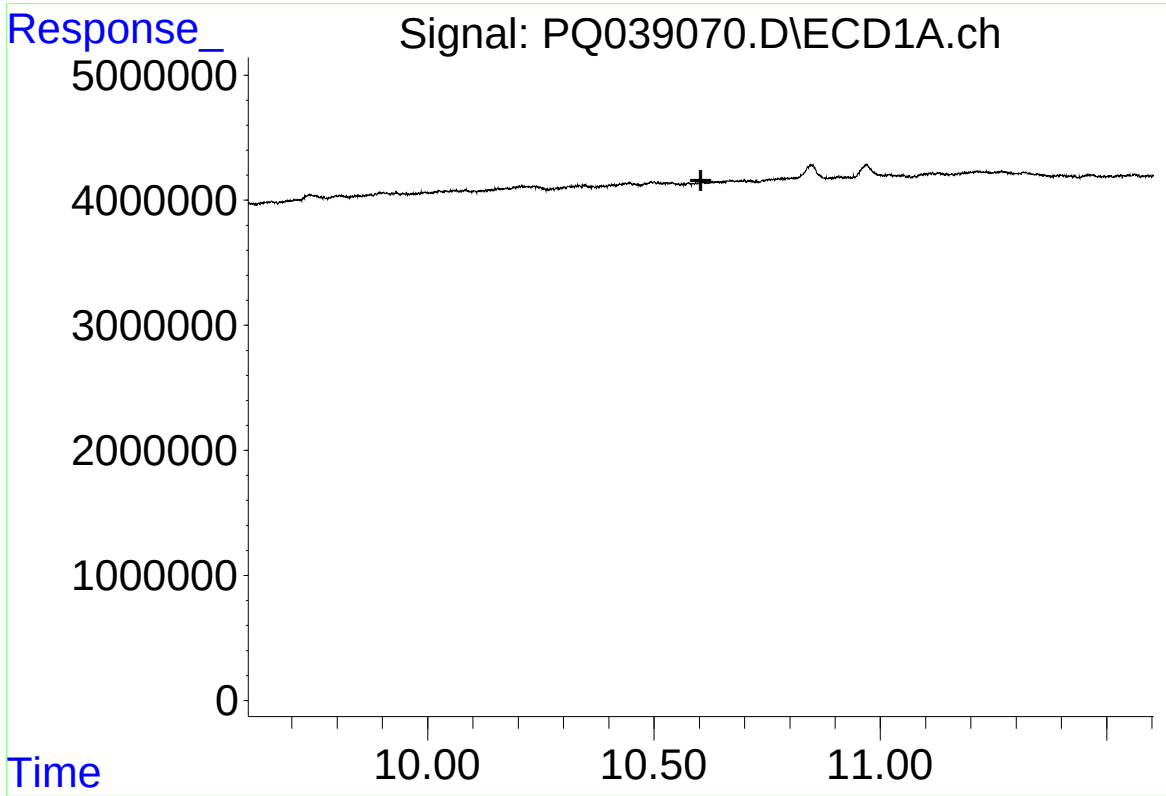

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 10.604 min
Response: 0
Conc: N.D.

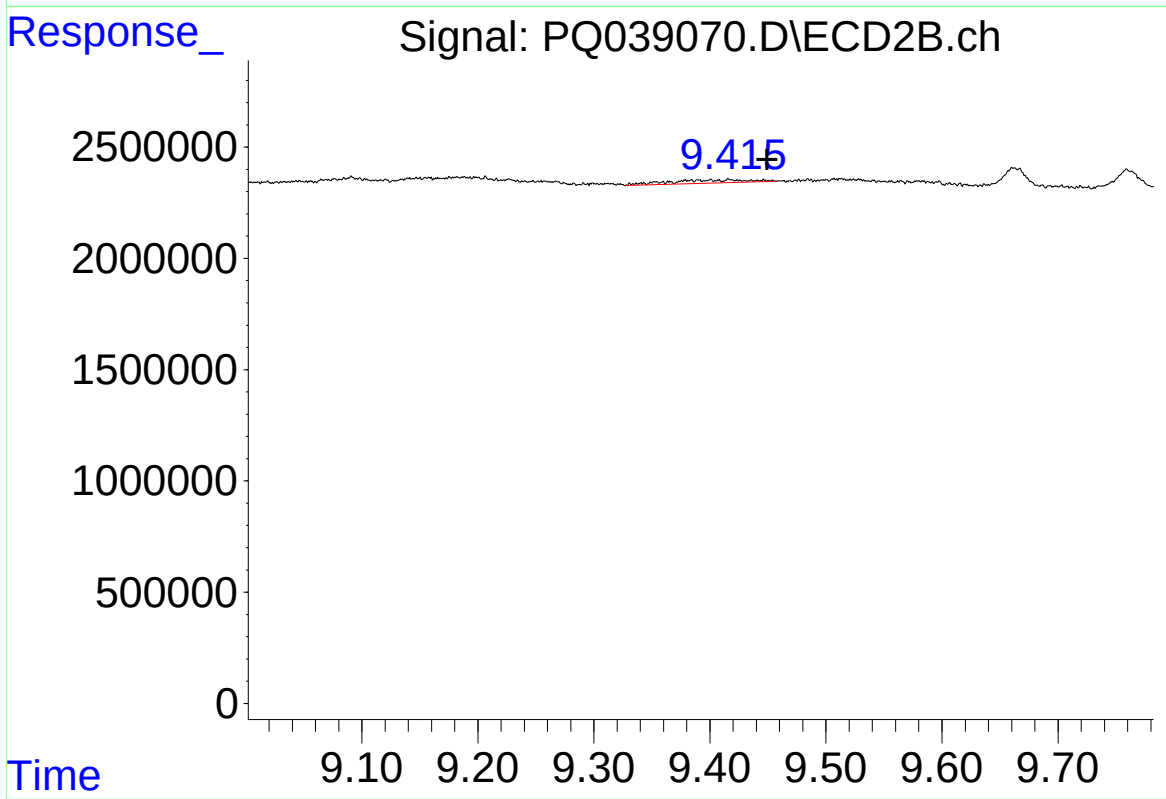

#42 AR-1268-2

R.T.: 9.401 min
Delta R.T.: -0.049 min
Response: 693709
Conc: 1.41 ng/ml

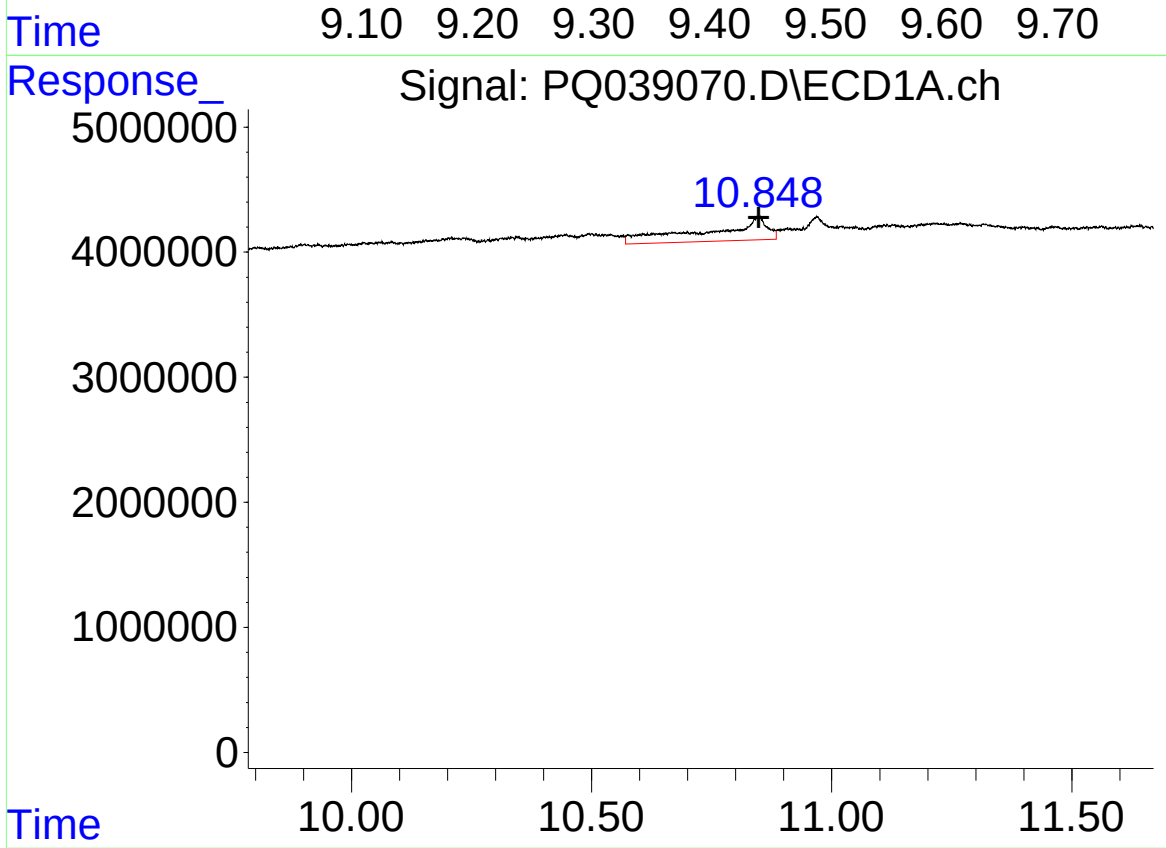

#43 AR-1268-3

R.T.: 10.848 min
Delta R.T.: 0.000 min
Response: 15640321
Conc: 23.72 ng/ml

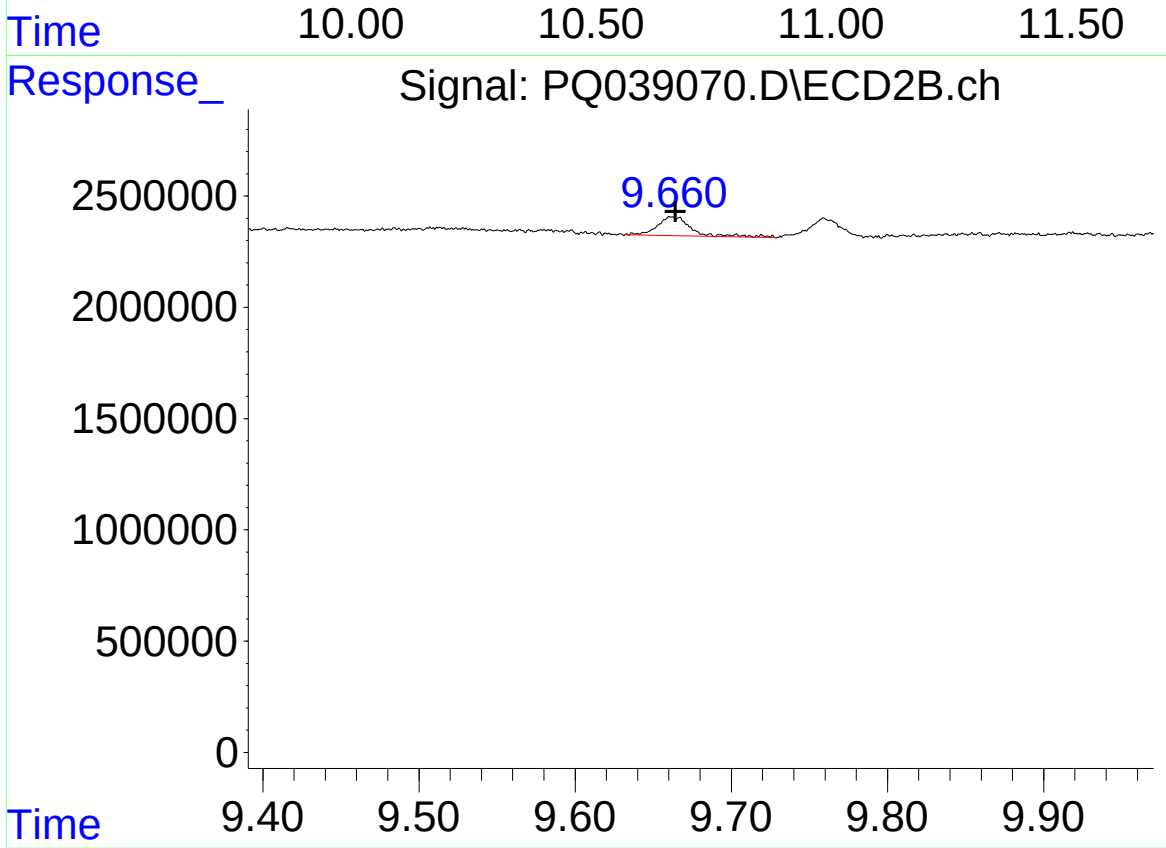

#43 AR-1268-3

R.T.: 9.663 min
Delta R.T.: -0.001 min
Response: 1319228
Conc: 3.31 ng/ml

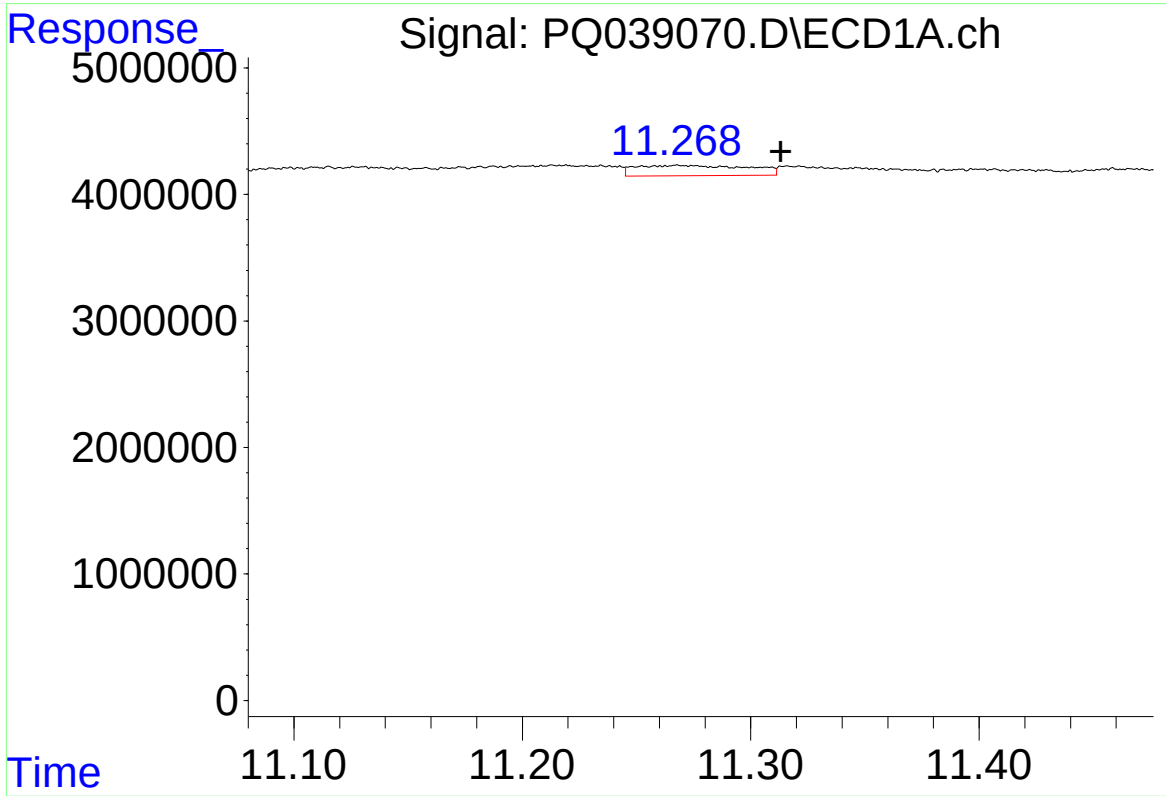

#44 AR-1268-4

R.T.:	11.269 min
Delta R.T.:	-0.044 min
Response:	2829704
Conc:	10.11 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

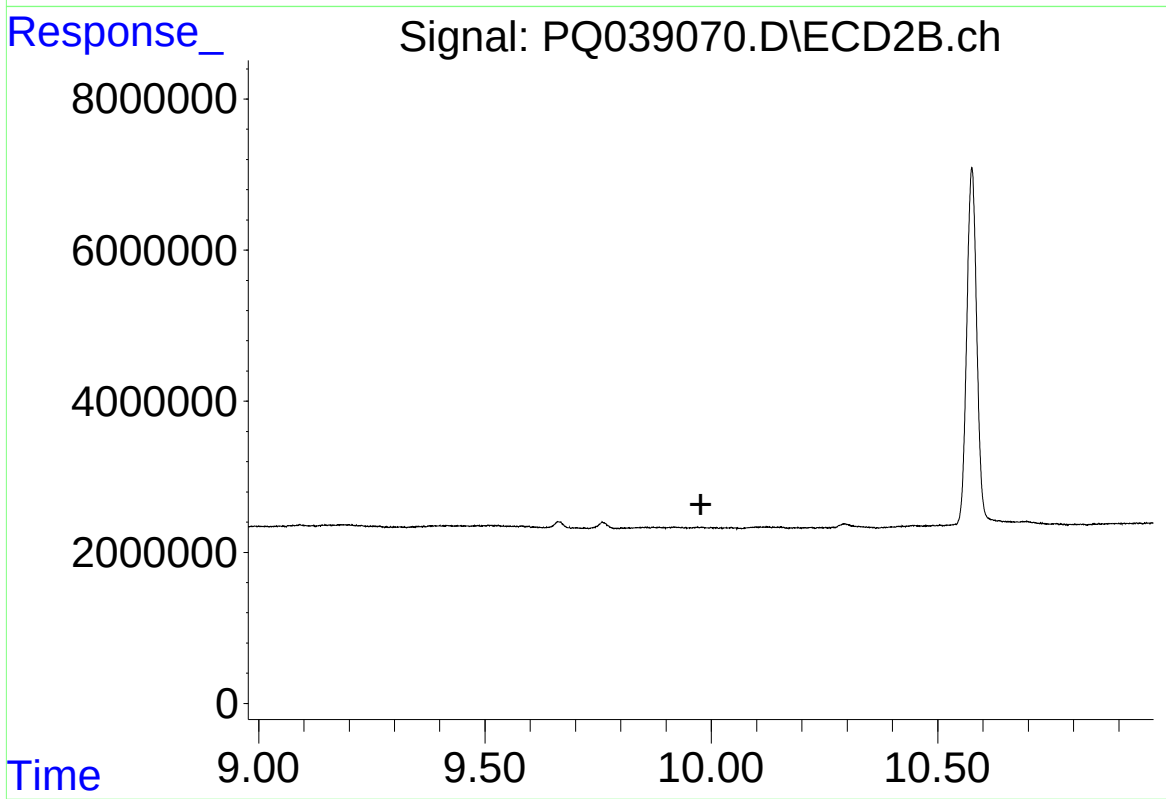

#44 AR-1268-4

R.T.:	0.000 min
Exp R.T. :	9.977 min
Response:	0
Conc:	N.D.

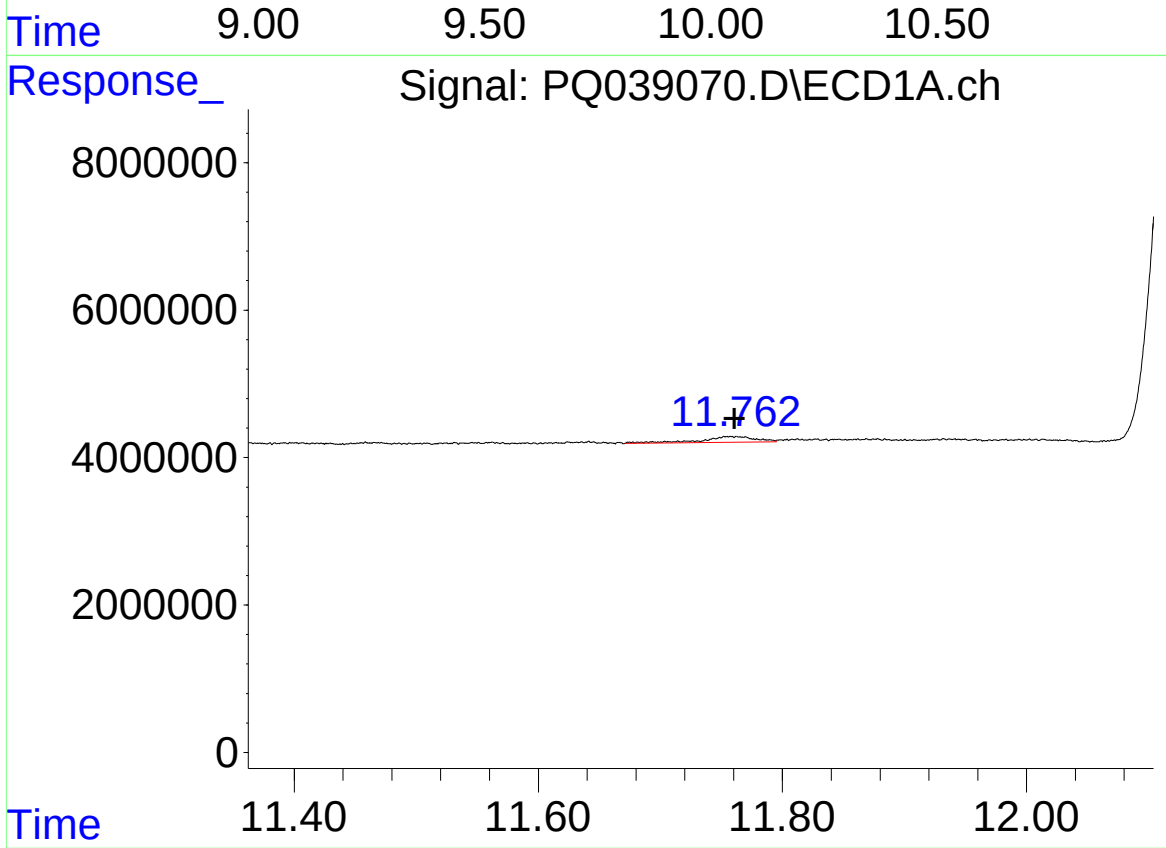

#45 AR-1268-5

R.T.:	11.758 min
Delta R.T.:	-0.002 min
Response:	2338726
Conc:	1.03 ng/ml

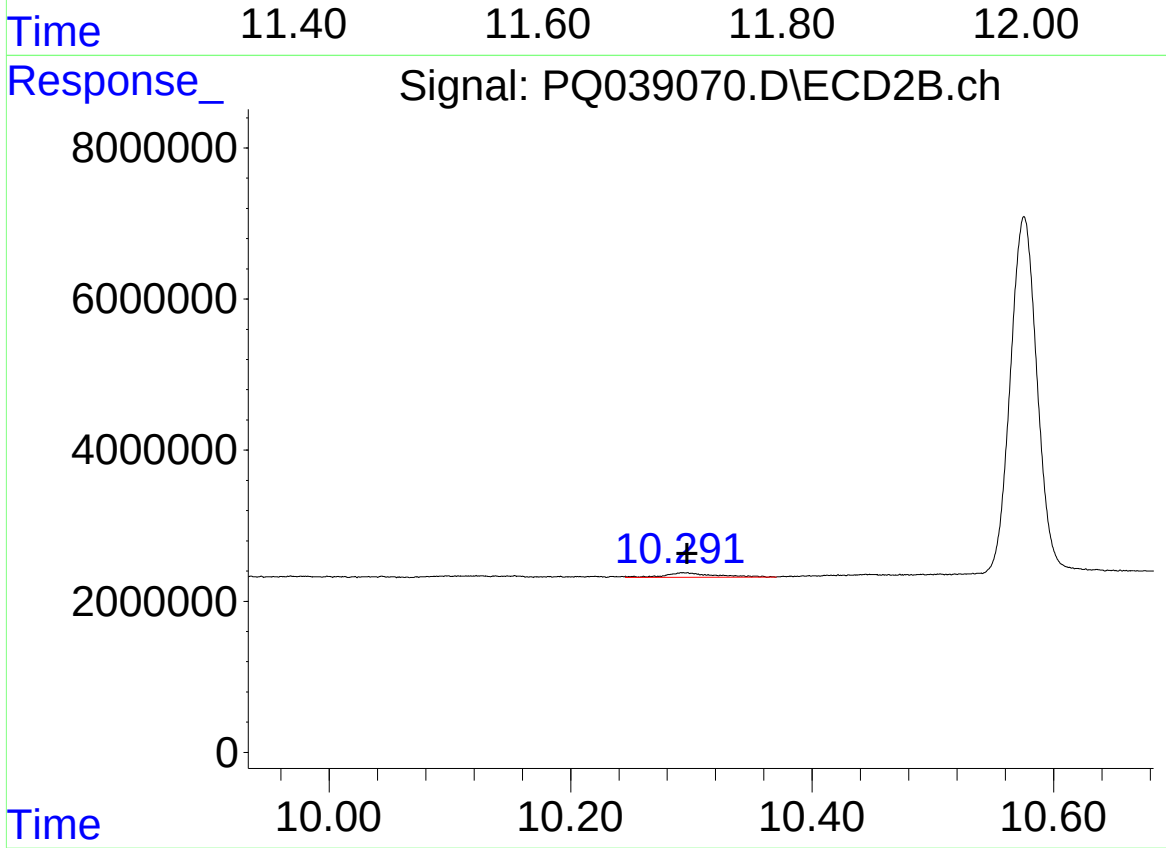

#45 AR-1268-5

R.T.:	10.294 min
Delta R.T.:	-0.002 min
Response:	1601840
Conc:	1.26 ng/ml