

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ041219\
 Data File : PQ039072.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2019 18:11
 Operator : AJ\SJ
 Sample : K1560-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 00:59:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ041219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Apr 13 00:36:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.719	4.815	84793498	45148214	19.133	20.247
2)	SA Decachlor...	12.122	10.574	168.4E6	85841401	24.277	24.602
Target Compounds							
3)	L1 AR-1016-1	0.000	6.270	0	1828073	N.D.	18.002 #
4)	L1 AR-1016-2	0.000	6.270	0	1828073	N.D.	12.342 #
5)	L1 AR-1016-3	0.000	6.557	0	1494382	N.D.	20.029 #
6)	L1 AR-1016-4	0.000	6.557	0	1494382	N.D.	23.969 #
7)	L1 AR-1016-5	7.706	6.807	4089632	1496398	28.816	16.863 #
8)	L2 AR-1221-1	0.000	5.054	0	2456067	N.D.	103.381 #
9)	L2 AR-1221-2	6.109	5.234	2379770	741386	70.103	35.554 #
10)	L2 AR-1221-3	0.000	5.344	0	275501	N.D.	4.490 #
11)	L3 AR-1232-1	0.000	5.344	0	275501	N.D.	7.265 #
12)	L3 AR-1232-2	0.000	6.270	0	1828073	N.D.	39.334 #
13)	L3 AR-1232-3	0.000	6.557	0	1494382	N.D.	70.455 #
14)	L3 AR-1232-4	0.000	6.604	0	365395	N.D.	17.356 #
15)	L3 AR-1232-5	7.477	6.807	3171157	1496398	77.044	61.396
16)	L4 AR-1242-1	0.000	6.270	0	1828073	N.D.	31.143 #
17)	L4 AR-1242-2	0.000	6.270	0	1828073	N.D.	21.270 #
18)	L4 AR-1242-3	0.000	6.557	0	1494382	N.D.	35.394 #
19)	L4 AR-1242-4	0.000	6.604	0	365395	N.D.	8.159 #
20)	L4 AR-1242-5	8.196	7.217	4238002	5807948	42.897	89.565 #
21)	L5 AR-1248-1	0.000	6.270	0	1828073	N.D.	41.021 #
22)	L5 AR-1248-2	7.477	6.557	3171157	1494382	27.756	25.029
23)	L5 AR-1248-3	7.706	6.604	4089632	365395	29.832	5.708 #
24)	L5 AR-1248-4	8.152	6.807	3839137	1496398	24.599	18.186 #
25)	L5 AR-1248-5	8.196	7.264	4238002	1711182	27.708	20.541 #
26)	L6 AR-1254-1	8.123	7.217	7393071	5807948	42.939	40.643
27)	L6 AR-1254-2	8.361	7.384	8978301	5470527	32.793	43.080 #
28)	L6 AR-1254-3	8.754	7.831	10921896	9590995	35.559	42.872
29)	L6 AR-1254-4	9.056	8.079	8877892	6294397	39.968	44.871
30)	L6 AR-1254-5	9.495	8.525	14987628	7497703	57.735	36.342 #
31)	L7 AR-1260-1	8.926	7.972	6479766	8155869	23.180	44.257 #
32)	L7 AR-1260-2	9.196	8.175	6758195	9075257	20.203	41.143 #
33)	L7 AR-1260-3	9.556	8.338	6544774	3583960	23.761	17.589 #
34)	L7 AR-1260-4	9.807	8.879	12532395	1333400	38.350	7.305 #
35)	L7 AR-1260-5	10.162	9.086	2569906	865430	3.864	1.937 #
36)	L8 AR-1262-1	0.000	8.525	0	7497703	N.D.	33.686 #
37)	L8 AR-1262-2	10.162	9.086	2569906	865430	4.053	2.004 #
38)	L8 AR-1262-3	0.000	9.446	0	1823630	N.D.	10.820 #
39)	L8 AR-1262-4	0.000	9.446	0	1823630	N.D.	5.436 #
41)	L9 AR-1268-1	0.000	9.446	0	1823630	N.D.	3.530 #
42)	L9 AR-1268-2	0.000	9.446	0	1823630	N.D.	3.697 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ041219\
 Data File : PQ039072.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2019 18:11
 Operator : AJ\SJ
 Sample : K1560-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 00:59:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ041219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Apr 13 00:36:36 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	10.845	9.662	3417023	3600406	5.182	9.035 #
45) L9	AR-1268-5	0.000	10.292	0	1049721	N.D.	0.823 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ041219\
Data File : PQ039072.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2019 18:11
Operator : AJ\SJ
Sample : K1560-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 00:59:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ041219.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Apr 13 00:36:36 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

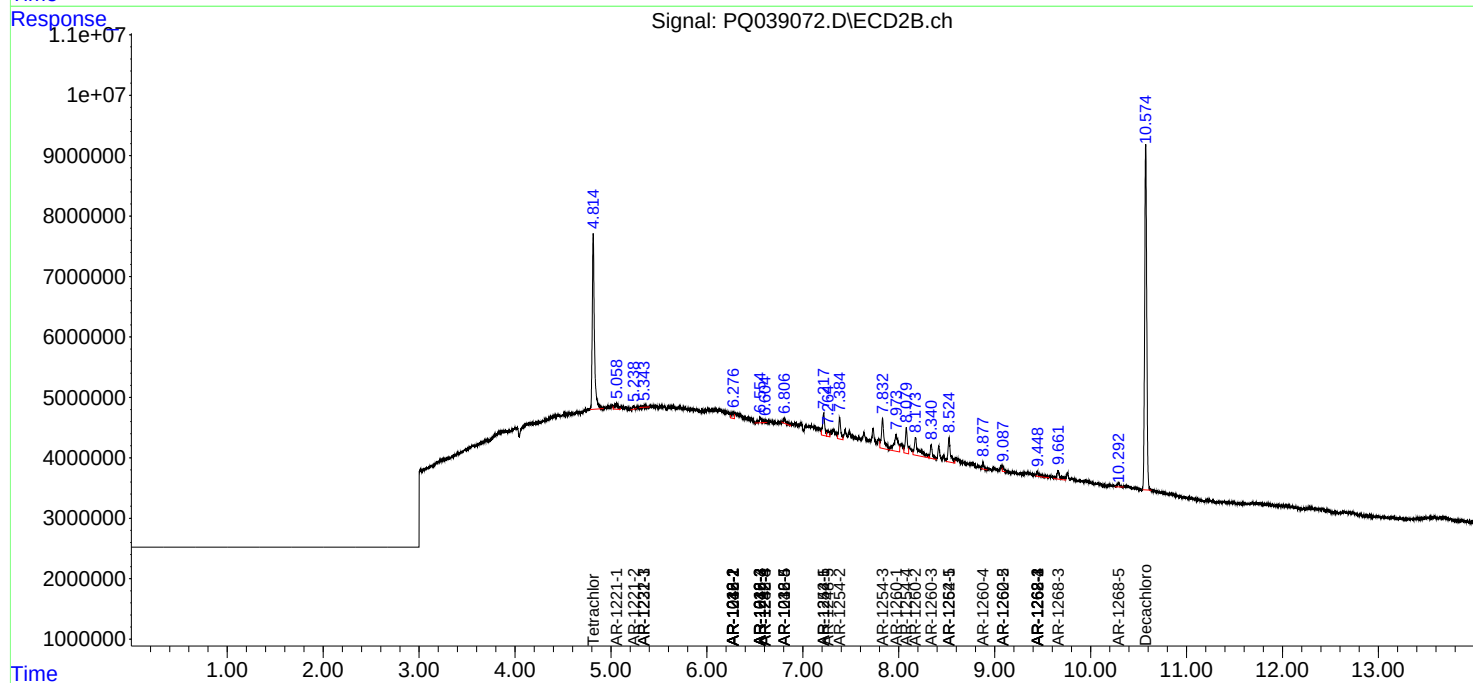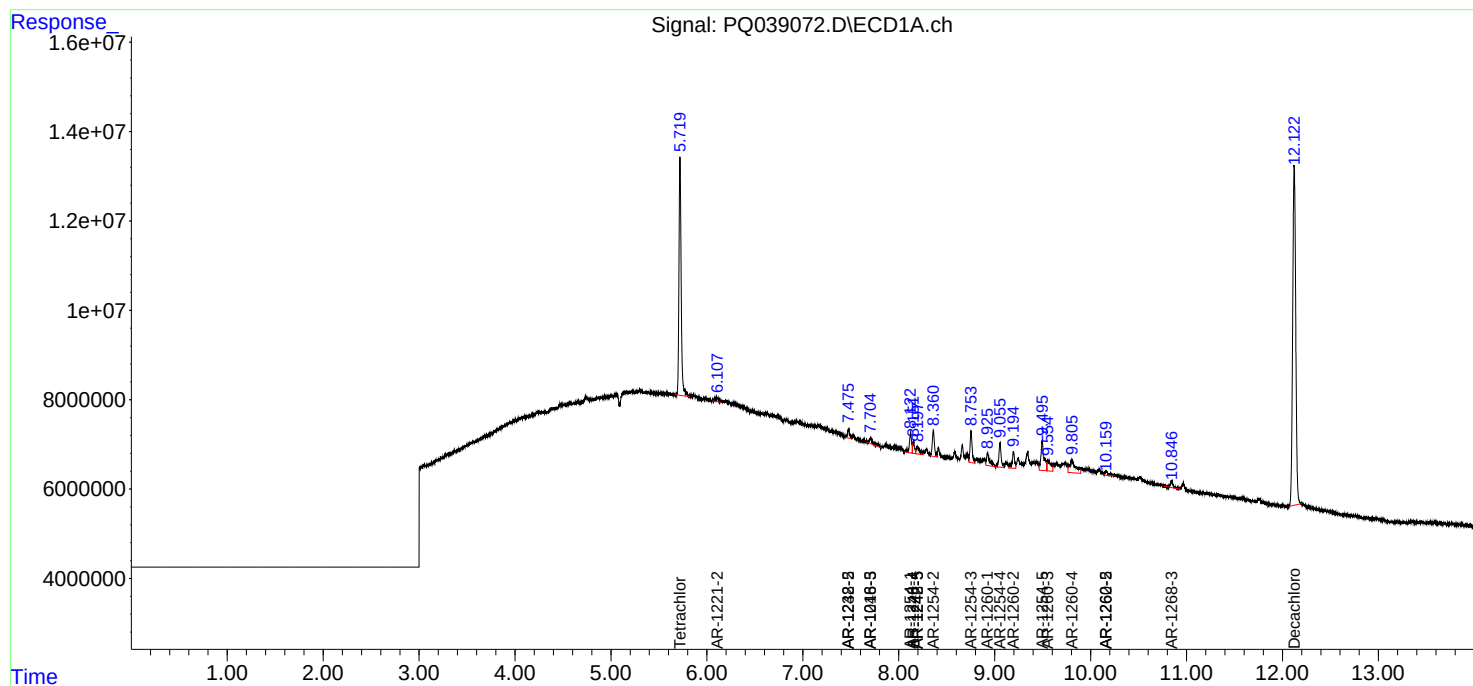


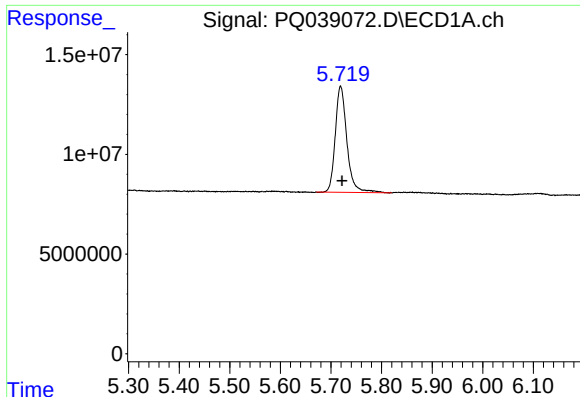

#1 Tetrachloro-m-xylene


R.T.: 5.719 min
Delta R.T.: -0.003 min
Response: 84793498
Conc: 19.13 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

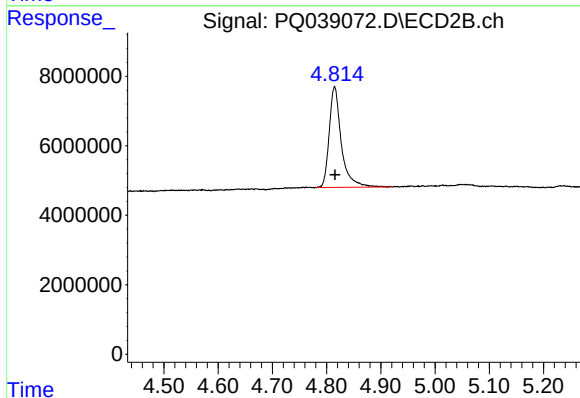


#1 Tetrachloro-m-xylene

R.T.: 4.815 min
Delta R.T.: -0.001 min
Response: 45148214
Conc: 20.25 ng/ml

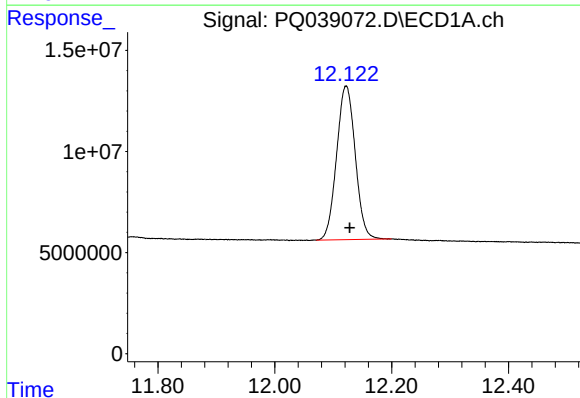


#2 Decachlorobiphenyl

R.T.: 12.122 min
Delta R.T.: -0.007 min
Response: 168448713
Conc: 24.28 ng/ml

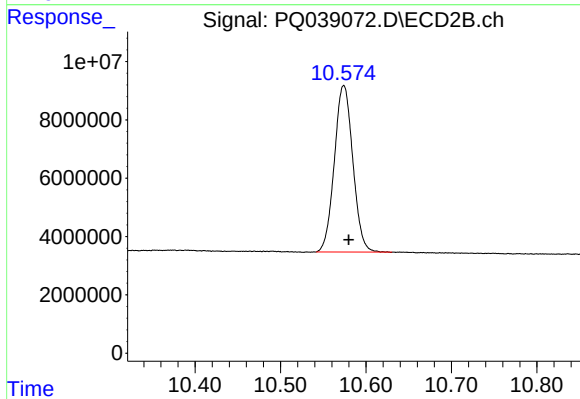

#2 Decachlorobiphenyl


R.T.: 10.574 min
Delta R.T.: -0.006 min
Response: 85841401
Conc: 24.60 ng/ml

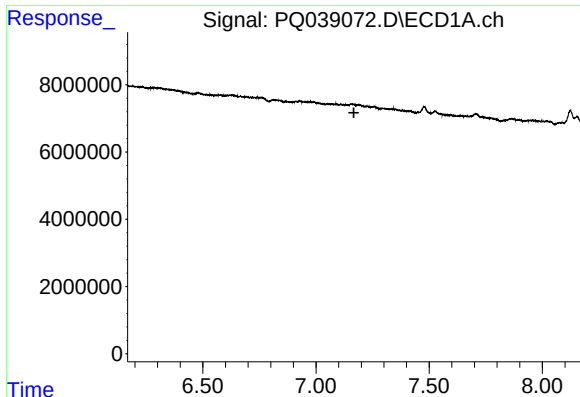

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 7.167 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

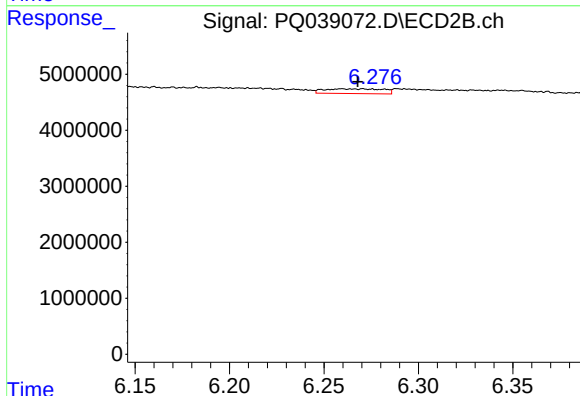


#3 AR-1016-1

R.T.: 6.270 min
Delta R.T.: 0.002 min
Response: 1828073
Conc: 18.00 ng/ml

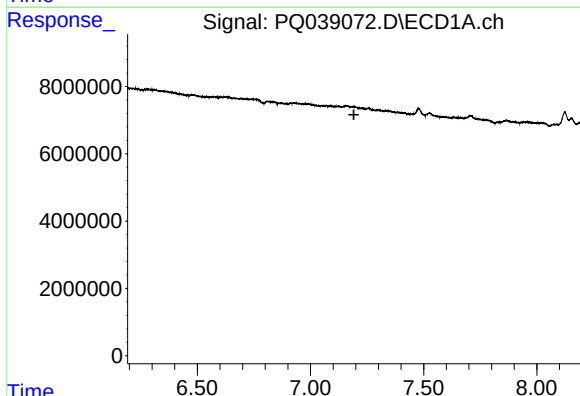


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 7.192 min
Response: 0
Conc: N.D.

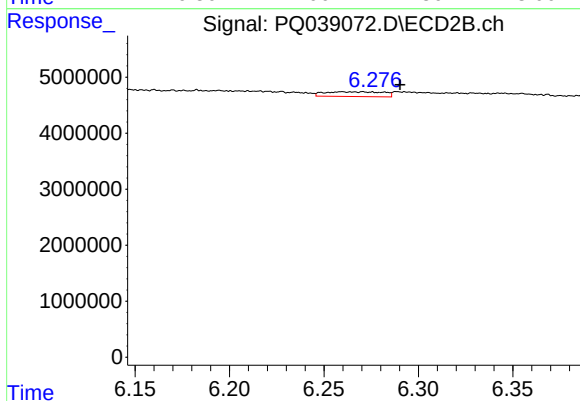

#4 AR-1016-2


R.T.: 6.270 min
Delta R.T.: -0.020 min
Response: 1828073
Conc: 12.34 ng/ml

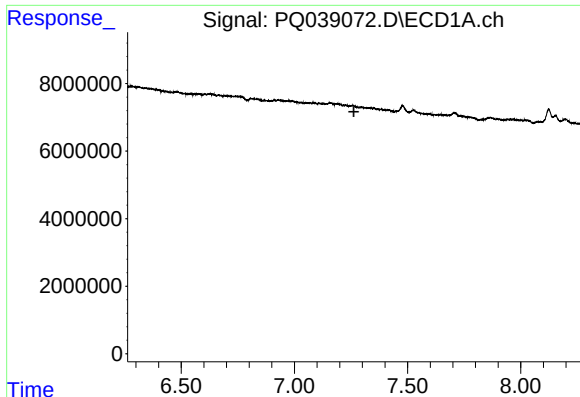

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 7.263 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

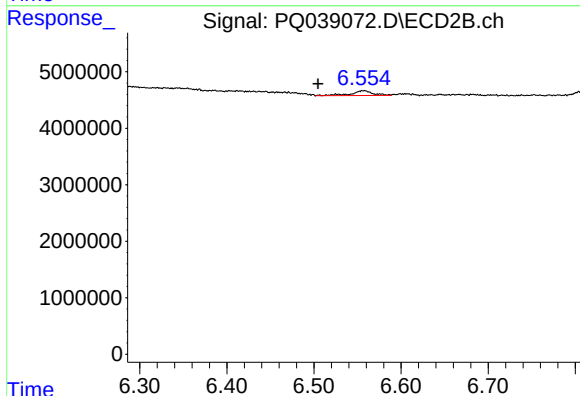


#5 AR-1016-3

R.T.: 6.557 min
Delta R.T.: 0.052 min
Response: 1494382
Conc: 20.03 ng/ml

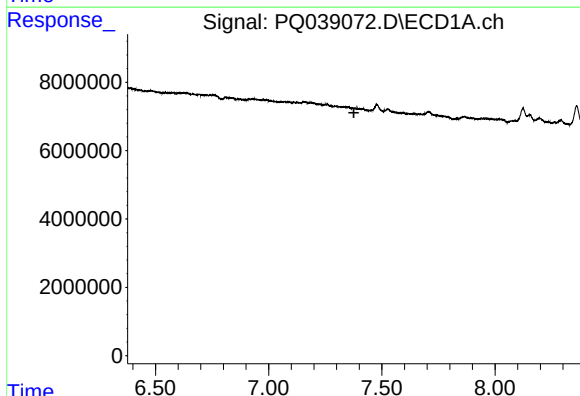


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 7.377 min
Response: 0
Conc: N.D.

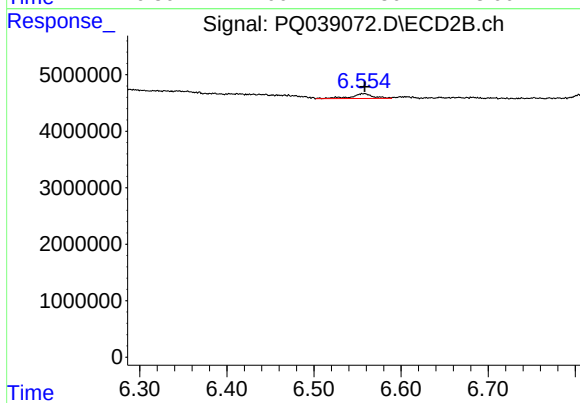

#6 AR-1016-4


R.T.: 6.557 min
Delta R.T.: -0.001 min
Response: 1494382
Conc: 23.97 ng/ml

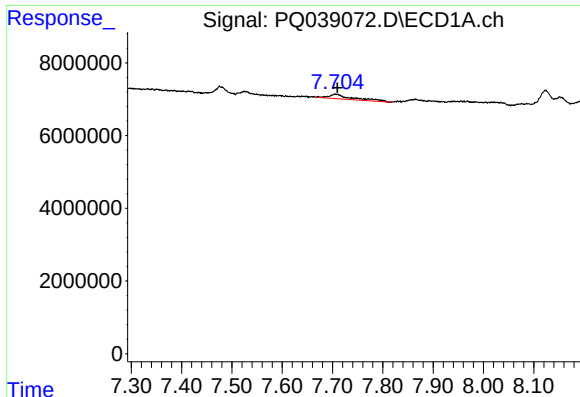

#7 AR-1016-5


R.T.: 7.706 min
Delta R.T.: -0.003 min
Response: 4089632
Conc: 28.82 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

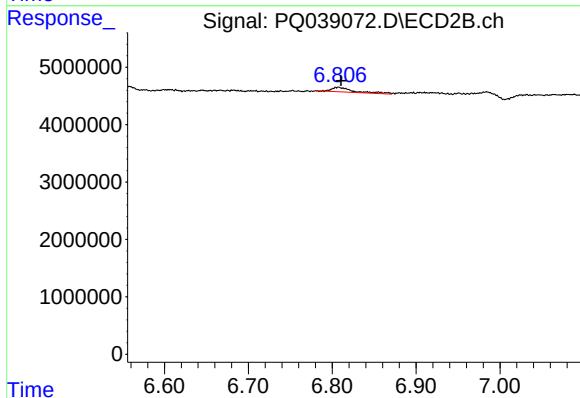


#7 AR-1016-5

R.T.: 6.807 min
Delta R.T.: -0.003 min
Response: 1496398
Conc: 16.86 ng/ml

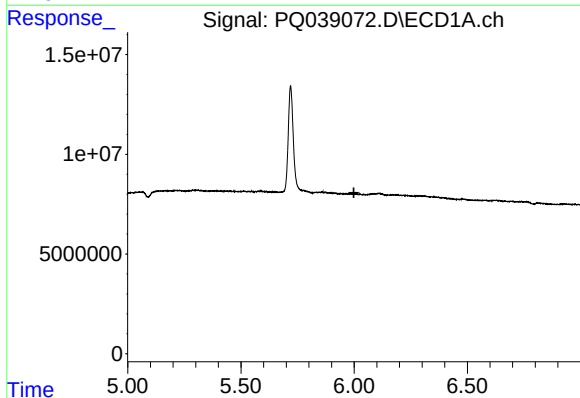


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 5.999 min
Response: 0
Conc: N.D.

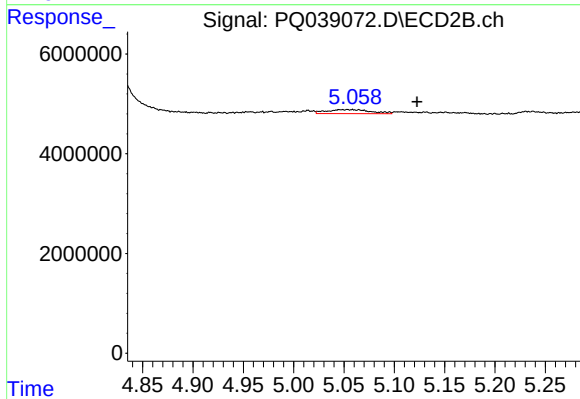

#8 AR-1221-1


R.T.: 5.054 min
Delta R.T.: -0.069 min
Response: 2456067
Conc: 103.38 ng/ml

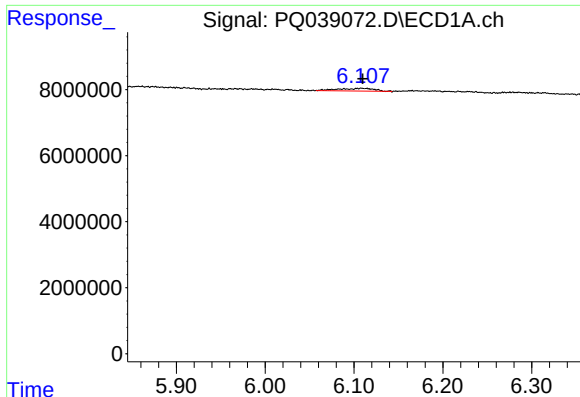

#9 AR-1221-2


R.T.: 6.109 min
Delta R.T.: 0.000 min
Response: 2379770
Conc: 70.10 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

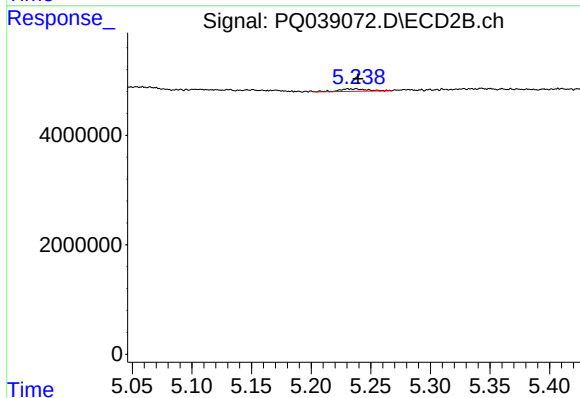


#9 AR-1221-2

R.T.: 5.234 min
Delta R.T.: -0.005 min
Response: 741386
Conc: 35.55 ng/ml

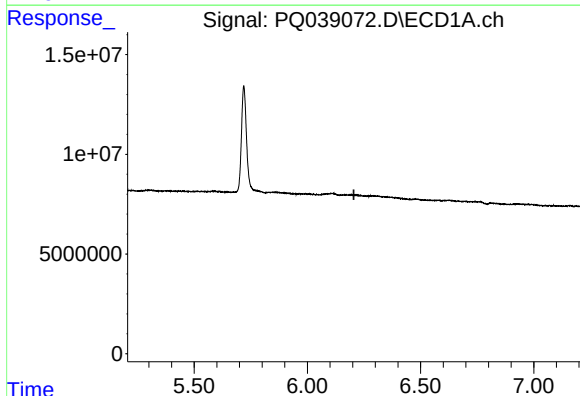


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

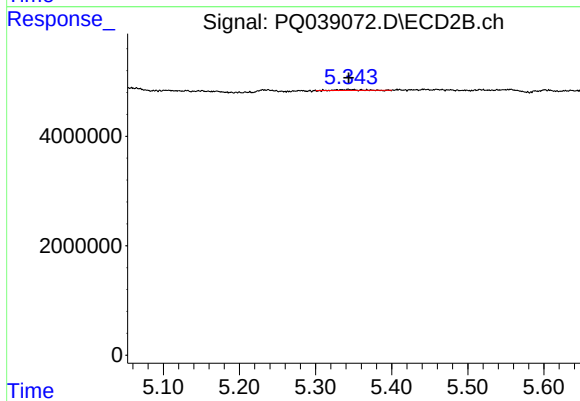

#10 AR-1221-3


R.T.: 5.344 min
Delta R.T.: 0.000 min
Response: 275501
Conc: 4.49 ng/ml

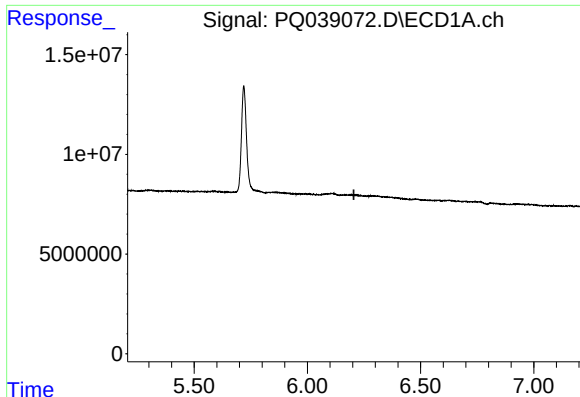

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 6.206 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

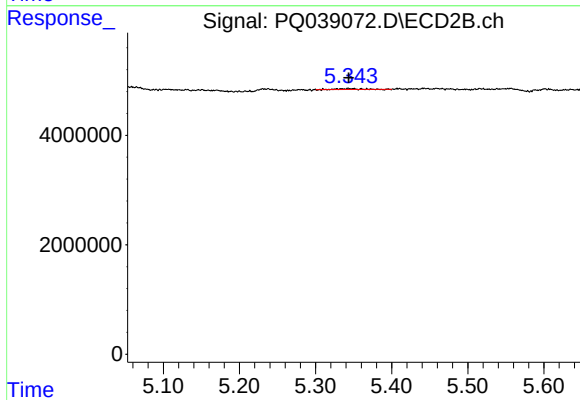


#11 AR-1232-1

R.T.: 5.344 min
Delta R.T.: 0.000 min
Response: 275501
Conc: 7.27 ng/ml

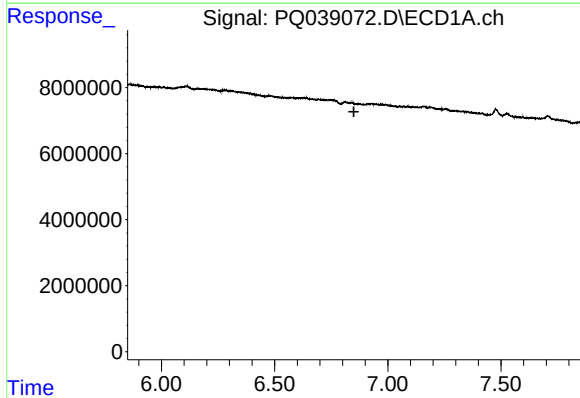


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T.: 6.850 min
Response: 0
Conc: N.D.

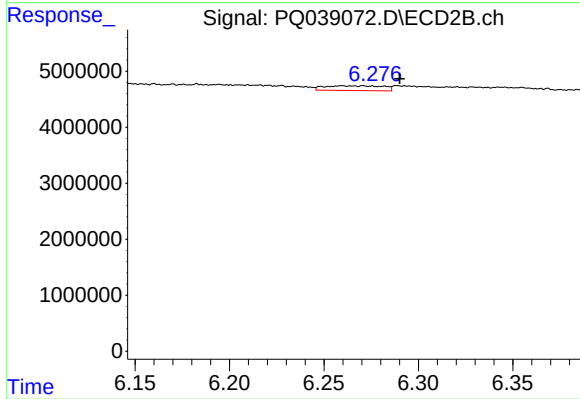

#12 AR-1232-2


R.T.: 6.270 min
Delta R.T.: -0.020 min
Response: 1828073
Conc: 39.33 ng/ml

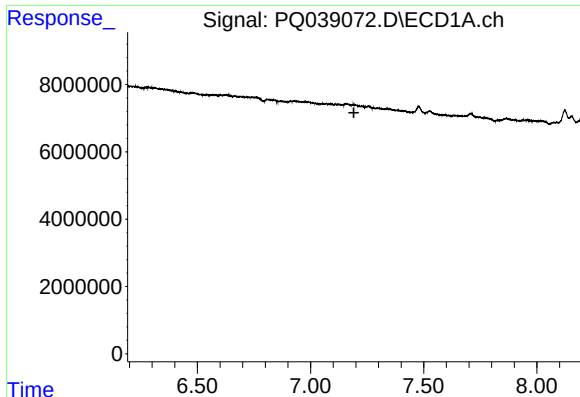

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T. : 7.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

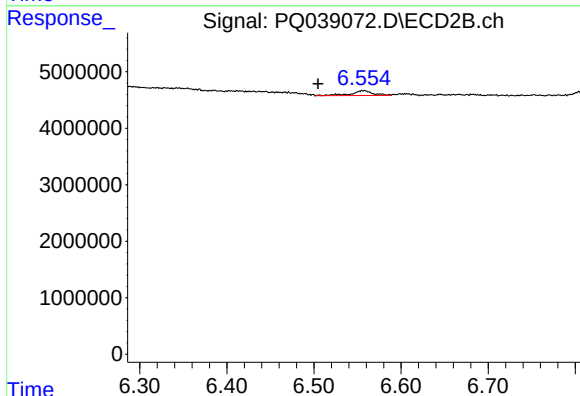


#13 AR-1232-3

R.T.: 6.557 min
Delta R.T.: 0.052 min
Response: 1494382
Conc: 70.45 ng/ml

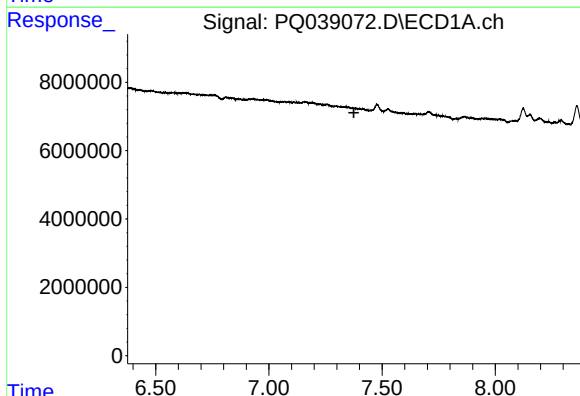


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 7.375 min
Response: 0
Conc: N.D.

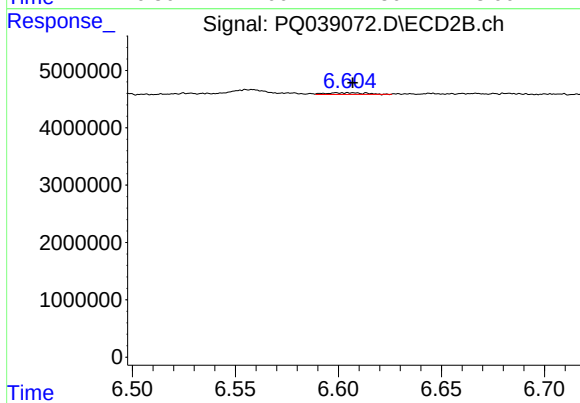

#14 AR-1232-4


R.T.: 6.604 min
Delta R.T.: -0.003 min
Response: 365395
Conc: 17.36 ng/ml

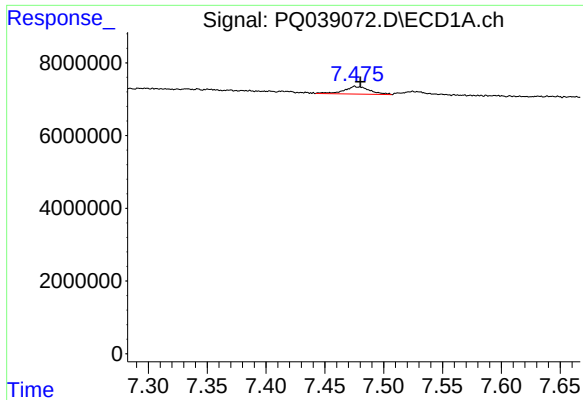

#15 AR-1232-5


R.T.: 7.477 min
Delta R.T.: -0.003 min
Response: 3171157
Conc: 77.04 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

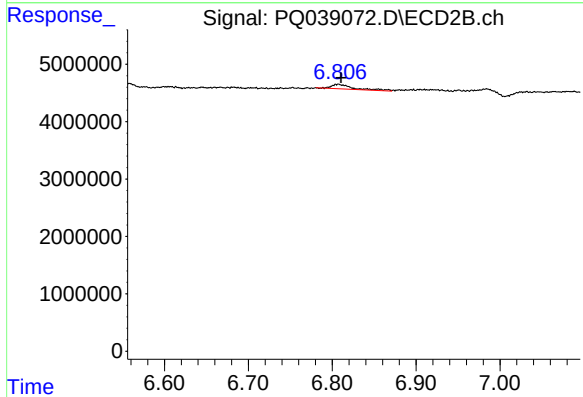


#15 AR-1232-5

R.T.: 6.807 min
Delta R.T.: -0.003 min
Response: 1496398
Conc: 61.40 ng/ml

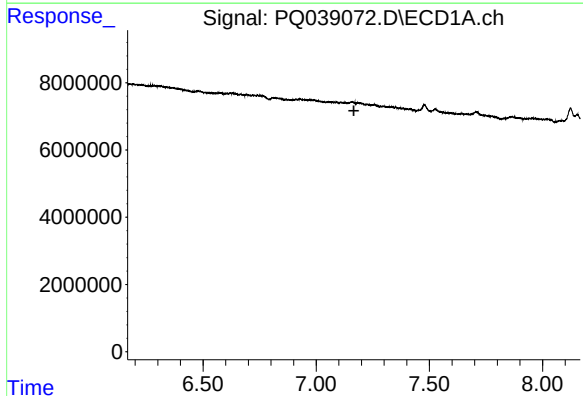


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 7.167 min
Response: 0
Conc: N.D.

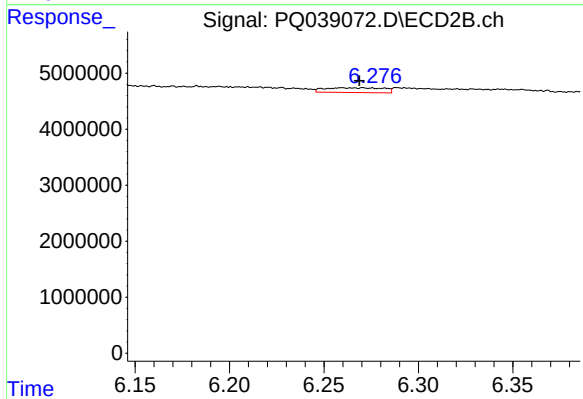

#16 AR-1242-1


R.T.: 6.270 min
Delta R.T.: 0.001 min
Response: 1828073
Conc: 31.14 ng/ml

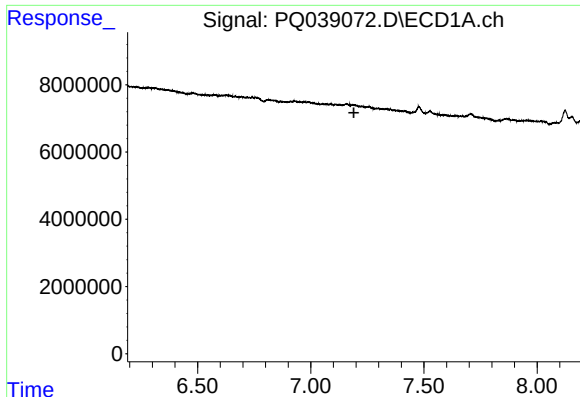

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 7.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

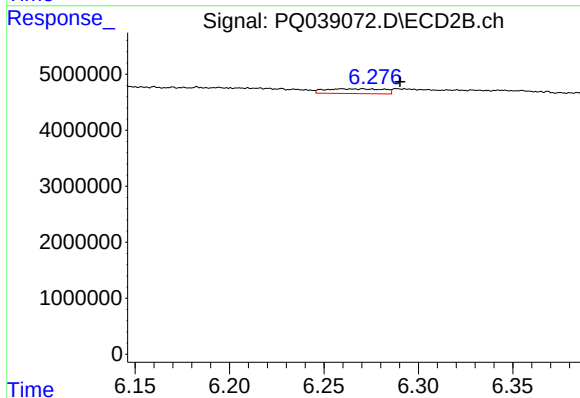


#17 AR-1242-2

R.T.: 6.270 min
Delta R.T.: -0.020 min
Response: 1828073
Conc: 21.27 ng/ml

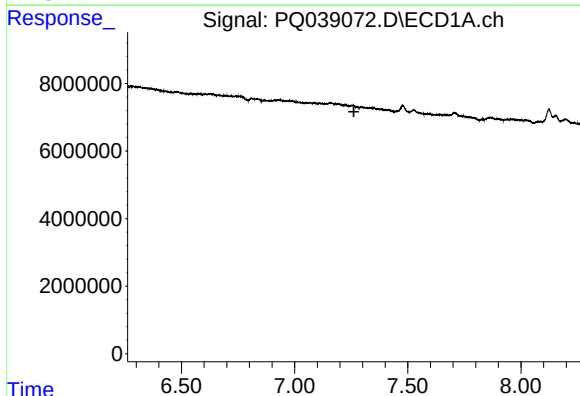


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T.: 7.262 min
Response: 0
Conc: N.D.

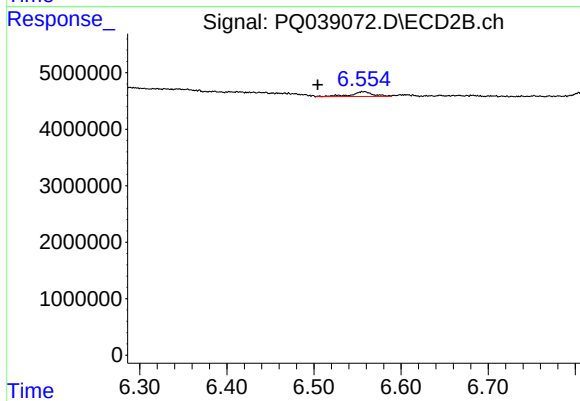

#18 AR-1242-3


R.T.: 6.557 min
Delta R.T.: 0.053 min
Response: 1494382
Conc: 35.39 ng/ml

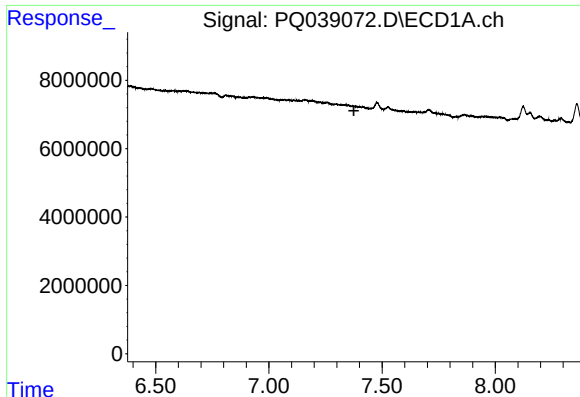

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 7.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

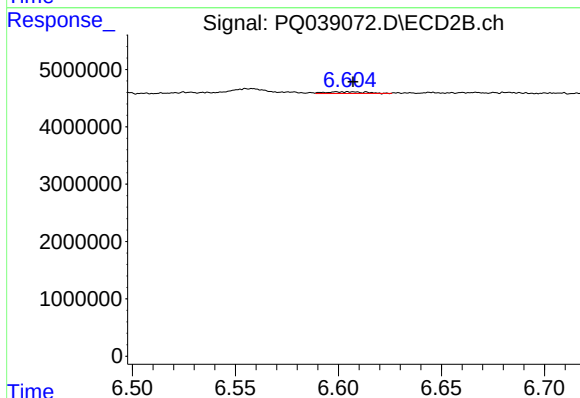


#19 AR-1242-4

R.T.: 6.604 min
Delta R.T.: -0.003 min
Response: 365395
Conc: 8.16 ng/ml

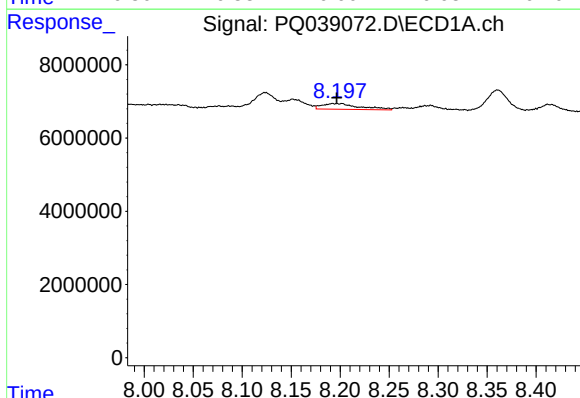


#20 AR-1242-5

R.T.: 8.196 min
Delta R.T.: 0.000 min
Response: 4238002
Conc: 42.90 ng/ml

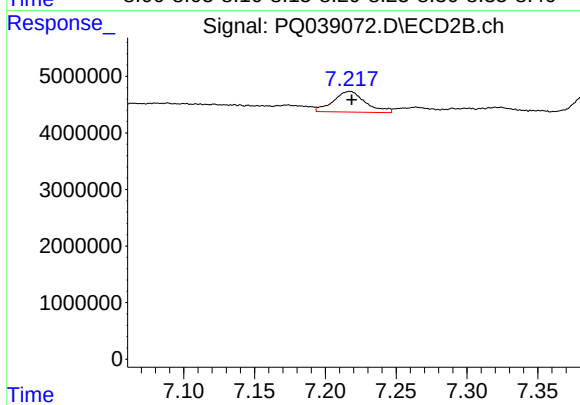

#20 AR-1242-5


R.T.: 7.217 min
Delta R.T.: -0.002 min
Response: 5807948
Conc: 89.56 ng/ml

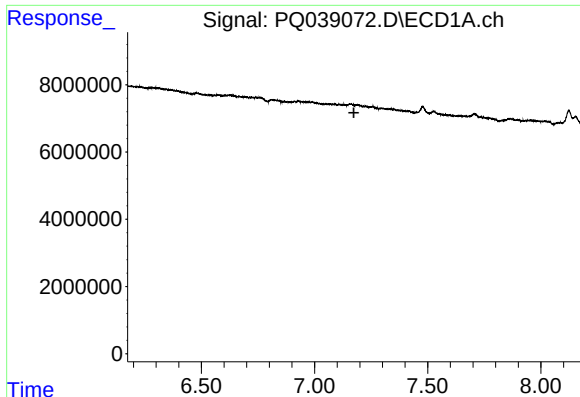

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 7.174 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

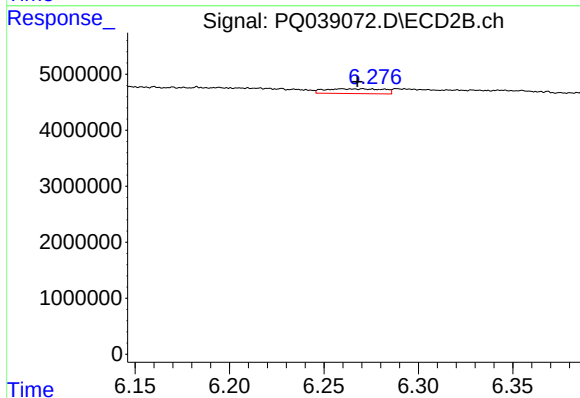


#21 AR-1248-1

R.T.: 6.270 min
Delta R.T.: 0.002 min
Response: 1828073
Conc: 41.02 ng/ml

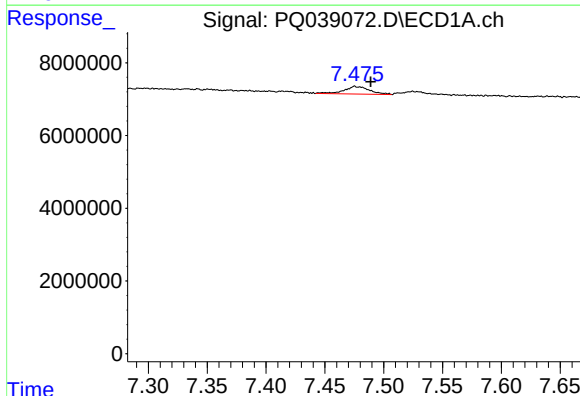


#22 AR-1248-2

R.T.: 7.477 min
Delta R.T.: -0.012 min
Response: 3171157
Conc: 27.76 ng/ml

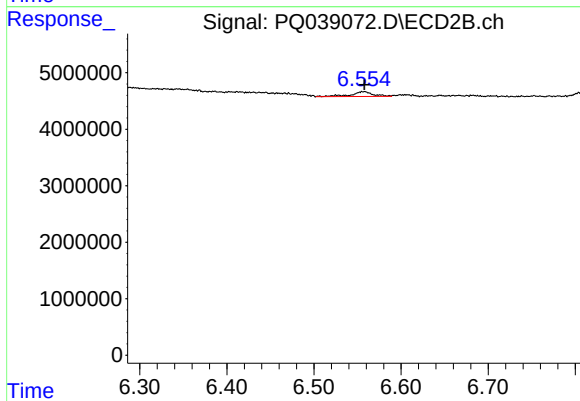

#22 AR-1248-2


R.T.: 6.557 min
Delta R.T.: -0.001 min
Response: 1494382
Conc: 25.03 ng/ml

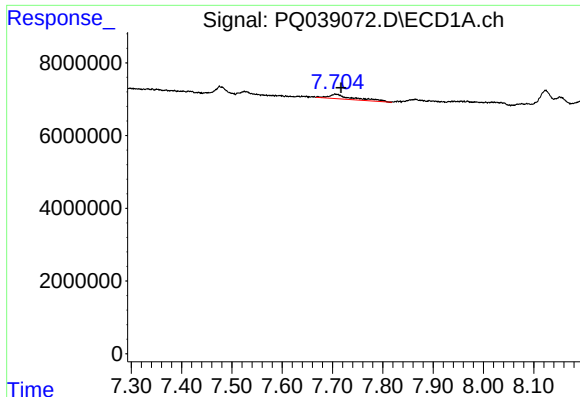

#23 AR-1248-3


R.T.: 7.706 min
Delta R.T.: -0.011 min
Response: 4089632
Conc: 29.83 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

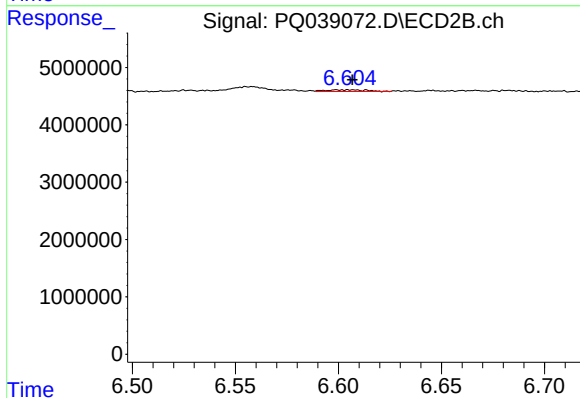


#23 AR-1248-3

R.T.: 6.604 min
Delta R.T.: -0.003 min
Response: 365395
Conc: 5.71 ng/ml

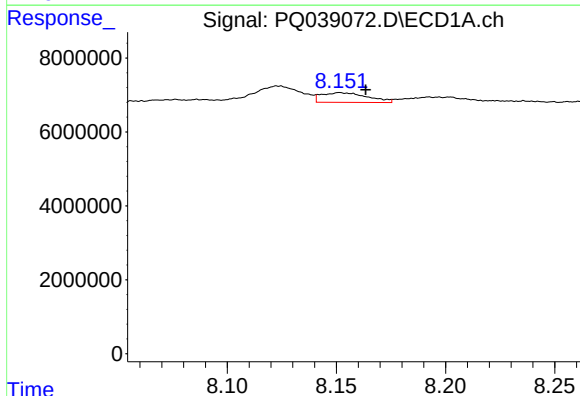


#24 AR-1248-4

R.T.: 8.152 min
Delta R.T.: -0.011 min
Response: 3839137
Conc: 24.60 ng/ml

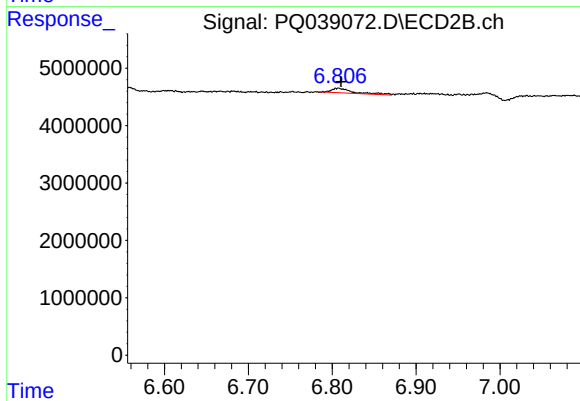

#24 AR-1248-4


R.T.: 6.807 min
Delta R.T.: -0.004 min
Response: 1496398
Conc: 18.19 ng/ml

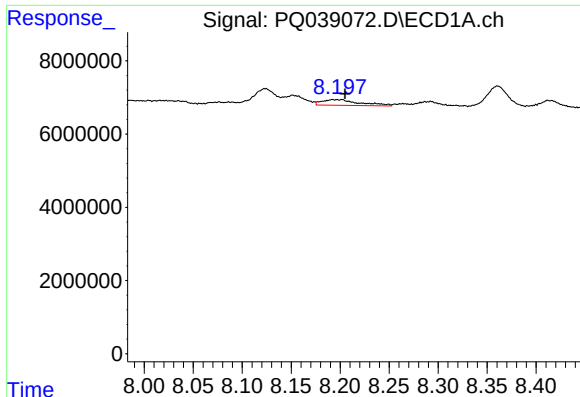

#25 AR-1248-5


R.T.: 8.196 min
Delta R.T.: -0.009 min
Response: 4238002
Conc: 27.71 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

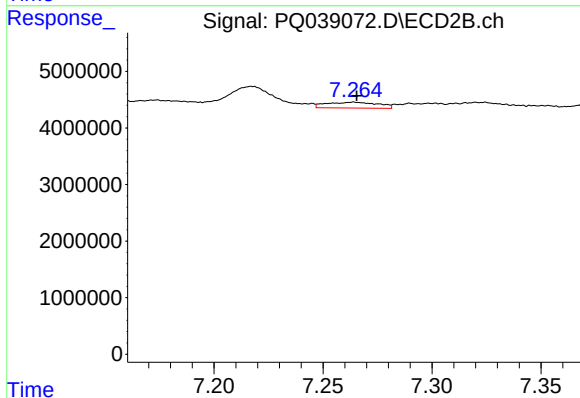


#25 AR-1248-5

R.T.: 7.264 min
Delta R.T.: -0.001 min
Response: 1711182
Conc: 20.54 ng/ml

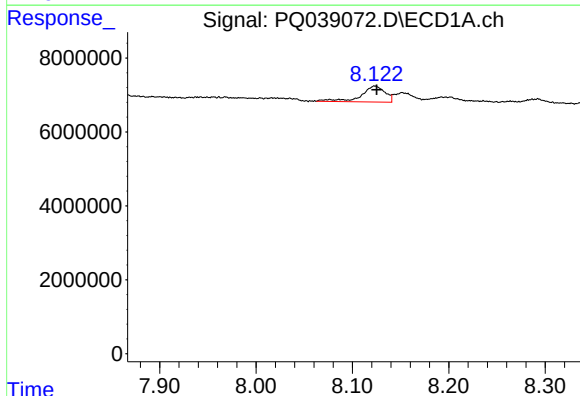


#26 AR-1254-1

R.T.: 8.123 min
Delta R.T.: -0.002 min
Response: 7393071
Conc: 42.94 ng/ml

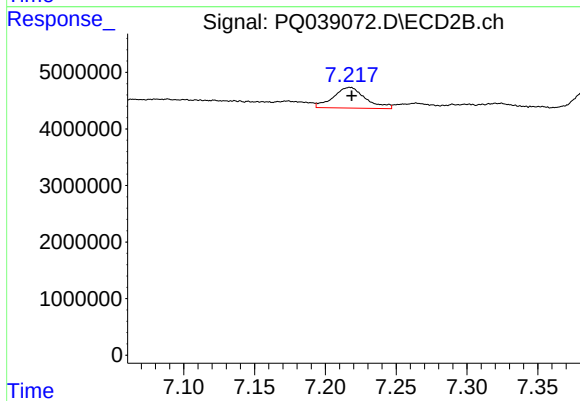

#26 AR-1254-1


R.T.: 7.217 min
Delta R.T.: -0.002 min
Response: 5807948
Conc: 40.64 ng/ml

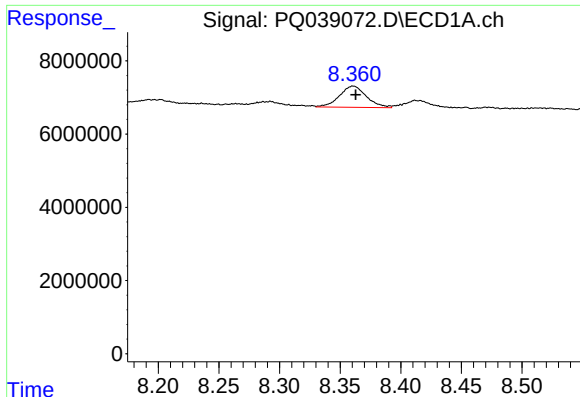

#27 AR-1254-2


R.T.: 8.361 min
Delta R.T.: -0.002 min
Response: 8978301
Conc: 32.79 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

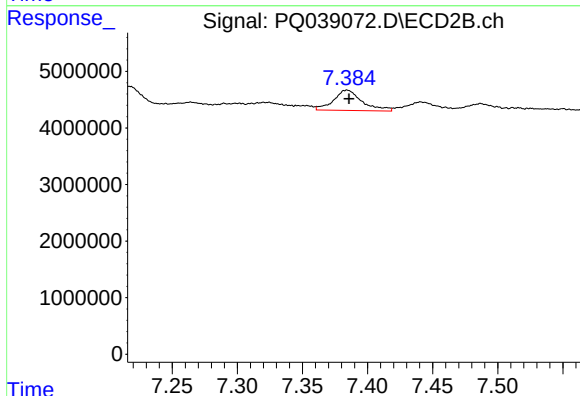


#27 AR-1254-2

R.T.: 7.384 min
Delta R.T.: -0.001 min
Response: 5470527
Conc: 43.08 ng/ml

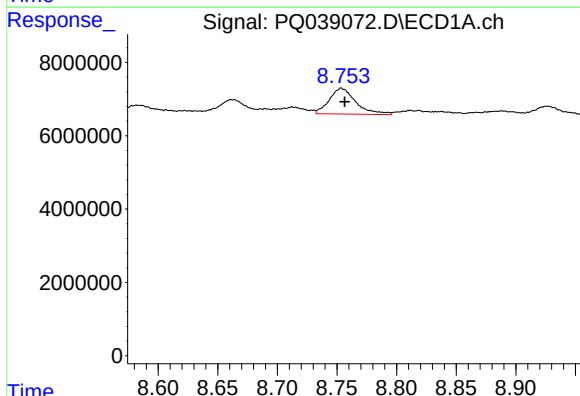


#28 AR-1254-3

R.T.: 8.754 min
Delta R.T.: -0.002 min
Response: 10921896
Conc: 35.56 ng/ml

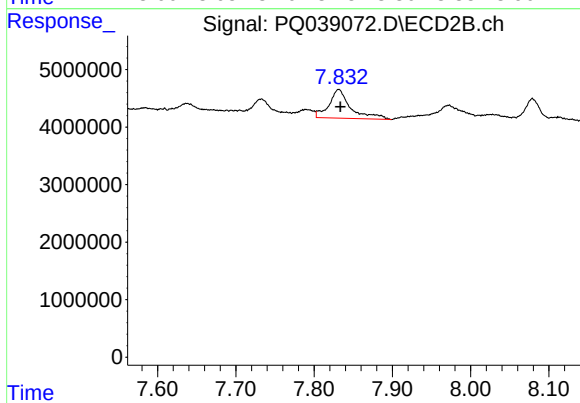

#28 AR-1254-3


R.T.: 7.831 min
Delta R.T.: -0.002 min
Response: 9590995
Conc: 42.87 ng/ml

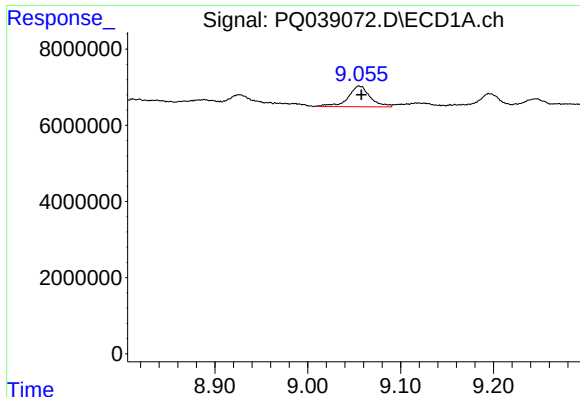

#29 AR-1254-4


R.T.: 9.056 min
Delta R.T.: -0.002 min
Response: 8877892
Conc: 39.97 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

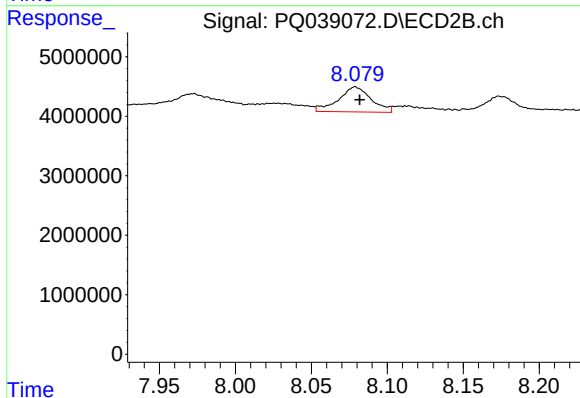


#29 AR-1254-4

R.T.: 8.079 min
Delta R.T.: -0.003 min
Response: 6294397
Conc: 44.87 ng/ml

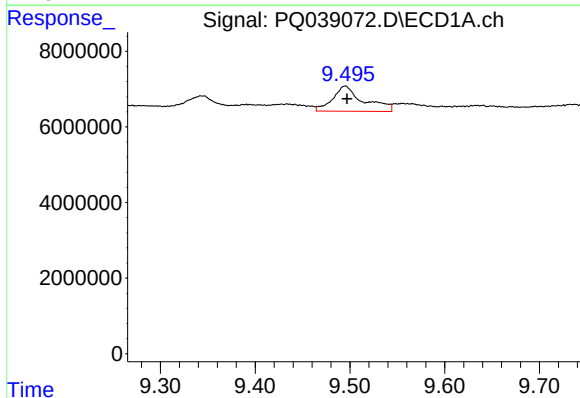


#30 AR-1254-5

R.T.: 9.495 min
Delta R.T.: -0.002 min
Response: 14987628
Conc: 57.74 ng/ml

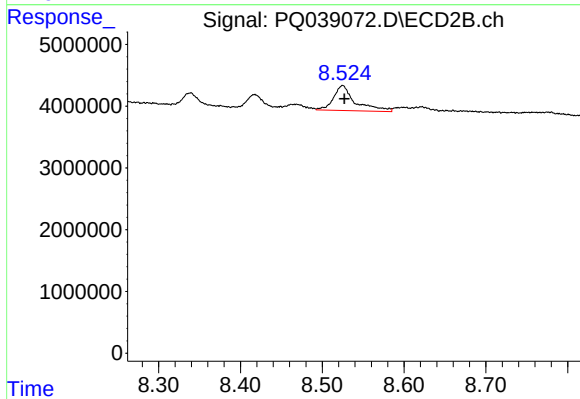

#30 AR-1254-5


R.T.: 8.525 min
Delta R.T.: -0.002 min
Response: 7497703
Conc: 36.34 ng/ml

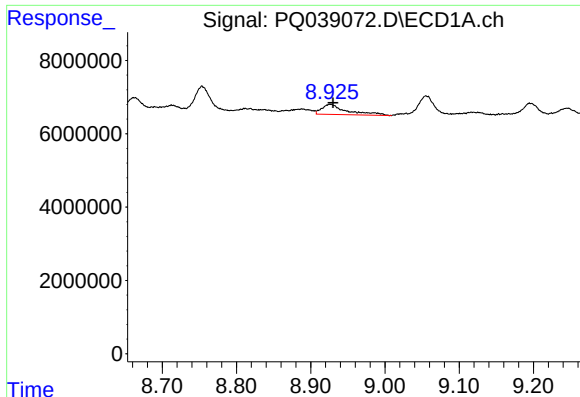

#31 AR-1260-1


R.T.: 8.926 min
Delta R.T.: -0.004 min
Response: 6479766
Conc: 23.18 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

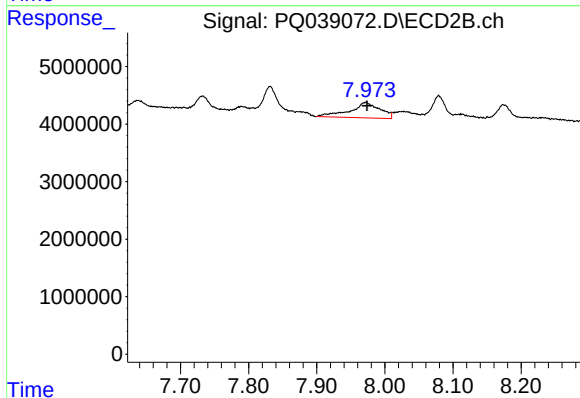


#31 AR-1260-1

R.T.: 7.972 min
Delta R.T.: -0.002 min
Response: 8155869
Conc: 44.26 ng/ml

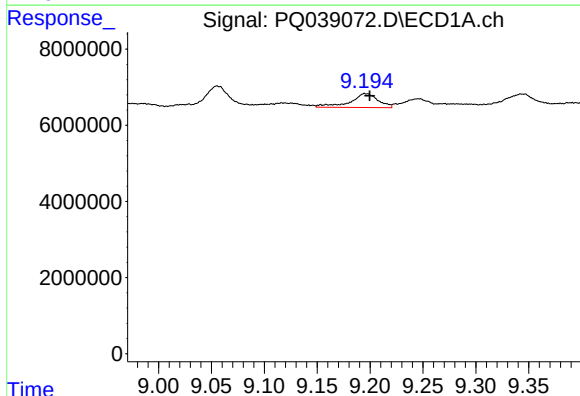


#32 AR-1260-2

R.T.: 9.196 min
Delta R.T.: -0.004 min
Response: 6758195
Conc: 20.20 ng/ml

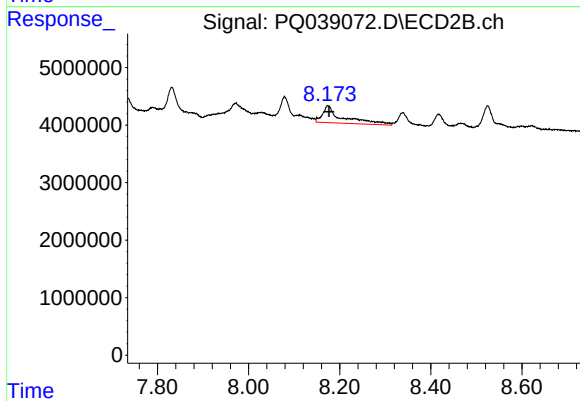

#32 AR-1260-2


R.T.: 8.175 min
Delta R.T.: -0.002 min
Response: 9075257
Conc: 41.14 ng/ml

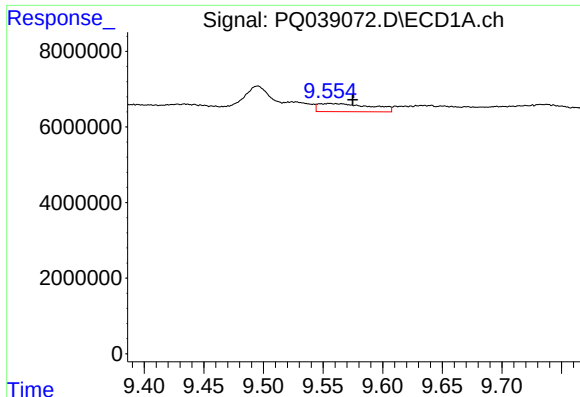

#33 AR-1260-3


R.T.: 9.556 min
Delta R.T.: -0.019 min
Response: 6544774
Conc: 23.76 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

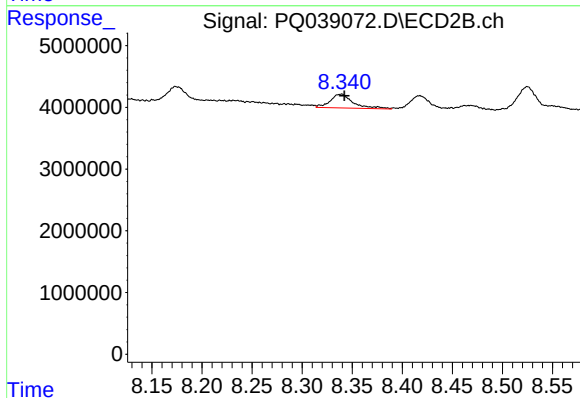


#33 AR-1260-3

R.T.: 8.338 min
Delta R.T.: -0.004 min
Response: 3583960
Conc: 17.59 ng/ml

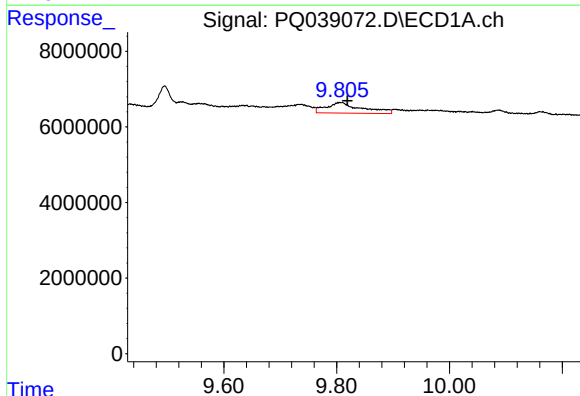


#34 AR-1260-4

R.T.: 9.807 min
Delta R.T.: -0.012 min
Response: 12532395
Conc: 38.35 ng/ml

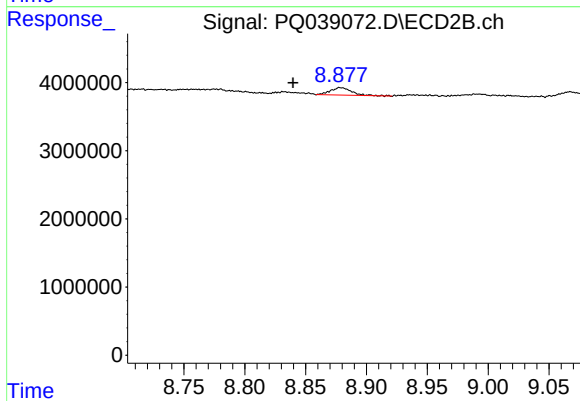

#34 AR-1260-4


R.T.: 8.879 min
Delta R.T.: 0.039 min
Response: 1333400
Conc: 7.31 ng/ml

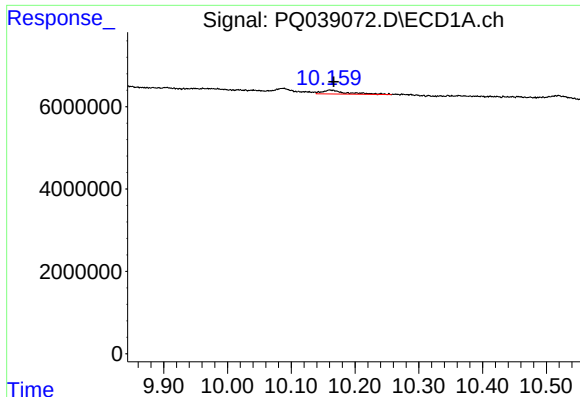

#35 AR-1260-5


R.T.: 10.162 min
Delta R.T.: -0.005 min
Response: 2569906
Conc: 3.86 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

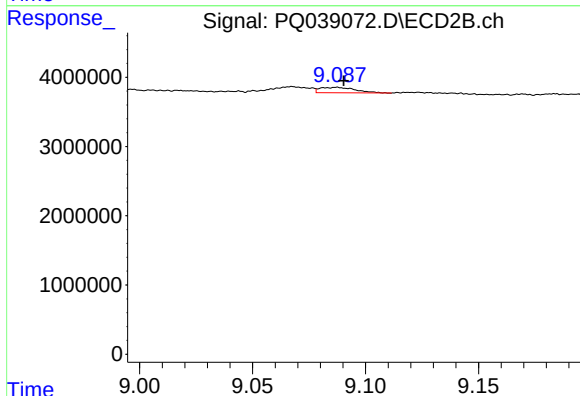


#35 AR-1260-5

R.T.: 9.086 min
Delta R.T.: -0.004 min
Response: 865430
Conc: 1.94 ng/ml

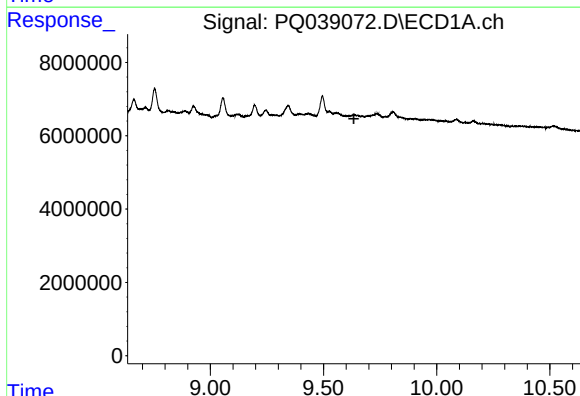


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 9.634 min
Response: 0
Conc: N.D.

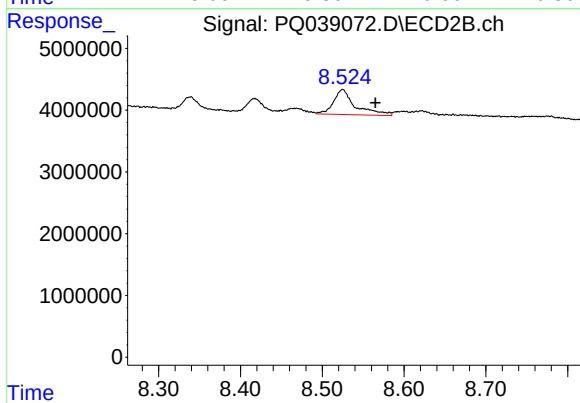

#36 AR-1262-1


R.T.: 8.525 min
Delta R.T.: -0.040 min
Response: 7497703
Conc: 33.69 ng/ml

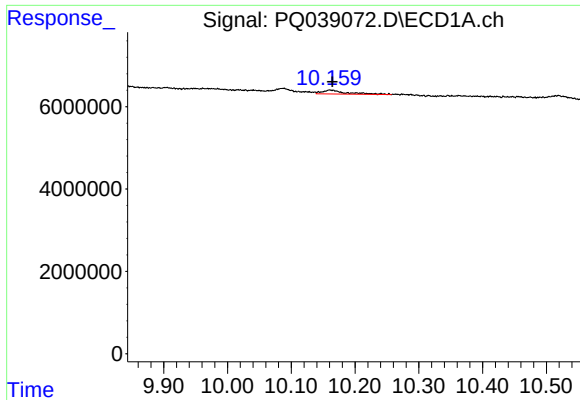

#37 AR-1262-2


R.T.: 10.162 min
Delta R.T.: -0.003 min
Response: 2569906
Conc: 4.05 ng/ml

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

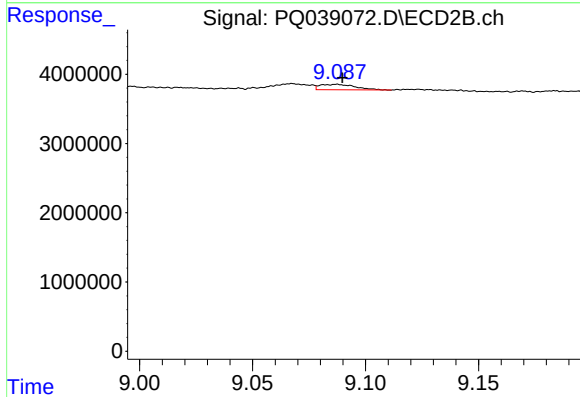


#37 AR-1262-2

R.T.: 9.086 min
Delta R.T.: -0.004 min
Response: 865430
Conc: 2.00 ng/ml

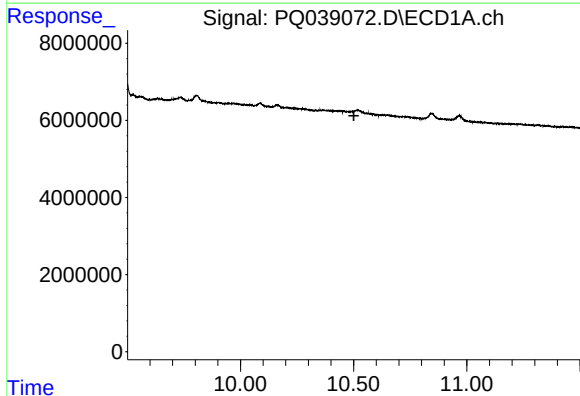


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 10.501 min
Response: 0
Conc: N.D.

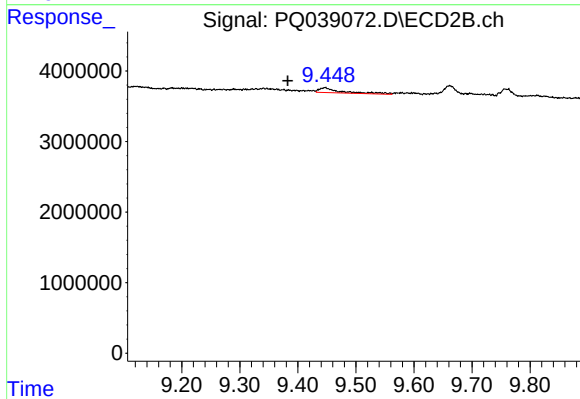

#38 AR-1262-3


R.T.: 9.446 min
Delta R.T.: 0.064 min
Response: 1823630
Conc: 10.82 ng/ml

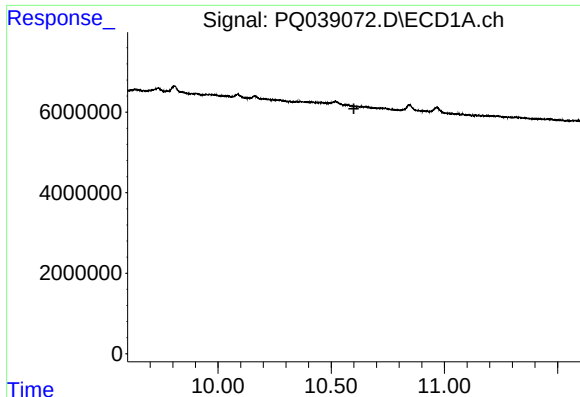

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 10.600 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

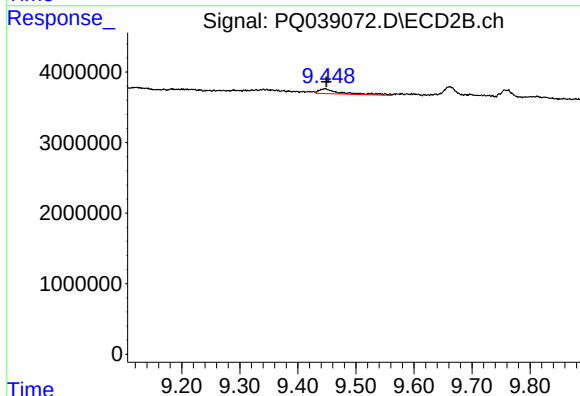


#39 AR-1262-4

R.T.: 9.446 min
Delta R.T.: -0.003 min
Response: 1823630
Conc: 5.44 ng/ml

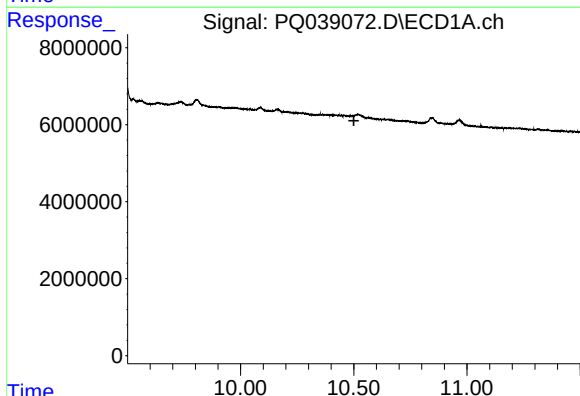


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 10.500 min
Response: 0
Conc: N.D.

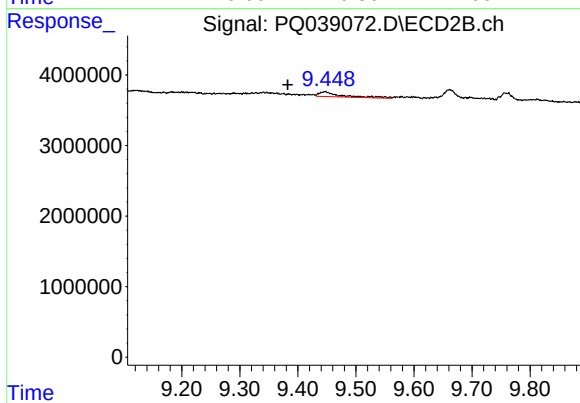

#41 AR-1268-1


R.T.: 9.446 min
Delta R.T.: 0.064 min
Response: 1823630
Conc: 3.53 ng/ml

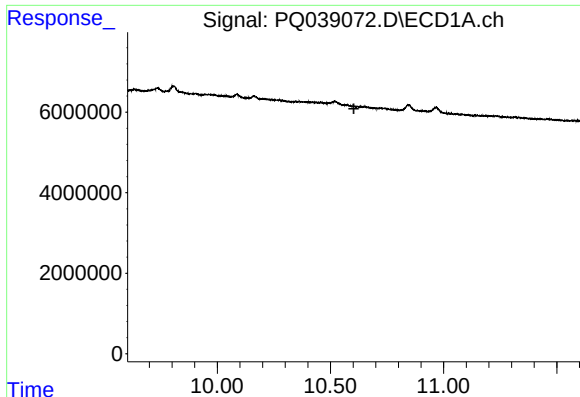

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 10.604 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

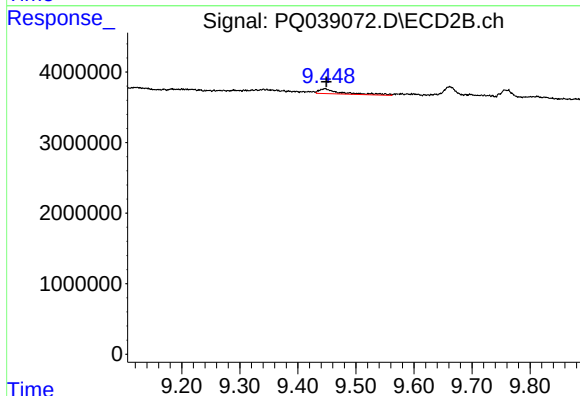


#42 AR-1268-2

R.T.: 9.446 min
Delta R.T.: -0.003 min
Response: 1823630
Conc: 3.70 ng/ml

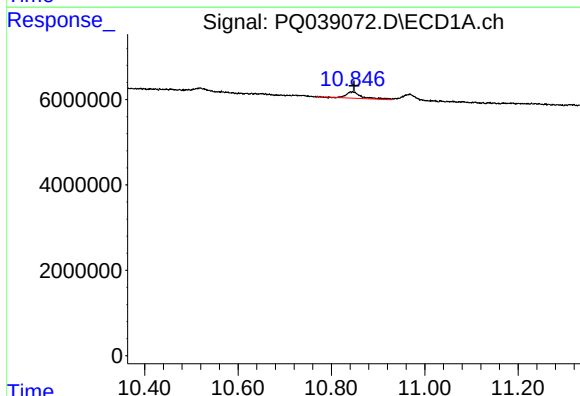


#43 AR-1268-3

R.T.: 10.845 min
Delta R.T.: -0.003 min
Response: 3417023
Conc: 5.18 ng/ml

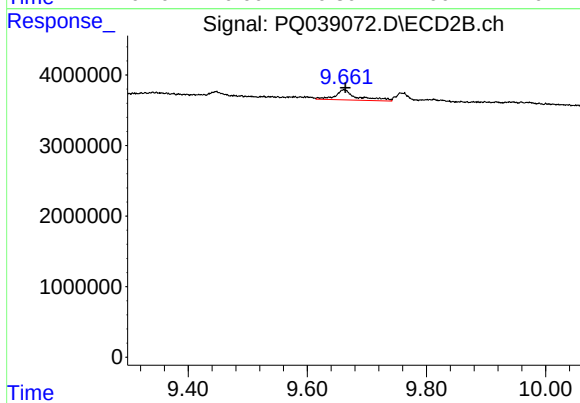

#43 AR-1268-3


R.T.: 9.662 min
Delta R.T.: -0.002 min
Response: 3600406
Conc: 9.03 ng/ml

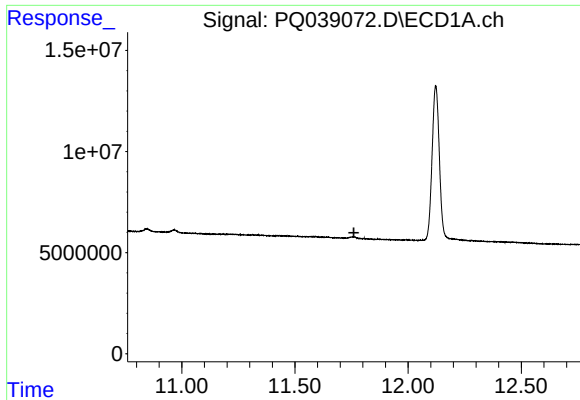

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 11.761 min
Response: 0
Conc: N.D.

Instrument :
ECD_Q
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

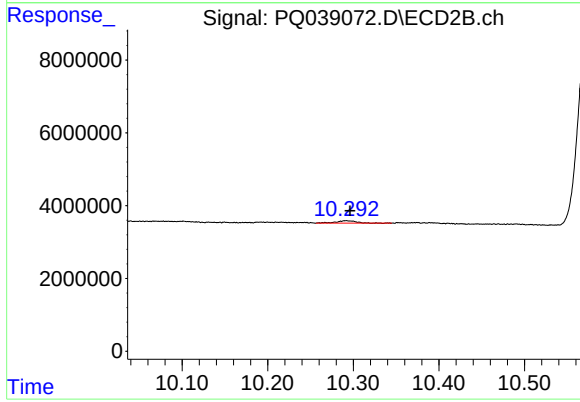

#45 AR-1268-5

R.T.: 10.292 min
Delta R.T.: -0.004 min
Response: 1049721
Conc: 0.82 ng/ml