

Data Path : P:\HPCHEM1\ECD_Q\Data\PQ041318\
 Data File : PQ027941.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2018 19:48
 Operator : UA/SM
 Sample : J2135-05DL 2X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 X2C43DL

Manual Integrations
 APPROVED

UGO
 4/18/2018 10:52:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 10:23:27 2018
 Quant Method : P:\HPCHEM1\ECD_Q\Method\PQ041018CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 10 04:16:48 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.620	3.779	915.9E6	107.2E6	11.078	11.127
2)	SA Decachlor...	10.384	8.733	1765.7E6	331.8E6	19.328	18.262
Target Compounds							
21)	L5 AR-1248-1	6.246	5.297	1502.1E6	222.6E6	425.530	429.320
22)	L5 AR-1248-2	6.385	5.608	1216.9E6	145.9E6	401.700	456.690
23)	L5 AR-1248-3	6.644	5.683	1795.5E6	252.3E6	421.451	439.612
24)	L5 AR-1248-4	6.684	6.097	1765.5E6	145.8E6	443.300	590.733 #
25)	L5 AR-1248-5	6.837	6.157	3041.4E6	56509491	739.301	390.457m#
31)	L7 AR-1260-1	7.363	6.313	2986.5E6	607.1E6	717.182	822.750
32)	L7 AR-1260-2	7.615	6.498	4186.0E6	681.5E6	708.352	712.847
33)	L7 AR-1260-3	7.974	6.650	2797.5E6	665.0E6	577.896	765.347 #
34)	L7 AR-1260-4	8.528	7.354	6359.0E6	1337.0E6	588.847	658.698
35)	L7 AR-1260-5	8.859	7.696	3598.9E6	905.5E6	595.987	611.594

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_Q\Data\PQ041318\
Data File : PQ027941.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2018 19:48
Operator : UA/SM
Sample : J2135-05DL 2X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampled :
X2C43DL

Manual Integrations
APPROVED

UGO
4/18/2018 10:52:51 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 10:23:27 2018
Quant Method : P:\HPCHEM1\ECD_Q\Method\PQ041018CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 10 04:16:48 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

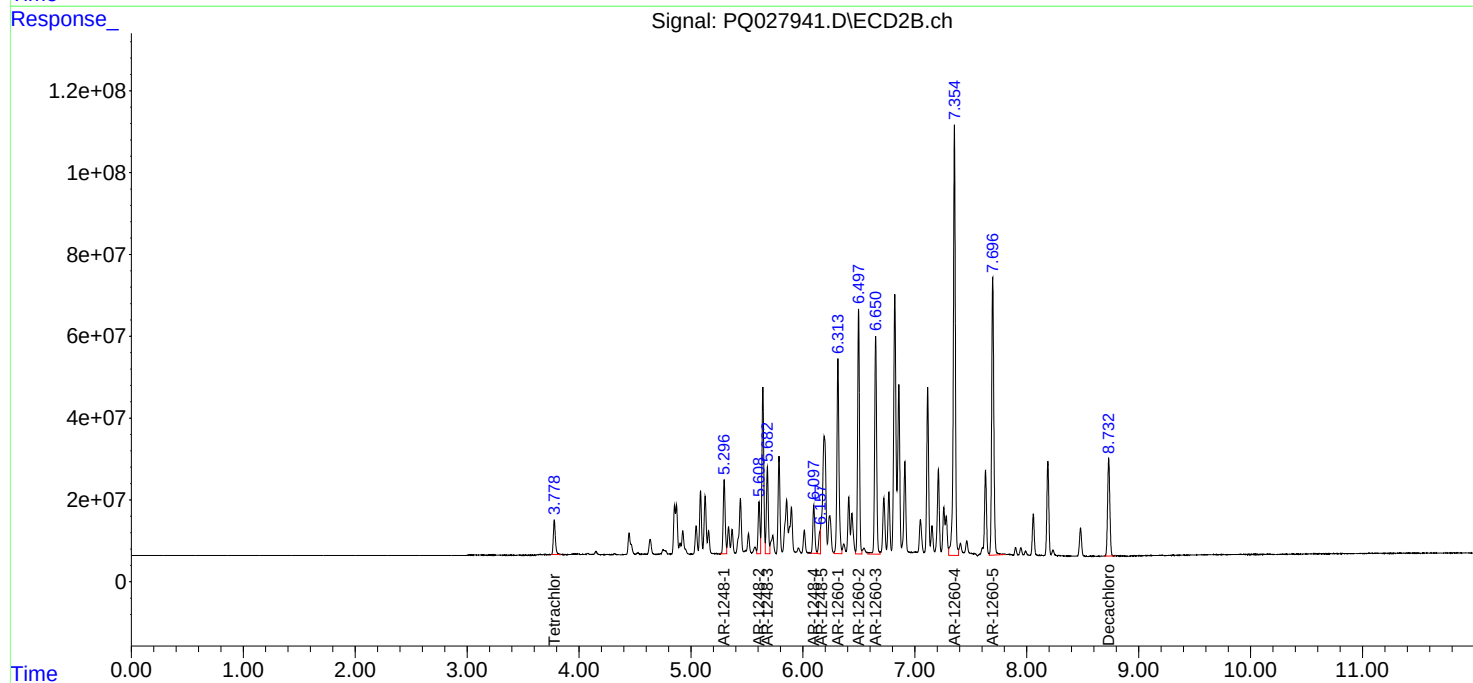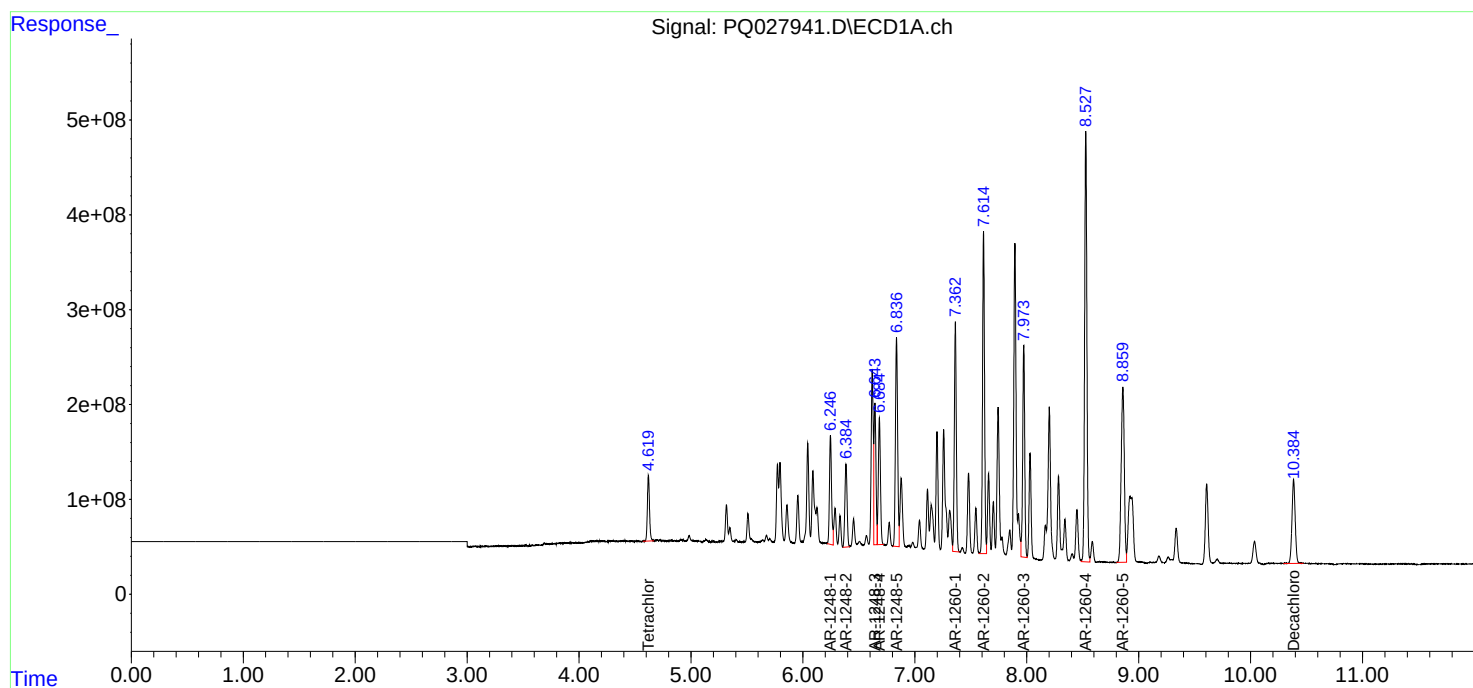

Data Path : P:\HPCHEM1\ECD_Q\Data\PQ041318\

Data File : PQ027941.D

Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch

Acq On : 11 Apr 2018 19:48

Operator : UA/SM

Sample : J2135-05DL 2X

Misc :

ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e

Integration File signal 2: autoint2.e

Quant Time: Apr 18 10:23:27 2018

Quant Method : P:\HPCHEM1\ECD_Q\Method\PQ041018CLP.M

Quant Title : GC EXTRACTABLES

QLast Update : Tue Apr 10 04:16:48 2018

Response via : Initial Calibration

Integrator: ChemStation

Volume Inj. : 1 µl

Signal #1 Phase : ZB MR1

Signal #2 Phase: ZB MR2

Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.620	3.779	915.9E6	107.2E6	11.078	11.127
2) SA Decachlor...	10.384	8.733	1765.7E6	331.8E6	19.328	18.262
Target Compounds						
21) L5 AR-1248-1	6.246	5.297	1502.1E6	222.6E6	425.530	429.320
22) L5 AR-1248-2	6.385	5.608	1216.9E6	145.9E6	401.700	456.690
23) L5 AR-1248-3	6.644	5.683	1795.5E6	252.3E6	421.451	439.612
24) L5 AR-1248-4	6.684	6.097	1765.5E6	145.8E6	443.300	590.733 #
25) L5 AR-1248-5	6.837	6.157	3041.4E6	56509491	739.301	390.457m#
31) L7 AR-1260-1	7.363	6.313	2986.5E6	607.1E6	717.182	822.750
32) L7 AR-1260-2	7.615	6.498	4186.0E6	681.5E6	708.352	712.847
33) L7 AR-1260-3	7.974	6.650	2797.5E6	665.0E6	577.896	765.347 #
34) L7 AR-1260-4	8.528	7.354	6359.0E6	1337.0E6	588.847	658.698
35) L7 AR-1260-5	8.859	7.696	3598.9E6	905.5E6	595.987	611.594

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :

ECD_Q

ClientSampleId :

X2C43DL

Manual Integrations

APPROVED

UGO

4/18/2018 10:52:51 AM

UA
04/18/2018