

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ042019\
Data File : PQ039126.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2019 17:50
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 00:47:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ042019.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Apr 20 00:43:12 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	5.708	4.797	68922638	40736912	16.660	16.204
2) SA Decachlor...	12.119	10.565	94538511	53304977	15.985	15.464

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ042019\
Data File : PQ039126.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2019 17:50
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 00:47:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ042019.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Apr 20 00:43:12 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

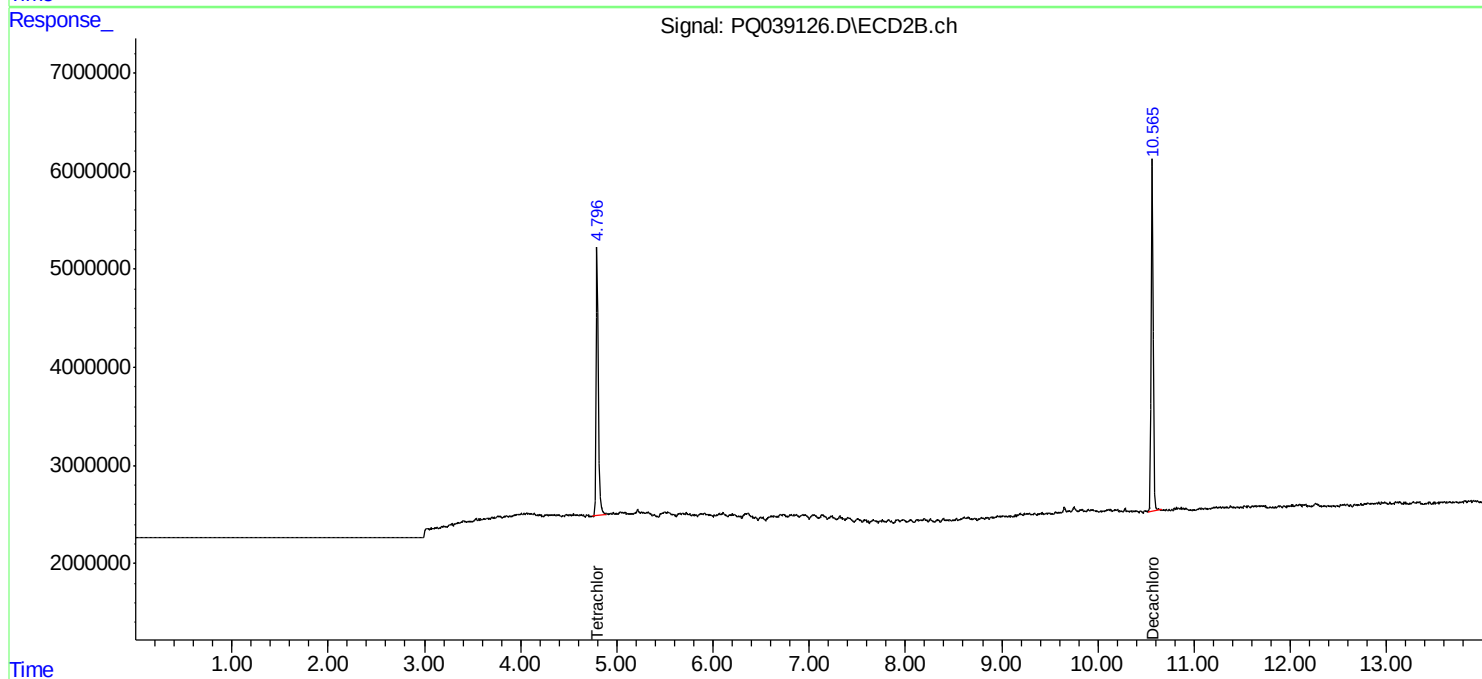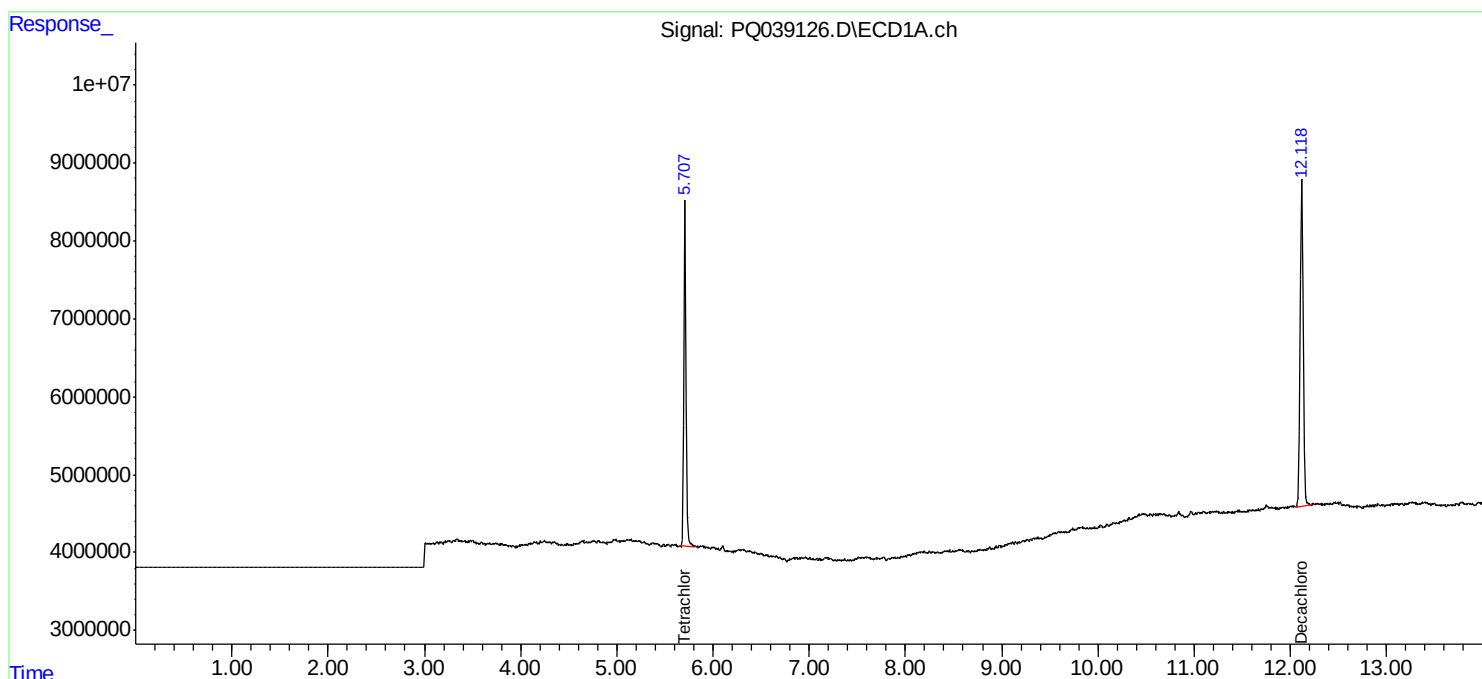


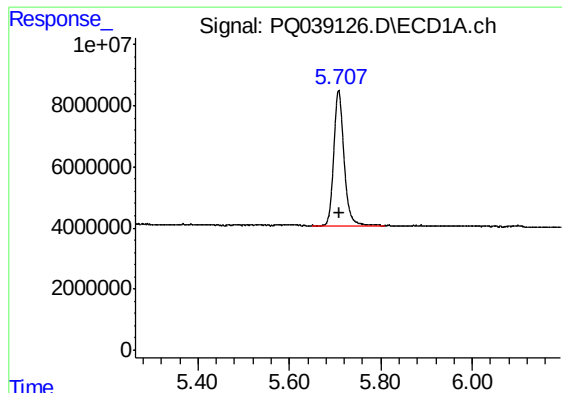

#1 Tetrachloro-m-xylene


R.T.: 5.708 min
Delta R.T.: -0.002 min
Response: 68922638
Conc: 16.66 ng/ml

Instrument :
ECD_Q
ClientSampleId :
I.BLK

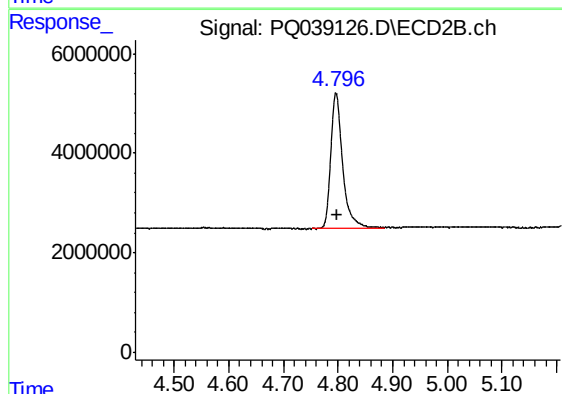


#1 Tetrachloro-m-xylene

R.T.: 4.797 min
Delta R.T.: -0.001 min
Response: 40736912
Conc: 16.20 ng/ml

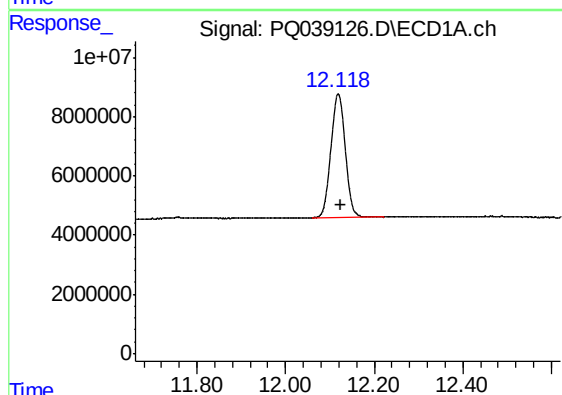

#2 Decachlorobiphenyl

R.T.: 12.119 min
Delta R.T.: -0.006 min
Response: 94538511
Conc: 15.98 ng/ml

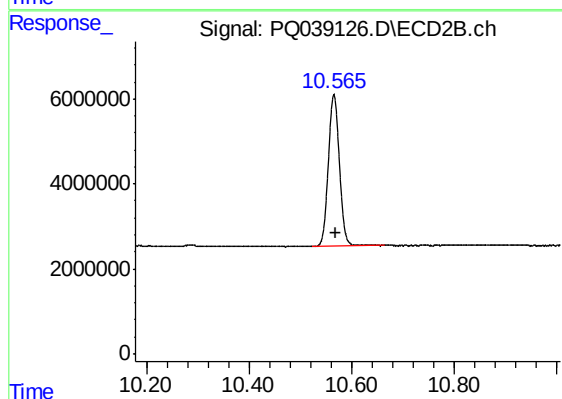

#2 Decachlorobiphenyl

R.T.: 10.565 min
Delta R.T.: -0.003 min
Response: 53304977
Conc: 15.46 ng/ml