

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ042023\
 Data File : PQ061019.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2023 11:16
 Operator : YP\AJ
 Sample : 02404-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 OK-2-041823

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 18:22:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ032723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 27 17:20:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.406	2.762	137.4E6	70576598	17.498	17.956
2) SA Decachlor...	8.586	7.539	78476870	53767716	13.907	11.409

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ042023\
Data File : PQ061019.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2023 11:16
Operator : YP\AJ
Sample : 02404-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
OK-2-041823

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 18:22:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ032723.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 27 17:20:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

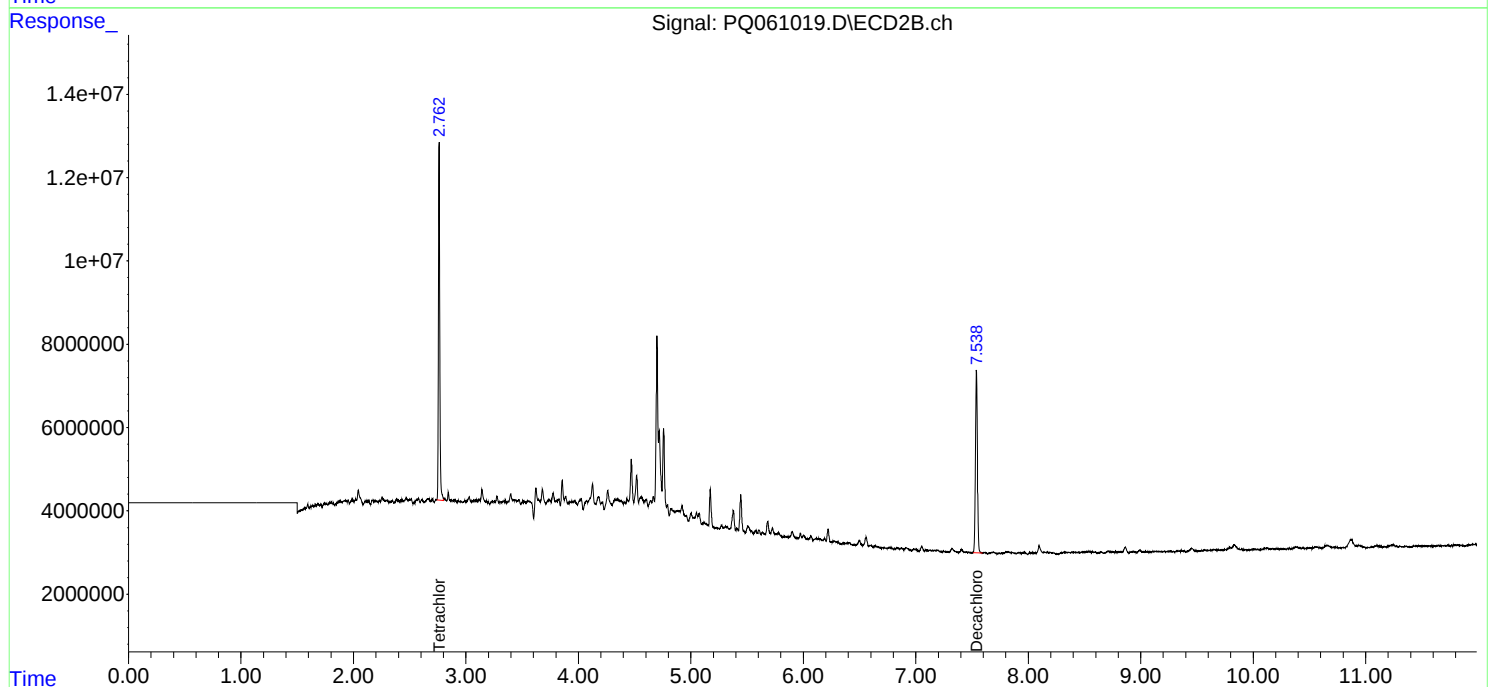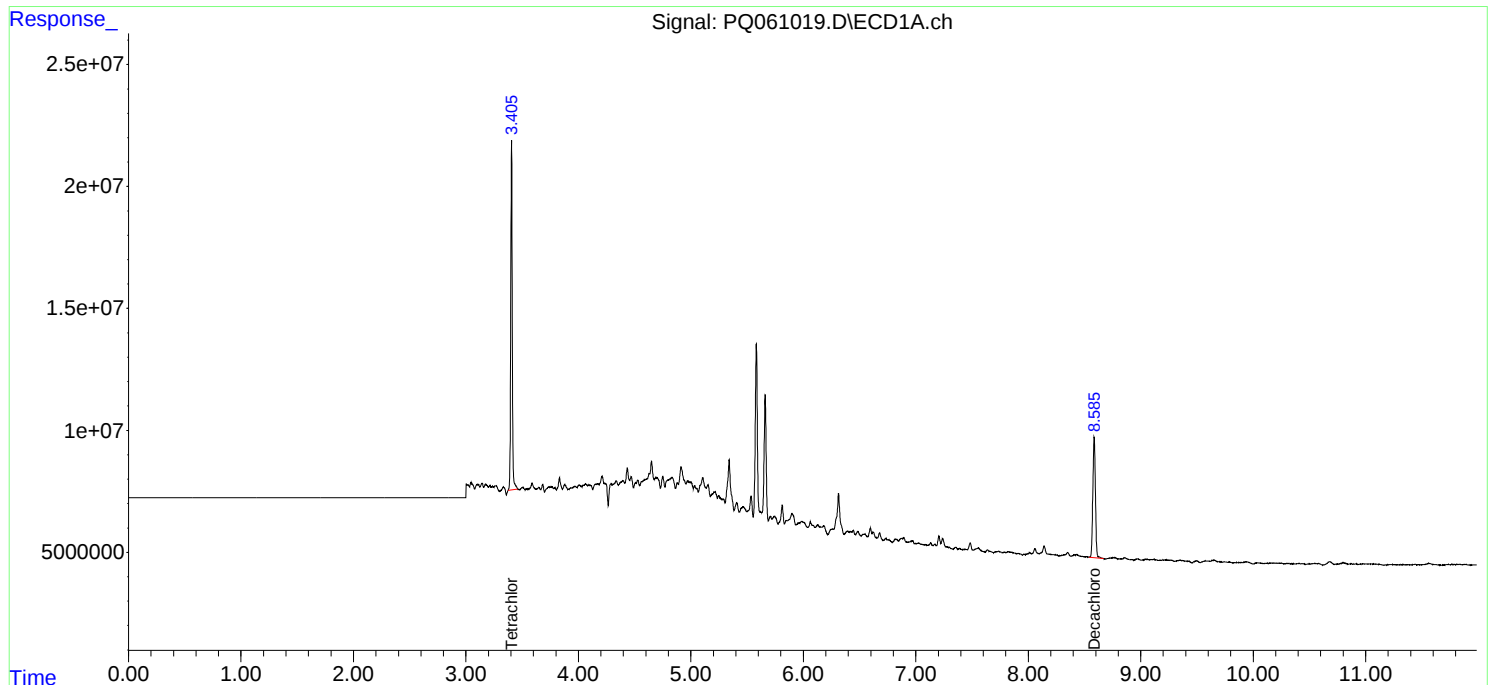


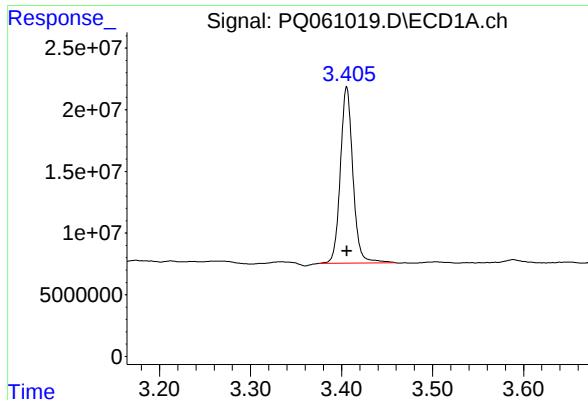

#1 Tetrachloro-m-xylene


R.T.: 3.406 min
Delta R.T.: 0.000 min
Response: 137360791
Conc: 17.50 ng/ml

Instrument :
ECD_Q
ClientSampleId :
OK-2-041823

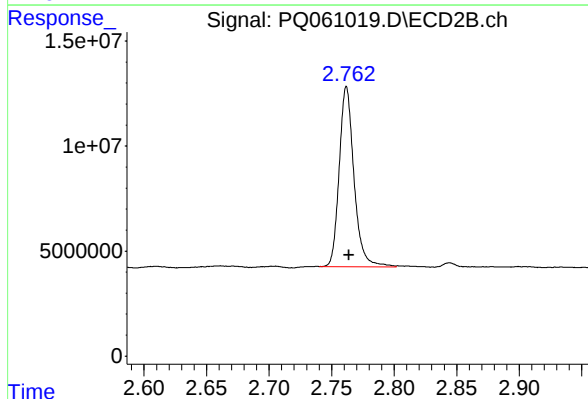


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: -0.002 min
Response: 70576598
Conc: 17.96 ng/ml

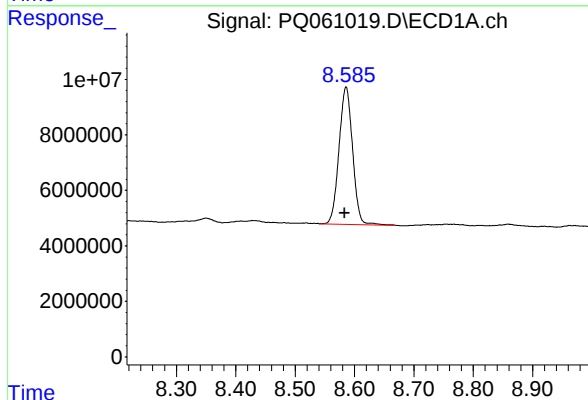

#2 Decachlorobiphenyl

R.T.: 8.586 min
Delta R.T.: 0.002 min
Response: 78476870
Conc: 13.91 ng/ml

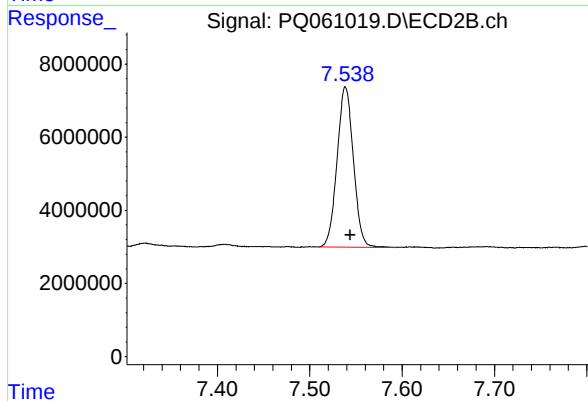

#2 Decachlorobiphenyl

R.T.: 7.539 min
Delta R.T.: -0.005 min
Response: 53767716
Conc: 11.41 ng/ml