

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ042423\
 Data File : PQ061037.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2023 11:11
 Operator : YP\AJ
 Sample : 02469-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 TWP-15

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/25/2023
 Supervised By :Ankita Jodhani 04/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 22:29:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ032723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 27 17:20:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.761	109.7E6	60743948	13.975m	15.454
2) SA Decachlor...	8.585	7.537	75591253	59599233	13.395	12.646

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ042423\
Data File : PQ061037.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2023 11:11
Operator : YP\AJ
Sample : 02469-02
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
TWP-15


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/25/2023
Supervised By :Ankita Jodhani 04/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 22:29:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ032723.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 27 17:20:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

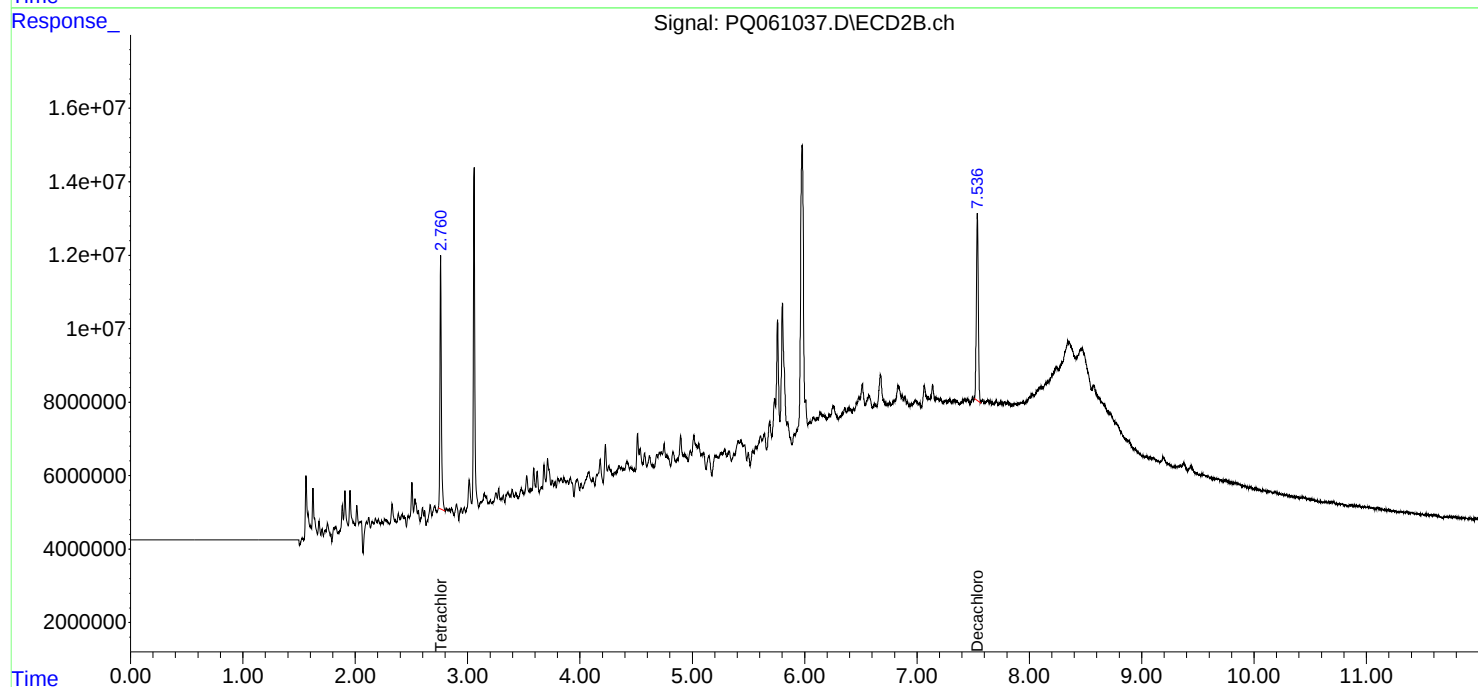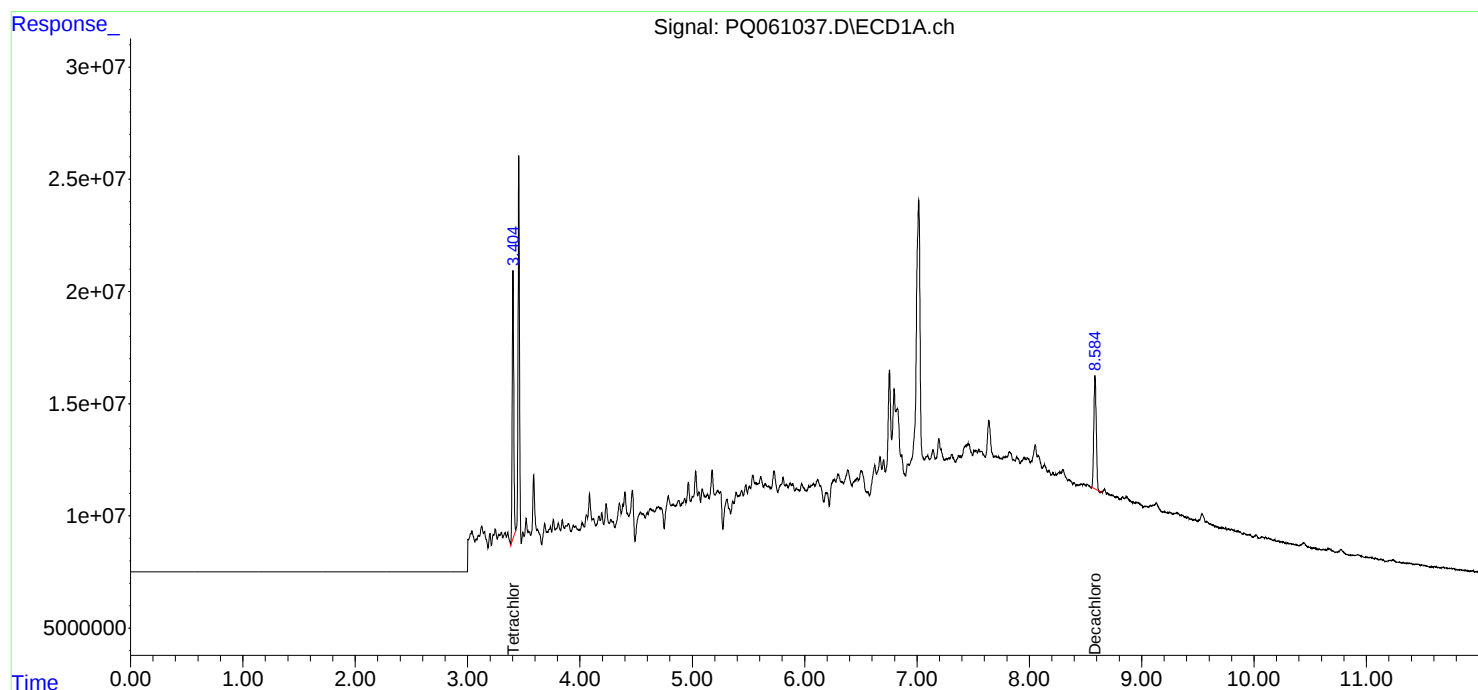

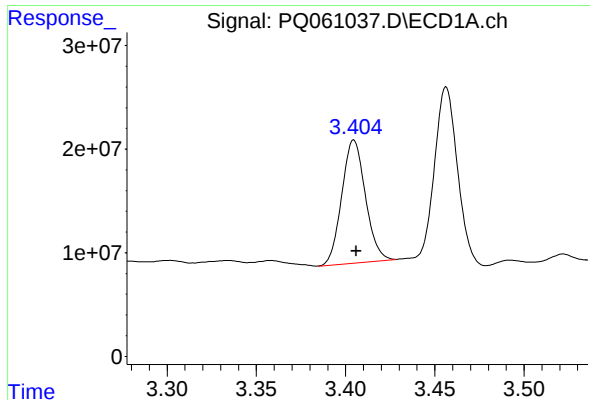


#1 Tetrachloro-m-xylene

R.T.: 3.404 min
Delta R.T.: -0.002 min
Response: 109708951
Conc: 13.98 ng/ml

Instrument :
ECD_Q
ClientSampleId :
TWP-15


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/25/2023
Supervised By :Ankita Jodhani 04/25/2023

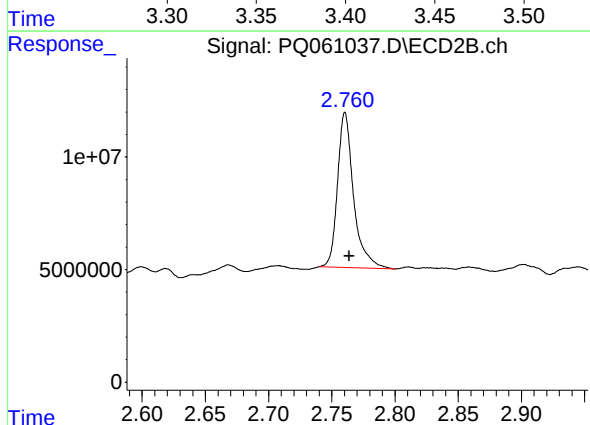


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: -0.003 min
Response: 60743948
Conc: 15.45 ng/ml

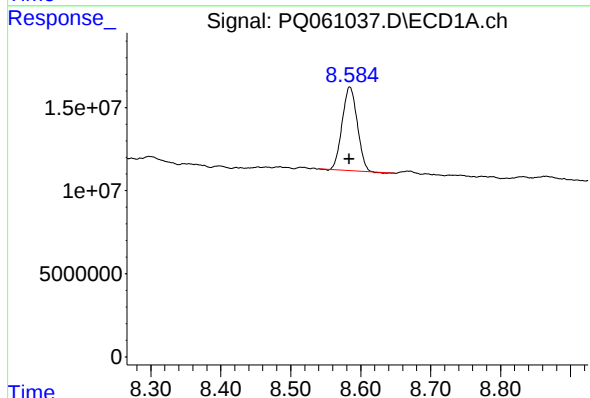

#2 Decachlorobiphenyl

R.T.: 8.585 min
Delta R.T.: 0.000 min
Response: 75591253
Conc: 13.40 ng/ml

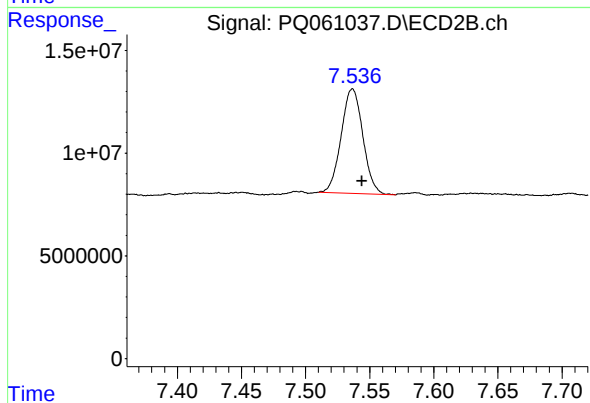

#2 Decachlorobiphenyl

R.T.: 7.537 min
Delta R.T.: -0.008 min
Response: 59599233
Conc: 12.65 ng/ml