

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ042423\
 Data File : PQ061043.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2023 12:38
 Operator : YP\AJ
 Sample : 02469-03RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 TWP-24RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/25/2023
 Supervised By :Ankita Jodhani 04/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 22:38:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ032723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 27 17:20:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.404	2.761	103.2E6	58055004	13.142m	14.770
2) SA Decachlor...	8.585	7.537	31941865	26063072	5.660	5.530

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ042423\
Data File : PQ061043.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2023 12:38
Operator : YP\AJ
Sample : 02469-03RE
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
TWP-24RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/25/2023
Supervised By :Ankita Jodhani 04/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 22:38:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ032723.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 27 17:20:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

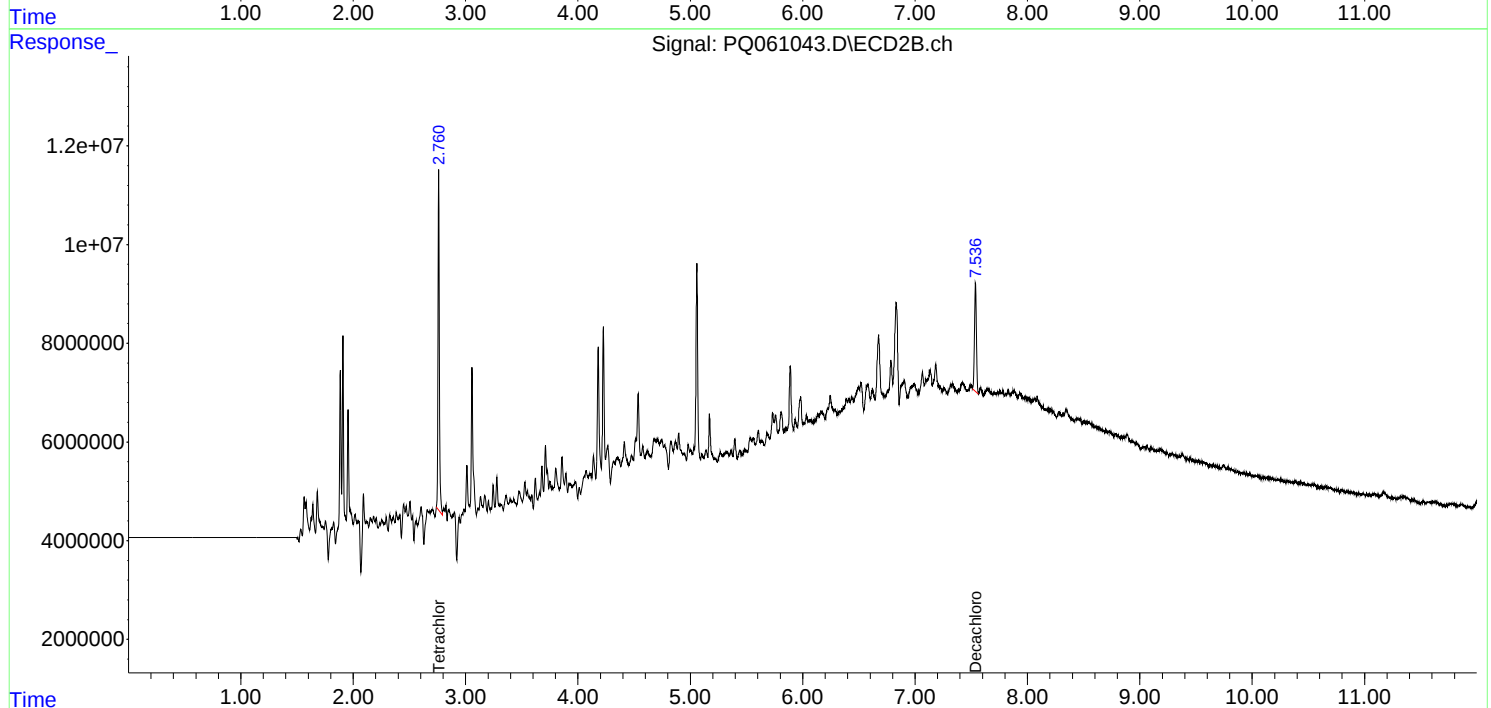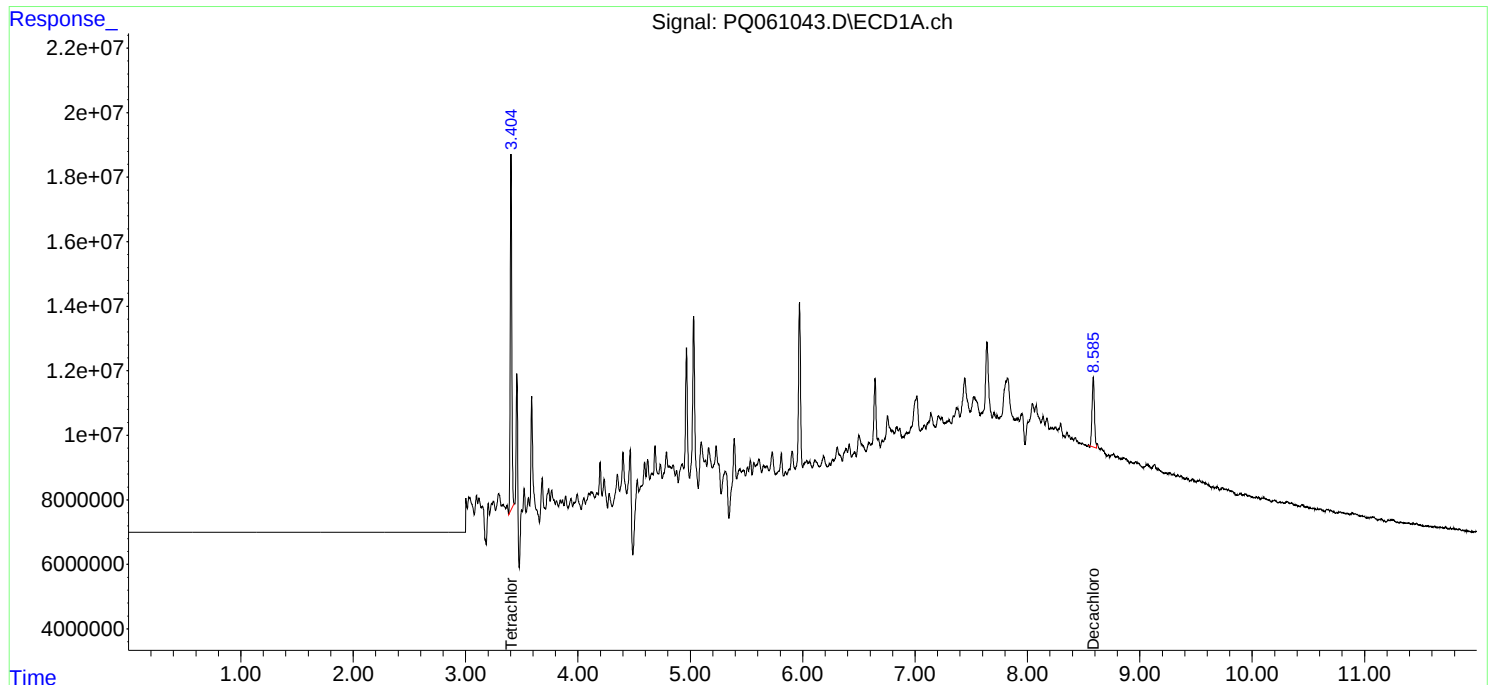

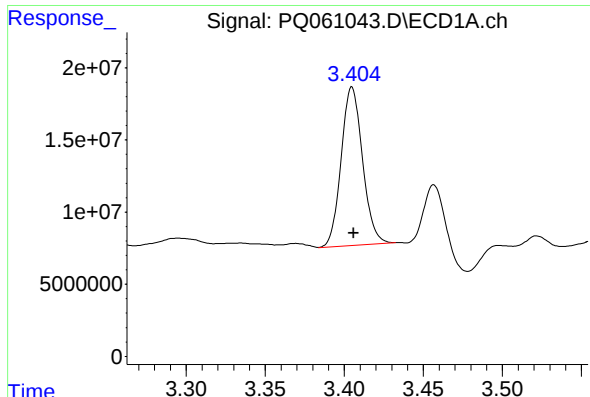


#1 Tetrachloro-m-xylene

R.T.: 3.404 min
Delta R.T.: -0.002 min
Response: 103164950
Conc: 13.14 ng/ml

Instrument :
ECD_Q
ClientSampleId :
TWP-24RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/25/2023
Supervised By :Ankita Jodhani 04/25/2023

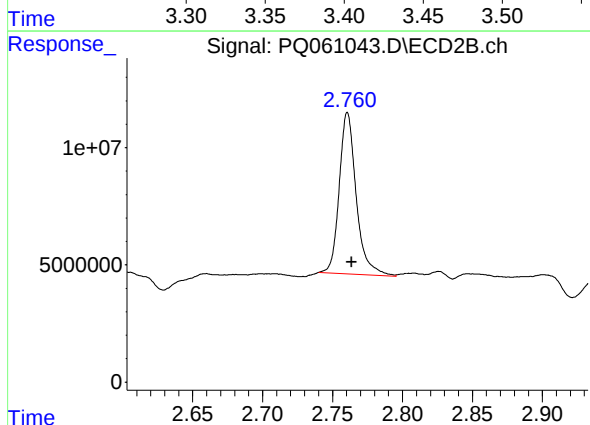


#1 Tetrachloro-m-xylene

R.T.: 2.761 min
Delta R.T.: -0.003 min
Response: 58055004
Conc: 14.77 ng/ml

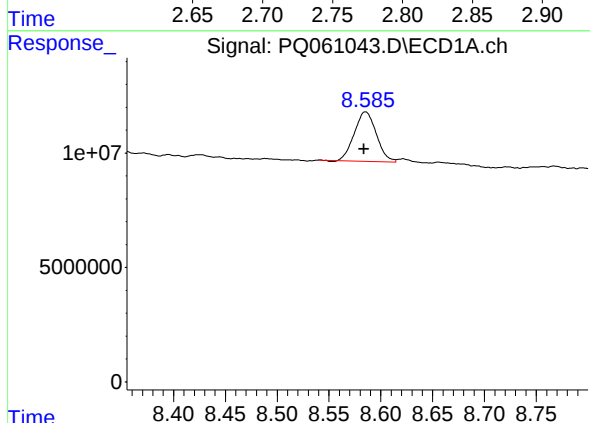

#2 Decachlorobiphenyl

R.T.: 8.585 min
Delta R.T.: 0.002 min
Response: 31941865
Conc: 5.66 ng/ml

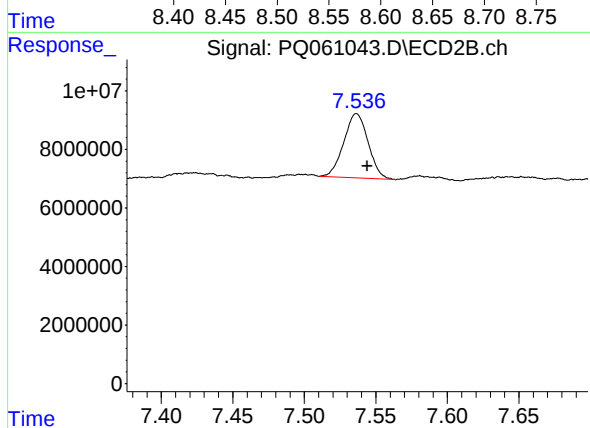

#2 Decachlorobiphenyl

R.T.: 7.537 min
Delta R.T.: -0.008 min
Response: 26063072
Conc: 5.53 ng/ml