

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ050624\
 Data File : PQ066370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 May 2024 13:16
 Operator : YP\AJ
 Sample : P2347-01RE 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 392

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/07/2024
 Supervised By :Ankita Jodhani 05/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 06 15:27:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ042324.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 24 04:24:21 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.439	2.732	1881410	2580533	0.433m	0.403
2) SA Decachlor...	8.646	7.496	1650548	3968029	0.671	0.631m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ050624\
Data File : PQ066370.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 May 2024 13:16
Operator : YP\AJ
Sample : P2347-01RE 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
392


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/07/2024
Supervised By :Ankita Jodhani 05/07/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 06 15:27:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ042324.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 24 04:24:21 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

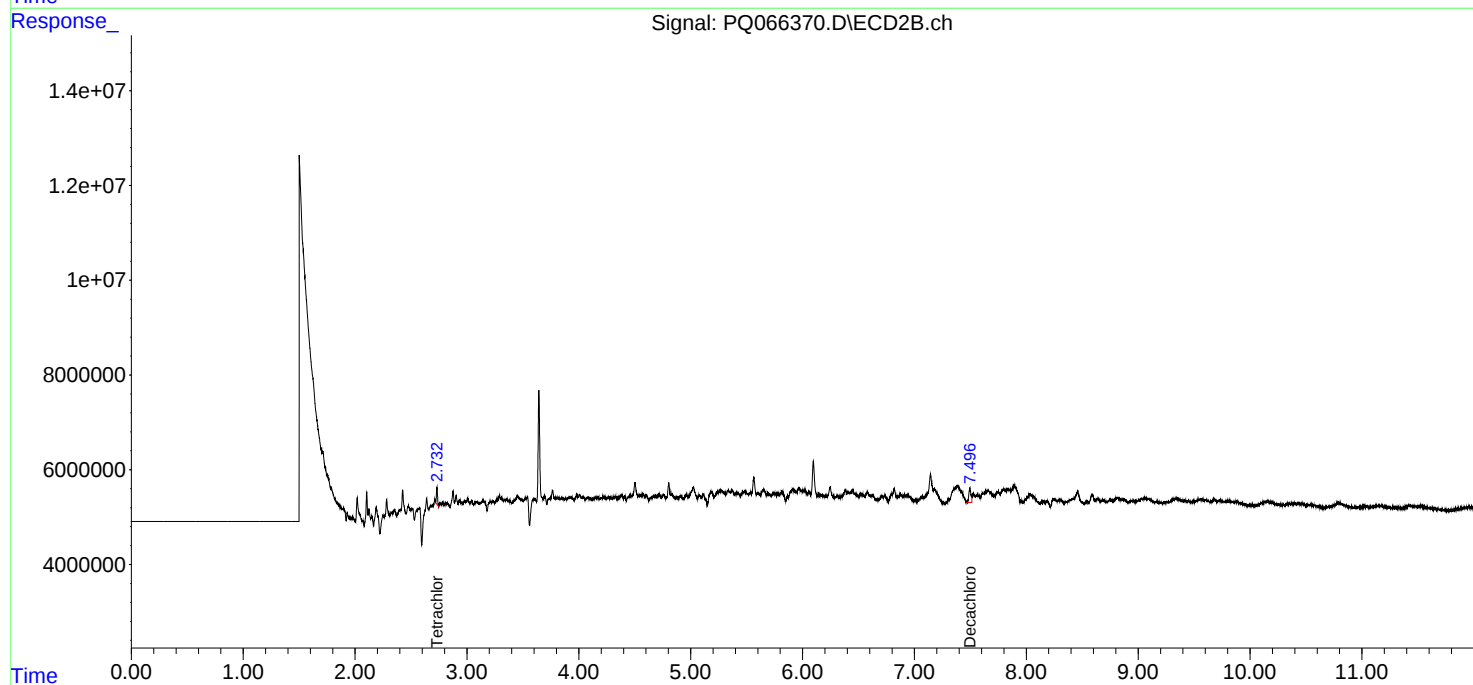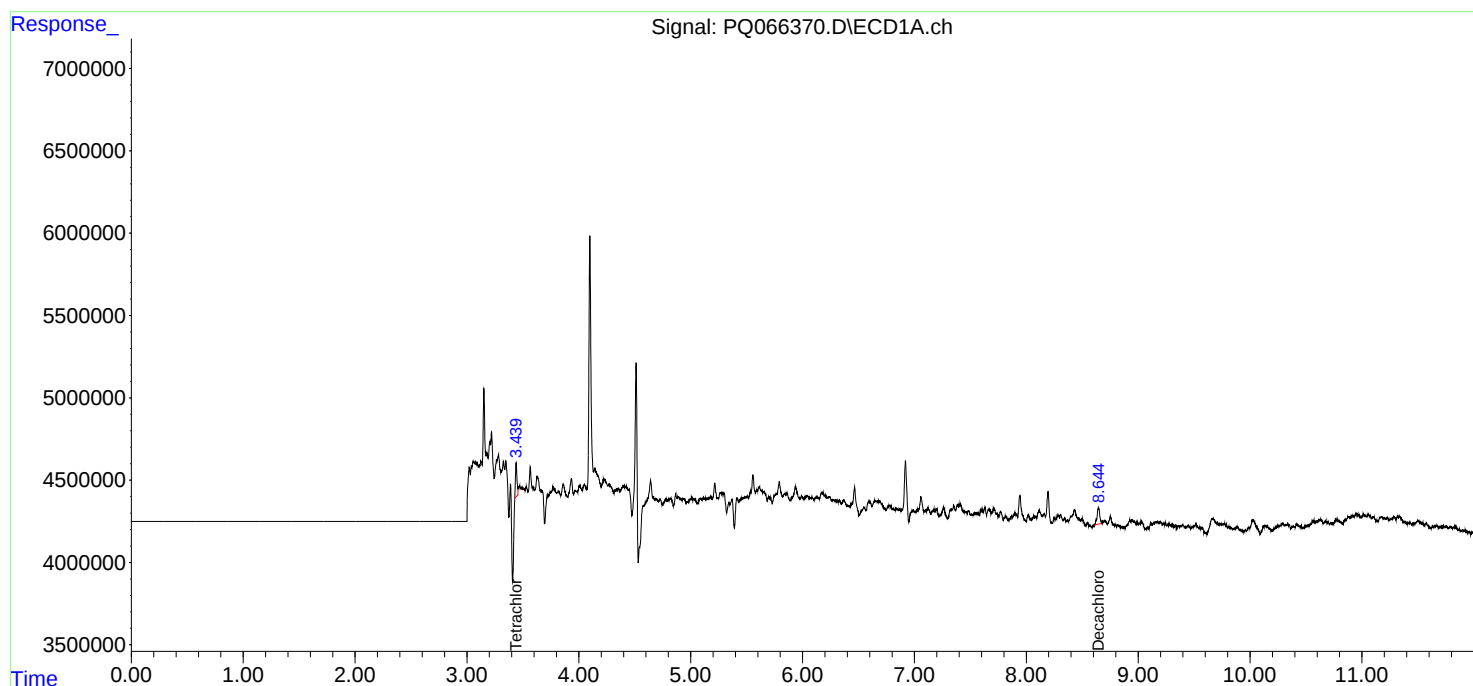

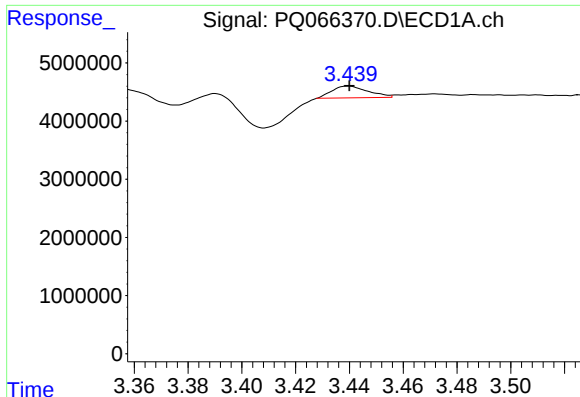


#1 Tetrachloro-m-xylene

R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 1881410
Conc: 0.43 ng/ml

Instrument :
ECD_Q
ClientSampleId :
392


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/07/2024
Supervised By :Ankita Jodhani 05/07/2024

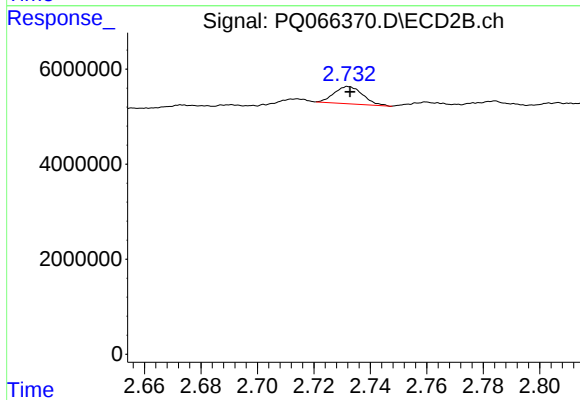


#1 Tetrachloro-m-xylene

R.T.: 2.732 min
Delta R.T.: 0.000 min
Response: 2580533
Conc: 0.40 ng/ml

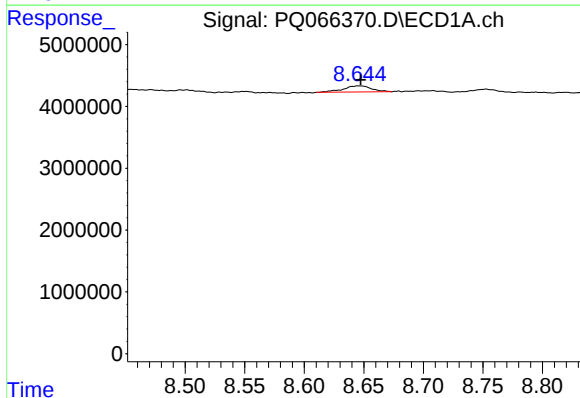

#2 Decachlorobiphenyl

R.T.: 8.646 min
Delta R.T.: -0.001 min
Response: 1650548
Conc: 0.67 ng/ml

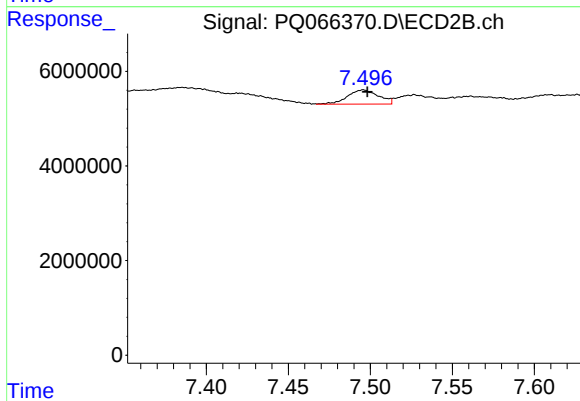

#2 Decachlorobiphenyl

R.T.: 7.496 min
Delta R.T.: -0.003 min
Response: 3968029
Conc: 0.63 ng/ml m