

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ051821\
 Data File : PQ053575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2021 13:36
 Operator : DD\AJ
 Sample : M2421-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 K328-DUP2

Manual Integrations
 APPROVED

Ankita
 5/20/2021 2:02:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 15:42:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ051321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 14 03:47:40 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.221	4.236	532.8E6	285.6E6	18.456	22.165
2) SA Decachlor...	11.407	9.573	399.0E6	192.4E6	13.359m	13.548m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ051821\
Data File : PQ053575.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2021 13:36
Operator : DD\AJ
Sample : M2421-13
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
K328-DUP2


Manual Integrations
APPROVED

Ankita
5/20/2021 2:02:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 15:42:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ051321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 14 03:47:40 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

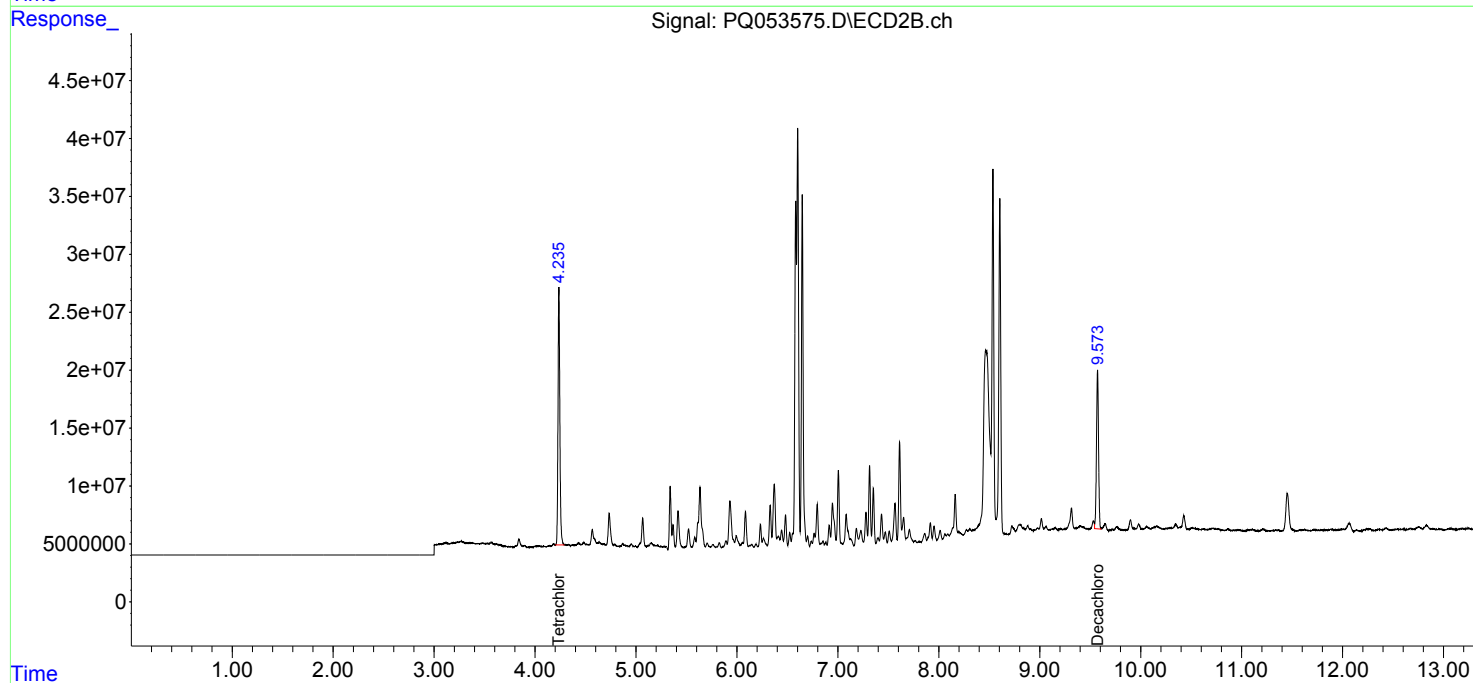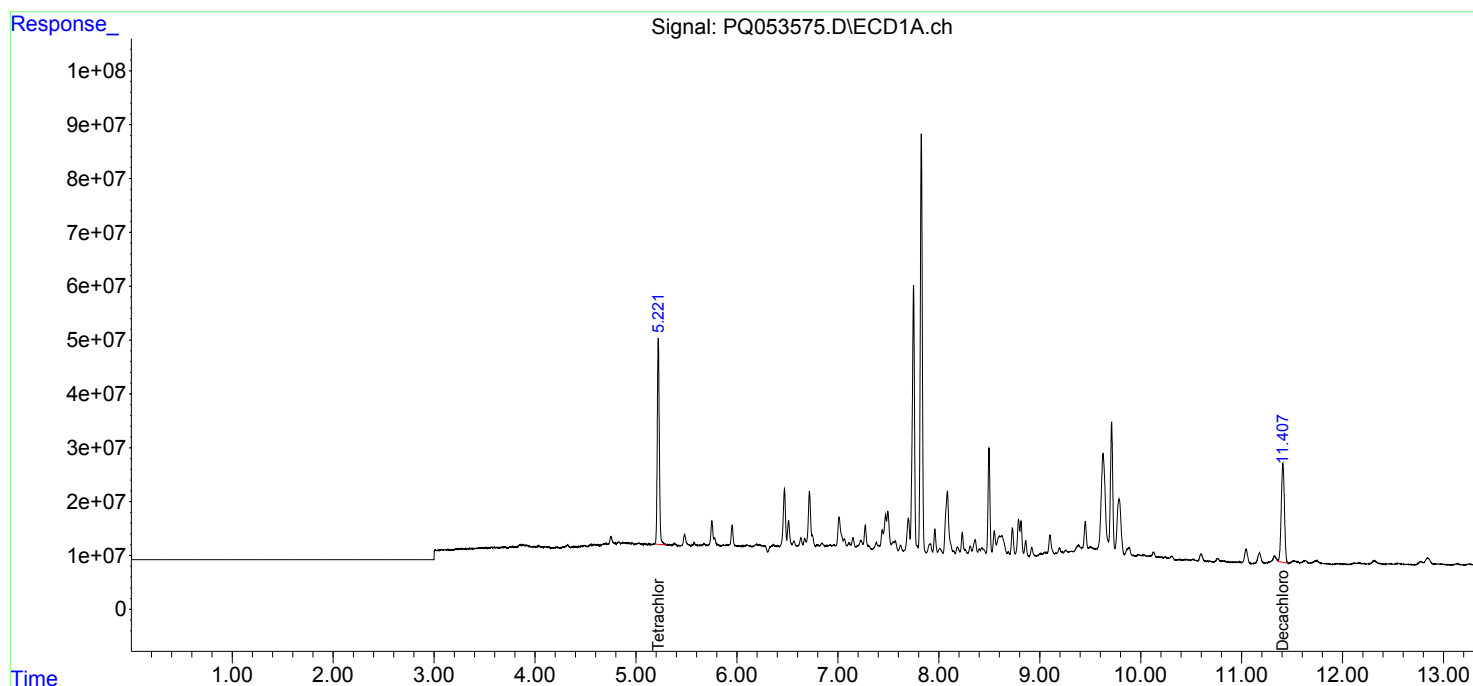

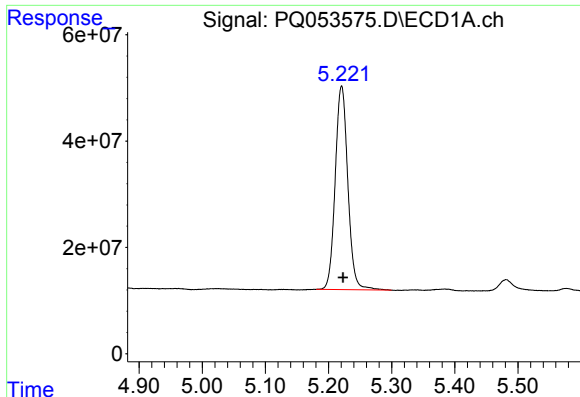


#1 Tetrachloro-m-xylene

R.T.: 5.221 min
Delta R.T.: -0.002 min
Response: 532839644
Conc: 18.46 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K328-DUP2


Manual Integrations
APPROVED

Ankita
5/20/2021 2:02:18 PM

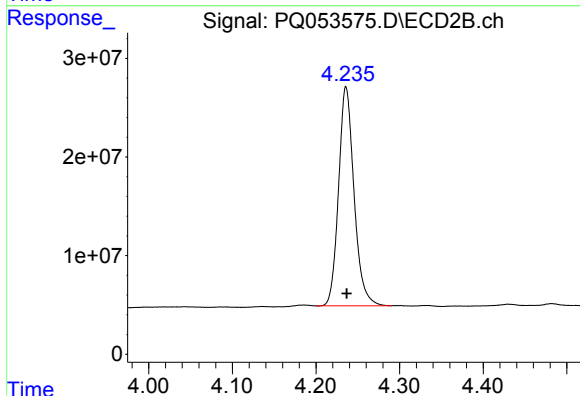


#1 Tetrachloro-m-xylene

R.T.: 4.236 min
Delta R.T.: -0.001 min
Response: 285586701
Conc: 22.16 ng/ml

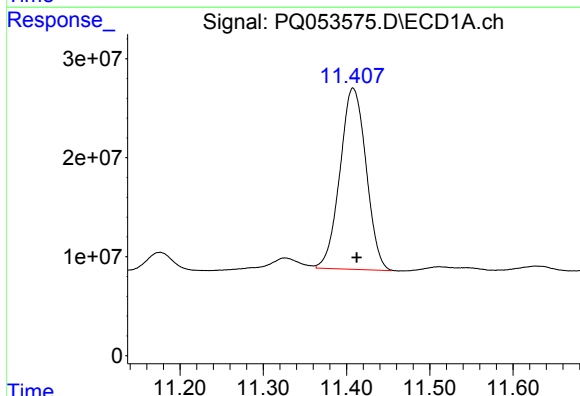

#2 Decachlorobiphenyl

R.T.: 11.407 min
Delta R.T.: -0.005 min
Response: 399001368
Conc: 13.36 ng/ml m

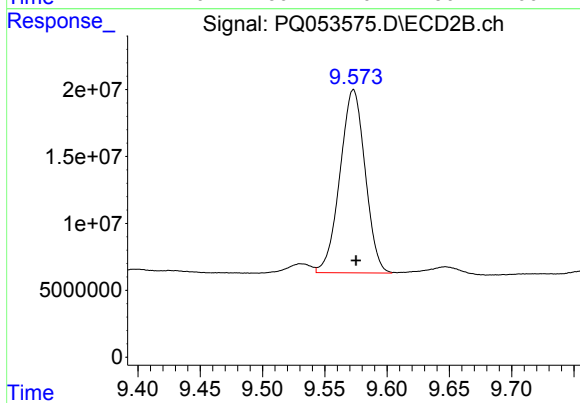

#2 Decachlorobiphenyl

R.T.: 9.573 min
Delta R.T.: -0.002 min
Response: 192355918
Conc: 13.55 ng/ml m