

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ051821\
 Data File : PQ053578.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2021 14:25
 Operator : DD\AJ
 Sample : M2422-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 K328-10A

Manual Integrations
 APPROVED

Ankita
 5/20/2021 2:02:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 16:58:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ051321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 14 03:47:40 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.220	4.237	516.9E6	264.9E6	17.905	20.555
2) SA Decachlor...	11.408	9.573	361.8E6	165.9E6	12.115m	11.684m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ051821\
Data File : PQ053578.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2021 14:25
Operator : DD\AJ
Sample : M2422-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampled :
K328-10A


Manual Integrations
APPROVED

Ankita
5/20/2021 2:02:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 16:58:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ051321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 14 03:47:40 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

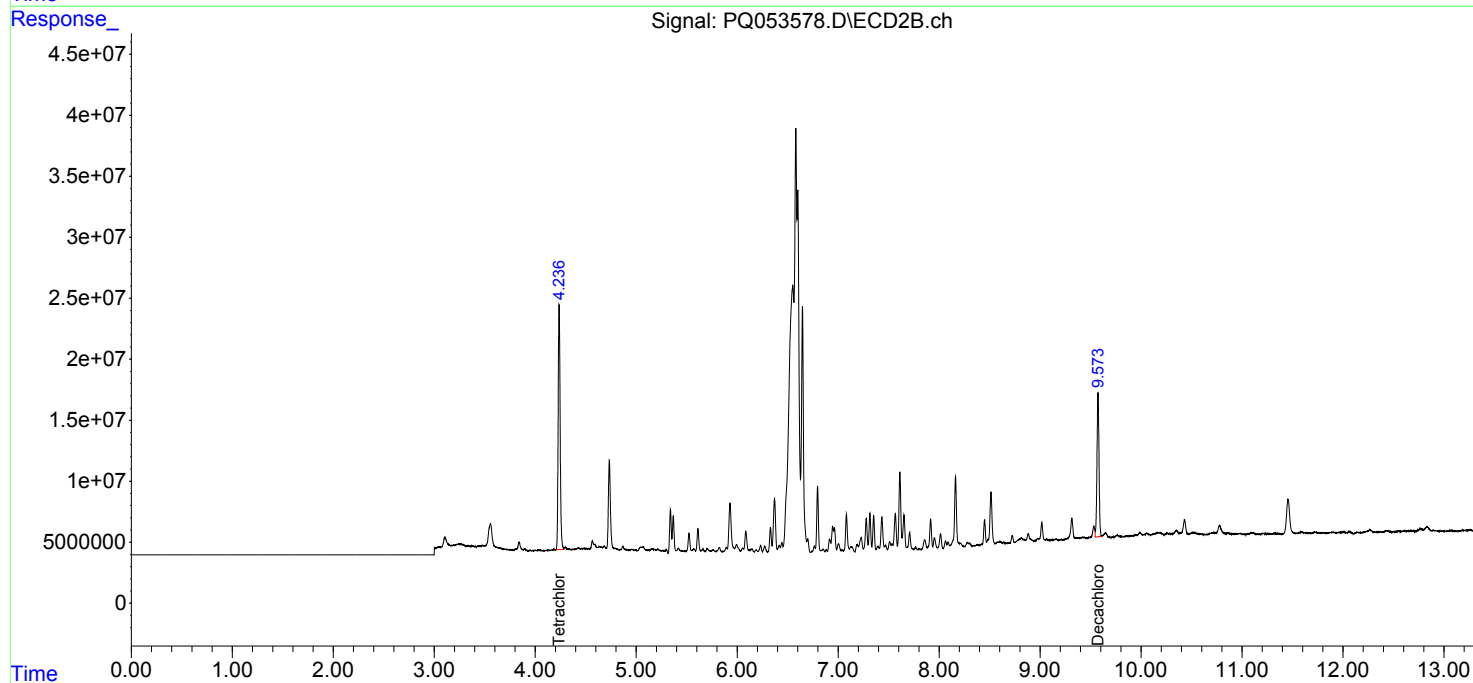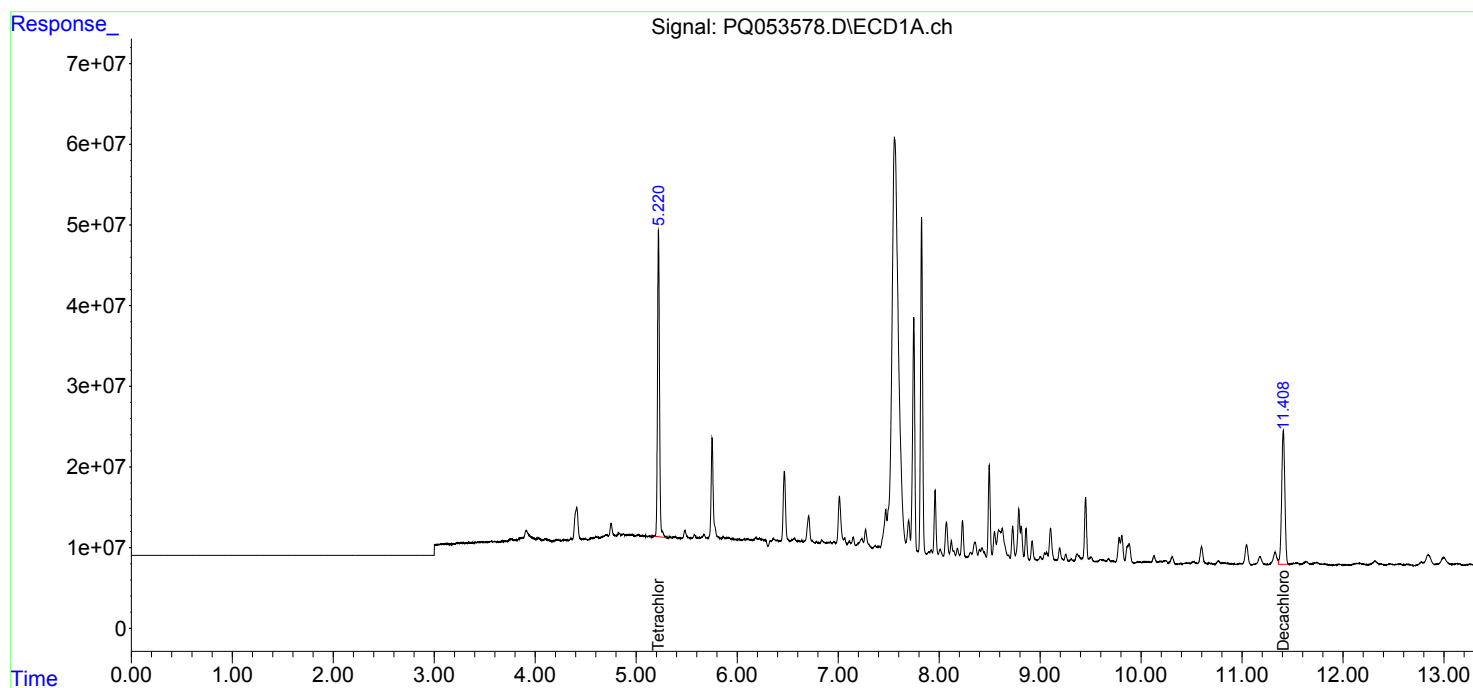

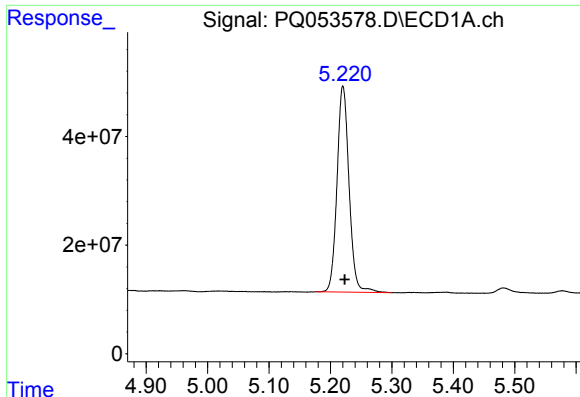


#1 Tetrachloro-m-xylene

R.T.: 5.220 min
Delta R.T.: -0.003 min
Response: 516922966
Conc: 17.91 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K328-10A


Manual Integrations
APPROVED

Ankita
5/20/2021 2:02:00 PM

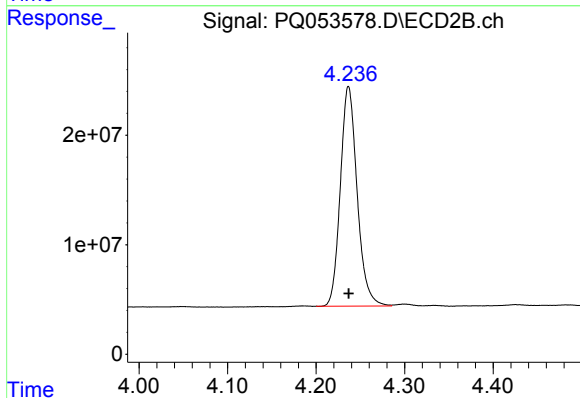


#1 Tetrachloro-m-xylene

R.T.: 4.237 min
Delta R.T.: 0.000 min
Response: 264853604
Conc: 20.56 ng/ml

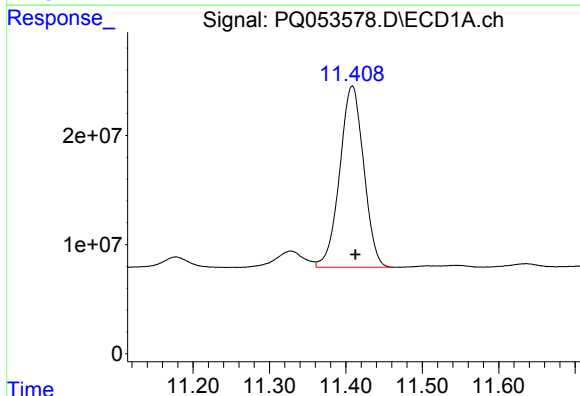

#2 Decachlorobiphenyl

R.T.: 11.408 min
Delta R.T.: -0.004 min
Response: 361833910
Conc: 12.11 ng/ml m

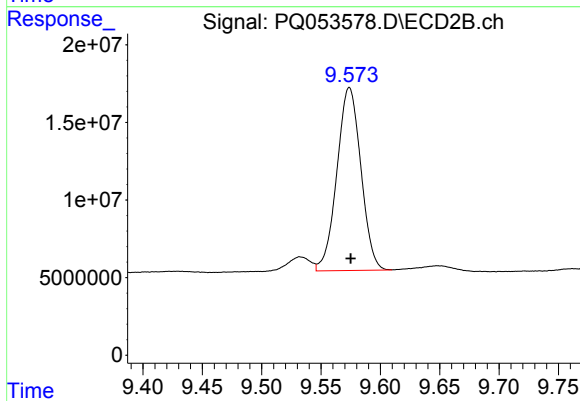

#2 Decachlorobiphenyl

R.T.: 9.573 min
Delta R.T.: -0.001 min
Response: 165884858
Conc: 11.68 ng/ml m