

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ051919\
Data File : PQ039963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2019 00:08
Operator : SM\AJ
Sample : K2917-04
Misc :
ALS Vial : 45 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
ETMD1

Manual Integrations
APPROVED

Ankita
5/20/2019 2:00:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 05:09:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ051819CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 18 00:58:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

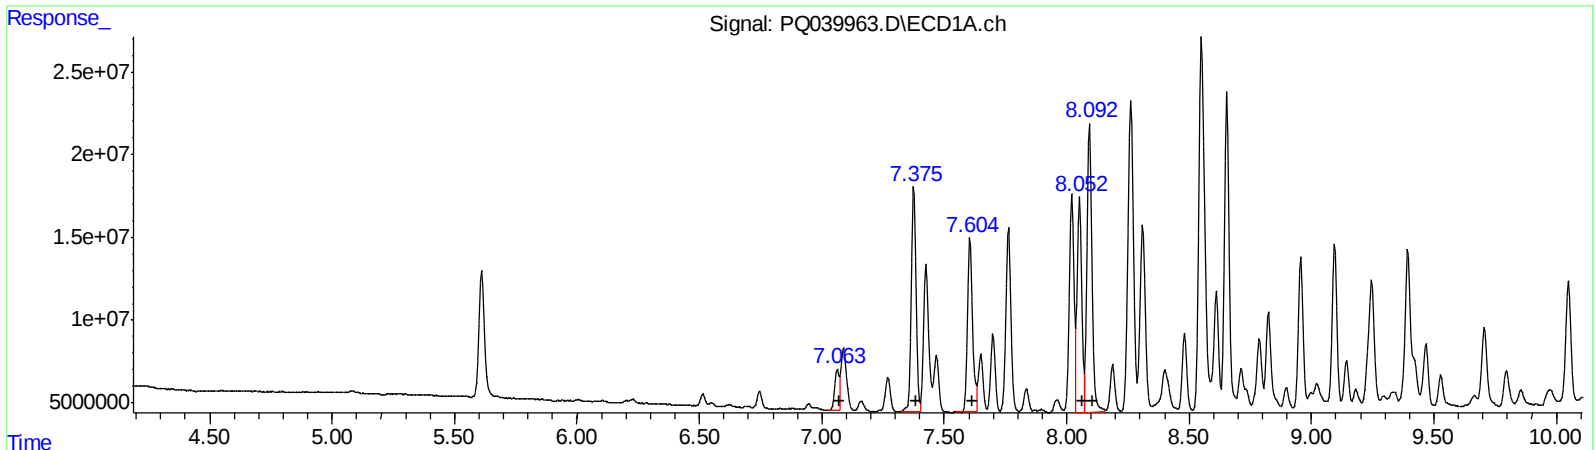

(21) AR-1248-1 (L5)
R.T. Response Conc
7.06 30531667 235.10
7.38 183692101 1118.82
7.60 149821657 771.90
8.05 169989564 787.63
8.09 249770992 1198.22

(21) AR-1248-1 #2 (L5)
R.T. Response Conc
6.20 57276422 566.82
6.47 144034994 1137.48
6.52 106699696 804.47
6.72 122993124 750.72
7.18 181225735 1118.41

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ051919\
Data File : PQ039963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2019 00:08
Operator : SM\AJ
Sample : K2917-04
Misc :
ALS Vial : 45 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
ETMD1

Manual Integrations
APPROVED

Ankita
5/20/2019 2:00:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 05:09:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ051819CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 18 00:58:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

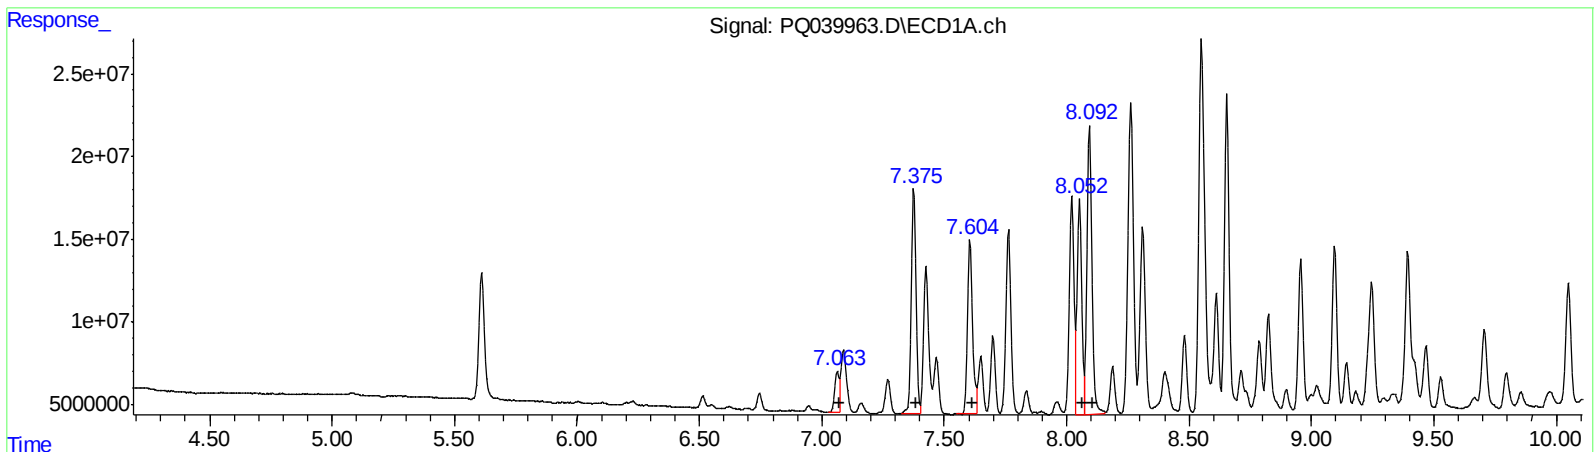

(21) AR-1248-1 (L5)
R.T. Response Conc
7.06 30531667 235.10
7.38 183692101 1118.82
7.60 149821657 771.90
8.05 169989564 787.63
8.09 249770992 1198.22

(21) AR-1248-1 #2 (L5)
R.T. Response Conc
6.18 22040075 218.11
6.47 144034994 1137.48
6.52 106699696 804.47
6.72 122993124 750.72
7.18 181225735 1118.41

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ051919\
Data File : PQ039963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2019 00:08
Operator : SM\AJ
Sample : K2917-04
Misc :
ALS Vial : 45 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
ETMD1

Manual Integrations
APPROVED

Ankita
5/20/2019 2:00:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 05:09:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ051819CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 18 00:58:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

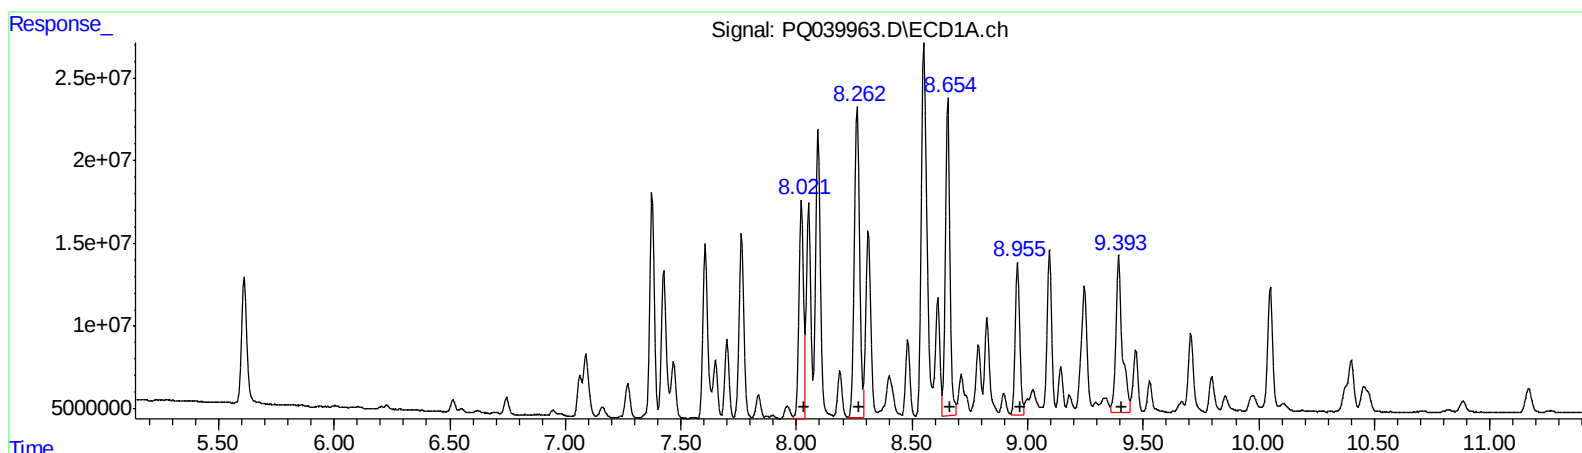

(26) AR-1254-1 (L6)
R.T. Response Conc
8.02 176810322 765.93
8.26 296783762 823.53
8.65 258063266 679.76
8.96 125575906 460.09
9.39 180209283 599.66

(26) AR-1254-1 #2 (L6)
R.T. Response Conc
7.13 227990391 860.83
7.30 126760311 555.28
7.75 250175464 677.08
8.00 104625858 455.85
8.44 137294939 440.98

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ051919\
Data File : PQ039963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2019 00:08
Operator : SM\AJ
Sample : K2917-04
Misc :
ALS Vial : 45 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
ETMD1

Manual Integrations
APPROVED

Ankita
5/20/2019 2:00:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 05:09:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ051819CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 18 00:58:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

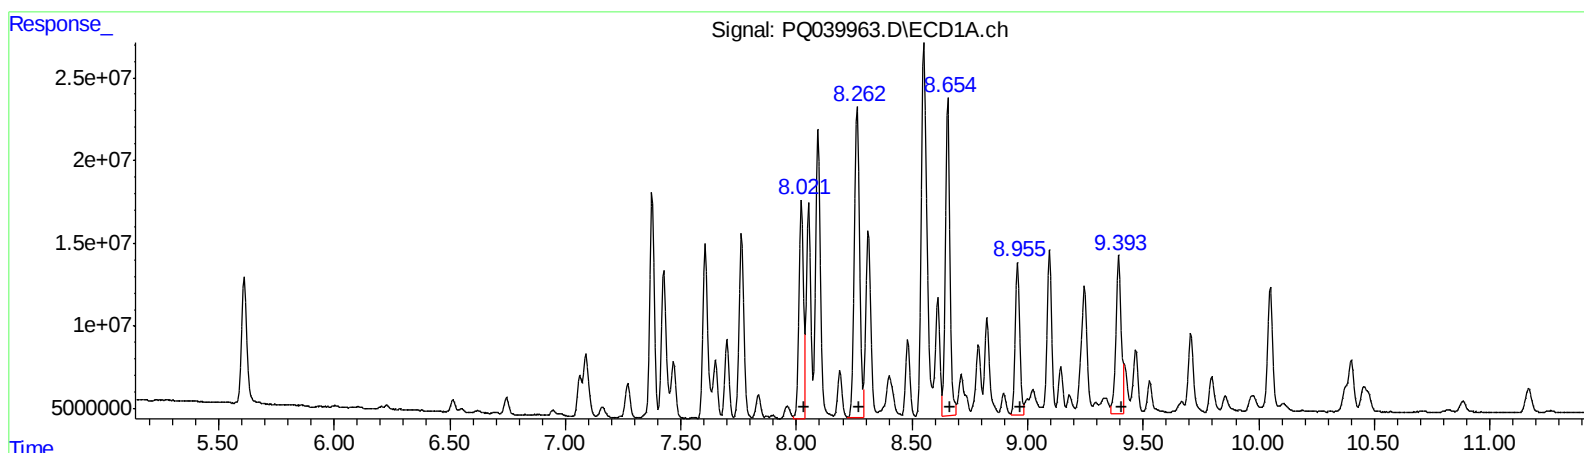

(26) AR-1254-1 #2 (L6)
R.T. Response Conc
8.02 176810322 765.93
8.26 296783762 823.53
8.65 258063266 679.76
8.96 125575906 460.09
9.39 148093098 492.79
(26) AR-1254-1 #2 (L6)
R.T. Response Conc
7.13 227990391 860.83
7.30 126760311 555.28
7.75 250175464 677.08
8.00 104625858 455.85
8.44 137294939 440.98

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ051919\
 Data File : PQ039963.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2019 00:08
 Operator : SM\AJ
 Sample : K2917-04
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 ETMD1

Manual Integrations
 APPROVED

Ankita
 5/20/2019 2:00:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 05:09:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ051819CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 18 00:58:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.610	4.731	118.3E6	84217249	17.547	17.534
2) SA Decachlor...	11.944	10.465	117.2E6	69444004	18.773	17.987
Target Compounds						
21) L5 AR-1248-1	7.063	6.182	30531667	22040075	235.104	218.113m
22) L5 AR-1248-2	7.375	6.472	183.7E6	144.0E6	1118.818	1137.480
23) L5 AR-1248-3	7.605	6.520	149.8E6	106.7E6	771.899	804.469
24) L5 AR-1248-4	8.052	6.725	170.0E6	123.0E6	787.634	750.723
25) L5 AR-1248-5	8.093	7.181	249.8E6	181.2E6	1198.221	1118.409
26) L6 AR-1254-1	8.021	7.134	176.8E6	228.0E6	765.928	860.833
27) L6 AR-1254-2	8.262	7.301	296.8E6	126.8E6	823.529	555.275 #
28) L6 AR-1254-3	8.654	7.748	258.1E6	250.2E6	679.759	677.079
29) L6 AR-1254-4	8.956	7.999	125.6E6	104.6E6	460.091	455.852
30) L6 AR-1254-5	9.393	8.442	148.1E6	137.3E6	492.789m	440.978

AJ
 05/21/19

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.