

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ052521\
Data File : PQ053661.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2021 20:36
Operator : DD\AJ
Sample : M2511-03
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
C0CL4

Manual Integrations
APPROVED

Ankita
5/27/2021 11:32:19 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 06:05:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052021CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 20 06:23:48 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

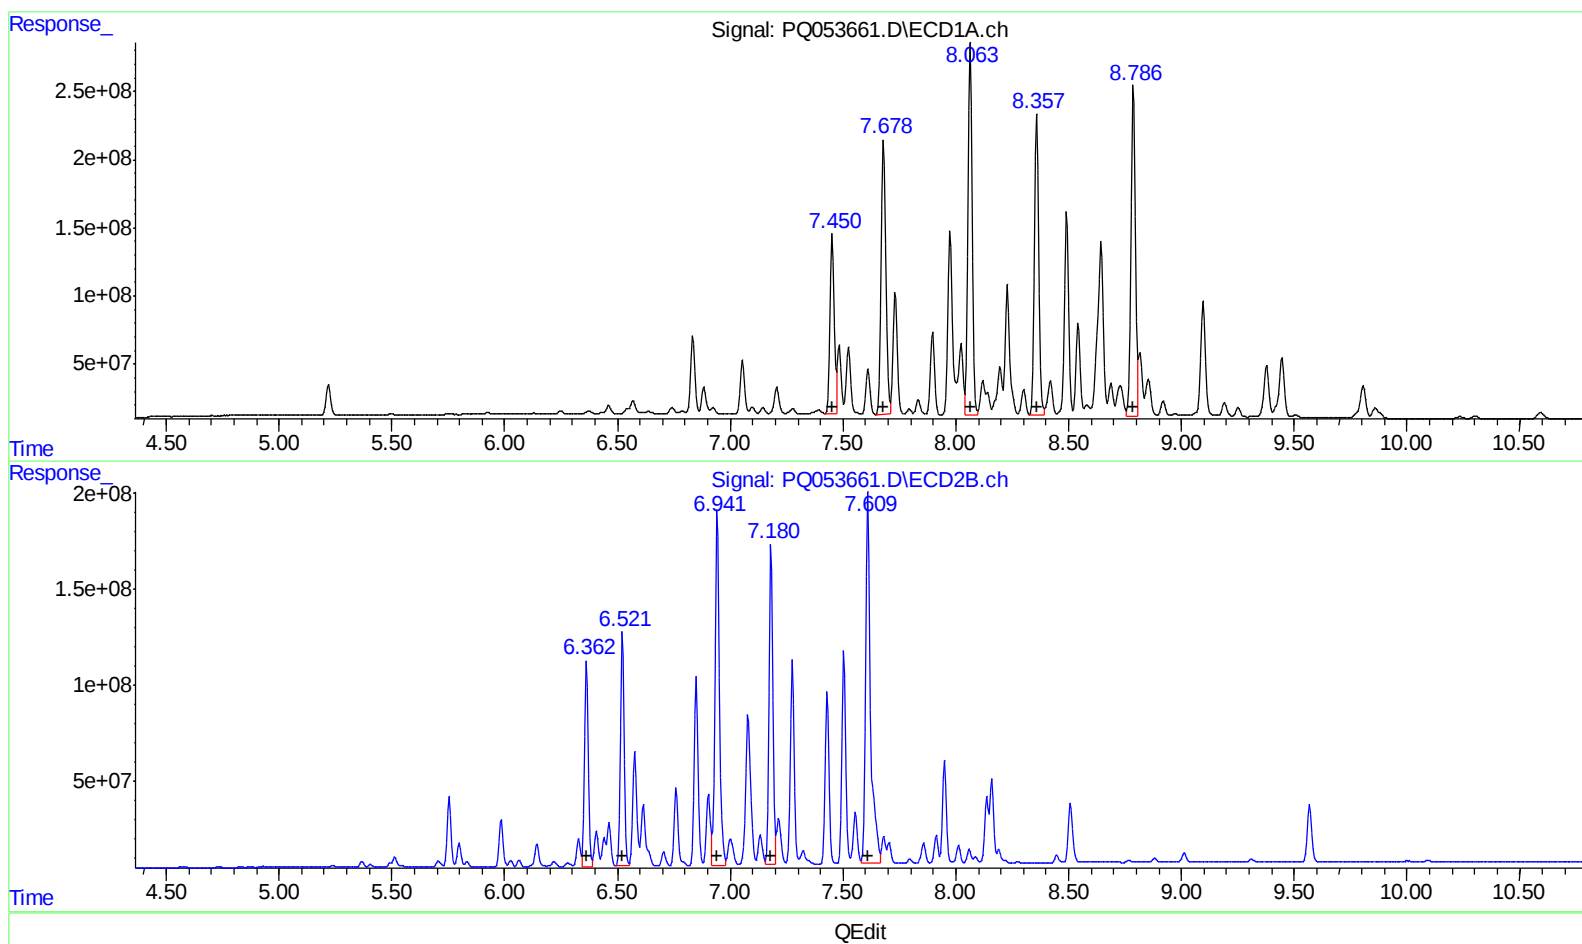

(26) AR-1254-1 #2 (L6)
R.T. Response Conc
7.45 1719367090 1209.65
7.68 2946951763 1309.97
8.06 3587445452 1513.75
8.36 2995010587 1626.32
8.79 3285071928 1817.90

(26) AR-1254-1 #2 (L6)
R.T. Response Conc
6.36 1251263934 1106.47
6.52 1398130898 1374.35
6.94 2428631542 1451.20
7.18 1940398116 1696.91
7.61 2912849048 1798.00

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ052521\
 Data File : PQ053661.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2021 20:36
 Operator : DD\AJ
 Sample : M2511-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 C0CL4

Manual Integrations
 APPROVED

Ankita
 5/27/2021 11:32:19 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 06:05:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052021CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 20 06:23:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	5.218	4.234	319.6E6	168.8E6	14.093	15.675
2) SA Decachlor...	11.399	9.568	676.3E6	395.2E6	30.044	35.791

Target Compounds

26) L6 AR-1254-1	7.451	6.362	1719.4E6	1251.3E6	1209.647	1106.465
27) L6 AR-1254-2	7.678	6.522	2947.0E6	1398.1E6	1309.969	1374.348
28) L6 AR-1254-3	8.063	6.942	3587.4E6	2428.6E6	1513.750	1451.199
29) L6 AR-1254-4	8.358	7.180	2995.0E6	1940.4E6	1626.324	1696.906
30) L6 AR-1254-5	8.786	7.609	3285.1E6	2912.8E6	1817.900m	1797.997

AJ
 05/28/21

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.