

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ053023\
 Data File : PQ061320.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 May 2023 14:22
 Operator : YP\AJ
 Sample : 02955-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 SB25

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/31/2023
 Supervised By :Ankita Jodhani 05/31/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 30 20:49:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 25 13:25:08 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.404	2.760	78880170	56605663	15.742	19.594
2) SA Decachlor...	8.584	7.533	37659530	39225309	9.736m	10.772m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ053023\
Data File : PQ061320.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 May 2023 14:22
Operator : YP\AJ
Sample : 02955-04
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
SB25


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/31/2023
Supervised By :Ankita Jodhani 05/31/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 30 20:49:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052523.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 25 13:25:08 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

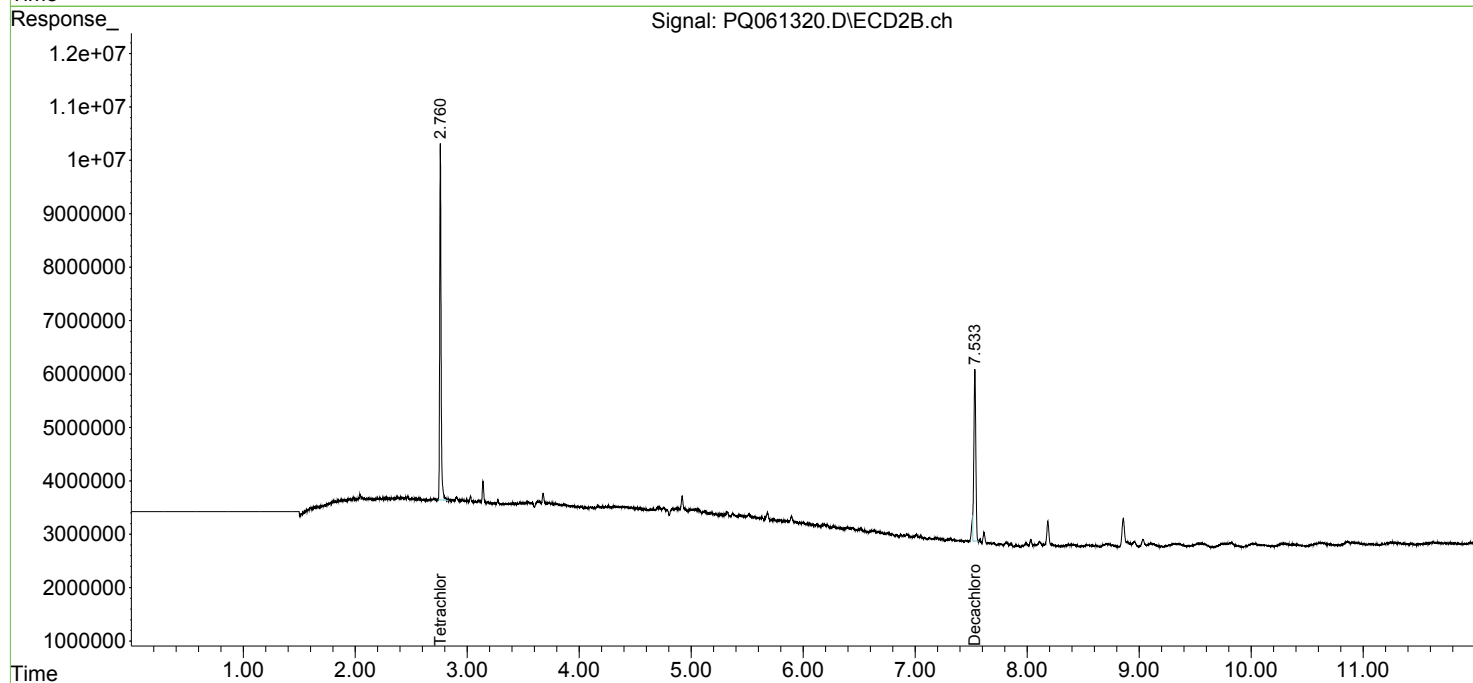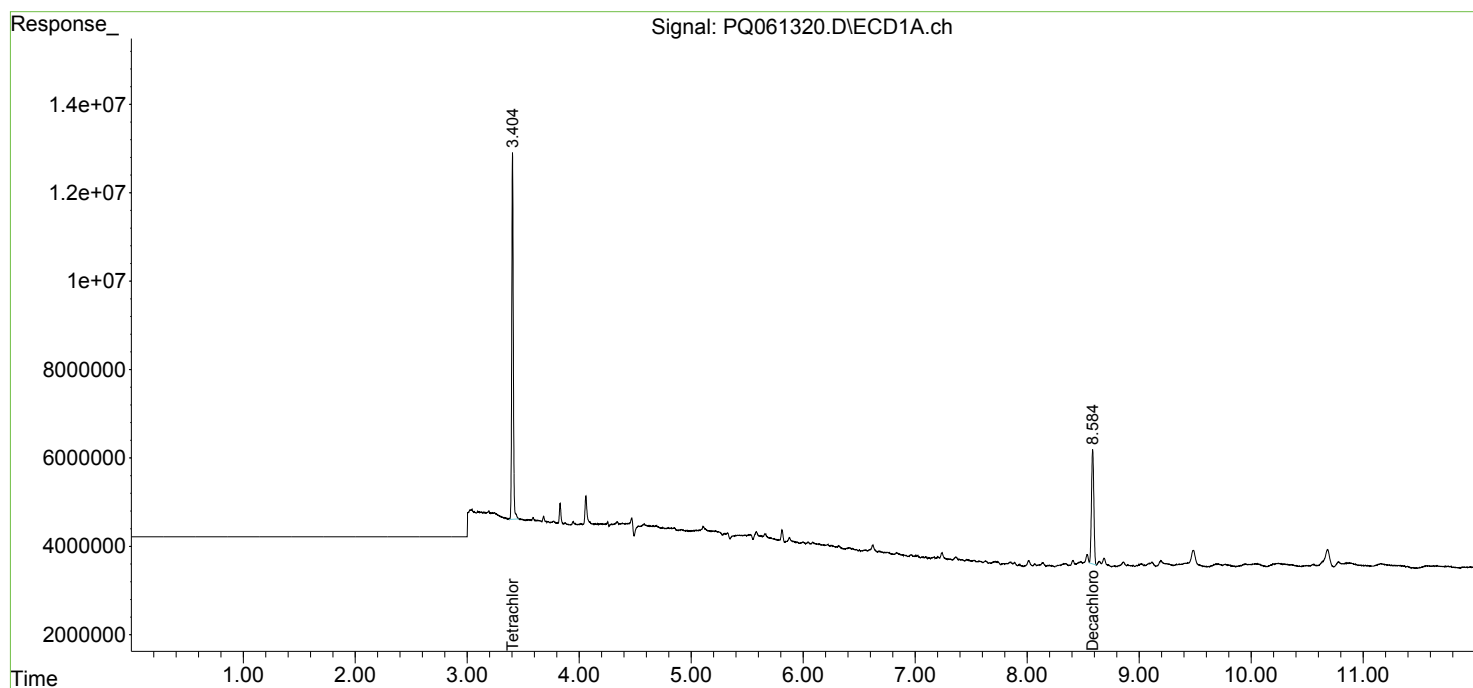

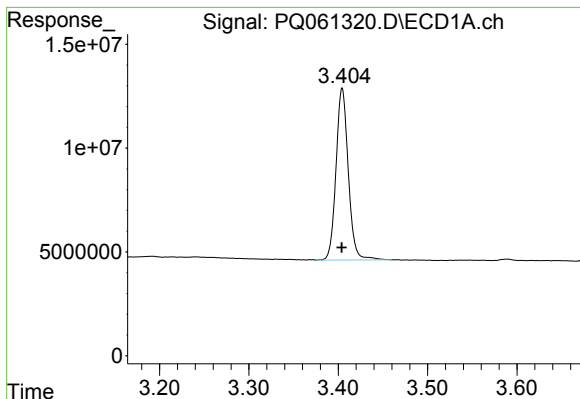


#1 Tetrachloro-m-xylene

R.T.: 3.404 min
Delta R.T.: 0.000 min
Response: 78880170
Conc: 15.74 ng/ml

Instrument :
ECD_Q
ClientSampleId :
SB25


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/31/2023
Supervised By :Ankita Jodhani 05/31/2023

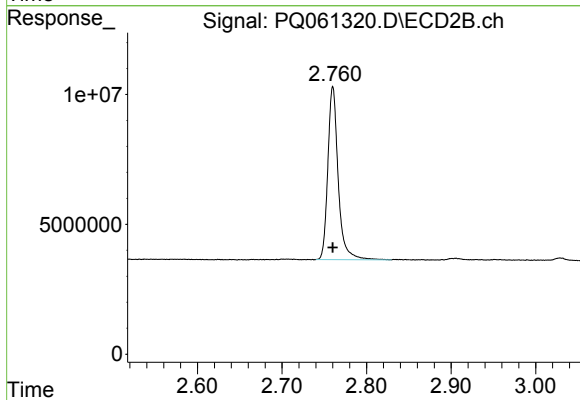


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: 0.000 min
Response: 56605663
Conc: 19.59 ng/ml

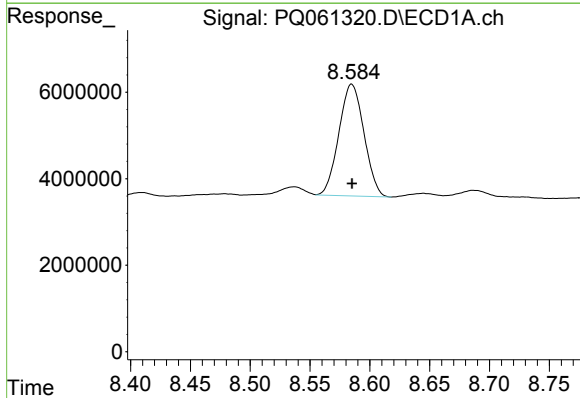

#2 Decachlorobiphenyl

R.T.: 8.584 min
Delta R.T.: 0.000 min
Response: 37659530
Conc: 9.74 ng/ml m

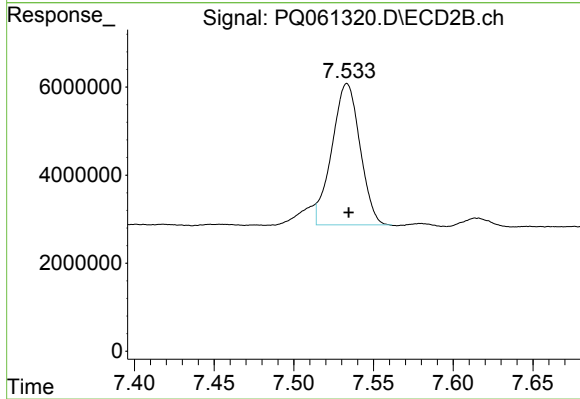

#2 Decachlorobiphenyl

R.T.: 7.533 min
Delta R.T.: -0.001 min
Response: 39225309
Conc: 10.77 ng/ml m