

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ053122\
 Data File : PQ057897.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2022 19:09
 Operator : YP\AJ
 Sample : N3099-05
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 20220426-SPLP-AMENDED-COMPOSITE-F

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 03:52:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 28 06:33:00 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.691	4.055	257.0E6	225.2E6	17.809	19.821
2) SA Decachlor...	10.614	9.208	215.2E6	156.9E6	17.160	16.534

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ053122\
Data File : PQ057897.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2022 19:09
Operator : YP\AJ
Sample : N3099-05
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
20220426-SPLP-AMENDED-COMPOSITE-F

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 03:52:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052822.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 28 06:33:00 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

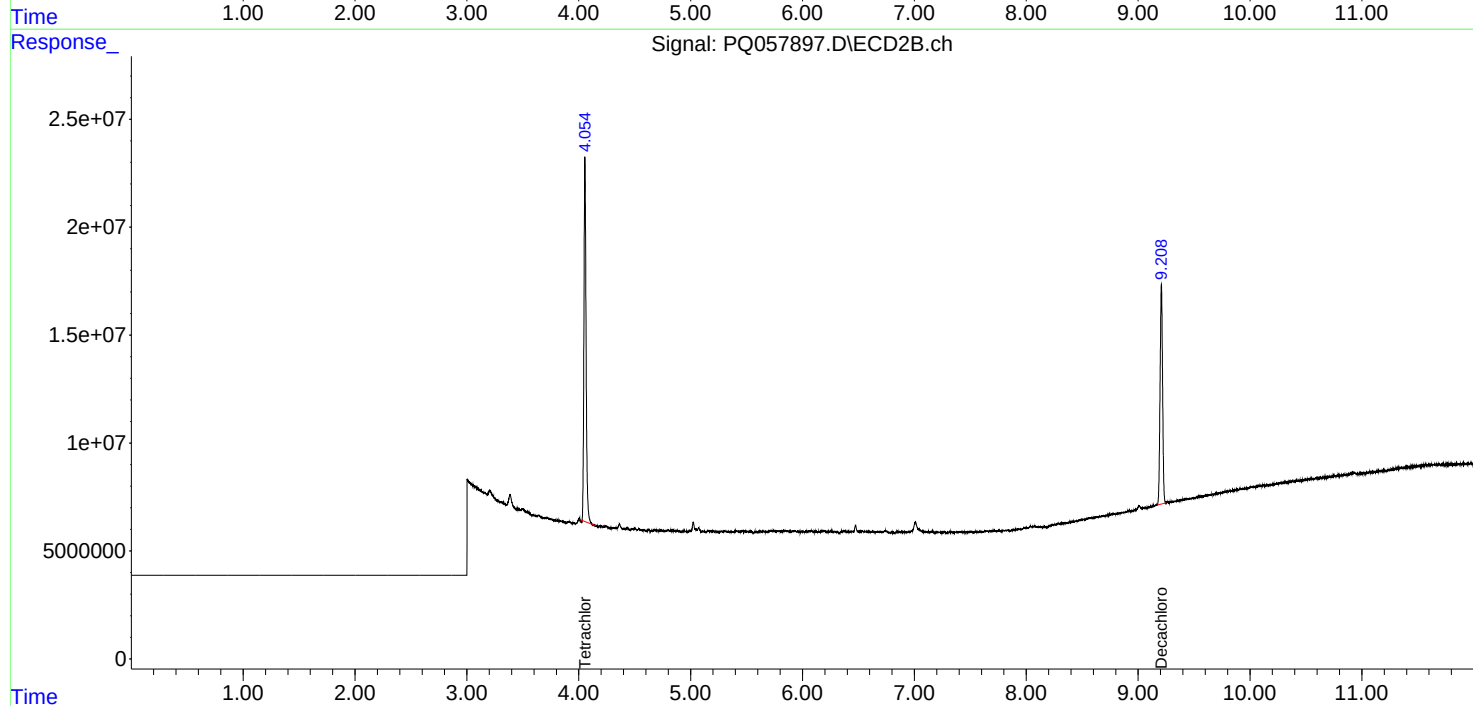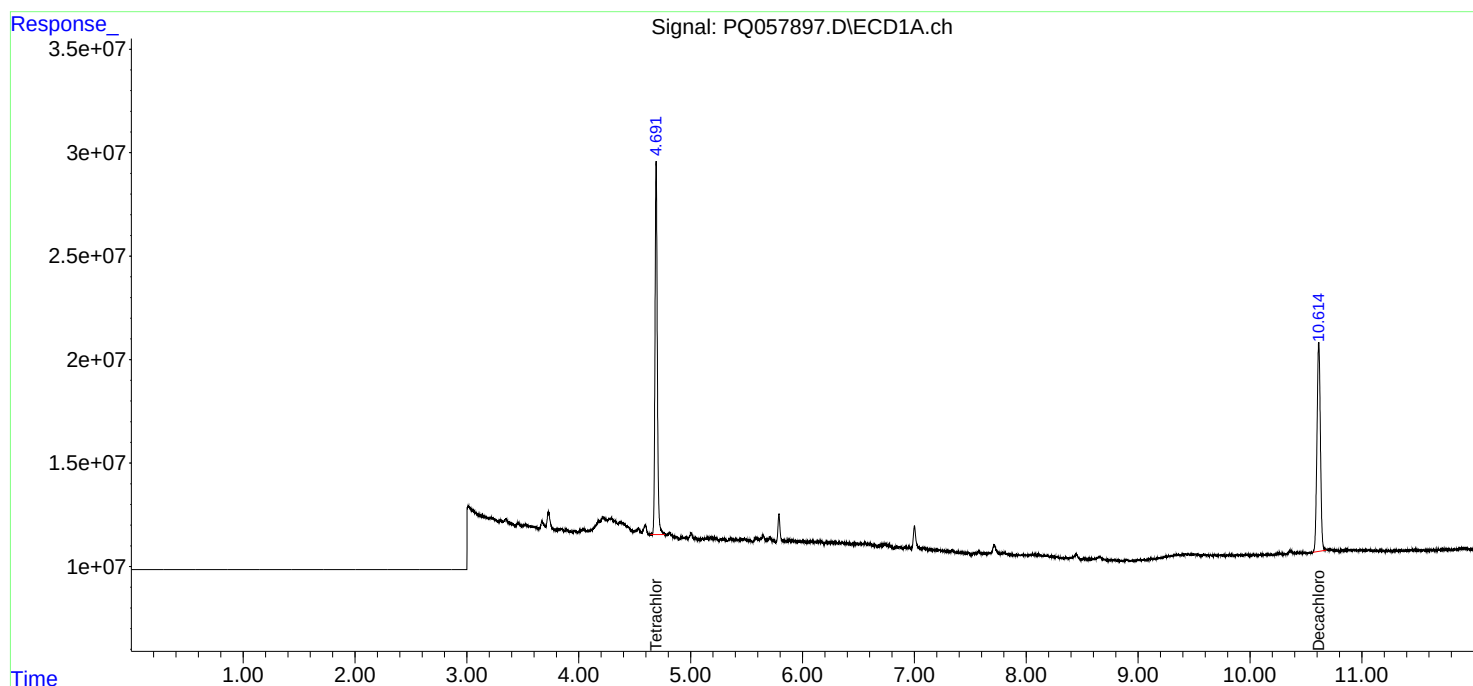

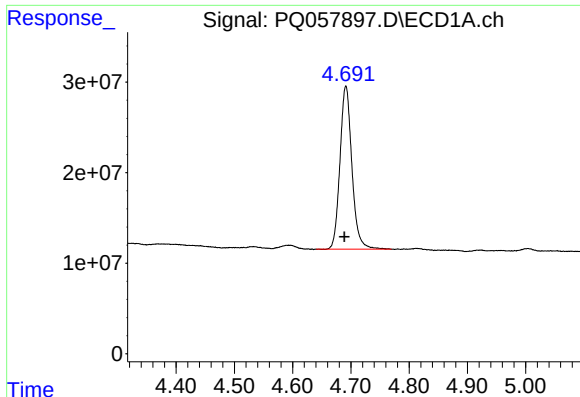

#1 Tetrachloro-m-xylene


R.T.: 4.691 min
Delta R.T.: 0.002 min
Response: 257017883
Conc: 17.81 ng/ml

Instrument :

ECD_Q


ClientSampleId :

20220426-SPLP-AMENDED-COMPOSITE-F

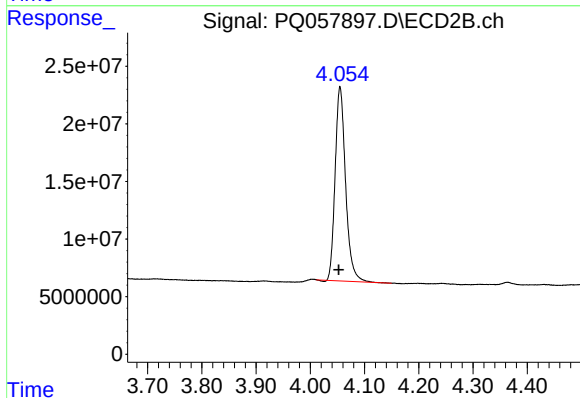


#1 Tetrachloro-m-xylene

R.T.: 4.055 min
Delta R.T.: 0.002 min
Response: 225225724
Conc: 19.82 ng/ml

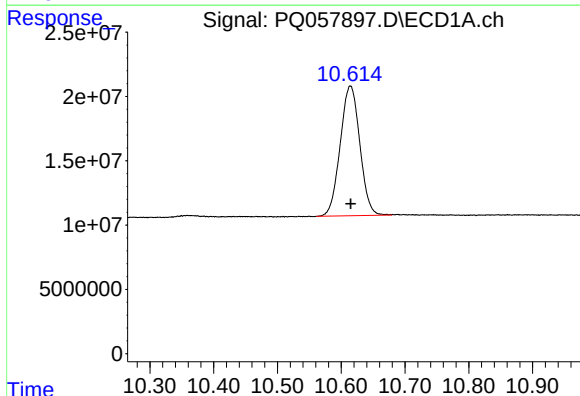

#2 Decachlorobiphenyl

R.T.: 10.614 min
Delta R.T.: 0.000 min
Response: 215213898
Conc: 17.16 ng/ml

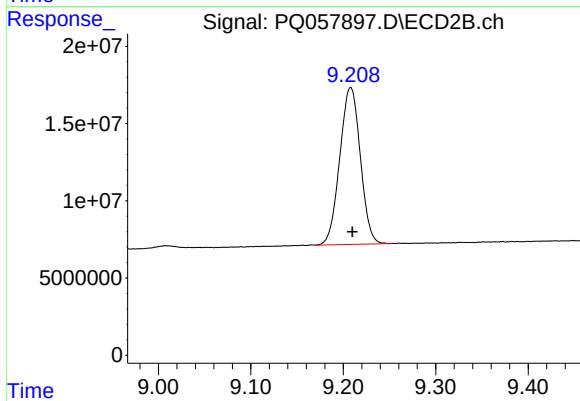

#2 Decachlorobiphenyl

R.T.: 9.208 min
Delta R.T.: -0.002 min
Response: 156907366
Conc: 16.53 ng/ml