

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ053122\
 Data File : PQ057900.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2022 19:53
 Operator : YP\AJ
 Sample : N3099-06
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 20220429-SPLP-AMENDED-COMPOSITE-I

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/01/2022
 Supervised By :Ankita Jodhani 06/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 03:54:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 28 06:33:00 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.690	4.055	259.7E6	226.0E6	17.993	19.889m
2) SA Decachlor...	10.611	9.206	234.6E6	170.1E6	18.703	17.922

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ053122\
Data File : PQ057900.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2022 19:53
Operator : YP\AJ
Sample : N3099-06
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
20220429-SPLP-AMENDED-COMPOSITE-I


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/01/2022
Supervised By :Ankita Jodhani 06/01/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 03:54:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052822.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 28 06:33:00 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

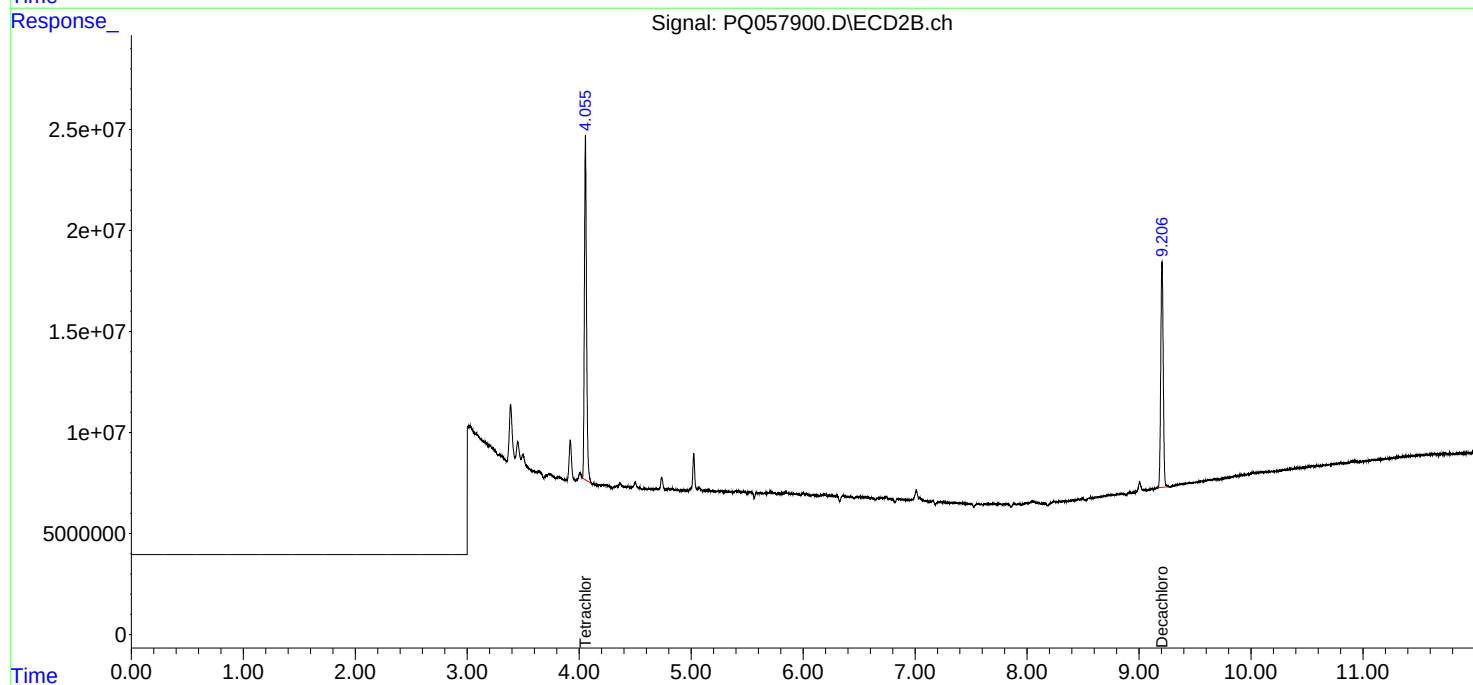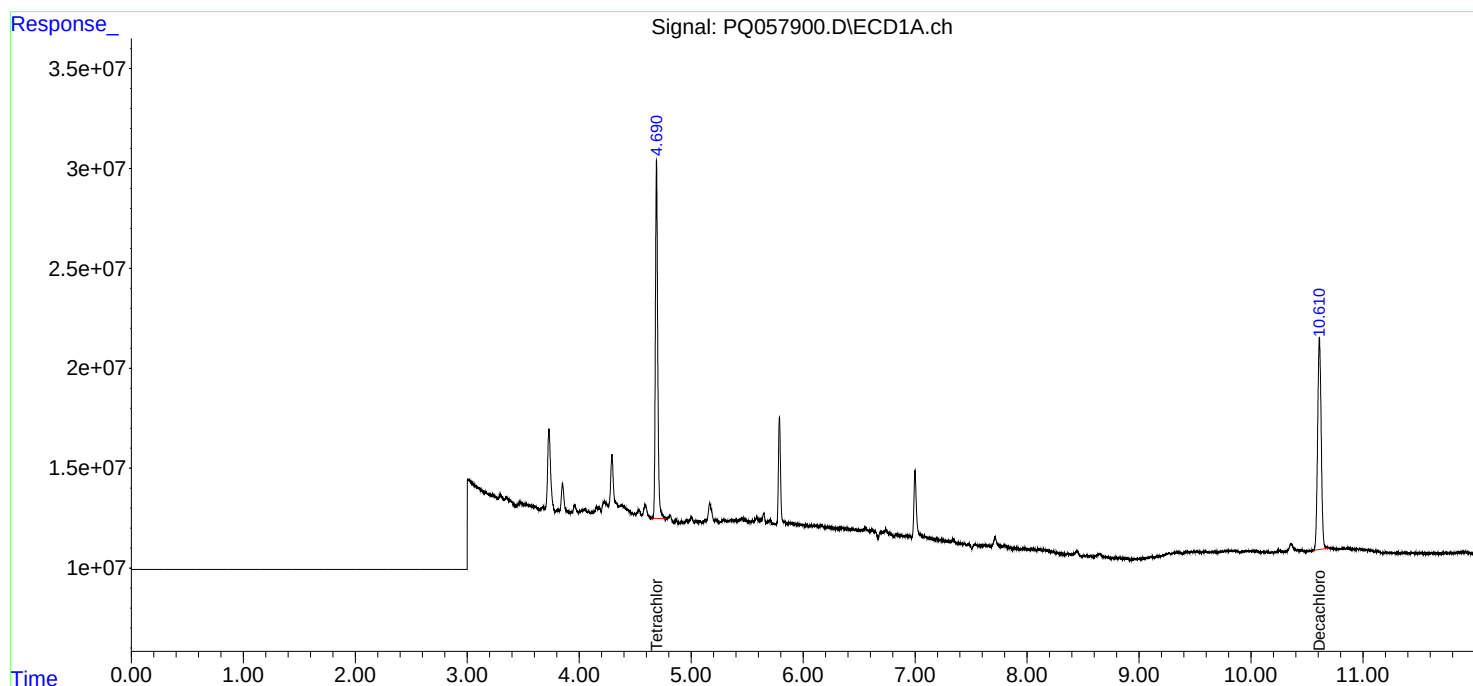

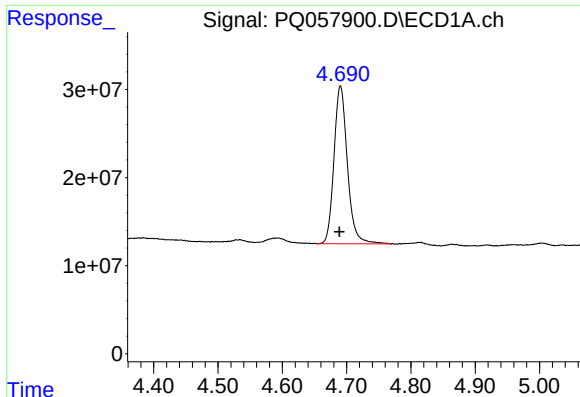

#1 Tetrachloro-m-xylene

R.T.: 4.690 min
Delta R.T.: 0.001 min
Response: 259677109
Conc: 17.99 ng/ml

Instrument :

ECD_Q


ClientSampleId :

20220429-SPLP-AMENDED-COMPOSITE-I

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 06/01/2022
Supervised By :Ankita Jodhani 06/01/2022

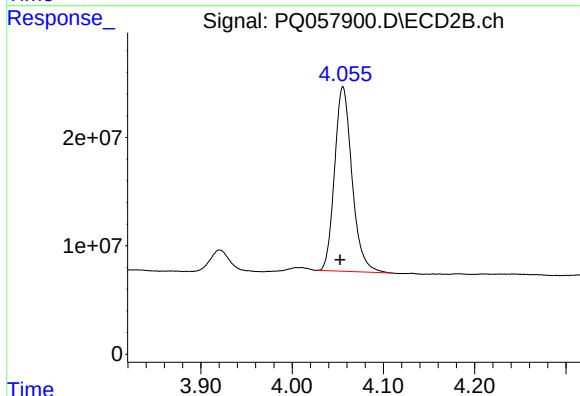


#1 Tetrachloro-m-xylene

R.T.: 4.055 min
Delta R.T.: 0.003 min
Response: 225995099
Conc: 19.89 ng/ml m

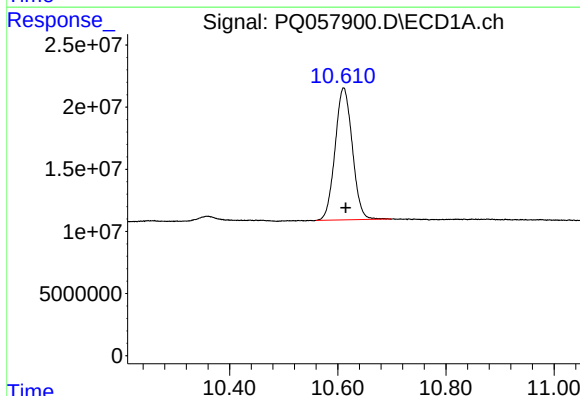

#2 Decachlorobiphenyl

R.T.: 10.611 min
Delta R.T.: -0.004 min
Response: 234566539
Conc: 18.70 ng/ml

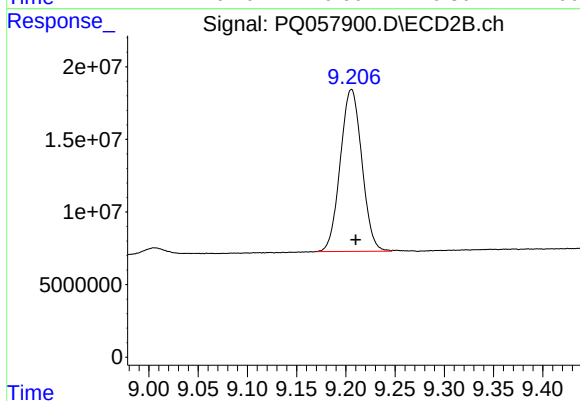

#2 Decachlorobiphenyl

R.T.: 9.206 min
Delta R.T.: -0.004 min
Response: 170082407
Conc: 17.92 ng/ml