

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060322\
 Data File : PQ057934.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2022 14:19
 Operator : YP\AJ
 Sample : PB145258BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 PB145258BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/03/2022
 Supervised By :Ankita Jodhani 06/03/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 23:00:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat May 28 06:33:00 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.689	4.051	284.8E6	268.9E6	19.735	23.667
2) SA Decachlor...	10.612	9.201	310.5E6	232.7E6	24.759	24.517m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060322\
Data File : PQ057934.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2022 14:19
Operator : YP\AJ
Sample : PB145258BL
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
PB145258BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/03/2022
Supervised By :Ankita Jodhani 06/03/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 23:00:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052822.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat May 28 06:33:00 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

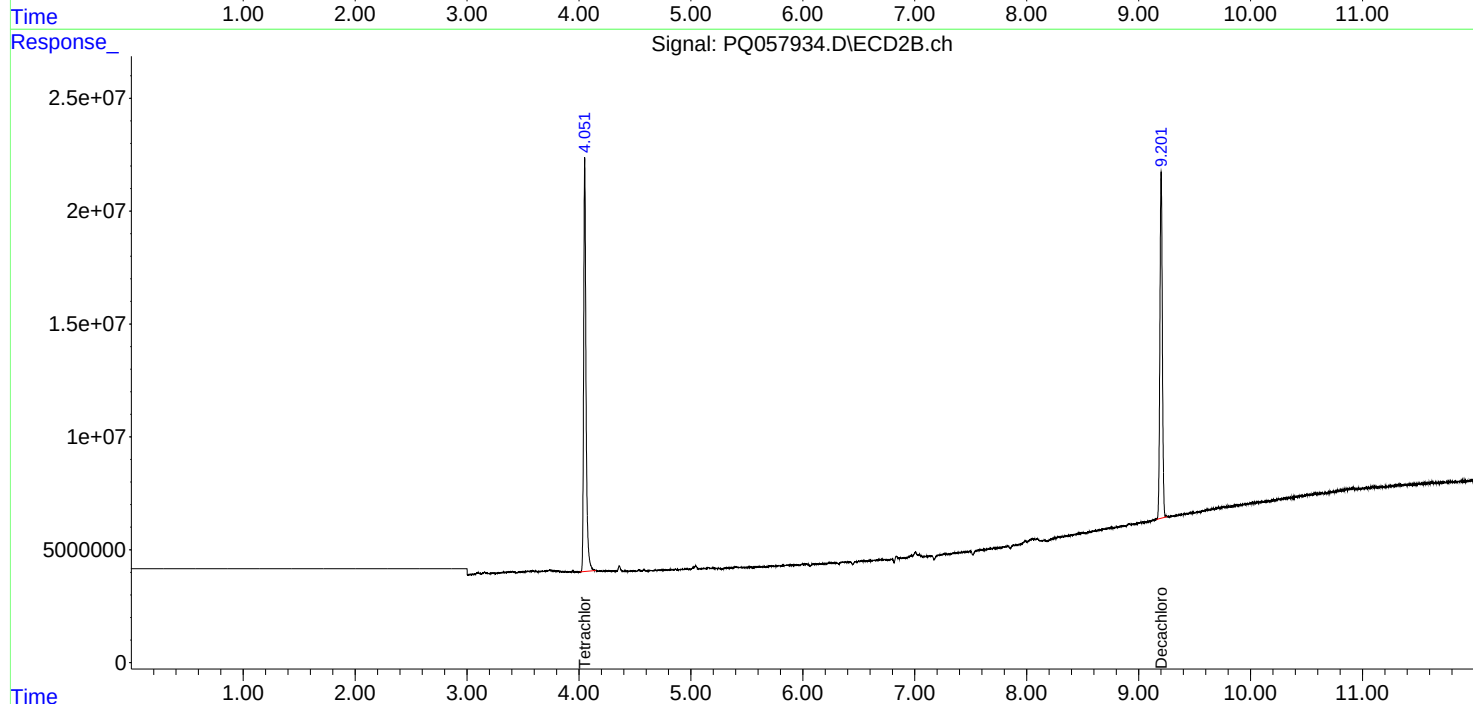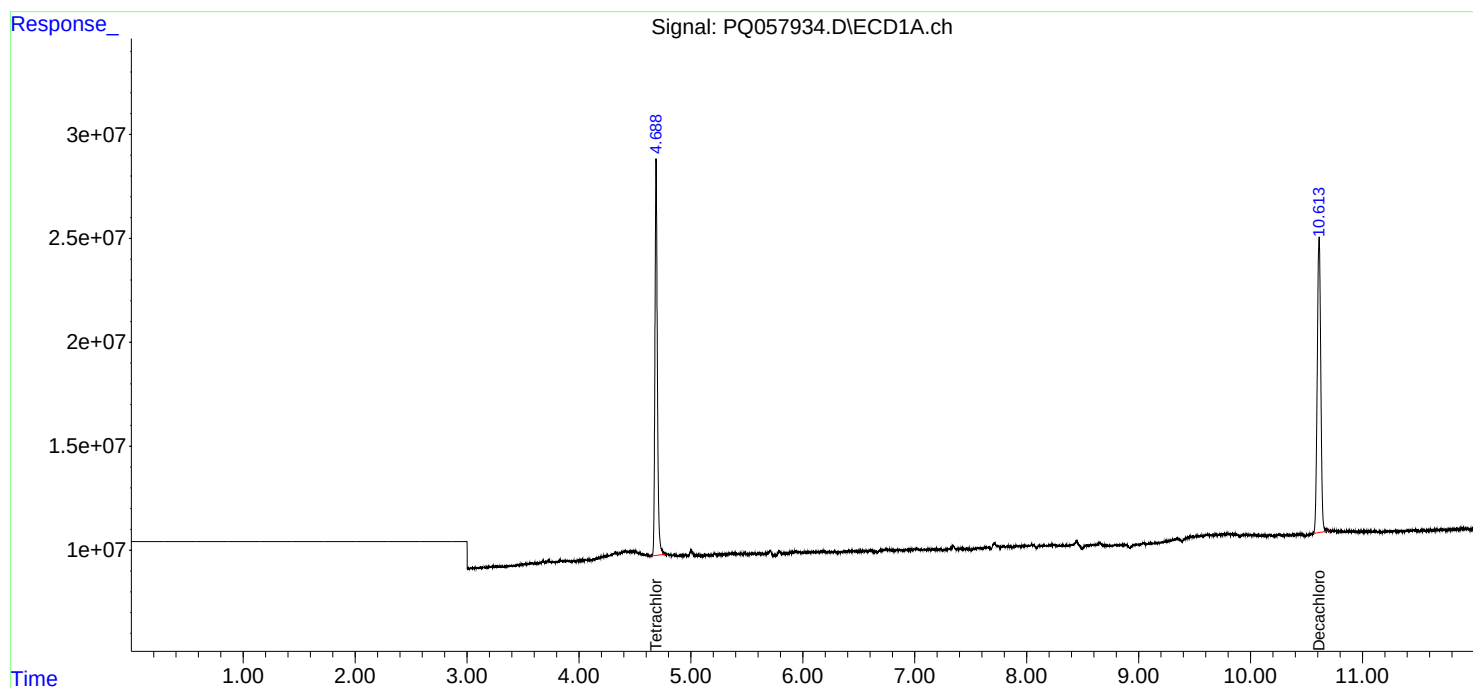

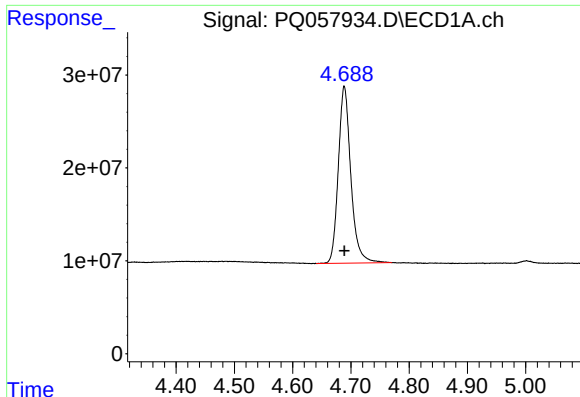

#1 Tetrachloro-m-xylene

R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 284812196
Conc: 19.73 ng/ml


Instrument :

ECD_Q

ClientSampleId :
PB145258BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/03/2022
Supervised By :Ankita Jodhani 06/03/2022

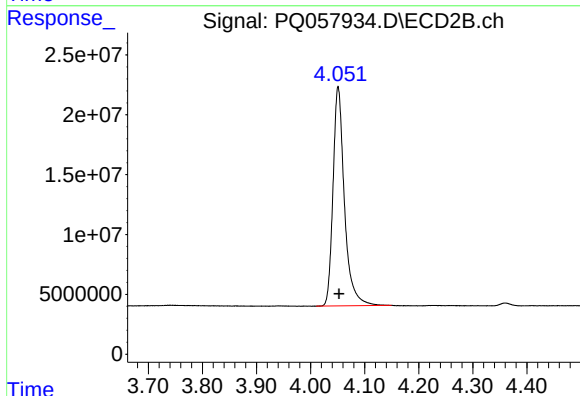


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: -0.002 min
Response: 268928986
Conc: 23.67 ng/ml

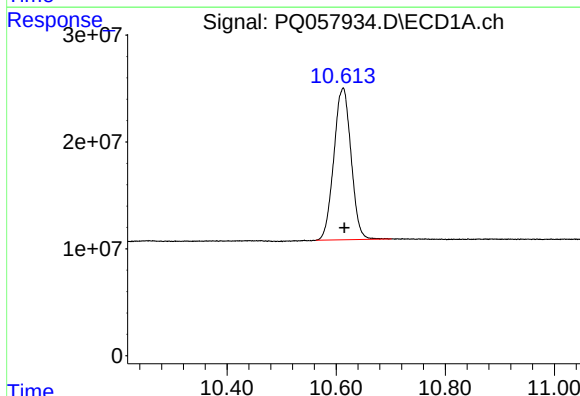

#2 Decachlorobiphenyl

R.T.: 10.612 min
Delta R.T.: -0.003 min
Response: 310521775
Conc: 24.76 ng/ml

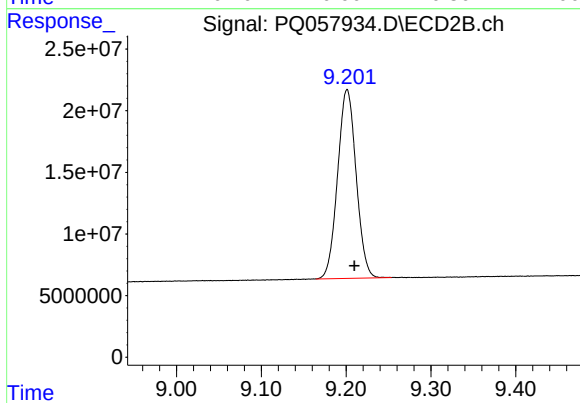

#2 Decachlorobiphenyl

R.T.: 9.201 min
Delta R.T.: -0.009 min
Response: 232667730
Conc: 24.52 ng/ml m