

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060419\
 Data File : PQ040557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2019 13:09
 Operator : SM\AJ
 Sample : K3134-14
 Misc :
 ALS Vial : 18 Sample Multiplier: 1



Instrument :
 ECD_Q
 ClientSampleId :
 PCB-GPC2-BLANK -SPIKE

Manual Integrations
 APPROVED

Ankita
 6/5/2019 9:34:37 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 02:05:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052219CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 23 04:10:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

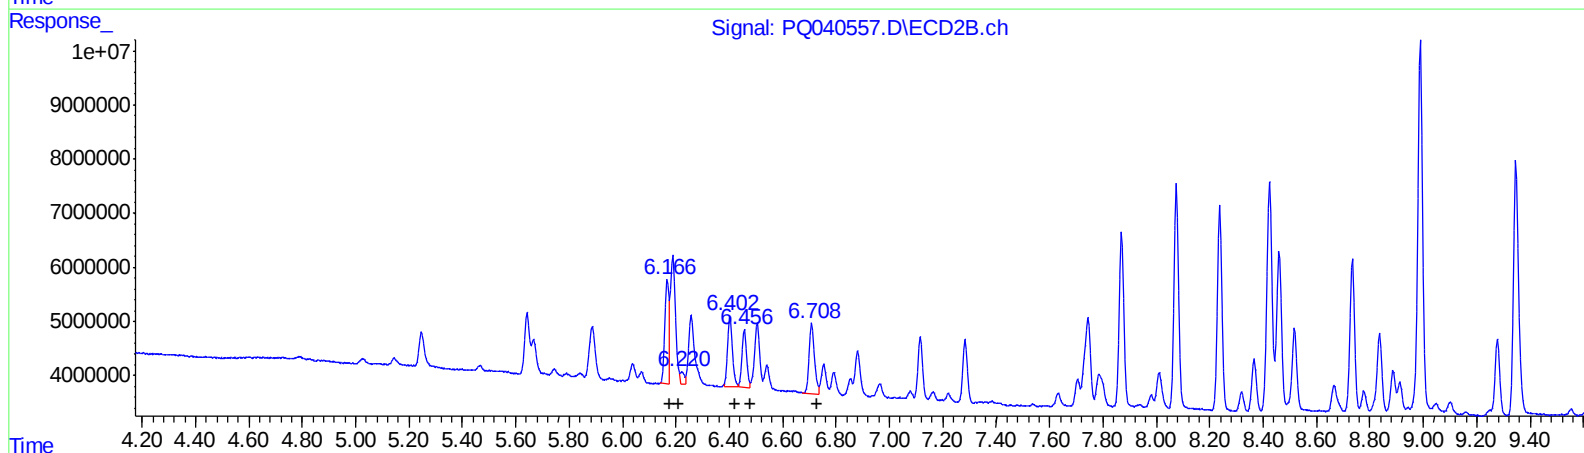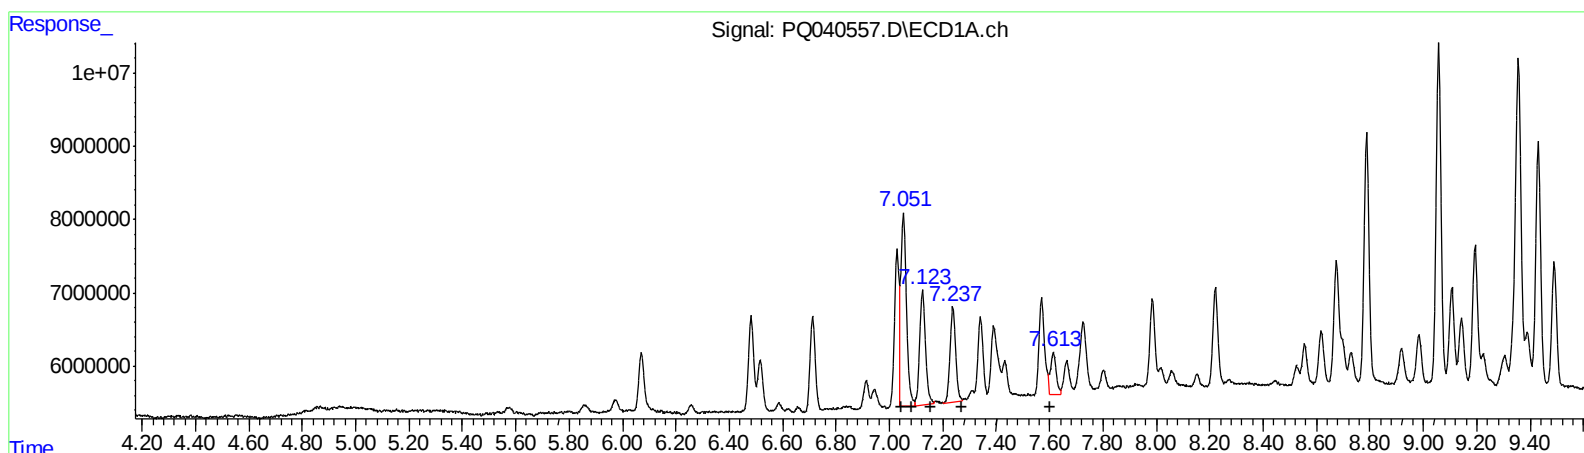

QEdit

(3) AR-1016-1 (L1)

R.T.	Response	Conc
7.05	38403761	229.56
7.05	38403761	146.08
7.12	23982272	140.51
7.24	19096566	138.16
7.61	8604857	62.03

(3) AR-1016-1 #2 (L1)

R.T.	Response	Conc
6.17	20842249	162.48
6.22	2348123	12.17
6.40	15887318	147.31
6.46	12908542	151.60
6.71	18150004	157.63

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060419\
Data File : PQ040557.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2019 13:09
Operator : SM\AJ
Sample : K3134-14
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
PCB-GPC2-BLANK -SPIKE

Manual Integrations
APPROVED

Ankita
6/5/2019 9:34:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 02:05:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052219CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 23 04:10:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

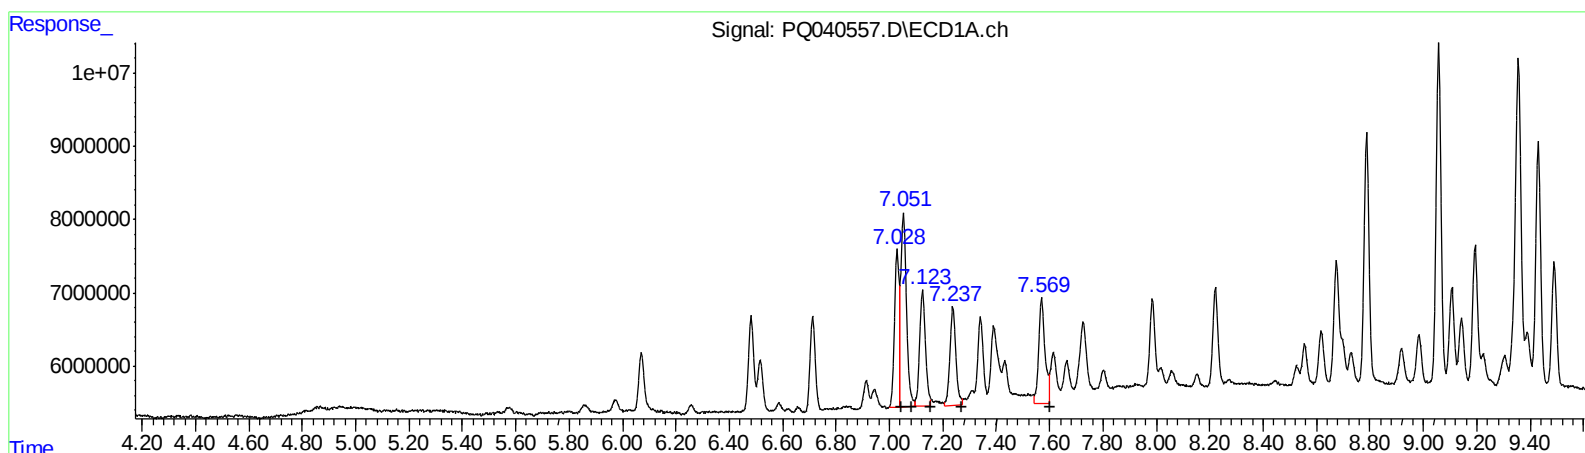

(3) AR-1016-1 #2 (L1)
R.T. Response Conc
7.03 26128694 156.19
7.05 38156905 145.14
7.12 24196675 141.77
7.24 20901078 151.21
7.57 23409586 168.75

(3) AR-1016-1 #2 (L1)
R.T. Response Conc
6.17 20842249 162.48
6.19 30725161 159.19
6.40 15887318 147.31
6.46 12908542 151.60
6.71 18150004 157.63

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060419\
Data File : PQ040557.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2019 13:09
Operator : SM\AJ
Sample : K3134-14
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
PCB-GPC2-BLANK -SPIKE

Manual Integrations
APPROVED

Ankita
6/5/2019 9:34:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 02:05:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052219CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 23 04:10:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

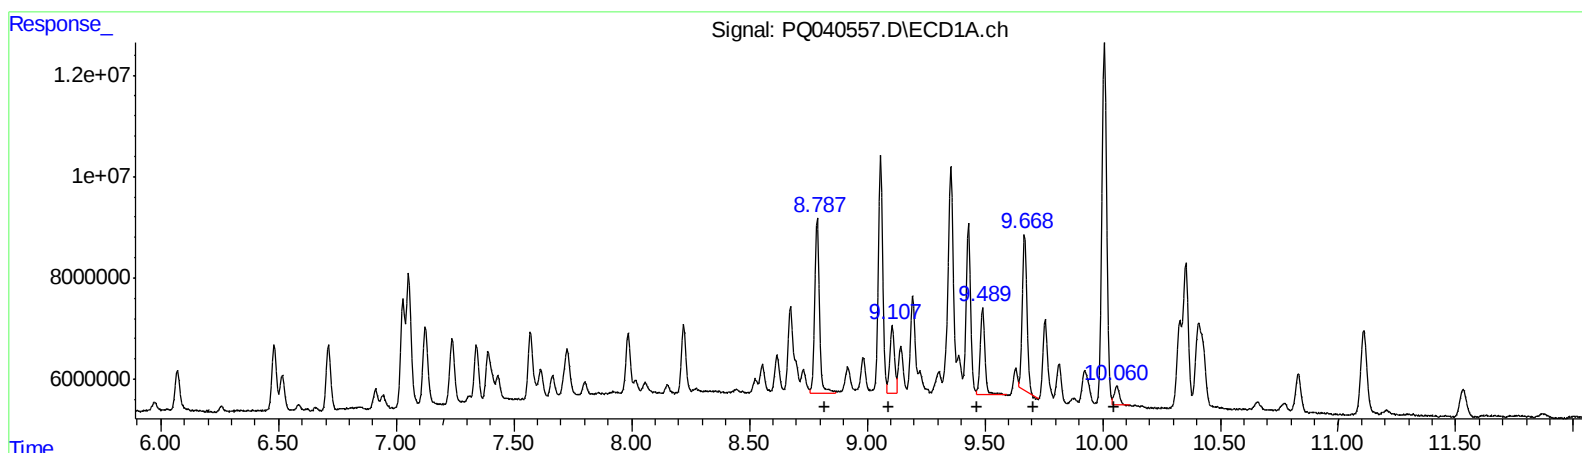

(31) AR-1260-1 (L7)

R.T.	Response	Conc
8.79	47977246	144.33
9.11	18548312	45.92
9.49	23230847	70.42
9.67	41783775	113.38
10.06	5826827	7.57

(31) AR-1260-1 #2 (L7)

R.T.	Response	Conc
7.87	40394696	147.35
8.07	50374610	145.63
8.24	44839953	139.82
8.78	4768727	17.55
8.99	87759944	130.56

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060419\
Data File : PQ040557.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Jun 2019 13:09
Operator : SM\AJ
Sample : K3134-14
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
PCB-GPC2-BLANK -SPIKE

Manual Integrations
APPROVED

Ankita
6/5/2019 9:34:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 02:05:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052219CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 23 04:10:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

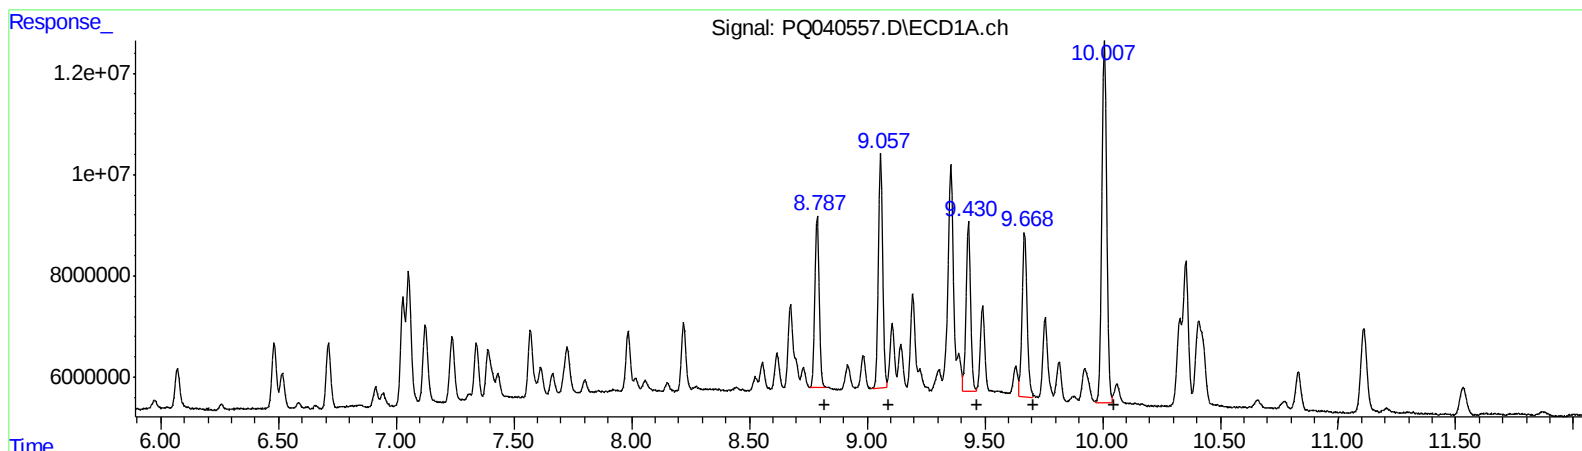

(31) AR-1260-1 #2 (L7)
R.T. Response Conc
8.79 43317741 130.31
9.06 58917230 145.85
9.43 44388896 134.56
9.67 47350372 128.48
10.01 102776185 133.46
(31) AR-1260-1 #2 (L7)
R.T. Response Conc
7.87 40394696 147.35
8.07 49373207 142.73
8.24 45080442 140.57
8.73 34248136 126.04
8.99 87759944 130.56

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060419\
 Data File : PQ040557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Jun 2019 13:09
 Operator : SM\AJ
 Sample : K3134-14
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 PCB-GPC2-BLANK -SPIKE

Manual Integrations
 APPROVED

Ankita
 6/5/2019 9:34:37 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 02:05:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ052219CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 23 04:10:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

3) L1	AR-1016-1	7.028	6.167	26128694	20842249	156.186m	162.477
4) L1	AR-1016-2	7.051	6.187	38156905	30725161	145.137m	159.187m
5) L1	AR-1016-3	7.123	6.402	24196675	15887318	141.768m	147.310
6) L1	AR-1016-4	7.237	6.456	20901078	12908542	151.212m	151.599
7) L1	AR-1016-5	7.569	6.708	23409586	18150004	168.749m	157.634
31) L7	AR-1260-1	8.787	7.869	43317741	40394696	130.315m	147.352
32) L7	AR-1260-2	9.057	8.074	58917230	49373207	145.847m	142.732m
33) L7	AR-1260-3	9.430	8.236	44388896	45080442	134.557m	140.567m
34) L7	AR-1260-4	9.668	8.733	47350372	34248136	128.483m	126.042m
35) L7	AR-1260-5	10.007	8.988	102.8E6	87759944	133.464m	130.560

AJ
 06/05/19

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.