

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060624\
 Data File : PQ066973.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2024 14:30
 Operator : YP\AJ
 Sample : P2477-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 ETGI-339

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/07/2024
 Supervised By :Ankita Jodhani 06/07/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 14:44:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ053124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 03 10:00:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.447	2.825	133.4E6	137.9E6	24.082	23.581
2) SA Decachlor...	8.706	7.612	60856606	105.0E6	16.047m	18.285

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060624\
Data File : PQ066973.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2024 14:30
Operator : YP\AJ
Sample : P2477-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
ETGI-339


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2024
Supervised By :Ankita Jodhani 06/07/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 14:44:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ053124.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 03 10:00:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

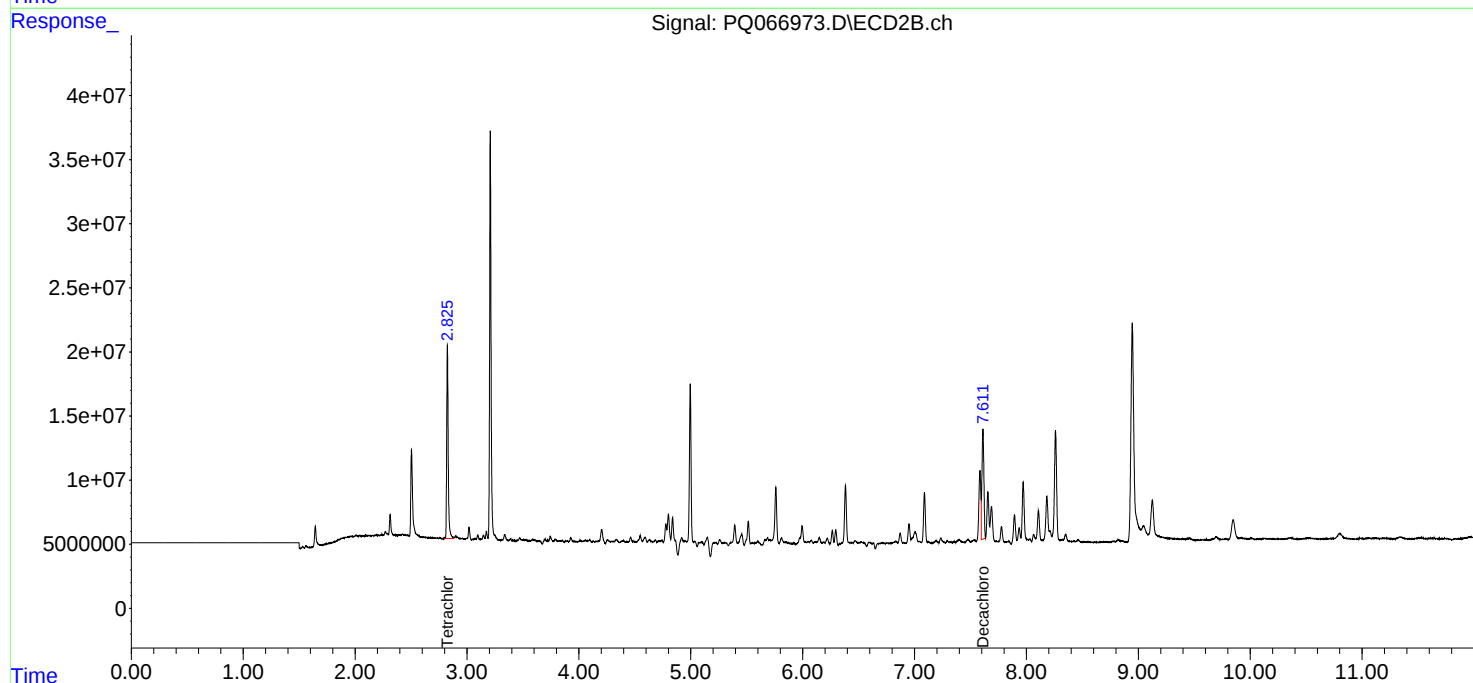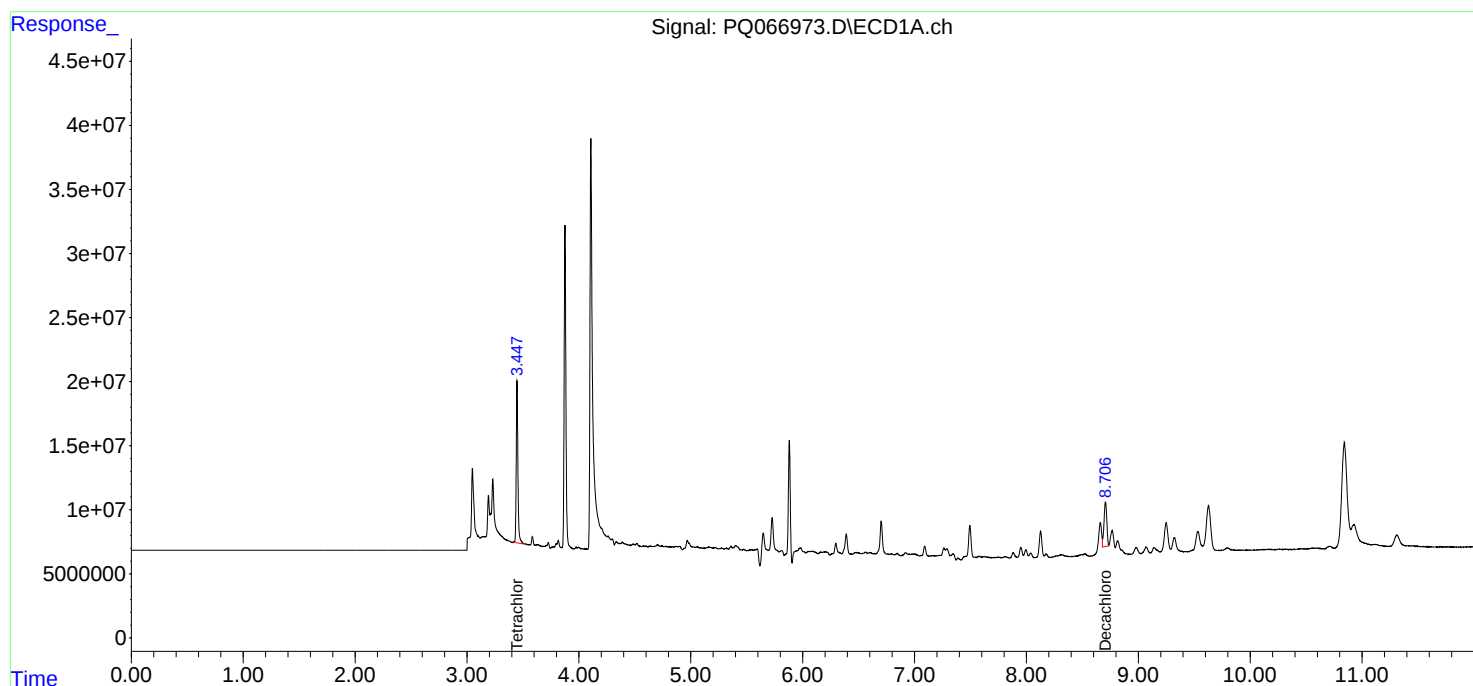

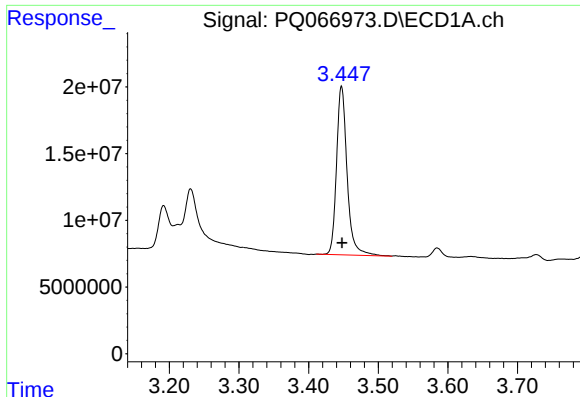

#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: 0.000 min
Response: 133378856
Conc: 24.08 ng/ml

Instrument :


ECD_Q

ClientSampleId :

ETGI-339


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2024
Supervised By :Ankita Jodhani 06/07/2024

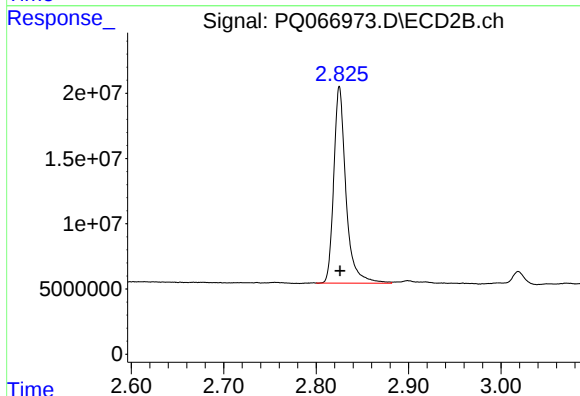


#1 Tetrachloro-m-xylene

R.T.: 2.825 min
Delta R.T.: 0.000 min
Response: 137947911
Conc: 23.58 ng/ml

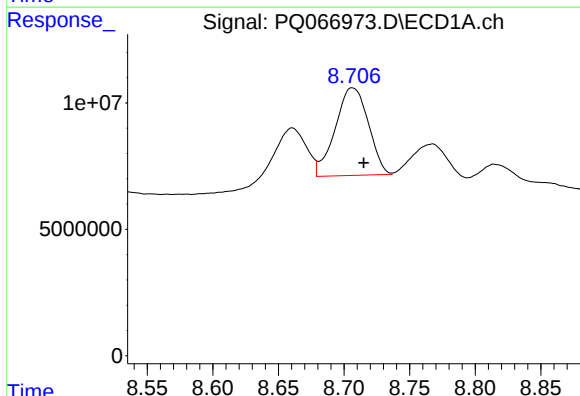

#2 Decachlorobiphenyl

R.T.: 8.706 min
Delta R.T.: -0.009 min
Response: 60856606
Conc: 16.05 ng/ml m

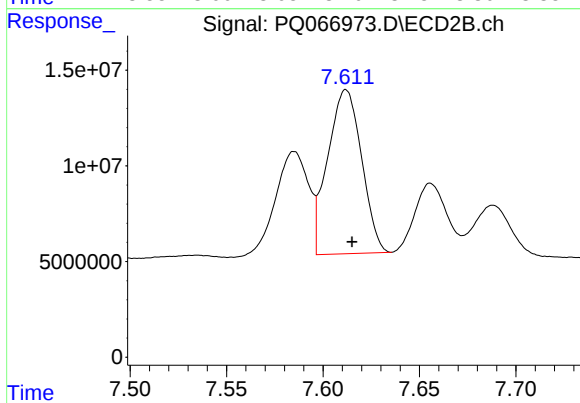

#2 Decachlorobiphenyl

R.T.: 7.612 min
Delta R.T.: -0.003 min
Response: 105014218
Conc: 18.29 ng/ml