

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060724\
 Data File : PQ067014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2024 17:47
 Operator : YP\AJ
 Sample : P2764-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 K-2211-ESSEX-SWITCHING-STATION

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 22:29:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ053124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 03 10:00:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.448	2.826	88829549	83364549	16.038	14.251
2)	SA Decachlor...	8.716	7.621	69467016	67387762	18.318	11.734 #
Target Compounds							
3)	L1 AR-1016-1	4.523f	3.828	9752076	2576995	57.611	12.605 #
4)	L1 AR-1016-2	4.618f	3.855	3698851	1041835	14.055	3.511 #
5)	L1 AR-1016-3	4.618	4.019	3698851	1084324	23.047	6.606 #
6)	L1 AR-1016-4	4.711	4.068	1286785	801599	10.041	5.820 #
7)	L1 AR-1016-5	5.026	4.259	5510064	195756	42.783	1.141 #
8)	L2 AR-1221-1	3.643	3.048	4446854	1231732	67.649	15.378 #
9)	L2 AR-1221-2	3.729	3.096	1998746	1762133	41.268	33.720
10)	L2 AR-1221-3	3.783	3.188	1641784	72014	10.812	0.412 #
11)	L3 AR-1232-1	3.783	3.188	1641784	72014	13.300	0.499 #
12)	L3 AR-1232-2	4.306	3.855	885945	1041835	13.436	7.333 #
13)	L3 AR-1232-3	4.618f	4.019	3698851	1084324	30.697	13.929 #
14)	L3 AR-1232-4	4.711	4.095	1286785	847577	22.387	12.746 #
15)	L3 AR-1232-5	4.851f	4.259	932657	195756	23.313	2.611 #
16)	L4 AR-1242-1	4.523f	3.828	9752076	2576995	68.391	14.815 #
17)	L4 AR-1242-2	4.618f	3.855	3698851	1041835	16.809	4.180 #
18)	L4 AR-1242-3	4.618	4.019	3698851	1084324	27.479	7.770 #
19)	L4 AR-1242-4	4.711	4.095	1286785	847577	12.158	6.489 #
20)	L4 AR-1242-5	5.439	4.615	2813218	1686234	24.629	10.158 #
21)	L5 AR-1248-1	4.523f	3.828	9752076	2576995	92.431	20.132 #
22)	L5 AR-1248-2	4.851f	4.068	932657	801599	6.361	4.182 #
23)	L5 AR-1248-3	5.026	4.095	5510064	847577	31.527	4.605 #
24)	L5 AR-1248-4	5.406	4.259	2082105	195756	10.615	0.868 #
25)	L5 AR-1248-5	5.439	4.642	2813218	317015	14.152	1.482 #
26)	L6 AR-1254-1	5.406	4.615	2082105	1686234	10.048	5.028 #
27)	L6 AR-1254-2	5.636f	4.747	540937	593175	1.677	2.055
28)	L6 AR-1254-3	5.952	5.121	1121387	190258	3.304	0.409 #
29)	L6 AR-1254-4	6.266	5.352	3410332	752935	14.486	2.703 #
30)	L6 AR-1254-5	6.670	5.786	4834948	1738270	18.248	4.148 #
31)	L7 AR-1260-1	6.135	5.260	377837	559606	1.465	1.691
32)	L7 AR-1260-2	6.397	5.472f	1109465	1160795	3.650	2.970
33)	L7 AR-1260-3	6.724f	5.585	3502885	278954	15.830	0.736 #
34)	L7 AR-1260-4	6.994	6.085f	2831647	4994957	11.689	15.899 #
35)	L7 AR-1260-5	7.281	6.291	2751863	1732936	5.624	2.625 #
36)	L8 AR-1262-1	6.724f	5.809	3502885	596459	10.595	1.380 #
37)	L8 AR-1262-2	7.281	6.291	2751863	1732936	5.137	2.378 #
38)	L8 AR-1262-3	7.580	6.568	5615045	2545498	15.978	8.173 #
39)	L8 AR-1262-4	7.673	6.637	677214	2903288	2.509	5.091 #
40)	L8 AR-1262-5	8.200f	7.122	8026227	589584	47.942	2.273 #
41)	L9 AR-1268-1	7.580	6.568	5615045	2545498	9.354	2.902 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060724\
Data File : PQ067014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2024 17:47
Operator : YP\AJ
Sample : P2764-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 22:29:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ053124.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 03 10:00:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	7.673	6.637	677214	2903288	1.254	3.627 #
43)	L9 AR-1268-3	7.831	6.841	4356805	2044904	9.349	2.949 #
44)	L9 AR-1268-4	8.200f	7.122	8026227	589584	45.555	2.078 #
45)	L9 AR-1268-5	8.480	7.420	648102	1423080	0.485	0.696 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060724\
Data File : PQ067014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2024 17:47
Operator : YP\AJ
Sample : P2764-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 22:29:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ053124.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 03 10:00:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

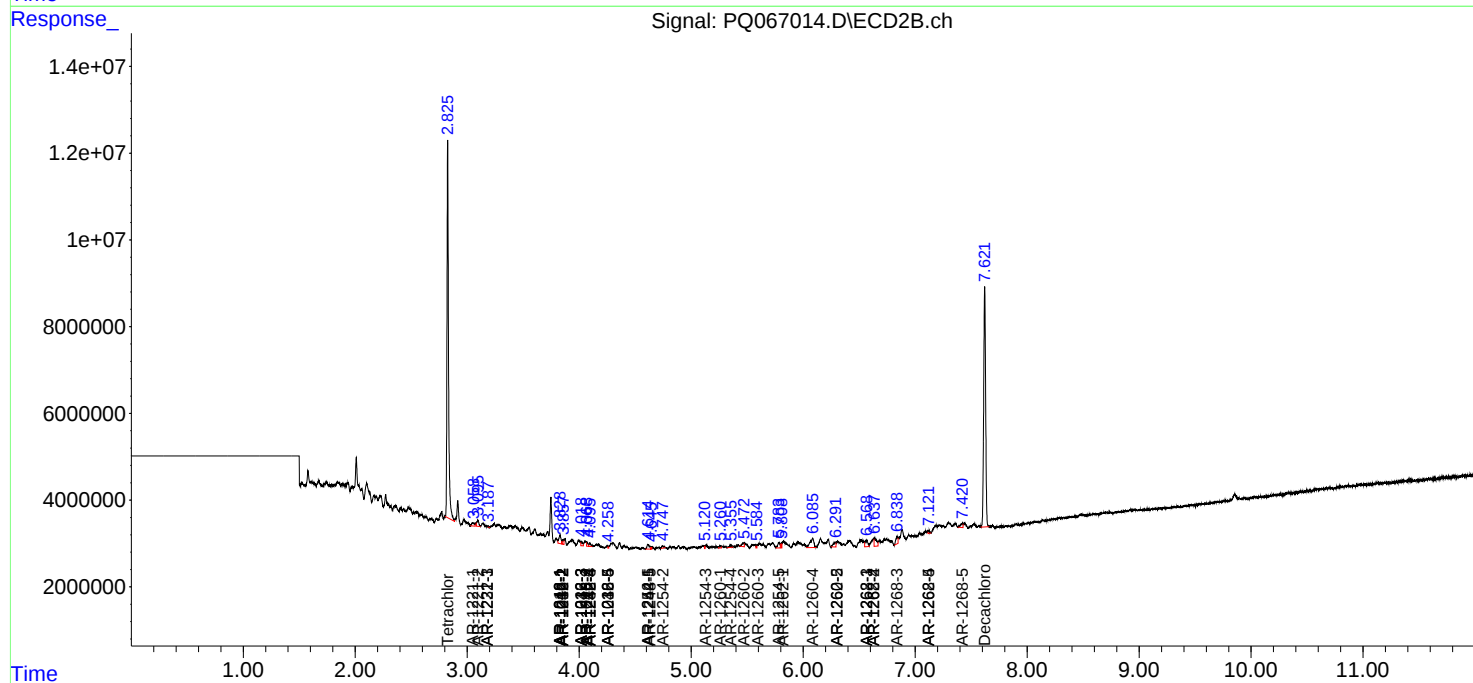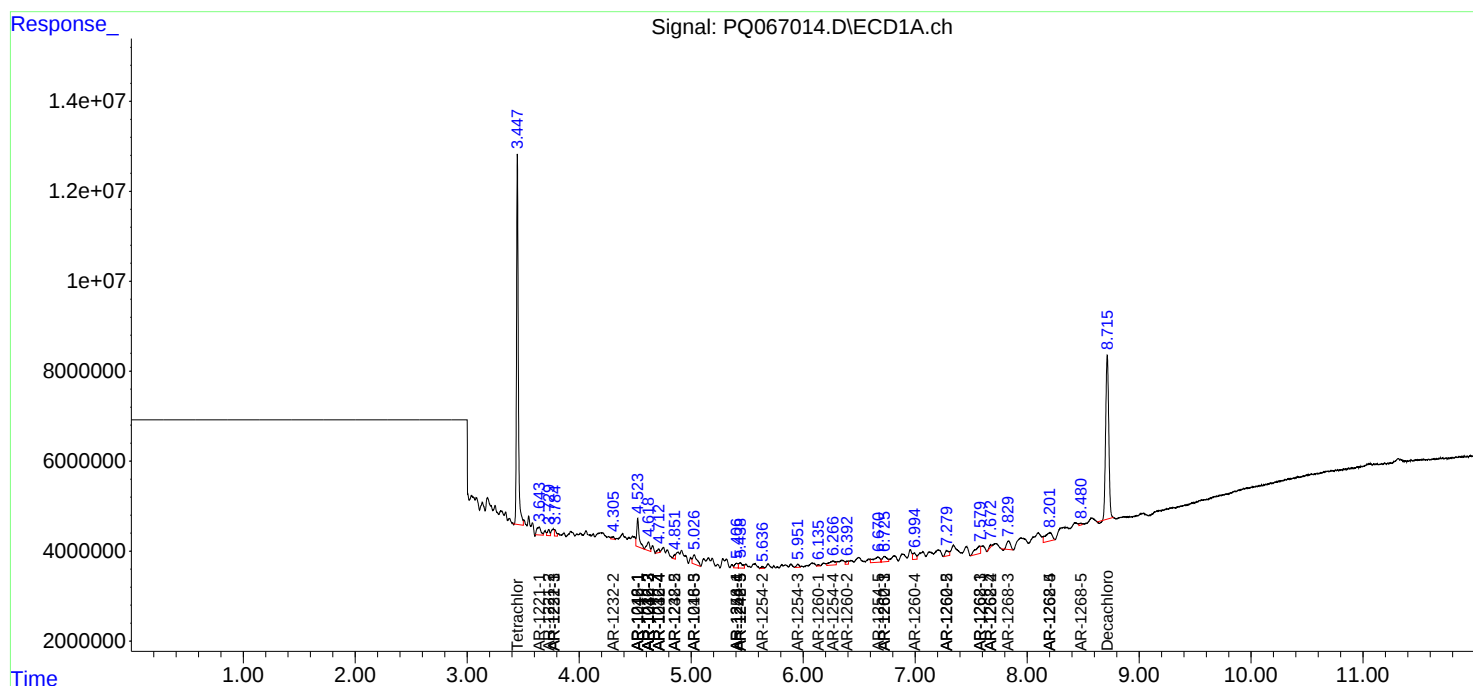

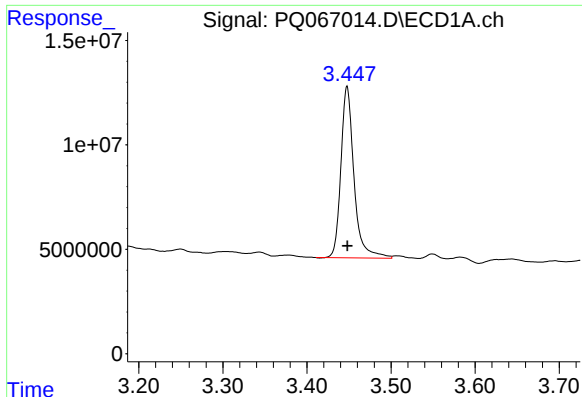

#1 Tetrachloro-m-xylene


R.T.: 3.448 min
Delta R.T.: 0.000 min
Response: 88829549
Conc: 16.04 ng/ml

Instrument :

ECD_Q


ClientSampleId :

K-2211-ESSEX-SWITCHING-STATION

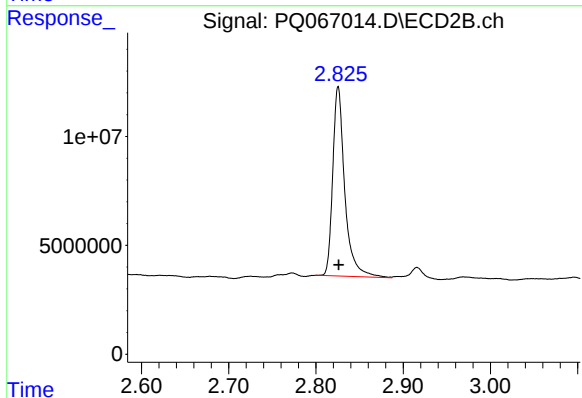


#1 Tetrachloro-m-xylene

R.T.: 2.826 min
Delta R.T.: 0.000 min
Response: 83364549
Conc: 14.25 ng/ml

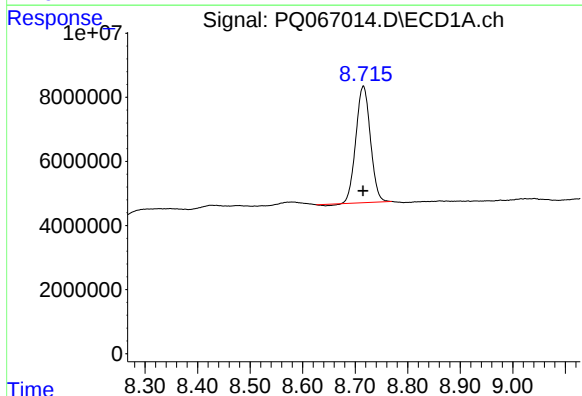


#2 Decachlorobiphenyl

R.T.: 8.716 min
Delta R.T.: 0.000 min
Response: 69467016
Conc: 18.32 ng/ml

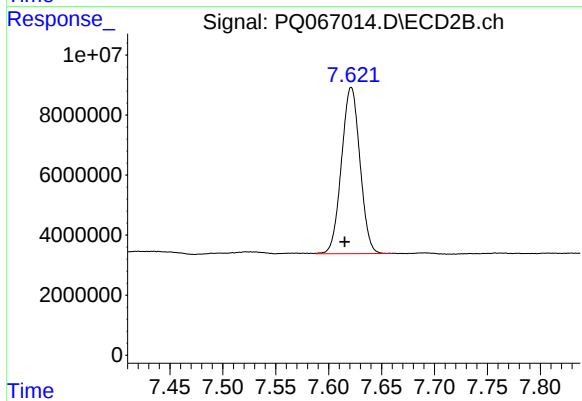

#2 Decachlorobiphenyl


R.T.: 7.621 min
Delta R.T.: 0.006 min
Response: 67387762
Conc: 11.73 ng/ml

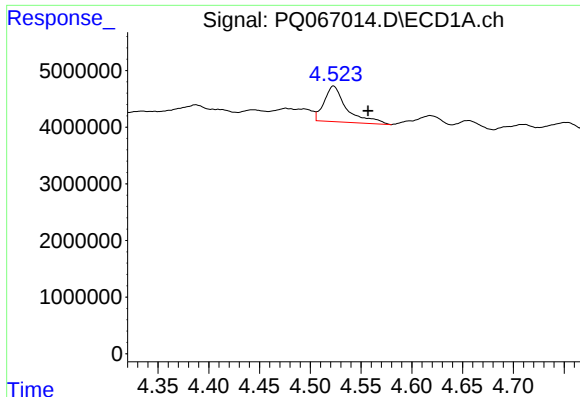

#3 AR-1016-1


R.T.: 4.523 min
Delta R.T.: -0.034 min
Response: 9752076
Conc: 57.61 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

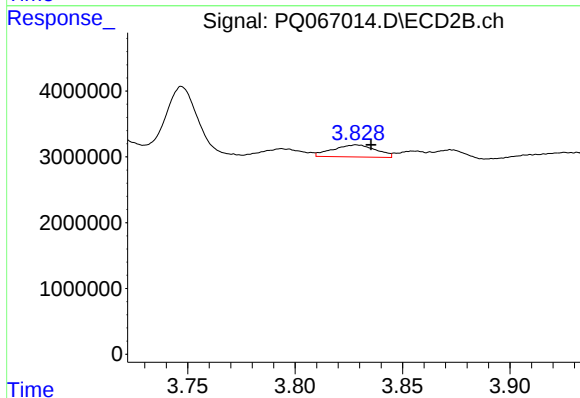


#3 AR-1016-1

R.T.: 3.828 min
Delta R.T.: -0.007 min
Response: 2576995
Conc: 12.61 ng/ml

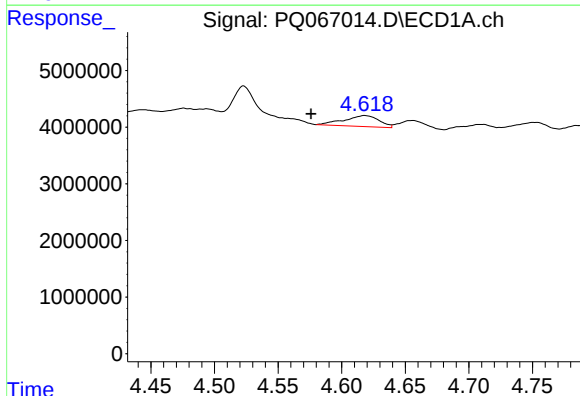


#4 AR-1016-2

R.T.: 4.618 min
Delta R.T.: 0.042 min
Response: 3698851
Conc: 14.06 ng/ml

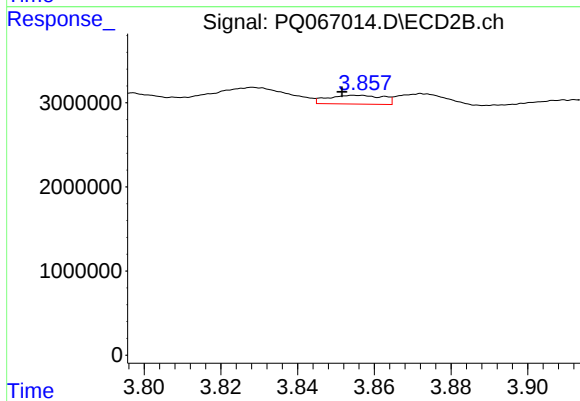

#4 AR-1016-2


R.T.: 3.855 min
Delta R.T.: 0.003 min
Response: 1041835
Conc: 3.51 ng/ml

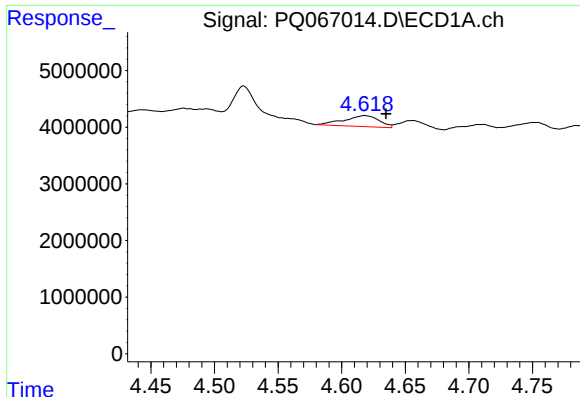

#5 AR-1016-3


R.T.: 4.618 min
Delta R.T.: -0.017 min
Response: 3698851
Conc: 23.05 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

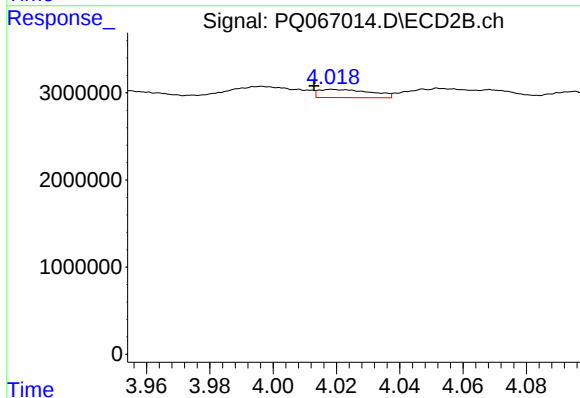


#5 AR-1016-3

R.T.: 4.019 min
Delta R.T.: 0.006 min
Response: 1084324
Conc: 6.61 ng/ml

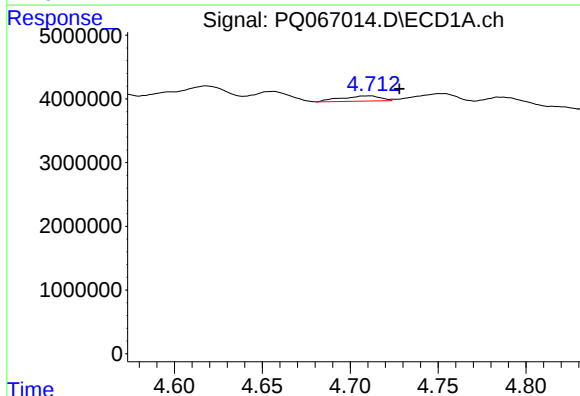


#6 AR-1016-4

R.T.: 4.711 min
Delta R.T.: -0.017 min
Response: 1286785
Conc: 10.04 ng/ml

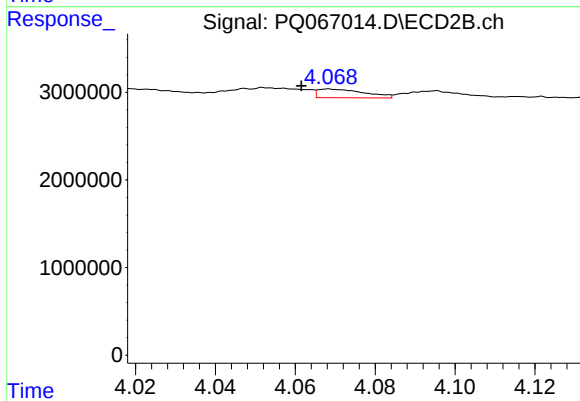

#6 AR-1016-4


R.T.: 4.068 min
Delta R.T.: 0.007 min
Response: 801599
Conc: 5.82 ng/ml

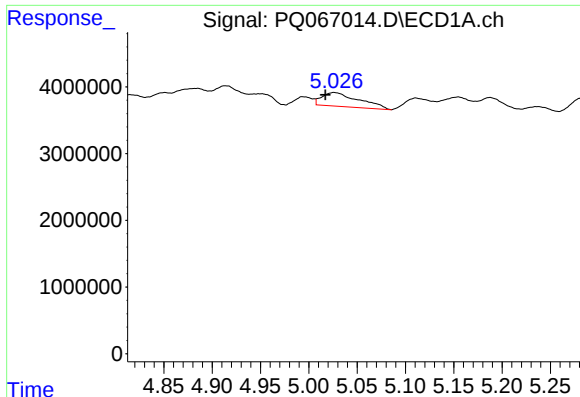

#7 AR-1016-5


R.T.: 5.026 min
Delta R.T.: 0.009 min
Response: 5510064
Conc: 42.78 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

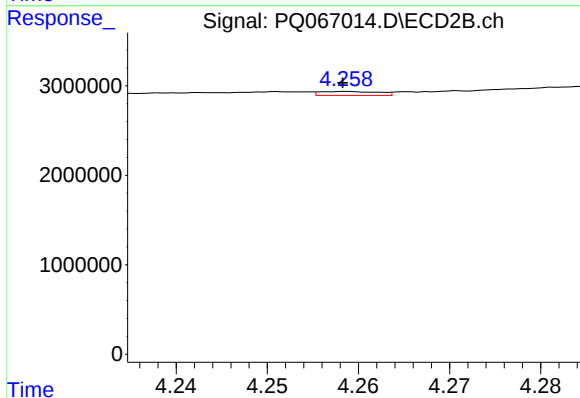


#7 AR-1016-5

R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 195756
Conc: 1.14 ng/ml

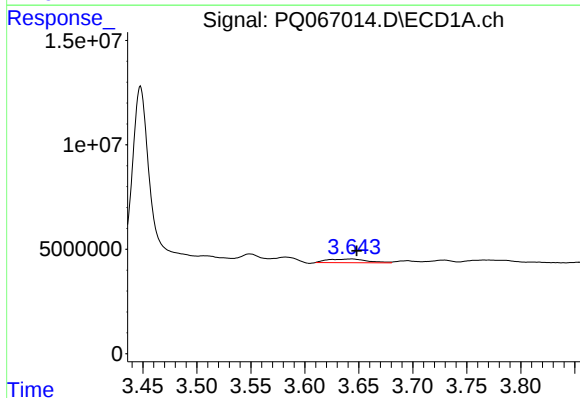


#8 AR-1221-1

R.T.: 3.643 min
Delta R.T.: -0.005 min
Response: 4446854
Conc: 67.65 ng/ml

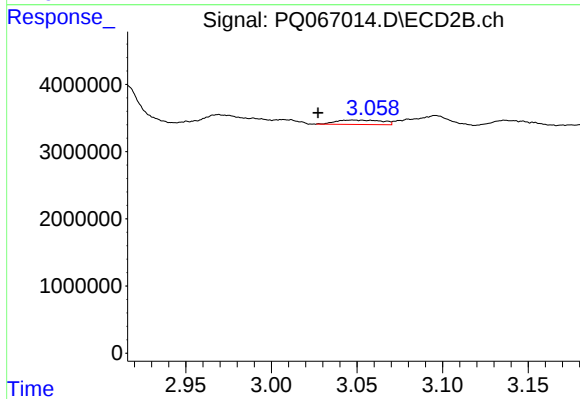

#8 AR-1221-1


R.T.: 3.048 min
Delta R.T.: 0.020 min
Response: 1231732
Conc: 15.38 ng/ml

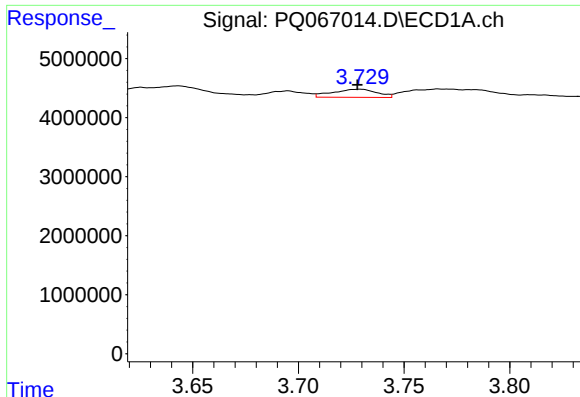

#9 AR-1221-2


R.T.: 3.729 min
Delta R.T.: 0.001 min
Response: 1998746
Conc: 41.27 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

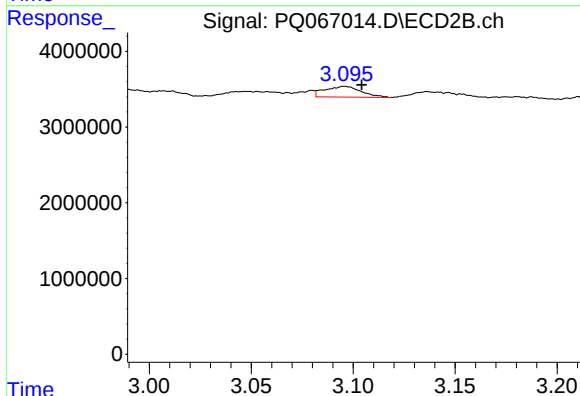


#9 AR-1221-2

R.T.: 3.096 min
Delta R.T.: -0.008 min
Response: 1762133
Conc: 33.72 ng/ml

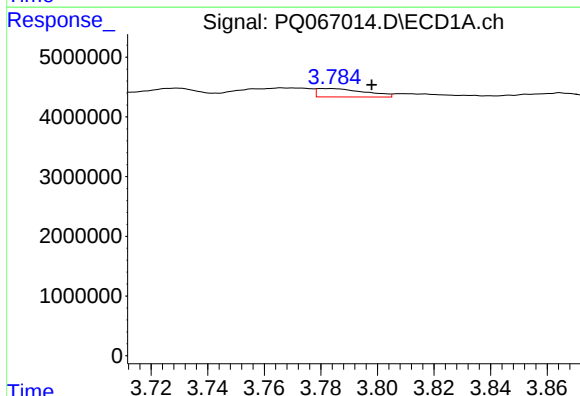


#10 AR-1221-3

R.T.: 3.783 min
Delta R.T.: -0.015 min
Response: 1641784
Conc: 10.81 ng/ml

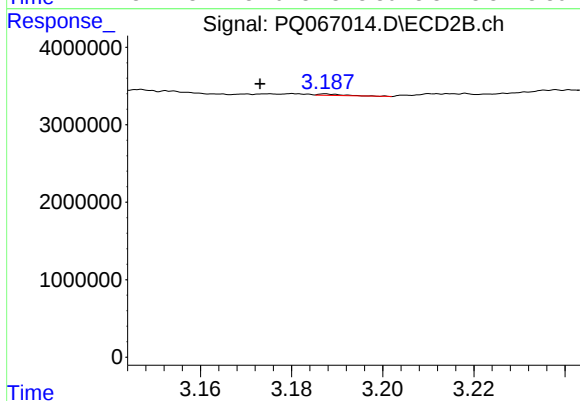

#10 AR-1221-3


R.T.: 3.188 min
Delta R.T.: 0.014 min
Response: 72014
Conc: 0.41 ng/ml

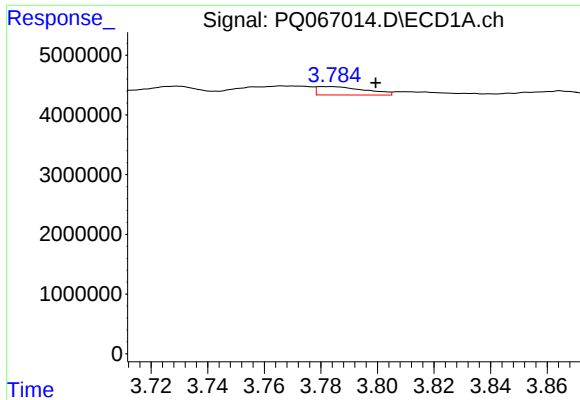

#11 AR-1232-1


R.T.: 3.783 min
Delta R.T.: -0.016 min
Response: 1641784
Conc: 13.30 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

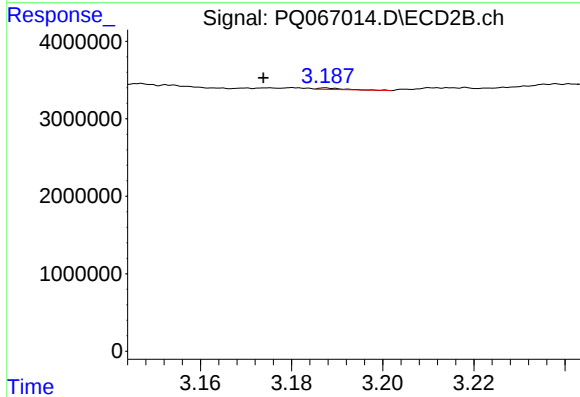


#11 AR-1232-1

R.T.: 3.188 min
Delta R.T.: 0.014 min
Response: 72014
Conc: 0.50 ng/ml

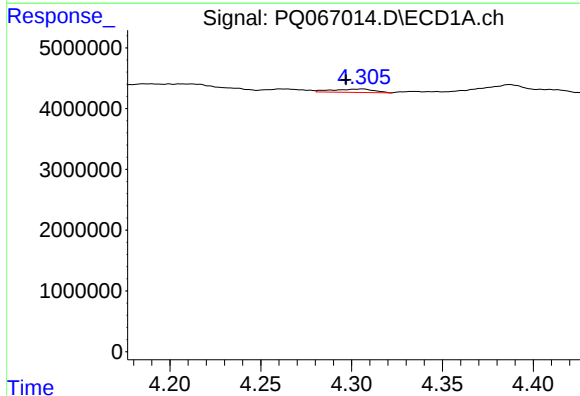


#12 AR-1232-2

R.T.: 4.306 min
Delta R.T.: 0.009 min
Response: 885945
Conc: 13.44 ng/ml

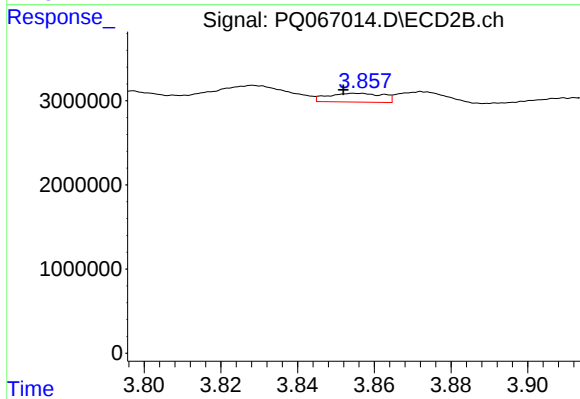

#12 AR-1232-2


R.T.: 3.855 min
Delta R.T.: 0.003 min
Response: 1041835
Conc: 7.33 ng/ml

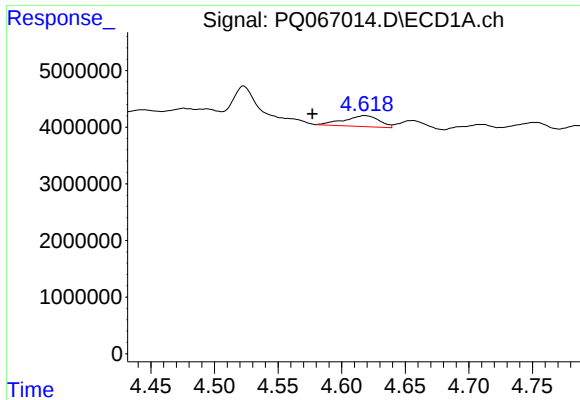

#13 AR-1232-3


R.T.: 4.618 min
Delta R.T.: 0.041 min
Response: 3698851
Conc: 30.70 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

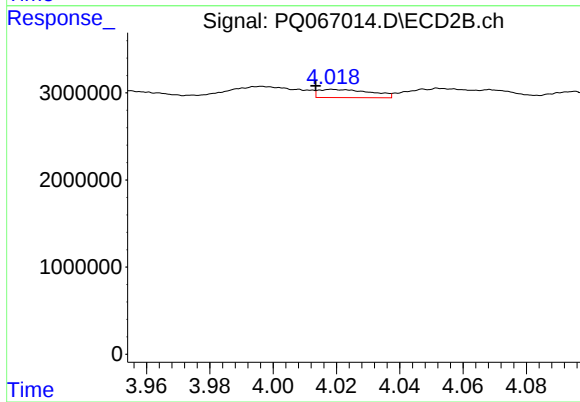


#13 AR-1232-3

R.T.: 4.019 min
Delta R.T.: 0.005 min
Response: 1084324
Conc: 13.93 ng/ml

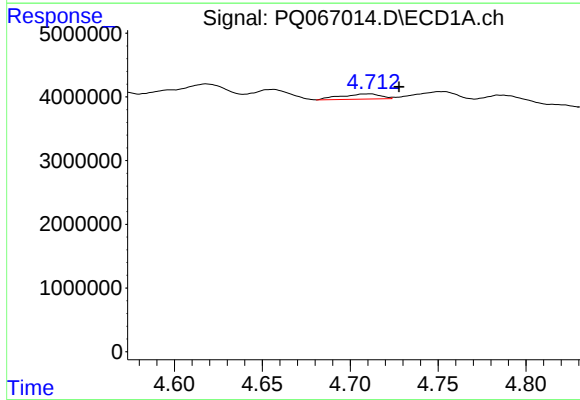


#14 AR-1232-4

R.T.: 4.711 min
Delta R.T.: -0.017 min
Response: 1286785
Conc: 22.39 ng/ml

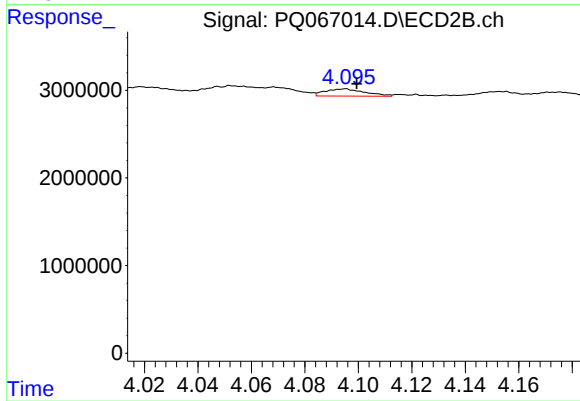

#14 AR-1232-4


R.T.: 4.095 min
Delta R.T.: -0.004 min
Response: 847577
Conc: 12.75 ng/ml

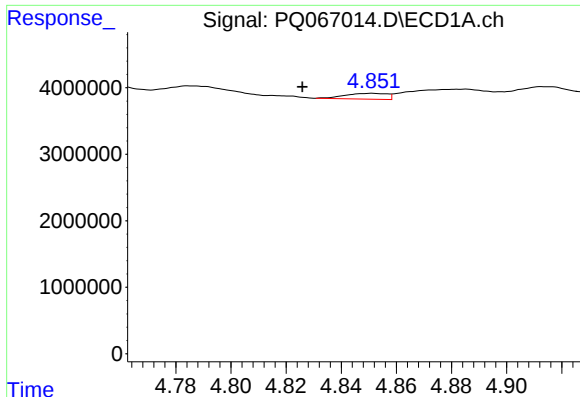

#15 AR-1232-5


R.T.: 4.851 min
Delta R.T.: 0.025 min
Response: 932657
Conc: 23.31 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

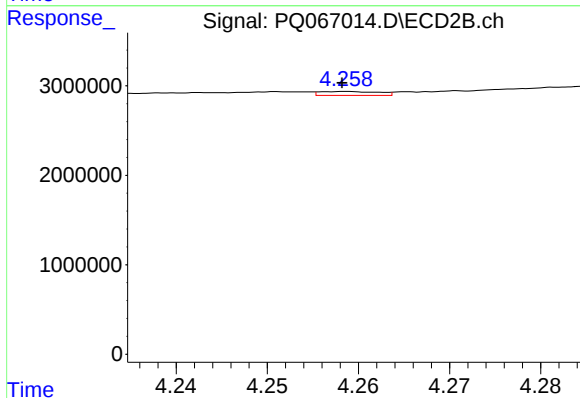


#15 AR-1232-5

R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 195756
Conc: 2.61 ng/ml

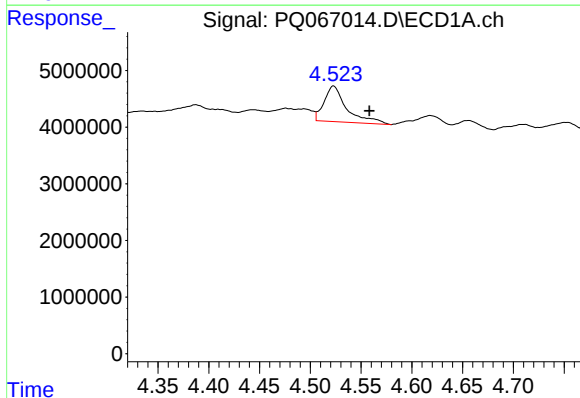


#16 AR-1242-1

R.T.: 4.523 min
Delta R.T.: -0.035 min
Response: 9752076
Conc: 68.39 ng/ml

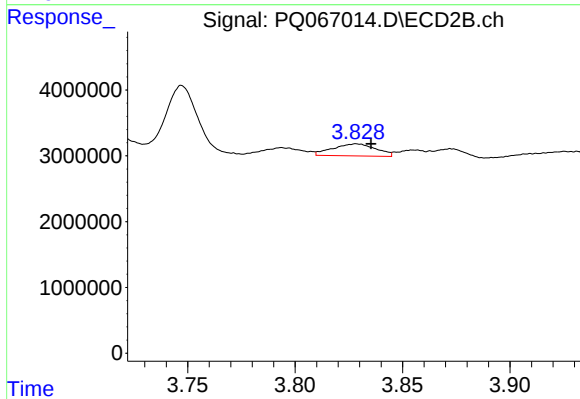

#16 AR-1242-1


R.T.: 3.828 min
Delta R.T.: -0.007 min
Response: 2576995
Conc: 14.82 ng/ml

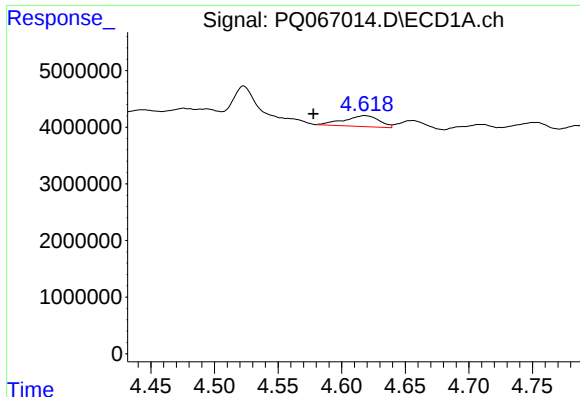

#17 AR-1242-2


R.T.: 4.618 min
Delta R.T.: 0.040 min
Response: 3698851
Conc: 16.81 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

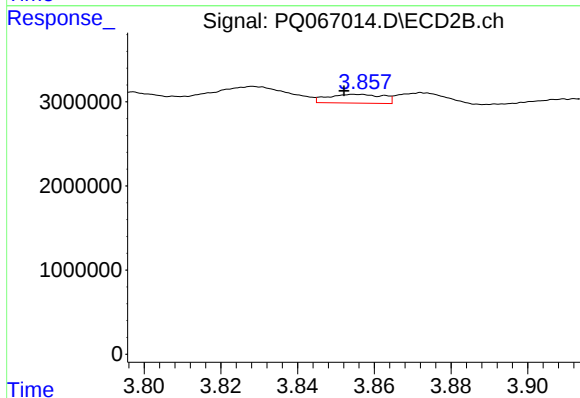


#17 AR-1242-2

R.T.: 3.855 min
Delta R.T.: 0.003 min
Response: 1041835
Conc: 4.18 ng/ml

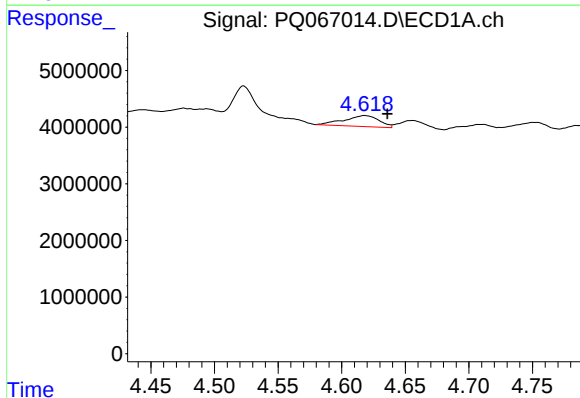


#18 AR-1242-3

R.T.: 4.618 min
Delta R.T.: -0.018 min
Response: 3698851
Conc: 27.48 ng/ml

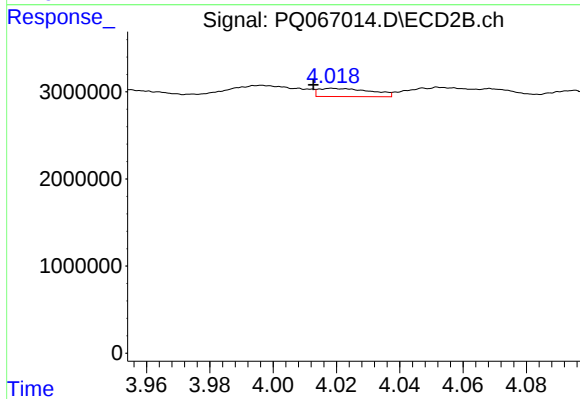

#18 AR-1242-3


R.T.: 4.019 min
Delta R.T.: 0.006 min
Response: 1084324
Conc: 7.77 ng/ml

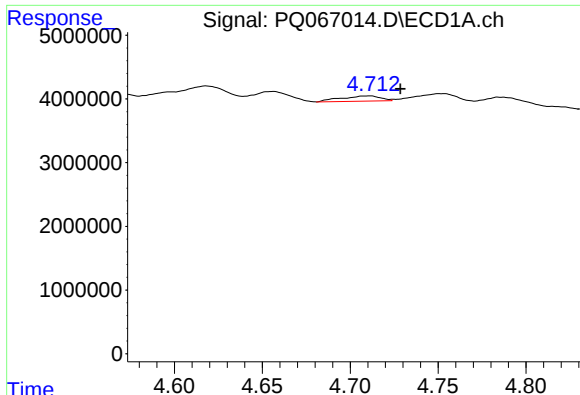

#19 AR-1242-4


R.T.: 4.711 min
Delta R.T.: -0.018 min
Response: 1286785
Conc: 12.16 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

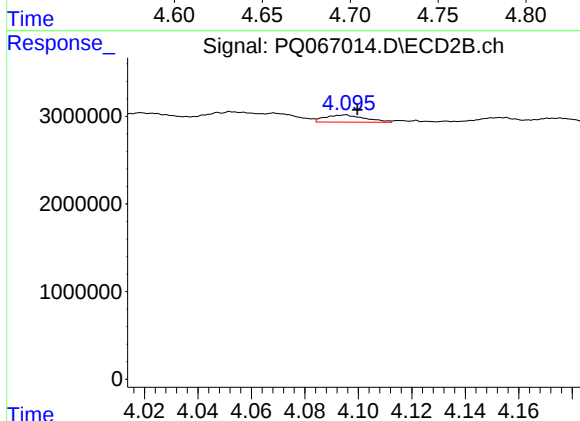


#19 AR-1242-4

R.T.: 4.095 min
Delta R.T.: -0.004 min
Response: 847577
Conc: 6.49 ng/ml

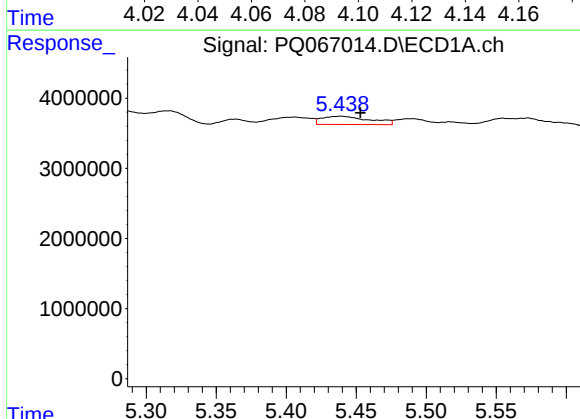


#20 AR-1242-5

R.T.: 5.439 min
Delta R.T.: -0.014 min
Response: 2813218
Conc: 24.63 ng/ml

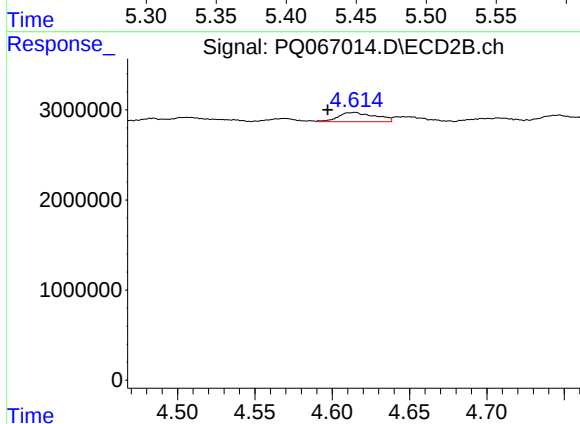

#20 AR-1242-5


R.T.: 4.615 min
Delta R.T.: 0.018 min
Response: 1686234
Conc: 10.16 ng/ml

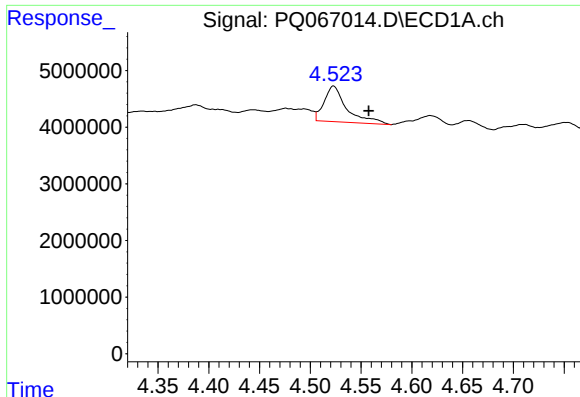

#21 AR-1248-1


R.T.: 4.523 min
Delta R.T.: -0.035 min
Response: 9752076
Conc: 92.43 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

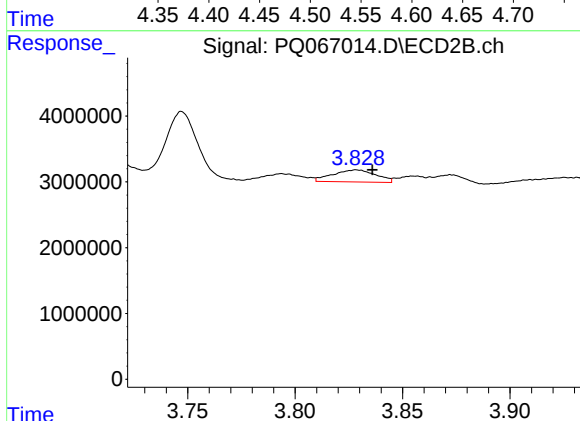


#21 AR-1248-1

R.T.: 3.828 min
Delta R.T.: -0.007 min
Response: 2576995
Conc: 20.13 ng/ml

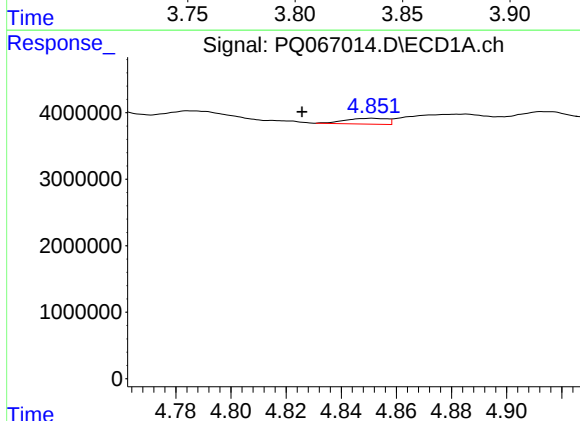


#22 AR-1248-2

R.T.: 4.851 min
Delta R.T.: 0.025 min
Response: 932657
Conc: 6.36 ng/ml

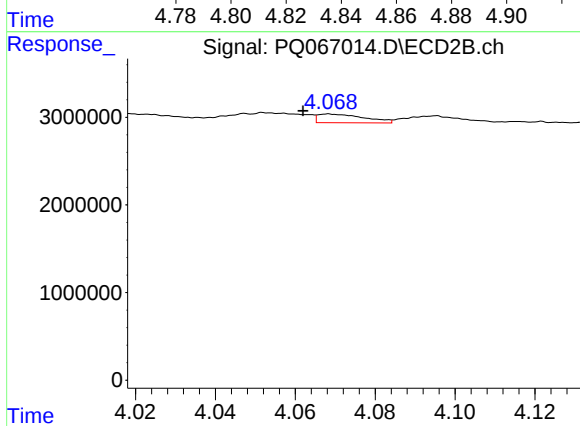

#22 AR-1248-2


R.T.: 4.068 min
Delta R.T.: 0.007 min
Response: 801599
Conc: 4.18 ng/ml

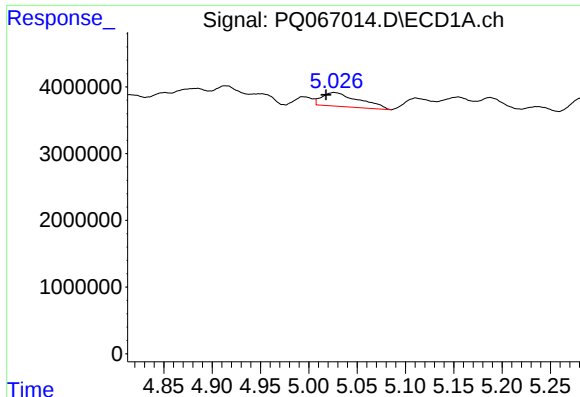

#23 AR-1248-3


R.T.: 5.026 min
Delta R.T.: 0.008 min
Response: 5510064
Conc: 31.53 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

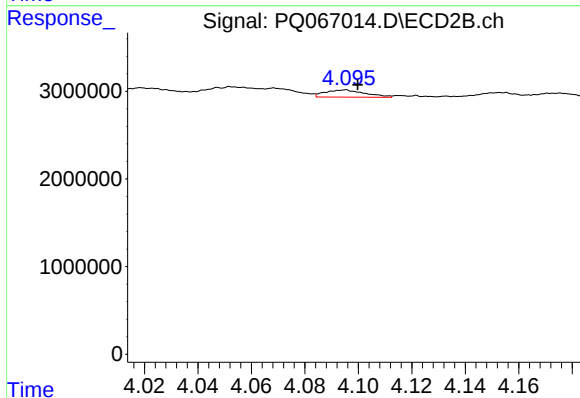


#23 AR-1248-3

R.T.: 4.095 min
Delta R.T.: -0.004 min
Response: 847577
Conc: 4.60 ng/ml

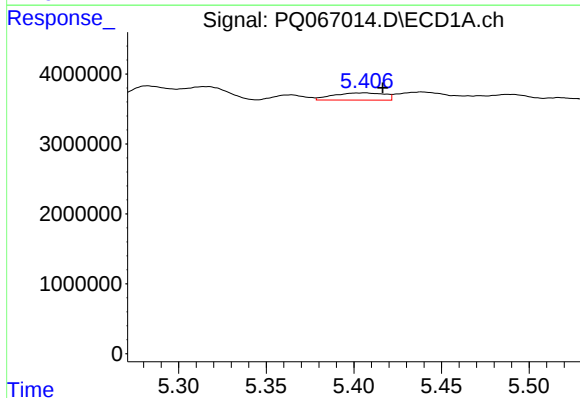


#24 AR-1248-4

R.T.: 5.406 min
Delta R.T.: -0.010 min
Response: 2082105
Conc: 10.61 ng/ml

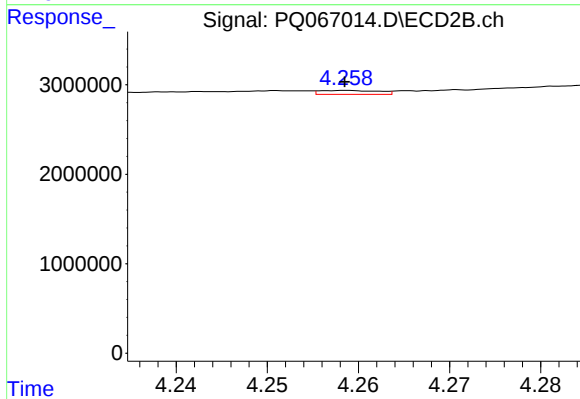

#24 AR-1248-4


R.T.: 4.259 min
Delta R.T.: 0.000 min
Response: 195756
Conc: 0.87 ng/ml

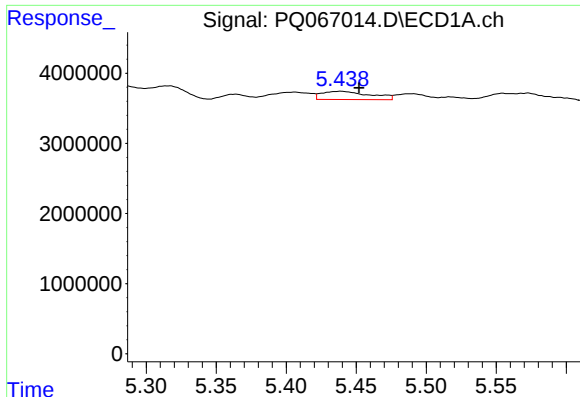

#25 AR-1248-5


R.T.: 5.439 min
Delta R.T.: -0.013 min
Response: 2813218
Conc: 14.15 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

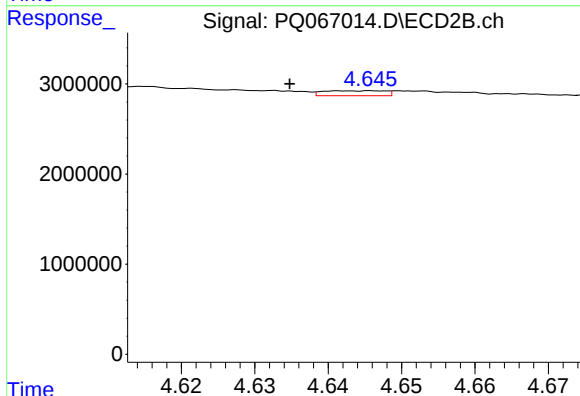


#25 AR-1248-5

R.T.: 4.642 min
Delta R.T.: 0.007 min
Response: 317015
Conc: 1.48 ng/ml

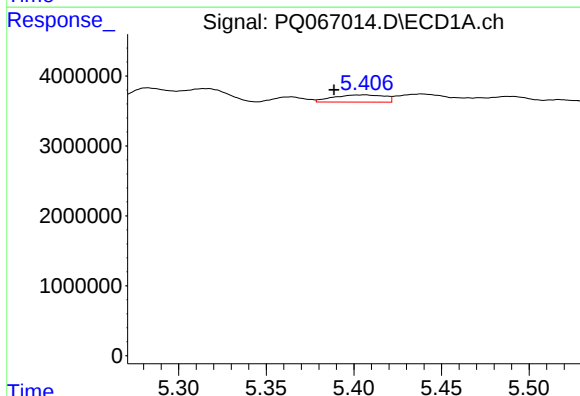


#26 AR-1254-1

R.T.: 5.406 min
Delta R.T.: 0.017 min
Response: 2082105
Conc: 10.05 ng/ml

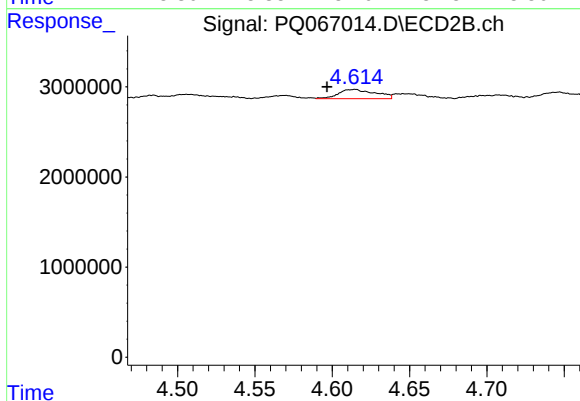

#26 AR-1254-1


R.T.: 4.615 min
Delta R.T.: 0.018 min
Response: 1686234
Conc: 5.03 ng/ml

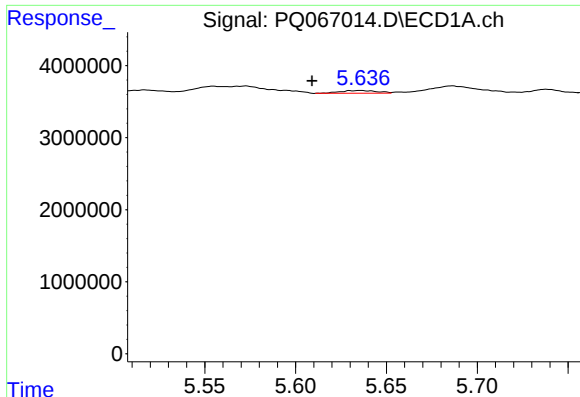

#27 AR-1254-2


R.T.: 5.636 min
Delta R.T.: 0.027 min
Response: 540937
Conc: 1.68 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

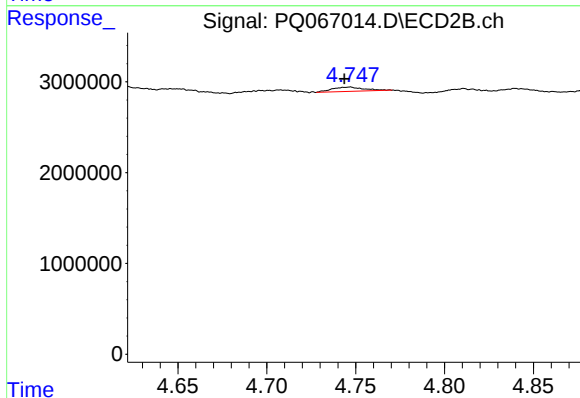


#27 AR-1254-2

R.T.: 4.747 min
Delta R.T.: 0.003 min
Response: 593175
Conc: 2.05 ng/ml

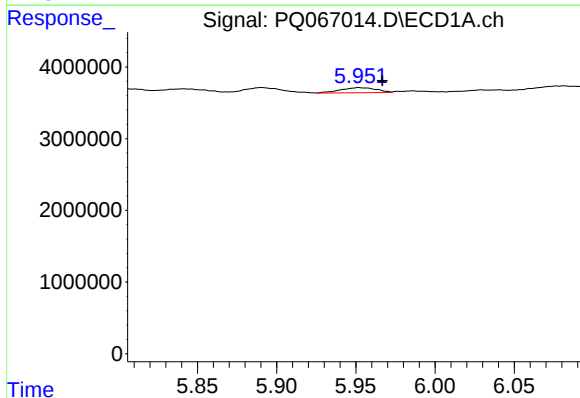


#28 AR-1254-3

R.T.: 5.952 min
Delta R.T.: -0.015 min
Response: 1121387
Conc: 3.30 ng/ml

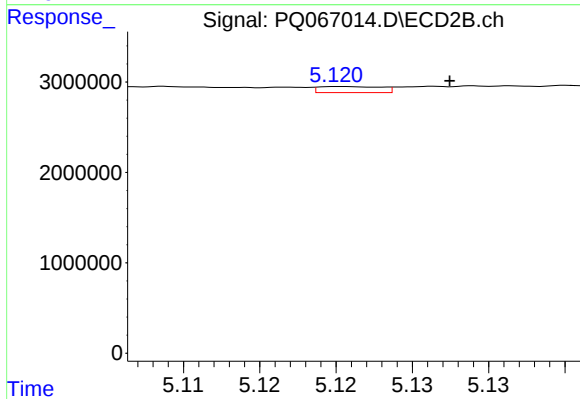

#28 AR-1254-3


R.T.: 5.121 min
Delta R.T.: -0.007 min
Response: 190258
Conc: 0.41 ng/ml

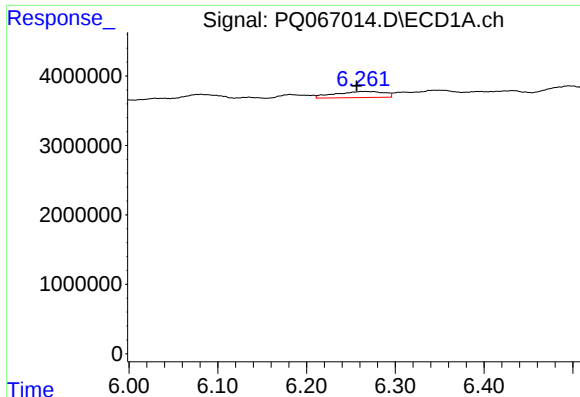

#29 AR-1254-4


R.T.: 6.266 min
Delta R.T.: 0.009 min
Response: 3410332
Conc: 14.49 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

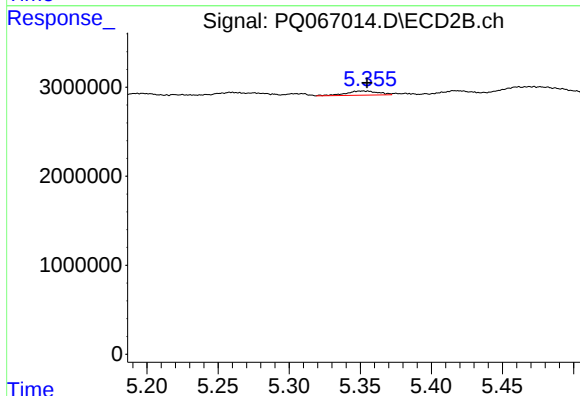


#29 AR-1254-4

R.T.: 5.352 min
Delta R.T.: -0.002 min
Response: 752935
Conc: 2.70 ng/ml

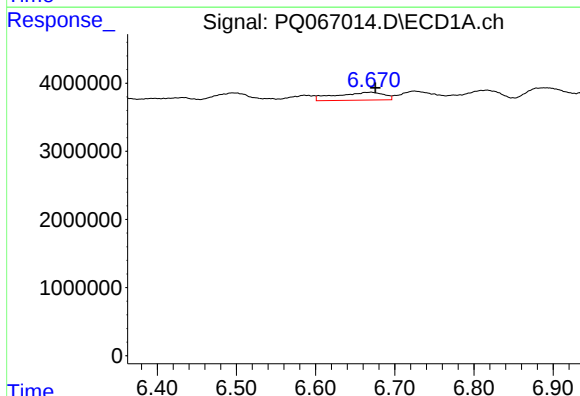


#30 AR-1254-5

R.T.: 6.670 min
Delta R.T.: -0.005 min
Response: 4834948
Conc: 18.25 ng/ml

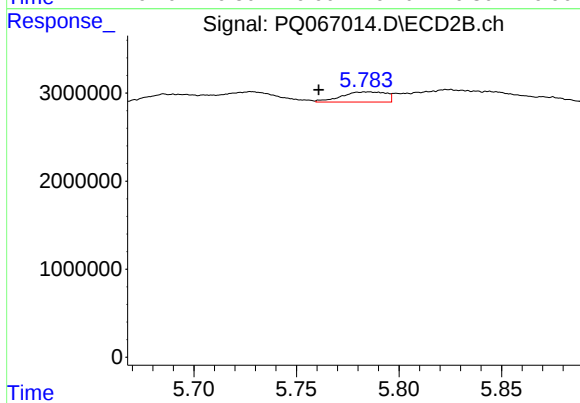

#30 AR-1254-5


R.T.: 5.786 min
Delta R.T.: 0.025 min
Response: 1738270
Conc: 4.15 ng/ml

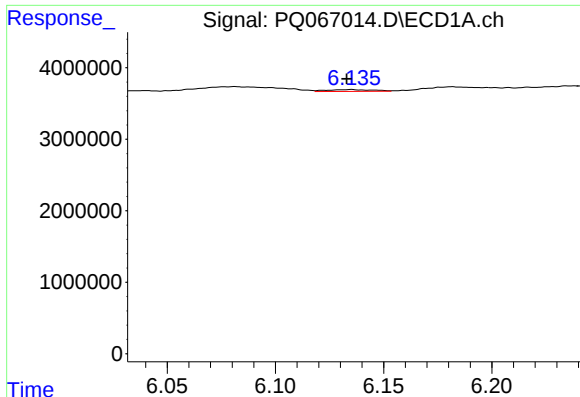

#31 AR-1260-1


R.T.: 6.135 min
Delta R.T.: 0.002 min
Response: 377837
Conc: 1.47 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

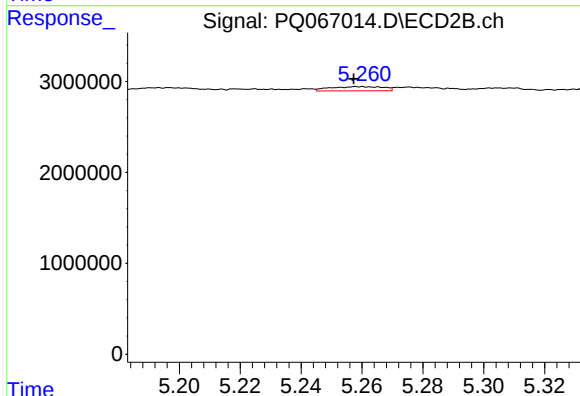


#31 AR-1260-1

R.T.: 5.260 min
Delta R.T.: 0.003 min
Response: 559606
Conc: 1.69 ng/ml

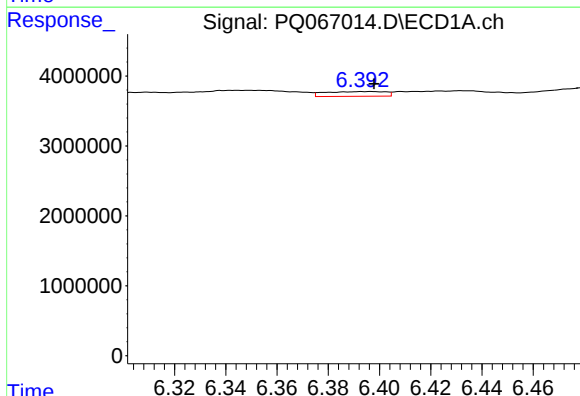


#32 AR-1260-2

R.T.: 6.397 min
Delta R.T.: -0.001 min
Response: 1109465
Conc: 3.65 ng/ml

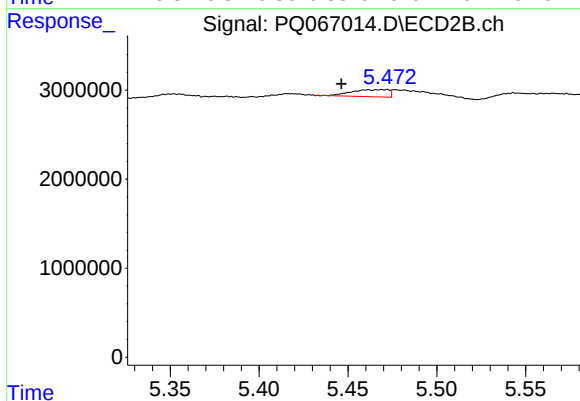

#32 AR-1260-2


R.T.: 5.472 min
Delta R.T.: 0.026 min
Response: 1160795
Conc: 2.97 ng/ml

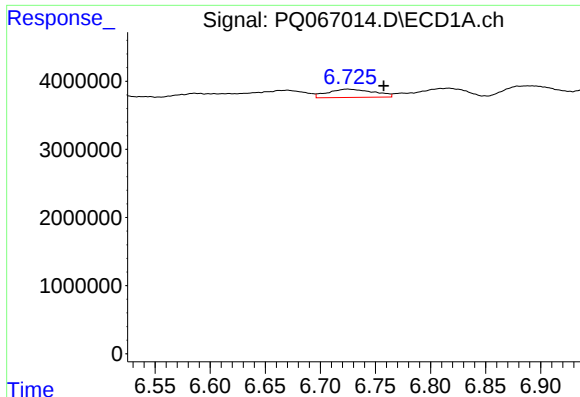

#33 AR-1260-3


R.T.: 6.724 min
Delta R.T.: -0.033 min
Response: 3502885
Conc: 15.83 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

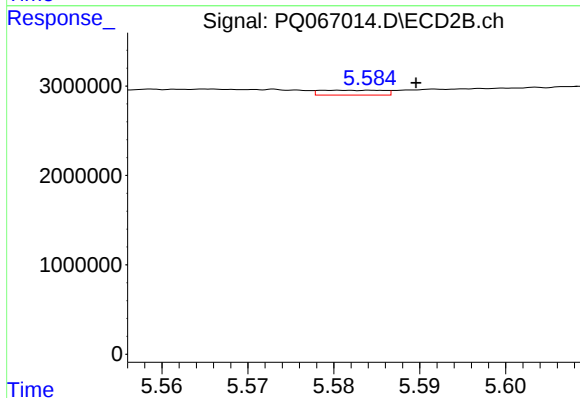


#33 AR-1260-3

R.T.: 5.585 min
Delta R.T.: -0.005 min
Response: 278954
Conc: 0.74 ng/ml

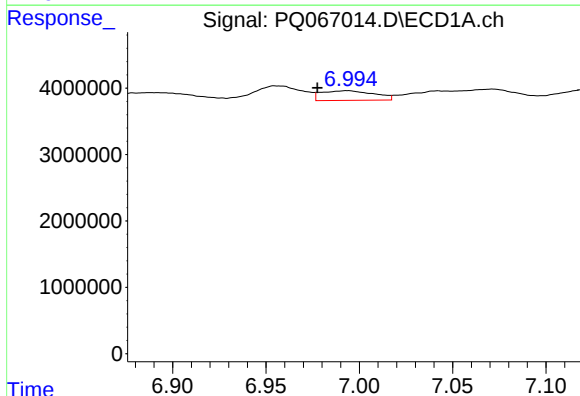


#34 AR-1260-4

R.T.: 6.994 min
Delta R.T.: 0.016 min
Response: 2831647
Conc: 11.69 ng/ml

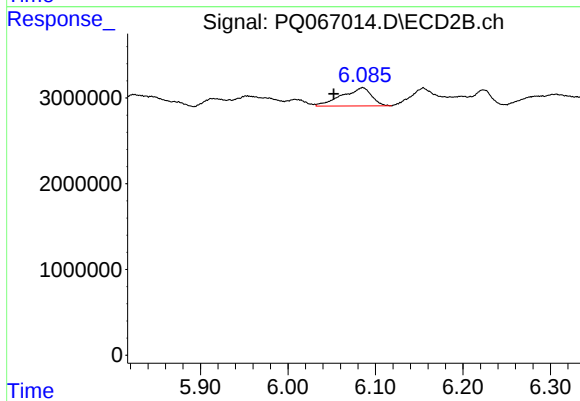

#34 AR-1260-4


R.T.: 6.085 min
Delta R.T.: 0.033 min
Response: 4994957
Conc: 15.90 ng/ml

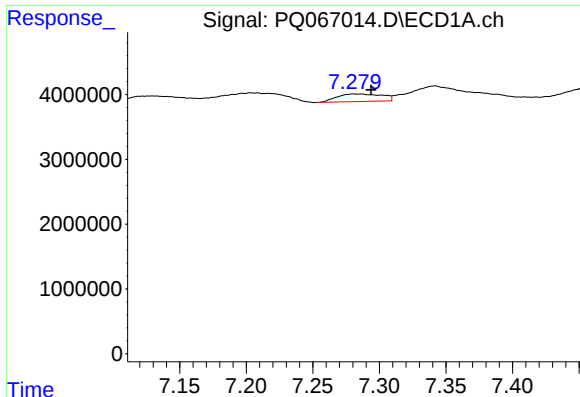

#35 AR-1260-5


R.T.: 7.281 min
Delta R.T.: -0.013 min
Response: 2751863
Conc: 5.62 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

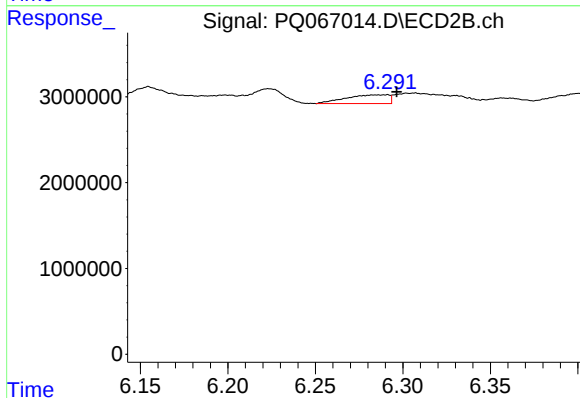


#35 AR-1260-5

R.T.: 6.291 min
Delta R.T.: -0.005 min
Response: 1732936
Conc: 2.63 ng/ml

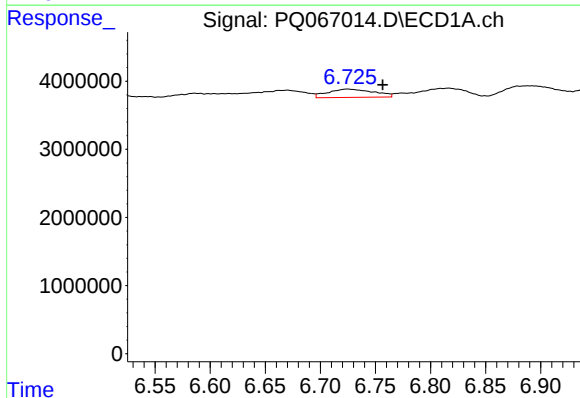


#36 AR-1262-1

R.T.: 6.724 min
Delta R.T.: -0.032 min
Response: 3502885
Conc: 10.60 ng/ml

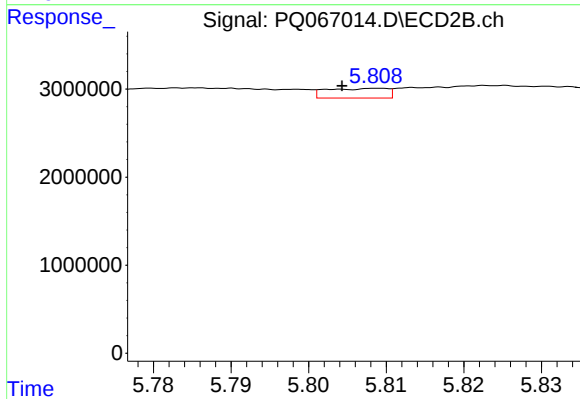

#36 AR-1262-1


R.T.: 5.809 min
Delta R.T.: 0.005 min
Response: 596459
Conc: 1.38 ng/ml

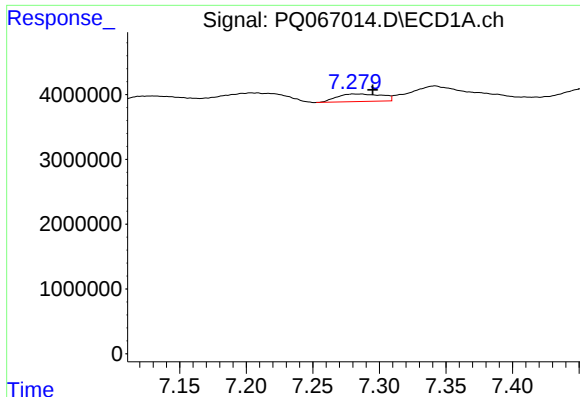

#37 AR-1262-2


R.T.: 7.281 min
Delta R.T.: -0.014 min
Response: 2751863
Conc: 5.14 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

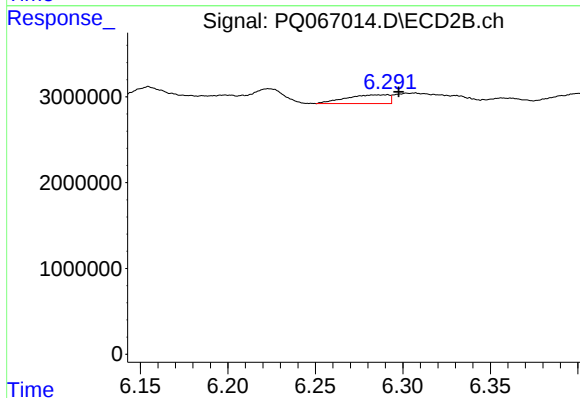


#37 AR-1262-2

R.T.: 6.291 min
Delta R.T.: -0.006 min
Response: 1732936
Conc: 2.38 ng/ml

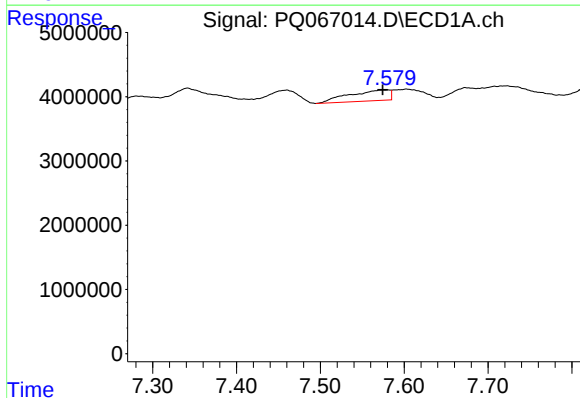


#38 AR-1262-3

R.T.: 7.580 min
Delta R.T.: 0.005 min
Response: 5615045
Conc: 15.98 ng/ml

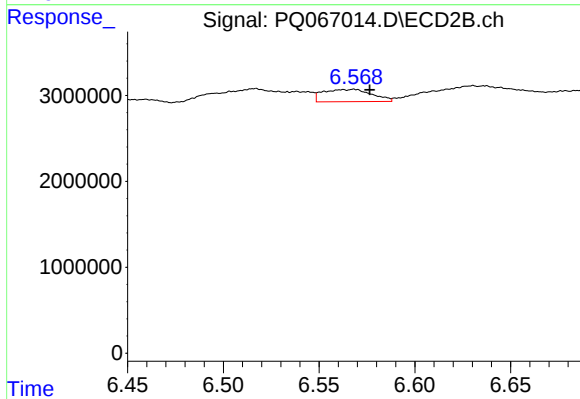

#38 AR-1262-3


R.T.: 6.568 min
Delta R.T.: -0.008 min
Response: 2545498
Conc: 8.17 ng/ml

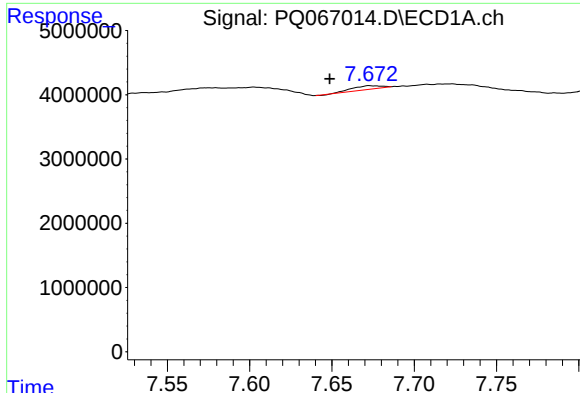

#39 AR-1262-4


R.T.: 7.673 min
Delta R.T.: 0.024 min
Response: 677214
Conc: 2.51 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

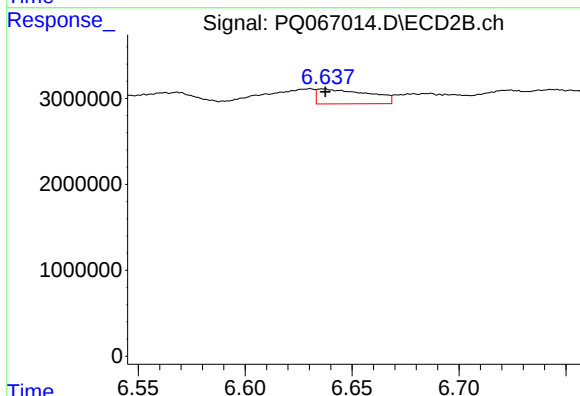


#39 AR-1262-4

R.T.: 6.637 min
Delta R.T.: 0.000 min
Response: 2903288
Conc: 5.09 ng/ml

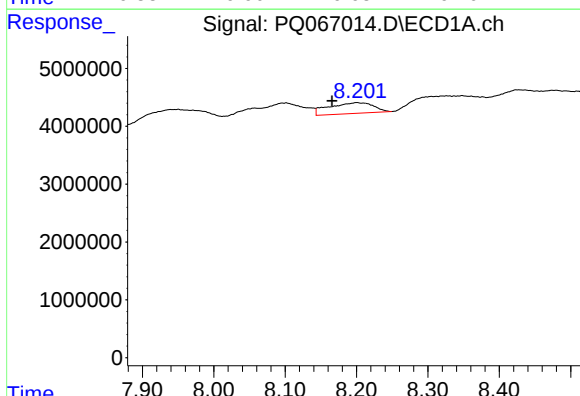


#40 AR-1262-5

R.T.: 8.200 min
Delta R.T.: 0.035 min
Response: 8026227
Conc: 47.94 ng/ml

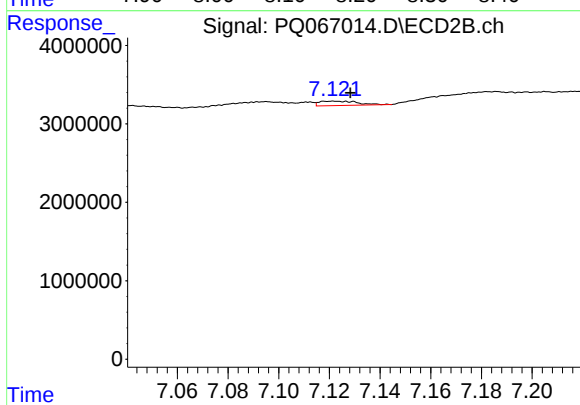

#40 AR-1262-5


R.T.: 7.122 min
Delta R.T.: -0.007 min
Response: 589584
Conc: 2.27 ng/ml

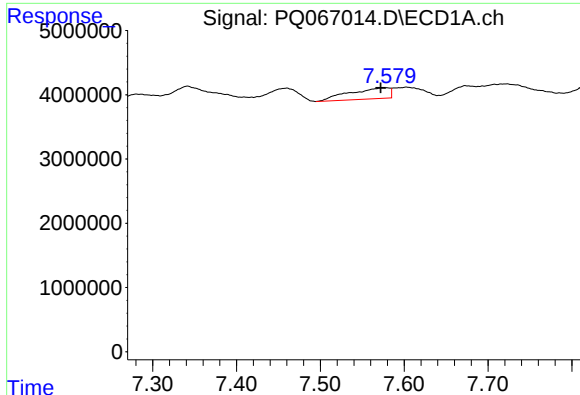

#41 AR-1268-1


R.T.: 7.580 min
Delta R.T.: 0.008 min
Response: 5615045
Conc: 9.35 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

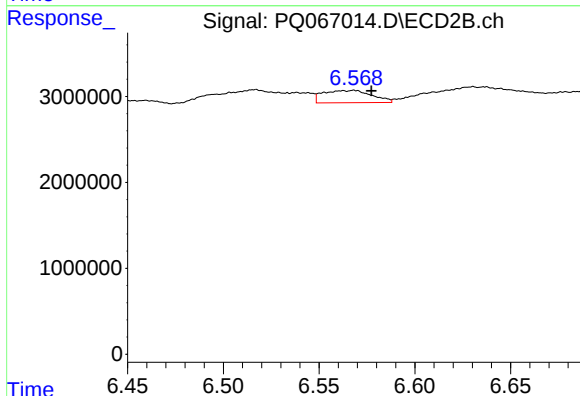


#41 AR-1268-1

R.T.: 6.568 min
Delta R.T.: -0.009 min
Response: 2545498
Conc: 2.90 ng/ml

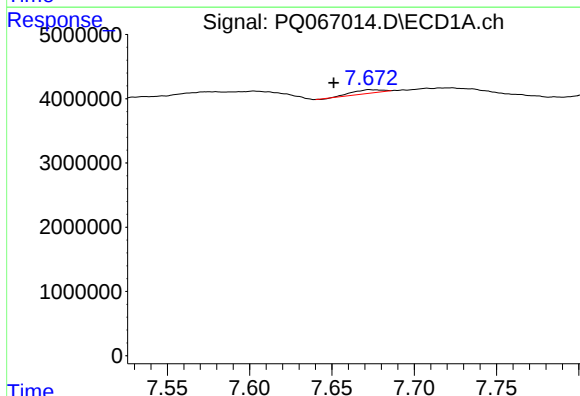


#42 AR-1268-2

R.T.: 7.673 min
Delta R.T.: 0.022 min
Response: 677214
Conc: 1.25 ng/ml

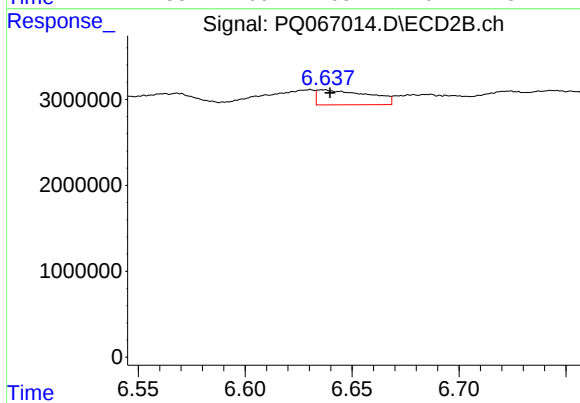

#42 AR-1268-2


R.T.: 6.637 min
Delta R.T.: -0.002 min
Response: 2903288
Conc: 3.63 ng/ml

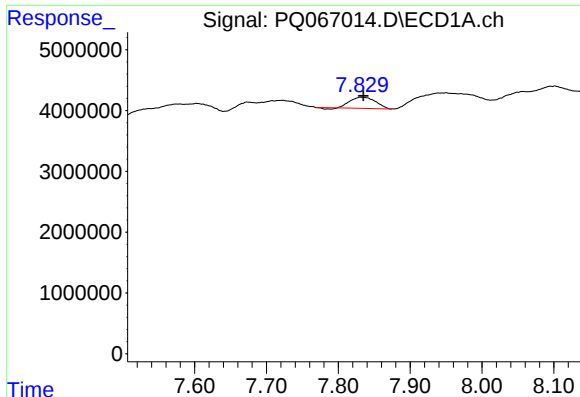

#43 AR-1268-3


R.T.: 7.831 min
Delta R.T.: -0.004 min
Response: 4356805
Conc: 9.35 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

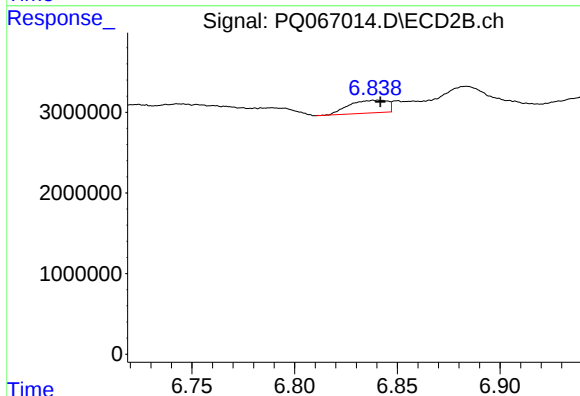


#43 AR-1268-3

R.T.: 6.841 min
Delta R.T.: 0.000 min
Response: 2044904
Conc: 2.95 ng/ml

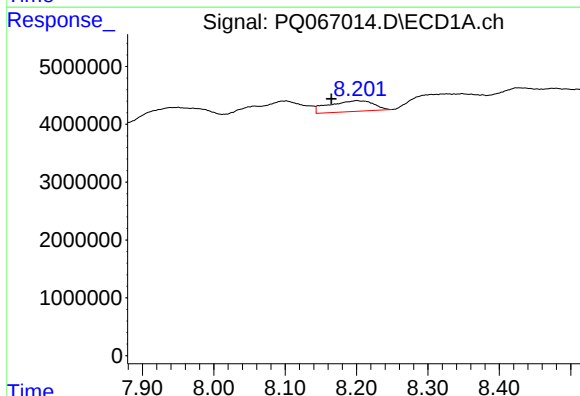


#44 AR-1268-4

R.T.: 8.200 min
Delta R.T.: 0.036 min
Response: 8026227
Conc: 45.55 ng/ml

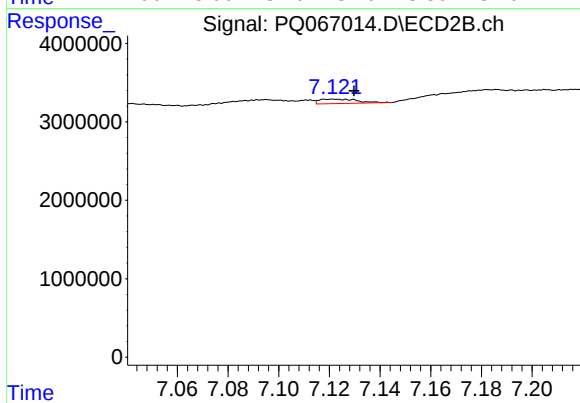

#44 AR-1268-4


R.T.: 7.122 min
Delta R.T.: -0.008 min
Response: 589584
Conc: 2.08 ng/ml

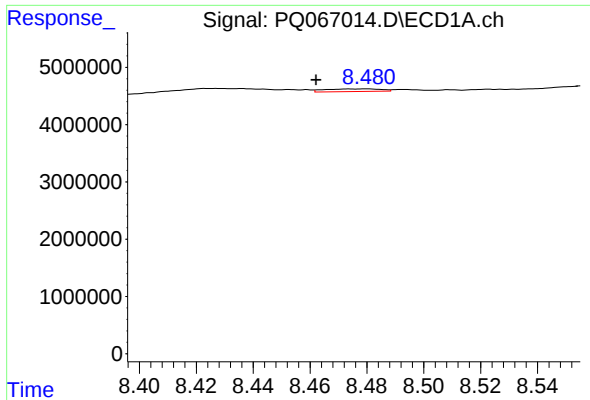

#45 AR-1268-5

R.T.: 8.480 min
Delta R.T.: 0.018 min
Response: 648102
Conc: 0.49 ng/ml

Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION

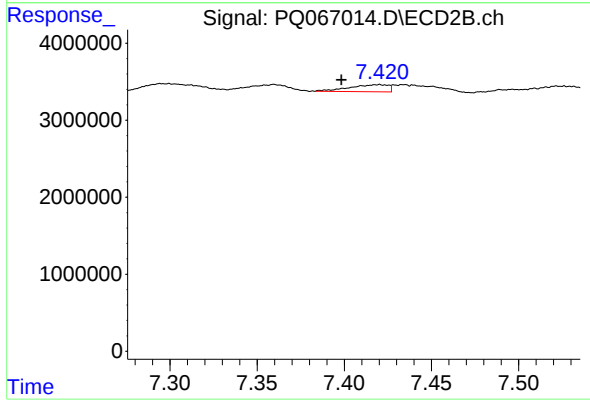

#45 AR-1268-5

R.T.: 7.420 min
Delta R.T.: 0.022 min
Response: 1423080
Conc: 0.70 ng/ml