

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060724\
 Data File : PQ067015.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2024 18:02
 Operator : YP\AJ
 Sample : P2764-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 H-1308-ESSEX-SWITCHING-STATION

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 22:29:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ053124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 03 10:00:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.452	2.832	69593135	65591649	12.565	11.213
2)	SA Decachlor...	8.711	7.616	65092882	64076106	17.165	11.157 #
Target Compounds							
3)	L1 AR-1016-1	4.585f	3.835	2989100	7711871	17.658	37.722 #
4)	L1 AR-1016-2	4.585	3.860	2989100	1423587	11.358	4.798 #
5)	L1 AR-1016-3	4.643	4.005	3061535	2343864	19.076	14.279 #
6)	L1 AR-1016-4	4.713	4.057	826098	4173815	6.446	30.302 #
7)	L1 AR-1016-5	5.029	4.260	959243	618257	7.448	3.603 #
8)	L2 AR-1221-1	3.662	3.048	1163922	231460	17.706	2.890 #
9)	L2 AR-1221-2	3.732	3.099	2160284	1809028	44.604	34.618
10)	L2 AR-1221-3	3.801	3.182	894398	92269	5.890	0.528 #
11)	L3 AR-1232-1	3.801	3.182	894398	92269	7.245	0.640 #
12)	L3 AR-1232-2	4.302	3.860	789434	1423587	11.972	10.020
13)	L3 AR-1232-3	4.585	4.005	2989100	2343864	24.806	30.108
14)	L3 AR-1232-4	4.713	4.110	826098	2386570	14.372	35.889 #
15)	L3 AR-1232-5	4.818	4.260	2319471	618257	57.978	8.246 #
16)	L4 AR-1242-1	4.585f	3.835	2989100	7711871	20.962	44.336 #
17)	L4 AR-1242-2	4.585	3.860	2989100	1423587	13.584	5.712 #
18)	L4 AR-1242-3	4.643	4.005	3061535	2343864	22.744	16.795 #
19)	L4 AR-1242-4	4.713	4.110	826098	2386570	7.806	18.272 #
20)	L4 AR-1242-5	5.460	4.611	976363	4073078	8.548	24.536 #
21)	L5 AR-1248-1	4.585f	3.835	2989100	7711871	28.331	60.248 #
22)	L5 AR-1248-2	4.818	4.057	2319471	4173815	15.819	21.778 #
23)	L5 AR-1248-3	5.029	4.110	959243	2386570	5.488	12.966 #
24)	L5 AR-1248-4	5.397	4.260	2589294	618257	13.201	2.740 #
25)	L5 AR-1248-5	5.460	4.646	976363	1598507	4.912	7.470 #
26)	L6 AR-1254-1	5.397	4.611	2589294	4073078	12.495	12.146
27)	L6 AR-1254-2	5.629	4.743	2937280	974668	9.105	3.376 #
28)	L6 AR-1254-3	5.951	5.140	2183827	3761334	6.434	8.091 #
29)	L6 AR-1254-4	6.260	5.346	606043	1303357	2.574	4.679 #
30)	L6 AR-1254-5	6.677	5.760	3201084	1029398	12.082	2.456 #
31)	L7 AR-1260-1	6.159f	5.267	1715005	244522	6.651	0.739 #
32)	L7 AR-1260-2	6.389	5.429	2470090	357578	8.126	0.915 #
33)	L7 AR-1260-3	6.763	5.616f	808961	2754848	3.656	7.271 #
34)	L7 AR-1260-4	6.950f	6.054	6105966	291514	25.206	0.928 #
35)	L7 AR-1260-5	7.299	6.301	580318	154932	1.186	0.235 #
36)	L8 AR-1262-1	6.763	5.811	808961	323774	2.447	0.749 #
37)	L8 AR-1262-2	7.299	6.301	580318	154932	1.083	0.213 #
38)	L8 AR-1262-3	7.571	6.575	128960	547123	0.367	1.757 #
39)	L8 AR-1262-4	7.604f	6.646	546076	145342	2.023	0.255 #
40)	L8 AR-1262-5	8.169	7.122	450369	188579	2.690	0.727 #
41)	L9 AR-1268-1	7.571	6.575	128960	547123	0.215	0.624 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060724\
 Data File : PQ067015.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2024 18:02
 Operator : YP\AJ
 Sample : P2764-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 H-1308-ESSEX-SWITCHING-STATION

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 22:29:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ053124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 03 10:00:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	7.604f	6.646	546076	145342	1.011	0.182 #
43) L9	AR-1268-3	7.816	6.849	993649	739554	2.132	1.066 #
44) L9	AR-1268-4	8.169	7.122	450369	188579	2.556	0.665 #
45) L9	AR-1268-5	8.468	7.395	764945	328827	0.572	0.161 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060724\
Data File : PQ067015.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2024 18:02
Operator : YP\AJ
Sample : P2764-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 22:29:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ053124.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 03 10:00:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

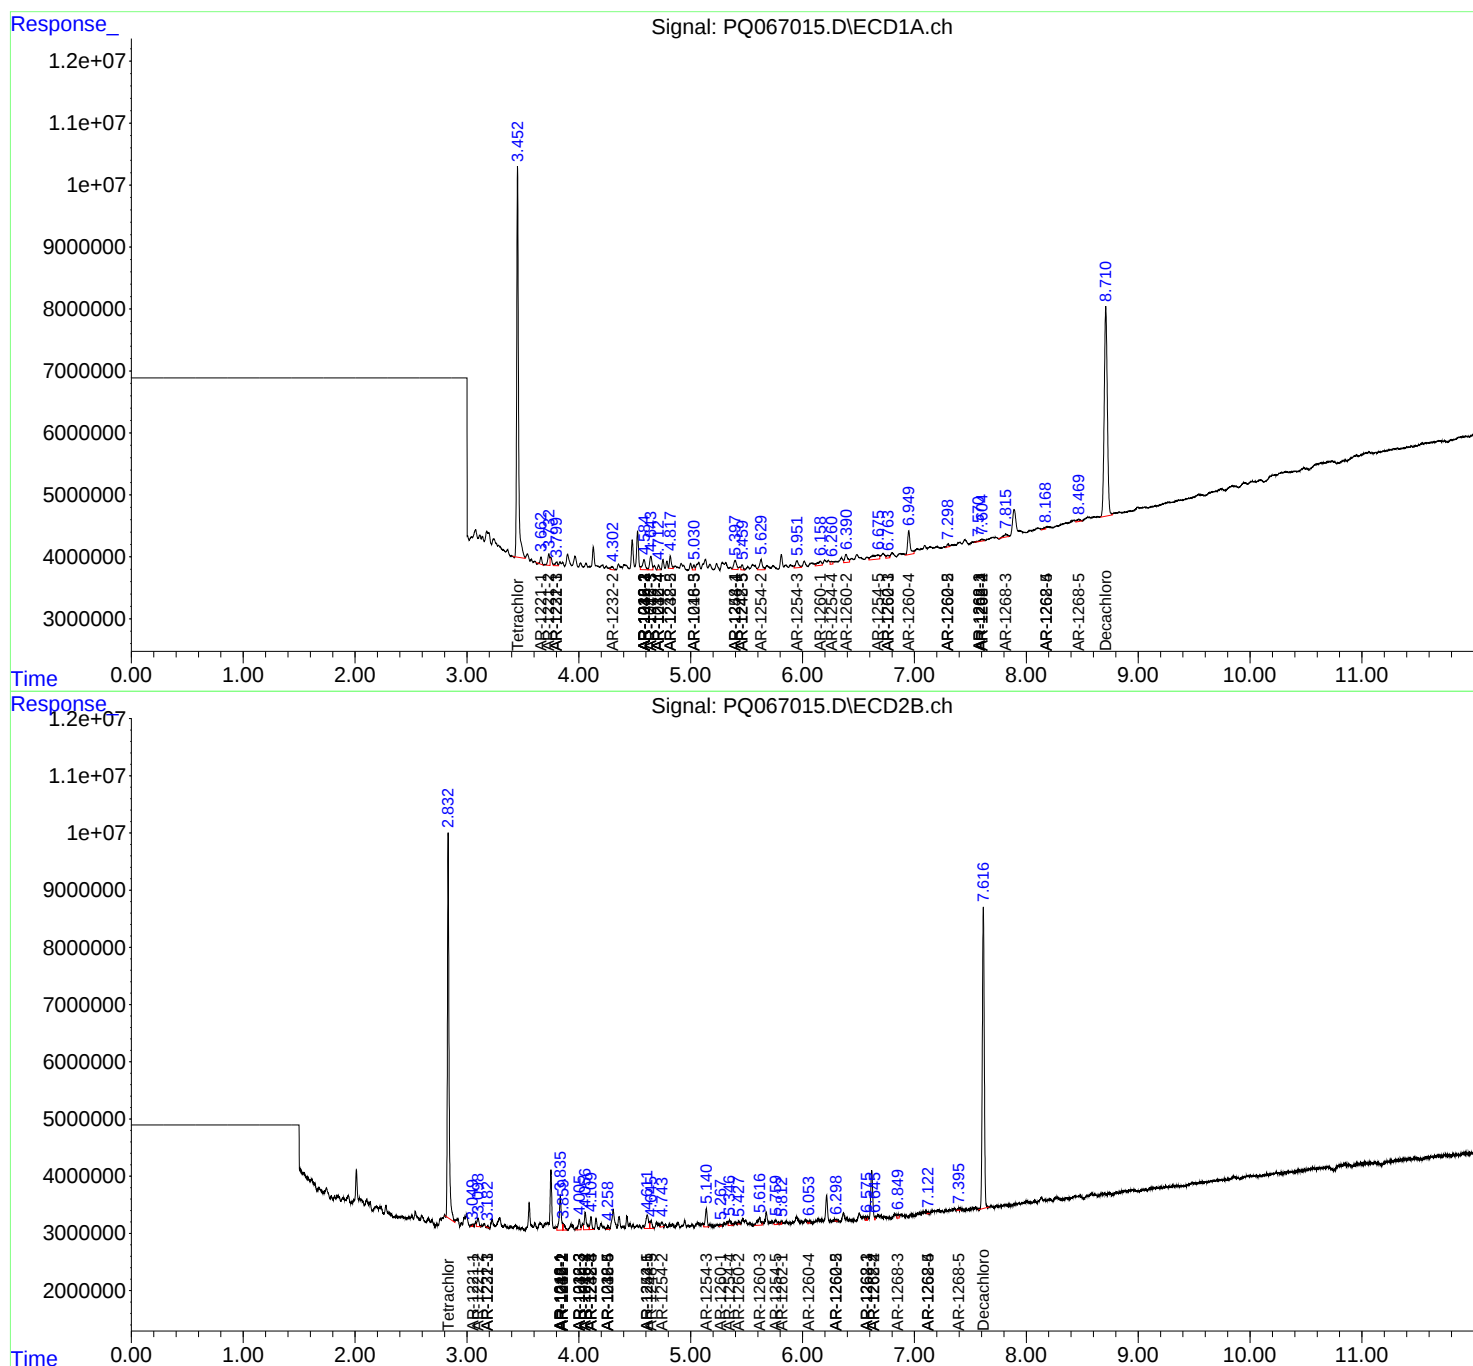


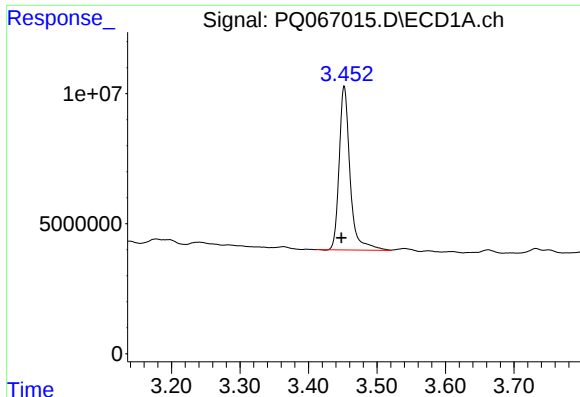

#1 Tetrachloro-m-xylene


R.T.: 3.452 min
Delta R.T.: 0.004 min
Response: 69593135
Conc: 12.57 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

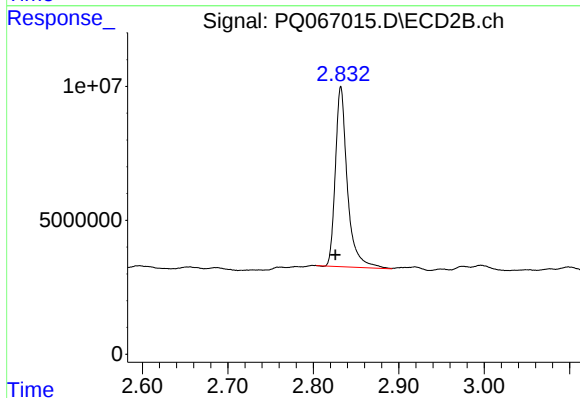


#1 Tetrachloro-m-xylene

R.T.: 2.832 min
Delta R.T.: 0.006 min
Response: 65591649
Conc: 11.21 ng/ml

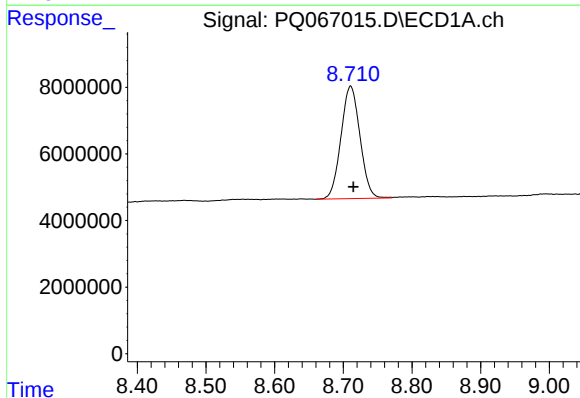


#2 Decachlorobiphenyl

R.T.: 8.711 min
Delta R.T.: -0.004 min
Response: 65092882
Conc: 17.16 ng/ml

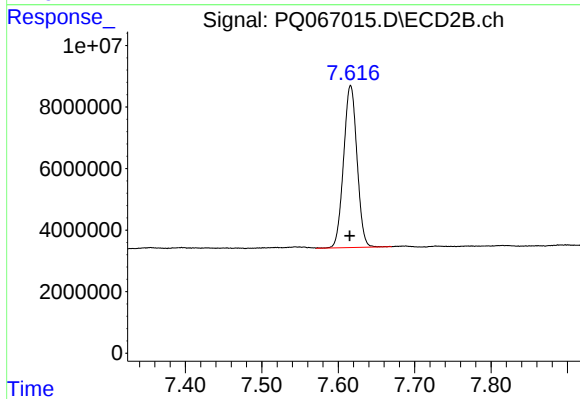

#2 Decachlorobiphenyl


R.T.: 7.616 min
Delta R.T.: 0.001 min
Response: 64076106
Conc: 11.16 ng/ml

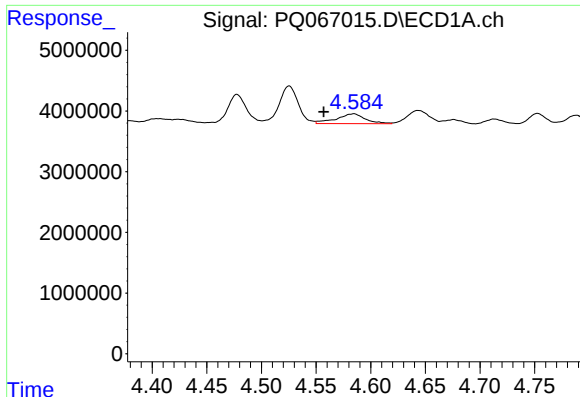

#3 AR-1016-1


R.T.: 4.585 min
Delta R.T.: 0.028 min
Response: 2989100
Conc: 17.66 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

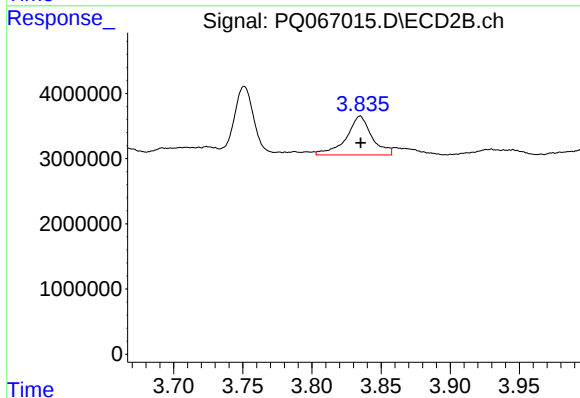


#3 AR-1016-1

R.T.: 3.835 min
Delta R.T.: 0.000 min
Response: 7711871
Conc: 37.72 ng/ml

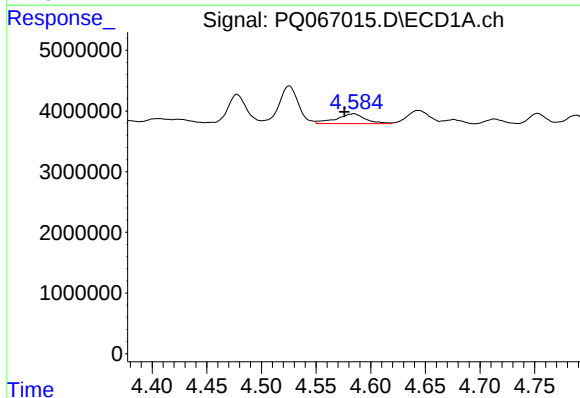


#4 AR-1016-2

R.T.: 4.585 min
Delta R.T.: 0.009 min
Response: 2989100
Conc: 11.36 ng/ml

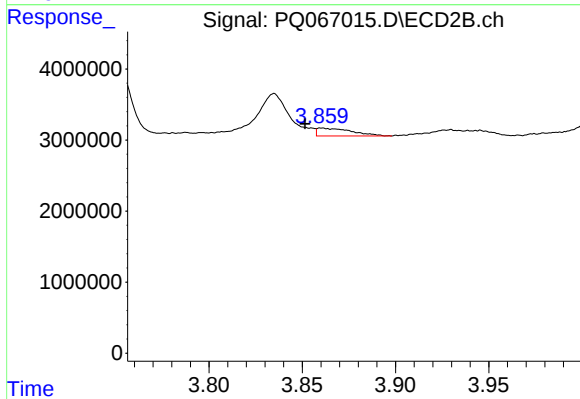

#4 AR-1016-2


R.T.: 3.860 min
Delta R.T.: 0.009 min
Response: 1423587
Conc: 4.80 ng/ml

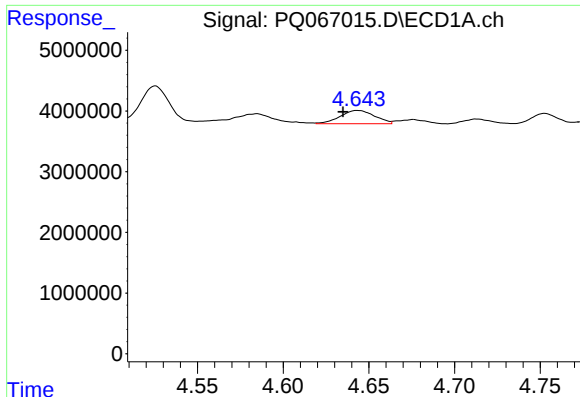

#5 AR-1016-3


R.T.: 4.643 min
Delta R.T.: 0.008 min
Response: 3061535
Conc: 19.08 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

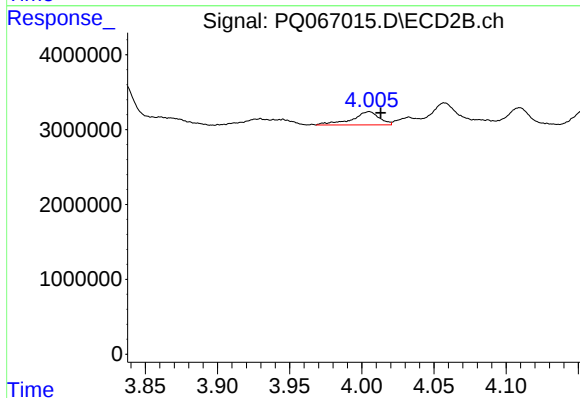


#5 AR-1016-3

R.T.: 4.005 min
Delta R.T.: -0.008 min
Response: 2343864
Conc: 14.28 ng/ml

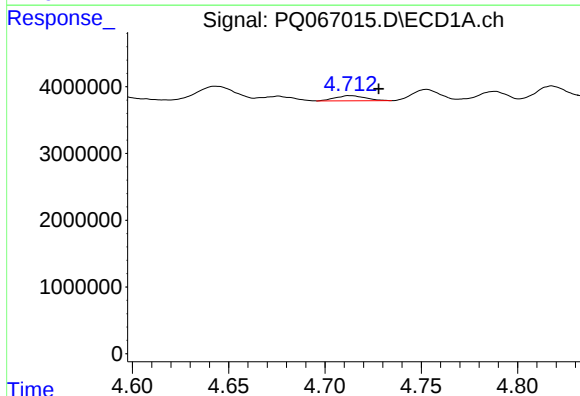


#6 AR-1016-4

R.T.: 4.713 min
Delta R.T.: -0.015 min
Response: 826098
Conc: 6.45 ng/ml

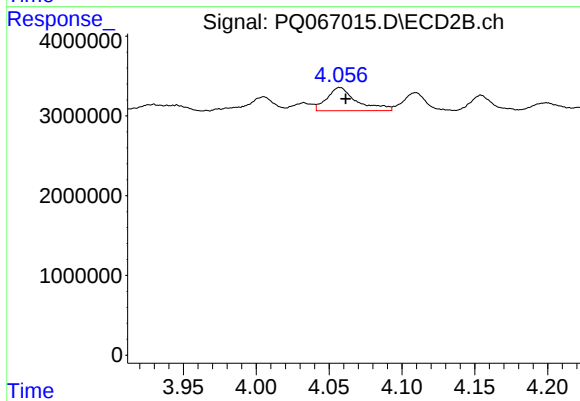

#6 AR-1016-4


R.T.: 4.057 min
Delta R.T.: -0.004 min
Response: 4173815
Conc: 30.30 ng/ml

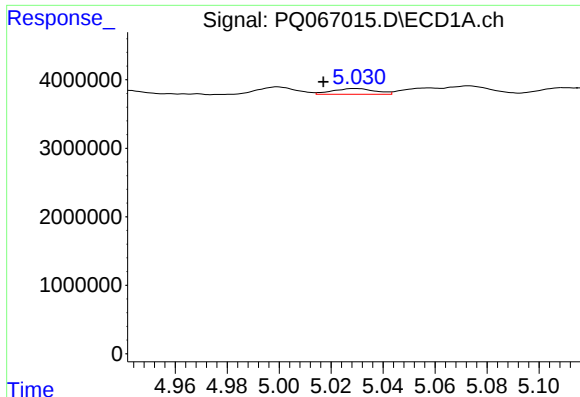

#7 AR-1016-5


R.T.: 5.029 min
Delta R.T.: 0.012 min
Response: 959243
Conc: 7.45 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

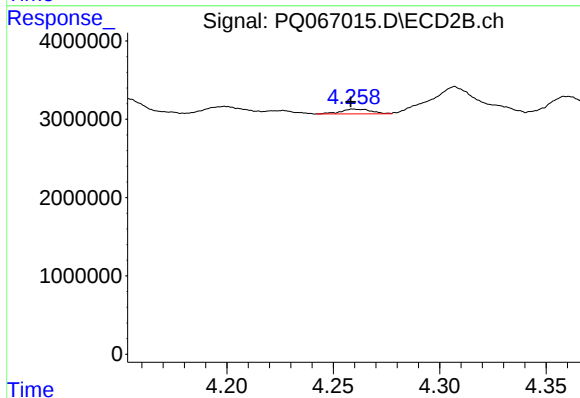


#7 AR-1016-5

R.T.: 4.260 min
Delta R.T.: 0.001 min
Response: 618257
Conc: 3.60 ng/ml

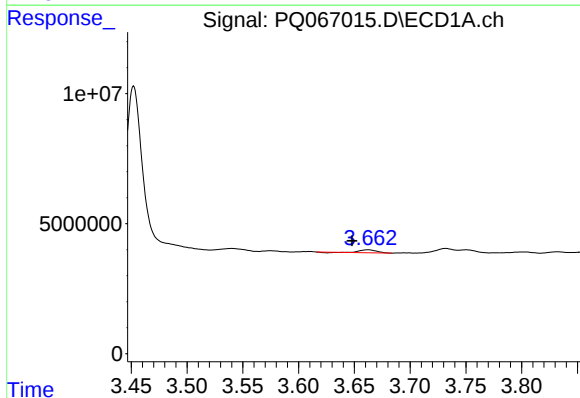


#8 AR-1221-1

R.T.: 3.662 min
Delta R.T.: 0.014 min
Response: 1163922
Conc: 17.71 ng/ml

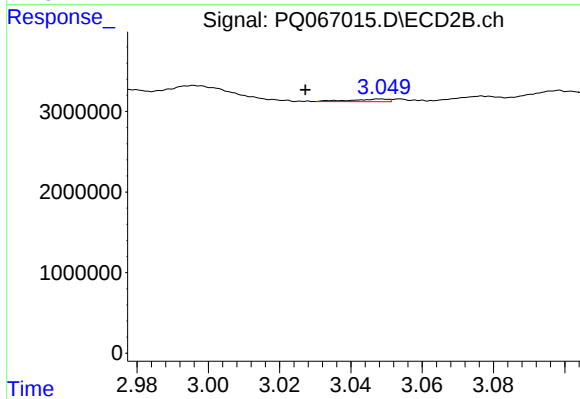

#8 AR-1221-1


R.T.: 3.048 min
Delta R.T.: 0.021 min
Response: 231460
Conc: 2.89 ng/ml

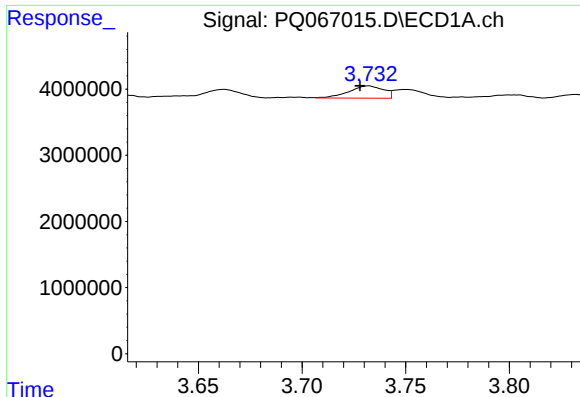

#9 AR-1221-2


R.T.: 3.732 min
Delta R.T.: 0.004 min
Response: 2160284
Conc: 44.60 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

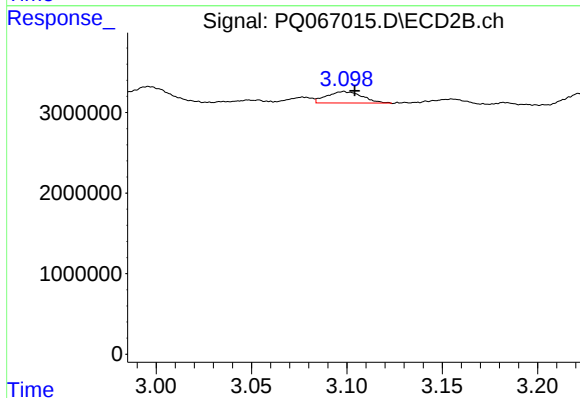


#9 AR-1221-2

R.T.: 3.099 min
Delta R.T.: -0.006 min
Response: 1809028
Conc: 34.62 ng/ml

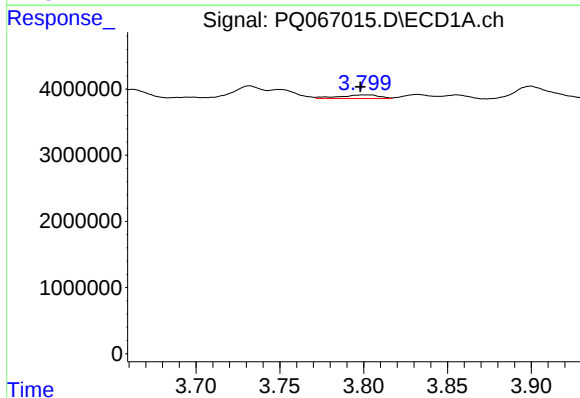


#10 AR-1221-3

R.T.: 3.801 min
Delta R.T.: 0.003 min
Response: 894398
Conc: 5.89 ng/ml

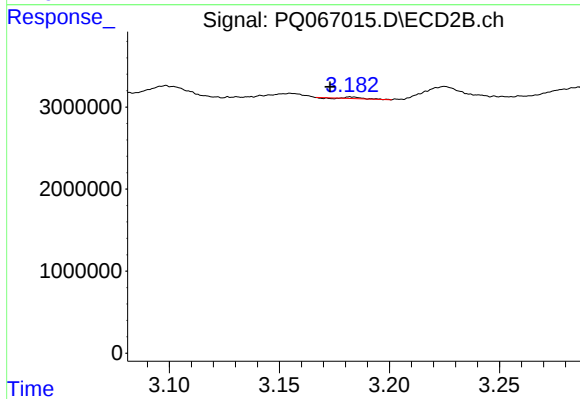

#10 AR-1221-3


R.T.: 3.182 min
Delta R.T.: 0.009 min
Response: 92269
Conc: 0.53 ng/ml

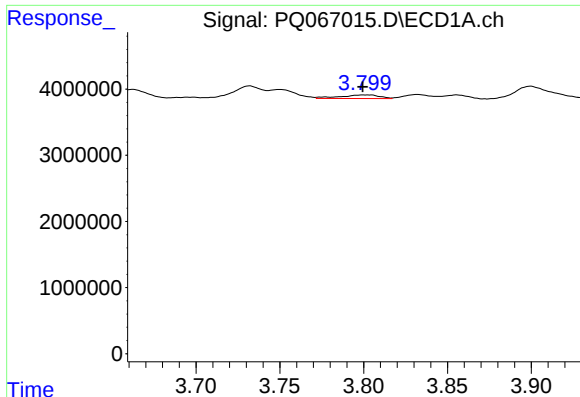

#11 AR-1232-1


R.T.: 3.801 min
Delta R.T.: 0.002 min
Response: 894398
Conc: 7.25 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

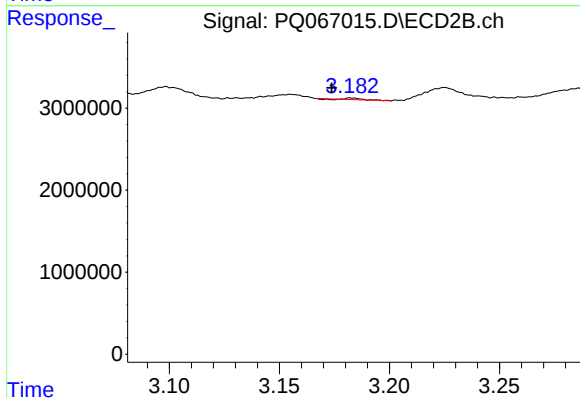


#11 AR-1232-1

R.T.: 3.182 min
Delta R.T.: 0.008 min
Response: 92269
Conc: 0.64 ng/ml

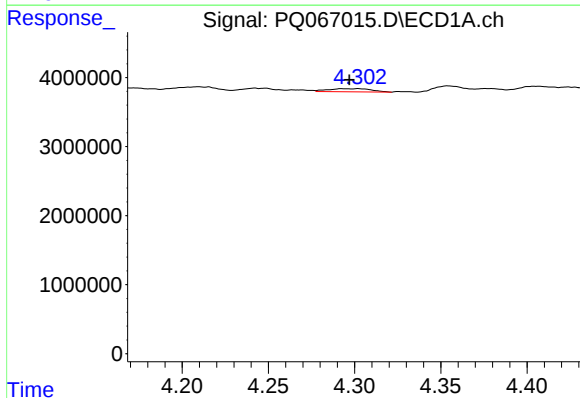


#12 AR-1232-2

R.T.: 4.302 min
Delta R.T.: 0.005 min
Response: 789434
Conc: 11.97 ng/ml

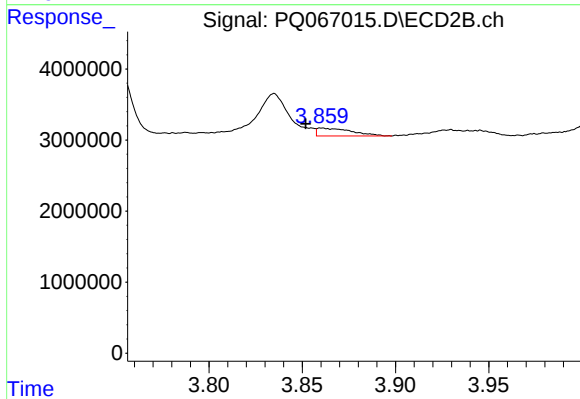

#12 AR-1232-2


R.T.: 3.860 min
Delta R.T.: 0.009 min
Response: 1423587
Conc: 10.02 ng/ml

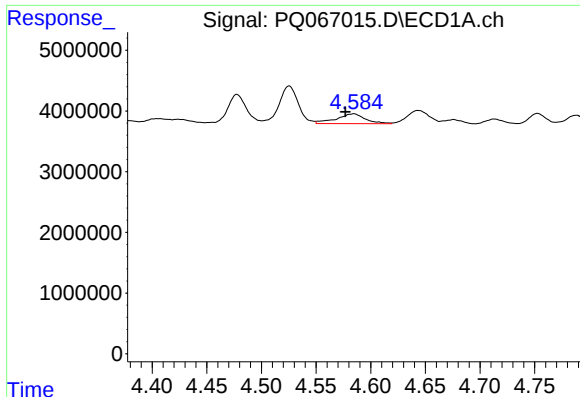

#13 AR-1232-3


R.T.: 4.585 min
Delta R.T.: 0.008 min
Response: 2989100
Conc: 24.81 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

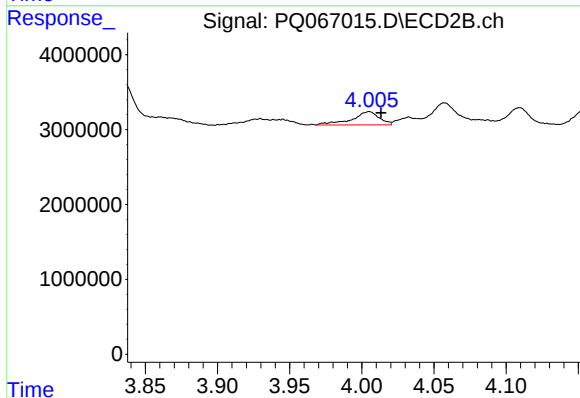


#13 AR-1232-3

R.T.: 4.005 min
Delta R.T.: -0.008 min
Response: 2343864
Conc: 30.11 ng/ml

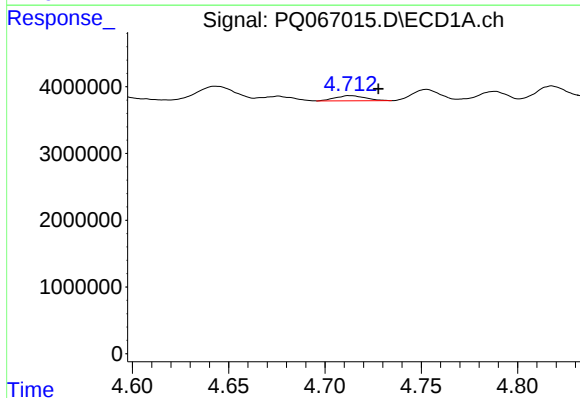


#14 AR-1232-4

R.T.: 4.713 min
Delta R.T.: -0.015 min
Response: 826098
Conc: 14.37 ng/ml

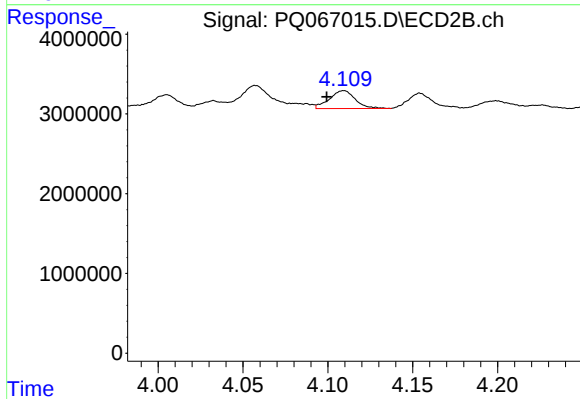

#14 AR-1232-4


R.T.: 4.110 min
Delta R.T.: 0.010 min
Response: 2386570
Conc: 35.89 ng/ml

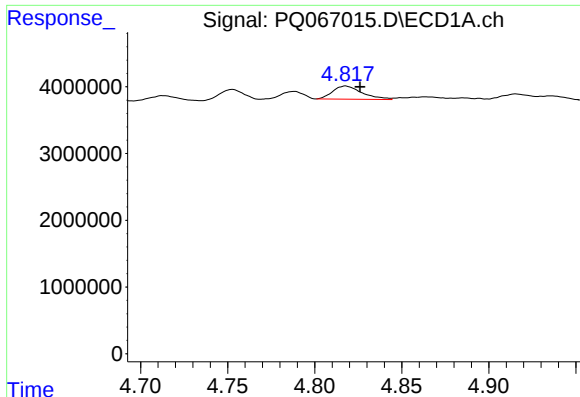

#15 AR-1232-5


R.T.: 4.818 min
Delta R.T.: -0.008 min
Response: 2319471
Conc: 57.98 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

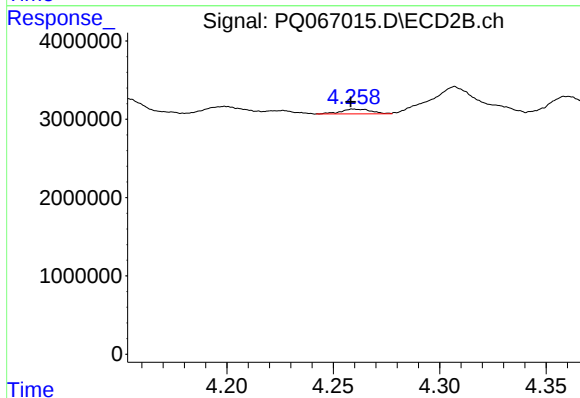


#15 AR-1232-5

R.T.: 4.260 min
Delta R.T.: 0.001 min
Response: 618257
Conc: 8.25 ng/ml

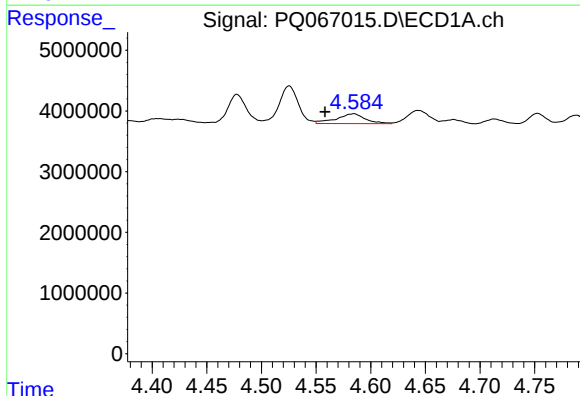


#16 AR-1242-1

R.T.: 4.585 min
Delta R.T.: 0.026 min
Response: 2989100
Conc: 20.96 ng/ml

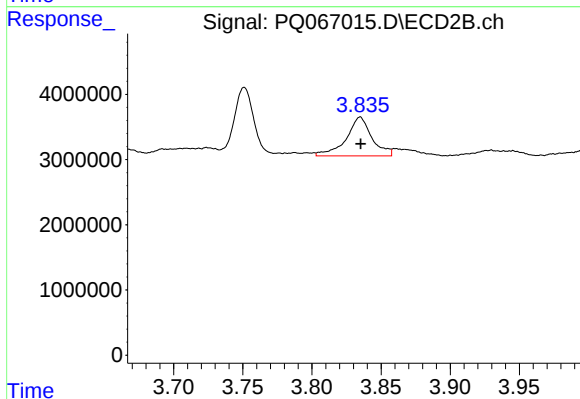

#16 AR-1242-1


R.T.: 3.835 min
Delta R.T.: 0.000 min
Response: 7711871
Conc: 44.34 ng/ml

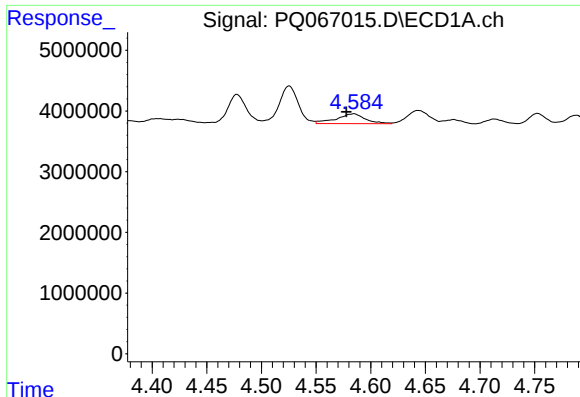

#17 AR-1242-2


R.T.: 4.585 min
Delta R.T.: 0.007 min
Response: 2989100
Conc: 13.58 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

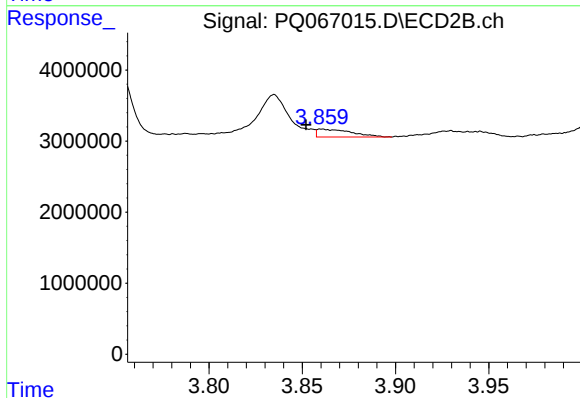


#17 AR-1242-2

R.T.: 3.860 min
Delta R.T.: 0.008 min
Response: 1423587
Conc: 5.71 ng/ml

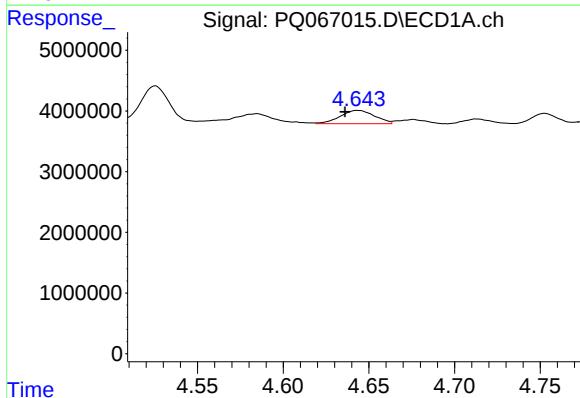


#18 AR-1242-3

R.T.: 4.643 min
Delta R.T.: 0.007 min
Response: 3061535
Conc: 22.74 ng/ml

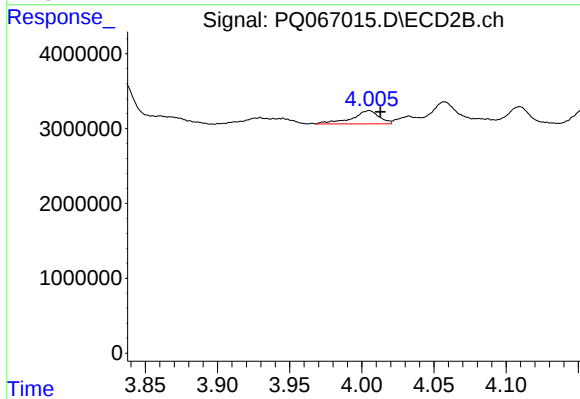

#18 AR-1242-3


R.T.: 4.005 min
Delta R.T.: -0.008 min
Response: 2343864
Conc: 16.80 ng/ml

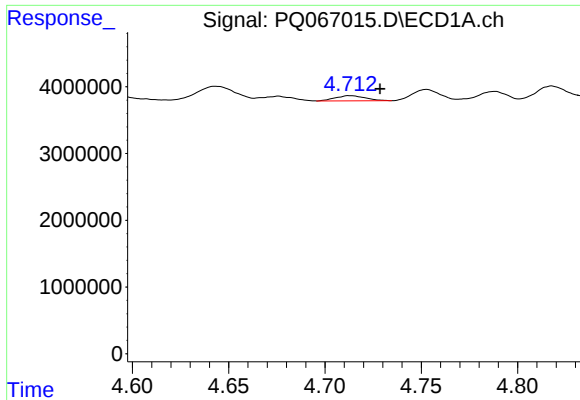

#19 AR-1242-4


R.T.: 4.713 min
Delta R.T.: -0.016 min
Response: 826098
Conc: 7.81 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

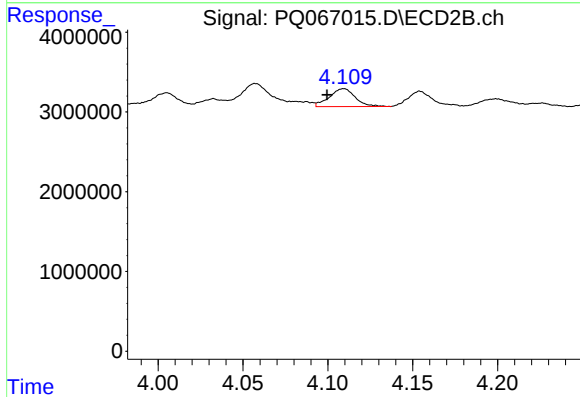


#19 AR-1242-4

R.T.: 4.110 min
Delta R.T.: 0.010 min
Response: 2386570
Conc: 18.27 ng/ml

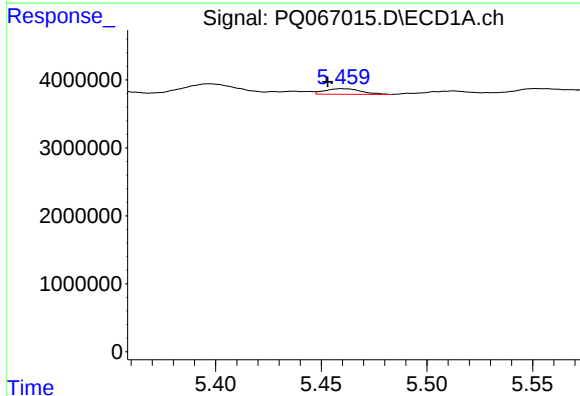


#20 AR-1242-5

R.T.: 5.460 min
Delta R.T.: 0.007 min
Response: 976363
Conc: 8.55 ng/ml

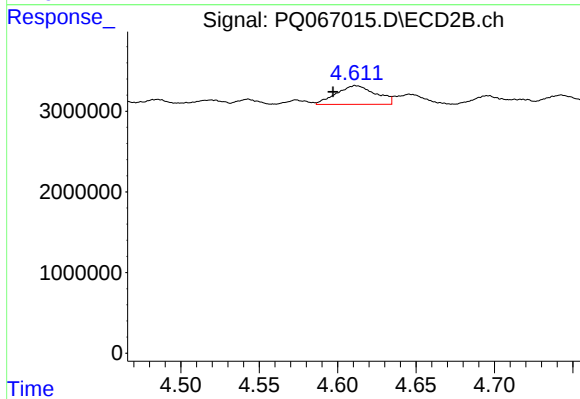

#20 AR-1242-5


R.T.: 4.611 min
Delta R.T.: 0.014 min
Response: 4073078
Conc: 24.54 ng/ml

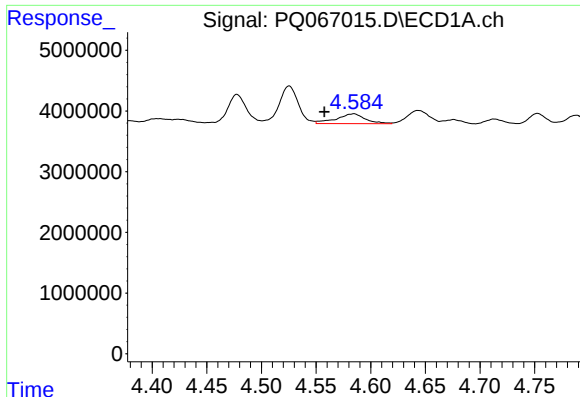

#21 AR-1248-1


R.T.: 4.585 min
Delta R.T.: 0.027 min
Response: 2989100
Conc: 28.33 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

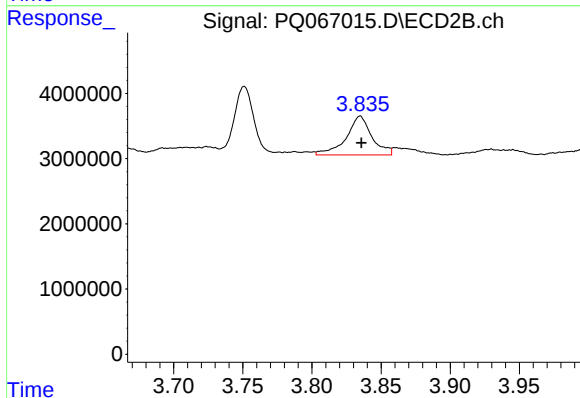


#21 AR-1248-1

R.T.: 3.835 min
Delta R.T.: 0.000 min
Response: 7711871
Conc: 60.25 ng/ml

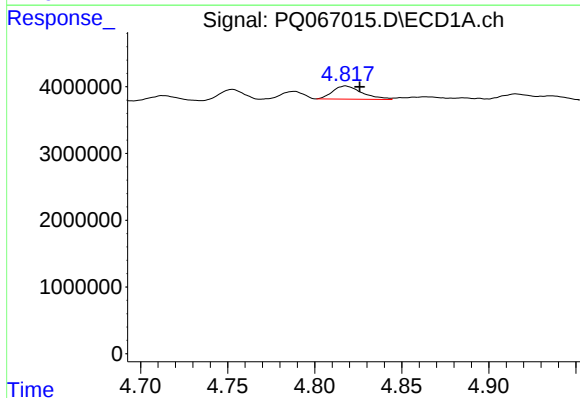


#22 AR-1248-2

R.T.: 4.818 min
Delta R.T.: -0.008 min
Response: 2319471
Conc: 15.82 ng/ml

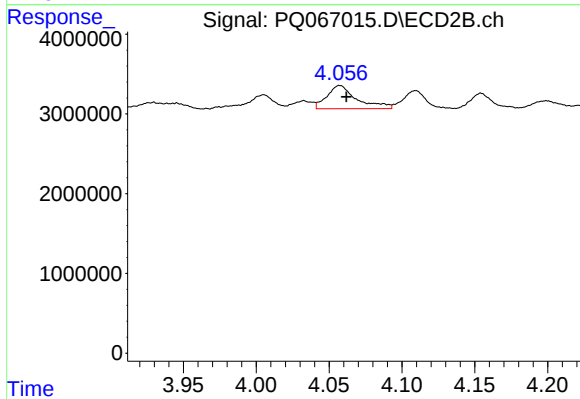

#22 AR-1248-2


R.T.: 4.057 min
Delta R.T.: -0.005 min
Response: 4173815
Conc: 21.78 ng/ml

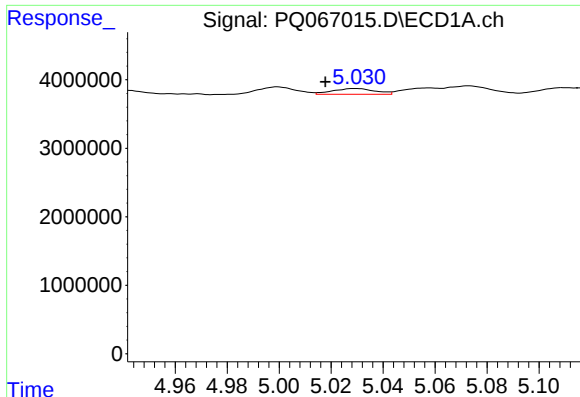

#23 AR-1248-3


R.T.: 5.029 min
Delta R.T.: 0.012 min
Response: 959243
Conc: 5.49 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

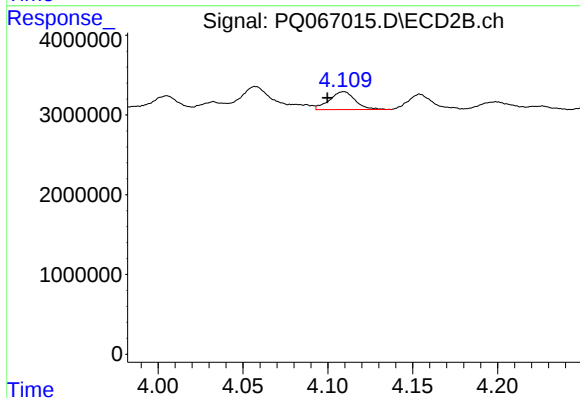


#23 AR-1248-3

R.T.: 4.110 min
Delta R.T.: 0.010 min
Response: 2386570
Conc: 12.97 ng/ml

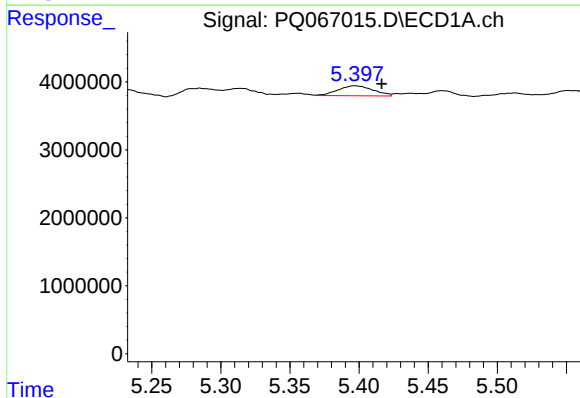


#24 AR-1248-4

R.T.: 5.397 min
Delta R.T.: -0.019 min
Response: 2589294
Conc: 13.20 ng/ml

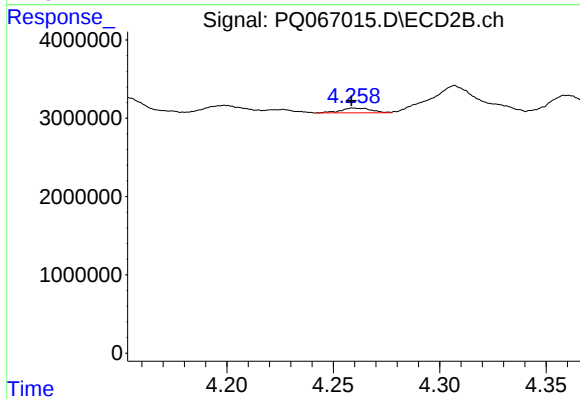

#24 AR-1248-4


R.T.: 4.260 min
Delta R.T.: 0.001 min
Response: 618257
Conc: 2.74 ng/ml

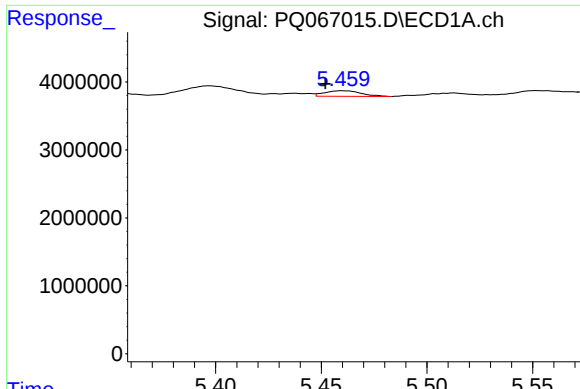

#25 AR-1248-5


R.T.: 5.460 min
Delta R.T.: 0.008 min
Response: 976363
Conc: 4.91 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

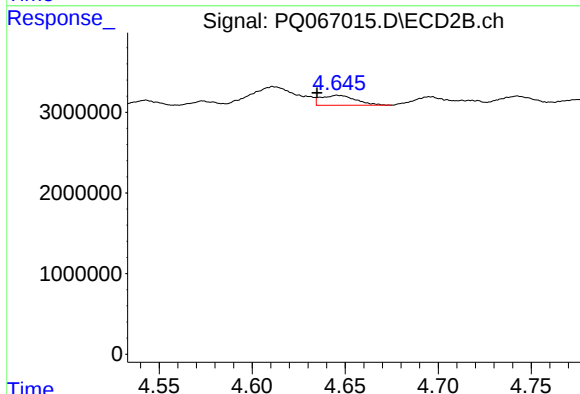


#25 AR-1248-5

R.T.: 4.646 min
Delta R.T.: 0.011 min
Response: 1598507
Conc: 7.47 ng/ml

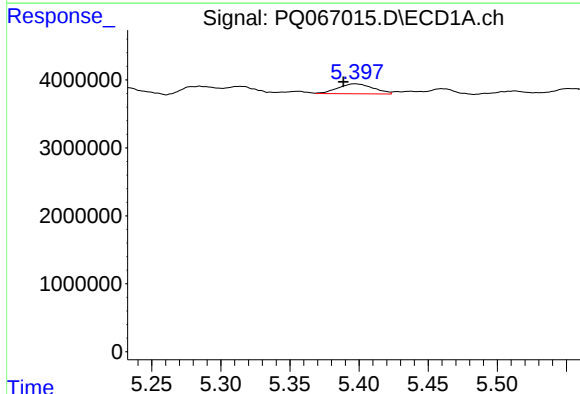


#26 AR-1254-1

R.T.: 5.397 min
Delta R.T.: 0.008 min
Response: 2589294
Conc: 12.50 ng/ml

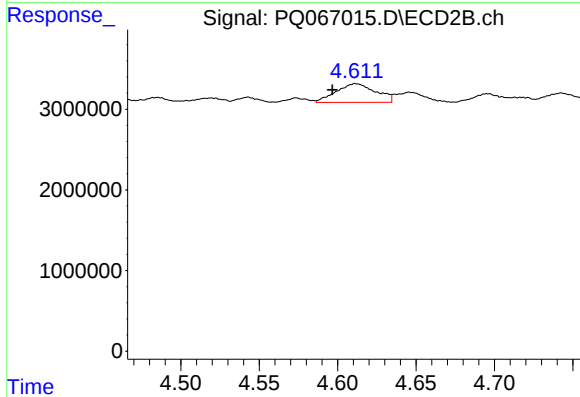

#26 AR-1254-1


R.T.: 4.611 min
Delta R.T.: 0.015 min
Response: 4073078
Conc: 12.15 ng/ml

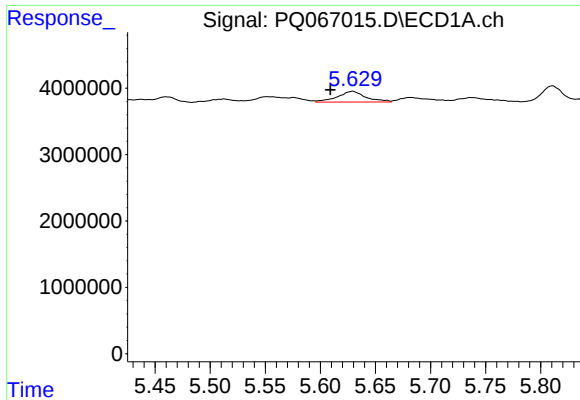

#27 AR-1254-2


R.T.: 5.629 min
Delta R.T.: 0.020 min
Response: 2937280
Conc: 9.10 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

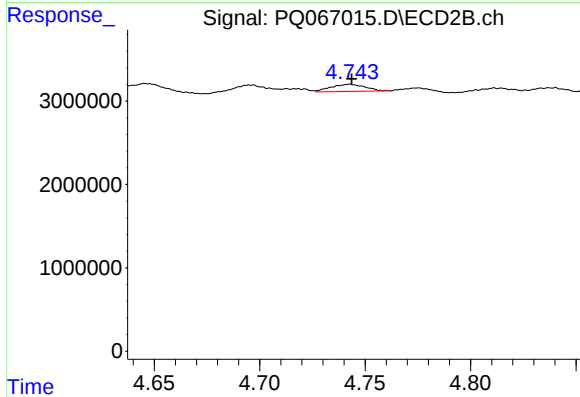


#27 AR-1254-2

R.T.: 4.743 min
Delta R.T.: -0.001 min
Response: 974668
Conc: 3.38 ng/ml

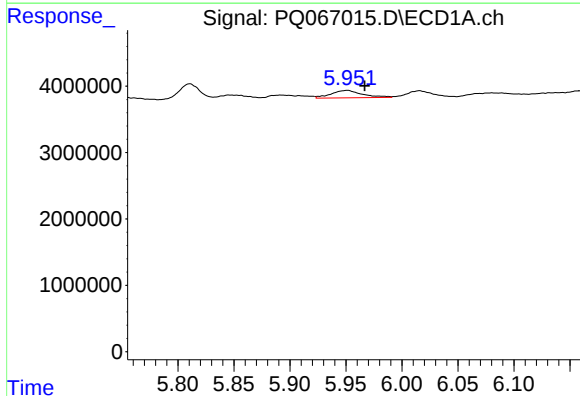


#28 AR-1254-3

R.T.: 5.951 min
Delta R.T.: -0.016 min
Response: 2183827
Conc: 6.43 ng/ml

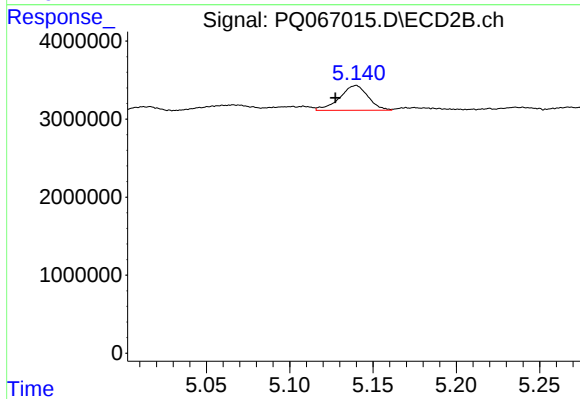

#28 AR-1254-3


R.T.: 5.140 min
Delta R.T.: 0.013 min
Response: 3761334
Conc: 8.09 ng/ml

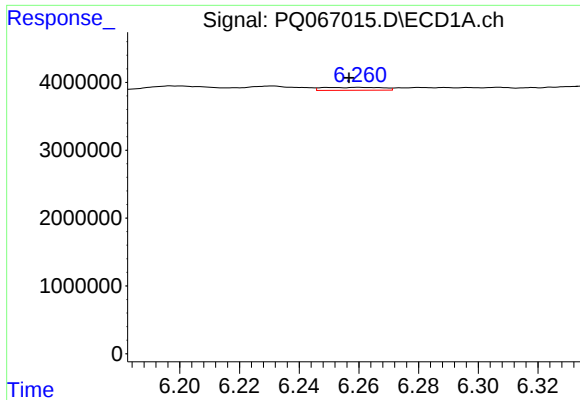

#29 AR-1254-4


R.T.: 6.260 min
Delta R.T.: 0.003 min
Response: 606043
Conc: 2.57 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

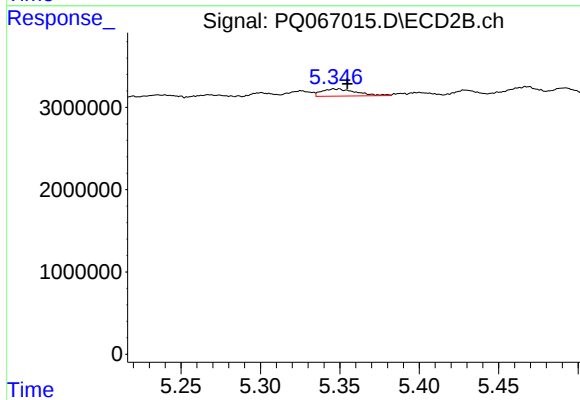


#29 AR-1254-4

R.T.: 5.346 min
Delta R.T.: -0.009 min
Response: 1303357
Conc: 4.68 ng/ml

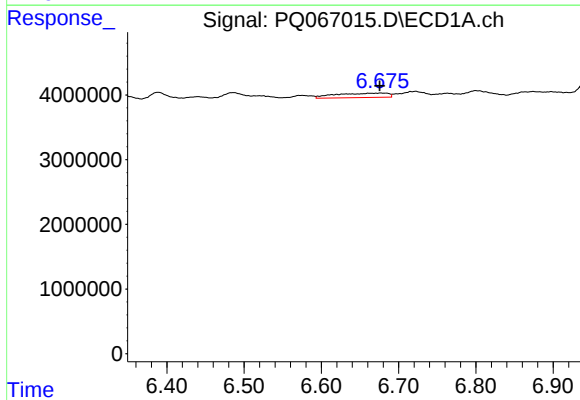


#30 AR-1254-5

R.T.: 6.677 min
Delta R.T.: 0.001 min
Response: 3201084
Conc: 12.08 ng/ml

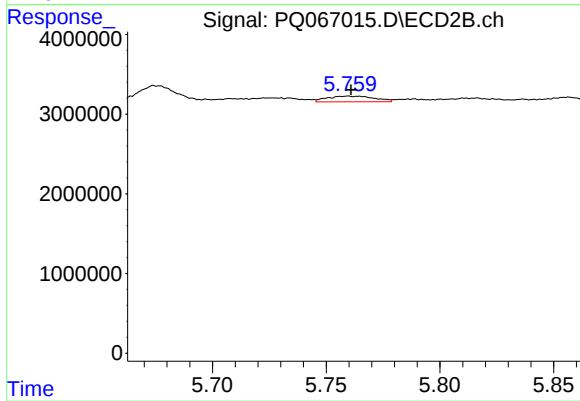

#30 AR-1254-5


R.T.: 5.760 min
Delta R.T.: -0.001 min
Response: 1029398
Conc: 2.46 ng/ml

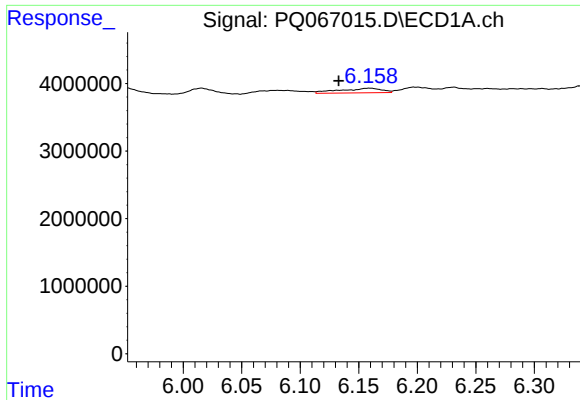

#31 AR-1260-1


R.T.: 6.159 min
Delta R.T.: 0.026 min
Response: 1715005
Conc: 6.65 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

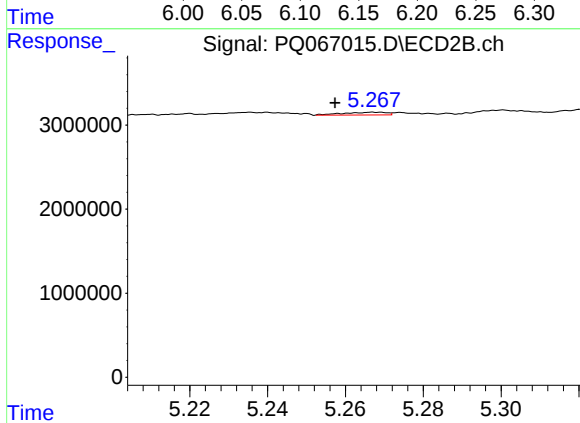


#31 AR-1260-1

R.T.: 5.267 min
Delta R.T.: 0.010 min
Response: 244522
Conc: 0.74 ng/ml

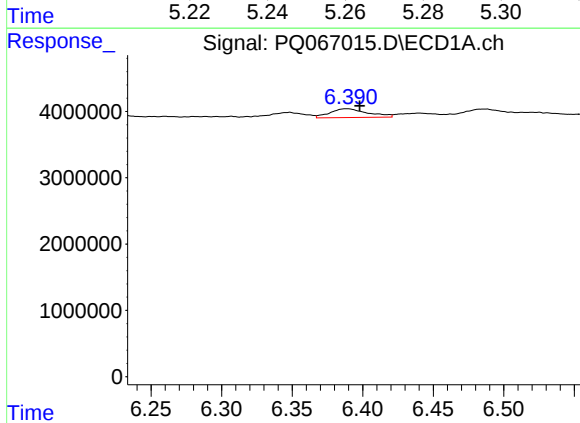


#32 AR-1260-2

R.T.: 6.389 min
Delta R.T.: -0.009 min
Response: 2470090
Conc: 8.13 ng/ml

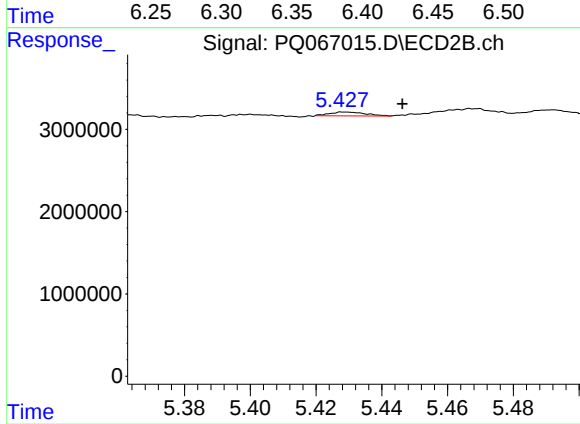

#32 AR-1260-2


R.T.: 5.429 min
Delta R.T.: -0.018 min
Response: 357578
Conc: 0.91 ng/ml

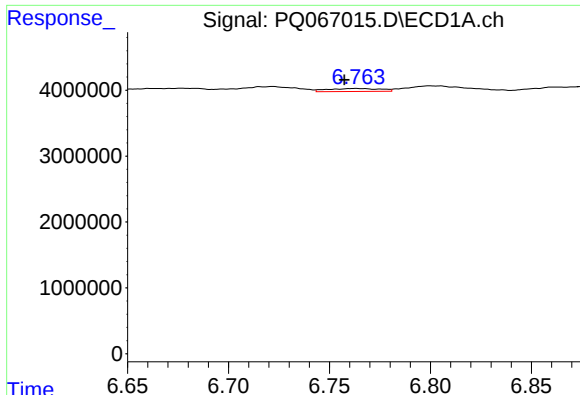

#33 AR-1260-3


R.T.: 6.763 min
Delta R.T.: 0.006 min
Response: 808961
Conc: 3.66 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

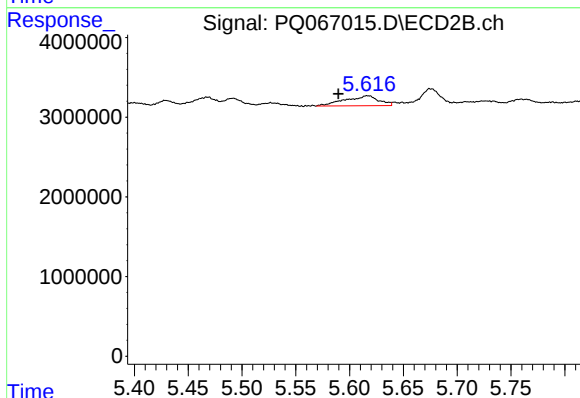


#33 AR-1260-3

R.T.: 5.616 min
Delta R.T.: 0.027 min
Response: 2754848
Conc: 7.27 ng/ml

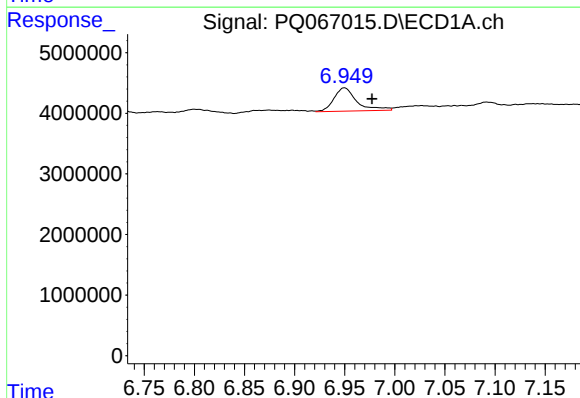


#34 AR-1260-4

R.T.: 6.950 min
Delta R.T.: -0.028 min
Response: 6105966
Conc: 25.21 ng/ml

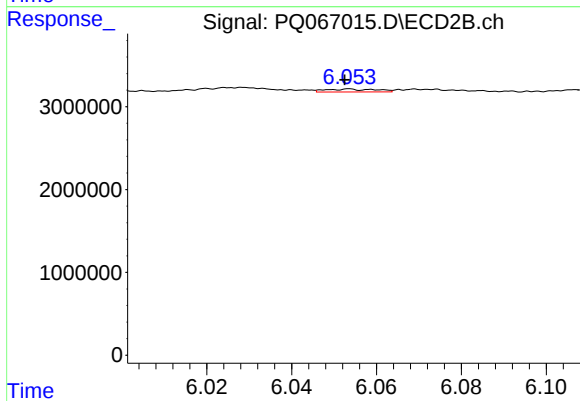

#34 AR-1260-4


R.T.: 6.054 min
Delta R.T.: 0.001 min
Response: 291514
Conc: 0.93 ng/ml

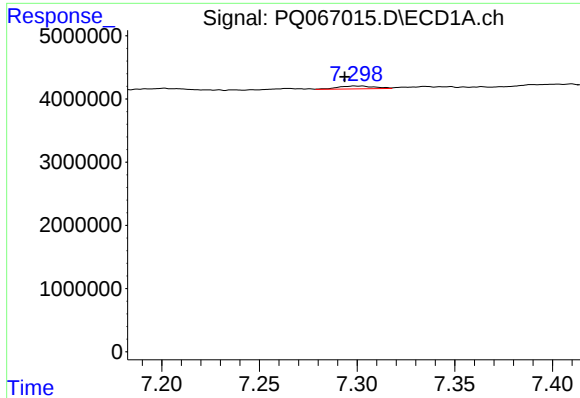

#35 AR-1260-5


R.T.: 7.299 min
Delta R.T.: 0.006 min
Response: 580318
Conc: 1.19 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

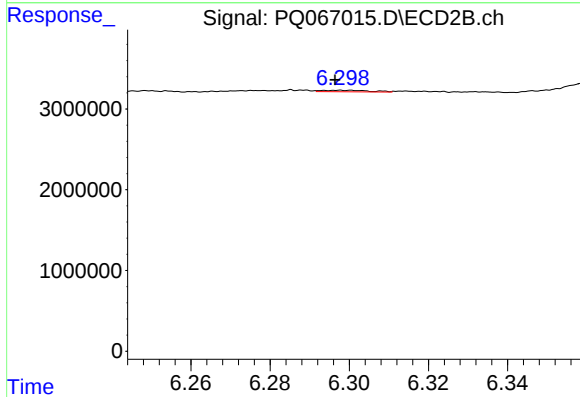


#35 AR-1260-5

R.T.: 6.301 min
Delta R.T.: 0.004 min
Response: 154932
Conc: 0.23 ng/ml

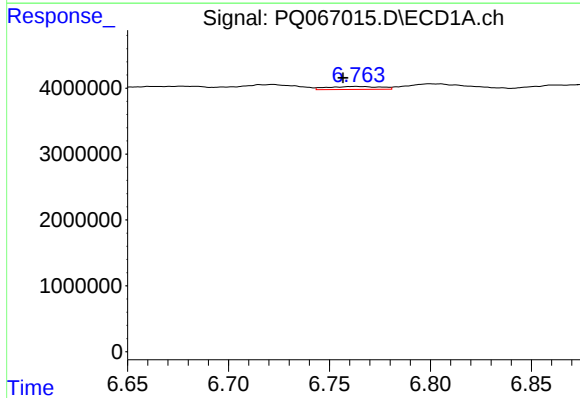


#36 AR-1262-1

R.T.: 6.763 min
Delta R.T.: 0.006 min
Response: 808961
Conc: 2.45 ng/ml

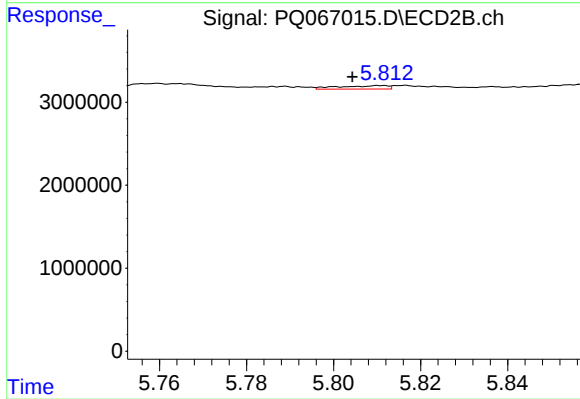

#36 AR-1262-1


R.T.: 5.811 min
Delta R.T.: 0.007 min
Response: 323774
Conc: 0.75 ng/ml

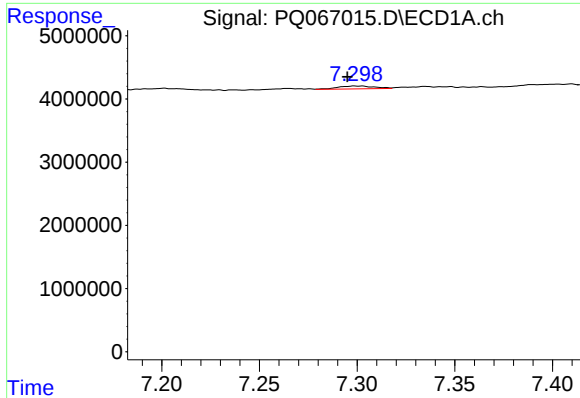

#37 AR-1262-2


R.T.: 7.299 min
Delta R.T.: 0.004 min
Response: 580318
Conc: 1.08 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

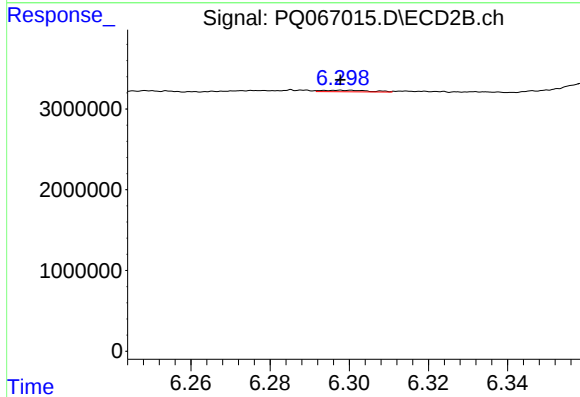


#37 AR-1262-2

R.T.: 6.301 min
Delta R.T.: 0.003 min
Response: 154932
Conc: 0.21 ng/ml

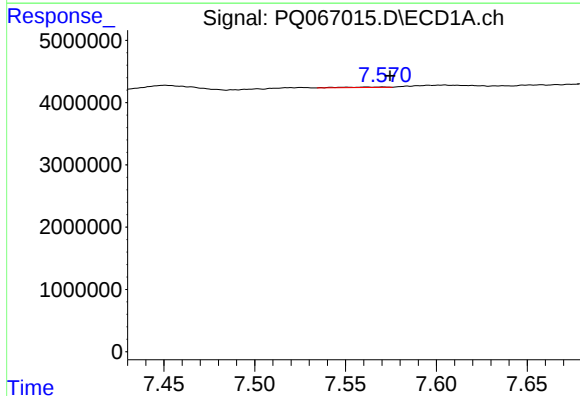


#38 AR-1262-3

R.T.: 7.571 min
Delta R.T.: -0.004 min
Response: 128960
Conc: 0.37 ng/ml

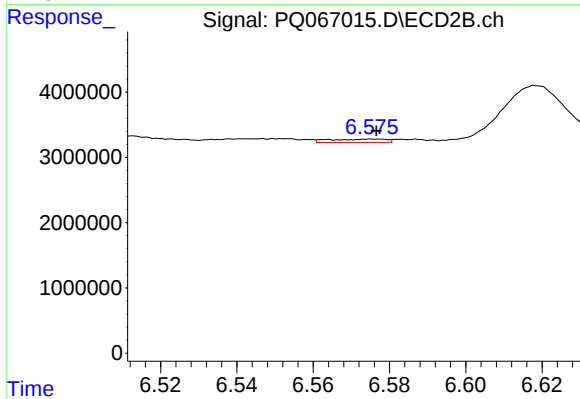

#38 AR-1262-3


R.T.: 6.575 min
Delta R.T.: -0.001 min
Response: 547123
Conc: 1.76 ng/ml

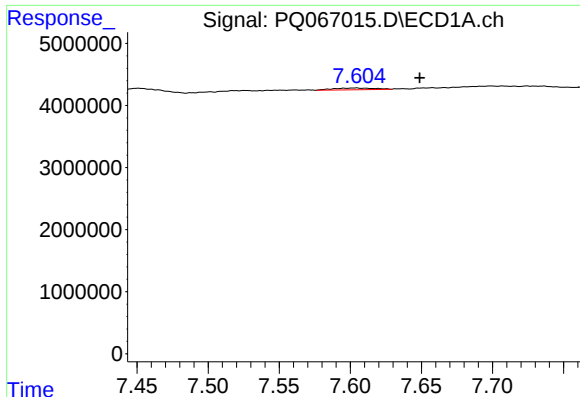

#39 AR-1262-4


R.T.: 7.604 min
Delta R.T.: -0.045 min
Response: 546076
Conc: 2.02 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

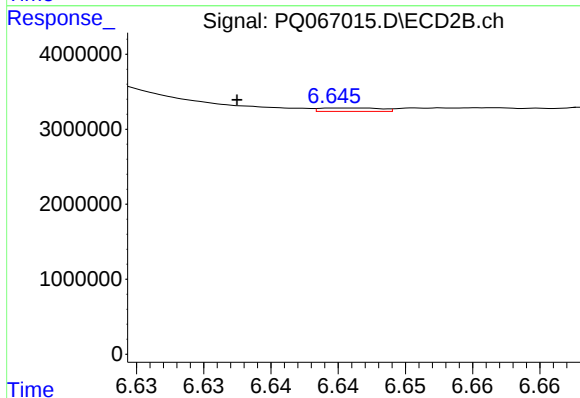


#39 AR-1262-4

R.T.: 6.646 min
Delta R.T.: 0.008 min
Response: 145342
Conc: 0.25 ng/ml

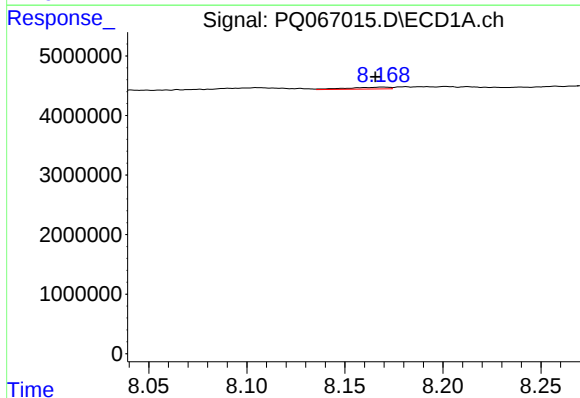


#40 AR-1262-5

R.T.: 8.169 min
Delta R.T.: 0.004 min
Response: 450369
Conc: 2.69 ng/ml

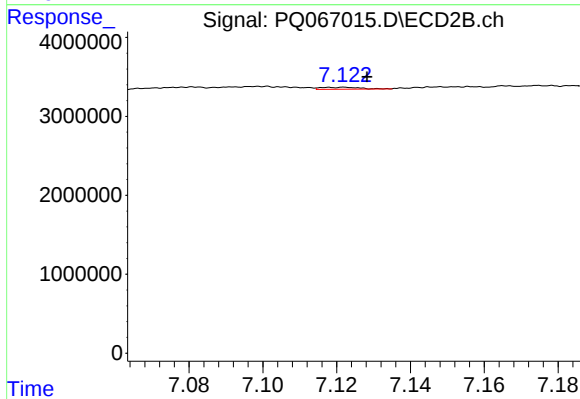

#40 AR-1262-5


R.T.: 7.122 min
Delta R.T.: -0.006 min
Response: 188579
Conc: 0.73 ng/ml

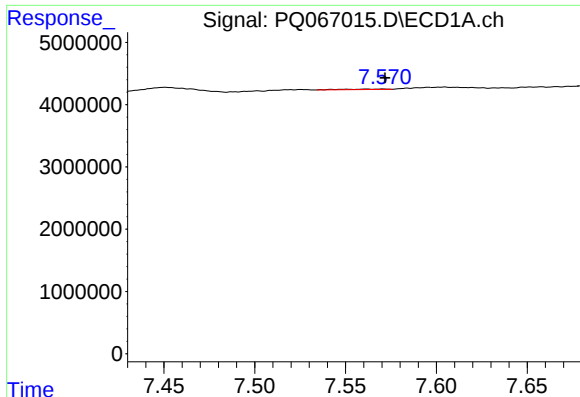

#41 AR-1268-1


R.T.: 7.571 min
Delta R.T.: 0.000 min
Response: 128960
Conc: 0.21 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

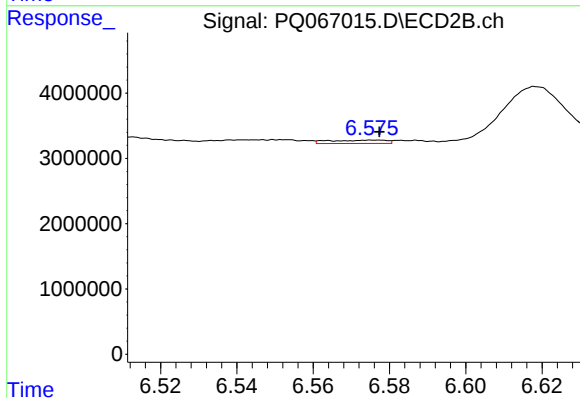


#41 AR-1268-1

R.T.: 6.575 min
Delta R.T.: -0.002 min
Response: 547123
Conc: 0.62 ng/ml

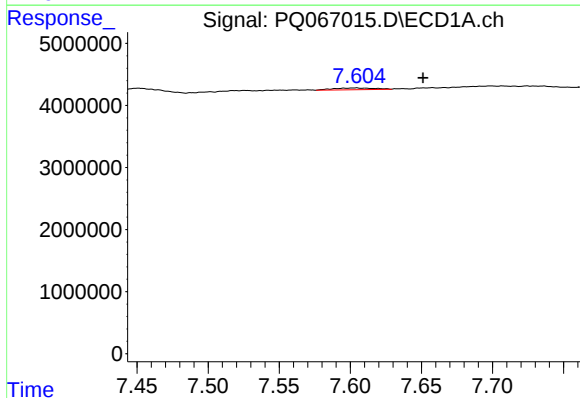


#42 AR-1268-2

R.T.: 7.604 min
Delta R.T.: -0.047 min
Response: 546076
Conc: 1.01 ng/ml

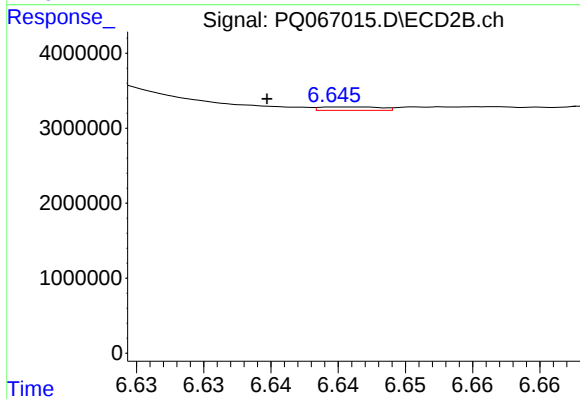

#42 AR-1268-2


R.T.: 6.646 min
Delta R.T.: 0.006 min
Response: 145342
Conc: 0.18 ng/ml

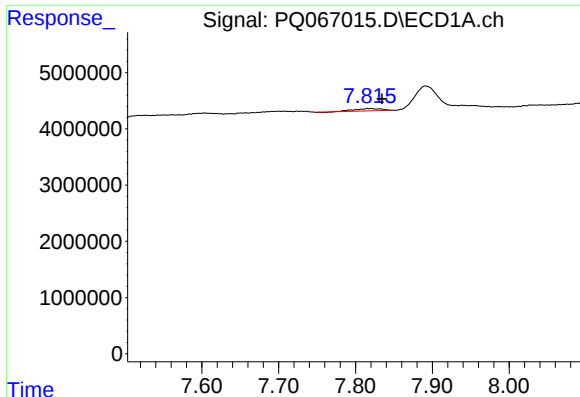

#43 AR-1268-3


R.T.: 7.816 min
Delta R.T.: -0.019 min
Response: 993649
Conc: 2.13 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

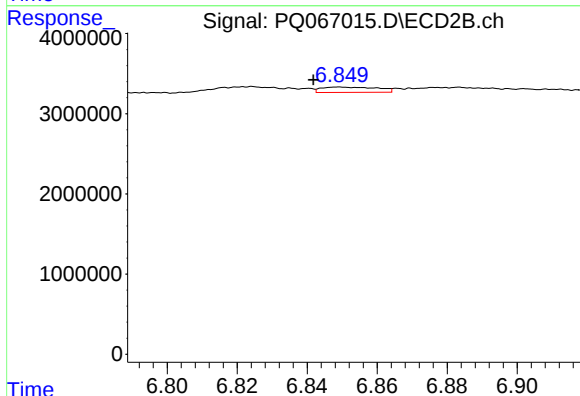


#43 AR-1268-3

R.T.: 6.849 min
Delta R.T.: 0.007 min
Response: 739554
Conc: 1.07 ng/ml

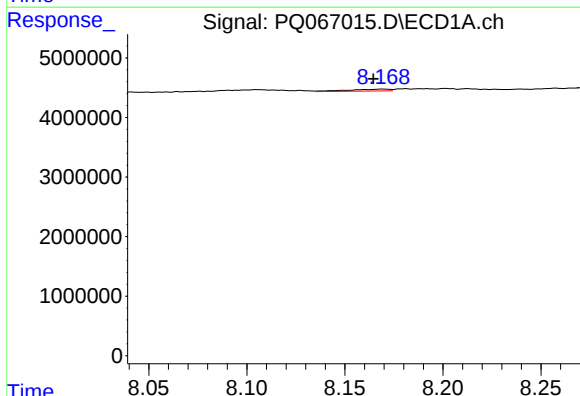


#44 AR-1268-4

R.T.: 8.169 min
Delta R.T.: 0.005 min
Response: 450369
Conc: 2.56 ng/ml

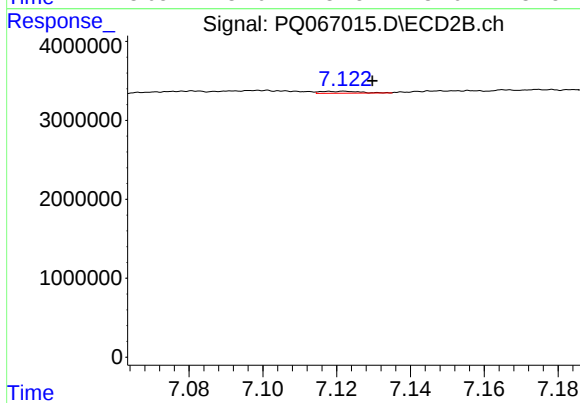

#44 AR-1268-4


R.T.: 7.122 min
Delta R.T.: -0.007 min
Response: 188579
Conc: 0.66 ng/ml

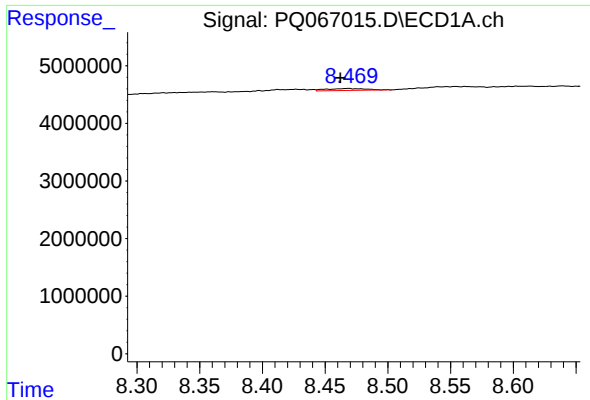

#45 AR-1268-5

R.T.: 8.468 min
Delta R.T.: 0.006 min
Response: 764945
Conc: 0.57 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

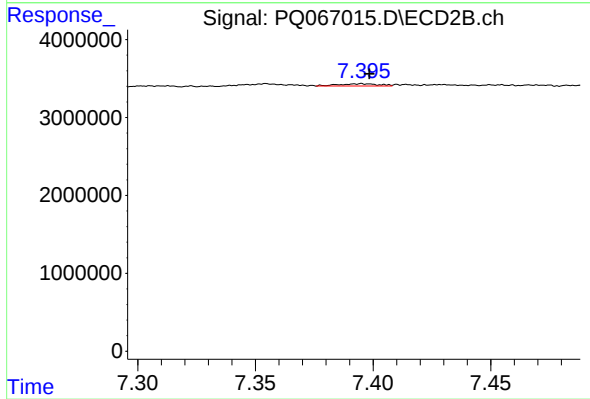

#45 AR-1268-5

R.T.: 7.395 min
Delta R.T.: -0.003 min
Response: 328827
Conc: 0.16 ng/ml