

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060724\
 Data File : PQ067014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2024 17:47
 Operator : YP\AJ
 Sample : P2764-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 K-2211-ESSEX-SWITCHING-STATION

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/10/2024
 Supervised By :Ankita Jodhani 06/10/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 22:29:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ053124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 03 10:00:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.448	2.826	88829549	83364549	16.038	14.251
2) SA Decachlor...	8.715	7.621	71152458	67387762	18.762m	11.734 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060724\
Data File : PQ067014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2024 17:47
Operator : YP\AJ
Sample : P2764-01
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
ECD_Q
ClientSampleId :
K-2211-ESSEX-SWITCHING-STATION


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/10/2024
Supervised By :Ankita Jodhani 06/10/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 22:29:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ053124.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 03 10:00:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

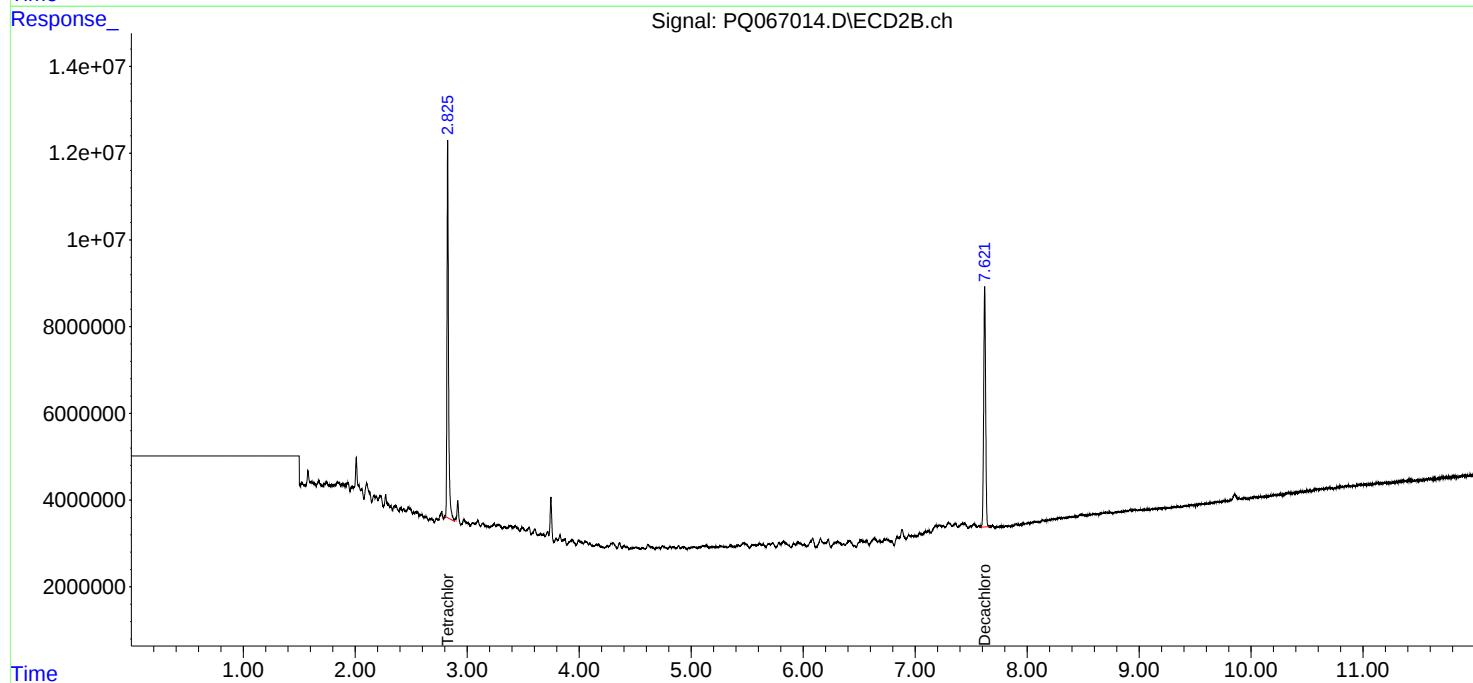

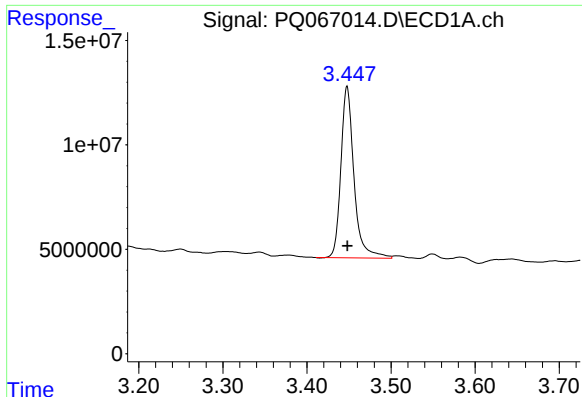

#1 Tetrachloro-m-xylene

R.T.: 3.448 min
Delta R.T.: 0.000 min
Response: 88829549
Conc: 16.04 ng/ml

Instrument :

ECD_Q


ClientSampleId :

K-2211-ESSEX-SWITCHING-STATION

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 06/10/2024
Supervised By :Ankita Jodhani 06/10/2024

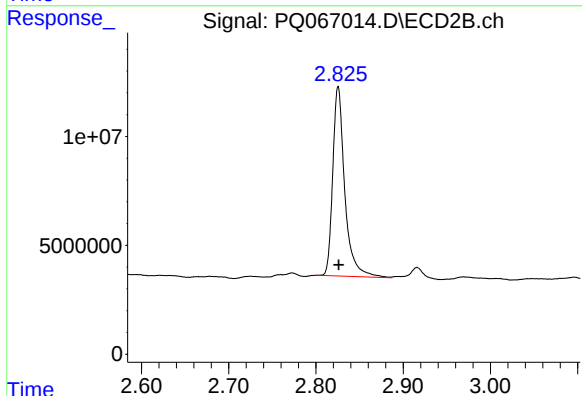


#1 Tetrachloro-m-xylene

R.T.: 2.826 min
Delta R.T.: 0.000 min
Response: 83364549
Conc: 14.25 ng/ml

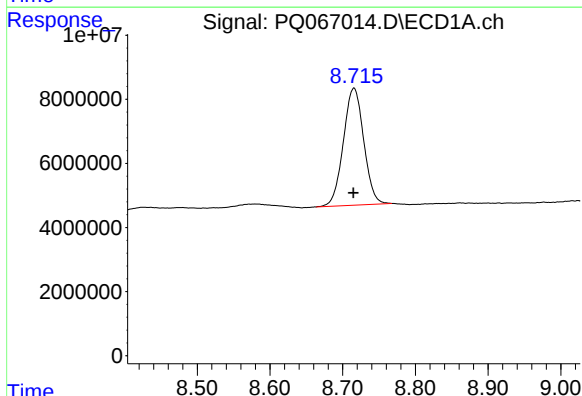

#2 Decachlorobiphenyl

R.T.: 8.715 min
Delta R.T.: 0.000 min
Response: 71152458
Conc: 18.76 ng/ml m

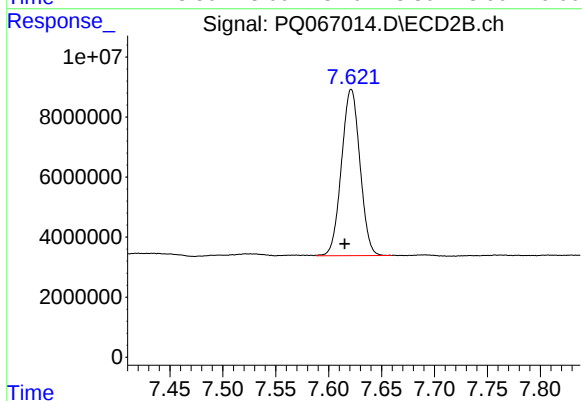

#2 Decachlorobiphenyl

R.T.: 7.621 min
Delta R.T.: 0.006 min
Response: 67387762
Conc: 11.73 ng/ml