

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060724\
 Data File : PQ067015.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2024 18:02
 Operator : YP\AJ
 Sample : P2764-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 H-1308-ESSEX-SWITCHING-STATION

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 22:29:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ053124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 03 10:00:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.452	2.832	69593135	65591649	12.565	11.213
2) SA Decachlor...	8.711	7.616	65092882	64076106	17.165	11.157 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060724\
Data File : PQ067015.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2024 18:02
Operator : YP\AJ
Sample : P2764-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 22:29:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ053124.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 03 10:00:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

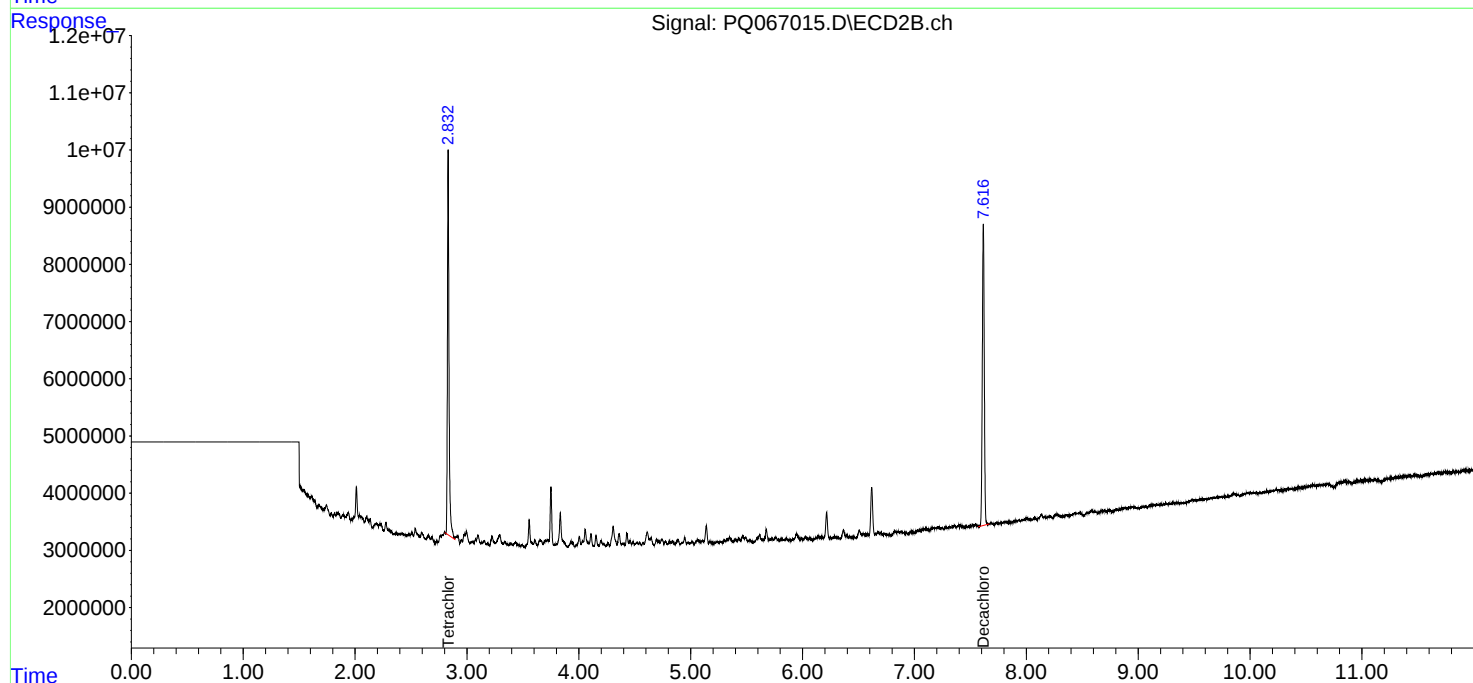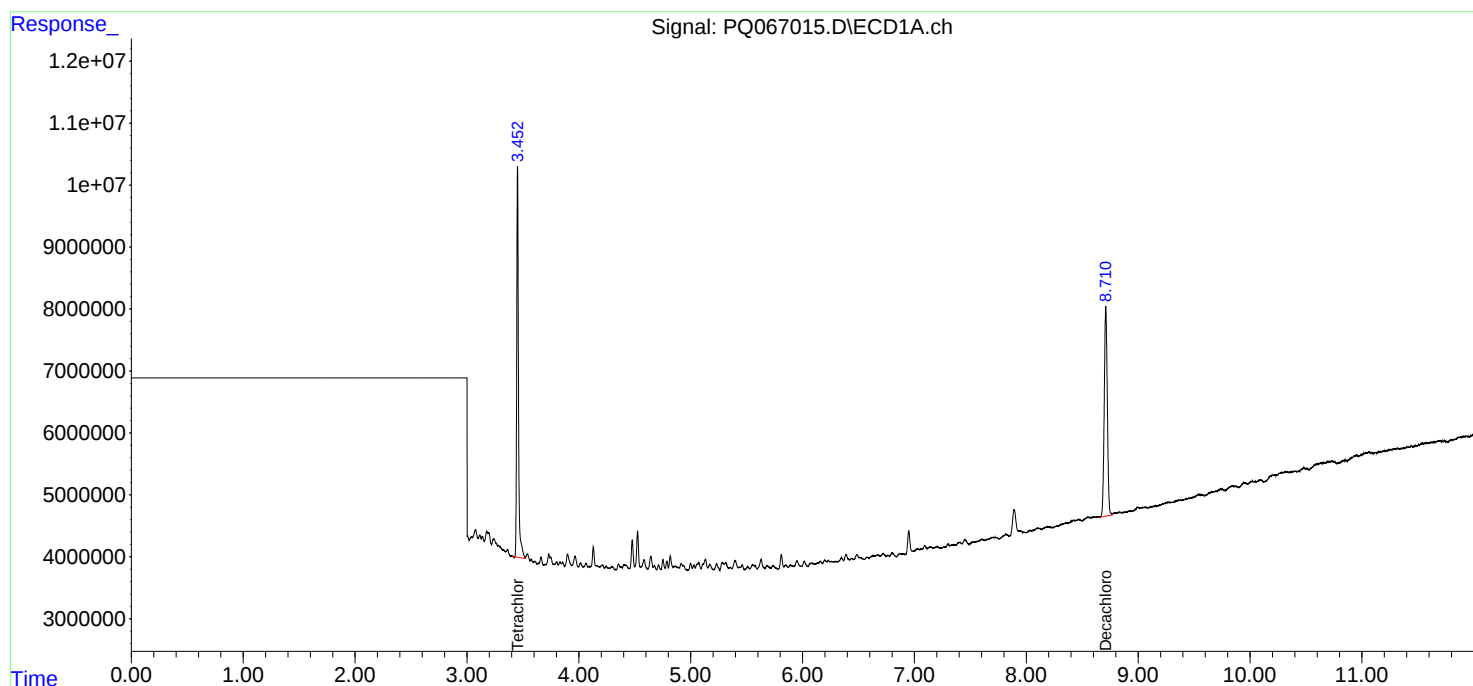


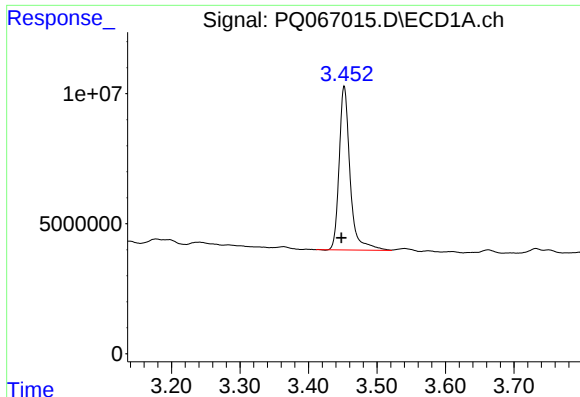

#1 Tetrachloro-m-xylene


R.T.: 3.452 min
Delta R.T.: 0.004 min
Response: 69593135
Conc: 12.57 ng/ml

Instrument :
ECD_Q
ClientSampleId :
H-1308-ESSEX-SWITCHING-STATION

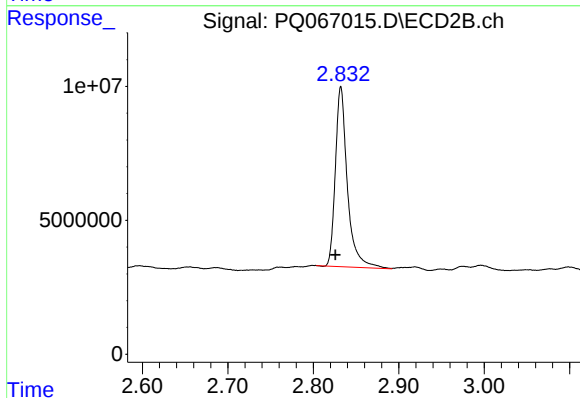


#1 Tetrachloro-m-xylene

R.T.: 2.832 min
Delta R.T.: 0.006 min
Response: 65591649
Conc: 11.21 ng/ml

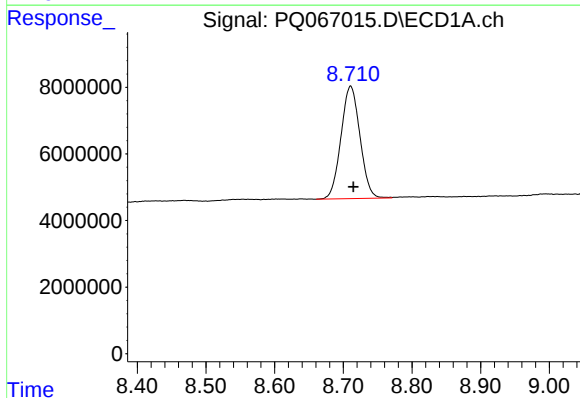

#2 Decachlorobiphenyl

R.T.: 8.711 min
Delta R.T.: -0.004 min
Response: 65092882
Conc: 17.16 ng/ml

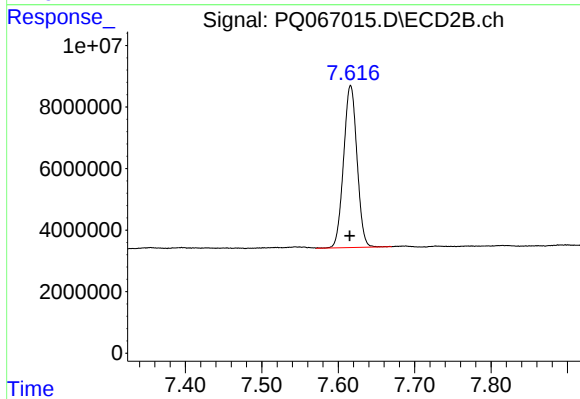

#2 Decachlorobiphenyl

R.T.: 7.616 min
Delta R.T.: 0.001 min
Response: 64076106
Conc: 11.16 ng/ml