

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060724\
 Data File : PQ067017.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2024 18:31
 Operator : YP\AJ
 Sample : P2766-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 M-2239-FAIRLAWN-SWITCH

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/10/2024
 Supervised By :Ankita Jodhani 06/10/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 22:30:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ053124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 03 10:00:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.453	2.834	65478858	60612180	11.822	10.361
2) SA Decachlor...	8.708	7.616	63949527	63941150	16.863	11.134 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ060724\
Data File : PQ067017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2024 18:31
Operator : YP\AJ
Sample : P2766-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
M-2239-FAIRLAWN-SWITCH


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/10/2024
Supervised By :Ankita Jodhani 06/10/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 22:30:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ053124.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 03 10:00:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

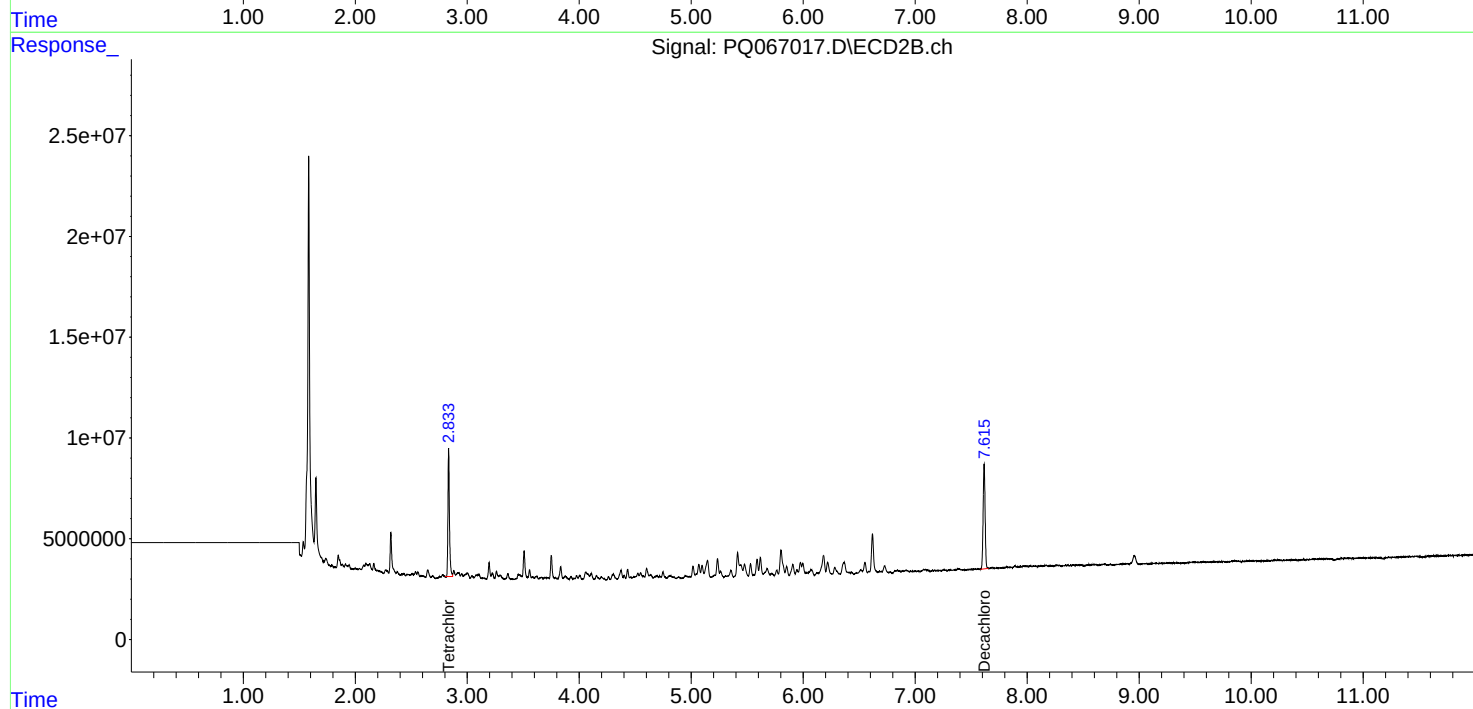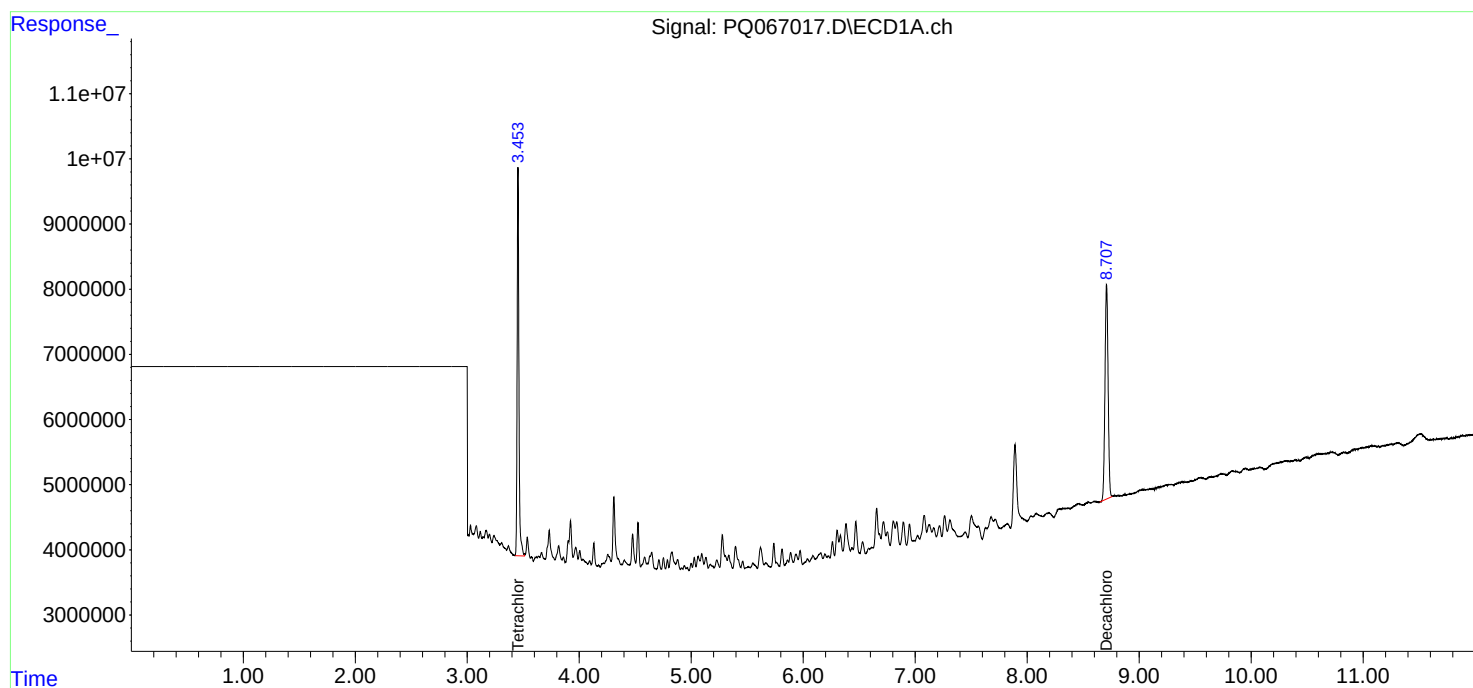

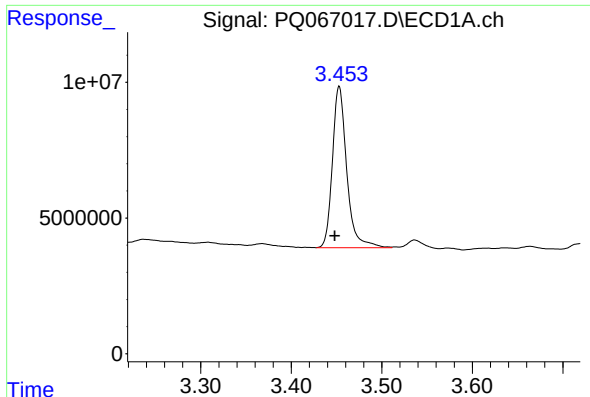


#1 Tetrachloro-m-xylene

R.T.: 3.453 min
Delta R.T.: 0.005 min
Response: 65478858
Conc: 11.82 ng/ml

Instrument :
ECD_Q
ClientSampleId :
M-2239-FAIRLAWN-SWITCH


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/10/2024
Supervised By :Ankita Jodhani 06/10/2024

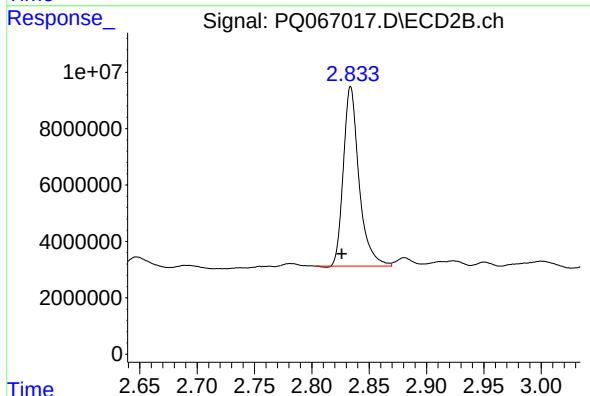


#1 Tetrachloro-m-xylene

R.T.: 2.834 min
Delta R.T.: 0.008 min
Response: 60612180
Conc: 10.36 ng/ml

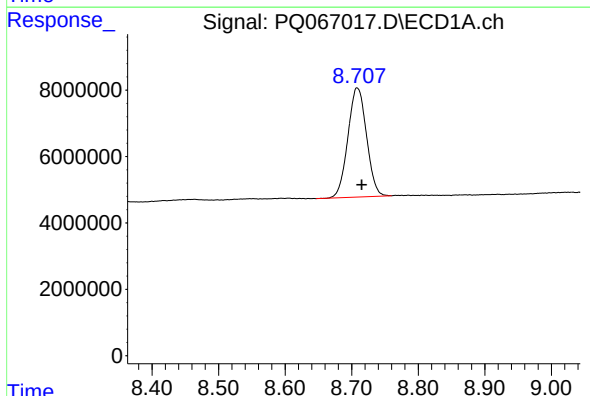

#2 Decachlorobiphenyl

R.T.: 8.708 min
Delta R.T.: -0.007 min
Response: 63949527
Conc: 16.86 ng/ml

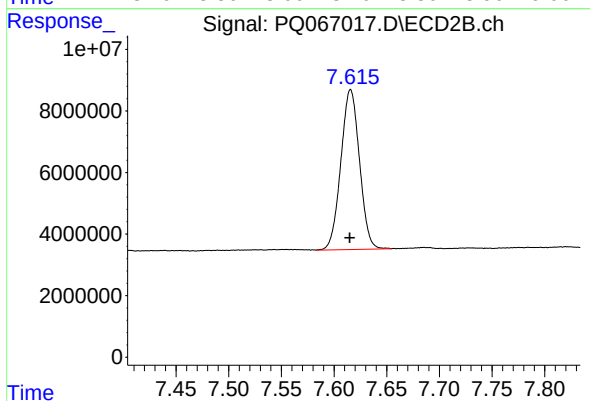

#2 Decachlorobiphenyl

R.T.: 7.616 min
Delta R.T.: 0.000 min
Response: 63941150
Conc: 11.13 ng/ml