

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ061323\
 Data File : PQ061395.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2023 19:49
 Operator : YP\AJ
 Sample : 03170-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_Q
 ClientSampleId :
 AUD-1971

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/14/2023
 Supervised By :Ankita Jodhani 06/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 21:46:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 09 18:19:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.410	2.760	62341744	119.1E6	13.869m	44.601 #
2) SA Decachlor...	8.592	7.542	62536487	50740262	18.564	15.117

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Data\PQ061323\
Data File : PQ061395.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2023 19:49
Operator : YP\AJ
Sample : 03170-03
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_Q
ClientSampleId :
AUD-1971


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/14/2023
Supervised By :Ankita Jodhani 06/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 21:46:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_Q\Method\PQ060923.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 09 18:19:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

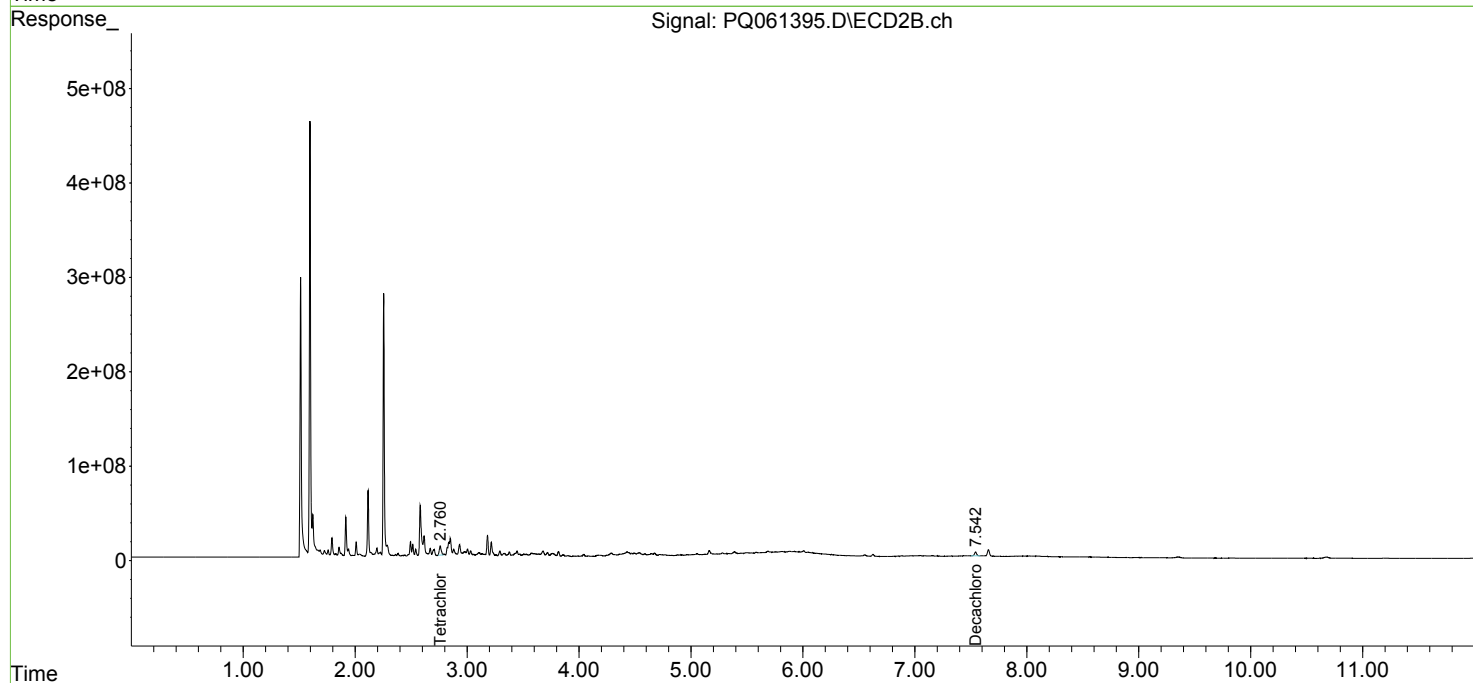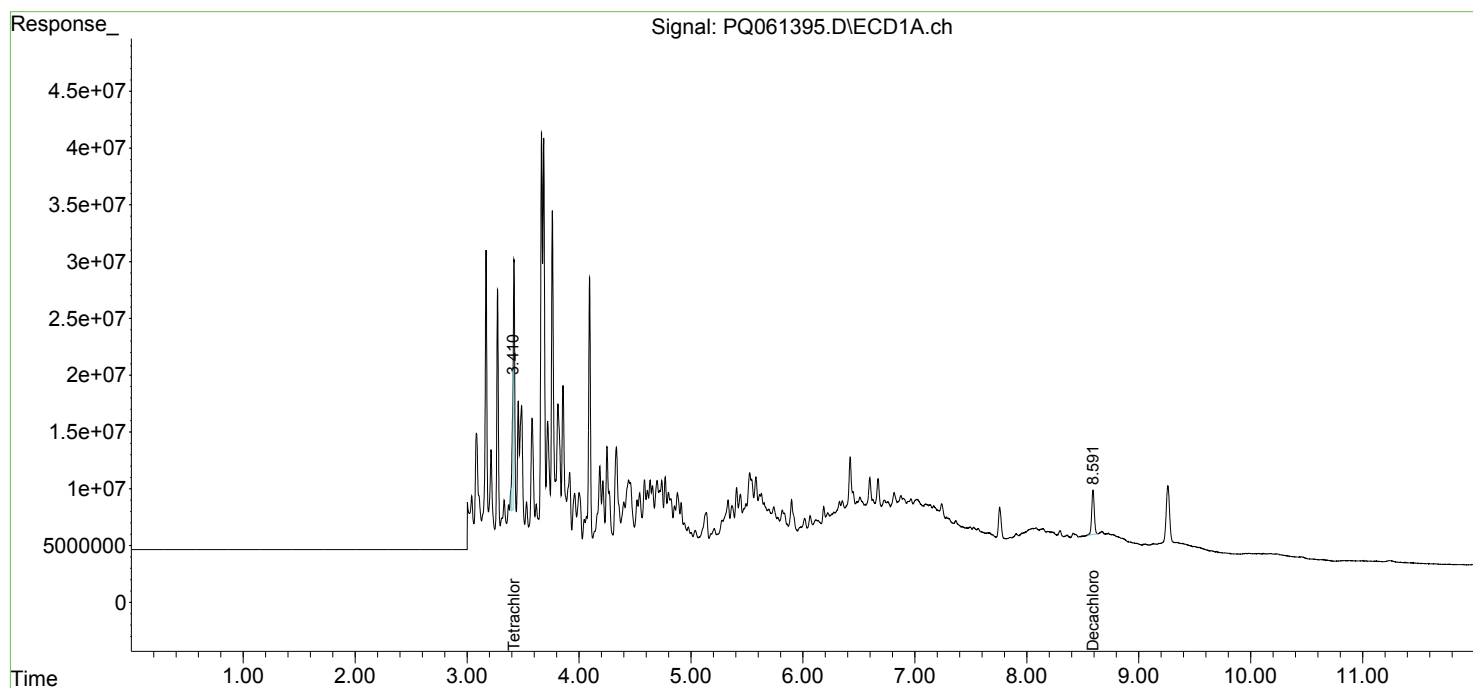

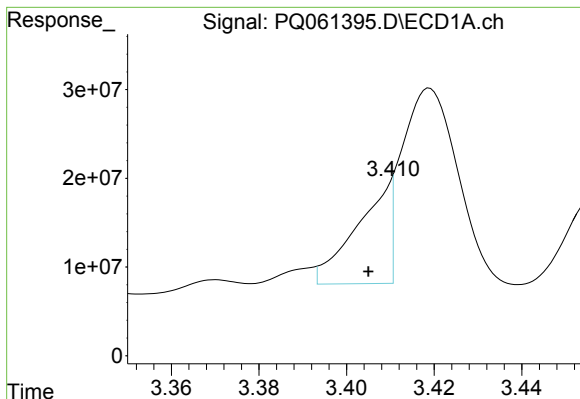


#1 Tetrachloro-m-xylene

R.T.: 3.410 min
Delta R.T.: 0.005 min
Response: 62341744
Conc: 13.87 ng/ml

Instrument :
ECD_Q
ClientSampleId :
AUD-1971


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/14/2023
Supervised By :Ankita Jodhani 06/14/2023

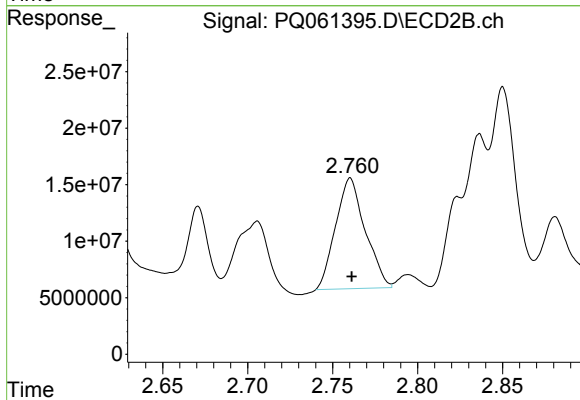


#1 Tetrachloro-m-xylene

R.T.: 2.760 min
Delta R.T.: 0.000 min
Response: 119101548
Conc: 44.60 ng/ml

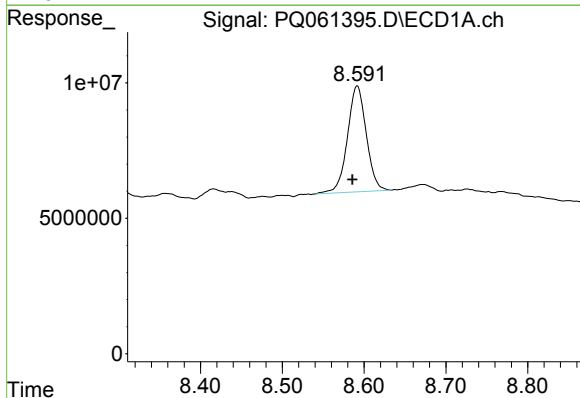

#2 Decachlorobiphenyl

R.T.: 8.592 min
Delta R.T.: 0.006 min
Response: 62536487
Conc: 18.56 ng/ml

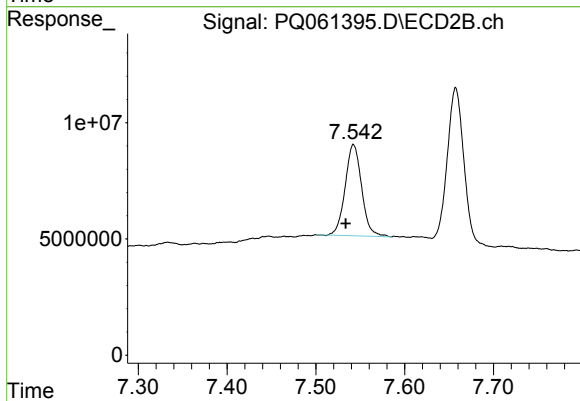

#2 Decachlorobiphenyl

R.T.: 7.542 min
Delta R.T.: 0.009 min
Response: 50740262
Conc: 15.12 ng/ml